



Institute for Reference
Materials and Measurements



European Reference Materials

CERTIFICATION REPORT

**Certification of Charpy V-notch Reference Test Pieces of
30 J Nominal Absorbed Energy**

Certified Reference Material ERM[®]-FA013be

EUR 24531 EN – 2010

The mission of the JRC-IRMM is to promote a common and reliable European measurement system in support of EU policies.

European Commission
Joint Research Centre
Institute for Reference Materials and Measurements

Contact information

Reference materials sales
Retieseweg 111
B-2440 Geel, Belgium
E-mail: jrc-irrm-rm-sales@ec.europa.eu
Tel.: +32 (0)14 571 705
Fax: +32 (0)14 590 406

<http://irrm.jrc.ec.europa.eu/>
<http://www.jrc.ec.europa.eu/>

Legal Notice

Neither the European Commission nor any person acting on behalf of the Commission is responsible for the use which might be made of this publication.

***Europe Direct is a service to help you find answers
to your questions about the European Union***

Freephone number (*):

00 800 6 7 8 9 10 11

(*) Certain mobile telephone operators do not allow access to 00 800 numbers or these calls may be billed.

A great deal of additional information on the European Union is available on the Internet. It can be accessed through the Europa server <http://europa.eu/>

JRC 60619

EUR 24531 EN
ISBN 978-92-79-15631-1
ISSN 1018-5593
doi:10.2787/30520

Luxembourg: Publications Office of the European Union

© European Union, 2010

Reproduction is authorised provided the source is acknowledged

Printed in Belgium

CERTIFICATION REPORT

Certification of Charpy V-notch Reference Test Pieces of 30 J Nominal Absorbed Energy

Certified Reference Material ERM[®]-FA013be

A. Lamberty, A. Dean, G. Roebben

European Commission, Joint Research Centre
Institute for Reference Materials and Measurements (IRMM), Geel (BE)

Disclaimer

Certain commercial equipment, instruments, and materials are identified in this report to specify adequately the experimental procedure. In no case does such identification imply recommendation or endorsement by the European Commission, nor does it imply that the material or equipment is necessarily the best available for the purpose.

Abstract

This certification report describes the processing and characterisation of ERM[®]-FA013be, a batch of Charpy V-notch certified reference test pieces. Sets of five of these test pieces are used for the verification of pendulum impact test machines according to EN 10045-2 (Charpy impact test on metallic materials, Part 2. Method for the verification of impact testing machines [1]) or according to ISO 148-2 (Metallic materials - Charpy pendulum impact test – Part 2: Verification of test machines [2]).

The certified value for KV (= energy required to break a V-notched test piece using a pendulum impact test machine) is 26.0 J. The associated uncertainty (0.9 J, $k = 2$ corresponding to a confidence level of about 95 %) is calculated for the mean of a set of five test pieces.

The absorbed energy (KV) is procedurally defined and refers to the impact energy required to break a V-notched bar of standardised dimensions, as defined in EN 10045-1 [3] and ISO 148-1 [4]. The certified value of ERM[®]-FA013be is traceable to the SI, via the SI-traceable certified value of the master batch ERM[®]-FA013ba, by testing samples of ERM[®]-FA013ba and ERM[®]-FA013be under repeatability conditions on an impact pendulum verified and calibrated with SI-traceably calibrated tools. The certified value is valid only for strikers with a 2 mm tip radius. The certified value is valid at (20 ± 2) °C.

Contents

Abstract	1
Contents	2
Glossary	4
1 Introduction: the Charpy pendulum impact test	6
2 The certification concept of Master Batch and Secondary Batch	7
2.1 <i>Difference between Master and Secondary Batches</i>	7
2.2 <i>Certification of a Secondary Batch of Charpy V-notch test pieces</i>	7
2.3 <i>Uncertainty of the certified value of a Secondary Batch of Charpy V-notch test pieces</i>	8
3 Participants	8
4 Processing	8
4.1 <i>Processing of hot-rolled bars</i>	9
4.2 <i>Heat treatment of hot-rolled bars</i>	9
4.3 <i>Machining of Charpy test pieces</i>	9
4.4 <i>Quality control</i>	9
4.5 <i>Packaging and storage</i>	10
5 Characterisation	10
5.1 <i>Characterisation tests</i>	10
5.2 <i>Data from Master Batch ERM[®]-FA013ba</i>	12
5.3 <i>Calculation of KV_{CRM} and of u_{char}</i>	13
6 Homogeneity	13
7 Stability	14
8 Calculation of certified value, combined and expanded uncertainty 14	
9 Metrological traceability	15
10 Commutability	15

11 Summary of results	16
12 Instructions for use	16
12.1 <i>Intended use</i>	16
12.2 <i>Sample preparation</i>	16
12.3 <i>Pendulum impact tests</i>	17
Acknowledgements	17
References.....	19
Annex 1	21
Annex 2.....	22

Glossary

AISI	American Iron and Steel Institute
ASTM	American Society for Testing and Materials
BCR	Community Bureau of Reference
CEN	European Committee for Standardization
CRM	Certified Reference Material
EC	European Commission
EN	European Norm
ERM [®]	European Reference Material
h	Hour
IMB	International Master Batch
IRMM	Institute for Reference Materials and Measurements
ISO	International Organization for Standardization
JRC	Joint Research Centre
<i>k</i>	Coverage factor
<i>KV</i>	Absorbed energy = energy required to break a V-notched test piece of defined shape and dimensions when tested with a pendulum impact testing machine
<i>KV_{CRM}</i>	Certified <i>KV</i> value of a set of 5 reference test pieces from the Secondary Batch
<i>KV_{MB}</i>	Certified <i>KV</i> value of the Master Batch test pieces
LNE	Laboratoire National de Métrologie et d'Essais
MB	Master Batch
min	Minute
<i>n_{MB}</i>	Number of samples of the Master Batch tested during certification of the Secondary Batch
<i>n_{SB}</i>	Number of samples of the Secondary Batch tested for certification
<i>RSD</i>	Relative standard deviation

s	Standard deviation
SB	Secondary Batch
s_h	Standard deviation of the results of the samples tested to assess the homogeneity of the Secondary Batch
s_{MB}	Standard deviation of the n_{MB} results of the samples of the Master Batch tested for the certification of the Secondary Batch
s_{SB}	Standard deviation of the n_{SB} results of the samples tested for the characterisation of the Secondary Batch
u_{CRM}	Combined standard uncertainty of KV_{CRM}
U_{CRM}	Expanded uncertainty ($k = 2$, confidence level 95 %) of KV_{CRM}
u_{char}	Standard uncertainty of the result of the characterisation tests
$u_{char,rel}$	Relative standard uncertainty of the result of the characterisation tests
u_h	Contribution to uncertainty from homogeneity
u_i	Value of uncertainty from contribution i
u_{MB}	Standard uncertainty of KV_{MB}
$u_{MB,rel}$	Relative standard uncertainty of KV_{MB}
% m/m	Mass fraction
\bar{X}_{MB}	Mean KV value of the n_{MB} measurements on samples of the Master Batch tested when characterising the Secondary Batch
\bar{X}_{SB}	Mean KV value of the n_{SB} results of the samples tested for the characterisation of the Secondary Batch
Δh	difference between the height of the centre of gravity of the pendulum prior to release and at the end of the half-swing during which the test sample is broken
ν_{RM}	Effective number of degrees of freedom associated with the uncertainty of the certified value

1 Introduction: the Charpy pendulum impact test

The Charpy pendulum impact test is designed to assess the resistance of a material to shock loading. The test, which consists of breaking a notched bar of the test material using a hammer rotating around a fixed horizontal axis, is schematically presented in Figure 1.

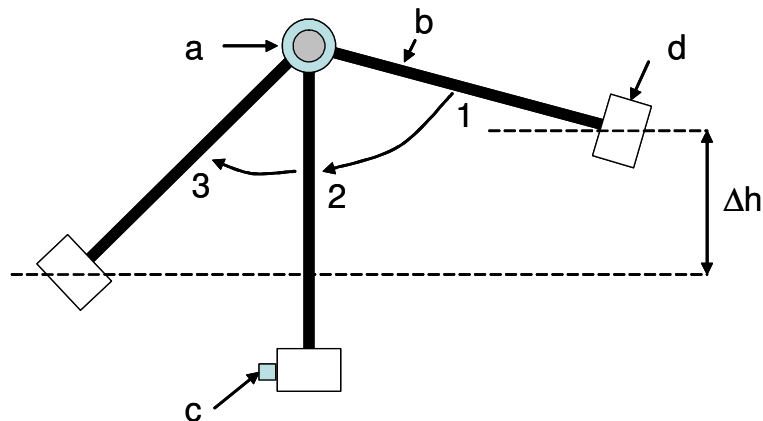


Figure 1: Schematic presentation of the Charpy pendulum impact test, showing a: the horizontal rotation axis of the pendulum, b: the stiff shaft on to which is fixed d: the hammer. The hammer is released from a well-defined height (position 1). When the hammer has reached maximum kinetic energy (shaft in vertical position 2), the hammer strikes c: the test sample, which is positioned on a support and against the pendulum anvils (not shown). The height reached by the hammer after having broken the sample (position 3) is recorded. The difference in height between position 1 and 3 (Δh) corresponds with a difference in potential energy, and is a measure of the energy required to break the test sample.

The energy absorbed by the test sample is very dependent on the impact pendulum construction and its dynamic behaviour. Methods to verify the performance of an impact pendulum require the use of reference test pieces as described in European, ISO and other international standards [1, 2, 5]. The reference test pieces dealt with in this report comply with a V-notched test piece shape of well-defined geometry [1,2], schematically shown in Figure 2.

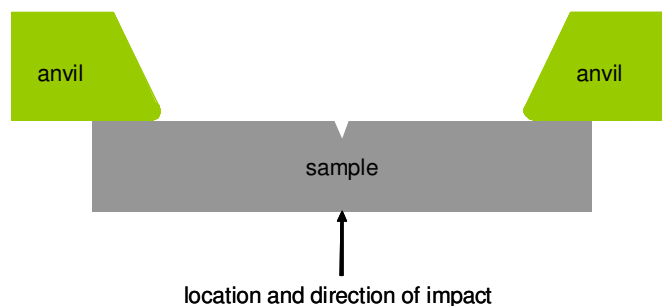


Figure 2: Schematic drawing of a V-notched Charpy sample (top-view), indicating the place and direction of impact.

2 The certification concept of Master Batch and Secondary Batch

2.1 Difference between Master and Secondary Batches

The BCR reports by Marchandise et al. [6] and Varma [7] provide details of the certification of BCR “Master Batches” (MB) of Charpy V-notch certified reference test pieces. The certified value of a Master Batch is obtained using an international laboratory intercomparison. Details of the most recent production of a Charpy Master Batch are given in [8].

This report describes the production of a “Secondary Batch” (SB) of Charpy V-notch certified reference test pieces at the Institute for Reference Materials and Measurements (IRMM) of the European Commission's (EC) Joint Research Centre (JRC). The work was performed in accordance with procedures described in the BCR reports [6] and [7]. The certification of a SB is based on the comparison of a set of SB test pieces with a set of test pieces from the corresponding MB under repeatability conditions on a single pendulum.

The BCR reports [6] and [7] were published in 1991 and 1999, respectively. Since 2000, the calculation of the certified value and the estimation of its uncertainty have been updated to an approach compliant with the ISO/IEC Guide to the Expression of Uncertainty in Measurement [9]. This revised approach was developed and presented by Ingelbrecht et al. [10, 11], and is summarised below.

2.2 Certification of a Secondary Batch of Charpy V-notch test pieces

The certified absorbed energy of a SB of Charpy V-notch reference test pieces (KV_{CRM}) is calculated from the mean KV -value of a set of SB-samples (\bar{X}_{SB}) tested on a single pendulum. This value \bar{X}_{SB} has to be corrected for the bias of this particular pendulum. The bias of the pendulum at the moment of testing the samples of the SB, is estimated by comparing the mean KV -value of a number of samples of the MB (\bar{X}_{MB}), tested together with the SB samples under repeatability conditions, with the certified value of the MB (KV_{MB}). KV_{CRM} is then calculated as follows [10]:

$$KV_{CRM} = \left[\frac{KV_{MB}}{\bar{X}_{MB}} \cdot \bar{X}_{SB} \right] \quad \text{Eq. 1}$$

For this approach to be reliable, the pendulum used for the tests on MB and SB in repeatability conditions, must be well performing. In other words, the ratio $\frac{KV_{MB}}{\bar{X}_{MB}}$ must be close to 1. IRMM now allows a difference of 5 % ($KV_{MB} > 40$ J) or 2 J ($KV_{MB} < 40$ J) between KV_{MB} and \bar{X}_{MB} , corresponding with the level of bias allowed for reference pendulums specified in EN 10045-2 [1] and ISO 148-3 [12].

Also, for reasons of commutability, a comparable response of the pendulum to the MB and SB samples is required. This is the reason why MB and SB samples are made from nominally the same steel. Moreover, it is checked that the ratio $\frac{KV_{CRM}}{KV_{MB}}$ is close to 1. IRMM now allows a difference of 20 % ($KV_{MB} > 40$ J) or 8 J ($KV_{MB} < 40$ J) between KV_{CRM} and KV_{MB} to ensure that the MB and SB samples have a comparable interaction with the pendulum.

2.3 Uncertainty of the certified value of a Secondary Batch of Charpy V-notch test pieces

The uncertainty of the certified value of the SB is a combination of the uncertainties of the right-hand side factors in Eq. 1. It is clear that the MB-SB approach necessarily results in a larger uncertainty of the certified value of SB in comparison with the MB. The additional uncertainty depends on the uncertainty of the ratio $\bar{X}_{MB}/\bar{X}_{SB}$. The full measurement uncertainty of the values \bar{X}_{MB} and \bar{X}_{SB} is relatively large. However, when all conditions mentioned above (repeatability conditions, pendulum performance, and commutability between Secondary and Master Batch) are fulfilled, then the uncertainties of the values \bar{X}_{MB} and \bar{X}_{SB} have several contributions in common, in particular the uncertainty due to the bias of the pendulum. These shared uncertainty components do not contribute to the uncertainty of the ratio $\bar{X}_{MB}/\bar{X}_{SB}$, and only the standard deviations of the SB and MB results in the MB-SB comparison test need to be taken into account (see also Section 5.3). Thus, the MB-SB comparison approach can produce a value for the uncertainty of KV_{CRM} that is sufficiently small to meet the requirements of the intended use of the certified reference material (CRM).

3 Participants

The processing of the SB (ERM[®]-FA013be) test pieces was carried out by the Laboratoire National de Métrologie et d'Essais (LNE), Trappes (FR), using steel bars produced at Cogne Acciai Speciali, Aosta (IT). The MB (ERM[®]-FA013ba) samples used in the characterisation of the SB were provided by IRMM, Geel (BE). The homogeneity of the SB was evaluated based on data obtained at LNE using a pendulum verified according to the criteria imposed by EN 10045-2 [1] and ISO 148-2 [2]. Characterisation of the SB was carried out at IRMM using a pendulum verified according to the criteria imposed by EN 10045-2 [1] and ISO 148-2 [2]. Data evaluation was performed at IRMM.

4 Processing

The ERM[®]-FA013be test pieces were prepared from AISI 4340 steel. The steel was cast and rolled into bars at Aubert&Duval (see section 4.1). Production of the test pieces from these bars was performed under the supervision of LNE (see sections 4.2, 4.3, 4.4 and 4.5).

4.1 Processing of hot-rolled bars

The base material consisted of AISI 4340 steel, produced at Cogne Acciai Speciali. To limit the amount of impurities potentially affecting the homogeneity of the fracture resistance, the following compositional tolerances were imposed on the selected steel batch: Mn 0.7 – 0.8, Mo 0.23 - 0.28, Ni 1.7 – 1.85, P < 0.01, Si 0.2 – 0.35, S < 0.008 (in % m/m), which is stricter than generally allowed for AISI 4340. The ingot was hot rolled, resulting in bars that were 4 m long and with a squared cross-section of 11.5x11.5 mm. For the ERM®-FA013be batch, steel was used from ingot number NC40MW, billet D and E. A full description of the processing and quality check of the steel bars is available [17].

4.2 Heat treatment of hot-rolled bars

The heat treatment of the hot-rolled bars was performed at Aubert&Duval. 22 bars were heat-treated together. Bars were placed onto rollers which slowly move the bars back and forth inside the furnace during the heat treatment to increase the homogeneity of the resulting microstructure. The first heat treatment was an austenisation treatment performed in a furnace of 'class 10 °C' ¹ at 850 °C for 30 min. From this furnace, the bars were quenched into oil at 40 °C. After the oil-quench, the samples were annealed in a furnace of 'class 5 °C' at 350 °C for 120 min. After this annealing treatment, the samples were cooled down in air.

After heat treatment, a limited number of samples (5) were machined for a preliminary check of the obtained energy level. Results indicated an average KV-level (23.6 J) within the desired energy range (25 to 30 J).

4.3 Machining of Charpy test pieces

After the heat treatment the samples were machined to dimensional tolerances imposed in EN 10045-2 [1] and ISO 148-3 [12]. The batch code (BE30) and the individual sample code were engraved twice on one long face of each sample, on both sides of the notch, for fully traceable sample coding also after fracture ('30' indicates the nominal absorbed energy level (30 J); 'BE' is the letter code as assigned consecutively to batches of the same nominal absorbed energy). The V-notch was introduced using an electro-erosion tool.

4.4 Quality control

When all samples from the batch were fully machined, a selection of 25 samples was made. The dimensions of the 25 samples were checked on March 10, 2010 against the criteria specified in ISO 148-3 [12] (length $55.0^{+0.0}_{-0.3}$ mm, height 10.00 ± 0.06 mm, width 10.00 ± 0.07 mm, notch angle 45 ± 1 °, height remaining at notch root 8.00 ± 0.06 mm, radius at notch root 0.250 ± 0.025 mm, distance between the plane of symmetry of the notch and

¹ In a furnace of 'class x °C', the variation of the temperature is smaller than x °C. The furnaces used have 10 heating zones. Each zone has 3 controlling thermocouples and 3 measurement thermocouples. These are regularly calibrated. When one faulty thermocouple is detected, it is replaced by a thermocouple produced with wire from the same roll. When a roll is exhausted, all thermocouples are replaced with new ones.

the longitudinal axis of the test piece 27.5 ± 0.2 mm). One of the samples was outside the ranges specified in ISO 148-3 [12].

The 25 samples checked for geometrical compliance were impact tested on March 10, 2010 on the Tinius Olsen, model 74 impact (serial number 126 385) pendulum - which is one of the French reference pendulums - at LNE. The results are reported in certificate LNE n° G080477/DE/3 [13]. The average *KV* of the 25 samples was 27.72 J, which is sufficiently close to the desired energy range (22.5 J to 27.5 J). The standard deviation of the test results ($s = 0.72$ J, $RSD = 2.6$ %) was smaller than the contractually fixed maximum allowed 3%. The variation was checked again during the certification tests at IRMM (see section 5).

4.5 Packaging and storage

Finally, the samples were cleaned and packed in sets of 5, in oil-filled and closed plastic bags. These oil-filled bags, together with a label, again were packed in a sealed plastic bag, and shipped to IRMM. After arrival (March 23, 2010), the 1150 samples (or 230 sets) were registered and stored at room temperature, pending distribution.

5 Characterisation

5.1 Characterisation tests

30 samples from ERM[®]-FA013be (sets 1, 18, 48, 81, 111 and 138) were tested under repeatability conditions with 25 samples from MB ERM[®]-FA013ba (sets 10, 59, 92, 144 and 190), using the Instron Wolpert PW 30 (serial number 7300 H1527) machine of IRMM, an impact pendulum yearly verified according to procedures described in EN 10045-2 [1] and ISO 148-2 [2]. Tests were performed on July 13, 2010 (laboratory temperature 20 ± 1 °C), in accordance with EN 10045-1 [3] and ISO 148-1 [4]. The measured absorbed energy values were corrected for friction and windage losses.

3 of the 30 samples tested for ERM[®]-FA013be and 1 of the 25 samples tested for ERM[®]-FA013ba gave excessively high absorbed energy values. Inspection of the broken samples reveals the same type of damage as observed on previous FA013 batches. After testing, all Charpy samples show 'first-strike' marks: these are the marks caused by the interaction between sample and anvils during the first and intended hammer impact. Upon fracture, the broken half samples loose contact with hammer and anvils and follow one of a variety of possible trajectories, away from the pendulum, depending on the properties of both pendulum and test material. Some samples show 'second-strike' marks. These are marks caused by a second impact of the already broken half samples back onto the anvils. This phenomenon has been described by Schmieder et al. [14]. Most of the broken FA013ba and FA013be samples show second-strike marks. A mere second impact of the broken half samples onto the anvils does not affect the measured *KV* value, since it does not involve or slow down the swinging pendulum.

For 4 samples, a significant post-fracture deformation mark on one of the long edges of the notched face of the sample was observed. Systematically, this

indent is accompanied by a broader deformation of the diagonally opposite long edge (on the face of the sample opposite the notch). This suggests that the samples, during the second strike onto the anvils, were briefly caught between anvil and a part of the swinging pendulum. This induces erroneously high measured absorbed energy values. For this technical reason, 4 data were eliminated from the analysis. All other data were accepted. An analysis of the normality of the distribution of remaining *KV* values did not indicate a skewed distribution towards higher or lower absorbed energy values.

The same parasitic energy absorbing phenomenon occurred also for some but not all of the other batches which were prepared previously. Also, the phenomenon did not occur during the pre-acceptance tests at LNE. Furthermore, the FA013ba batch was tested on 12 pendulums during a laboratory intercomparison, revealing that post-fracture energy absorption occurs only for a minority of the pendulums involved (2 out of 12).

The above observations indicate that excessive post-fracture energy absorption affecting the measured *KV* values can occur, but only for a limited number of combinations of pendulum and material. In each case, excessively high measured values are easily related to large post-fracture deformation marks on the broken samples. Users of ERM-FA013be reference materials encountering outlier values that can be related to post-fracture indentation marks on the broken samples are requested to eliminate the corresponding data from the analysis of their results.

The comparison of the indirect verification results with the certified value and uncertainty is based on the mean of the 5 measured *KV* values, because this is the sample size for which the uncertainty of the certified value has been calculated. If outlier values have to be eliminated because of post-fracture indentation, the corresponding expanded uncertainty for $n = 4$ remaining results is $U = 1.0$ J, for $n = 3$ remaining results $U = 1.1$ J.

The accepted data obtained on individual test pieces are shown in Figure 3 and in Annex 1. In Figure 3 linear trend-lines are added to illustrate the absence of a significant trend in the results with the analysis sequence. The results of the measurements are summarised in Table 1: Results of characterisation of Batch ERM®-FA013be by comparison with Master Batch ERM®-FA013ba.

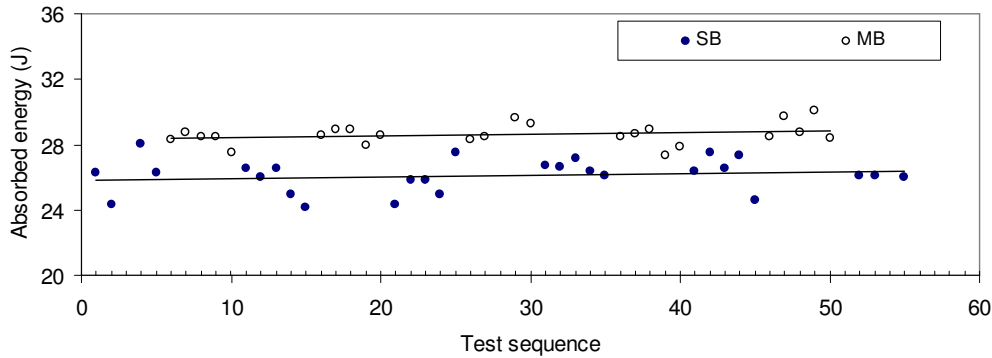


Figure 3: Absorbed energy values of the 27 test pieces of ERM®-FA013be and 24 test pieces of ERM®-FA013ba displayed in the actual test sequence.

Table 1: Results of characterisation of Batch ERM®-FA013be by comparison with Master Batch ERM®-FA013ba.

	Number of test pieces	Mean value	Standard deviation	Relative standard deviation
	n_{MB} or n_{SB}	\bar{X}_{MB} or \bar{X}_{SB} (J)	s_{MB} or s_{SB} (J)	RSD (%)
ERM®-FA013ba (MB)	24	28.62	0.64	2.2
ERM®-FA013be (SB)	27	26.11	1.02	3.9

The SB-results meet the EN 10045-2 and ISO 148-3 acceptance criteria for a batch of reference materials ($s_{SB} < 2$ J), as well as the more stringent acceptance criterion ($s_{SB} < 1.5$ J) contractually fixed between IRMM and its sample supplier for batches of this nominal absorbed energy level (30 J).

5.2 Data from Master Batch ERM®-FA013ba

To calculate KV_{CRM} for ERM®-FA013be one needs KV_{MB} of the MB used, i.e. ERM®-FA013ba. Table 2 shows the main MB-data, taken from the Certificate of Analysis of ERM®-FA013ba (Annex 2).

Table 2: Data from the certification of Master Batch ERM®-FA013ba.

	Certified absorbed energy of Master Batch	Standard uncertainty of KV_{MB}	Standard uncertainty of KV_{MB}
	KV_{MB} (J)	u_{MB} (J)	$u_{MB,rel}$ (%)
ERM®-FA013ba	28.46	0.23	0.81

5.3 Calculation of KV_{CRM} and of u_{char}

From the data in Table 1 and Table 2, and using Eq. 1, one readily obtains that $KV_{CRM} = 26.0$ J. The uncertainty associated with the characterisation of the SB, u_{char} , is assessed as in Eq. 2 [11], which sums the relative uncertainties of the three factors in Eq. 1:

$$u_{char} = KV_{CRM} \sqrt{\frac{u_{MB}^2}{KV_{MB}^2} + \frac{s_{SB}^2}{n_{SB} \cdot \bar{X}_{SB}^2} + \frac{s_{MB}^2}{n_{MB} \cdot \bar{X}_{MB}^2}} \quad \text{Eq. 2}$$

\bar{X}_{SB} and \bar{X}_{MB} were obtained under repeatability conditions. Therefore, the uncertainty of the ratio $\bar{X}_{SB} / \bar{X}_{MB}$ is not affected by the contributions from reproducibility and bias of the pendulum used to compare MB and SB. Table 3 summarises the input quantities of the u_{char} uncertainty budget, their respective statistical properties, and shows how they were combined. The effective number of degrees of freedom for u_{char} is obtained using the Welch-Satterthwaite equation [9]].

Table 3: Uncertainty budget for u_{char}

symbol	source of uncertainty	measured value (J)	standard uncertainty (J)	probability distribution	divisor	sensitivity coefficient	relative uncertainty (%)	degrees of freedom
KV_{MB}	Certification of MB	28.46	0.23	normal	1	1	0.81	14
\bar{X}_{SB}	comparison of SB and MB in repeatability conditions	26.11	0.20	normal	1	1	0.75	26
\bar{X}_{MB}		28.62	0.13	normal	1	1	0.45	23
$u_{char,rel}$ (%)							1.19	45
u_{char} (J)							0.31	

6 Homogeneity

The test pieces are sampled from the SB, which is sufficiently, but not perfectly, homogeneous. Therefore, an appropriate homogeneity contribution u_h to the uncertainty of the certified value is required. u_h is related to s_h , the standard deviation between the samples in the SB (*sample-to-sample heterogeneity*), but also depends on the number of samples over which the KV -value is averaged. EN 10045-2 [1] and ISO 148-2 [2] specify that the pendulum verification must be performed using 5 test pieces, which is why a CRM-unit consists of a set of 5 test pieces. The appropriate uncertainty contribution must be an estimate of the *set-to-set heterogeneity*, which in the

case of a set of 5 test pieces can be calculated as $u_h = \frac{s_h}{\sqrt{5}}$.

Here, u_h is estimated from the results obtained at LNE on March 10, 2010 ($s_h = 0.72$ J), which leads to $u_h = \frac{s_h}{\sqrt{5}} = 0.33$ J. As is required for a homogeneity test, the samples were randomly selected from the whole batch. The number of samples tested (25) is sufficiently large to reflect the homogeneity of the full SB (1150 samples). It can be noted that u_h is probably a slight overestimation, since it contains also the repeatability of the instrument. However, the latter cannot be separated or separately measured.

7 Stability

The stability of the absorbed energy of Charpy V-notch certified reference test pieces was first systematically investigated for samples of nominally 120 J by Pauwels et al., who did not observe measurable changes of absorbed energy [15]. New evidence for the stability of the reference test pieces produced from AISI 4340 steel of lower energy levels (nominally 15 J, 30 J and 100 J) has been obtained recently, during the International Master Batch (IMB) project [16]. In the IMB-project, the stability of the certified test pieces is judged from the change of the mean of means of the absorbed energy obtained on 7 reference pendulums over a three year period. None of the three regression slopes for the tested energy levels was statistically significant at the 0.05 level. Given the large sample-to-sample heterogeneity and the limited number of samples (5) in a CRM unit, the uncertainty contribution from instability is considered to be insignificant in comparison to that of homogeneity.

The main reason for the microstructural stability of the certified reference test pieces is the annealing treatment to which the samples were subjected after the austenisation treatment. Annealing is performed at temperatures where the equilibrium phases are the same as the (meta-)stable phases at ambient temperature (α -Fe and Fe_3C). The only driving force for instability stems from the difference in solubility of interstitial elements in the α -Fe matrix, between annealing and ambient temperature. Relaxation of residual (micro-)stress by short-range diffusion or the additional formation or growth of precipitates during the shelf-life of the certified reference test pieces is expected to proceed but slowly.

Rather than neglecting the stability issue, efforts are spent to better establish the stability of the certified values of batches of Charpy CRMs. Until such further notice, it is decided to specify a limited shelf-life. A period of 10 years is chosen, counting from the date of the characterisation tests on the SB. Since batch ERM[®]-FA013be was characterised in July, 2010, the validity of the certificate reaches until July, 2020.

8 Calculation of certified value, combined and expanded uncertainty

As shown in 5.2, $KV_{CRM} = 26.0$ J. The uncertainty of the certified value is obtained by combining the contributions from the characterisation study, u_{char} ,

and from the homogeneity assessment, u_h , as is summarized in the following uncertainty budget (Table 4).

The relevant number of degrees of freedom calculated using the Welch-Satterthwaite equation [9], is sufficiently large ($\nu_{RM} = 60$) to justify the use of a coverage factor $k = 2$ to expand the confidence level to about 95 %. The obtained expanded uncertainty provides justification for the SB-MB approach followed: U_{CRM} is sufficiently smaller than the verification criterion of 4 J or even 2 J for reference pendulums.

Table 4: Uncertainty budget of KV_{CRM}

symbol	source of uncertainty	absolute value (J)	u_i (J)	degrees of freedom
u_{char}	characterisation of SB	0.31	0.31	45
u_h	homogeneity of SB	0.33	0.33	24
Combined standard uncertainty, u_{CRM}			0.45 J	60
Expanded Uncertainty, $k = 2$, U_{CRM}			0.9 J	ν_{RM}

9 Metrological traceability

The certified property is defined by the Charpy pendulum impact test procedure described in EN 10045-1 [3] and ISO 148-1 [4].

The certified value of the MB ERM[®]-FA013ba is traceable to the SI, since it was obtained using an interlaboratory comparison, involving a representative selection of qualified laboratories performing the tests in accordance with the standard procedures and using instruments verified and calibrated with SI-traceable calibration tools.

The certified value of ERM[®]-FA013be is made traceable to the SI-traceable certified value of the MB by testing SB and MB samples in repeatability conditions on an impact pendulum verified and calibrated with SI-traceably calibrated tools. Therefore, the certified value of ERM[®]-FA013be is traceable to the International System of Units (SI) via the corresponding Master Batch ERM[®]-FA013ba of the same nominal absorbed energy (30 J). Absorbed energy KV is a method-specific value, and can only be obtained by following the procedures specified in EN 10045-1 [3] and ISO 148-1 [4].

10 Commutability

The intended use of the certified reference test pieces is the verification of Charpy impact pendulums. During the certification of the MB, different pendulums were used, each equipped with an ISO-type striker of 2 mm tip radius. Until further notice, the certified values are not to be used when the test pieces are broken with an ASTM-type striker of 8 mm tip radius, although the expected differences can be small for materials with relatively low

absorbed energy such as the ERM[®]-FA013 batches of 30 J nominal absorbed energy [15].

11 Summary of results

The certified value and associated uncertainties are summarized in Table 5.

Table 5: Certified value and associated uncertainties for ERM[®]-FA013be.

Steel Charpy V-notch test pieces		
	Certified value ²⁾ [J]	Uncertainty ³⁾ [J]
Absorbed energy (<i>KV</i>) ¹⁾	26.0	0.9
<p>1) The absorbed energy (<i>KV</i>) is a method defined measurand. <i>KV</i> is the impact energy required to break a V-notched bar of standardised dimensions, as defined in EN 10045-1 and ISO 148-1. The certified value is valid only for strikers with a 2 mm tip radius, and in the temperature range of (20 ± 2) °C.</p> <p>2) The certified value of ERM[®]-FA013be, and its uncertainty, are traceable to the International System of Units (SI), via the master batch ERM[®]-FA013ba of the same nominal absorbed energy (30 J) by testing samples of ERM[®]-FA013ba and ERM[®]-FA013be under repeatability conditions on an impact pendulum verified and calibrated with SI-traceably calibrated tools.</p> <p>3) Estimated expanded uncertainty of the mean <i>KV</i> of the 5 specimens (delivered as 1 set), with a coverage factor $k = 2$, corresponding to a level of confidence of about 95 %, as defined in the ISO/IEC Guide 98-3:2008; Uncertainty of measurement – Part 3: Guide to the expression of uncertainty in measurement (GUM). The number of degrees of freedom of the certified uncertainty, $\nu_{RM} = 60$.</p>		

12 Instructions for use

12.1 Intended use

Samples of ERM[®]-FA013be correspond to the '(certified) BCR test pieces' as referred to in EN 10045-2 [1], as well as to the 'certified reference test pieces' as defined in ISO 148-3 [12]. Sets of five of these certified reference test pieces are intended for the indirect verification of impact testing machines with a striker of 2 mm tip radius according to procedures described in detail in EN 10045-2 [1] and ISO 148-2 [2].

The indirect verification provides an assessment of the bias of the user's Charpy pendulum impact machine. This bias assessment can be used in the calculation of the measurement uncertainty of Charpy tests on the pendulum after indirect verification. Such uncertainty calculation requires the certified value, the associated uncertainty, and in some cases also the degrees of freedom of the uncertainty, all given on page 1 of the certificate.

12.2 Sample preparation

Special attention is drawn to cleaning of the specimens prior to the tests. It is mandatory to remove the oil from the sample surface prior to testing, without damaging the edges of the sample. Between the moment of removing the protective oil layer and the actual test, corrosion can occur. This must be avoided by limiting this period of time, while keeping the sample clean.

The following procedure is considered a good practice.

1. First use absorbent cleaning-tissue to remove the excess oil. Pay particular attention to the notch of the sample, but do not use hard (e.g. steel) brushes to remove the oil from the notch.
2. Submerge the samples in ethanol for about 5 min. Use of ultrasonication is encouraged, but only if the edges of the samples are prevented from rubbing against each other. To reduce the consumption of solvent, it is allowed to make a first cleaning step with detergent, immediately prior to the solvent step.
3. Once samples are removed from the solvent, only manipulate the samples wearing clean gloves. This is to prevent development of corrosion between the time of cleaning and the actual test.
4. Before testing, bring the specimens to the test temperature (20 ± 2) °C. To assure thermal equilibrium is reached, move the specimens to the test laboratory at least 3 h before the tests.

12.3 Pendulum impact tests

After cleaning, the 5 samples constituting a CRM-unit need to be broken with a pendulum impact test machine in accordance with EN 10045-2 [1] or ISO 148-2 [2] standards. Prior to the tests, the anvils must be cleaned. It must be noted that Charpy test pieces sometimes leave debris on the Charpy pendulum anvils. Therefore, the anvils must be checked regularly and if debris is found, it must be removed. The uncertainty of the certified value applies to the mean of the 5 KV-values.

Acknowledgements

The authors wish to thank Mr. V. Kestens, Mr. G. Buttinger, Mr. T.P.J. Linsinger, Mr. R. Koeber, and Mr. H. Emons (all IRMM) for reviewing of the certification report.

References

1. *EN 10045-2 Charpy impact test on metallic materials - Part 2. Method for the verification of impact testing machines*, European Committee for Standardization, Brussels (BE), 1993
2. *ISO 148-2: Metallic materials - Charpy pendulum impact test - Part 2: Verification of testing machines*, International Organization for Standardization, Geneva (CH), 2008.
3. *EN 10045-1: Metallic materials - Charpy impact test - Part 1: Test method*, European Committee for Standardization, Brussels (BE), 1990
4. *ISO 148-1: Metallic materials - Charpy pendulum impact test - Part 1: Test method*, International Organization for Standardization, Geneva (CH), 2006
5. *ASTM E 23 - 02a Standard Test Methods for Notched Bar Impact Testing of Metallic Materials*, C. E-28, Editor. ASTM International, West Conshohocken (PA, USA), 2002
6. Marchandise, H., Perez-Sainz, A., Colinet, E., *Certification of the impact toughness of V-notch Charpy specimens*, in *BCR information series*. Community Bureau of Reference - BCR, Brussels (BE), 1991
7. Varma, R.K., *The certification of two new master batches of V-notch Charpy impact toughness specimens in accordance with EN 10045-2: 1992*, in *BCR information series*. Office for Official Publications of the European Communities, Luxembourg (LU), 1999
8. Roebben, G., Dean A., Lamberty A., *Certification of Master Batches of Charpy V-notch reference test pieces of nominal absorbed energy levels 30 J, 80 J and 120 J; Certified Reference Material ERM-FA013ba, ERM-FA015v and ERM-FA016ax*, Report EUR 23760 EN, ISBN 978-92-79-11327-7, Office for Official Publications of the European Communities, Luxembourg (LU), 2009
9. *ISO/IEC Guide 98-3:2008, Uncertainty of measurement - Part 3: Guide to the expression of uncertainty in measurement (GUM:1995)*, International Organization for Standardization, Geneva (CH), 2008
10. Ingelbrecht, C. and Pauwels J., *EC Reference Materials for Impact Toughness - Traceability and uncertainty*. Presentation at Eurachem Eurolab symposium on Reference Materials for Technologies in the New Millennium, Berlin, May 22-23, 2000.
11. Ingelbrecht, C., Pauwels, J., and Gyppaz, D., *Charpy specimens from BCR for machine verification according to EN 10045-2*. Poster presentation at Charpy Centenary Conference, October 2-5, Poitiers (FR), 2001
12. *ISO 148-3: Metallic materials - Charpy pendulum impact test - Part 3: Preparation and characterization of Charpy V-notch test pieces for indirect verification of pendulum impact machines*, International Organization for Standardization, Geneva (CH), 2008
13. Lefrançois, S., *Certificat d'étalonnage G080477/DE/3*. Laboratoire National de métrologie et d'essais, Trappes (FR), 2010
14. Schmieder, A. K., Purtscher P. T., Vigliotti, D. P., *The role of strike marks on the reproducibility of Charpy impact test results*, in *Pendulum impact machines: procedures and specimens for verification*, ASTM

- STP 1248, ed. Siewert, T. A. and Schmieder A. K., American Society for Testing and Materials, Philadelphia (USA), 1995
15. Pauwels, J., Gyppaz, D., Varma, R., Ingelbrecht, C., *European certification of Charpy specimens: reasoning and observations*, in *Pendulum Impact testing: A Century of Progress*. Seattle, Washington: American Society for Testing and Materials, 1999
 16. McCowan, C.N., Roebben, G., Yamaguchi, Y., Lefrançois, S., Splett, J. D., Takagi, S., Lamberty, A., *International Comparison of Impact Reference Materials (2004)*, J. ASTM International, Vol. 3(2), 2004
 17. Gyppaz, D., *Elaborazione e verifica acciaio SAE 4340 per provette Charpy V di riferimento - colata 960133, Cogne Acciai Speciali, Aosta (1999)*.

Annex 1

Results of characterisation measurements of ERM[®]-FA013be as measured according to EN 10045-1 and ISO 148-1 at IRMM, July 12, 2010.

	Master Batch ERM[®]-FA013ba	Secondary Batch ERM[®]-FA013be
	<i>KV</i> (J)	<i>KV</i> (J)
1	28.32	26.25
2	28.71	24.35
3	28.45	28.05
4	28.45	26.25
5	27.54	26.51
6	28.58	26.00
7	28.97	26.51
8	28.97	24.99
9	27.93	24.12
10	28.58	24.35
11	28.32	25.81
12	28.45	25.81
13	29.63	24.92
14	29.24	27.47
15	28.51	26.70
16	28.64	26.64
17	28.91	27.15
18	27.34	26.39
19	27.86	26.13
20	28.52	26.33
21	29.70	27.48
22	28.78	26.58
23	30.10	27.35
24	28.39	24.56
25		26.06
26		26.13
27		26.00
28		
29		
30		
Mean (J)	28.62	26.11
Standard deviation (J)	0.64	1.02
<i>RSD</i> (%)	2.2	3.9

Annex 2



CERTIFICATE OF ANALYSIS

ERM®- FA013ba

STEEL		
	Impact toughness	
	Certified value ²⁾ [J]	Uncertainty ³⁾ [J]
Absorbed energy (KV) ¹⁾	28.46	0.23

1) The absorbed energy (KV) is procedurally defined and refers to the impact energy required to break a V-notched bar of standardised dimensions, as defined in EN 10045-1 and ISO 148-1.

2) The certified value is estimated as the mean of means of absorbed energies measured at 15 laboratories. At each laboratory, 20 test pieces were broken. The instruments used by these laboratories are regularly verified with equipment that is calibrated in a manner that is traceable to the International System of Units (SI). Therefore, the certified value is traceable to the International System of Units (SI).

3) Standard uncertainty u of the certified mean absorbed energy of batch ERM-FA013ba, estimated as the standard deviation of the mean of the 15 laboratory mean values, corresponding with a confidence level of about 68 %.

This certificate is valid until January 2018.

NOTE

European Reference Material ERM®-FA013ba was produced and certified under the responsibility of the Institute for Reference Materials and Measurements of the European Commission's Joint Research Centre according to the principles laid down in the technical guidelines of the European Reference Materials® co-operation agreement between BAM-IRMM-LGC. Information on these guidelines is available on the internet (<http://www.erm-crm.org>).

Accepted as an ERM®, Geel, January 2009.

Signed: _____

Prof. Dr. Hendrik Emons
European Commission
Joint Research Centre
Institute for Reference Materials and Measurements
Retieseweg 111
B-2440 Geel, Belgium



Registration No. 268-TEST
ISO Guide 34 for the
production of reference materials

All following pages are an integral part of the certificate.

Page 1 of 3

DESCRIPTION OF THE SAMPLE

A unit consists of five Charpy V-notch test pieces, which are rectangular steel bars of nominal dimensions 55 mm x 10 mm x 10 mm, with one V-notch, accurately machined to tolerances imposed in EN 10045-2 and ISO 148-3. The five specimens are packed together in a plastic bag filled with oil to prevent oxidation.

ANALYTICAL METHOD USED FOR CERTIFICATION

Charpy pendulum impact tests in accordance with EN 10045-1 and ISO 148-1, using pendulum impact machines with a 2 mm striker tip radius.

PARTICIPANTS

- Aubert&Duval, Les Ancizes and Gennevilliers (FR)
- Bodycote Materials Testing, Emmen (NL)* (RvA testen L085)
- Bodycote Materials Testing, Spijkenisse (NL)* (RvA testen L085)
- Bundesanstalt für Materialforschung und -prüfung (BAM), Abteilung V Werkstofftechnik, Berlin (DE)* (DAP-PL-2614.16)
- Centro de Apoio Tecnológico a Indústria Metalomecânica (CATIM), Laboratório de Ensaios, Porto (PT)* (IPAC L009)
- Cogne Acciai Speciali, Aosta (IT)
- Fraunhofer Gesellschaft, Institut für Werkstoffmechanik, Freiburg (DE)
- European Commission Joint Research Centre (JRC), Institute for Reference Materials and Measurements, Geel (BE) (BELAC 268-Test)
- Korea Research Institute of Standards and Science, Strength Evaluation Group, Daejeon, Korea
- Laboratoire National de Métrologie et d'Essais, Charpy Laboratory, Trappes (FR)* (COFRAC SMH 2-1287)
- National Institute of Standards and Technology (NIST), Materials Reliability Division, Boulder, USA
- SCK-CEN, Labo Reactormaterialenonderzoek, Mol (BE)* (BELAC 015-Test)
- SIRRI-S, Beproevinglaboratorium Gent, Zwijnaarde (BE)* (BELAC 232-Test)
- U.S. Steel Košice, Labortest, Košice (SK)* (SNAS 026/S012)
- Universität Stuttgart, Materialprüfungsanstalt, Stuttgart (DE)* (DAP-PL-2907.02)
- VTT, Espoo (FI)

* Measurements within the scope of accreditation to ISO 17025.

SAFETY INFORMATION

Precautions need to be taken to avoid injury of the operator by broken specimens when operating the Charpy impact pendulum.

INSTRUCTIONS FOR USE

Samples of ERM-FA013ba correspond with the '(certified) BCR test pieces' as referred to in EN 10045-2 (Method for the verification of impact testing machines), as well as with the 'certified reference test pieces' as defined in ISO 148-3 (Preparation and characterisation of Charpy V reference test pieces for verification of test machines).

The ERM-FA013ba batch is one of the 'Master Batches'. Master Batch test pieces are not for sale. They are intended solely to traceably certify Secondary Batches of the same nominal absorbed energy (here 30 J). The certified value and its associated uncertainty of the Master Batch are used in the calculation of the certified value and combined and expanded uncertainty of a set of 5 specimens from a Secondary Batch.

When characterising a secondary batch, a number of Master Batch test pieces are broken under repeatability conditions together with a selection of samples from the secondary batch. Special attention is drawn to the cleaning and conditioning of the specimens prior to testing. It is mandatory to remove the oil from the sample surface prior to testing, without damaging the edges of the sample. Between the moment of

removing the protective oil layer and the actual test, corrosion can occur. This must be avoided by limiting this period of time, while keeping the sample clean.

The following cleaning and conditioning procedure is considered to be good practice.

1. First use absorbent cleaning-tissue to remove the excess oil. Pay particular attention to the notch of the sample, but do not use hard (e.g. steel) brushes to remove the oil from the notch.
2. Submerge the samples in technically pure ethanol for about 5 minutes. Use of ultrasonication is encouraged, but only if the edges of the samples are prevented from rubbing against each other. To reduce the consumption of solvent, it is allowed to make a first cleaning step with detergent, immediately prior to the solvent step.
3. Once samples are removed from the solvent, only manipulate the samples wearing clean gloves. This is to prevent development of corrosion between the time of cleaning and the actual test.
4. Before testing, bring the specimens to the test temperature (20 ± 2 °C). To assure thermal equilibrium is reached, move the specimens to the test laboratory at least 3 h before the tests.

After cleaning and equilibration, the samples need to be broken with a pendulum impact test machine operated in accordance with EN 10045-1 or ISO 148-1 standards. Prior to the tests, the anvils must be cleaned. It must be noted that Charpy test pieces sometimes leave debris on the Charpy pendulum anvils. Therefore, the anvils must be checked regularly and if debris is found, it must be removed.

For some pendulums and for some samples, post-fracture interaction between broken samples and pendulum hammer can affect the measured KV values. The resulting excessively high values can be related to indentations and deformations of the broken samples. Outlier values that can be related to post-fracture indentation marks on the broken samples must be eliminated from the analysis of the results.

STORAGE

Specimens should be kept at room temperature in their original packing until used. However, the European Commission cannot be held responsible for changes that happen during storage of the material at the customer's premises, especially of opened samples.

LEGAL NOTICE

Neither the European Commission, its contractors nor any person acting on their behalf:

(a) make any warranty or representation, express or implied, that the use of any information, material, apparatus, method or process disclosed in this document does not infringe any privately owned intellectual property rights; or

(b) assume any liability with respect to, or for damages resulting from, the use of any information, material, apparatus, method or process disclosed in this document save for loss or damage arising solely and directly from the negligence of the Institute for Reference Materials and Measurements of the European Commission's Joint Research Centre.

NOTE

A detailed technical report can be obtained from the Joint Research Centre, Institute for Reference Materials and Measurements on request.

European Commission – Joint Research Centre
Institute for Reference Materials and Measurements (IRMM)
Retieseweg 111, B - 2440 Geel (Belgium)
Telephone: +32-(0)14-571.722 - Fax: +32-(0)14-590.406

European Commission

EUR 24531 EN – Joint Research Centre – Institute for Reference Materials and Measurements

Title: Certification of Charpy V-notch Reference Test Pieces of 30 J Nominal Absorbed Energy, ERM[®]-FA013be

Author(s): A. Lamberty, A. Dean, G. Roebben

Luxembourg: Publications Office of the European Union

2010 – 24 pp. – 21.0 x 29.7 cm

EUR – Scientific and Technical Research series – ISSN 1018-5593

ISBN 978-92-79-15631-1

DOI 10.2787/30520

Abstract

This certification report describes the processing and characterisation of ERM[®]-FA013be, a batch of Charpy V-notch certified reference test pieces. Sets of five of these test pieces are used for the verification of pendulum impact test machines according to EN 10045-2 (Charpy impact test on metallic materials, Part 2. Method for the verification of impact testing machines) or according to ISO 148-2 (Metallic materials - Charpy pendulum impact test – Part 2: Verification of test machines).

The certified value for KV (= energy required to break a V-notched test piece using a pendulum impact test machine) is 26.0 J. The associated uncertainty (0.9 J, $k = 2$ corresponding to a confidence level of about 95 %) is calculated for the mean of a set of five test pieces.

The absorbed energy (KV) is procedurally defined and refers to the impact energy required to break a V-notched bar of standardised dimensions, as defined in EN 10045-1 and ISO 148-1. The certified value of ERM[®]-FA013be is traceable to the SI, via the SI-traceable certified value of the master batch ERM[®]-FA013ba, by testing samples of ERM[®]-FA013ba and ERM[®]-FA013be under repeatability conditions on an impact pendulum verified and calibrated with SI-traceably calibrated tools. The certified value is valid only for strikers with a 2 mm tip radius. The certified value is valid at (20 ± 2) °C.

How to obtain EU publications

Our priced publications are available from EU Bookshop (<http://bookshop.europa.eu>), where you can place an order with the sales agent of your choice.

The Publications Office has a worldwide network of sales agents. You can obtain their contact details by sending a fax to (352) 29 29-42758.

The mission of the JRC is to provide customer-driven scientific and technical support for the conception, development, implementation and monitoring of EU policies. As a service of the European Commission, the JRC functions as a reference centre of science and technology for the Union. Close to the policy-making process, it serves the common interest of the Member States, while being independent of special interests, whether private or national.

LA-NA-24531-EN-C

