

Hickey, M., Kyriacou, P. A., Samuels, N., Randive, N., Chang, S. H., Maney, K. & Langford, R. M. (2009). Photoplethysmographic signals recorded from human abdominal organs using a fibreoptic probe. *British Journal of Anaesthesia*, 102(4), 579P-580P. doi: 10.1093/bja/aep007



**CITY UNIVERSITY
LONDON**

[City Research Online](#)

Original citation: Hickey, M., Kyriacou, P. A., Samuels, N., Randive, N., Chang, S. H., Maney, K. & Langford, R. M. (2009). Photoplethysmographic signals recorded from human abdominal organs using a fibreoptic probe. *British Journal of Anaesthesia*, 102(4), 579P-580P. doi: 10.1093/bja/aep007

Permanent City Research Online URL: <http://openaccess.city.ac.uk/13349/>

Copyright & reuse

City University London has developed City Research Online so that its users may access the research outputs of City University London's staff. Copyright © and Moral Rights for this paper are retained by the individual author(s) and/ or other copyright holders. All material in City Research Online is checked for eligibility for copyright before being made available in the live archive. URLs from City Research Online may be freely distributed and linked to from other web pages.

Versions of research

The version in City Research Online may differ from the final published version. Users are advised to check the Permanent City Research Online URL above for the status of the paper.

Enquiries

If you have any enquiries about any aspect of City Research Online, or if you wish to make contact with the author(s) of this paper, please email the team at publications@city.ac.uk.

Photoplethysmographic signals recorded from human abdominal organs using a fibre-optic probe

M. Hickey*, P.A. Kyriacou*, N. Samuels*, N. Randive*, S.H. Chang, K.M. Maney* and
R.M. Langford

Barts and The London NHS Trust and City University, London, UK

There is a need for reliable continuous monitoring of visceral organ oxygen saturation (SpO_2) [1]. Splanchnic ischaemia may contribute to the development of multiple organ failures and increased mortality [2]. In an attempt to develop a suitable abdominal pulse oximeter we have recorded photoplethysmographic (PPG) signals from various abdominal organs to determine their suitability for pulse oximetry.

We constructed a reflectance fibre optic PPG probe. A transmitting fibre illuminated the tissue (using two wavelengths) and backscattered light from the tissues was returned to a photodetector via the detecting fibre. Ethics Committee approval has been obtained to study healthy adults undergoing elective laparotomy. The PPG probe was held for two minutes at each abdominal organ such as the bowel, liver, stomach and kidney. For comparison purposes an identical fibre optic PPG probe was also placed on the finger or toe. Both probes were connected to an electrically isolated processing system, with identical gain for each channel, and signals were displayed on a computer.

Figure 1 shows PPG traces obtained from the liver with the PPG amplitude approximately twice the simultaneous toe PPG. PPG's of good quality were obtained from all investigated organs.

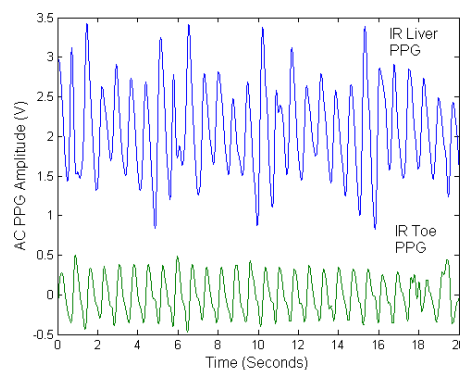


Figure 1: Infrared PPG Traces for the liver and toe

The red and infrared wavelengths used are suitable for pulse oximetry and the PPG amplitudes from the abdominal organs are consistently of good quality and of similar amplitude than those obtained from the extremity. Therefore, the new developed fibre optic PPG probe may well be suitable to estimate arterial oxygen saturation of abdominal organs.

1. Crerar-Gilbert AJ, Kyriacou PA, Jones DP and Langford RM. *Anaesthesia* 2002; 57: 442-445
2. Jury of the Consensus. *Intensive Care Med* 1996; 22: 1250-1257

The authors thank EPSRC for financial support.