

Yang, G., Nawaz, T., Barrick, T. R., Howe, F. A. & Slabaugh, G.G. (2015). Discrete Wavelet Transform-Based Whole-Spectral and Subspectral Analysis for Improved Brain Tumor Clustering Using Single Voxel MR Spectroscopy. *IEEE Transactions on Biomedical Engineering*, 62(12), pp. 2860-2866. doi: 10.1109/TBME.2015.2448232



**CITY UNIVERSITY
LONDON**

[City Research Online](#)

Original citation: Yang, G., Nawaz, T., Barrick, T. R., Howe, F. A. & Slabaugh, G.G. (2015). Discrete Wavelet Transform-Based Whole-Spectral and Subspectral Analysis for Improved Brain Tumor Clustering Using Single Voxel MR Spectroscopy. *IEEE Transactions on Biomedical Engineering*, 62(12), pp. 2860-2866. doi: 10.1109/TBME.2015.2448232

Permanent City Research Online URL: <http://openaccess.city.ac.uk/14029/>

Copyright & reuse

City University London has developed City Research Online so that its users may access the research outputs of City University London's staff. Copyright © and Moral Rights for this paper are retained by the individual author(s) and/ or other copyright holders. All material in City Research Online is checked for eligibility for copyright before being made available in the live archive. URLs from City Research Online may be freely distributed and linked to from other web pages.

Versions of research

The version in City Research Online may differ from the final published version. Users are advised to check the Permanent City Research Online URL above for the status of the paper.

Enquiries

If you have any enquiries about any aspect of City Research Online, or if you wish to make contact with the author(s) of this paper, please email the team at publications@city.ac.uk.

Discrete Wavelet Transform Based Whole-Spectral and Sub-Spectral Analysis for Improved Brain Tumour Clustering using Single Voxel MR Spectroscopy

Guang Yang*, Member, IEEE, Tahir Nawaz, Thomas R. Barrick, Franklyn A. Howe, and Greg Slabaugh, Senior Member, IEEE

Abstract—Many approaches have been considered for automatic grading of brain tumours by means of pattern recognition with magnetic resonance spectroscopy (MRS). Providing an improved technique which can assist clinicians in accurately identifying brain tumour grades is our main objective. The proposed technique, which is based on the discrete wavelet transform (DWT) of whole-spectral or sub-spectral information of key metabolites, combined with unsupervised learning, inspects the separability of the extracted wavelet features from the MRS signal to aid the clustering. In total, we included 134 short echo time single voxel MRS spectra (SV MRS) in our study that cover normal controls, low grade and high grade tumours. The combination of DWT-based whole-spectral or sub-spectral analysis and unsupervised clustering achieved an overall clustering accuracy of 94.8% and a balanced error rate of 7.8%. To the best of our knowledge, it is the first study using DWT combined with unsupervised learning to cluster brain SV MRS. Instead of dimensionality reduction on SV MRS or feature selection using model fitting, our study provides an alternative method of extracting features to obtain promising clustering results.

Index Terms—Brain tumour, glioma grade, clustering, dimension reduction, discrete wavelet transform, magnetic resonance spectroscopy, unsupervised learning.

I. INTRODUCTION

Magnetic resonance imaging (MRI) is a widely-used modality that facilitates the diagnosis and prognosis of brain tumours. Standard MRI sequences are routinely used to differentiate among various brain tumour types based on qualitative visual analyses of the represented soft tissue contrast. Indeed, more than 120 classes of brain tumours are known [1], which are categorised into four grades depending on the level of malignancy by the world health organisation (WHO) [2]. The grading from low to high (I-IV) represents malignancy levels from biologically least aggressive to most aggressive brain tumours as shown by histological criteria, e.g., invasiveness, vascularity, and tumour growth rate [1]. Gliomas are the most common primary brain tumour and

pre-treatment assessment of grade is required; however, the sole use of standard MRI sequences may be insufficient for an accurate diagnosis [3]. The current gold standard for diagnosis of a suspicious abnormal mass is the histopathological analysis of a biopsy sample [4]. However, due to tumour heterogeneity a tumour may be under-graded if the area of greatest malignancy is not selected for biopsy.

Alternatively, in-vivo ^1H magnetic resonance spectroscopy (MRS) can be used to non-invasively inspect the biochemical information of the metabolites present in the living tissue, and can improve characterisation of human brain tumours compared to using standard MRI alone. There are up to 12 different metabolites in the brain that can be measured using ^1H MRS at clinical field strengths of 1.5T or 3T [5]. In particular, single voxel (SV) MRS extracts metabolic information of a specific region of interest (ROI), and it is a unique non-invasive tool to aid classification of human brain tumours with appropriate spectral analysis such as with pattern recognition [6].

Analysis of ^1H MRS data for data clustering and tissue classification generally requires some form of data reduction, either to reduce the noise or extract the most salient features. Mainardi et al. [7] designed a quantification model for in-vivo MRS parameters using the discrete wavelet packet decomposition (WPD). Mahmoodabadi et al. proposed a modified frequency ordered WPD method combined with fuzzy classification framework to analyse pediatric metabolic brain diseases using wavelet transform based features extracted from both MRS and diffusion-weighted imaging [8]. Tiwari et al. investigated combining wavelet (Gabor and Haar filters) features extracted from both T_2 -weighted MRI and MRS modalities, applied to supervised prostate cancer detection [9]. The discrete wavelet transform (DWT) has the advantage of providing multi-resolution discriminatory information [10] from different acquisition modalities, including but not limited to digital signals and images [9]. However, there is very limited research in the literature on fully-automating an unsupervised brain tumour data clustering using DWT based analysis that does not require labelled data or incur possible overfitting during the training procedure.

Here we hypothesise that unsupervised learning based clustering on extracted DWT features can improve brain tumour grading compared to dimension reduction techniques, which are based on second and higher-order statistics (e.g., PCA and ICA) or manifold learning based nonlinear methods (e.g., Laplacian Eigenmaps (LE)). We extract DWT features of the whole-spectra and sub-spectra (as shown in Figure 1), and hypothesise that local information from only a few key metabolites of the sub-spectra is sufficient to distinguish between tumour grades,

This work was supported by CRUK C1459/A13303 and a City University London Pump Priming Grant. Data was originally acquired as part of the EU FP7 eTUMOUR project LSHC-CT-2004-503094. Asterisk indicates corresponding author.

G. Yang is with Neuroscience Research Centre, Cardiovascular and Cell Sciences Institute, St. George's, University of London, Cranmer Terrace, London, U.K., SW17 0RE. (email: gyang@sgul.ac.uk).

T.R. Barrick and F.A. Howe are with Neuroscience Research Centre, Cardiovascular and Cell Sciences Institute, St George's, University of London, Cranmer Terrace, London, U.K., SW17 0RE.

T. Nawaz and G. Slabaugh are with Department of Computer Science, School of Mathematics, Computer Science, and Engineering, City University London, Northampton Square, London, U.K., EC1V 0HB.

because those metabolites exhibit discriminative characteristics for specific tumour grades [6].

To accomplish this, we build a feature vector by using the DWT coefficients of the whole-spectra or by encoding the non-parametric statistics of the computed DWT coefficients of the sub-spectra corresponding to different metabolites. Then in an agglomerative hierarchical clustering framework the MR spectra belonging to different tumour grades are separated. We show the effectiveness of the proposed method on SV MRS data (134 spectra), acquired from normal brain tissue and from low and high grade gliomas. The proposed methods show encouraging performance by achieving an unsupervised clustering accuracy of 94.8% for both whole-spectral and sub-spectral analysis that outperforms our previous analyses of this data. Instead of extracting eigen-decomposed features using dimensionality reduction techniques, this study explores DWT features using whole-spectral and sub-spectral analysis, and obtains promising clustering results for separating different brain tissue types. Section II details the materials and main methods of this study. Section III demonstrates our experimental results followed by elaborated discussions (Section IV) and a conclusion (Section V).

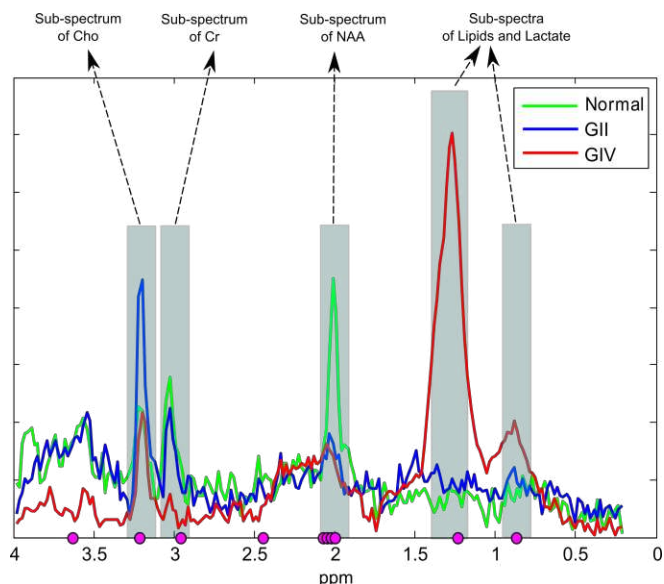


Figure 1: Decomposition of a whole MR spectrum into a set of sub-spectra (sub-regions coloured in cyan) corresponding to different metabolites. Representative Grade II (GII) tumour, Grade IV (GIV) tumour and Normal spectra are shown in blue, red and green colours. The selected features using mRMR are shown with magenta circles.

II. MATERIALS AND METHODS

A. Data Acquisition and Patient Subjects

MR data were obtained at St. George's University of London using a 1.5-Tesla scanner (GE Healthcare, Milwaukee, WI, USA), which was equipped with 22 mT/m gradients and a quadrature head coil. Written informed consent was obtained from all participants in accordance with local ethics procedures. Either biopsy or resected tumour tissue samples obtained as part of the patients' clinical diagnosis or treatment were used to provide a

histological diagnosis of the tumour type and grade as the overall gold standard (ground truth).

In total $N = 134$ SV MRS were obtained including 24 Grade II (GII) tumours (2 oligodendroglioma, 3 oligoastrocytoma, 3 fibrillary astrocytoma, 4 gemistocytic astrocytoma and 12 diffuse astrocytoma) and 31 Grade IV (GIV, glioblastoma multiforme). A further 79 MR spectra were obtained from three normal controls using multiple voxel MRS with the same acquisition parameters (i.e., which had compatible TR/TE) as the SV MRS (Table 1).

TABLE 1
 NUMBER OF PATIENTS STUDIED AND NUMBER OF SPECTROSCOPIC VOXELS ANALYSED FOR EACH TISSUE CLASS.

	Tissue Class			Total
	Normal	Grade II	Grade IV	
Number of Subjects Studied	3	24	31	58
Number of MRS Voxels Analysed	79	24	31	134

All SV MRS data were acquired at short Echo Time (TE) using the GE developed point-resolved spectroscopic sequence (PRESS) protocol (Repetition Time (TR) = 2000ms, Echo time (TE) = 30ms, 2048 data points with 2500Hz bandwidth).

An expert panel (including spectroscopists, pathologists and radiologists) validated the brain tissue types included in this study as part of the eTUMOUR project, with a histopathological diagnosis of the central nervous system (CNS) tumours according to WHO criteria [2]. Individual voxels were placed to encompass predominantly viable tumour tissue as much as possible and avoid areas of pure necrosis. Apodisation in the time domain was performed using a half Hann window followed by a fast Fourier transform and automatic phasing according to [11]. Each spectrum was referenced to both N-acetyl Aspartate (NAA at 2ppm and a search region 2.20ppm – 1.80ppm) and Choline (Cho at 3.21ppm and a search region 3.30ppm – 3.12ppm) for chemical shift alignment, and then truncated to the chemical shift range of 4.0 to 0.2ppm. In addition, the phased real part of the spectra were used for further analysis [12]–[14]. Each whole spectrum consisted of $M = 198$ data points representing the majority of metabolic information.

B. Feature Extraction

All SV MRS data were stored as a 2D matrix, $\mathbf{S} \in \mathbb{R}^{M \times N}$, where $\mathbf{S} = (\mathbf{s}_1, \mathbf{s}_2, \dots, \mathbf{s}_N)$ contains each spectrum as a column vector $\mathbf{s}_n \in \mathbb{R}^M$. The column vectors were L_2 normalised,

$$\mathbf{s}_n^* = \frac{\mathbf{s}_n}{\sqrt{\sum_m s_{nm}^2}} \quad \forall n \in \{1, 2, \dots, N\} \quad (1)$$

to form the matrix $\mathbf{S}^* = \{\mathbf{s}_i^*\}_{i=1}^N$ with $\mathbf{S}^* \in \mathbb{R}^{M \times N}$, which is a set of normalised MR spectra. N is the number of the spectra and M is the number of the data points of each spectrum.

We used the DWT to encode the MR spectral information. For both the whole-spectral and sub-spectral analysis, we compared widely-used wavelet basis functions including Daubechies (Db1, Db2, Db3), Coiflets (Coif1, Coif2, Coif3) and Symlets (Sym1, Sym2, Sym3).

For the whole-spectral analysis, we tested multiple levels (i.e., 1 to 12 levels) of decomposition. At each level of

resolution or octave, the spectral signal \mathbf{s}_i^* is convolved (\otimes) simultaneously with a high-pass filter (φ_h) and a low-pass filter (ψ_l) to obtain the corresponding coefficients (h_c and l_c) as $h_c = (\mathbf{s}_n^* \otimes \varphi_h) \downarrow 2$ and $l_c = (\mathbf{s}_n^* \otimes \psi_l) \downarrow 2$ with the subsampling or decimation (\downarrow) by a factor of 2 after each pass through the paired filters [15]. The feature vectors are computed for all \mathbf{s}_i^* to obtain the feature matrix, of size $134 \times F_L$, in which F_L is the size of the approximation and detail coefficients at different levels $L = 1, 2, \dots, 12$ (Table 2).

For the sub-spectral analysis by given \mathbf{s}_i^* we built the feature vector, \mathbf{f}_i , as follows. We extracted information for the key metabolites by taking the sub-spectra windowed symmetrically around their respective ppms (Figure 1). We performed a mutual information based feature selection (i.e., mRMR, minimum redundancy and maximum relevance method [16]) to identify the key metabolites, which are the most powerful discriminants in terms of separating the three tissue types (Normal, GII and GIV). The only parameter specified in the mRMR method is the number of features, which was set to 10 in order to obtain a moderate sample per feature ratio to avoid overfitting [17]. The mRMR method resulted in 10 selected features (Figure 1) at 3.62, 3.24, 2.99, 2.49, 2.05, 2.03, 2.01, 1.99, 1.19, and 0.85 ppm. For sub-spectral analysis we chose dominant high signal to noise ratio biochemicals [18] whose peak areas are mostly strongly associated with these regions: NAA (main singlet at 2.05 ppm), Cho (3.21 ppm), Creatine (Cr) (3.02 ppm) and lipids and macromolecules (main peaks at 1.3 and 0.9 ppm). The excluded points of 3.62 ppm and 2.49 ppm include strongly overlapping multiplet peaks from Myo-inositol with glutamate and glutamine (Glx) and those from Glx with NAA respectively. Note in high-grade tumours there may also be a contribution from lactate (doublet centred at 1.33 ppm). Boxplots of the five selected features among three different tissue types are shown in Figure 2, and statistical significances were given by two-sample Wilcoxon rank-sum test between each two tissue types (significance level of $p < 0.01$ subject to the Bonferroni correction [19]). In general, NAA and Cr are decreased and Cho increased in tumours

compared to normal brain [20]. Additionally, the Lipid and lactate signal observable at short TE increase with tumour grade [20]. The sub-spectra for NAA, Cho, Cr, Lipid (0.9 ppm) and Lipid and Lactate (1.3 ppm) were denoted as \mathbf{s}_i^{*NAA} , \mathbf{s}_i^{*Cho} , \mathbf{s}_i^{*Cr} , \mathbf{s}_i^{*Lip1} , and \mathbf{s}_i^{*Lip2} , respectively. The window sizes for each \mathbf{s}_i^* were fixed and denoted as w^{NAA} , w^{Cho} , w^{Cr} , w^{Lip1} , and w^{Lip2} , respectively. We applied the DWT using the single-level implementation of Mallat's approach [10] on each of the \mathbf{s}_i^{*NAA} , \mathbf{s}_i^{*Cho} , \mathbf{s}_i^{*Cr} , \mathbf{s}_i^{*Lip1} , and \mathbf{s}_i^{*Lip2} signals to obtain the corresponding set of (approximation and detail) coefficients \mathbf{D}_i^{NAA} , \mathbf{D}_i^{Cho} , \mathbf{D}_i^{Cr} , \mathbf{D}_i^{Lip1} , \mathbf{D}_i^{Lip2} , respectively. The higher levels of decomposition were not needed given the smaller sub-spectra window sizes compared to the whole-spectral analysis, and single-level decomposition was expected to be sufficient to effectively capture the frequency information.




Figure 2: Boxplot of the five selected features among three tissue types (Normal: green; GII: blue; GIV: red). Red circled dots are the outliers of each group (***) indicates $p < 0.0001$ and ** indicates $p < 0.001$.

The choice of the window sizes (w) for different metabolites can influence the performance of the system. In addition, the window size must be kept small to avoid

TABLE 2

PARAMETER SETTINGS OF THE DWT METHOD USING WHOLE-SPECTRAL ANALYSIS AND SUB-SPECTRAL ANALYSIS (WBF: WAVELET BASIS FUNCTIONS; LD: LEVEL OF DECOMPOSITION). BOLD TEXT INDICATES THE BEST PARAMETER SETTINGS.

Whole-spectral	WF	LD	Accuracy (Mean \pm Standard Deviation)	Best Accuracy (with WF and LD Settings)
Daubechies (DbAll)	Db1	[1-12]	83.1% \pm 1.6%	94.8% (with Db1 and 7 levels of decomposition)
	Db2	[1-12]	82.5% \pm 2.1%	
	Db3	[1-12]	78.3% \pm 2.5%	
Coiflets (CoifAll)	Coif1	[1-12]	81.0% \pm 2.5%	94.8% (with Coif1 and 6 levels of decomposition)
	Coif2	[1-12]	83.2% \pm 1.6%	
	Coif3	[1-12]	79.8% \pm 2.2%	
Symlets (SymAll)	Sym1	[1-12]	83.2% \pm 1.6%	92.5% (with Sym1 and 7 or 9 levels of decomposition)
	Sym2	[1-12]	83.2% \pm 1.6%	
	Sym3	[1-12]	83.1% \pm 1.6%	

Sub-spectral	WF	LD	Window Sizes for Each Metabolite	Best Accuracy (with WF and WS)
Daubechies	Db1	1	$\omega = [0.02\text{ppm}, 0.04\text{ppm}, \dots, 0.28\text{ppm}, 0.30\text{ppm}]$	94.8% (with Coif1 and $\omega^{NAA}=0.16\text{ppm}$, $\omega^{Cho}=0.16\text{ppm}$, $\omega^{Cr}=0.04\text{ppm}$, $\omega^{Lip1}=0.18\text{ppm}$, and $\omega^{Lip2}=0.20\text{ppm}$)
	Db2	1		
	Db3	1		
Coiflets	Coif1	1	$\omega = [0.02\text{ppm}, 0.04\text{ppm}, \dots, 0.28\text{ppm}, 0.30\text{ppm}]$	94.8% (with Coif1 and $\omega^{NAA}=0.16\text{ppm}$, $\omega^{Cho}=0.16\text{ppm}$, $\omega^{Cr}=0.04\text{ppm}$, $\omega^{Lip1}=0.18\text{ppm}$, and $\omega^{Lip2}=0.20\text{ppm}$)
	Coif2	1		
	Coif3	1		
Symlets	Sym1	1	$\omega = [0.02\text{ppm}, 0.04\text{ppm}, \dots, 0.28\text{ppm}, 0.30\text{ppm}]$	94.8% (with Coif1 and $\omega^{NAA}=0.16\text{ppm}$, $\omega^{Cho}=0.16\text{ppm}$, $\omega^{Cr}=0.04\text{ppm}$, $\omega^{Lip1}=0.18\text{ppm}$, and $\omega^{Lip2}=0.20\text{ppm}$)
	Sym2	1		
	Sym3	1		

overlap between of adjacent metabolites, and we also need enough data points for further data clustering. We analysed the effect of the variation that $w = [0.02\text{ppm}, 0.04\text{ppm}, \dots, 0.28\text{ppm}, 0.30\text{ppm}]$, i.e., 15 sets of window sizes $[-0.01\text{ppm}, 0.01\text{ppm}]$, $[-0.02\text{ppm}, 0.02\text{ppm}]$, ..., $[-0.14\text{ppm}, 0.14\text{ppm}]$, $[-0.15\text{ppm}, 0.15\text{ppm}]$ around each peak of the metabolites) with respect to clustering performance (Table 2). The window size for each metabolite was varied in turn with the window sizes of the remaining metabolites kept fixed, and inherent to this process is the assumption that the window sizes are independent in terms of optimisation. The first key metabolite was Cho (centred at 3.21ppm) and the window was varied with window size for the other metabolites fixed at the initial smallest value. Subsequently, the window sizes for Cr centred at 3.02 ppm, NAA at 2 ppm, Lip2 at 1.3 ppm, and Lip1 at 0.9ppm were optimized in turn.

Inspired by [21], we further encapsulated the distribution of the computed DWT coefficients non-parametrically for a metabolite, e.g., NAA, as follows:

$$\mathbf{f}_i^{\text{NAA}} = \{\min(\mathbf{D}_i^{\text{NAA}}), Q_{25}(\mathbf{D}_i^{\text{NAA}}), Q_{50}(\mathbf{D}_i^{\text{NAA}}), Q_{75}(\mathbf{D}_i^{\text{NAA}}), \max(\mathbf{D}_i^{\text{NAA}})\}, \quad (2)$$

where $\mathbf{f}_i^{\text{NAA}}$ denotes the feature vector that encodes the non-parametric statistics for the DWT coefficients ($\mathbf{D}_i^{\text{NAA}}$) of $\mathbf{s}_i^{\text{NAA}}$ using the minimum coefficient value ($\min(\mathbf{D}_i^{\text{NAA}})$), 25th percentile ($Q_{25}(\mathbf{D}_i^{\text{NAA}})$), 50th percentile ($Q_{50}(\mathbf{D}_i^{\text{NAA}})$), 75th percentile ($Q_{75}(\mathbf{D}_i^{\text{NAA}})$), and the maximum coefficient value ($\max(\mathbf{D}_i^{\text{NAA}})$). $\mathbf{f}_i^{\text{NAA}}$ comprehensively captures the information of $\mathbf{s}_i^{\text{NAA}}$ by encoding the overall distribution of its coefficients [21]. Similarly to Equation 2, the feature vectors for $\mathbf{s}_i^{\text{Cho}}$, \mathbf{s}_i^{Cr} , $\mathbf{s}_i^{\text{Lip1}}$, and $\mathbf{s}_i^{\text{Lip2}}$ can be computed and denoted as \mathbf{f}_i^{Cr} , $\mathbf{f}_i^{\text{Cho}}$, $\mathbf{f}_i^{\text{Lip1}}$, $\mathbf{f}_i^{\text{Lip2}}$, respectively. The feature vector, \mathbf{f}_i , is therefore defined as follows:

$$\mathbf{f}_i = \{\mathbf{f}_i^{\text{NAA}}, \mathbf{f}_i^{\text{Cho}}, \mathbf{f}_i^{\text{Cr}}, \mathbf{f}_i^{\text{Lip1}}, \mathbf{f}_i^{\text{Lip2}}\}, \quad (3)$$

and \mathbf{f}_i is a 25-dimensional row vector. Using Equation 3 the feature vectors are computed for all \mathbf{s}_i^* to obtain the feature matrix, of size 134×25 .

Unsupervised learning based hierarchical clustering is then performed on the feature matrix extracted using whole-spectral or sub-spectral analysis as described below.

C. Data Clustering

To quantitatively validate and compare the efficacy of our DWT based feature extraction method to previous studies, we applied agglomerative hierarchical clustering algorithms to the feature extraction outputs. Compared to widely used

k-means clustering, hierarchical clustering requires no initialisation settings, and thus can avoid possible local minima that could trap the k-means algorithm.

For hierarchical clustering a dissimilarity measure was specified (the Euclidean distance) between disjoint groups of observations according to pairwise dissimilarities between the observations in the two groups. An agglomerative (i.e., bottom-up) paradigm was used which recursively merges pairs of clusters into a single cluster at each level [22]. Pairs were merged based on the smallest inter-group dissimilarity and representation of the recursive binary agglomeration was achieved using dendrograms (i.e., rooted binary trees).




Figure 3: Comparison between different wavelet basis functions in terms of the obtained clustering accuracy (A) for both whole-spectral and sub-spectral analysis. Error bars represent the standard error of the mean (SEM). For the whole-spectral analysis, SEM was calculated with respect to different decomposition levels. For the sub-spectral analysis, SEM was computed with respect to various window sizes. Circles above the error bars indicate the maximum accuracy achieved by different wavelet basis functions.

D. Performance Assessment

We evaluated the performance of the proposed method from a clinical point of view using the following measures: precision (P), recall/sensitivity (R), F-score (F) and clustering accuracy (A). $P = \frac{TP}{TP+FP}$ where TP and FP are the number of true positives (correct estimations) and false positives (incorrect estimations). $R = \frac{TP}{TP+FN}$ where FN is the number of false negatives (missed estimations). In addition, $F = 2 \frac{P \times R}{P+R}$. Furthermore, A provides the overall clustering accuracy as a ratio of the number of correct clustering (N_{Correct}) and total number of input spectra (N) that is $A = \frac{N_{\text{Correct}}}{N}$. P, R, F and $A \in [0,1]$, and the higher

TABLE 3
PERFORMANCE COMPARISON OF THE PROPOSED DWT METHOD (WHOLE-SPECTRAL ANALYSIS USING COIF1 WITH 6 LEVELS OF DECOMPOSITION OR SUB-SPECTRAL ANALYSIS USING COIF1 WITH 1 LEVEL OF DECOMPOSITION) WITH PCA, PCA+ICA AND NONLINEAR LE METHODS.

Method	Brain Tissue Types	Predicted Group Membership			Precision (P)	Recall (R)	F-Score (F)	Accuracy (A)	Silhouette Statistics ($\mu_{sw} \pm \sigma_{sw}$)	BER
		Normal	GII	GIV						
PCA	Normal	71	8	0	1.00	0.90	0.95	0.873	0.521±0.230	0.140
	GII	0	21	3	0.60	0.88	0.71			
	GIV	0	6	25	0.89	0.81	0.85			
PCA+ICA	Normal	79	0	0	1.00	1.00	1.00	0.933	0.551±0.213	0.106
	GII	0	21	3	0.78	0.88	0.82			
	GIV	0	6	25	0.89	0.81	0.85			
LE	Normal	79	0	0	1.00	1.00	1.00	0.933	0.612±0.201	0.106
	GII	0	21	3	0.78	0.88	0.82			
	GIV	0	6	25	0.89	0.81	0.85			
DWT	Normal	79	0	0	1.00	1.00	1.00	0.948	0.743±0.278	0.078
	GII	0	23	1	0.79	0.96	0.87			
	GIV	0	6	25	0.96	0.81	0.88			

P, R, F and A , the better the performance. In addition, we also calculated the balanced error rate [23] (BER), which is the average of the errors on each class, and is suitable for unbalanced datasets.

We also evaluated the discriminative ability of the feature vector, \mathbf{f}_i , in terms of quantifying intra-cluster tightness and inter-cluster separability. To this end we used the silhouette statistics that is computed for the i -th data point as follows [24]: $sw_i = \frac{(b_i - a_i)}{\max(a_i, b_i)} \in [-1, 1]$, where a_i is the average distance of the i -th data point to the remaining points within the same cluster and b_i is the minimum average distance of the i -th data point to any of the remaining clusters. We used the mean (μ_{SW}) and the standard deviation (σ_{SW}) of sw_i values as performance indicators. Higher μ_{SW} with lower σ_{SW} indicate better partitioning of the clustering results and hence the better discriminative ability of the feature used. $\mu_{SW} > 0.5$ indicates a proper partitioning whereas $\mu_{SW} < 0.2$ indicates an improper partitioning [24].

III. RESULTS

Figure 3 shows the comparison of the widely-used wavelet basis functions based on the clustering accuracy (A) for both whole-spectral and sub-spectra analysis. Examples of using Daubechies (Db1, Db2, Db3), Coiflets (Coif1, Coif2, Coif3) and Symlets (Sym1, Sym2, Sym3) of the whole spectra are shown as DbAll, CoifAll and SymAll. For the whole spectra, we tested multiple levels of decomposition with standard error of the mean (SEM) shown in the Figure 3. The minimum accuracy (40.3%) was obtained using Coif1 with 3 levels of decomposition while the maximum accuracy (94.8%) was achieved by Coif1 using 6 levels or Db1 using 7 levels of decomposition (Table 2). The Coif1 basis function achieved the highest clustering accuracy with a low level of decomposition, hence this represents the best option for the whole-spectral analysis. In addition, for the sub-spectral analysis, we display the SEM with respect to various window sizes (Figure 3). We tested different values for w^{NAA} , w^{Cho} , w^{Cr} , w^{Lip1} , and w^{Lip2} as aforementioned to maximise clustering accuracy for each wavelet basis function. In so doing, we obtained the best clustering accuracy (94.8% in Table 2) using the Coif1 basis function with window sizes found to be $w^{NAA} = 0.16\text{ppm}$, $w^{Cho} = 0.16\text{ppm}$, $w^{Cr} = 0.04\text{ppm}$, $w^{Lip1} = 0.18\text{ppm}$ and $w^{Lip2} = 0.20\text{ppm}$, respectively. The whole-spectral analysis (using Coif1 basis function with 6 levels of decomposition) and sub-spectral analysis (using Coif1 with 1 level of decomposition) performed identically (Table 2). For the whole-spectral analysis, clustering accuracies obtained by the Coif1 basis function with different decomposition levels showed no significant difference compared to the results of using the Db1 basis function, but showed significant differences compared to the results of other basis functions. For the sub-spectral analysis, clustering accuracies obtained by the Coif1 basis function with various window sizes showed significant differences compared to the results of using other basis functions (Non-parametric Kruskal-Wallis test with Dunn's multiple comparisons was performed with a significance level of $p < 0.05$).

Comparison results between DWT and other methods are provided quantitatively (Table 3). From a clinical point of view, the whole (6 levels of decomposition) and sub-spectral (1 level of decomposition) DWT method using Coif1 (from this point onwards referred to as the proposed DWT method with the best settings as seen in Table 2) showed the best performance for GII, GIV and Normal spectra, as reflected by its highest precision (P), recall (R) and F-score (F) values (Table 3). For the case of Normal spectra, PCA+ICA, LE and the proposed DWT method obtained $P = R = 1$ meaning that all of the Normal spectra were perfectly separated without any false positives ($FP = 0$) and false negatives ($FN = 0$). PCA also obtained a precision of 1 but its recall rate of $R = 0.9$ is lower, as it misclassified 8 Normal spectra ($FN = 8$). For the case of GIV spectra, PCA, PCA+ICA and LE produce $FP = 3$ each with $P = 0.89$. The proposed DWT method produced $FP = 1$ and thus resulted in a better $P = 0.96$. On the other hand, all methods missed 6 GIV spectra with $R = 0.81$. For the case of GII spectra, the proposed DWT method outperformed the remaining methods both in terms of precision and recall. This method produced the least number of incorrect classifications ($N - N_{\text{Correct}} = 7$) thus obtaining the best A (Table 3), but incorrectly classified one GII spectrum as a GIV spectrum, and six GIV spectra as GII spectra. In this case, the incorrect clustering of GIV spectra in the GII cluster, show spectral characteristics that make it non-trivial to distinguish them as GIV spectra. Moreover, the proposed DWT method showed the highest $\mu_{SW} = 0.743$, demonstrating better separability of clusters of the feature, \mathbf{f}_i , than for those extracted using PCA, PCA+ICA and LE methods (Table 3). In terms of σ_{SW} LE shows the smallest variation in the silhouette values (Table 3).

IV. DISCUSSION

Overall, the experimental results suggest that our wavelet based feature extraction (by whole-spectral or sub-spectral analysis) and clustering provides the maximum accuracy of 94.8% for tissue separation, which demonstrates an improvement compared to the PCA, PCA+ICA, and nonlinear LE methods. In addition, our accuracies for distinguishing GII from GIV tumours using DWT and hierarchical clustering compares well to the results of Garcia-Gomez et al. [25], who achieved 92.58% accuracy for distinguishing low from high grade gliomas by combining data from SV long echo and short echo data, which would be difficult to routinely achieve with MRS acquisitions due to time limits for patient scanning. A more recent approach [26] used Non-negative Matrix Factorisation (NMF) to accomplish the feature extraction task for SV tumour spectra. However, NMF methods inevitably converge to local minima and various initialisations provide different dimensionality reduction; therefore, NMF requires an elaborate initialisation scheme as discussed in previous investigation [26]. In addition, we achieved similar BER (0.078 in Table 2) using an unsupervised learning based clustering as Ortega-Martorell

et al. [26] obtained with a supervised learning based framework. The short echo SV MRS data used in the current study is a subset of the INTERPRET and eTUMOUR project data used in [25] and [26] and are compatible for acquisition parameters and ground truth diagnosis from the histopathological and clinical information.

Interestingly, our results on whole spectra showed large variance of the clustering accuracy with respect to different decomposition levels. The decomposition of the MRS signals using multiple levels of resolution present with much larger variance in accuracy compared to the sub-spectra analysis while varying the window sizes. Suggesting sub-spectral DWT analysis may be more stable. In addition, average results of using different basis functions of the sub-spectral analysis are superior to the average results of using the whole spectra (Figure 3). However, the maximum clustering accuracy determined from the whole spectra is 94.8% using the Coif1 basis function and 6 levels of decomposition, which is still superior to PCA, PCA+ICA and nonlinear LE methods. Nevertheless, the minimum clustering accuracy is 40.3% using Coif1 basis function with 3 levels of decomposition indicating that DWT analysis on whole spectra is unstable with respect to decomposition levels.




Figure 4: (a) FLAIR image of the misclassified GII case; (b) T2-weighted image of one misclassified GIV case; (c) Blue curve: SV MRS signal of (a); (d) Blue curve: SV MRS signal of (b); Planned SV MRS acquisitions are shown in cyan boxes overlaid on structural MRI images.

The improvement provided by the proposed DWT method is a better separation between GII and GIV tumours. There is one misclassified GII spectrum as GIV (Figure 4(a) and (c)), and 6 misclassified GIV as GII (one example shown in Figure 4(b) and (d)). The one misclassified GII spectrum has unexpectedly high peaks of Lipid (Figure 4(c)). In contrast, all misclassified GIV spectra have very low Lipid signal, and so resemble GII spectra. The misclassification of these tumour spectra may be due to the fact that our ground truth

is defined by local biopsy or resected tumour samples that do not accurately represent the tissue that has been investigated by MRS. The tumour biopsy samples used for histopathology have typical volumes in mm^3 , whereas the SV MRS data are acquired from a volume in cm^3 [14]. In particular, the highest grade tumour cells observed in the biopsy determine the clinical assignment of tumour grade and may only represent a small proportion of the tissue in the MRS voxel. Additionally GIV tumours are frequently large heterogeneous masses that have areas of low-grade appearance by ^1H MRS [27], and the most malignant region may not have been sampled by a single voxel placement.

Our analysis may have some potential limitations. As aforementioned, the whole-spectral analysis suffers from large variance of the clustering accuracy when decomposition levels of the DWT are varied. For the sub-spectral analysis, we rely upon pre-definition of the key biochemical peaks, which require elaborate tuning prior to application of DWT. However, once the window sizes are fixed, more SV MRS data (i.e., more normal, GII, and GIV SV MRS data) may be added without retuning. In addition, there may be diagnostically useful contributions to the spectra from biochemicals with lower overall visibility. For example quantified levels of myo-inositol, glutathione, glutamate-glutamine have been used in previous tumour classification studies, metabolites whose major contributions to an MR spectrum are outside of our selected spectral regions [13], [18]. Our selection of five key biochemical used in this study may have certain subjectivity. Nevertheless, these metabolites and lipid peaks are well known and widely used, features to discriminate brain tumour grades. For example, Opstad et al. [18] indicated that Choline, Creatine, Lactate and Lipid (1.3 ppm) were the most discriminative for GII and GIV tumour, and NAA and Lipid (0.9 ppm) were useful for classifying normal spectra. Moreover, we only included GII and GIV patients for this study due to lack of reliable GIII MRS data. However, we can envisage a straightforward application of the current DWT based feature extraction and unsupervised clustering framework for SV MRS dataset incorporating GIII cases.

V. CONCLUSIONS

To the best of our knowledge, this is the first study using DWT and unsupervised clustering to separate SV MRS data from different brain tumour types. We tested both DWT based whole-spectral and sub-spectral analysis, and we have concluded that a sub-spectral analysis is sufficient by using windowed key metabolites to distinguish different grades of the brain tumour. The achievement is threefold: (a) we compared different DWT settings including various wavelet basis functions for both whole-spectral and sub-spectral analysis, different window sizes for the sub-spectral analysis, and multiple levels of decomposition for the whole-spectral analysis, and we have found that Coif1 wavelet obtained the best clustering results; (b) we compared DWT based sub-spectral analysis with DWT feature extraction on the whole spectra. Quantitative evidence show that our sub-spectral analysis is more stable irrespective of the window

sizes selected for the key metabolites; (c) we also compared to conventional feature extraction methods such as PCA, PCA+ICA, and newly applied nonlinear LE algorithm, and the comparison demonstrated that both our DWT based whole-spectral and sub-spectral analysis can further improve the separation between GII and GIV tissue types while maintaining the accuracy of separating tumour spectra from normal brain spectra in controls. In summary, our DWT based feature extraction and hierarchical clustering produces promising brain tumour classification that has potential for analysis of larger multi-centre datasets and be applicable to automated analysis of the large datasets obtained in multivoxel ^1H MRS using chemical shift imaging.

REFERENCES

- [1] V. P. Collins, "Brain tumours: classification and genes," *J. Neurol. Neurosurg. Psychiatry*, vol. 75, no. suppl_2, pp. ii2–ii11, Jun. 2004.
- [2] D. N. Louis et al., "The 2007 WHO classification of tumours of the central nervous system.," *Acta Neuropathol.*, vol. 114, no. 2, pp. 97–109, Aug. 2007.
- [3] J. Faehndrich et al., "Neuroradiological viewpoint on the diagnostics of space-occupying brain lesions.," *Clin. Neuroradiol.*, vol. 21, no. 3, pp. 123–39, Sep. 2011.
- [4] M. Caulo et al., "Data-driven Grading of Brain Gliomas: A Multiparametric MR Imaging Study," *Radiology*, vol. 272, no. 2, 2014.
- [5] R. de Graaf, *In vivo NMR spectroscopy*, 2nd Ed. John Wiley & Sons, Ltd., 2007.
- [6] A. Devos et al., "Classification of brain tumours using short echo time ^1H MR spectra," *J. Magn. Reson.*, vol. 170, no. 1, pp. 164–175, Sep. 2004.
- [7] L. T. Mainardi et al., "A wavelet packets decomposition algorithm for quantification of in vivo (^1H) -MRS parameters.," *Med. Eng. Phys.*, vol. 24, no. 3, pp. 201–8, Apr. 2002.
- [8] S. Z. Mahmoodabadi et al., "A Novel m CAD for pediatric metabolic brain diseases incorporating DW imaging and MR spectroscopy," *Expert Syst.*, vol. 30, no. 1, pp. 21–33, Feb. 2013.
- [9] P. Tiwari et al., "Multimodal wavelet embedding representation for data combination (MaWERiC): integrating magnetic resonance imaging and spectroscopy for prostate cancer detection.," *NMR Biomed.*, vol. 25, no. 4, pp. 607–19, Apr. 2012.
- [10] S. Mallat, "A theory for multiresolution signal decomposition: the wavelet representation," *Pattern Anal. Mach. Intell. IEEE*, vol. I, no. 7, pp. 674–693, 1989.
- [11] L. Chen et al., "An efficient algorithm for automatic phase correction of NMR spectra based on entropy minimization," *J. Magn. Reson.*, vol. 158, no. 1–2, pp. 164–168, Sep. 2002.
- [12] G. Yang et al., "Nonlinear Laplacian Eigenmaps Dimension Reduction of in-vivo Magnetic Resonance Spectroscopic Imaging Analysis," in *International Society for Magnetic Resonance in Medicine (ISMRM) 21st Annual Meeting*, 2013, p. 1967.
- [13] G. Yang et al., "Classification of Brain Tumour ^1H MR Spectra : Extracting Features by Metabolite Quantification or Nonlinear Manifold Learning?," in *Biomedical Imaging (ISBI), 2014 IEEE 11th International Symposium on. IEEE*, 2014, pp. 1039–1042.
- [14] G. Yang et al., "Manifold Learning in MR Spectroscopy using Nonlinear Dimensionality Reduction and Unsupervised Clustering," *Magn. Reson. Med.*, pp. 1039–1042, 2014.
- [15] M. Weeks, *Digital Signal Processing Using MATLAB and Wavelets*, 2nd editio. Jones & Bartlett Learning, 2010, pp. 271–343.
- [16] H. Peng et al., "Feature selection based on mutual information criteria of max-dependency, max-relevance, and min-redundancy," *Pattern Anal. Mach. Intell. IEEE Trans.*, vol. 27, no. 8, pp. 1226–1238, 2005.
- [17] R. L. Somorjai et al., "Class prediction and discovery using gene microarray and proteomics mass spectroscopy data: curses, caveats, cautions," *Bioinformatics*, vol. 19, no. 12, pp. 1484–1491, Aug. 2003.
- [18] K. S. Opstad et al., "Linear discriminant analysis of brain tumour ^1H MR spectra: a comparison of classification using whole spectra versus metabolite quantification," *NMR Biomed.*, vol. 20, no. 8, pp. 763–770, 2007.
- [19] H. Abdi, "The Bonferonni and Šidák Corrections for Multiple Comparisons," in *Encyclopedia of Measurement and Statistics*, 1st ed., N. J. Salkind, Ed. SAGE Publications, Inc, 2007, pp. 103–107.
- [20] F. A. Howe and K. S. Opstad, " ^1H MR spectroscopy of brain tumours and masses," *NMR Biomed.*, vol. 16, no. 3, pp. 123–131, May 2003.
- [21] T. Nawaz et al., "Trajectory clustering for motion pattern extraction in aerial videos," in *Proc. of IEEE Int. Conference on Image Processing*, 2014.
- [22] W. Press et al., "Section 16.4. Hierarchical Clustering by Phylogenetic Trees," in *Numerical Recipes: The Art of Scientific Computing*, New York: Cambridge University Press, 2007, pp. 868–881.
- [23] Y. Chen and C. Lin, "Combining SVMs with various feature selection strategies," in *Feature Extraction: Foundations and Applications*, I. Guyon, M. Nikravesh, S. Gunn, and L. A. Zadeh, Eds. Springer Berlin Heidelberg, 2006, pp. 315–324.
- [24] P. J. Rousseeuw, "Silhouettes: A graphical aid to the interpretation and validation of cluster analysis," *J. Comput. Appl. Math.*, vol. 20, pp. 53–65, Nov. 1987.
- [25] J. García-Gómez et al., "On the use of long TE and short TE SV MR spectroscopy to improve the automatic brain tumor diagnosis," *Technical Report*, Katholieke University Leuven, 2007.
- [26] S. Ortega-Martorell et al., "Non-negative matrix factorisation methods for the spectral decomposition of MRS data from human brain tumours.," *BMC Bioinformatics*, vol. 13, no. 1, p. 38, Jan. 2012.
- [27] F. Raschke et al., " ^1H 2D MRSI tissue type analysis of gliomas.," *Magn. Reson. Med.*, vol. 73, no. 4, pp. 1–9, Jun. 2014.