




# SRF

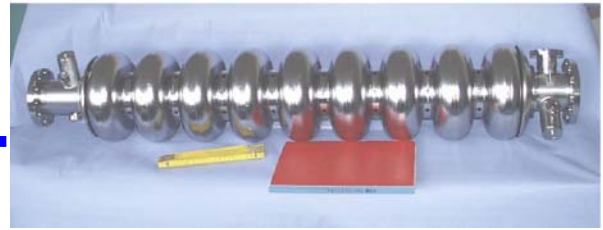

## FURTHER IMPROVEMENTS WITH DRY-ICE CLEANING ON SRF-CAVITIES

Arne Brinkmann, Jens Iversen, Detlef Reschke, Jörg Ziegler DESY D-22603  
Hamburg/Germany

### Abstract

Looking for advanced potentials to clean surfaces of superconducting accelerator cavities, a dry-ice cleaning method promises to be a useful additional application to the standard high pressure rinsing with ultra pure water. Dry-ice cleaning using the sublimation-impulse method removes particles and film contaminations, especially carbonhydrates, without residues. First cleaning tests on single-cell cavities showed Q-values at low fields up to  $4 \times 10^{10}$  at 1.8 K. Gradients up to  $E_{\text{acc}} = 33$  MV/m were achieved, but field emission still is the limiting effect. Further tests are planned to optimize the dry-ice cleaning technique.

Contribution to the SRF 2005, Ithaca, New York, USA

Work supported by the European Community-Research Infrastructure Activity under the FP6 "Structuring the European Research Area" programme (CARE, contract number RII3-CT-2003-506395).

## FURTHER IMPROVEMENTS WITH DRY-ICE CLEANING ON SRF-CAVITIES

Arne Brinkmann<sup>#</sup>, Jens Iversen, Detlef Reschke, Jörg Ziegler  
DESY D-22603 Hamburg/Germany

### Abstract

Looking for advanced potentials to clean surfaces of superconducting accelerator cavities, a dry-ice cleaning method promises to be a useful additional application to the standard high pressure rinsing with ultra pure water.

Dry-ice cleaning using the sublimation-impulse method removes particles and film contaminations, especially carbonhydrates, without residues. First cleaning tests on single-cell cavities showed Q-values at low fields up to  $4 \times 10^{10}$  at 1.8 K. Gradients up to  $E_{acc} = 33$  MV/m were achieved, but field emission still is the limiting effect. Further tests are planned to optimize the dry-ice cleaning technique.

### INTRODUCTION

Although many improvements of cavity preparation procedures had been done, enhanced field emission still limits the high gradient of superconducting cavities.[1] Advanced final cleaning steps and handling procedures must be applied to avoid surface contaminations like particles and hydrocarbons etc. High pressure rinsing with ultra pure water is a powerful method to reduce enhanced field emission, but dry-ice cleaning might have additional cleaning potential. Dry-ice cleaning avoids a wet cavity surface, removes carbonhydrates and is applicable to ceramics, so the possibility to clean a cavity with power couplers is given. First tests on flat Nb samples and on single-cell cavities [2] showed promising results, so that additional improvements on the dry-ice cleaning apparatus had been installed.

### DRY-ICE CLEANING

A jet of pure carbon dioxide snow is able to remove different types of surface contaminations, by a combination of mechanical, thermal and chemical effects. Relaxation of liquid CO<sub>2</sub> in a nozzle (Figs.1 - 2), results in a snow/gas mixture with app. 45 % snow with a temperature of 194.3 K. In addition a supersonic jet of N<sub>2</sub> surrounds the CO<sub>2</sub>-jet so that an acceleration and focussing of the jet is given. Furthermore the N<sub>2</sub> prevents condensation of humidity on the cavity surface. The mechanical cleaning effect is based on shock-freezing of the contaminations, strong impact of the snow crystals and a 500 times increasing of volume after sublimation. Contaminations gets brittle and start to flake off from the surface. When snow particles hits the surface and melts at the point of impact, the chemical cleaning effect occurs.

Liquid CO<sub>2</sub> is a good solvent especially for hydrocarbons and silicons. Achieving an optimal cleaning process, it is necessary to reach a high thermal gradient between jet and surface. Furthermore an exhaust system is needed to carry out contaminations. Basic cleaning parameters are shown in Table 1.

Table 1: Dry ice cleaning parameters

CO <sub>2</sub> -pressure	~ 50 bar
N <sub>2</sub> -pressure	12 – 18 bar
Particle filtration	< 0.05 μm
Temp. of liquid CO <sub>2</sub>	-5° - -40° C
Environment of cleaning	Laminar flow class 10



Figure 1: Nozzle inside a cavity

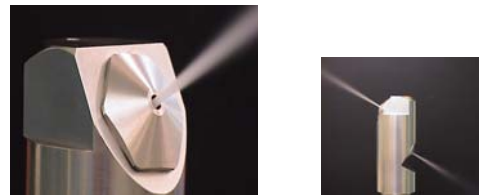


Figure 2: Nozzle system

### IMPROVEMENTS

- Applying dry ice cleaning as final preparation step, a horizontal orientation of a cavity during cleaning is necessary. Also cleaning of multicell cavities in the future will be much easier. Room-height is not a limiting factor. In the new apparatus the cavity therefore is installed horizontally.

<sup>#</sup> arne.brinkmann@desy.de

- A new liquifier with more capacity is installed. The approved maximum temperature of  $-5^{\circ}\text{C}$  can be kept. Cooldown-time is now not longer than 15 minutes (before  $> 1\text{h}$ ).
- To ensure a high thermal gradient, a heating-system with IR-heaters is installed. Without any heaters water will freeze on the outer cavity-surface in a very short time.
- Temperature of cavity, concentration of  $\text{CO}_2$  in room-air and exhaust is now monitored and will in future be controlled by software.

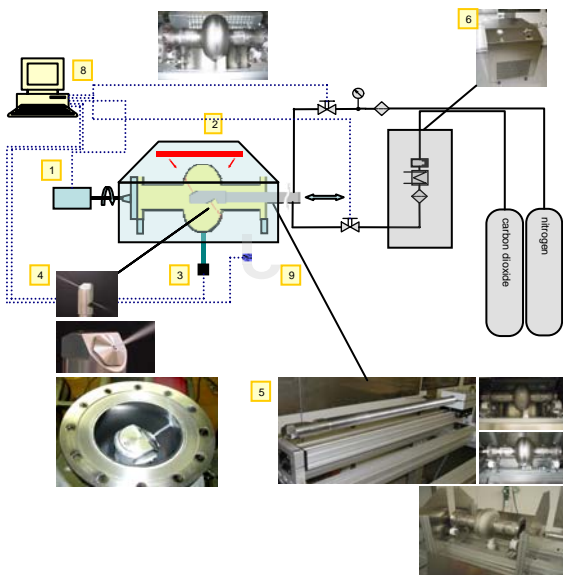


Figure 3: Schematic layout

Figure 3 shows some new objects which have been installed. Infrared-Heater (2), Infrared-Temp.Sensor (3), horizontal nozzle system (4,5), new liquifier (6), motion control and monitoring (8), exhaust of  $\text{N}_2$  and  $\text{CO}_2$  (9).

### CAVITY TEST RESULT

All RF-tests show typical  $Q$ -values above  $10^{10}$  at 2 K for superconducting cavities at 1.3 GHz. The highest  $Q$ -value of  $4 \times 10^{10}$  at 1.8 K indicates that almost no surface contamination is caused by dry-ice cleaning. Gradients up to  $E_{\text{acc}} = 33\text{MV/m}$  are achieved, but still more optimisation of cleaning process and handling procedures has to be done to reduce field emission, which still is the limiting effect. Fig. 4 shows RF-test results of a 1-cell cavity before and after cleaning with the improved

apparatus. Between the tests the cavity was stored under air for several month and no high pressure water rinsing was applied to the cavity.

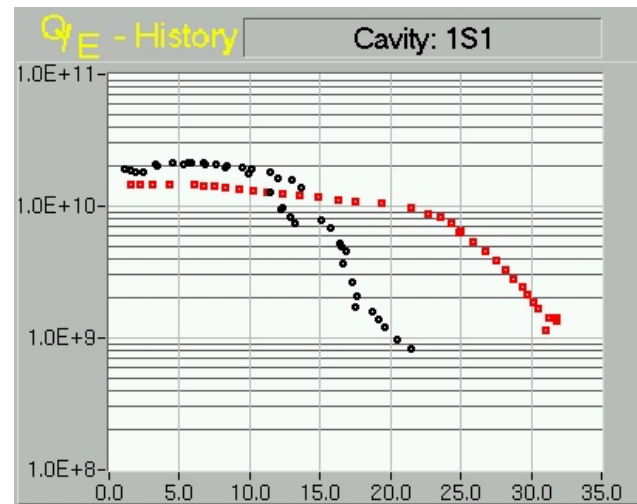


Figure 4: Test results. Black curve: Test after dry-ice cleaning with old setup. Red curve: Test after storage under air and dry-ice cleaning with optimized equipment

### SUMMARY

Test results shows that in principle no previous cleaning steps with high pressure water rinsing is necessary to obtain high  $Q$ -values and gradients. The major problem is still field emission, but there is evidence that handling of the cavity after cleaning is the limiting factor. Heating the cavity, to reach a high thermal gradient, should be optimized more. A countoured Infrared-Heater with an optimal wavelength, adequate to Niobium is ordered and will be installed in near future. Optimisation of cleaning parameters like speed of nozzle support, rotation speed of the cavity and pressure of  $\text{N}_2$  etc. is in progress.

### ACKNOWLEDGEMENT

We acknowledge the support of the European Community Research Infrastructure Activity under FP6 "Structuring the European Research Area" program (CARE, contract number RII-CT-2003-506395).

### REFERENCES

[1] D.Reschke, Proc. 10<sup>th</sup> Workshop on RF Superconductivity, Tsukuba, Japan, p.144 (2001).  
 [2] D.Reschke et al., Proc. LINAC 2004, Lübeck, Germany, p.776 (2004).