



Taylor & Francis
Taylor & Francis Group



GEODESY AND CARTOGRAPHY

ISSN 2029-6991 print / ISSN 2029-7009 online

2013 Volume 39(1): 7–10

doi:10.3846/20296991.2013.786879

UDC 528.52

POLYNOMIAL ERROR APPROXIMATION OF A PRECISION ANGLE MEASURING SYSTEM

Lauryna Šiaudinytė¹, Domantas Bručas², Mindaugas Rybokas³, Genadijus Kulvietis⁴

^{1, 2}*Institute of Geodesy, Vilnius Gediminas Technical University, Saulėtekio al. 11, LT-10223 Vilnius, Lithuania*

^{3, 4}*Department of Information Technologies, Vilnius Gediminas Technical University, Saulėtekio al. 11, LT-10223 Vilnius, Lithuania*

E-mails: ¹lauryna.siaudinyte@vgtu.lt (corresponding author); ²domka@ktv.lt;

³mindaugas.rybokas@vgtu.lt; ⁴gk@vgtu.lt

Received 05 February 2013; accepted 26 February 2013

Abstract. The paper deals with the calibration of a flat angle measuring system. The article describes a comparative method for using a multi-angular prism (polygon) with autocollimator along with an angle measuring system. The components of angle measuring system is analysed in the paper. The article also presents polynomial error approximation and the obtained results of calibrating the precision angle measuring system as well as discusses preliminary assumptions for further research.

Keywords: accuracy, angle encoders, angle measurement, calibration, measuring systems.

Reference to this paper should be made as follows: Šiaudinytė, L.; Bručas, D.; Rybokas, M.; Kulvietis, G. 2013. Polynomial error approximation of a precision angle measuring system, *Geodesy and Cartography* 39(1): 7–10.

Introduction

Precision angle measuring systems are widely used for manufacturing various types of machinery embedding them into devices and instruments such as total stations, metal cutting machines, etc. An angle encoder is the main part of an angle measuring system. They may vary in sizes, types and accuracy. Depending on the required accuracy, the whole angle measuring system must be accordingly calibrated. Calibration of such systems is essential to determine errors and increase measurement accuracy.

Calibration process is frequently a very complicated procedure requiring specific equipment, including standards for achieving the best results. Precision angle measurement is compulsory for engineering at various levels of precision, and therefore many artefacts and instruments such as angle gauge blocks, optical polygons and rotary tables are used for angle metrology. To ensure high reliability, they should be calibrated using standard instruments such as an indexing table along with an autocollimator (Just *et al.* 2003; Kim *et al.* 2011).

1. Equipment and method used for flat angle calibration

To determine the accuracy of an angle measuring system, a comparative method was chosen. This method is based on a comparison of the measurand and standard angle

determining a deviation between those angles. Equipment selected for realisation of this method consists of a precision angle comparator, 36 mirror-sided polygon and an autocollimator. The angle standard as a mirror polygon is an important measurement object used in applied for an angle calibration world wide. When measuring the angle accuracy of a product, many application fields of using the polygon could be used (Watanabe *et al.* 2003). The angle comparator consists of the basis that includes a precision mechatronic rotary device, a device for detecting circular scale graduation and its relative rotation according to the circular scale measuring system. A section view of the angle comparator is presented in Fig. 1. Another critical element is a calculation system for both the control of the calibration process and data processing. The basic mechatronic system is designed for direct limb and angular encoder calibration. The basis of such system consists of a massive small-grain grey granite brick with aerostatic rotational mechanism mounted on it through a suspension ring. It is rotated using a worm gear. To ensure proper rotation of this gear, combined aerostatic and rolling bearings are installed. The worm gear is mounted on aerostatic bearings and supported radially by rolling bearings. The rotation axis approximately matches the axis of the aerostatic rotational device. For this reason, suspension and radial bearings are mounted on position-correction

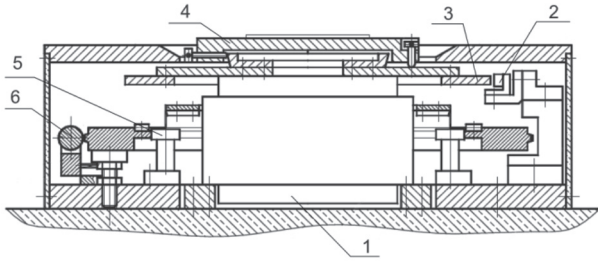


Fig. 1. Section view of an angle comparator

devices. The whole system is covered with a special cover and a precisely finished top surface protecting the system of damage coming from environmental pollutants. Additional measurement equipment can also be placed on this surface (Kasparaitis, Šukys 2008).

There are two diverse requirements for the gear of the comparator: it has to ensure constant angular rotation and the possibility of precise positioning while providing a stable angular position within given time.

The gear has not to create any other forces except for torque or tangential rotational force. It is also important that the gear does not generate intensive thermal activity or vibration. To perform accurate measurements, the laboratory should be isolated from any external vibrations under stable temperature.

Important parts of an angle measuring system are shown in the section view in Fig. 1: 1 – precision aerostatic shaft, 2 – reading head, 3 – reference circular scale, 4 – measured table, 5 – rolling bearing, 6 – worm gear.

One of the variants of the gear that meets the requirements mentioned before is a worm gear offering autonomous mechanism for the rotation of the gear combined with a precise connection with a rotation device that is rigid along the tangent direction of the spindle and slender in other directions.

The examined comparator has an elastic worm gear connection with the spindle generating pure torque without any radial or axial forces and ensures the stability of the spindle. The worm gear is rotated by an electric motor through a mechanical reducer and can be disconnected to rotate the spindle manually.

The limb of the angle measuring system has a rigid connection avoiding any intermediate sliding mechanical parts. It helps in eliminating negative effects of hys-

teresis and reverse errors that have a negative effect on precision and are common to mechanical coupling devices (Kasparaitis, Šukys 2008; Sydenham, Thorn 1992).

There are two precise guiding devices made of small-grain granite mounted on the basis of the comparator that have two sliding carriages with stroke-detection microscopes mounted on them. They are placed orthogonally to the axis of the spindle on aerostatic supports.

A 36 sided polygon is placed on the top of the precision angle measuring system with the embedded Renishaw angle encoder. The system is precisely centred and levelled. The autocollimator Hilger & Watts is pointed directly to the mirror face of the polygon and the system is set to the position in which the readout of the autocollimator is 0.00 arc seconds as shown in Fig. 2.

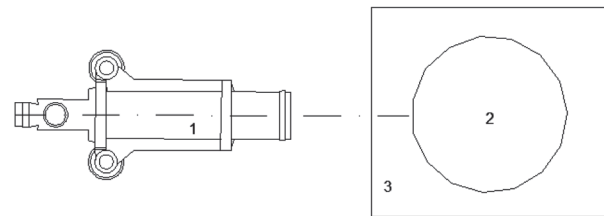


Fig. 2. Schematic view of instrument layout:

1 – autocollimator, 2 – 36 sided polygon placed on the top of the angle measuring system, 3 – angle measuring system

2. Data processing

A systematic error along with the evaluation of its possible cause is one of the key procedures in data processing (Rabinovich 2010). One of the main features influencing the precision of any rotary device is the eccentricity of mounting a rotating or measuring element (eccentricity of bearing or the measuring scale etc.). Having obtained scale calibration results, the eccentricity of the scale (or a disc mounting) can be calculated. Data on encoder systematic errors allow determining the mechanical systematic errors of the elements of the test rig such as the eccentricity of bearings or the scale itself (Kim *et al.* 2011, Stone *et al.* 2004). The encoder was calibrated using one reading head and the first harmonic was noticed in the chart. The results of calibrating the encoder are displayed in Fig. 3.

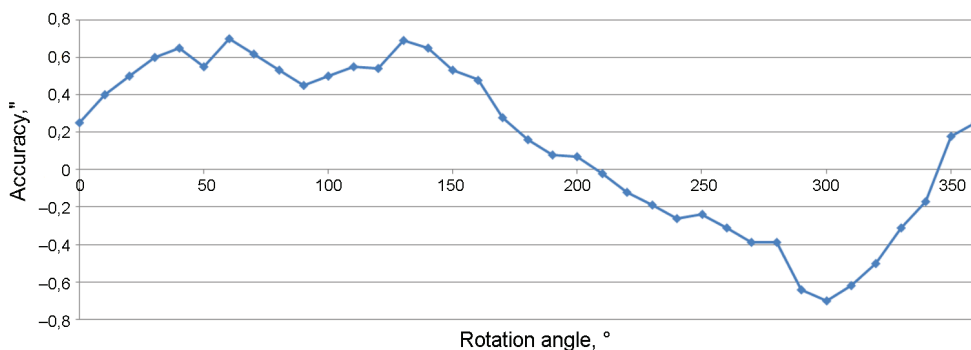


Fig. 3. Errors of the encoder

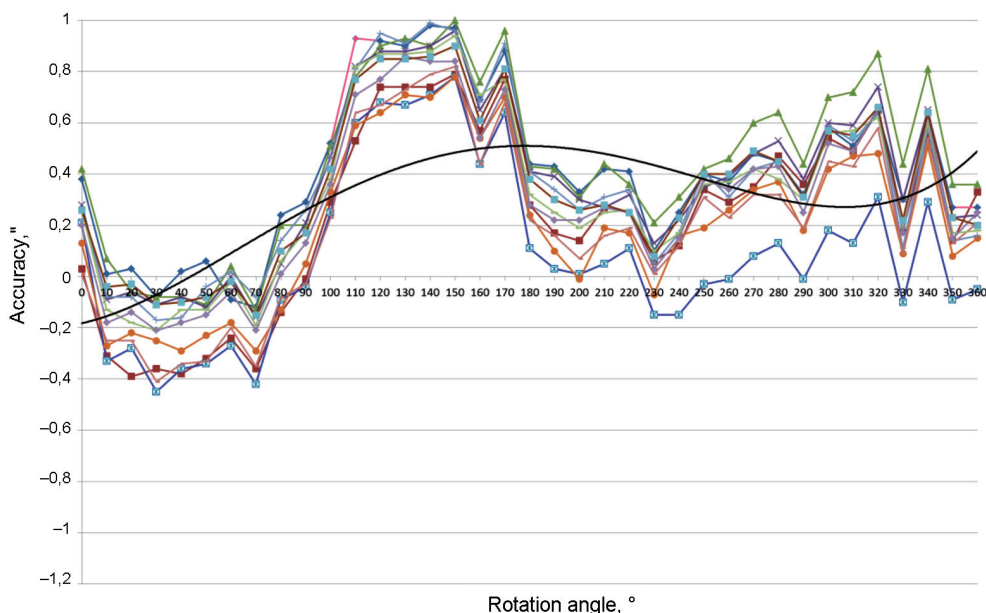


Fig. 4. The results of calibrating the angle measuring system

The measurement results are displayed in Fig. 4. The measurement errors were calculated following the evaluation of the results of polygon calibration and the accuracy of the autocollimator. Two reading sensors were embedded in the measuring system to eliminate eccentricity errors. Fig. 4 displays the results of twelve circles rotating the angle measuring system forwards and backwards.

Having the smoothed data and using Fourier analysis, the harmonics of measurements could be calculated (Bručas, Giniotis 2008; Bručas *et al.* 2006). Finite Fourier series can be expressed applying the following formula:

$$\delta\tilde{\varphi}(\varphi) = A_0 + 2 \sum_{m=1}^{n-1} (A_m \cos 2\pi m f_1 \varphi + B_m \sin 2\pi m f_1 \varphi) + A_n \cos 2\pi m f_1 \varphi, \quad (1)$$

The coefficients of the equation for each type of harmonics can be calculated as

$$A_m = \frac{1}{N} \sum_{r=-n}^{n-1} \delta\varphi_r \cos \frac{2\pi m r}{N}; \quad (2)$$

$$B_m = \frac{1}{N} \sum_{r=-n}^{n-1} \delta\varphi_r \sin \frac{2\pi m r}{N}, \quad (3)$$

where: m – the number of harmonics, N – the total number of measurements, r – the measurement number.

The amplitude of each type of harmonics is

$$R_m = \sqrt{A_m^2 + B_m^2}. \quad (4)$$

The phase shift of each type of harmonics (regarding the zero point) is

$$\varphi_m = \arctg\left(-\frac{B_m}{A_m}\right). \quad (5)$$

The received results indicate that the polynomial curve of the fourth order reflects the view of the present measurement data. The equation for the fourth order polynomial curve is

$$y = (7 \cdot 10^{-4})x^4 - (4 \cdot 10^{-7})x^3 + (6 \cdot 10^{-5})x^2 + 0,0022x - 0,1824. \quad (6)$$

The calculation of a standard deviation is shown in Fig. 5.

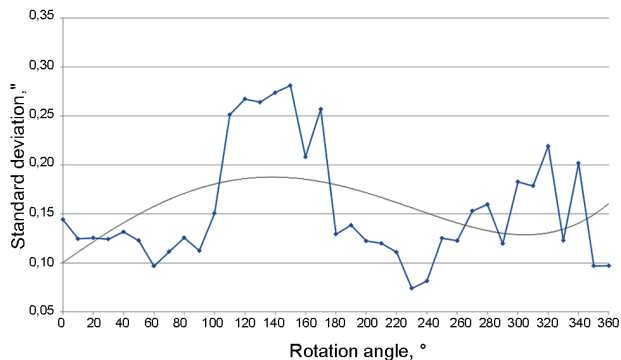


Fig. 5. Standard deviation

The equation for the polynomial curve of the standard deviation can be expressed as

$$y = (6 \cdot 10^{-11})x^4 - (2 \cdot 10^{-8})x^3 - 10^{-6}x^2 + 0,0011x + 0,1003. \quad (7)$$

Conclusions

Systematic errors of the angle measuring system have been determined. Calculating the errors of the polygon and the accuracy of the evaluated autocollimator and encoder has displayed the results of systematic errors that

tend to have the highest values in the range of the 36 sided polygon of 100° – 170° . This leads to the assumption that obvious systematic errors may be caused by other components of the angle measuring system (such as bearings) or the accuracy of installing the measurement system.

Acknowledgement

This research was funded by the European Social Fund under the Global Grant measure.

References

- Bručas, D.; Giniotis, V. 2008. Circular scale eccentricity analysis, *Mechanika* 2(57): 48–53. ISSN 1392-1207.
- Bručas, D.; Giniotis, V.; Petroškevičius, P. 2006. The construction of the test bench for calibration of geodetic instruments. *Geodesy and Cartography* 32(3): 66–70. ISSN 1392-1541.
- Just, A.; Krause, M.; Probst, R.; Wittekopf, R. 2003. Calibration of high-resolution electronic autocollimators against an angle comparator, *Metrologia* 40: 288–294. <http://dx.doi.org/10.1088/0026-1394/40/5/011>
- Kasparaitis, A.; Šukys, A. 2008. *Metrologinio ūkio ir matavimų organizavimas*. Vilnius: Technika. 192 p. ISBN 978-9-9552-8306-5. <http://dx.doi.org/10.3846/991-S>
- Kim, J. A., et al. 2011. Precision angle comparator using self-calibration of scale errors based on the equal-division-averaged method, in *Proc. of MacroScale 2011*. Wabern, 1–4.
- Rabinovich, S. G. 2010. *Evaluating measurement accuracy*. New York: Springer. 278 p. ISBN 978-1-4419-1455-2. <http://dx.doi.org/10.1007/978-1-4419-1456-9>
- Stone, J. A.; Amer, M.; Faust, B.; Zimmerman, J. 2004. Uncertainties in small-angle measurement systems used to calibrate angle artifacts, *Journal of Research of the National Institute of Standards and Technology* 109(3): 319–333. <http://dx.doi.org/10.6028/jres.109.024>
- Sydenham, P. H.; Thorn, R. 1992. *Handbook of Measurement science: Elements of Change*, vol. 3. Chichester. New York. Brisbane. Toronto. Singapore: John Wiley & Sons. 600 p.
- Watanabe, T.; Fujimoto, H.; Nakayama, K.; Kajitani, M.; Masuda, T. 2003. Calibration of polygon mirror by the rotary encoder calibration system, in *Proc. of XVII IMEKO World Congress*, June 22–27, 2003, Dubrovnik, Croatia, 1890–1893.
-
- Lauryna ŠIAUDINYTĖ.** Junior research fellow at the Institute of Geodesy. Saulėtekio al. 11, LT-10223 Vilnius, Lithuania, Ph. +370 5 274 4705, e-mail: lauryna.siaudinyte@vgtu.lt
MSc from VGTU in 2010. Currently, PhD student at the Department of Geodesy and Cadastre, Vilnius Gediminas Technical University.
Research interests: calibration of geodetic instruments, angle measurements, measurement accuracy and precision.
-
- Domantas BRUČAS.** Head of Space Science and Technology Institute, Saulėtekio al. 15, LT-10223 Vilnius, Lithuania. Doctor (2008). The author of two educational books and more than 30 scientific papers. Participated in a number of international conferences, owns three registered patents.
Research interests: comparator development for angular measurements, automation of processing measurement results.
-
- Mindaugas RYBOKAS.** Assoc. Prof., Dr at the Department of Information Technologies, Vilnius Gediminas Technical University, Saulėtekio al. 11, LT-10223 Vilnius, Lithuania (Ph. +370 5 274 4832), e-mail: mindaugas.rybokas@vgtu.lt.
The author of more than 35 scientific papers; participated in a number of International conferences.
Research interests: analysis of information measuring systems.
-
- Genadijus KULVIETIS.** Prof., Dr Habil at the Department of Information Technologies, Vilnius Gediminas Technical University, Saulėtekio al. 11, LT-10223 Vilnius, Lithuania. E-mail: gk@vgtu.lt.
The author of two educational books and more than 50 scientific papers. Participated in a number of international conferences.
Research interests: analysis of information measuring systems.