



the AERATOR group (2021). Identification of the source events for aerosol generation during oesophago-gastro-duodenoscopy. *Gut*. <https://doi.org/10.1136/gutjnl-2021-324588>

Peer reviewed version

License (if available):
CC BY-NC

Link to published version (if available):
[10.1136/gutjnl-2021-324588](https://doi.org/10.1136/gutjnl-2021-324588)

[Link to publication record in Explore Bristol Research](#)
PDF-document

This is the author accepted manuscript (AAM). The final published version (version of record) is available online via BMJ Publishing Group at <https://gut.bmj.com/content/early/2021/06/29/gutjnl-2021-324588> . Please refer to any applicable terms of use of the publisher.

University of Bristol - Explore Bristol Research

General rights

This document is made available in accordance with publisher policies. Please cite only the published version using the reference above. Full terms of use are available: <http://www.bristol.ac.uk/red/research-policy/pure/user-guides/ebr-terms/>

Title. Identification of the source events for aerosol generation during oesophago-gastro-duodenoscopy

Authors: Gregson F.K.A.^{1*}, Shrimpton A.J.^{2,3,6*}, Hamilton F.⁴, Cook T.M.⁵, Reid J.P.¹, Pickering A.E.^{2,6}, Pournaras D.J.⁷, Bzdek B.R.¹ and Brown J.M.³

* - these authors contributed equally to this work.

Affiliations

1 - School of Chemistry, University of Bristol, Bristol, BS8 1TS;

2 - School of Physiology, Pharmacology & Neuroscience, University of Bristol, Bristol, BS8 1TD.

3 - Department of Anaesthesia and Intensive Care Medicine, North Bristol NHS Trust, Bristol, BS10 5NB;

4 – Population Health Sciences, Bristol Medical School, University of Bristol, BS8 2PH

5 - Department of Anaesthesia and Intensive Care Medicine, Royal United Hospitals NHS Trust, Bath, UK and Bristol Medical School, University of Bristol, BS8 1TS

6 – Bristol Anaesthesia, Pain & Critical Care Sciences, Translational Health Sciences, Bristol Medical School, BS2 8HW.

7 – Department of Upper Gastrointestinal and Bariatric/Metabolic Surgery, North Bristol NHS Trust, Bristol, BS10 5NB

Author for Correspondence – JB: Email for Correspondence - jules.brown@nbt.nhs.uk

Word count: 3737 words.

Keywords: Oesophago-gastro-duodenoscopy, Aerosol, SARS-CoV-2, Coughing

Abstract (250 words)**Objective**

To determine if oesophago-gastro-duodenoscopy (OGD) generates increased levels of aerosol in conscious patients and identify the source events.

Design

A prospective, environmental aerosol monitoring study, undertaken in an ultraclean environment, on patients undergoing OGD. Sampling was performed 20cm away from the patient's mouth using an optical particle sizer. Aerosol levels during OGD were compared to tidal breathing and voluntary coughs within subject.

Results

Patients undergoing bariatric surgical assessment were recruited (mean BMI 44, mean age 40yrs, n=15). A low background particle concentration in theatres (3 L^{-1}) enabled detection of aerosol generation by tidal breathing (mean particle concentration 118 L^{-1}). Aerosol recording during OGD showed an average particle number concentration of 595 L^{-1} with a wide range ($3 - 4,320 \text{ L}^{-1}$). Bioaerosol generating events, namely coughing or burping, were common. Coughing was evoked in 60% of the endoscopies, with a greater peak concentration and a greater total number of sampled particles than the patient's reference voluntary coughs ($11,710$ v 2320 L^{-1} and 780 v 191 particles, n=9, $P=0.008$). Endoscopies with coughs generated a higher level of aerosol than tidal breathing whereas those without coughs were not different to background. Burps also generated increased aerosol concentration, similar to those recorded during voluntary coughs. The insertion and removal of the endoscope was not aerosol generating unless a cough was triggered.

Conclusion

Coughing evoked during OGD is the main source of the increased aerosol levels and therefore OGD should be regarded as a procedure with high risk of producing respiratory aerosols. OGD should be conducted with airborne personal protective equipment and appropriate precautions in those patients who are at risk of having COVID-19 or other respiratory pathogens.

SUMMARY**What is already known about this subject?**

Oesophago-gastro-duodenoscopy (OGD) is currently classified as an Aerosol Generating Procedure. Recent aerosol sampling studies have demonstrated increased particle concentration above background during OGD but not identified the source events.

What are the new findings?

An uneventful OGD (without coughing or burping) does not generate aerosol above that associated with tidal breathing. More specifically, insertion and removal of an endoscope for OGD does not generate an increase in aerosol concentration. However, the process of OGD frequently triggers coughs in conscious patients. Such OGD-evoked coughs generate higher aerosol concentration than volitional coughs and the resultant plumes of airborne particles are likely to be associated with an increased risk of transmission of respiratory pathogens. Our study puts the aerosol generated during endoscopy into a meaningful context of normal respiratory events and identifies the index risk events.

How might it impact on clinical practice in the foreseeable future?

OGD-evoked coughs are common. Therefore, OGD should be treated as having a high risk of aerosol generation and should be conducted with airborne personal protective equipment and appropriate precautions in those patients who are at risk of having COVID-19 or other respiratory pathogens. Strategies to reduce coughing and eructation would reduce aerosol generation.

INTRODUCTION

The Coronavirus-19 (COVID-19) pandemic, caused by severe acute respiratory syndrome coronavirus-2 (SARS-CoV-2), has led to dramatic and widespread changes in the way hospital medicine is practised. SARS-CoV-2 has the potential to be spread by three main routes: droplet, contact and airborne. The extent of airborne transmission of SARS-CoV-2 remains debated [1, 2, 3, 4] but is of increasing concern especially with the advent of new strains of the virus (e.g. B.1.1.7) that have increased transmissibility [5, 6]. Infectious respiratory aerosols are considered by the World Health Organisation as being composed of particles <5 micrometres in diameter [7] which remain in suspension in the air for many minutes or hours, potentially leading to distant transport of viral particles [8, 9]. Importantly, particles of this dimension are respirable, enabling deposition deep within the human respiratory tract leading to transmission of disease [8].

A number of medical interventions have been designated 'aerosol generating procedures' (AGPs). These AGPs are considered to carry the highest risk of airborne transmission of respiratory pathogens to healthcare workers. The interventions currently categorised as AGPs are based predominantly on epidemiological data from the 2003 SARS-COV-1 epidemic [10, 11]. The WHO list of AGPs has been adopted or adapted by many national healthcare organisations such as the Center for Disease Control and Prevention (CDC) [12] and Public Health England (PHE) [13]. Oesophago-gastro-duodenoscopy (OGD) is classified as an AGP and this designation has led to development of joint guidelines for safe endoscopy by the Gastroenterological societies in the UK[14], Europe [15] and USA [16].

Current national and international guidance recommends the use of airborne precaution personal protective equipment (PPE) when undertaking AGPs, which includes the use of respirators (e.g. FFP3 or N95 masks). Other recommendations include performing AGPs in a closed space with good ventilation [17, 18] and allowing a sufficient 'fallow' interval such that aerosol may disperse after the procedure [19]. These precautions inevitably slow the turnover within an operating room or procedural suite, and the wearing of PPE may impact on the quality of care delivered due to physical and communication difficulties.

The categorisation of OGD as an AGP was not based on evidence demonstrating aerosol generation from this intervention, nor from being associated with an increased incidence of SARS-CoV-2 transmission to healthcare workers conducting the procedures. Recent work directly measuring aerosol levels in the clinical environment has questioned the validity of inclusion of several procedures defined as 'aerosol generating' including tracheal intubation and extubation [20]; percutaneous tracheostomy [21]; and respiratory supportive treatments such as continuous positive airway pressure delivered via a face mask [22, 23, 24].

Two recent proof-of-concept studies reported increased levels of aerosol measured during OGD and concluded that the procedure is an AGP [25, 26]. However, these studies have been unable to definitively identify the specific source event responsible for the aerosol generation (i.e. endoscope insertion / removal, coughing, deep breathing, gastrointestinal eructation or retching), nor were they able to place the findings in the context of the risk of aerosol generation by natural respiratory events (tidal breathing, coughing). This is important as respiratory events such as coughing, speaking and breathing have been shown to generate measurable concentrations of aerosol [27, 28, 29, 30, 31]. To strengthen the evidence base underlying designation of AGPs, and the rationale for stringent airborne transmission-based precautions, it is essential to determine how much aerosol these procedures generate compared to natural respiratory events. We therefore quantitated the extent to which OGD, performed in conscious patients, generates aerosols and compared this to the aerosol generated by coughing and tidal breathing in the same patients in an ultra-clean ventilation operating theatre.

METHODS

Ethics

A prospective environmental sampling study was undertaken to measure the amount and size distribution of particles generated by conscious patients undergoing OGD in a UK hospital (North Bristol NHS Trust). Ethical approval was granted by the Greater Manchester REC committee (Reference: 20/NW/0393) as part of the AERATOR study (approved 18/09/2020). The study is registered in the ISRCTN registry (ISRCT:N21447815) and granted Urgent Public Health status by the NIHR. Patients or the public were not involved in the design, or conduct, or reporting, or dissemination plans of our research.

Selection of patients

Study participants were over 18 years of age and undergoing diagnostic OGD as part of a bariatric surgical assessment. The indication for endoscopy was in line with the International Federation for the Surgery of Obesity and Metabolic Disorders (IFSO) Position Statement [32] which recommends consideration of OGD in patients without upper gastrointestinal symptoms prior to bariatric and metabolic surgery procedures. All patients had self-isolated for two weeks, had a negative SARS-CoV-2 polymerase chain reaction test in the 72-hours before admission and gave written informed consent before entry to the study.

Study conduct

The objective of the study was to measure aerosol generated during the routine conduct of OGD. To sensitively detect aerosols generated by either natural respiratory events or AGPs, the measurements must be undertaken in an environment where background airborne particle concentrations are very low. Therefore, recordings were undertaken in operating theatres with an ultra-clean ventilation system (EXFLOW 32; Howorth Air Technology, Farnworth, UK) with high efficiency particulate air (HEPA) filtration. The ultra-clean ventilation system (UCV) provides an environment which is both ultra-clean and highly ventilated. We have previously demonstrated that the UCV ensures a very low background particle concentration, enabling detection of aerosols generated by natural respiratory events and AGPs [20, 21, 31, 33].

The UCV was placed in standby mode during recordings to minimise any effect the high air change rate may have on particle detection [33]. When fully operational, the UCV system generates a 'surgical canopy' of clean air, which is directed vertically downward over the operating table within a perimeter delineated by markings on the floor. The air handling unit runs at 50Hz to generate this ultra-clean zone which results in 500-600 air changes per hour within the perimeter. When the system is placed

in 'standby mode' the frequency of the inverter in the air handling unit is reduced to 25Hz and the 'surgical canopy' of constrained laminar airflow is lost, this reduces the number of air changes to 25 per hour (equivalent to a standard operating theatre). The air flow velocity is $0.25\text{m}\cdot\text{s}^{-1}$ at 1m above the ground. This still provides an ultraclean environment (minimising interference from background aerosol) [33] but without the high number of air changes, ensuring any findings are generalisable to more typical operating theatre settings.

All healthcare workers, and members of the investigating team, wore contact and droplet precaution PPE in line with both trust, and national policy. The number of staff in the room and their movement were kept to a minimum throughout the study to minimise extrinsic and artefactual aerosol generation.

A portable Optical Particle Sizer (OPS, TSI Incorporated, model 3330, Shoreview, NM, USA) was used. The OPS samples air at $1\text{L}\cdot\text{min}^{-1}$ and detects particles by laser optical scattering, reporting the particle number concentration and size distribution within the range 300 nm to 10 μm diameter, with a sampling bin width of 1 s. All air sampled was via a 3D printed funnel (formed of Polylactic acid on a RAISE3D Pro2 Printer, 3DGBIRE, Chorley, UK) with a maximum diameter of 150 mm, cone height of 90 mm with a 10-mm exit port. Conductive silicone sampling tubing (3001788, TSI, 1m length, 4.8 mm internal diameter) connected the funnel to the OPS. The silicone tube had an internal volume of 72.5 ml giving a transit lag between the funnel and the particle sizer (with a flow of $1\text{L}\cdot\text{min}^{-1}$) of 4.3 s which was taken into account in the time registration of measurements. In previous work, we have established that the transmission sampling loss of particles $< 5\ \mu\text{m}$ diameter with this set up is $<10\%$ [31]. It should be noted that we cannot report the absolute number of particles generated, only the number sampled and detected, recognising that we do not sample all of the air from the activity into the OPS instrument.

Reference aerosol generation was measured in each patient before endoscopy with the patient positioned supine on the operating table in the theatre. The sampling funnel was handheld by the investigator approximately 20cm in front and directed towards the patient's face. The reference sequences consisted of one-minute quiet tidal breathing, followed by three maximal voluntary coughs at 30 second intervals, with tidal breathing in between. Background aerosol was then measured with the funnel at 1 metre distance, facing away from the patient (and any other staff) but still within the central area of the UCV system while the patient was prepared for the endoscopy as below.

All patients had topical anaesthesia of their oropharynx with Lidocaine 10% (Xylocaine, 50 ml/500 spray, AstraZeneca, Sweden). The OGD was performed in the left lateral position, with conscious sedation achieved with intravenous midazolam as necessary by the endoscopist, according to their

normal practice. A mouthguard was inserted prior to insertion of the endoscope (8.9mm GIF-H290 Video Gastrointestinal Scope with EVIS X1 CV-1500 Video System; Olympus, Tokyo, Japan).

Aerosol generation during endoscopy was measured with the sampling funnel, handheld 20 cm from the patient's mouth. This enabled insertion of the endoscope between the funnel and the mouth. The aerosol generated during OGD was analysed for all periods between endoscope insertion through the mouthguard until endoscope removal. These periods were aggregated for those patients where more than one endoscope insertion was undertaken. Aerosol sampling commenced for reference recordings, undertaken prior to initial endoscope insertion, and was continuous until after final endoscope removal. All events of significance were timestamped (i.e. endoscope insertion, endoscope removal, coughs, burping). Cough events (both voluntary and evoked during endoscopy) were averaged within subject and then aggregated across the whole group.

Data were exported from the OPS, processed in the TSI Aerosol Instrument Manager software, and analysed in Origin Pro (Originlab, Northampton, MA, USA) and Prism v8 (Graphpad, San Diego, CA, USA). We report the sampled mean aerosol concentration as well as the peak concentration over 1 s sampling time, reported as mean (SD). We used paired or unpaired t-tests or Mann-Witney and Wilcoxon tests to conduct statistical comparisons as appropriate. The criterion for statistical significance was set at $P < 0.05$.

RESULTS

Fifteen patients were recruited: fourteen were being assessed before bariatric surgery and one patient attended for assessment 2 years after gastric bypass surgery. There were two males and thirteen females with a mean BMI of 46 ± 9.3 kg/m² and an average age of 42 years (range 21-75). Four patients requested and received additional conscious sedation with endoscopist-administered midazolam.

Background sampling showed the air was very clean with a mean aerosol number concentrations, referred to below simply as the *concentration*, of 3.1 (3.7) particles.L⁻¹ (corresponding to ~3 particles detected each minute of sampling). The patient's tidal breathing, via the mouth, generated a mean particle concentration of 118 (97.2) L⁻¹ and an average peak particle concentration of 540 (410) L⁻¹ (n=15 patients) (Figure 1). In nine patients a further minute of nasal breathing was recorded, this generated a mean particle concentration of 63.5 (72.0) L⁻¹ and a peak particle concentration of 327 (283) L⁻¹ (n=9). Nasal breathing produced a lower aerosol concentration than mouth breathing (P=0.008, Wilcoxon).

[Figure 1]

The expulsive phase of a cough typically lasts less than 1 second [34], and the aerosol concentration rises rapidly to a sharp peak, with a subsequent decay as the remaining aerosol reaches the sampling funnel, dissipates and becomes diluted by clean background air (Figure 2). The reference voluntary coughs for the 15 patients each generated an aerosol concentration profile clearly detectable above the baseline with a mean peak concentration of 2330 (2120) L⁻¹, an average total number of particles detected per cough of 192 (183) and mean duration of 19.8 (5.8) s.

[Figure 2]

The mean aerosol particle concentration measured during endoscopy was 595 (1110) L⁻¹ (n=15, Figure 1a) and the average duration of endoscopy was 222 s (range 129 – 457s). This aerosol concentration was well above background levels but was not significantly higher than the level of aerosol measured during mouth breathing (vs 118 L⁻¹, P=0.17, Wilcoxon test). We noted that there was a very large range of average aerosol concentrations between endoscopy sessions from 3 L⁻¹ (indistinguishable from background – see figure 3a) to 4320 L⁻¹ (figure 3b). Coughs were frequently evoked during the endoscopy (figure 3b, 9/15 subjects were observed to cough – with a median of 4 coughs [range 1-10]). Likewise, burps were induced during some procedures (figure 2b, 4/15 subjects burped – median of 2 burps per endoscopy [range 1-4]).

The OGD-evoked coughs generated high concentrations of aerosol (Figure 2a & 3b) with a mean peak concentration of 11,710 (13,700) L⁻¹, and total number of particles detected per cough of 780 (1010).

The total number of particles from evoked coughs was significantly greater than the volitional coughs recorded from the same patients (780 vs 191, $n=9$, $P=0.008$, Wilcoxon) and the peak mass concentration was higher (4.51 vs 0.54 $\mu\text{g}/\text{m}^3$, $P=0.008$, Wilcoxon). Similarly, the peak particle concentration was greater for evoked versus volitional coughs ($11,710$ vs 2320 L^{-1} , $P=0.008$ Wilcoxon). The profile of the particle concentration generated by evoked coughs remained detectable above the baseline for a mean duration of 14.5 (4.8) s. Analysis of the size distribution of these evoked coughs showed them to have a similar profile to volitional coughs, reported as number concentration distribution across the size-resolved bins of the OPS, but with an increase in the total numbers of particles in each size bin (Figure 4).

[Figure 3]

Burps observed during OGD procedures generated a mean peak concentration of 3060 (3830) L^{-1} and a total number of particles detected per burp of 205 (280). There was no significant difference between the peak particle concentration or total number of detected particles of a voluntary cough and burp by the same patient. Analysis of the particle size distribution of these evoked burps showed them to have a different profile to coughs, with a decrease in the total numbers of particles in the size range between 0.5 and $1.5\mu\text{m}$ (Figure 4).

As an evoked cough or a burp had a large effect on the particle concentration, our subsequent analysis split the patients into those who had such “bioaerosol generating events” (BGEs) versus those who did not. The mean aerosol number concentration sampled during the eleven endoscopies with BGEs was higher than that recorded during the four endoscopies where no cough or burp was triggered (808 (1240) L^{-1} vs 10.0 (7.2) L^{-1} , Mann-Whitney test, $P=0.0015$). When these transient and discrete coughing or burping events were excluded from the analysis, the mean particle concentration during the rest of the endoscopy was 31.4 (33.9) L^{-1} identifying the discrete BGEs as being responsible for the overall elevation in aerosol during the procedure.

[Figure 4]

A focussed analysis of aerosol concentration fluctuations during a 30 s sampling window surrounding endoscope insertion ($n=12$) and removal ($n=11$) (starting 10 s prior to insertion or removal), excluding those which triggered BGEs, showed a low concentration of aerosol which was not significantly different to background and was less than both tidal breathing and voluntary coughs (Figure 5). No other significant aerosol generating events were identified during the conduct of the OGDs.

[Figure 5]

DISCUSSION

We have measured aerosol generation in patients undergoing OGD. In the patients who coughed during the procedure (60%), very high particle concentrations were detected - around five-fold higher than those seen during volitional coughs. This suggests that OGD meets the criterion for being a high risk procedure for generating aerosol in those patients in whom endoscopy evokes a cough. This is consistent with the findings of recent studies which also concluded that OGD was associated with increased aerosol generation [25, 26]. However, we specifically identify that evoked coughs and belches are the index risk events rather than the insertion and removal of the endoscope from the oesophagus.

Conducting aerosol sampling during OGD in a HEPA-filtered ultraclean environment provides an optimal setting for detecting aerosols due to the extremely low background concentration. Sampling in an adjacent operating theatre (non UCV) revealed a baseline particle content of 16,000 particles L⁻¹ (compared to 3 L⁻¹) [33]. Sampling in such a theatre would mean the aerosol detected in this study (for example associated with tidal breathing) would be impossible to detect over background 'noise'. We note that a previous study of OGD aerosol generation also found high background counts (25-40,000 particles per Cubic Foot equating to ~900-1400 particles L⁻¹) in their procedure room, which had a standard ventilation system [25]. This would preclude detection of the aerosol generated by breathing or even a volitional cough over the background particle count (likely mostly inorganic 'dust' rather than bioaerosol). Importantly, the high temporal resolution (1Hz measurements of airborne particles) in combination with the low background aerosol concentration enables the definitive attribution of specific respiratory or procedural events as being the source of the aerosol (rather than attempting to make the link by inference when using a minute by minute analysis [26]).

A novel aspect of our study design is using each patient's own respiratory events as a comparator. This puts the aerosol measurements made during endoscopy into a meaningful biological context of normal respiratory events. This approach also reduces the impact of between-subject variation and so increases the power to detect significant changes even within a relatively small sample size. We used tidal breathing as a lower reference for natural aerosol generation and could reliably detect this aerosol concentration above background (the first time such a measure has been possible in a study of patients). For the patients who did not cough during the procedure lower concentrations were detected than during coughing or even normal tidal breathing. This may be due to the presence of the bite guard, attenuation by the endoscope itself or the endoscopist's hands, or due to shallow / nasal breathing during the procedure.

The sampling method used in our study is appropriate to detect aerosol particles generated from the respiratory system which are generally in the range of 10 nm to 20 μm , with a large predominance in the sub-micron range [29]; we do not detect droplets larger than 20 μm and can make no statement about their presence or absence from these procedures. We set out to study aerosol levels close to the source of generation. By sampling close to the patient (20cm) we achieve an accurate measure of exposure risk for the endoscopist and assistant who will be within the near vicinity of the patient (within 1m) so any emitted plumes of aerosol are highly relevant to their risk of transmission. The WHO have defined aerosols as being composed of particles $<5\mu\text{m}$ in size but recently, such a strict delineation in size has been questioned: moist exhaled droplets smaller than 100 μm can decrease considerably in size, showing similar aerodynamic behaviour to aerosol such that they can present a transmission risk over many metres [35]. This is relevant particularly when considering the dispersal of particles within the room which is currently not directly experimentally quantifiable for respiratory aerosols given the relatively low concentrations of particles and the enormous degree of dilution that occurs with dispersal even in a room with standard ventilation. We believe that the primary risk to the endoscopy team is from the close-quarters exposure to respiratory aerosol near the site of generation (the patient) but the issue of potential particle persistence and dispersal within the room as a route of transmission may also be a factor that merits further investigation (for review see [36]).

Respiratory aerosols are considered to be well represented by a bimodal distribution, with mean aerodynamic diameters of the two modes in the range 800 to 1500 nm; the smaller mode is considered to arise in the lower respiratory tract, the bronchioles, and the larger is assigned as the laryngeal mode [29]. The OPS cannot intrinsically differentiate between respiratory and non-respiratory aerosols, but by timestamping events, minimising movement of the investigator, sampling close to the patient and using a funnel to directionally focus on sources originating from the patient we reduced the risk of artefactual particle detection or detection of aerosol from staff in the room. We did not take any specific precautions such as limiting staff movement or altering their routine care during the conduct of these endoscopies and so our results are characteristic of aerosol generated during typical clinical practice. The size distribution of the particles detected during the study was typical of respiratory aerosols; it formed a log-normal distribution of particles with the peak lying in the submicron size range [20, 29, 30] and had a similar profile for both voluntary and procedure-evoked coughs [20]. This suggests the mechanism generating the aerosol is similar in both cases and provides a characteristic fingerprint distinguishing respiratory aerosols from other potential particle sources (ie from fabric / bedding dust released by movement of staff and patient).

The increased number of particles produced by OGD-evoked coughs, above those produced by a volitional cough, may relate either to a more forceful reflexively-generated protective cough, to the

presence of fluid in the oropharynx associated with the endoscopy, or to partial occlusion of the oropharynx during endoscopy reducing the diameter of the airway and increasing the amount of turbulent flow. Interestingly burps (eructations) also produced measurable aerosol but this had a different size distribution to coughs (with an order of magnitude fewer particles in the size range from 0.5-1.5 μm) reflecting the different site of origin of the aerosol. However, although the gastric source of the BGE is unlikely to represent a reservoir for SARS-CoV-2 (unlike the lungs), the passage of turbulent gas flow over the oro- and naso-pharyngeal membranes still could result in generation of virus containing aerosol so should not be discounted as a risk.

Our study was not designed to look at the potential mitigating effect of using sedation to reduce coughing. Midazolam was administered to four patients for conscious sedation at patient request. All of the patients receiving midazolam coughed compared to 50% of the remainder. A subsequent exploratory study of the incidence of coughing in patients having upper GI endoscopy in our institution showed similar findings with 67% (n=8/12) coughing with midazolam sedation and 40% without (n=4/10). This fits with the known lack of antitussive properties of benzodiazepines which tend to preserve airway reflexes (generally considered a safety advantage for endoscopy in reducing the incidence of aspiration and hypoxia). Likewise, both of the previous studies of aerosol generation during endoscopy [25, 26] found no association with either the presence or quantity of sedation on aerosol generation (both with midazolam). A randomised controlled study would be needed to answer the question as to whether conscious sedation can be used to reduce aerosol generation during endoscopy. However, we also note that this would be a difficult trial to translate into change in guidelines as even a large reduction in the incidence of coughing (of say 50% as has been noted for combinations of midazolam and opiate [37, 38]) could not exclude the possibility that any individual patient would cough or burp and hence airborne PPE would still be needed. This would also have to be balanced against the possible detrimental effect of suppression of protective airway reflexes which could increase the risk of hypoxia.

There are several limitations to our study. Our sample size was relatively small, and 14 out of the 15 participants had a BMI > 40 kg.m⁻². It is possible that these patients with higher BMI may have generated more aerosol than leaner patients (as was suggested by the study of Sagami and colleagues [26]), but this effect is likely to apply both for the baseline cough measurements and during endoscopy and so is controlled for in our study design looking at relative levels of airborne particles. It is not possible to extrapolate our findings to patients with active respiratory disease or COVID-19 infection as all participants were screened for COVID-19 and had no acute illness. Our study cannot be used to determine the risk of COVID-19 transmission during endoscopy where the risk status of the patient (i.e. the likelihood of having COVID) is the major determinant. Our sampling methodology does not

detect aerosols smaller than 300 nm (approximately three times the diameter of the SARS-CoV-2 virus) however, respiratory particles less than 300 nm in diameter are extremely unlikely to carry viable virions unless the patient's viral titre is extremely high. This lower size limit excludes aerosols of sub-virus size which cannot contain the virus [39] but are always present in any environment at the highest concentration and number – so our sampling method reduces this irrelevant 'noise' signal. Similarly, aerosols greater than 10 µm are not detected using our techniques. However, particles larger than 5 µm are classified as droplets and protection is afforded by droplet precaution PPE (ie fluid resistant surgical facemasks).

Our findings are clinically relevant, particularly in the context of the COVID pandemic. Performing an OGD may unpredictably trigger coughing whenever the oropharynx is instrumented, and such OGD-evoked coughs generate more aerosol than either breathing or volitional coughs. Based on our observations, OGD should continue to be designated an aerosol generating procedure in conscious patients. Therefore, airborne protection PPE including a FFP3/N95 facemask and eye protection should be used in the care of any patient known or suspected to have COVID-19. These precautions will likely have to continue while SARS-CoV-2 is still in circulation in the community and beyond for the management of any patients with respiratory pathogens. We also note there is currently an absence of epidemiological evidence demonstrating that OGD is associated with an increased risk of COVID transmission, but this may reflect the widespread adoption of airborne PPE and precautions by endoscopists and endoscopy staff. Given the increased risk of aerosol generation we suggest that upper GI endoscopy should be conducted in an environment with a high level of air changes and carefully designed air flows to ensure rapid clearance and dispersal of aerosol [19]. We find no evidence for any other sources of increased aerosol generation during the OGD and therefore if a patient does not cough or belch during the OGD then consideration may be given to decreasing the time interval for air changes in the room between cases. In addition, strategies to reduce the incidence of coughing and eructation should be explored as a means to decrease the risk of aerosol generation.

ACKNOWLEDGEMENTS

The authors acknowledge the AERATOR group, which consists of (in alphabetical order): Arnold, D; Brown, J; Bzdek, B; Davidson, A; Dodd, J; Gormley M; Gregson, F; Hamilton, F; Maskell, N; Murray, J; Keller, J; Pickering, A.E; Reid, J; Sheikh, S; Shrimpton, A.

The AERATOR study was fully funded by an NIHR-UKRI rapid rolling grant (Ref: COV0333).

This report presents independent research commissioned by the National Institute for Health Research (NIHR). The views and opinions expressed by authors in this publication are those of the authors and do not necessarily reflect those of the NHS, the NIHR, UKRI, or the Department of Health. B.R.B. is supported by the Natural Environment Research Council (NE/P018459/1).

AUTHOR CONTRIBUTIONS

FKAG and AJS are joint first authors on this article. AJS, JMB, DJP and FH collected the data. FKAG, AJS and AEP performed the data analysis. JMB, AEP, AJS, FKAG and TMC drafted the manuscript. BRB, JPR and AEP provided technical guidance and advice. All authors read and approved the final manuscript.

COMPETING INTERESTS

The authors declare no competing interests.

REFERENCES

- 1 Miller SL, Nazaroff WW, Jimenez JL, Boerstra A, Buonanno G, Dancer SJ, *et al.* Transmission of SARS-CoV-2 by inhalation of respiratory aerosol in the Skagit Valley Chorale superspreading event. *Indoor Air* 2020.
- 2 Schutzer-Weissmann J, Magee DJ, Farquhar-Smith P. Severe acute respiratory syndrome coronavirus 2 infection risk during elective peri-operative care: a narrative review. *Anaesthesia* 2020;**75**:1648-58.
- 3 Asadi S, Bouvier N, Wexler AS, Ristenpart WD. The coronavirus pandemic and aerosols: Does COVID-19 transmit via expiratory particles? *Aerosol Science and Technology* 2020;**54**:635-8.
- 4 Morawska L, Milton DK. It Is Time to Address Airborne Transmission of Coronavirus Disease 2019 (COVID-19). *Clin Infect Dis* 2020;**71**:2311-3.
- 5 Mahase E. Covid-19: What have we learnt about the new variant in the UK? *British Medical Journal* 2020;**371**:m4944.
- 6 NERVTAG. Meeting on SARS-CoV-2 variant under investigation VUI-202012/01., 2020.
- 7 W.H.O. Infection prevention and control of epidemic and pandemic-prone acute respiratory infections in health care. Geneva: World Health Organization, 2014.
- 8 Gralton J, Tovey E, McLaws M-L, Rawlinson WD. The role of particle size in aerosolised pathogen transmission: A review. *Journal of Infection* 2011;**62**:1-13.
- 9 Walker JS, Archer J, Gregson FKA, Michel SES, Bzdek BR, Reid JP. Accurate Representations of the Microphysical Processes Occurring during the Transport of Exhaled Aerosols and Droplets. *ACS Central Science* 2021;**7**:200-9.
- 10 Boswell C, Longstaff J. Aerosol Generating Procedures (AGPs). 2020; https://hpspubsrepo.blob.core.windows.net/hps-website/nss/2893/documents/1_tbp-lr-agp-v1.pdf: accessed:
- 11 Tran K, Cimon K, Severn M, Pessoa-Silva CL, Conly J. Aerosol generating procedures and risk of transmission of acute respiratory infections to healthcare workers: a systematic review. *PLoS One* 2012;**7**:e35797.
- 12 Which procedures are considered aerosol generating procedures in healthcare settings. Healthcare workers FAQs. 2020; https://www.cdc.gov/coronavirus/2019-ncov/hcp/faq.html?CDC_AA_refVal=https%3A%2F%2Fwww.cdc.gov%2Fcoronavirus%2F2019-ncov%2Fhcp%2Finfection-control-faq.html: accessed: 30/12/2020
- 13 COVID-19 infection prevention and control guidance: aerosol generating procedures. 20 October 2020. ; <https://www.gov.uk/government/publications/wuhan-novel-coronavirus-infection-prevention-and-control/covid-19-infection-prevention-and-control-guidance-aerosol-generating-procedures> accessed: 18/12/20
- 14 Endoscopy activity and COVID-19: BSG and JAG guidance. 2020; <https://www.bsg.org.uk/covid-19-advice/endoscopy-activity-and-covid-19-bsg-and-jag-guidance/>: accessed: 30th December 2020
- 15 Gralnek IM, Hassan C, Beilenhoff U, Antonelli G, Ebigbo A, Pellise M, *et al.* ESGE and ESGENA Position Statement on gastrointestinal endoscopy and COVID-19: An update on guidance during the post-lockdown phase and selected results from a membership survey. *Endoscopy* 2020;**52**:891-8.
- 16 American Society for Gastrointestinal Endoscopy : Guidance for GI endoscopy and practice operations during the COVID-19 pandemic. 2021; https://www.asge.org/docs/default-source/default-document-library/guidance-for-gi-endoscopy-and-practice-operations-during-the-covid-19-pandemic_updated_final-march-2021.pdf: accessed: 11/4
- 17 Cook TM. Personal protective equipment during the coronavirus disease (COVID) 2019 pandemic – a narrative review. *Anaesthesia* 2020;**75**:920-7.
- 18 COVID-19 Guidance for the Remobilisation of services within health and care settings: infection prevention and control (IPC) recommendations. August 2020;

<https://www.gov.uk/government/publications/wuhan-novel-coronavirus-infection-prevention-and-control>: accessed:

- 19 Cook TM, Harrop-Griffiths W. Aerosol clearance times to better communicate safety after aerosol-generating procedures. *Anaesthesia* 2020;**75**:1122-3.
- 20 Brown J, Gregson FKA, Shrimpton A, Cook TM, Bzdek BR, Reid JP, *et al.* A quantitative evaluation of aerosol generation during tracheal intubation and extubation. *Anaesthesia* 2021;**76**:174-81.
- 21 Ramesh AV, Collin I, Gregson FKA, Brown J. Aerosol generation during percutaneous tracheostomy insertion. *Journal of the Intensive Care Society*, 2020:1751143720977278.
- 22 Gaekle NT LJ, Park Y, Kreykes G, Evans MD, Hogan CJ. Aerosol Generation from the Respiratory Tract with Various Modes of Oxygen Delivery. *Am J Respir Crit Care Med* 2020;**202**:1115–24.
- 23 Wilson NM, Marks GB, Eckhardt A, Clarke A, Young F, Garden FL, *et al.* The effect of respiratory activity, ventilatory therapy and facemasks on total aerosol emissions. medRxiv, 2021:DOI: 10.1101/2021.02.07.21251309.
- 24 Hamilton F, Gregson F, Arnold D, Sheikh S, Ward K, Brown J, *et al.* Aerosol emission from the respiratory tract: an analysis of relative risks from oxygen delivery systems. medRxiv 2021:DOI: 10.1101/2021.01.29.21250552.
- 25 Chan SM, Ma TW, Chong MK, Chan DL, Ng EKW, Chiu PWY. A Proof of Concept Study: Esophagogastroduodenoscopy Is an Aerosol-Generating Procedure and Continuous Oral Suction During the Procedure Reduces the Amount of Aerosol Generated. *Gastroenterology* 2020;**159**:1949-51 e4.
- 26 Sagami R, Nishikiori H, Sato T, Tsuji H, Ono M, Togo K, *et al.* Aerosols Produced by Upper Gastrointestinal Endoscopy: A Quantitative Evaluation. *Am J Gastroenterol* 2021;**116**:202-5.
- 27 Stelzer-Braid S, Oliver BG, Blazey AJ, Argent E, Newsome TP, Rawlinson WD, *et al.* Exhalation of respiratory viruses by breathing, coughing, and talking. *J Med Virol* 2009;**81**:1674-9.
- 28 Yang S LG, Chen CM, Wu CC, Yu KP. The size and concentration of droplets generated by coughing in human subjects. *Journal of Aerosol Medicine* 2007;**20**:484– 94.
- 29 Johnson GR, Morawska L, Ristovski ZD, Hargreaves M, Mengersen K, Chao CYH, *et al.* Modality of human expired aerosol size distributions. *Journal of Aerosol Science* 2011;**42**:839-51.
- 30 Morawska L, Johnson GR, Ristovski ZD, Hargreaves M, Mengersen K, Corbett S, *et al.* Size distribution and sites of origin of droplets expelled from the human respiratory tract during expiratory activities. *Journal of Aerosol Science* 2009;**40**:256-69.
- 31 Gregson FKA, Watson NA, Orton CM, Haddrell AE, McCarthy LP, Finnie TJR, *et al.* Comparing aerosol concentrations and particle size distributions generated by singing, speaking and breathing. *Aerosol Science and Technology* 2021:1-15.
- 32 Brown WA, Johari Halim Shah Y, Balalis G, Bashir A, Ramos A, Kow L, *et al.* IFSO Position Statement on the Role of Esophago-Gastro-Duodenal Endoscopy Prior to and after Bariatric and Metabolic Surgery Procedures. *Obesity Surgery* 2020;**30**:3135-53.
- 33 Shrimpton A, Gregson FKA, Cook TM, Brown J, Bzdek BR, Reid JP, *et al.* A quantitative evaluation of aerosol generation during tracheal intubation and extubation: a reply. *Anaesthesia* 2021;**76 Suppl 3**:16-8.
- 34 Widdicombe J, Fontana G. Cough: what's in a name? *Eur Respir J* 2006;**28**:10-5.
- 35 Prather KA, Marr LC, Schooley RT, McDiarmid MA, Wilson ME, Milton DK. Airborne transmission of SARS-CoV-2. *Science* 2020;**370**:303-4.
- 36 Tang JW, Bahnfleth WP, Bluysen PM, Buonanno G, Jimenez JL, Kurnitski J, *et al.* Dismantling myths on the airborne transmission of severe acute respiratory syndrome coronavirus-2 (SARS-CoV-2). *J Hosp Infect* 2021;**110**:89-96.
- 37 Greig JH, Cooper SM, Kasimbazi HJ, Monie RD, Fennerty AG, Watson B. Sedation for fibre optic bronchoscopy. *Respir Med* 1995;**89**:53-6.

38 Stolz D, Chhajed PN, Leuppi JD, Brutsche M, Pflimlin E, Tamm M. Cough suppression during flexible bronchoscopy using combined sedation with midazolam and hydrocodone: a randomised, double blind, placebo controlled trial. *Thorax* 2004;**59**:773-6.

39 Robinson JF, de Anda IR, Moore FJ, Gregson FKA, Reid JP, Husain L, *et al.* How effective are face coverings in reducing transmission of COVID-19? medRxiv 2020:DOI: 10.1101/2020.12.01.20241992.

FIGURE LEGENDS:

Figure 1

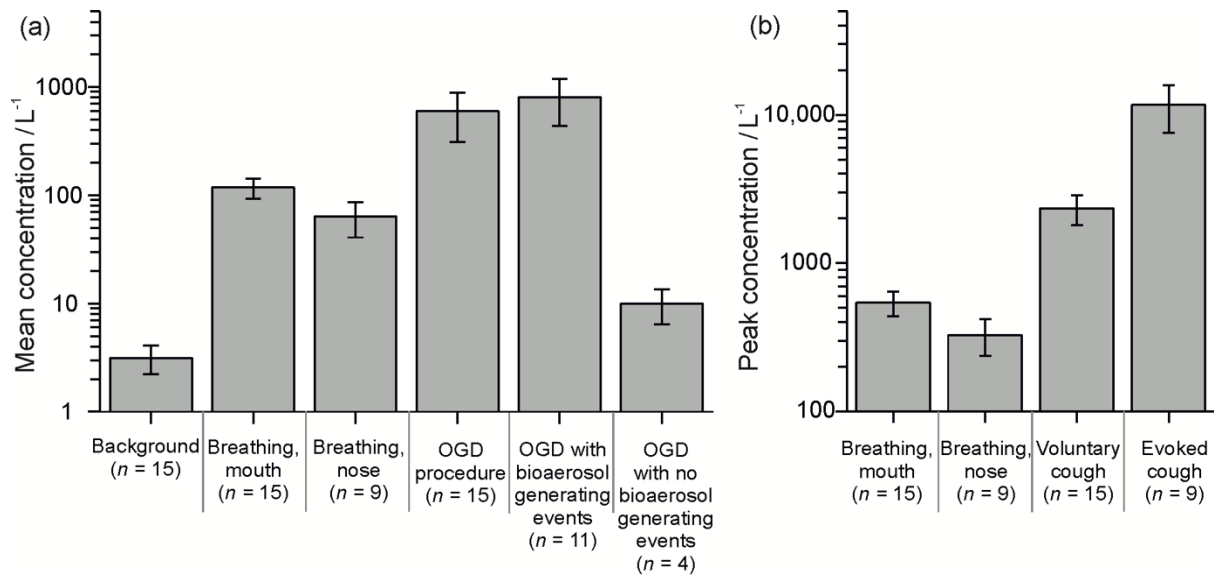


Figure 1. a) Mean particle concentrations and b) peak particle concentrations generated during the recording protocol. Note log scale for concentrations plotted as mean \pm SEM.

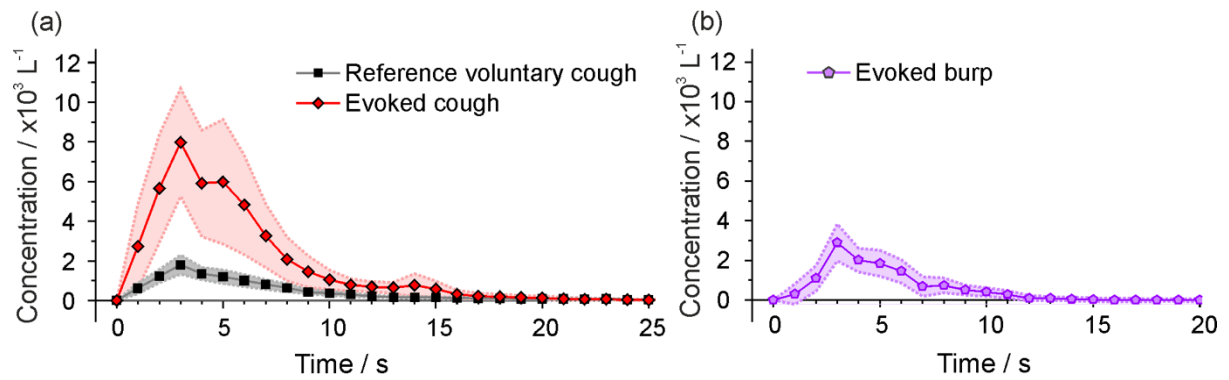
Figure 2

Figure 2 Mean particle concentration sampled during reference voluntary coughs (n=15 patients) overlaid with those for coughs evoked during OGD (n=9 patients) and burps observed during OGD (n=4 patients). The shaded region represents SEM.

Figure 3

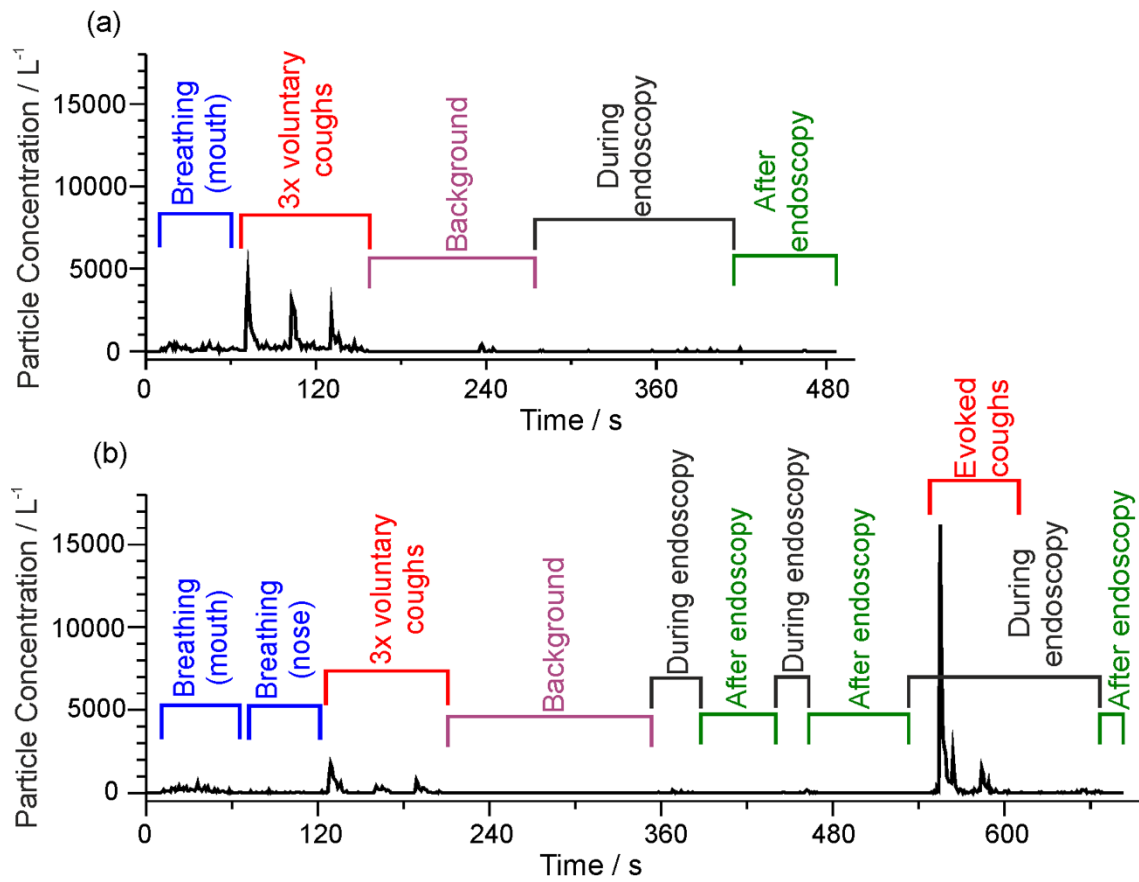


Figure 3 Continuous time series of aerosol detected during respiratory manoeuvres (tidal breathing and voluntary coughs) followed after a period of background monitoring by OGD

- Uneventful OGD without any significant aerosol generation.
- A more challenging endoscopy requiring multiple attempts at scope insertion which triggered coughing during the final episode

Figure 4

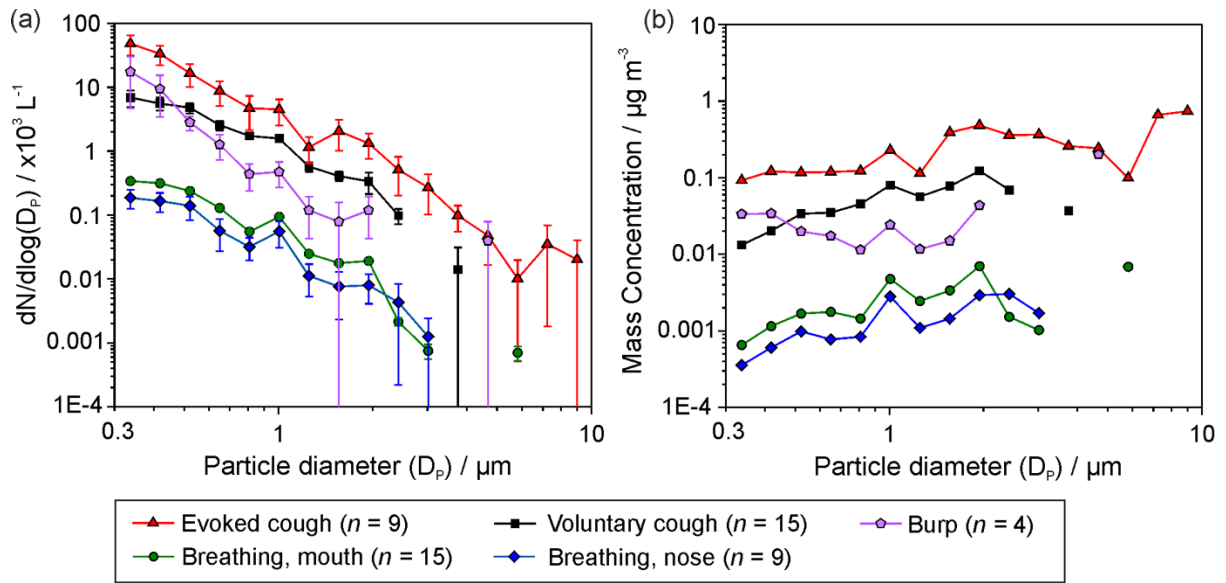


Figure 4 (a) Particle size distribution of the events. $dN/d\log(D_p)$ is the concentration sampled within each bin normalised by the logarithm of the bin width. The error bars represent the standard error of the mean. (b) The size distribution of the average aerosol concentration generated by each activity represented in terms of a mass concentration, calculated assuming unit density.

Figure 5

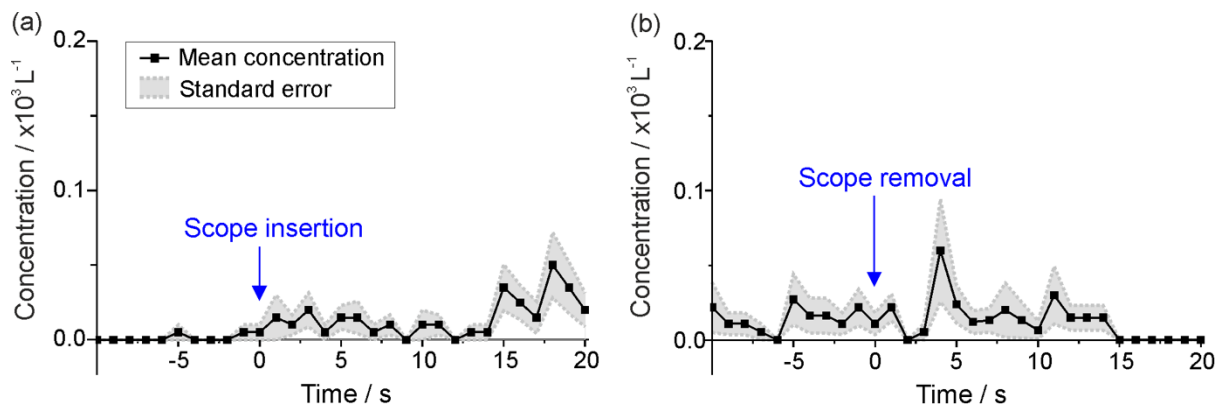


Figure 5 Profile of aerosol concentration detected during endoscope (a) insertion (n=12) (b) removal (n=11). A low mean concentration of aerosol was detected in the 30 second time period around endoscope insertion (10.3 (9.5) particles.L⁻¹) and removal (15.1 (12.4) particles.L⁻¹) where the concentrations were not significantly different to background. Note endoscope insertions (n=3) and removals (n=4) that immediately triggered coughing or burping (i.e. during this sampling window) were excluded from the pooled analysis.