

This is a repository copy of *An automated image analysis framework for segmentation and division plane detection of single live Staphylococcus aureus cells which can operate at millisecond sampling time scales using bespoke Slimfield microscopy.*

White Rose Research Online URL for this paper:
<https://eprints.whiterose.ac.uk/106182/>

Version: Published Version

Article:

Wollman, Adam J M orcid.org/0000-0002-5501-8131, Miller, Helen, Foster, Simon et al. (1 more author) (2016) An automated image analysis framework for segmentation and division plane detection of single live *Staphylococcus aureus* cells which can operate at millisecond sampling time scales using bespoke Slimfield microscopy. *Physical Biology*. 055002. ISSN 1478-3975

<https://doi.org/10.1088/1478-3975/13/5/055002>

Reuse

This article is distributed under the terms of the Creative Commons Attribution (CC BY) licence. This licence allows you to distribute, remix, tweak, and build upon the work, even commercially, as long as you credit the authors for the original work. More information and the full terms of the licence here:
<https://creativecommons.org/licenses/>

Takedown

If you consider content in White Rose Research Online to be in breach of UK law, please notify us by emailing eprints@whiterose.ac.uk including the URL of the record and the reason for the withdrawal request.

An automated image analysis framework for segmentation and division plane detection of single live *Staphylococcus aureus* cells which can operate at millisecond sampling time scales using bespoke Slimfield microscopy

This content has been downloaded from IOPscience. Please scroll down to see the full text.

View [the table of contents for this issue](#), or go to the [journal homepage](#) for more

Download details:

IP Address: 144.32.92.176

This content was downloaded on 18/10/2016 at 15:51

Please note that [terms and conditions apply](#).

You may also be interested in:

[Optical tweezers assisted imaging of the Z-ring in Escherichia coli: measuring its radial width](#)

G Carmon, P Kumar and M Feingold

[Timing of Z-ring localization in Escherichia coli](#)

R Tsukanov, G Reshes, G Carmon et al.

[Robustness of the division symmetry in Escherichia coli and functional consequences of symmetry breaking](#)

Abhishekh Gupta, Jason Lloyd-Price, Samuel M D Oliveira et al.

[Using bespoke fluorescence microscopy to study the soft condensed matter of living cells at the single molecule level](#)

Q Xue, O Harriman and M C Leake

[Timing the start of division in E. coli: a single-cell study](#)

G Reshes, S Vanounou, I Fishov et al.

[Consequences of lipidic nanoemulsions on membrane integrity and ultrastructural morphology of Staphylococcus aureus](#)

Neeru Singh, Saurabh Manaswita Verma, Sandeep Kumar Singh et al.

Physical Biology



PAPER

OPEN ACCESS

RECEIVED
8 March 2016

REVISED
18 August 2016

ACCEPTED FOR PUBLICATION
22 August 2016

PUBLISHED
17 October 2016

Original content from this work may be used under the terms of the [Creative Commons Attribution 3.0 licence](#).

Any further distribution of this work must maintain attribution to the author(s) and the title of the work, journal citation and DOI.



An automated image analysis framework for segmentation and division plane detection of single live *Staphylococcus aureus* cells which can operate at millisecond sampling time scales using bespoke Slimfield microscopy

Adam J M Wollman^{1,3}, Helen Miller^{1,3}, Simon Foster² and Mark C Leake¹

¹ Biological Physical Sciences Institute (BPSI), Departments of Physics and Biology, University of York, Heslington, York YO10 5DD, UK

² Krebs Institute, Department of Molecular Biology and Biotechnology, University of Sheffield, Sheffield S10 2TN, UK

³ Authors contributed equally.

E-mail: mark.leake@york.ac.uk

Keywords: fluorescence microscopy, fluorescent protein, image analysis

Supplementary material for this article is available [online](#)

Abstract

Staphylococcus aureus is an important pathogen, giving rise to antimicrobial resistance in cell strains such as Methicillin Resistant *S. aureus* (MRSA). Here we report an image analysis framework for automated detection and image segmentation of cells in *S. aureus* cell clusters, and explicit identification of their cell division planes. We use a new combination of several existing analytical tools of image analysis to detect cellular and subcellular morphological features relevant to cell division from millisecond time scale sampled images of live pathogens at a detection precision of single molecules. We demonstrate this approach using a fluorescent reporter GFP fused to the protein EzrA that localises to a mid-cell plane during division and is involved in regulation of cell size and division. This image analysis framework presents a valuable platform from which to study candidate new antimicrobials which target the cell division machinery, but may also have more general application in detecting morphologically complex structures of fluorescently labelled proteins present in clusters of other types of cells.

Introduction

The application of novel biophysics tools is generating important new insight into processes of infection [1–5]; in particular, biophysical instrumentation in the form of bespoke light microscopy hardware, and of bespoke image analysis software tools to extract meaningful information from the images that are generated in an often low signal-to-noise ratio regime, is generating promising new understanding of the biological mechanisms which underlie the process of antimicrobial resistance in a range of different pathogens. An example of such a pathogen relevant to human disease is *Staphylococcus aureus*, a bacterium that reproduces through binary fission into cellular clusters. *S. aureus* is a normal member of human skin microflora [6, 7] but causes serious infections on reaching underlying tissues. To study the process of *S. aureus* cell division,

we combined several existing image analysis tools into a new framework which, for the first time, was applied to living *S. aureus* pathogens imaged at millisecond time scales to single molecule detection precision using the bespoke biophysical optical imaging technique of Slimfield microscopy. This analysis framework enabled us to detect the cell division plane of individual cells, their boundaries and other subcellular morphological features.

S. aureus infection of skin and lung may lead to advanced systemic bacterial infection, or bacteraemia, a fatal condition if the strain is resistant to antibiotics [8]. Methicillin resistant *S. aureus* (MRSA) is resistant to beta-lactam antibiotics, such as those based on penicillins and cephalosporins, and most broad spectrum fluoroquinolones such as Ciprofloxacin [9, 10]. Antibiotic resistance is an enormous problem now in clinical treatment centres, especially so for surgical

procedures involving joint replacement and secondary infections arising following chemotherapy. MRSA can be treated currently with the glycopeptide vancomycin, however strains have recently been identified with reduced susceptibility to vancomycin [11] and even complete resistance [12], so-called VRSA. Many traditional antibiotics operate through targeting of cell wall components in invading microbes. For example, beta-lactam antibiotics inhibit cell wall synthesis of peptidoglycan to disrupt the cell's ability to withstand high osmotic cellular pressure. They bind irreversibly to the active site of penicillin binding proteins, preventing them from building cross links in the cell wall [13, 14]. Resistance to beta-lactam antibiotics is however prevalent, having evolved into strains which have binding sites with significantly reduced binding affinity to the antibiotics, or have developed new forms of enzymatic degradation of the beta-lactam motif [15]. Others such as the fluoroquinolones operate through targeting DNA replication. The process of cell division may present alternative molecular candidates for targeted disruption by newly developed antibiotics. However, cell division processes have been studied primarily in the model rod-shaped organisms *Bacillus subtilis* and *Escherichia coli*, which have less specific relevance to biomedically more harmful pathogens such as *S. aureus*.

Cell division in *S. aureus* is driven by a complex mix of several proteins, many essential, termed the divisome [16]. The protein FtsZ forms a ring structure at a future division site at mid-cell, known as the 'Z ring'. The exact role of many of the proteins involved in cell division, and the extent of their essential nature or not in different organisms, are unknown. The protein EzrA (denoted so for 'Extra Z rings A') is crucial in *S. aureus* [17, 18]. In *B. subtilis* EzrA acts as an inhibitor, preventing the formation of multiple Z rings per cycle, and EzrA is also recruited to the mid-cell early in the cell division process [19]. In *in vitro* assays, EzrA is observed to interact with the C terminus of FtsZ which prevents it from assembling the Z ring [20, 21]. The idea that an inhibitor of Z ring formation is recruited to the divisome is surprising, but in *S. aureus* EzrA was found to also regulate cell size [17, 18], preventing cells from getting so large that the Z ring could not form correctly. This agrees with the finding that in *S. aureus* inhibition of cell division produces cells up to twice as large as normal [17, 22].

The localisation of EzrA changes through the cell cycle. In *S. aureus*, EzrA is known to locate to the mid-cell and form a ring at the nascent division plane early in the division process [17, 23], during which period *S. aureus* becomes oblatelly ellipsoidal rather than truly spherical [24]. EzrA can therefore be used as a useful marker for the cell division plane in the early stages of cell division, without observing the cell division event itself and thus its identification may provide a useful platform from which to study antimicrobial activity

which affects cell division processes, or its absence in resistant strains.


Light microscopy has developed from its inception over 300 years ago into being an invaluable biophysical tool for studying complex biological processes in living cells [25]. Similarly, automated analytical and computational tools of theoretical biophysics are proving useful in the interpretation of new forms of imaging data [26, 27]. In particular, the use of fluorescence microscopy, and associated analyses of the resultant images for studying complex processes, has added much to our understanding of complex molecular architectures inside living cells. For example, our previous work in this area includes studying cellular bioenergetics [28–30], protein transport [33–35], DNA replication and repair [36, 37], cell movement and sensing [38–41], chromosome architecture [42–44] and developing new experimental and analytical imaging tools to probe general molecular machines in live cells at a single molecule precision [26, 45–53].

Earlier attempts at monitoring cell division processes in *S. aureus* used labour-intensive manual image segmentation methods [54], highly prone to user subjectivity. Other attempts have utilised super-resolution images on fixed (i.e. dead) cells [24], limiting the study of dynamic biological processes. Although several standard methods already exist for the rough segmentation of bacterial cell clusters and the simultaneous detection of fluorescence from a labelled intracellular protein [55, 56] these have never been applied to *S. aureus* cell clusters over a challenging millisecond time scale relevant to *in vivo* molecular mobility. Our image analysis framework uses fluorescence and brightfield image data as an input and interrogates these with automated image segmentation and watershed algorithms to detect individual *S. aureus* cells, determine the location of their cell walls, and identify cell division planes in cells containing fluorescently labelled EzrA. Importantly, these techniques can be applied to imaging data from Slimfield microscopy [4, 36, 37, 43, 49] which enables tracking of single-molecule complexes over millisecond time scales which are comparable to diffusive molecular mobility inside living cells [27, 57], as well as being compatible with advanced analytical methods which employ single cell copy number quantification through convolution modelling [58].

Methods

Cell strains

S. aureus cell strains SH1000 (the parental wild type strain used for native autofluorescence measurements) and SH1000 EzrA-GFP+ (EryR) were stored in glycerol frozen stocks at -80°C . Cell cultures were grown as detailed previously for these strains [17] in rich media TSB (Tryptic Soy Broth; 17 g Trypticase peptone, 3 g Phytone peptone, 5 g sodium chloride,



2.5 g Dibasic potassium phosphate, 2.5 g glucose, 1 l deionised water, pH 7.3) at 37 °C.

Fluorescence microscopy

We used a bespoke single-molecule fluorescence microscope constructed around the chassis of a Nikon TE2000 inverted microscope using a 100×1.49 NA oil immersion total internal reflection fluorescence (TIRF) objective lens (Nikon) and a *xyz* nano positioning stage (Nanodrive, Mad City Labs). Here we used fluorescence excitation from a 50 mW Obis 488 nm laser to excite GFP fluorescence. A dual-pass GFP/mCherry dichroic mirror with 20 nm transmission windows centred on 488 nm and 561 nm was used below the objective lens turret. The beam was expanded to generate Slimfield excitation of 10 μm full width at half maximum in the sample plane of excitation intensity 1.5 W cm^{-2} . Slimfield illumination operates by underfilling the back aperture of a high NA objective lens using a collimated laser beam [49]. Underfilling results in a conflated confocal volume in the sample plane which can be adjusted by changing the upstream beam expansion optics to be marginally larger than a single cell, or cluster of cells, as required. In doing so the local laser excitation intensity is high enough to permit millisecond time scale image sampling of entire single live cells or small groups of cells with no requirement for slow scanning, at a detection precision to detect single fluorescent protein molecules while still producing an emission signal above the level of camera readout noise [4, 36, 37, 49, 59]. The Slimfield beam intensity profile was measured directly in a separate experiment by


raster scanning in the focal plane while imaging a sample of 100 nm diameter fluorescent beads (Molecular Probes) immobilised to the coverslip surface. A high speed camera (Photometrix Evolve Delta) was used to image at 5 ms frame^{-1} (this is the time between consecutive frames, of which 0.6 ms is the ‘dead’ time in the 5 ms window during which the camera is unable to acquire data) with the magnification set at 80 nm per pixel. The microscope was controlled using Micro-Manager software [60].

Sample preparation and imaging

Microscope flow cells, or ‘tunnel slides’, for imaging were constructed from BK7 glass microscope slides (Fisher) and plasma-cleaned coverslips (Menzel Glaser) by laying two lines of double-sided tape (Scotch) approximately 5 mm apart on the slide and dropping a coverslip onto the tape and tapping down (avoiding the imaging region), to produce a watertight linear channel [41]. The tunnel slide was coated in 0.01% poly-L-lysine to immobilise cells, and inverted for 5 min. This was then flushed through with 200 μl phosphate buffered saline (PBS). Following this, a tunnel volume of cells were flushed through and the slide was left inverted for 5 min to allow cells to attach to the coverslip. After 5 min any unattached cells were washed out with 200 μl PBS buffer prior to Slimfield imaging (figure 1).

Imaging analysis framework—(1) Image segmentation of cells


Brightfield and fluorescence images were segmented initially by simple pixel thresholding. Here, we defined



the background intensity from the modal (i.e. peak) value of the pixel intensity histogram as follows. The density of cells in a tunnel slide was optimised such that there were typically >80% more background pixels than foreground pixels (i.e. those associated with cells) (figures 2(a) and (b)). This ensured a distinct modal peak in the pixel intensity histogram corresponding to the first fluorescence image in a kinetic series, which was associated with the local background value. We then used an automated thresholding method to find the pixel intensity values which were greater than the background peak value plus one full width half maximum (FWHM) of the background peak itself as a simple and automated initial method to discriminate the background from the foreground cell-containing regions, which contained one or more commonly more (up to ~10 cells) in a cluster in

fluorescence images (figure 2(c)). In the case of simple isolated single cells standard morphological transformations can in principle be used to fill holes in segmented regions and remove small objects and single pixels [58], however in general *S. aureus* cells appear in clusters, requiring further image segmentation.

Our simple brightfield images are slightly defocused by a few hundred nm compared to fluorescence images to provide greater image contrast, resulting in a dark ring appearance around the perimeter of cells which results in under segmentation artefacts if the simple pixel thresholding method is applied (figure 2(d)). Segmenting the fluorescence image is advantageous as there is typically a low-level, uniform autofluorescence in cells due to the presence of natively fluorescent flavins and nucleotide derivatives



[41, 43, 58] which gives a more accurate boundary between the cell image and the background [58]. The disadvantage of this method is that close-packed cells, such as the clusters typical of *S. aureus*, are normally manifest as often contiguous regions of very similar pixel intensity since the cells are not separated by clear regions of background intensity (figure 3(c)). For elongated objects standard methods to separate overlapping cells with cell-background boundaries exist [61]; however, for cells with only cell-cell boundaries we found that using the brightfield segmentation outputs (figure 3(d)) to define primary seeds in a watershedding algorithm allowed the separate cell boundaries to be determined accurately.

We developed software implementing these algorithms written in MATLAB (Mathworks) which automatically determined the segmentation pixel thresholds of the fluorescence image and brightfield image to determine images masks corresponding to the spatial extent of individual cell clusters (figure 2(c)), and individual cell seeds for watershedding (figure 2(d)) respectively. The watershedding algorithm estimates which pixels are associated with each individual cell in a cell cluster (figure 2(e)). This raw pixelated watershed segmentation output is then modelled as a 2D ellipse function, with fitting optimisation generating estimates for the minor and major axes, centroid position and orientation of each segmented cell region (figure 2(f)).

Watershedding algorithms derive their name from the concept of river catchment basins; the areas of land from which surface water will drain into that river. The ridges in the landscape form dividers (or watersheds) between adjacent catchment basins. Our primary image segmentation step uses the

autofluorescence signal of the cells to first determine the outer boundaries of cell clusters, and we then apply a watershedding algorithm to find the borders of the individual cells within each cluster. By inverting the pixel values of the fluorescence image we generate a contour map such that the positions of the centres of cells correspond to valleys and the ridges between the valleys mark the cell boundaries (figure 3).

The pixel positions of each cell centre determined from simple brightfield segmentation are, in the case of *S. aureus* cell clusters, good estimates for the minima of the valleys, the seeds, but several alternative automated methods could in principle also be used to determine their locations [62]. The watersheds can now be found by progressively flooding the landscape until the cell regions defined by the seeds merge [62, 63]. Each seed pixels' eight neighbouring pixels are then sorted from lowest pixel intensity value (i.e. pixels which are most similar to the seed, or, in the analogy of the river basin, closest to the bottom of the valley) to highest. Pixels are considered in turn by looking at which of their eight neighbours have already been assigned to a cell. If a pixel's only labelled neighbours have all been assigned to the same cell it is also assigned to that cell, and its unassigned neighbours are added to the queue at their appropriate heights. If a pixel has two neighbours with different cell assignments, it is considered to lie on the boundary between them, and is therefore defined as part of the watershed. This process is repeated until all pixels in the region have been assigned uniquely to one cell, and a separate 2D ellipse function fit is then applied solely to the pixels within each watershed-defined cellular region.

Imaging analysis framework—(2) Thresholding inside cells (determining EzrA ring localisation)

Once the pixels corresponding to single cell foreground images have been identified, as above, it is relatively easy to threshold again inside these segmented cell images. Here, we used Otsu's method [64]. Otsu's method is a robust, standard approach which aims to separate a general distribution of values of a parameter into a number of classes through the process of minimising the intra-class variance. In our case here the parameter is that of pixel intensity, and we assume in the simplest hypothesis for there being just two classes, one which corresponds to putative EzrA rings and is manifest as a higher mean pixel intensity due to distinct fluorescently labelled EzrA rings tightly packed at the cell mid-plane, and a second class which comprises more diffusive components of lower mean pixel intensity which corresponds to a combination of background autofluorescence and rapidly diffusing EzrA subunits prior to association with a ring structure. To threshold an image ideally there would be two well separated peaks on the pixel intensity distribution. However, in reality, especially in the case of low signal-to-noise regimes of millisecond Slimfield microscopy, the valley between the two peaks is typically not clearly defined, due to imaging noise and differences in foreground and background pixel distributions. Otsu's method performs well under these conditions, and also offers advantages over other methods such as fitting Gaussian functions [65] or valley sharpening [66] as the peaks are rarely symmetrical Gaussian shapes, and valley sharpening only considers a highly localised area of the distribution, rather than all of the data in an image. GFP labelled EzrA rings appear as relatively brighter objects on a darker cell body background, and so are well suited to Otsu's method with just a single threshold.

Imaging analysis framework—(3) Simulating brightfield and fluorescence images

To validate our approach for segmenting the outer cellular boundaries and subcellular morphological features, exemplified by GFP-labelled EzrA rings, we simulated realistic brightfield and fluorescence images of *S. aureus* cells. These included image features of distinct EzrA-GFP rings, a subcellular diffusive background of EzrA-GFP, and a background not associated with GFP which comprised autofluorescence plus camera readout background. Cell background and EzrA-GFP ring fluorescence were modelled by adapting a previously reported method [58] for integrating a model point spread function over a $0.8\ \mu\text{m}$ diameter sphere (figure 4(a)) and a randomly orientated, parallel or perpendicular ring (figure 4(b)) of diffraction limited width (here set at $0.3\ \mu\text{m}$) respectively. Here, we retained the same basic tightly packed pattern and relative orientations of 7 cells in a cluster throughout.



The spacing between cells in cell clusters was not observed to vary in our experimental data and so was not varied in our simulations. These images were summed (figure 4(c)) and then scaled to realistic pixel intensity values, measured from mean pixel intensity inside cells in fluorescence images (supplementary information), before realistic levels of pixel noise, trained on experimental fluorescence image data, were added (figure 4(d)). Brightfield images (figure 4(e)) were simulated by subtracting $0.8\ \mu\text{m}$ diameter rings and circles from each other to generate bright central regions surrounded by dark rings, and were added to a uniform bright background. Images were then segmented using precisely the same algorithms and same parameter set as for real experimental image data (figures 4(f)–(h)).

Results

Segmenting cells

Candidate automatically detected cell masks were accepted for subsequent image analysis if the summed pixel area was in the range $0.03\text{--}3.00\ \mu\text{m}^2$; this is the equivalent area of a circle whose diameter is in the range $0.2\text{--}2\ \mu\text{m}$, which tallies with prior structural observations of the length scale of *S. aureus* cells during their complete cell cycle. In our proof-of-concept study here this resulted in accepting $\sim 60\%$ of initially detected candidate foreground objects (here, 34 out of 60 initially detected foreground objects from 20 separate fields of view). Example cell boundaries found are shown in figure 5. Most cell boundaries are slightly elliptical (figures 5(a), (b) and (d)) with aspect ratios (ratio of major and minor axis length) close to 1, but a minority had extended boundaries detected with larger aspect ratios closer to 2 (figure 5(c)). These examples with extended boundaries are consistent with the appearance of pairs of dividing cells which have been erroneously segmented together as a single cell.


The mean cell length we measure to be $1.2 \pm 0.3\ \mu\text{m}$ (\pm s.d.) (figure 6(a)), in good agreement to within experimental error with estimates [67, 68], though as noted from super-resolution studies there can be significant variation of cell length depending on the specific stage in the cell cycle [24]. The majority of our data have a major axis which is 30%–50% longer than the minor axis, indicating a mean cell aspect ratio of 1.4 ± 0.3 (figures 6(b) and (c)). The recent super-resolution investigations of Monteiro *et al* [24] made measurements of the aspect ratio and cell dimensions using structured illumination microscopy images of vancomycin-labelled peptidoglycan in *S. aureus*. Here they measured similar ranges of aspect ratio (1.1–1.4), close to within experimental error for cells in the P2 and P3 phases when the cells were dividing and EzrA was located at the division plane. Our measured aspect ratio was not divided into division

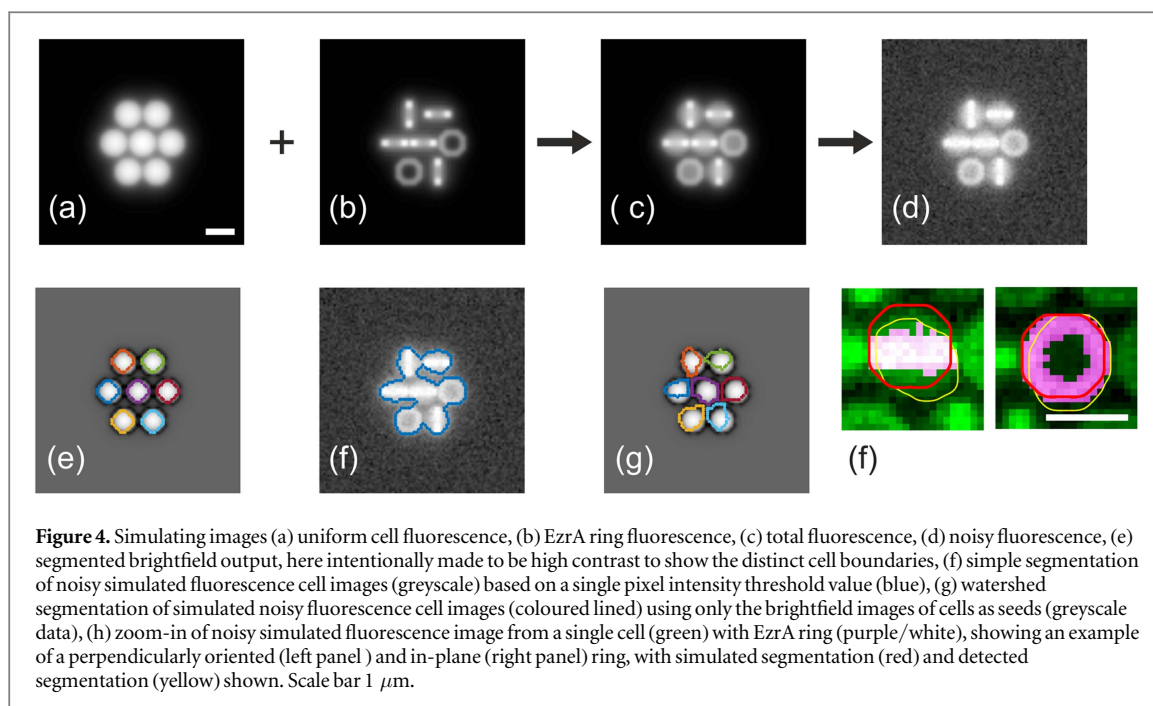

phases and is at the higher end of the range measured by Monteiro *et al* possibly indicating our cells spent longer in the P2 and P3 division phases in our growth and imaging conditions.

We used simulations to determine the cell boundary determination error of our image analysis framework, defined as the mean deviation of the cell boundary from the watershedded boundary. The deviation for any point on the detected boundary is defined as the absolute value of the shortest distance between the simulated and detected boundary.

Figure 6(d) shows the distribution of boundary errors for 70 simulated cells with different levels of simulated intensity and random normally distributed pixel intensity noise (supplementary information). Experimentally measured pixel intensity values for cells had a standard deviation of as much as $\sim 50\%$ of the mean cell background pixel intensity, but with a more typical level of $\sim 20\%$. In our simulations we found that although brightness variation does generate more outliers the boundary determination was relatively insensitive to these relatively large fluctuations in pixel

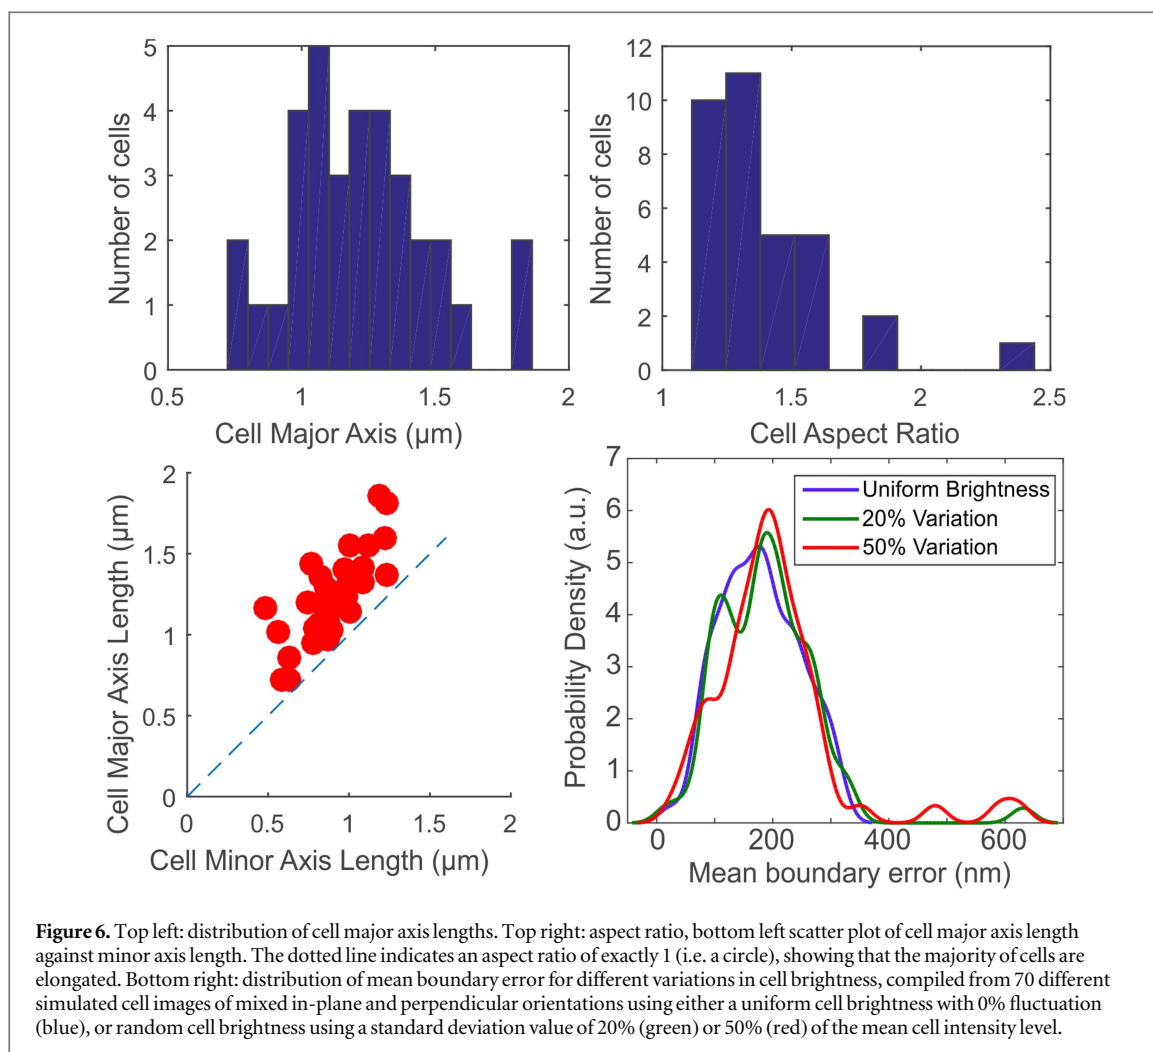


intensity, culminating in a typical boundary precision in the range 100–300 nm.

In our simulations, 100% of cells were detected successfully. However, in real experimental data the same image analysis framework rejected up to ~40% of initially detected candidate foreground objects. Failure to detect cells may occur in principle when insufficient fluorescence signal is present, or if there is some misalignment between the brightfield and fluorescence images, or if the measured cell mask area is beyond the imposed area acceptance range limit. We observed examples of all three categories in our data. Gene expression both for the EzrA protein and for natively autofluorescent proteins is stochastic in nature, and so there will inevitably be a minority of cells which have low intrinsic levels of fluorescence too close to the level of camera readout noise to permit robust image segmentation. Longer exposure times to increase cell signal above background noise might increase cell detection efficiency of these dim cells at the expense of time resolution but would not enhance the software's ability to distinguish very close cells as this information comes from segmenting the brightfield image. Similarly, misalignment between fluorescence and brightfield images more commonly occurs

when using differential interference contrast (DIC), since a Wollaston prism slider is placed just under the objective lens and can often result in mechanical based misalignment of the sample (e.g. slight knocks on the sample stage) in addition to the polarization optics resulting in a lateral shift of the image on the camera detector. Although DIC was not used here, we included some accidentally misaligned data intentionally (as revealed upon close inspection of figure 2 for example) to demonstrate that our image analysis framework is in general sufficiently robust to cope with minor misalignment issues.

The most relevant rejection category we found for our data was on the basis of the area acceptance range limit. Here, we set the upper limit to correspond to an effective cell diameter of 2 μm to therefore exclude the majority of clusters of >1 cell which our algorithm had failed to segment into individual cells. The majority of rejected cell masks were of this type. However, some were rejected by being less than the lower area limit threshold, equivalent to an effective cell diameter of 0.2 μm . These included images which were consistent with being cell fragments from dead cells, however there were also a minority of instances in which the primary segmentation step would detect the

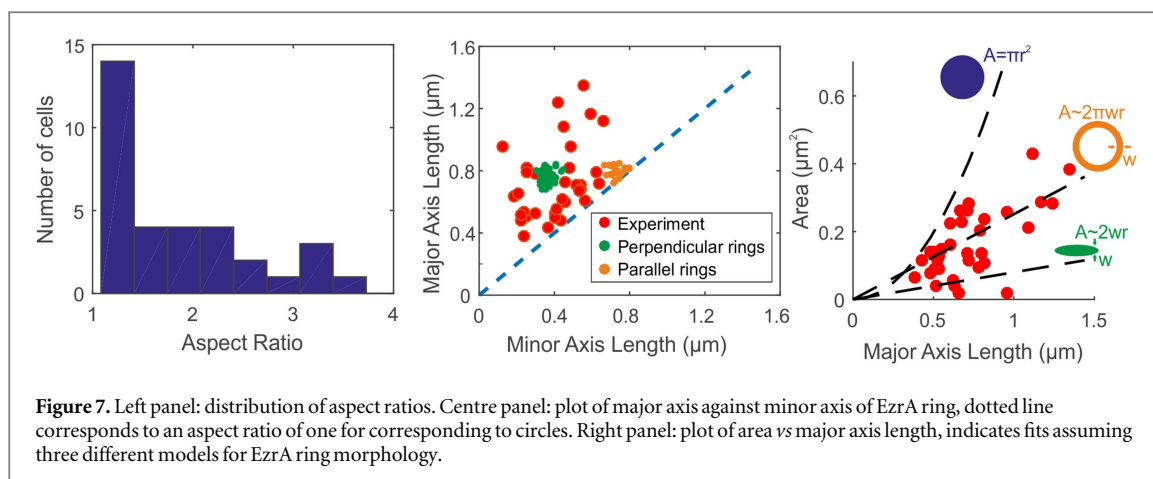

outline of the EzrA ring itself as opposed to the outline of the cell boundary—these were instances of a minority of cells which had a much lower intrinsic level of fluorescence for the cell background. These detection limits do not preclude using our image analysis framework for determination of cell lineages, since the same 60% acceptance level, is not random and will be propagated over time such that the same 40% of cells may be missed in each frame if these cells maintain the properties discussed above which would exclude them from the analysis. And it should be noted that our aim here was not to achieve 100% detection efficiency, but rather to intentionally have a stricter acceptance policy to increase the confidence for data interpretation of the accepted segmented cell images.

Identifying EzrA rings

A range of different shaped regions of fluorescently labelled EzrA can be found by applying pixel thresholding inside the cellular boundary regions (figure 3). Elliptical fits to these regions produce some thin extended ellipses but also more circular fits. The distribution of aspect ratios of these pixel regions and a scatter plot of major against minor axis length (figures 7(a) and (b)) show that $\sim 50\%$ of cells have extended structures with aspect ratios far in excess of 1, almost as high as 4, consistent with EzrA rings perpendicularly oriented to the image plane. We confirmed this by using simulations of perpendicularly oriented and in-plane rings. Unlabelled (wild type) cells, do not contain any visible rings in fluorescence image (supplementary figure 1). The line profile through a putative in-plane ring shows a clear double peak (figure 5(e)), as would be expected. The remaining structures are more circular, either corresponding to in-plane rings or a completely delocalised diffusive EzrA-GFP. These can be distinguished on the basis of their estimated areas as a function of major axis length, which accounts for cell orientation projection effects onto the camera detector. Figures 7(c) summarises, from simple geometrical considerations, how the area, A , varies as a function of major axis

length, $2r$, for a fixed diffraction limited ring width, w , for a continuous circular region as produced by delocalised diffusive EzrA-GFP molecules, an in-plane ring and an ellipse produced by a perpendicularly oriented EzrA-GFP ring. Most of the accepted cell foreground objects are consistent with the presence of a ring, although a few are consistent with continuous but truncated localised EzrA-GFP structures, indicative more of short protofilaments than rings, and suggesting that these cells are not actively dividing.

Discussion

Our straightforward image analysis framework detects cells and characterises their size and shape assuming an ellipsoidal model for the general 3D shape of *S. aureus* cells, manifest as a 2D ellipse on an image projection. It then detects bright pixels inside the cell corresponding to EzrA rings, characterises their shape and determines their orthogonality to the image plane. Our method is valuable for investigating *S. aureus* cells, which do not move apart following the conclusion of the cell division process. The analysis framework can be extended to study other fluorescently labelled proteins in *S. aureus*, but also in other clustering cells since it does not require the foreground objects to be spatially separated by regions of background pixels. The watershed method, which here uses bright-field cell centres as seeds, is robust to imaging data for which the brightfield image is not precisely aligned with the fluorescence image. Here, we are not claiming to have developed any single novel image segmentation method *per se*—our image analysis framework here uses existing, standard methods, quite clearly. Rather, we use these in combination to create a framework which has previously never been applied to challenging data from millisecond images of live cells which have morphologically heterogenous subcellular features, as exemplified by the pathogen *S. aureus* with subcellular EzrA ring structures.

The aspect ratios we find for cells are in agreement with those found by Monteiro *et al* [24], indicating

that super-resolution imaging is not necessarily required to extract this parameter. Using the auto-fluorescence of the cell potentially leaves other spectrally delimited channels open for protein studies (i.e. multi-colour fluorescence imaging). We find EzrA rings are localised to the division plane in agreement with the expected distributions during cell division.

Other studies have required manual segmentation [54] or relied on super-resolution images [24] to achieve similar results. Our simple framework is fully automated and does not require costly and potentially damaging super-resolution imaging. However it is still compatible with super-resolution microscopy images, but also with millisecond microscopy such as Slimfield illumination as well as other time-resolved fluorescence localisation microscopy tools which enable tracking of single-molecule complexes [27, 57, 69], for example to enable quantification of protein copy number in Erza rings using convolution modelling [58].

Conclusion

We have constructed a simple bespoke automated image analysis framework using a combination of several standard approaches which enables segmentation of individual *S. aureus* live cell images within cell clusters, and can detect the cell division planes using fluorescently labelled EzrA protein as a marker, from millisecond sampled images. The framework can be used to investigate cell aspect ratios, other labelled proteins that may be involved in division in *S. aureus*, and it may also have wider applicability for studying other clustering cells since it does not require cells to be separated by non-cellular background pixels. *S. aureus* is an increasing healthcare problem, particularly methicillin resistant and vancomycin resistant strains. It thus has value towards gaining new insight into the operating mechanism of cell division to facilitate the development of future new cell division targeting antibiotics.

Acknowledgments

We acknowledge technical assistance for cell preparation (Robert Turner) and image acquisition (Richard Nudd). The research was supported by the White Rose Consortium (WRC), the Biological Physical Sciences Institute (BPSI), University of York and the Medical Research Council (grant number MR/K01580X/1).

References

- [1] Leake M C 2016 The biophysics of infection *Adv. Exp. Med. Biol.* **915** 1–3
- [2] Zhou Z and Leake M C 2016 Force spectroscopy in studying infection *Adv. Exp. Med. Biol.* **915** 307–27
- [3] Miller H, Wollman A J M and Leake M C 2016 Designing a single-molecule biophysics tool for characterising DNA damage for techniques that kill infectious pathogens through DNA damage effects *Adv. Exp. Med. Biol.* **915** 115–27
- [4] Wollman A J M, Syeda A H, McGlynn P and Leake M C 2016 Single-molecule observation of DNA replication repair pathways in *E. coli* *Adv. Exp. Med. Biol.* **915** 5–16
- [5] Leake M C 2016 Biophysics of Infection. Preface *Adv. Exp. Med. Biol.* **915** (accepted)
- [6] Kluytmans J, van Belkum A and Verbrugh H 1997 Nasal carriage of *Staphylococcus aureus*: epidemiology, underlying mechanisms, and associated risks *Clin. Microbiol. Rev.* **10** 505–20
- [7] Gorwitz R J *et al* 2008 Changes in the prevalence of nasal colonization with *Staphylococcus aureus* in the United States, 2001–2004 *J. Infect. Dis.* **197** 1226–34
- [8] Tong S Y C, Davis J S, Eichenberger E, Holland T L and Fowler V G 2015 *Staphylococcus aureus* infections: epidemiology, pathophysiology, clinical manifestations, and management *Clin. Microbiol. Rev.* **28** 603–61
- [9] Foster J, Lentino J, Strodtman R and Divincenzo C 1986 Comparison of *in vitro* activity of quinolone antibiotics and vancomycin against gentamicin-resistant and methicillin-resistant *Staphylococcus aureus* by time-kill kinetic studies *Antimicrob. Agents Chemother.* **30** 823–7
- [10] Miller H, Wollman A J M and Leake M C 2016 Designing a single-molecule biophysics tool for characterizing DNA damage for techniques that kill infectious pathogens through DNA damage effects *Adv. Exp. Med. Biol.* **915** 115–27
- [11] Hiramatsu K *et al* 1997 Dissemination in Japanese hospitals of strains of *Staphylococcus aureus* heterogeneously resistant to vancomycin *Lancet* **350** 1670–3
- [12] Koch G *et al* 2014 Evolution of resistance to a last-resort antibiotic in *Staphylococcus aureus* via bacterial competition *Cell* **158** 1060–71
- [13] Waxman D J and Strominger J L 1983 Penicillin-binding proteins and the mechanism of action of beta-lactam antibiotics *Annu. Rev. Biochem.* **52** 825–69
- [14] Neu H C 1992 The crisis in antibiotic resistance *Science* **257** 1064–73
- [15] Chambers H F and Deleo F R 2009 Waves of resistance: *Staphylococcus aureus* in the antibiotic era *Nat. Rev. Microbiol.* **7** 629–41
- [16] Bottomley A L, Kabli A F, Hurd A F, Turner R D, Garcia-Lara J and Foster S J 2014 *Staphylococcus aureus* DivIB is a peptidoglycan-binding protein that is required for a morphological checkpoint in cell division *Mol. Microbiol.* **94** 1041–64
- [17] Steele V R, Bottomley A L, Garcia-Lara J, Kasturiarachchi J and Foster S J 2011 Multiple essential roles for EzrA in cell division of *Staphylococcus aureus* *Mol. Microbiol.* **80** 542–55
- [18] Jorge A M, Hoiczuk E, Gomes J P and Pinho M G 2011 EzrA contributes to the regulation of cell size in *Staphylococcus aureus* *PLoS One* **6** e27542
- [19] Levin P A, Kurtser I G and Grossman A D 1999 Identification and characterization of a negative regulator of FtsZ ring formation in *Bacillus subtilis* *Proc. Natl Acad. Sci.* **96** 9642–7
- [20] Haeusser D P, Schwartz R L, Smith A M, Oates M E and Levin P A 2004 EzrA prevents aberrant cell division by modulating assembly of the cytoskeletal protein FtsZ *Mol. Microbiol.* **52** 801–14
- [21] Singh J K, Makde R D, Kumar V and Panda D 2007 A membrane protein, EzrA, regulates assembly dynamics of FtsZ by interacting with the C-terminal tail of FtsZ *Biochemistry Am. Chem. Soc.* **46** 11013–22
- [22] Pinho M G and Errington J 2003 Dispersed mode of *Staphylococcus aureus* cell wall synthesis in the absence of the division machinery *Mol. Microbiol.* **50** 871–81
- [23] Pereira P M, Veiga H, Jorge A M and Pinho M G 2010 Fluorescent reporters for studies of cellular localization of proteins in *Staphylococcus aureus* *Appl. Environ. Microbiol.* **76** 4346–53

- [24] Monteiro J M *et al* 2015 Cell shape dynamics during the staphylococcal cell cycle *Nat. Commun.* **6** 8055
- [25] Wollman A J M, Nudd R, Hedlund E G and Leake M C 2015 From animaculum to single molecules: 300 years of the light microscope *Open Biol.* **5** 150019
- [26] Leake M C 2014 Analytical tools for single-molecule fluorescence imaging in cellulose *Phys. Chem. Chem. Phys.* **16** 12635–47
- [27] Wollman A J M, Miller H, Zhou Z and Leake M C 2015 Probing DNA interactions with proteins using a single-molecule toolbox: inside the cell, in a test tube and in a computer *Biochem. Soc. Trans.* **43** 139–45
- [28] Lenn T, Leake M C and Mullineaux C W 2008 Clustering and dynamics of cytochrome bd-I complexes in the *Escherichia coli* plasma membrane *in vivo* *Mol. Microbiol.* **70** 1397–407
- [29] Lenn T, Leake M C and Mullineaux C W 2008 Are *Escherichia coli* OXPPOS complexes concentrated in specialized zones within the plasma membrane? *Biochem. Soc. Trans.* **36** 1032–6
- [30] Llorente-Garcia I *et al* 2014 Single-molecule *in vivo* imaging of bacterial respiratory complexes indicates delocalized oxidative phosphorylation *Biochim. Biophys. Acta* **1837** 811–24
- [31] Bryan S J *et al* 2014 Localisation and interactions of the Vipp1 protein in cyanobacteria *Mol. Microbiol.* (doi:10.1111/mmi.12826)
- [32] Lenn T and Leake M C 2016 Single-molecule studies of the dynamics and interactions of bacterial OXPPOS complexes *Biochim. Biophys. Acta* **1857** 224–31
- [33] Leake M C *et al* 2008 Variable stoichiometry of the TatA component of the twin-arginine protein transport system observed by *in vivo* single-molecule imaging *Proc. Natl Acad. Sci. USA* **105** 15376–81
- [34] Robson A, Burrage K and Leake M C 2013 Inferring diffusion in single live cells at the single-molecule level *Philos. Trans. R. Soc. B* **368** 20120029
- [35] Nenninger A *et al* 2014 Independent mobility of proteins and lipids in the plasma membrane of *Escherichia coli* *Mol. Microbiol.* **92** 1142–53
- [36] Reyes-Lamothe R, Sherratt D J D J and Leake M C M C 2010 Stoichiometry and architecture of active DNA replication machinery in *Escherichia coli* *Science* **328** 498–501
- [37] Badrinarayanan A, Reyes-Lamothe R, Uphoff S, Leake M C M C and Sherratt D J D J 2012 *In vivo* architecture and action of bacterial structural maintenance of chromosome proteins *Science* **338** 528–31
- [38] Lo C-J, Leake M C and Berry R M 2006 Fluorescence measurement of intracellular sodium concentration in single *Escherichia coli* cells *Biophys. J.* **90** 357–65
- [39] Lo C-J, Leake M C, Pilizota T and Berry R M 2007 Nonequivalence of membrane voltage and ion-gradient as driving forces for the bacterial flagellar motor at low load *Biophys. J.* **93** 294–302
- [40] Chiu S-W, Roberts M A J, Leake M C and Armitage J P 2013 Positioning of chemosensory proteins and FtsZ through the Rhodobacter sphaeroides cell cycle *Mol. Microbiol.* **90** 322–37
- [41] Leake M C, Chandler J H, Wadhams G H, Bai F, Berry R M and Armitage J P 2006 Stoichiometry and turnover in single, functioning membrane protein complexes *Nature* **443** 355–8
- [42] Badrinarayanan A and Leake M C 2016 Using fluorescence recovery after photobleaching (FRAP) to study dynamics of the structural maintenance of chromosome (SMC) complex *in vivo* *Methods Mol. Biol.* **1431** 37–46
- [43] Wollman A J M and Leake M C 2016 Single molecule narrowfield microscopy of protein-DNA binding dynamics in glucose signal transduction of live yeast cells *Methods Mol. Biol.* **1431** 5–15
- [44] Leake M C 2016 New advances in chromosome architecture *Methods Mol. Biol.* **1431** 1–3
- [45] Dobbie I M, Robson A, Delalez N and Leake M C 2009 Visualizing single molecular complexes *in vivo* using advanced fluorescence microscopy *J. Vis. Exp.* **31** 1508
- [46] Chiu S-W and Leake M C 2011 Functioning nanomachines seen in real-time in living bacteria using single-molecule and super-resolution fluorescence imaging *Int. J. Mol. Sci.* **12** 2518–42
- [47] Lenn T and Leake M C 2012 Experimental approaches for addressing fundamental biological questions in living, functioning cells with single molecule precision *Open Biol.* **2** 120090
- [48] Leake M C 2010 Shining the spotlight on functional molecular complexes: the new science of single-molecule cell biology *Commun. Integr. Biol.* **3** 415–8
- [49] Plank M, Wadhams G H and Leake M C 2009 Millisecond timescale slimfield imaging and automated quantification of single fluorescent protein molecules for use in probing complex biological processes *Integr. Biol.* **1** 602–12
- [50] Harriman O L J and Leake M C 2011 Single molecule experimentation in biological physics: exploring the living component of soft condensed matter one molecule at a time *J. Phys. Condens. Matter* **23** 503101
- [51] Leake M C 2013 The physics of life: one molecule at a time *Philos. Trans. R. Soc. B* **368** 20120248
- [52] Leake M C, Wadhams G H and Armitage J P 2008 Parts exchange: why molecular machines are like used cars *Biologist.* **55** 33–9
- [53] Cordes T *et al* 2015 Plasmonics, Tracking and Manipulating, and Living Cells: general discussion *Faraday Discuss.* **184** 451–73
- [54] Wheeler R, Mesnage S, Boneca I G, Hobbs J K and Foster S J 2011 Super-resolution microscopy reveals cell wall dynamics and peptidoglycan architecture in ovococcal bacteria *Mol. Microbiol.* **82** 1096–109
- [55] Rosenfeld N, Young J W, Alon U, Swain P S and Elowitz M B 2005 Gene regulation at the single-cell level *Science* **307** 1962–5
- [56] Sliusarenko O, Heinritz J, Emonet T and Jacobs-Wagner C 2011 High-throughput, subpixel precision analysis of bacterial morphogenesis and intracellular spatio-temporal dynamics *Mol. Microbiol.* **80** 612–27
- [57] Miller H, Zhou Z, Wollman A J M and Leake M C 2015 Superresolution imaging of single DNA molecules using stochastic photoblinking of minor groove and intercalating dyes *Methods* **88** 81–8
- [58] Wollman A J M and Leake M C 2015 Millisecond single-molecule localization microscopy combined with convolution analysis and automated image segmentation to determine protein concentrations in complexly structured, functional cells, one cell at a time *Faraday Discuss.* **184** 401–24
- [59] Sonnleitner A, Schütz G J and Schmidt T 1999 Free Brownian motion of individual lipid molecules in biomembranes *Biophys. J.* **77** 2638–42
- [60] Edelstein A, Amodaj N, Hoover K, Vale R and Stuurman N 2010 Computer control of microscopes using μ Manager *Curr. Protoc. Mol. Biol.* (ch 14: unit14.20) (doi:10.1002/2F0471142727.mb1420s92)
- [61] Xue Q, Jones N S and Leake M C 2010 A general approach for segmenting elongated and stubby biological objects: extending a chord length transform with the radon transform *Proc. 2010 IEEE Int. Symp. on Biomedical Imaging: From Nano to Macro* pp 161–4 ISBI 2010
- [62] Meyer F 1994 Topographic distance and watershed lines *Signal Process.* **38** 113–25
- [63] Vincent L and Soille P 1991 Watersheds in digital spaces: an efficient algorithm based on immersion simulations *IEEE Trans. Pattern Anal. Mach. Intell.* **13** 583–98
- [64] Otsu N 1979 A threshold selection method from gray-level histograms *IEEE Trans. Syst. Man Cybern.* **9** 62–6
- [65] Chow C K and Kaneko T 1972 Automatic boundary detection of the left ventricle from cineangiograms *Comput. Biomed. Res.* **5** 388–410

- [66] Weszka J S, Nagel R N and Rosenfeld A 1974 A threshold selection technique *IEEE Trans. Comput.* **C-23** 1322–6
- [67] Touhami A, Jericho M H and Beveridge T J 2004 Atomic force microscopy of cell growth and division in *Staphylococcus aureus* *J. Bacteriol.* **186** 3286–95
- [68] Bailey R G, Turner R D, Mullin N, Clarke N, Foster S J and Hobbs J K 2014 The interplay between cell wall mechanical properties and the cell cycle in *Staphylococcus aureus* *Biophys. J.* **107** 2538–45
- [69] Xue Q and Leake M C 2009 A novel multiple particle tracking algorithm for noisy *in vivo* data by minimal path optimization within the spatio-temporal volume *Proc. 2009 IEEE Int. Symp. on Biomedical Imaging: From Nano to Macro* pp 1158–61 ISBI 2009