

Southern Illinois University Edwardsville

**SPARK**

---

SIUE Faculty Research, Scholarship, and Creative Activity

---

Spring 4-16-2020

## Extensible Interface for a Compact Spectrophotometer for Teaching Molecular Absorption in the Undergraduate Laboratory

Edward Navarre  
enavarr@siue.edu

Follow this and additional works at: [https://spark.siu.edu/siue\\_fac](https://spark.siu.edu/siue_fac)

 Part of the [Analytical Chemistry Commons](#)

---

### Recommended Citation

Navarre, Edward, "Extensible Interface for a Compact Spectrophotometer for Teaching Molecular Absorption in the Undergraduate Laboratory" (2020). *SIUE Faculty Research, Scholarship, and Creative Activity*. 141.

[https://spark.siu.edu/siue\\_fac/141](https://spark.siu.edu/siue_fac/141)

This Article is brought to you for free and open access by SPARK. It has been accepted for inclusion in SIUE Faculty Research, Scholarship, and Creative Activity by an authorized administrator of SPARK. For more information, please contact [magrase@siue.edu](mailto:magrase@siue.edu), [tdvorak@siue.edu](mailto:tdvorak@siue.edu).

---

# An extensible interface for a compact spectrophotometer for teaching molecular absorption in the undergraduate laboratory

Edward C. Navarre \*

5 Department of Chemistry, Southern Illinois University Edwardsville, Edwardsville IL 62026-1652

## ABSTRACT

A simple computer interface for controlling a compact spectrograph for use as a spectrophotometer in an undergraduate teaching laboratory was developed. The project was implemented on a Raspberry Pi computer which permits the integration of a light source into the software. The interface was written in Python to facilitate modification by the user and because of its compatibility with several computing platforms. An implementation of the project in Linux on a Raspberry Pi computer is described.

## KEYWORDS

First-Year Undergraduate / General; Second-Year Undergraduate; Laboratory Instruction; Hands-On Learning / Manipulatives; Spectroscopy; Laboratory Equipment / Apparatus

## INTRODUCTION

Absorbance spectrophotometry is widely used throughout the chemistry curriculum to the extent that it is described at least qualitatively in most introductory chemistry textbooks and often basic univariate quantitative methods are included.<sup>1,2</sup> The theoretical and quantitative aspects of absorbance spectrophotometry are often presented for the first time in a classical quantitative chemical analysis course<sup>3,4</sup> taken in an undergraduate student's second or third year at university.<sup>5</sup> As a result, simple and cost-effective equipment is essential to teaching this technique in a variety of university laboratory situations with levels of student sophistication from first-semester university students to students in their final semester of an undergraduate degree. Many commercial solutions are offered ranging from about \$400 to \$2000 for basic absorbance systems and considerably more for advanced features. Additionally, many publications in this journal describe low-cost approaches to making absorbance spectrophotometry more accessible<sup>6,7</sup> and innovative ways to use low-cost instruments.<sup>8,9</sup>

1  
2  
3 The author was recently faced with the decision of how to replace a set of Bausch and Lomb  
4 Spectronic 20 used in chemistry teaching laboratories. Although the ThermoScientific Spectronic 200  
5 would be a 'one-for-one' replacement, the author pursued a different premise: how could existing  
6 spectrophotometric resources be used to solve the replacement issue? The author's academic  
7 department possessed several compact spectrographs that were originally acquired for an upper-level  
8 teaching laboratory. The technical solution described below is the author's attempt to develop a  
9 compact, economical replacement to the functionality of the Spectronic 20 in a sophomore-level  
10 quantitative analysis laboratory. The project sought to replicate the features without adding  
11 complexity to the use of the instrument.  
12  
13  
14  
15  
16  
17  
18  
19  
20

21 An additional motivation for the project was two limitations related to the manufacturer-  
22 provided software: space considerations and complexity. The laboratory into which this project would  
23 be deployed has limited space and an earlier trial of the compact spectrographs with small form factor  
24 PCs proved too unwieldy for regular use. Additionally, the compact spectrograph manufacturer  
25 justifiably wants to offer all of the hardware features in the software interface. This wealth of options  
26 was more confusing than helpful to students in the early trial of the hardware.  
27  
28  
29  
30  
31  
32

33 The author pursued an interface design that presented all of the important spectrophotometric  
34 conditions to the student in one place. As a result, the student user would be able to focus on  
35 learning about spectrophotometry rather than spend time understanding a software interface.  
36 Presenting only the essential experimental conditions limits the available spectrometer functions by  
37 removing features like derivatives, smoothing, and event triggers. Additionally, convenience features,  
38 such as automatic plotting of calibration curves detract from the pedagogical value of  
39 spectrophotometry. The project objective was a deliberately limited functionality that focused on  
40 students learning the experimental aspects of spectrophotometry.  
41  
42  
43  
44  
45  
46  
47

48 Other manufacturers offer small format spectrophotometry equipment that can address the space  
49 considerations. For example, the Pasco wireless spectrometer (model PS-2600) is very small.  
50 However, it requires a connected computer for the software that records the data or the company's  
51 SPARK LXi Datalogger (model PS-3600). Likewise, Vernier has several compact options, the most  
52 appropriate of which is the Go Direct® SpectroVis® Plus Spectrophotometer. The spectrophotometer  
53  
54  
55  
56  
57  
58

1  
2  
3 can be connected to a computer for recording data or to a Vernier LabQuest2 data-collection system.  
4  
5 Approaching this project with a Pasco or Vernier spectrophotometer connected to a computer doesn't  
6  
7 change the space issues significantly and would have required purchasing the spectrophotometers.  
8  
9 Using the SPARK LXi or LabQuest2 system would have been extremely space-efficient. Ultimately this  
10  
11 60 option was not selected, largely for economic considerations; the complete spectrometer and data-  
12  
13 collection system would be several times more expensive than the chosen solution.  
14

## 15 **EQUIPMENT**

16 The spectrograph used for recording visible spectra in this work was a StellarNet Black Comet  
17  
18 C-25 (StellarNet Inc, Tampa, Florida). The particular model had a 2048-pixel CCD, 16-bit ADC, and a  
19  
20  $\Delta\lambda_{\text{effective}}$  of about 1 nm across the spectral range 179 to 1016 nm. The project was also tested on an  
21 65  
22 Ocean Optics HR4000 (Ocean Insights Inc., Largo, Florida). The software interface was developed in  
23  
24 Python (version 2.7 and 3.7, Python Software Foundation) on a Pi-top CEED (Pi-top, London, UK). A  
25  
26 wireless compact keyboard (model RT-MWK12+, Riitek Technology, Shenzhen, China) was selected to  
27  
28 minimize space requirements.  
29

30 70 There are two versions of the project. One simply controls the spectrograph and would require  
31  
32 the use of existing light sources and cuvette holders. The second integrates a light source into the  
33  
34 software and Raspberry Pi hardware. Two light sources were investigated: a "cool white" LED (LTW-  
35  
36 2R3D7, Lite-On Inc.) and a "warm white" LED (334-15/X1C5-1QSA, Everlight Electronics Co Ltd).  
37  
38 The spectra of the two LEDs are shown in Figure 1 under conditions that place the maximum emission  
39  
40 75 at the upper limit of the spectrometer range. The choice between the LEDs is up to the user  
41  
42 depending on the spectral range in which they are interested. A cuvette holder was manufactured by  
43  
44 the author from Delrin thermoplastic for direct attachment to the face of the spectrograph. The  
45  
46 cuvette holder is designed for use with the integrated LED light source; other cuvette holders can be  
47  
48 used if an external light source is used. Fabrication plans for the cuvette holder are available in the  
49  
50 80 supplementary material. In the project version with an integrated LED light source, the brightness of  
51  
52 the LED is adjustable in the software interface via a pulse width modulation (PWM) circuit shown in  
53  
54 Figure 2. The PWM frequency can be adjusted in the code but is set initially to 2000 Hz which is  
55  
56 sufficiently fast to avoid the appearance of signal flickering at integration times greater than or equal  
57  
58

to 3 ms (the spectrometer minimum integration time). The PWM duty cycle was tested from 1 % to 100 % and found to produce constant LED intensity at all values.

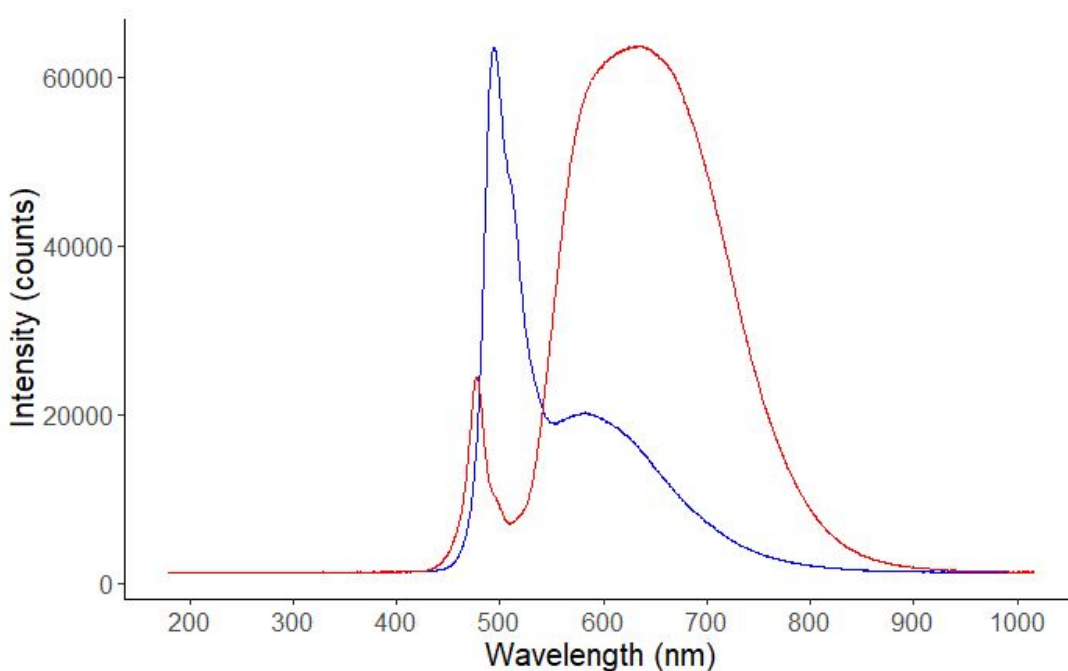


Figure 1. The emission spectra of the LEDs. The spectrum of the LTW-2R3D7 is drawn in blue and the 334-15/X1C5-1QSA is drawn in red. The spectra were recorded with 5-ms integration time and an LED duty-cycle of 99 % (red trace) and 31 % (blue trace) so that the maximum intensity values are equivalent and near the maximum of the spectrometer range.

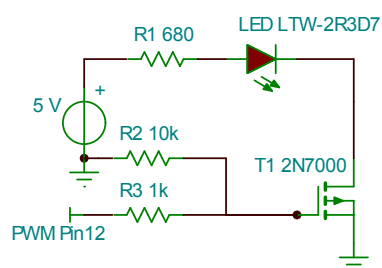


Figure 2. The pulse width modulation circuit for controlling the brightness of an LED light source. The pin number is relevant to a Raspberry Pi implementation of the circuit.

## HAZARDS AND SAFETY PRECAUTIONS

There are not any inherent chemical hazards in the implementation of this project as a spectrophotometer. Its use in a teaching laboratory will need to respect the risks and hazards of the chemical system that is studied with the spectrophotometer.

## RESULTS

The major product of the project is a simple software interface for performing spectrophotometry measurements. The software written for this project consists of a Python module that collects the physical parameters of the spectrograph at startup and provides an interactive interface for spectrophotometry. The code for the interface is located on GitHub (<https://github.com/acpo/>) with versions for StellarNet and Ocean Optics spectrographs. Instructions for installing the project are available in the supplemental information. There are versions available with and without an integrated LED light source. The integration of the LED light source provides control of all parts of the spectrophotometry instrument within the interface. A description of the user interaction with the interface is shown in Table 1 for the cases in which most experimental conditions are preset in the code (*e.g.*, for the least experienced users) and the case in which the user must work with all of the experimental conditions.

**Table 1. User Interaction with for a Typical Spectrophotometric measurement**

	Case: some conditions preset in code	Case: all conditions set by user
Select integration time such that 100 % T signal is on scale <sup>a</sup> ( <i>text box</i> )	Not required	Required
Select wavelength boundaries appropriate to the light source ( <i>text box</i> )	Not required	Required
Select the number of spectra to average <sup>b</sup> ( <i>text box</i> )	Not required	Required
Record 0 % T ( <i>button click</i> )	Required	Required
Record 100 % T ( <i>button click</i> )	Required	Required
Switch to Absorbance mode ( <i>button click</i> )	Required	Required
Select wavelength to monitor ( <i>text box</i> )	Required	Required
Observe absorbances	Required	Required

<sup>a</sup> if the integrated LED is used then the LED duty-cycle and the integration time both must be adjusted to give an on-scale signal.

<sup>b</sup> averaging performs the arithmetic mean of the number of successive spectra indicated by this value, and acquisition requires a total time of the integration time × averages

An example of the complete system hardware and software interface are shown in Figure 3.

The Raspberry Pi-based system used in this project was useful to demonstrate that a very low-power computer was suitable. On the Pi-top system the response times of the interface and spectrum redrawing were fast enough for most students to be comfortable using it. The project could readily be

adapted to a small (3.5 or 5-inch) touch screen display to radically reduce the size of the device,  
including the elimination of the keyboard.

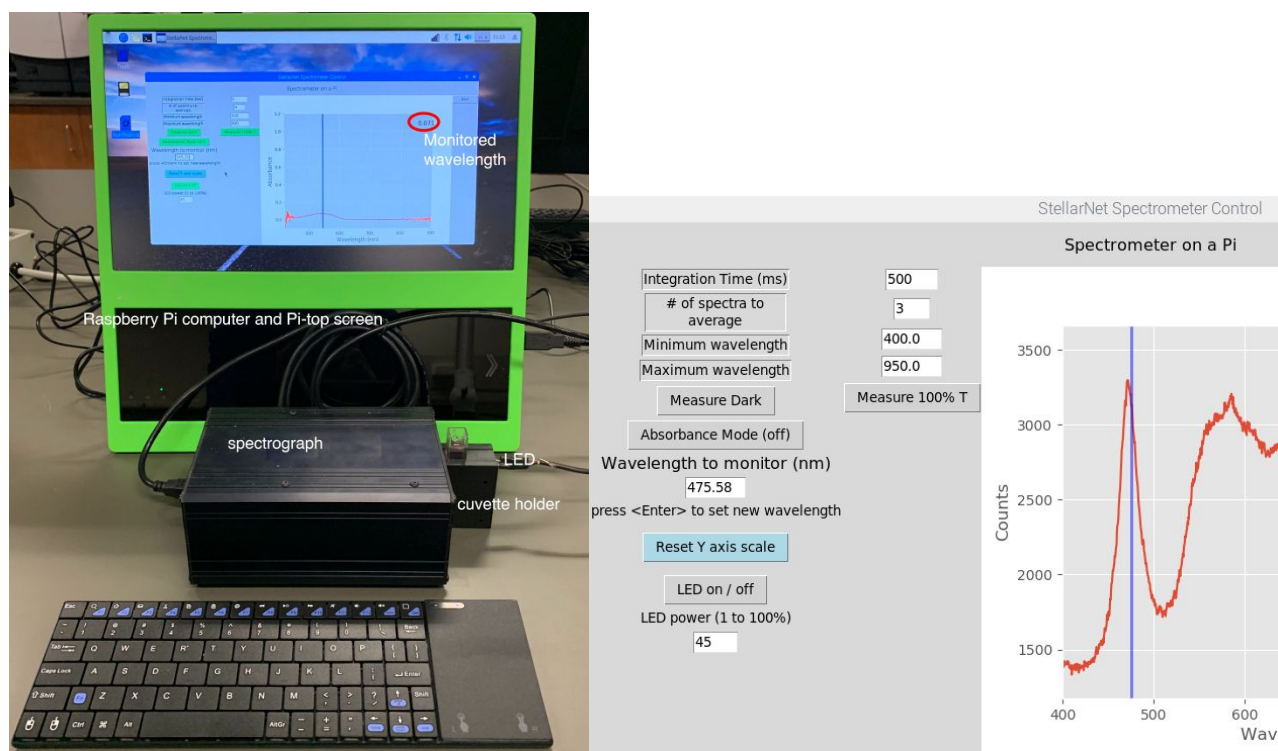


Figure 3. The complete spectrophotometer implementation (left) and the Python interface (right).

The project as implemented on a Pi-top computer and StellarNet spectrograph was tested with a quantitative analysis laboratory of 45 students divided into sections of about 12 each. Each student worked independently on a spectrophotometric determination of iron with *o*-phenanthroline by external calibration.<sup>10, 11</sup> Relative to the student results of prior years in which a Spectronic 20 was used in this experiment, the data showed similar linearity in the range of 0 to 0.6 absorbance units. Linearity of data above 0.6 absorbance was slightly better with the compact spectrograph. It should be noted that the spectrophotometric performance of the system is largely dependent upon the particular hardware that a user selects, so the author's experience may not be the same as other users. However, in the transition from a Spectronic 20 ( $\Delta\lambda_{\text{effective}} \approx 20$  nm) to a modern compact spectrograph ( $\Delta\lambda_{\text{effective}}$  typically less than 2 nm) it would be unusual to find poorer performance related to deviations from the Beer-Lambert law.

The student experience with this project was similar to the Spectronic 20, with some advantages. Both systems required the student to record a 0 % and 100 % transmittance

1  
2  
3 measurement at the start of analysis. The Spectronic 20 accomplished this task via two analog dials  
4  
5 whereas in this project students clicked two buttons on the interface; effectively the student  
6  
7 experience is identical. Once the prerequisites were recorded, the absorbance at the selected monitor  
8  
9 wavelength was continuously displayed on the spectrum window (see Fig. 3). Selection of the  
10  
11 135 monitored wavelength was done via a numerical entry box on the interface. An important advantage  
12  
13 in this project was that the absorbance spectrum was displayed continuously during use. The  
14  
15 continuous display of the complete absorbance spectrum offers the instructor an opportunity to have  
16  
17 students easily explore the concept of  $\lambda_{\max}$  and other properties of the Beer-Lambert law.

18  
19 A pedagogical advantage to this project is that the Python code for this project is available to be  
20  
21 140 edited and customized to an instructor's needs. The distributed version sets the wavelength range to  
22  
23 the range reported by the spectrograph firmware. An instructor has the choice to modify two lines of  
24  
25 code to preset the boundaries or to ask students to select with the interface the appropriate  
26  
27 boundaries for the light source that they are using. For example, if a white light LED is used, the  
28  
29 range can be restricted to 450 to 850 nm. Likewise, the integration time of the detector can be preset  
30  
31 145 in the code by the instructor to appropriately utilize the dynamic range of the detector or students can  
32  
33 be asked to explore the how the integration time can be used to make best use of the available light.  
34  
35 Additionally, the interface developed in this project gives the user access to the raw signal from the  
36  
37 spectrograph and can be used for emission (*e.g.*, fluorescence or chemiluminescence) measurements  
38  
39 which were never part of the Spectronic 20 scope of functions.

40  
41 150 Lastly, to the author's knowledge, the interface developed in this project is the first free  
42  
43 spectrophotometry interface for StellarNet spectrometers on the Linux platform. While this project  
44  
45 was being tested, the company introduced a Mac OS compatible software, but there are not currently  
46  
47 any solutions for the Raspberry Pi or other Linux distributions. This project also offers a free, open-  
48  
49 source Linux interface to Ocean Optics instruments which the company does not currently provide.

## 51 155 **ASSOCIATED CONTENT**

### 52 **Supporting Information**

53 The Supporting Information is available on the ACS Publications website at DOI:

54  
55 10.1021/acs.jchemed.XXXXXXX. [ACS will fill this in.]  
56  
57  
58



Notes to guide the installation of the project. NotesForInstallation.pdf (PDF)

Cuvette holder fabrication plans. FabricationPlans.pdf (PDF)

A description of each functional unit in the software. SoftwareDescription.pdf (PDF)

A description of the hardware requirements for Raspberry PI, Windows, and Apple systems.

HardwareDescription.pdf (PDF)

## AUTHOR INFORMATION

Edward C. Navarre

\*E-mail: enavarr@siue.edu

## ACKNOWLEDGMENTS

The students of the Summer and Fall 2019 sessions of the quantitative analytical chemistry laboratory at SIUE are thanked for their patience in testing this project. The reviewers of the manuscript are thanked for their comments that helped to reveal several issues with earlier versions of the project.

Edward C. Navarre received funding from the Southern Illinois University Edwardsville Excellence in Undergraduate Education Program for part of this project.

## REFERENCES

1. Brown, T. L. *Chemistry: The Central Science*, 13<sup>th</sup> edition.; Pearson: Boston, 2015. pp. 1019-1020.
2. Robinson, J. K.; McMurry, J.; Fay, R. C. *Chemistry*, 8<sup>th</sup> Ed.; Pearson Education, Inc: Hoboken, NJ, 2020. pp. 929-930.
3. Skoog, D. A. *Fundamentals of Analytical Chemistry*, 9<sup>th</sup> Ed.; Cengage - Brooks/Cole: Belmont, CA, 2012. pp. 650-674.
4. Harris, D. C.; Lucy, C. A. *Quantitative Chemical Analysis*, 9<sup>th</sup> Ed.; W.H. Freeman & Company: New York, 2016. pp. 432-443.
5. Griffiths, P. R. Whither "Quant"? An Examination of the Curriculum and Testing Methods for Quantitative Analysis Courses Taught in Universities and Colleges in the Western USA. *Anal. Bioanal. Chem.* **2008**, 391 (3), 875–880. <https://doi.org/10.1007/s00216-008-2080-2>.
6. Grasse, E. K.; Torcasio, M. H.; Smith, A. W. Teaching UV–Vis Spectroscopy with a 3D-Printable Smartphone Spectrophotometer. *J. Chem. Educ.* **2016**, 93 (1), 146–151. <https://doi.org/10.1021/acs.jchemed.5b00654>. And references 3 – 9 therein.

- 
- 1  
2  
3 7. Vanderveen, J. R.; Martin, B.; Ooms, K. J. Developing Tools for Undergraduate Spectroscopy: An  
4 Inexpensive Visible Light Spectrometer. *J. Chem. Educ.* **2013**, *90* (7), 894–899.  
5 190 <https://doi.org/10.1021/ed300396x>.  
6  
7 8. Bougot-Robin, K.; Paget, J.; Atkins, S. C.; Edel, J. B. Optimization and Design of an Absorbance  
8 Spectrometer Controlled Using a Raspberry Pi To Improve Analytical Skills. *J. Chem.*  
9 *Educ.* **2016**, *93* (7), 1232–1240. <https://doi.org/10.1021/acs.jchemed.5b01006>.  
10  
11 9. Cell Phone Spectrometer  
12 195 [https://www.asdlib.org/onlineArticles/elabware/Scheeline\\_Kelly\\_Spectrophotometer/](https://www.asdlib.org/onlineArticles/elabware/Scheeline_Kelly_Spectrophotometer/index.html)  
13 [index.html](https://www.asdlib.org/onlineArticles/elabware/Scheeline_Kelly_Spectrophotometer/index.html) (accessed Oct 28, 2019).  
14  
15 10. Fortune, W. B.; Mellon, M. G. Determination of Iron with O-Phenanthroline: A  
16 Spectrophotometric Study. *Ind. Eng. Chem. Anal. Ed.* **1938**, *10* (2), 60–64.  
17 <https://doi.org/10.1021/ac50118a004>.  
18 19 200  
19 20  
20 21 11. Atkins, R. C. Colorimetric Determination of Iron in Vitamin Supplement Tablets. A General  
22 Chemistry Experiment. *J. Chem. Educ.* **1975**, *52* (8), 550. <https://doi.org/10.1021/ed052p550>.  
23  
24  
25  
26  
27  
28  
29  
30  
31  
32  
33  
34  
35  
36  
37  
38  
39  
40  
41  
42  
43  
44  
45  
46  
47  
48  
49  
50  
51  
52  
53  
54  
55  
56  
57  
58