



Scoring System to Evaluate the Performance of ICU Ventilators in the Pandemic of COVID-19: A Lung Model Study

Xingshuo Hu^{1†}, Fei Xie^{1†}, Kaifei Wang^{1†}, Hongjun Gu^{1†}, Guoxin Mo¹, Ruoxuan Wen¹, Ying Zhao¹, Qingyun Yang¹, Knut Möller², Zhanqi Zhao^{2,3*} and Lixin Xie^{1*}

¹ Critical Care, College of Pulmonary and Critical Care Medicine, Chinese PLA General Hospital, Beijing, China, ² Institute of Technical Medicine, Furtwangen University, Villingen-Schwenningen, Germany, ³ Department of Biomedical Engineering, Fourth Military Medical University, Xi'an, China

OPEN ACCESS

Edited by:

F. Javier Belda,
University of Valencia, Spain

Reviewed by:

Savino Spadaro,
University of Ferrara, Italy
Ildiko Toth,
University of Pécs, Hungary

*Correspondence:

Zhanqi Zhao
zhanqi.zhao@hs-furtwangen.de
Lixin Xie
xielx301@126.com

†These authors have contributed
equally to this work

Specialty section:

This article was submitted to
Intensive Care Medicine and
Anesthesiology,
a section of the journal
Frontiers in Medicine

Received: 04 February 2021

Accepted: 14 June 2021

Published: 14 July 2021

Citation:

Hu X, Xie F, Wang K, Gu H, Mo G,
Wen R, Zhao Y, Yang Q, Möller K,
Zhao Z and Xie L (2021) Scoring
System to Evaluate the Performance
of ICU Ventilators in the Pandemic of
COVID-19: A Lung Model Study.
Front. Med. 8:663608.
doi: 10.3389/fmed.2021.663608

Ventilators in the intensive care units (ICU) are life-support devices that help physicians to gain additional time to cure the patients. The aim of the study was to establish a scoring system to evaluate the ventilator performance in the context of COVID-19. The scoring system was established by weighting the ventilator performance on five different aspects: the stability of pressurization, response to leaks alteration, performance of reaction, volume delivery, and accuracy in oxygen delivery. The weighting factors were determined with analytic hierarchy process (AHP). Survey was sent out to 66 clinical and mechanical experts. The scoring system was built based on 54 valid replies. A total of 12 commercially available ICU ventilators providing non-invasive ventilation were evaluated using the novel scoring system. A total of eight ICU ventilators with non-invasive ventilation mode and four dedicated non-invasive ventilators were tested according to the scoring system. Four COVID-19 phenotypes were simulated using the ASL5000 lung simulator, namely (1) increased airway resistance (IR) (10 cm H₂O/L/s), (2) low compliance (LC) (compliance of 20 ml/cmH₂O), (3) low compliance plus increased respiratory effort (LCIE) (respiratory rate of 40 and inspiratory effort of 10 cmH₂O), (4) high compliance (HC) (compliance of 50 ml/cmH₂O). All of the ventilators were set to three combinations of pressure support and positive end-expiratory pressure levels. The data were collected at baseline and at three customized leak levels. Significant inaccuracies and variations in performance between different non-invasive ventilators were observed, especially in the aspect of leaks alteration, oxygen and volume delivery. Some ventilators have stable performance in different simulated phenotypes whereas the others have over 10% scoring differences. It is feasible to use the proposed scoring system to evaluate the ventilator performance. In the COVID-19 pandemic, clinicians should be aware of possible strengths and weaknesses of ventilators.

Keywords: scoring system, ventilator performance, stability of pressurization, leakage correction, accuracy in volume delivery, performance of triggering, analytic hierarchy process

INTRODUCTION

Ventilator in the intensive care units (ICU) is life-support device that helps physicians gaining additional time to cure the patients. Several previous studies have compared the performance of different ventilators regarding triggering (1), system leaks (2, 3), and accuracy in volume and pressure delivery (4). The performance varied from device to device, and depended on the testing items. One device might be accurate in volume but not in pressure delivery. A complex scoring system to evaluate the overall performance of ventilator regarding various aspects is missing.

The outbreak of the novel coronavirus disease 2019 (COVID-19) has spread rapidly around the world (5). About 19% of patients in China developed hypoxic respiratory failure and required certain level of ventilation support (6). The situation in other countries is similar. Patients with COVID-19 show various phenotypes that may require different respiratory treatments, characterized as low compliance (LC) due to lung collapse or high airway resistance due to inflammation and mucus (7, 8). The performance of ventilator could be various for different phenotypes, which was not well-studied. Since the number of infected patients is large and still increases dramatically, a large number of ventilators required to support patients' respiratory system (9). New companies are recruited to build ventilators, which might have no experience on manufacturing ventilators or even medical devices prior to the pandemic. A well-designed scoring system may be helpful for the evaluation and improvement of the ventilators.

The aim of the study was to establish a scoring system to evaluate the ventilator overall performance, as well as different aspects. Based on the proposed scoring system, ICU most commonly used ventilators in China were compared in order to demonstrate the feasibility of the novel scoring system. We hypothesized that the performances of the ventilators evident.

MATERIALS AND METHODS

The scoring system was established using the analytic hierarchy process (AHP) (10). The AHP hierarchy consisted of five criteria regarding the ventilator performance, which were selected based on our experiences and previous studies (2–4).

The Stability of Pressurization

The stability of pressurization refers to the control precision of pressurization during ventilation. It contains three alternatives: (1) maximum pressure drop, the absolute difference between expiratory positive airway pressure (EPAP) and the lowest pressure during inspiration; (2) inspiratory positive airway pressure (IPAP) error, the absolute difference between the actual pressure and the set IPAP during inspiration; (3) EPAP error, the absolute difference between the actual pressure and the set EPAP during expiration.

Abbreviations: ICU, intensive care units; COVID-19, the novel coronavirus disease 2019; AHP, analytic hierarchy process; EPAP, expiratory positive airway pressure; IPAP, inspiratory positive airway pressure.

Response to Leaks Alteration

Leak correction represents the ability of the ventilator to adapt to the changes of a systematic leak. It has two alternatives: time needed from the moment a leak was increased or decreased until the tidal volume was within 2 standard deviations of the mean tidal volume for each leak level. They were denoted as time to settle (increase) and time to settle (decrease).

Performance of Reaction

To evaluate the performance of reaction, the following alternatives are considered: (1) Exp T90, the time to accomplish 90% of the drop from peak pressure to EPAP; (2) Insp T90, the time to accomplish 90% of the rise to IPAP; (3) trigger time, point in time at which airway pressure has returned to baseline after downward deflection (start of inspiration effort).

Volume Delivery


Volume delivery assesses the gas output of a ventilator, includes (1) peak flow rising ratio during inhalation (peak flow divided by Insp T90) and (2) tidal volume.

Accuracy in Oxygen Delivery

The accuracy in oxygen delivery refers to the difference between the preset oxygen concentration and the actual one delivered.

The AHP evaluation criteria are illustrated in **Figure 1**. The relative weights of the nodes in the hierarchy were determined using a survey (<https://www.wjx.cn/jq/102986570.aspx>). The participants consisted of senior intensivists (chief physician) and engineers of ventilator manufacturers (>5 years as senior engineer). The participants evaluated the hierarchy through a series of pairwise comparisons that derive numerical scales of measurement for the nodes (i.e., 0 or 1). The criteria are pairwise compared for importance. The alternatives are pairwise compared against each of the criteria for preference. The priorities are derived correspondingly for each node as described in the previous study (11).

Further, eight ICU ventilators with non-invasive ventilation mode and four dedicated non-invasive ventilators were tested according to the scoring system. The features of the tested ventilators are summarized in **Table 1**. The setting of the ventilators was the same: spontaneous timed mode, 10/min, Inspiratory rise time, when adjustable, was set to the fastest value that did not cause an initial pressure overshoot that would shut down the lung model, and triggering was set at the most sensitive value that did not cause auto-triggering. Four COVID-19 phenotypes were simulated using the ASL5000 lung simulator (IngMar Medical, PA, USA), namely (1) LC, low compliance (compliance of 20 ml/cmH₂O), (2) IR, increased airway resistance (10 cm H₂O/L/s), (3) LCIE, low compliance plus increased respiratory effort (respiratory rate of 40 and inspiratory effort of 10 cmH₂O), and (4) HC, high compliance (compliance of 50 ml/cmH₂O). All of the ventilators were set to three combinations of IPAP and EPAP levels (10 and 4 cmH₂O, 20 and 8 cmH₂O, 30 and 12 cmH₂O, IPAP and EPAP, respectively). The data were collected at baseline and at three customized leak levels for dedicated non-invasive ventilators (50, 70, and 90 L/min) and

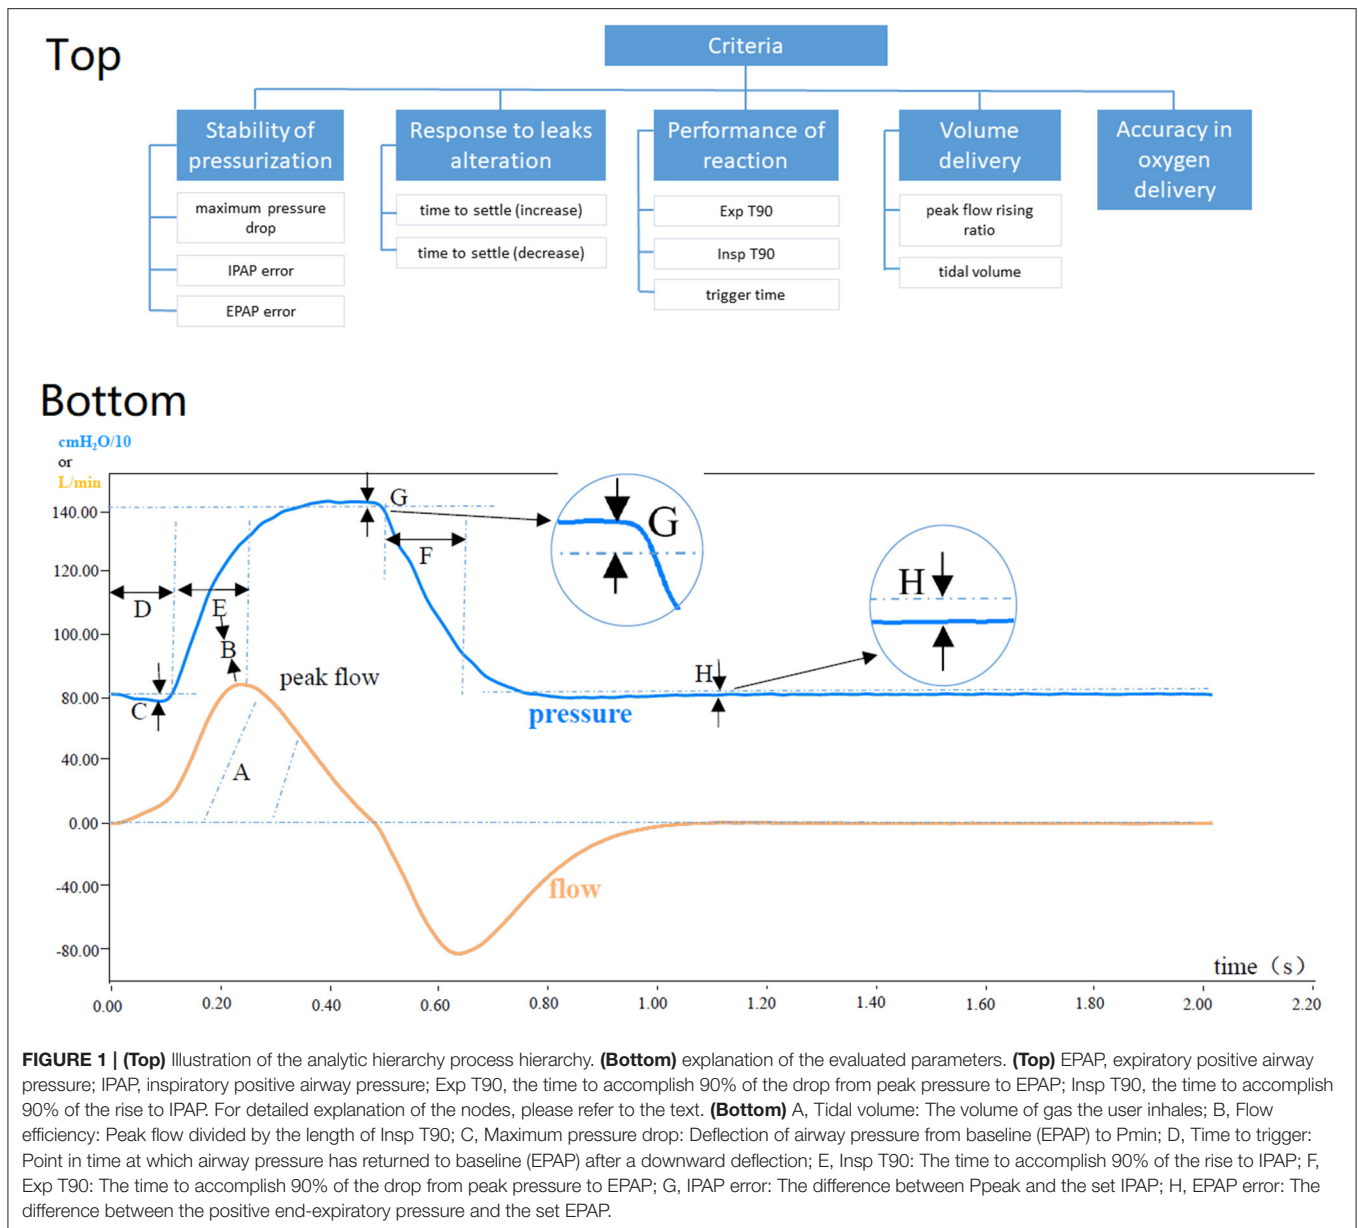

for ICU ventilators using non-invasive mode (14, 19 and 25 L/min).

Data Collection

Test hardware and its connection are illustrated in **Figure 2**. The test process consists of four steps: (1) Start the test after setting the lung simulator according to the parameters described previously, and adjustment of the control valve reaching the specified air leakage of the ventilator. (2) Keep the opening of the control valve and restart the lung simulator for testing for 1 min. (3) Repeat the above two steps until three different air leakages have been tested. (4) Dynamic air leakage test was carried out through a control


valve with three gears. Data acquisition was done at 512 Hz and stored in a desktop computer.

Statistical Analysis

Offline analysis on a breath by breath basis was done by the ASL5000 Lab view software (National Instruments, Austin, TX, USA). All breaths were visually inspected and five breaths during equilibrium state were selected for analysis. Outliers were defined as 1.5 times interquartile range. The outliers were eliminated from further analysis. The ranges of the targeted parameters are listed in **Table 2**. When a ventilator performance was outside of the range, it scored 1 or 0 for better or worse performance, respectively. Mean values of the score were

TABLE 1 | Summary of ventilators examined in the study.

Ventilator	Connection type (circuit)	Manufacturer	Leakage compensation (L/min)	Trigger type	Cycling type
BiPAP V60	Single	Philips, NL	60	Auto-flow	Auto-flow
Bellavista 1000	Single	Imtmedical, CH	120	Auto-pressure, flow	Auto-pressure, flow, volume
ST-30K	Single	Micomme, CN	120	Auto-flow	Auto-flow
carina	Single	Draeger Medical, DE	50	Manual-pressure, flow	Manual-pressure, flow
VG55	Single	AeonMed, CN	200	Manual-flow	Manual-flow
GA	Single	ResMedandCurative, CN	120	Manual-pressure, flow	Manual-flow
VG70	Double	AeonMed, CN	60	Manual-pressure, flow	Manual-pressure, flow
SV800	Double	Mindray, CN	65	Manual-pressure, flow	Manual-pressure, flow
Servo-I	Double	GetingeGroup, SE	65	Manual-pressure, flow	Manual-flow
R860	Double	GE Medical, US	100	Manual-pressure, flow	Manual-flow
VELA	Double	CareFusion, US	60	Manual-flow	Manual-pressure, flow, volume
V200	Double	Philips, NL	60	Auto-flow	Auto-flow

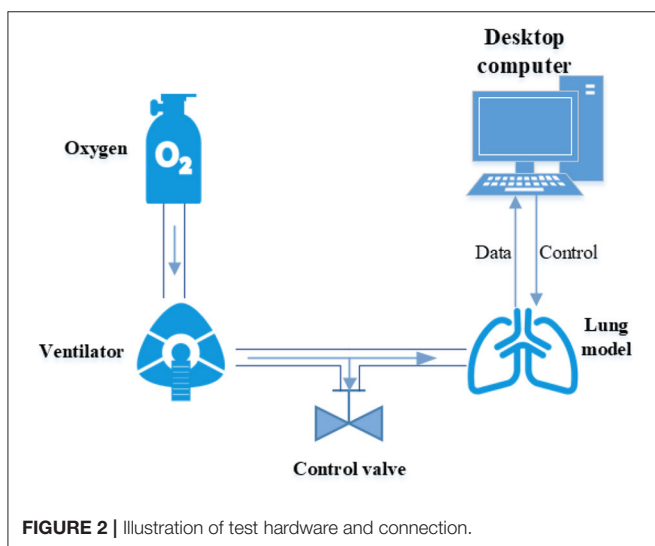**FIGURE 2** | Illustration of test hardware and connection.

calculated when multiple levels of testing were performed. The overall performance is weight sum of all nodes.

RESULTS

The survey was sent out to 66 clinical and engineering experts. The weighting factors were defined based on 54 valid replies (16 from senior intensivist and 38 from engineers). The final weights of the nodes are summarized in **Table 3**. The nodes of the criterion “pressurization” had similar weights. The experts considered time to settle (increase) and tidal volume much more important than the time to settle (decrease) and peak flow rising ratio, respectively. Trigger time was the most important node in the criterion “reaction”.

Overall performances of the ventilators under four simulated COVID-19 phenotypes were summarized in **Figure 3**. V60 and Servo-I have the best overall performance among the

ventilators tested (for single and double circuits). Some ventilators have stable performance in different simulated phenotypes whereas the others have over 10% scoring differences (e.g., 30 K and V200). Nevertheless, the overall performances among the ventilators for double circuits were similar. The performances of the ventilators in five criteria were illustrated using radar charts (**Figure 4**). Significant inaccuracies and variations in performance among different ventilators were observed, especially in the aspect of response to leaks alteration, oxygen, and volume delivery. For example, Servo-I had excellent performance in response to leaks alteration in all simulated phenotypes, however, its performance in volume delivery was much weaker. The accuracy in oxygen delivery for VG70 strongly depended on the simulated phenotypes.

DISCUSSION

In the present study, we demonstrated the process of establishing a scoring system to evaluate the overall performance of ventilators. Further, with help of the proposed scoring system, 12 ventilators were evaluated. It was found that the performance of ventilators depended on targeted lung models and varied significantly among different investigated criteria.

COVID-19 may affect the respiratory system in various ways. In patients with respiratory failure, the oxygen level may drop to a low level that meets the definition of acute respiratory distress syndrome. However, the respiratory system compliance may still be normal (7). The compliance may decrease during disease progression, which might be caused by inappropriate settings of ventilator (12). If the performance of the ventilator is unacceptable with large discrepancy between set values and actual ones, ventilator-induced lung injury might occur even the ventilator settings were optimized. In combination with other existing lung diseases in the patients, such as chronic obstructive lung disease, more frequent monitoring and modified respiratory therapy are required in ICU (13). In the present study, we simulated four phenotypes of COVID-19, with possibly increase of airway resistance (IR), decrease of compliance (LC),

TABLE 2 | Ranges of the targeted parameters.

Parameters	score	Preset pressure (cmH ₂ O)											
		LC			IR			LCIE			HC		
		4-10	8-20	12-30	4-10	8-20	12-30	4-10	8-20	12-30	4-10	8-20	12-30
Tidal volume (ml)	0	120	200	250	190	350	480	180	184	229	300	400	450
	1	270	400	540	490	780	1,025	416	561	572	600	900	1,200
Peak flow rising ratio (l/s ²)	0	0			0			0			0		
	1	10			6			15			3		
Trigger time (ms)	0	400			600			400			600		
	1	60			90			60			60		
Maximum pressure drop (cmH ₂ O)	0	3.55			2.55			7			2.55		
	1	0			0			0			0		
Exp T90 (ms)	0	600			1,000			600			1,400		
	1	100			150			100			100		
Insp T90(ms)	0	900			1,200			900			1,400		
	1	100			150			100			300		
IPAP error (cmH ₂ O)	0	±5	±10	±15	±5	±10	±15	±5	±10	±15	±5	±10	±15
	1	0	0	0	0	0	0	0	0	0	0	0	0
EPAP error (cmH ₂ O)	0	±2	±4	±6	2	±4	±6	2	±4	±6	2	±4	±6
	1	0	0	0	0	0	0	0	0	0	0	0	0
Time to settle (increase) (s)	0	20											
	1	0											
Time to settle (decrease) (s)	0	12											
	1	0											
Oxygen delivery %	setting	60%											
	0	±10											
	1	0											
	setting	100%											
	0	80											
1	98												

IR, increased airway resistance; LC, low compliance; LCIE, low compliance plus increased respiratory effort; HC, high compliance.

TABLE 3 | The final weights of nodes of the scoring system.

First level criteria	Second level criteria		
The stability of pressurization	0.223 Maximum pressure drop	0.337	
	EPAP error	0.278	
	IPAP error	0.385	
Response to leaks alteration	0.229 Time to settle (increase)	0.622	
	Time to settle (decrease)	0.378	
Volume delivery	0.160 Peak flow rising ratio during inhalation	0.385	
	Tidal volume	0.615	
Performance of reaction	0.242 Insp T90	0.341	
	Exp T90	0.160	
	Trigger time	0.498	
Accuracy in oxygen delivery	0.146 –	–	

increase of inspiratory effort (LCIE), or HC. The ventilators evaluated in the study showed different performances under different lung models. In clinical practice, if more than one type of ventilator was available, the one that best fits the underlying disease should be selected. If only limited types of ventilators are at disposal, intensivists, or respiratory therapists should be aware of the pitfalls of the ventilators during application. Taking the ventilator Bellavista for example, when it is applied on COVID-19 patient with LC, and the measured leakage is ~60 L/min, we suggest that the ventilator should be adjusted according to the findings of the present study (Figure 5). In particular, response to leaks alteration and volume delivery of this ventilator scored low. Leakage reduction and IPAP increase should be considered in this scenario.

The current pandemic has created medical resource scarcities, especially in regions where ventilators and trained personnel are already in short supply. Many new attempts of ventilator manufacturing were presented, including some low cost ventilator (14), and shared ventilator setup for multi-patient simultaneous use (15). The scoring system established in the present study should be able to help evaluating the performance of ventilators in a standard manner. Next generation of ventilator is toward physiological closed-loop systems (16). Decision making would be still in the hands of physicians but with the extensive physiological monitoring in current clinical environment, a physiological parameter could be accurately fed back to the controller and solve the high-stress environments as COVID-19 pandemic with a shrinking workforce (17). To develop the correct feedback loop, a full understanding of the ventilator performance is required. The current study might be a step toward the physiological closed-loop system. Besides, the proposed scoring system and the models simulated by ASL5000 may help the medical students to further understand the interaction between patients and ventilator in addition to mannequin-based and computer screen-based simulation (18).


The following limitations are acknowledged. (1) The five criteria of the AHP hierarchy (and the corresponding alternatives) were predefined. Only these aspects of ventilator performance were evaluated and considered in the scoring system. Some importance aspects could have been missed when




we designed this scoring system for non-invasive ventilation. For invasive ventilation mode, other parameters should be considered as well. Nevertheless, the knowledge and procedure of building the scoring system can be easily transferred. (2) The definition of the parameter value ranges in Table 2 might have influence on the overall score of particular ventilator. But if the same ranges are used for all comparison, the scores of the ventilators are comparable. (3) This was a lung model study with limited number of variations simulating COVID-19 patients. We demonstrated the performance of various ventilators under the preselected scenarios. The study design was not intended to validate the scoring system. In the future study, actual outcomes and influences on real subjects could be considered.

Clinicians should be aware of possible strength and weakness of ventilators. Performance of other ventilators can be conducted using the scoring system developed in the present study.

It is feasible to use the proposed scoring system to evaluate the ventilator performance. In the COVID-19 pandemic, clinicians should be aware of possible strength and weakness of ventilators.

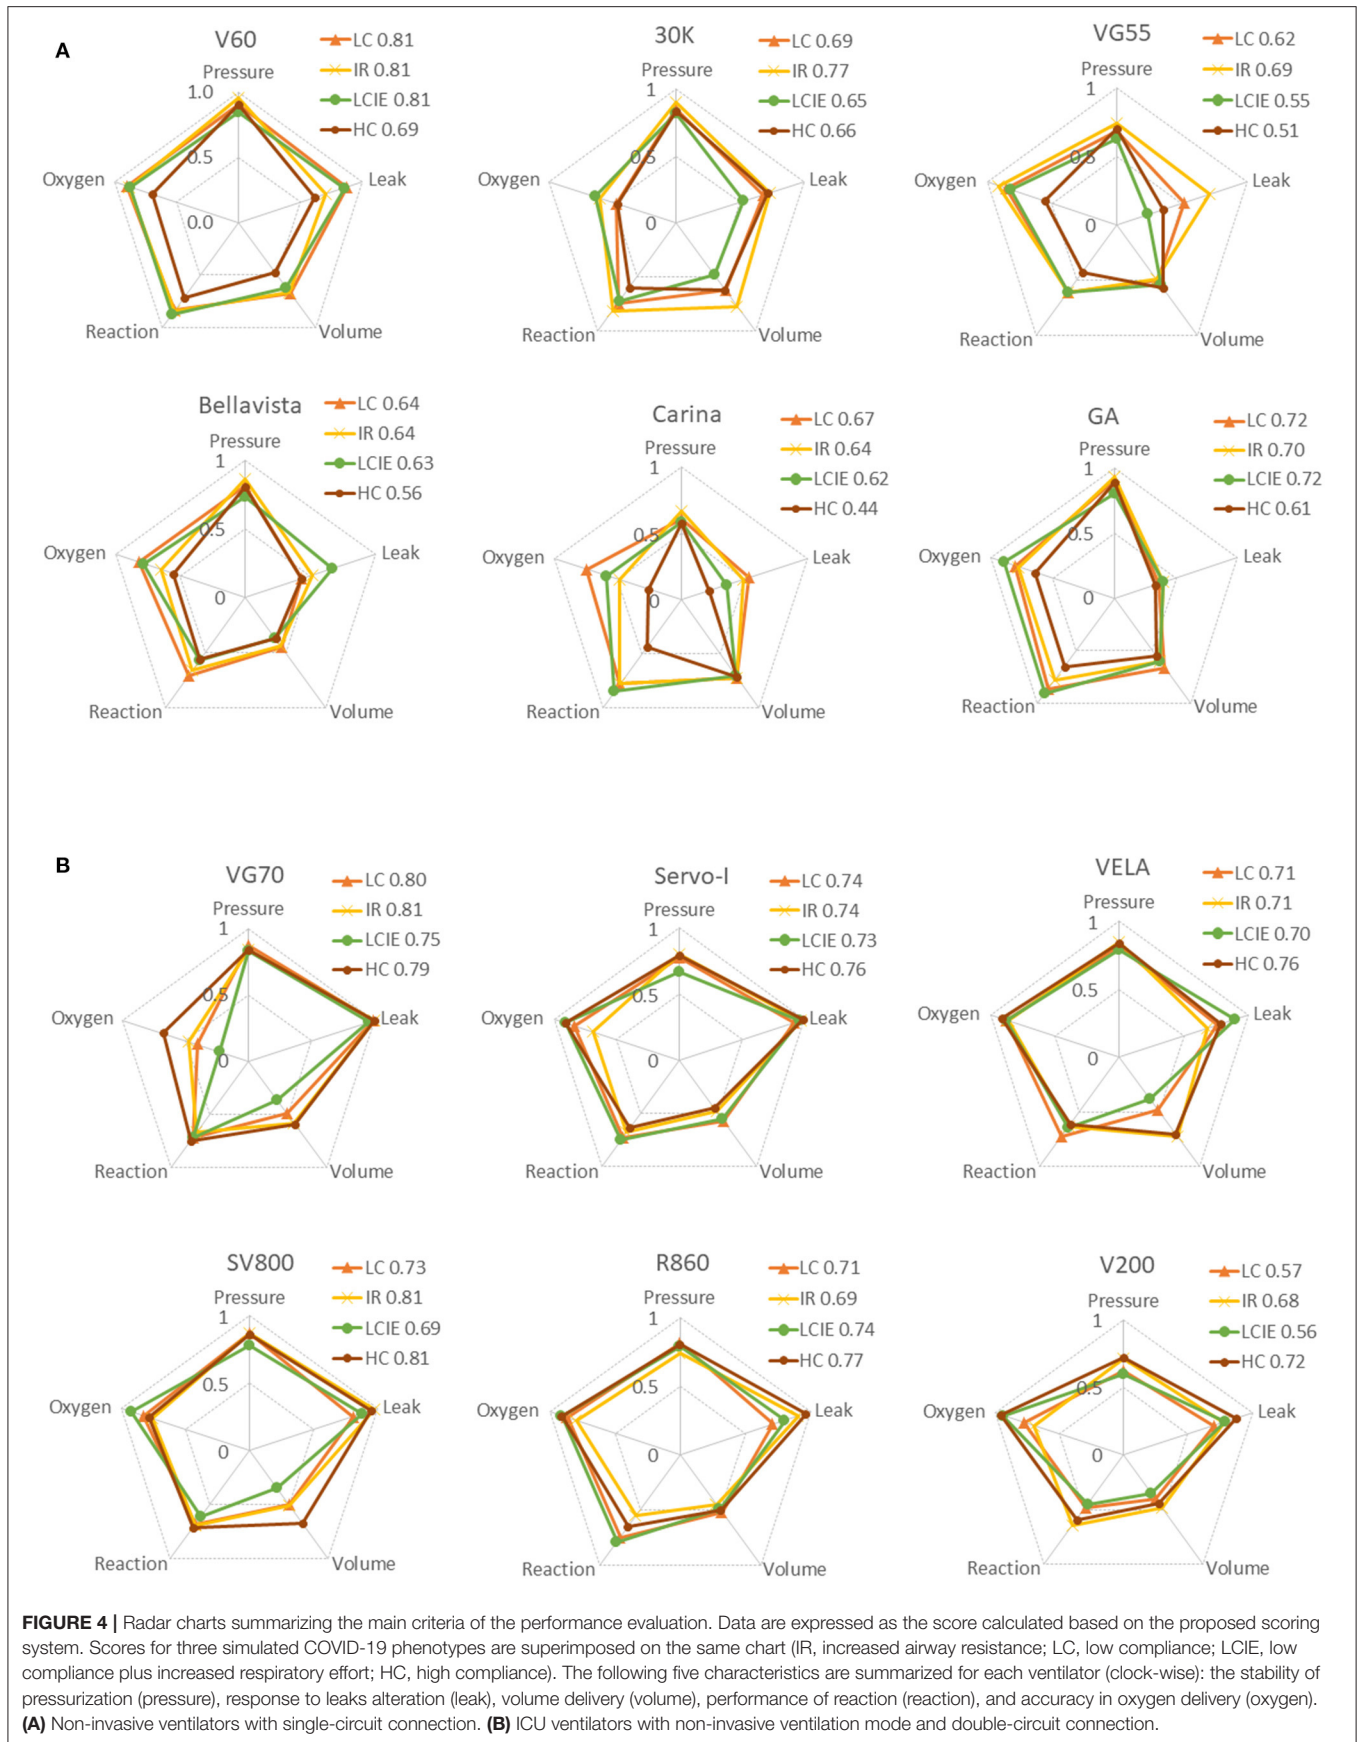

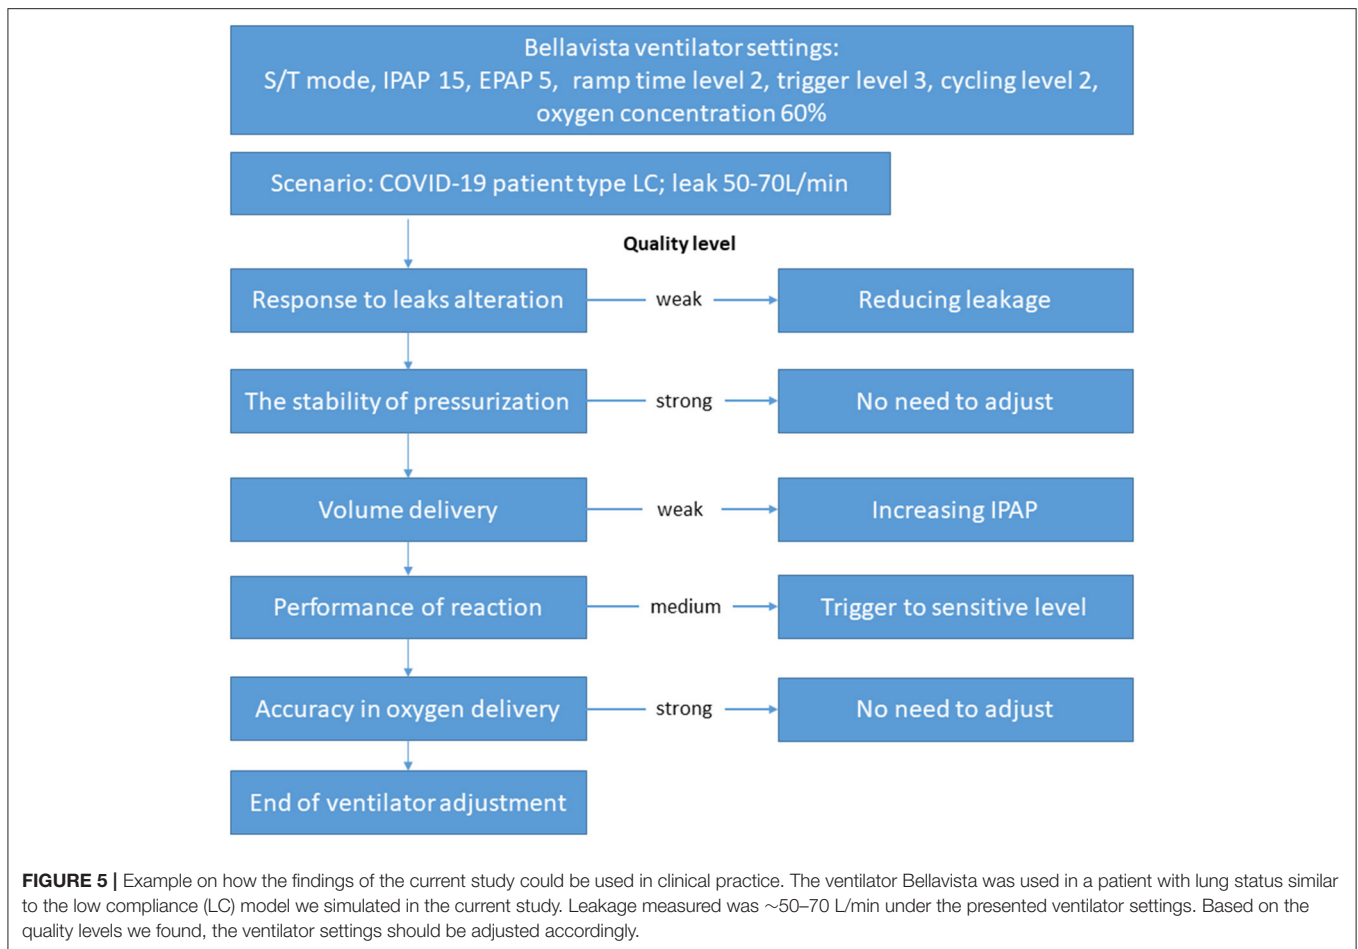

DATA AVAILABILITY STATEMENT

The original contributions generated for the study are included in the article/supplementary material, further inquiries can be directed to the corresponding author/s.

AUTHOR CONTRIBUTIONS

XH had full access to all of the data in the study and takes responsibility for the integrity of the data and the accuracy of the data analysis. XH, FX, KW, and HG had designed the study and analyzed the data, and revised the manuscript significantly. GM, RW, YZ, and QY had collected the data and revised the manuscript significantly. ZZ and LX contributed to study design and data interpretation, and drafted the manuscript.

REFERENCES

1. Ferreira JC, Chipman DW, Kacmarek RM. Trigger performance of mid-level ICU mechanical ventilators during assisted ventilation: a bench study. *Intensive Care Med.* (2008) 34:1669–75. doi: 10.1007/s00134-008-1125-5
2. Ferreira JC, Chipman DW, Hill NS, Kacmarek RM. Bilevel vs ICU ventilators providing noninvasive ventilation: effect of system leaks. *Chest.* (2009) 136:448–56. doi: 10.1378/chest.08-3018
3. Oto J, Chenelle CT, Marchese AD, Kacmarek RM. A comparison of leak compensation in acute care ventilators during noninvasive and invasive ventilation: a lung model study. *Respir Care.* (2013) 58:2027–37. doi: 10.4187/respcare.02466
4. Garnier M, Quesnel C, Fulgencio JP, Degrain M, Carteaux G, Bonnet E, et al. Multifaceted bench comparative evaluation of latest intensive care unit ventilators. *Br J Anaesth.* (2015) 115:89–98. doi: 10.1093/bja/aev028

All authors contributed to the article and approved the submitted version.

FUNDING

This work was supported by China PLA Key Grant (BLB18J008), National Key Research Program of China (2019YFC0121703), PLA General Hospital Translational Medicine Key Project (2018TM-03), and PLA General Hospital Clinical Support Fund (2018FC-WJFWZX-2-04). The funder had no role in study design, data collection and analysis, decision to publish, or preparation of the manuscript. Chinese National Science and Technology Key Grant (2021YFC0122500). PLA innovative project CX19030.

5. WHO. *Coronavirus Disease (COVID-2019) Situation Report – 106*. (2020). Available online at: https://www.who.int/docs/default-source/coronaviruse/situation-reports/20200505covid-19-sitrep-106.pdf?sfvrsn=47090f63_2 (accessed May 6, 2020).
6. Wu Z, McGoogan JM. Characteristics of and important lessons from the coronavirus disease 2019 (COVID-19) outbreak in China: summary of a report of 72314 cases from the chinese center for disease control and prevention. *JAMA*. (2020) 33:1239–42. doi: 10.1001/jama.2020.2648
7. Gattinoni L, Chiumello D, Rossi S. COVID-19 pneumonia: ARDS or not? *Crit Care*. (2020) 24:154. doi: 10.1186/s13054-020-02880-z
8. Liu, Y., Lv, J., Liu, J., Li, M., Xie, J., Lv, Q., et al. Mucus production stimulated by IFN-AhR signaling triggers hypoxia of COVID-19. *Cell Res*. (2020) 30:1078–87 doi: 10.1038/s41422-020-00435-z
9. Armocida B, Formenti B, Ussai S, Palestra F, Missoni E. The Italian health system and the COVID-19 challenge. *Lancet Public Health*. (2020) 5:e253. doi: 10.1016/S2468-2667(20)30074-8
10. Saaty TL. Relative measurement and its generalization in decision making why pairwise comparisons are central in mathematics for the measurement of intangible factors the analytic hierarchy/network process. *Rev. R. Acad. Cien. Serie A. Mat.* (2008) 102:251–318. doi: 10.1007/BF03191825
11. Vaidya OS, Kumar S. Analytic hierarchy process: An overview of applications. *Eur J Oper Res*. (2006) 169:1–29. doi: 10.1016/j.ejor.2004.04.028
12. Marini JJ, Gattinoni L. Time course of evolving ventilator-induced lung injury: the “shrinking baby lung.” *Crit Care Med*. (2020) 48:1203–9. doi: 10.1097/CCM.0000000000004416
13. Halpin DMG, Criner GJ, Papi A, Singh D, Anzueto A, Martinez FJ, et al. Global initiative for the diagnosis, management, and prevention of chronic obstructive lung disease: the 2020 gold science committee report on COVID-19 and COPD. *Am J Respir Crit Care Med*. (2021) 203:24–36. doi: 10.1164/rccm.202009-3533SO
14. Vivas Fernández FJ, Sánchez Segovia J, Martel Bravo I, García Ramos C, Ruiz Castilla D, Gamero López J, et al. ResUHUrge: a low cost and fully functional ventilator indicated for application in COVID-19 patients. *Sensors*. (2020) 20:6774 doi: 10.3390/s20236774
15. Doukas DJ, Paladino L, Hanuscin C, McMahon J, Quale J, Bhatt I, et al. Evaluating cross contamination on a shared ventilator. *Emerg Med J*. (2020) 38:220–3. doi: 10.1136/emermed-2020-209972
16. Platen PV, Pomprapa A, Lachmann B, Leonhardt S. The dawn of physiological closed-loop ventilation—a review. *Crit Care*. (2020) 24:121. doi: 10.1186/s13054-020-2810-1
17. Angus DC, Kelley MA, Schmitz RJ, White A, Popovich JJr. *Caring for the critically ill patient*. Current and projected workforce requirements for care of the critically ill and patients with pulmonary disease: can we meet the requirements of an aging population? *JAMA*. 284:2762–70. doi: 10.1001/jama.284.21.2762
18. Spadaro S, Karbing DS, Fogagnolo A, Ragazzi R, Mojoli F, Astolfi L, et al. Simulation training for residents focused on mechanical ventilation. *Simul Healthc*. (2017) 12:349–55. doi: 10.1097/SIH.0000000000000249

Conflict of Interest: The authors declare that the research was conducted in the absence of any commercial or financial relationships that could be construed as a potential conflict of interest.

Copyright © 2021 Hu, Xie, Wang, Gu, Mo, Wen, Zhao, Yang, Möller, Zhao and Xie. This is an open-access article distributed under the terms of the Creative Commons Attribution License (CC BY). The use, distribution or reproduction in other forums is permitted, provided the original author(s) and the copyright owner(s) are credited and that the original publication in this journal is cited, in accordance with accepted academic practice. No use, distribution or reproduction is permitted which does not comply with these terms.