



AALBORG UNIVERSITY
DENMARK

Aalborg Universitet

Basic Troubleshooting for Experimental Equipment

Johra, Hicham

Publication date:
2021

Document Version
Publisher's PDF, also known as Version of record

[Link to publication from Aalborg University](#)

Citation for published version (APA):

Johra, H. (2021). *Basic Troubleshooting for Experimental Equipment*. (1 ed.) Department of the Built Environment, Aalborg University. DCE Lecture notes No. 77

General rights

Copyright and moral rights for the publications made accessible in the public portal are retained by the authors and/or other copyright owners and it is a condition of accessing publications that users recognise and abide by the legal requirements associated with these rights.

- Users may download and print one copy of any publication from the public portal for the purpose of private study or research.
- You may not further distribute the material or use it for any profit-making activity or commercial gain
- You may freely distribute the URL identifying the publication in the public portal -

Take down policy

If you believe that this document breaches copyright please contact us at vbn@aub.aau.dk providing details, and we will remove access to the work immediately and investigate your claim.



DEPARTMENT OF THE BUILT ENVIRONMENT
AALBORG UNIVERSITY

Basic Troubleshooting for Experimental Equipment

Hicham Johra



Aalborg University
Department of the Built Environment
Division of Sustainability, Energy & Indoor Environment

Lecture Notes No. 77

Basic Troubleshooting for Experimental Equipment

by

Hicham Johra

September 2021

© Aalborg University

Scientific Publications at the Department of the Built Environment

Technical Reports are published for timely dissemination of research results and scientific work carried out at the Department of the Built Environment at Aalborg University. This medium allows publication of more detailed explanations and results than typically allowed in scientific journals.

Technical Memoranda are produced to enable the preliminary dissemination of scientific work by the personnel of the Department of the Built Environment where such release is deemed to be appropriate. Documents of this kind may be incomplete or temporary versions of papers—or part of continuing work. This should be kept in mind when references are given to publications of this kind.

Contract Reports are produced to report scientific work carried out under contract. Publications of this kind contain confidential matter and are reserved for the sponsors and the Department of the Built Environment. Therefore, Contract Reports are generally not available for public circulation.

Lecture Notes contain material produced by the lecturers at the Department of the Built Environment for educational purposes. This may be scientific notes, lecture books, example problems or manuals for laboratory work, or computer programs developed at the Department of the Built Environment.

Theses are monographs or collections of papers published to report the scientific work carried out at the Department of the Built Environment to obtain a degree as either PhD or Doctor of Technology. The thesis is publicly available after the defence of the degree.

Latest News is published to enable rapid communication of information about scientific work carried out at the Department of the Built Environment. This includes the status of research projects, developments in the laboratories, information about collaborative work and recent research results.

Published 2021 by
Aalborg University
Department of the Built Environment
Thomas Manns Vej 23
DK-9220 Aalborg Ø, Denmark

Printed in Aalborg at Aalborg University

ISSN 1901-7286
Lecture Notes No. 77

Table of Contents

1. Foreword	6
2. Simple Tests.....	7
3. General Approach to Troubleshooting Experimental Equipment.....	7
References.....	13

1. Foreword

The aim of this lecture note is to provide some basic knowledge and guidelines to troubleshoot typical problems occurring in experimental facilities and laboratories of Aalborg University, Department of the Built Environment [1], concerning only experimental equipment and instruments that perform measurements. This troubleshooting guidelines focus on the measurement capabilities of such equipment. Many of those common problems are due to a lack of caution when setting equipment up. It is thus believed that following the simple advice, guidelines and good practices of this document will probably solve 99% of all problems encountered by the operators.

2. Simple Tests


Always perform simple tests to verify that the sensor/instrument is reacting, that is reacting in the right direction (increase or decrease of the measured signal), that the reaction is not delayed, and that it measures what is expected for a known simple case. For example, a temperature sensor in a room should react quickly (with regards to its time constant), should not have large electric noise, should increase the measured temperature when pressing warm fingers on it, and should record room temperature if left in a room.

3. General Approach to Troubleshooting Experimental Equipment

As mentioned before, this document focuses on the measurement capabilities of experimental equipment and instruments. Experimental setups for measurements are usually composed of the following main elements:

- Sensors: transforming the measurand into a signal (usually electrical signal).
- Transducer/data acquisition card: acquiring (measuring), processing and transforming the sensors' signals into digital information. This digital information can be treated to generate valuable measurement information.
- Datalogger: usually software that records the digital information into a file in the memory of a computer.
- User interface: displays the measurement results onto a display for the experimental operator.

These different elements are linked together into a chain-of-information by connections: electrical wires, electrical cables, instrument drivers, software, screen, etc. If the operation of the instrument cannot proceed correctly or if there is no proper measurement recorded by the device and displayed to the operator, the most probable reason for the malfunction is that one of those connections is broken, inadequate or not configured properly. Consequently, systematically checking those elements will lead to rapid identification of the problem in most cases.

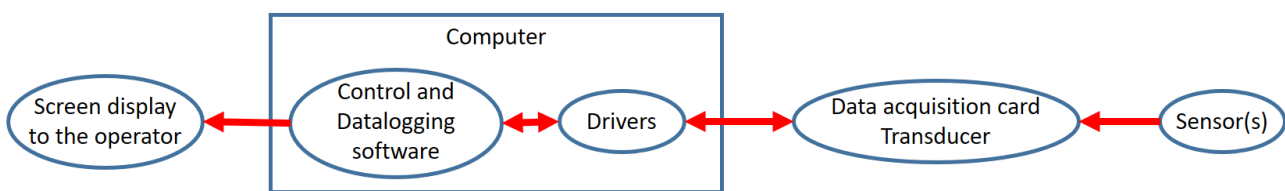


The chain-of-information


To optimize the chances of fixing rapidly the issue, it is recommended to follow a systematic problem location method: starting by checking what is the closest to the eyes of the operator and going down the chain-of-information until reaching the sensors. Some of the pieces of advice presented hereafter might seem obvious, common sense, or useless. However, one should not underestimate the probability of them solving most of the problems because many of those problems are due to simple (stupid) mistakes that all experimental operators make (even the ones with years of experience).

Basic troubleshooting workflow (from the most common to the least common problems):

1. **Check loose cables** and loose plugs for the computer display, the computer and the equipment connected to the computer. Also check proper connections of the sensors: some sensors might be mounted with loose screws or unsoldered wires. The connection plug of the sensor might be broken or unsoldered. There might be some short circuit due to wires without protective plastic sheath that are in direct contact. If in doubt of the integrity of the connections plugs inside a sensor or a device, contact the person in charge of the laboratory. Once permission has been granted from the latter, switch the device off, disconnect it from the power plug, and carefully dismount the casing to inspect the integrity of the wiring and soldering inside and that no loose wires create a short circuit.

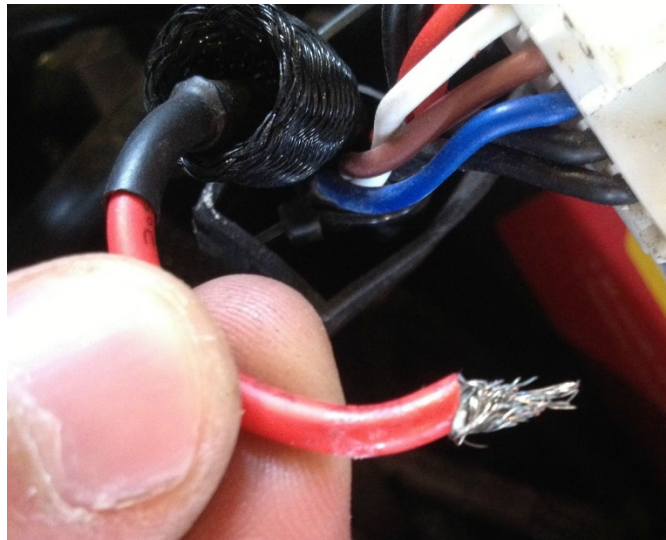


2. **Restart** the computer (switch off and on again), restart the equipment (switch off and on again), restart the software. This is usually perceived as a running joke, but it actually solves most of the problems in the daily tasks of an engineer.

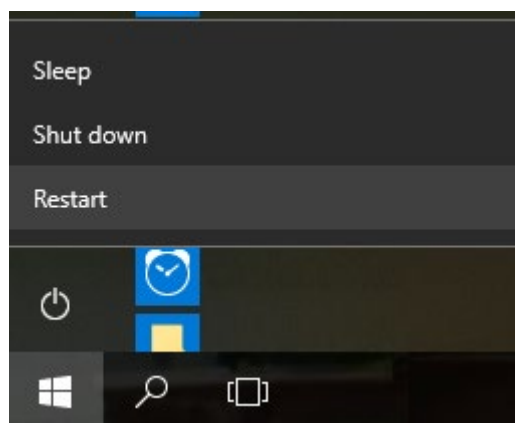

3. Check that all elements and **equipment are actually powered up** (power cable connected to a power socket that has power) and switched on. Switched off and on and make sure that something has changed in the equipment. Most devices do not have the same state when switched on or off: they make some

noise (ventilation fans), they have some LED switching on when powered up. Look for LED and verify in documentation if they should light up when the equipment is powered up. If the LED that is supposed to be on is not, or if ventilation fans are not running, then it probably means that the equipment is not powered up. Several possibilities: no electricity in the electrical socket (verify electrical socket of the electrical network with another device such as a desktop lamp); the power cable is broken (test another power cable); the fuse of the equipment is broken; the equipment is damaged.

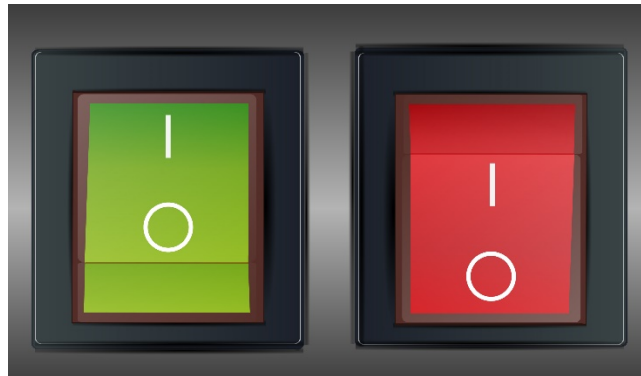


4. **Verify and change fuses:** Most experimental devices have one or several fuses to protect its power supply. Check that the fuses are not jumped off or burnt. You can usually access equipment's fuse by dismantling a small hatch next to the power supply block where the power cable is plugged in. Test the fuse with a multimeter (check for current continuity) if a visual inspection is not conclusive. If the fuse is broken, make sure to replace it with a new fuse that has the appropriate rated current (maximum current above which the fuse interrupts the circuit).



7. **Check measurement's parameters:** check that the measurement settings of the instrument are adequate for the measurement signal that is acquired: measurement mode, measurement channel, measurement range, filter, sampling/integration time, etc.
8. **Check Adapters:** Some connections from device to computers require adapters such as USB-serial adapter, GPIB-USB adapter, or 5-pin serial to 12-pin serial adapter. These adapters contain electronic chips that can be damaged, leading to information loss or total loss of communication. Similarly to communication cables, verify that the adapter is working properly by testing it on another device or setup that is working properly and that is using the same type of adapter.



9. **Verify the communication protocol parameters:** communication via serial, GPIB or USB cables (and many others) use communication protocols that require some specific communication parameters: COM port number, address number, baud rate, handshake control, stop bit, etc. Make sure that the software communicating with the device is using the right communication protocol parameters. Read the device's documentation to find this information. For serial, GPIB and Modbus communication protocol (among others), it is possible to download free software to test direct communication and manual basic commands: auto-detect, identification, polling. You can also verify with the computer device manager that it detects the connection of a device or adapter: detection of USB or serial device. For National Instruments hardware, use the dedicated management software NI-MAX. For Ethernet device with an IP, you can "ping" it directly with the cmd window of the computer. It should be noted that the automatic IP address allocation mode can prevent communication with the connected device. It is thus recommended to manually set the IP address to a fixed IP address that is not used by any other device in the local network.

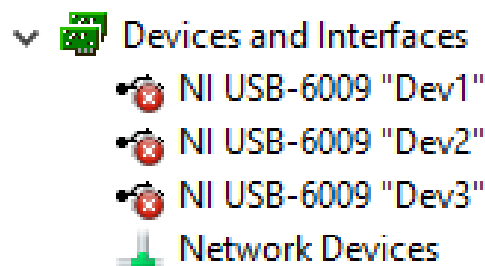

10. **Check drivers:** make sure that the adequate software drivers have been installed for the different hardware elements of your setup, including adapters such as Serial-USB or GPIB-USB adapters, or data acquisition cards. If in doubt, uninstall and reinstall the drivers, and check for the recent update of the drivers.

11. **Check sensor's response manually:** for sensors having an electric signal as an output signal, disconnect the sensor from the device and connect it directly to an oscilloscope or an electric signal acquisition board. Remember to power the sensor up adequately if the sensor is an active sensor (in opposition to passive sensors that do not require external power source). Measure the electric response of the sensor while varying the measurand and verify that the sensor's output signal is correct. It is thus possible to detect the potential malfunctions of the sensor itself: no signal, out-of-range signal, electric noise, inverted output signal, etc.



References

- [1] Aalborg University, Department of the Built Environment, Aalborg, Denmark.
<https://www.en.build.aau.dk/>

Recent publications in the Lecture Note Series

Hicham Johra. Simple data pre-processing of the laser flash analysis results from the LFA 447 apparatus. DCE Lecture Notes No. 72. Department of Civil Engineering, Aalborg University, 2019.

Hicham Johra. Description of the laser flash analysis method for thermal diffusivity measurement with the LFA 447. DCE Lecture Notes No. 73. Department of Civil Engineering, Aalborg University, 2019.

Hicham Johra. Guide to manually refill the liquid nitrogen tank of the LFA 447 apparatus. DCE Lecture Notes No. 74. Department of Civil Engineering, Aalborg University, 2019.

Hicham Johra. Description of the Guarded Hot Plate Method for Thermal Conductivity Measurement with the EP500. DCE Lecture Notes No. 75. Department of Civil Engineering, Aalborg University, 2019.

Hicham Johra. Thermophysical Properties of Building Materials: Lecture Notes. DCE Lecture Notes No. 76. Department of Civil Engineering, Aalborg University, 2019.

