

University of Groningen

Interpretation of Folate Results in Hemolytic Plasma Samples

Minovic, Isidor; Dikkeschei, Lambert D.; Vos, Michel J.; Kootstra-Ros, Jenny E.

Published in:
Annals of laboratory medicine

DOI:
[10.3343/alm.2021.41.5.485](https://doi.org/10.3343/alm.2021.41.5.485)

IMPORTANT NOTE: You are advised to consult the publisher's version (publisher's PDF) if you wish to cite from it. Please check the document version below.

Document Version
Publisher's PDF, also known as Version of record

Publication date:
2021

[Link to publication in University of Groningen/UMCG research database](#)

Citation for published version (APA):

Minovic, I., Dikkeschei, L. D., Vos, M. J., & Kootstra-Ros, J. E. (2021). Interpretation of Folate Results in Hemolytic Plasma Samples: A Practical Approach. *Annals of laboratory medicine*, 41(5), 485-488. <https://doi.org/10.3343/alm.2021.41.5.485>

Copyright

Other than for strictly personal use, it is not permitted to download or to forward/distribute the text or part of it without the consent of the author(s) and/or copyright holder(s), unless the work is under an open content license (like Creative Commons).

The publication may also be distributed here under the terms of Article 25fa of the Dutch Copyright Act, indicated by the "Taverne" license. More information can be found on the University of Groningen website: <https://www.rug.nl/library/open-access/self-archiving-pure/taverne-amendment>.

Take-down policy

If you believe that this document breaches copyright please contact us providing details, and we will remove access to the work immediately and investigate your claim.

Downloaded from the University of Groningen/UMCG research database (Pure): <http://www.rug.nl/research/portal>. For technical reasons the number of authors shown on this cover page is limited to 10 maximum.



Interpretation of Folate Results in Hemolytic Plasma Samples: A Practical Approach

Isidor Minović , Pharm.D., Ph.D.¹, Lambert D. Dikkeschei , Ph.D.², Michel J. Vos , Ph.D.¹, and Jenny E. Kootstra-Ros , Ph.D.¹

¹Department of Laboratory Medicine, University of Groningen, University Medical Center Groningen, Groningen, The Netherlands; ²Department of Laboratory Medicine, Isala, Zwolle, The Netherlands

Folate analysis in plasma is affected by hemolysis, which can lead to biased results. However, the degree of hemolysis that is considered acceptable is unclear. We explored the relationship between folate concentration and degree of hemolysis. Heparin plasma samples (N=77, hemolysis index ≤ 10 $\mu\text{mol/L}$) were spiked with increasing amounts of corresponding patient-specific hemolysate. Subsequently, the folate concentration and hemolysis index were measured using two Roche Cobas platforms, and their incremental relationship was investigated. The folate concentration ranged from 2.9 to 30.9 nmol/L with a median (interquartile range) of 11.4 (8.6–19.1) nmol/L. The linear relationship between the increments in folate concentration and hemolysis index was approximated by the function $y = 1.86x + 1.56$ ($R^2 = 0.996$), where x represents the laboratory-specific critical difference in folate concentration, which can be calculated from the analytical variation of the employed folate assay(s), and y represents the hemolysis threshold. The hemolysis threshold did not significantly differ between the tertiles of plasma folate concentration ($P = 0.10$). In conclusion, we have provided an evidence-based approach that can be used to reliably interpret folate concentrations in hemolytic samples, independent of the patient's folate status.

Key Words: Folate, Hemolysis, Hemolysis index, Relationship

Reliable assessment of folate status in clinical and non-clinical settings is greatly needed, as both deficiency and excessive exposure to folate can have serious adverse health effects [1, 2]. Folate status is frequently assessed by measuring the folate concentration in plasma using immunochemical assays available from various manufacturers [3]. The Roche Cobas e platform (Roche Diagnostics, Mannheim, Germany) is the most frequently used automated platform in Dutch hospitals according to external quality assessment schemes of the Dutch Foundation for Quality Assessment in Clinical Laboratories (SKML) [2, 4]. In the circulation, folate is mainly present in red blood cells (RBCs), and folate concentrations in RBCs are several fold higher than those in the plasma [5]. Consequently, there is a risk of overestimating folate concentration and underdiagnosing

folate deficiency when measuring folate concentration in hemolytic plasma samples. However, to our knowledge, the effect of hemolysis on plasma folate concentration remains elusive, leaving many clinical laboratories uninformed about interpreting folate status in hemolytic samples. It is largely unknown how hemolysis affects folate analysis in samples with a low, medium, and high plasma folate concentration. Therefore, in the most elaborate study conducted thus far, we investigated the relationship between folate concentration and degree of hemolysis in patient samples using Roche Cobas 8000 platforms. We established an evidence-based approach that aids in the interpretation of the folate concentration in slightly hemolytic plasma samples and examined whether this interpretation depends on the plasma folate concentration. This study was approved by

Received: September 4, 2020
Revision received: November 21, 2020
Accepted: March 15, 2021

Corresponding author:

Isidor Minović, Pharm.D, Ph.D.
Department of Laboratory Medicine,
University Medical Center Groningen,
Hanzeplein 1, 9713GZ, Groningen, the
Netherlands
Tel: +31 50-361-3781
Fax: +31 50-361-3932
E-mail: i.minovic@umcg.nl



© Korean Society for Laboratory Medicine

This is an Open Access article distributed under the terms of the Creative Commons Attribution Non-Commercial License (<https://creativecommons.org/licenses/by-nc/4.0>) which permits unrestricted non-commercial use, distribution, and reproduction in any medium, provided the original work is properly cited.

the Institutional Review Board of the University Medical Center Groningen, Groningen, the Netherlands (M20.262950).

Seventy-seven discarded and de-identified lithium heparin-anticoagulated plasma samples with a hemolysis index ≤ 10 $\mu\text{mol/L}$ and corresponding EDTA-anticoagulated whole blood samples (i.e., from the same patient and sampling time) used for routine patient care were collected randomly and retrospectively over a six-month period (July to December 2019). These samples had already been transported from the clinical units and general practitioners to the laboratories of the University Medical Center Groningen and Isala and had undergone centrifugation ($1,885 \times g$ for 5 minutes at 18°C), thus excluding a significant effect of either hemoglobin or folate from RBCs due to *in vitro* hemolysis. Hemolysates were prepared according to the osmotic shock procedure adapted from the CLSI guidelines (EP7-A2 and EP56) for interference analysis in clinical chemistry [6, 7]. Briefly, RBCs from 0.5 mL of whole blood were washed twice with a standard phosphate-buffered saline solution (VWR, Radnor, PA, USA) and hemolysates were obtained by adding 1 mL distilled water. Thereafter, all samples were stored in a dark container immediately at -80°C for at least 24 hours and were centrifuged before use.

Hemolysis was simulated by spiking the plasma samples with their corresponding hemolysate. To avoid any potential matrix effect, a three-level dose–response series was prepared for each patient by adding 2 μL (level 1), 4 μL (level 2), and 10 μL (level 3) of hemolysate to 198 μL , 196 μL , and 190 μL of plasma, respectively. The folate concentration and hemolysis index were analyzed at the University Medical Center Groningen on two Cobas 8000 platforms with c702 and e602 modules (Roche Diagnostics), and increments were calculated relative to the blank (i.e., unspiked) plasma. The CV_{folate} was 9.6% at a concentration of 6.3 nmol/L. Samples above the upper detection limit (folate >45.4 nmol/L) were excluded. The hemolysis index had a CV of 3.3%.

Hematology parameters [i.e., hemoglobin, RBC, mean corpuscular volume (MCV), and white blood cell count (WBC)] were measured on an XN-10 analyzer (Sysmex Corporation, Kobe, Japan). For hemoglobin and MCV, the inter-assay CV was 1.1% and 0.9%, respectively. Data analyses and computations were performed using SPSS 22.0 (IBM Corp., Armonk, NY, USA) and GraphPad Prism version 5.01 (GraphPad Software, San Diego, CA, USA). All data are presented as the median and interquartile range (IQR), because they were considered to be non-normally distributed. The potential influence of sample transportation, centrifugation, and cellular constitution (notably WBCs, which may alter the plasma fluid fraction [8] and may

also contain folate [9, 10]) on baseline folate concentrations, and the potential associations of the baseline hemolysis index, RBC, and WBC with baseline folate concentration were analyzed using univariate and multivariate linear regression analyses.

Since hemolysis was previously reported to be associated with an increase in plasma folate concentration [11], the critical difference in the laboratory-specific plasma folate concentration (CD_{folate}) was calculated with the formula [12]: $CD_{\text{folate}} = 1.65 \times \sqrt{2} \times CV_{\text{folate}}$. Changes greater than the CD_{folate} were interpreted as interference due to the hemolysate. The CD_{folate} was used to calculate the hemolysis threshold from the regression equations of the relationships between the increments in folate concentration and hemolysis index in the dose–response series. To explore the effect of hemolysis on to the plasma folate concentration, the samples were divided into tertiles according to the plasma folate concentration, and hemolysis thresholds were analyzed using an independent-samples median test. A two-sided $P < 0.05$ indicated statistical significance. To determine the implications of the newly established hemolysis threshold for folate concentration reporting, which was recently adopted in our laboratory, we compared it to our previous practice, in which folate concentrations with a hemolysis index > 2 $\mu\text{mol/L}$ were automatically flagged and reported with the cautionary comment “Hemolytic sample, result increased.” This comparison was based on a retrospective analysis, using folate concentrations and corresponding hemolysis indices reported over a one-yr period (April 1, 2019 to April 1, 2020). Folate concentrations in the plasma samples ranged from 2.9 to 30.9 nmol/L, with a median (IQR) of 11.4 (8.6–19.1) nmol/L. The median (IQR) hemolysis index was 4 (2–5) $\mu\text{mol/L}$. The folate concentration was not associated with the hemolysis index (standardized $\beta = -0.07$, $P = 0.57$; Table 1), indicating that the effect of a marginal degree of hemolysis on folate concentration in the plasma samples was neg-

Table 1. Associations of plasma folate concentration with the hemolysis index and red and white blood cell counts in patient samples

	Standardized β	<i>P</i> for trend
Univariate models		
Hemolysis index ($\mu\text{mol/L}$)	−0.07	0.57
Red blood cell count ($\times 10^{12}/\text{L}$)	−0.02	0.88
White blood cell count ($\times 10^9/\text{L}$)	−0.04	0.76
Multivariate model		
Hemolysis index ($\mu\text{mol/L}$)	−0.08	0.52
Red blood cell count ($\times 10^{12}/\text{L}$)	−0.03	0.80
White blood cell count ($\times 10^9/\text{L}$)	−0.05	0.67

ligible. The median (IQR) hemoglobin, RBC, MCV, and WBC in the whole blood samples were 129 (113–139) g/L, 4.2 (3.6–4.6) $\times 10^{12}$ /L, 92 (88–95) fL, and 7.2 (5.7–8.8) $\times 10^9$ /L, respectively. Neither RBC nor WBC was associated with the baseline plasma folate concentration (Table 1).

Based on the combined analytical variation of the folate assays (9.6%), a CD_{folate} of 22% was calculated. The linear function describing the relationship between the increment in folate concentration (x) and hemolysis index (y) was defined as $y = 1.86x + 1.56$ ($R^2 = 0.996$). The equation yielded a hemolysis threshold of 42 $\mu\text{mol/L}$ for our laboratory. These data extend the existing literature [11] by providing a tangible approach for defining the acceptable degree of hemolysis, which considers the biological variation of plasma folate, RBC folate, and hemoglo-

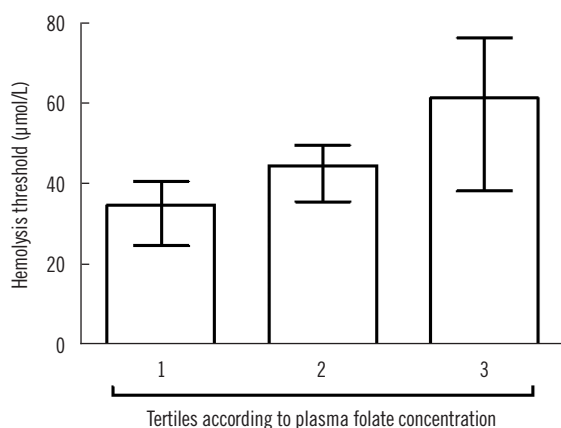


Fig. 1. Hemolysis thresholds across tertiles of plasma folate concentration. Columns represent median (IQR) hemolysis thresholds that were calculated from the dose–response series with a CD_{folate} of 22%. Abbreviations: IQR, interquartile range; CD_{folate} , critical difference in folate concentration.

bin concentration. Our approach considers the fact that the hemolysis threshold is dependent on the analytical variation of the folate assay and may differ across laboratories.

The median (IQR) hemolysis thresholds were not significantly different across tertiles of plasma folate concentration, at 35 (24–41), 44 (35–49), and 61 (39–77) $\mu\text{mol/L}$ for the first, second, and third tertile, respectively ($P = 0.10$; Fig. 1). This was likely due to the large combined inter-individual variation of hemoglobin [13, 14] and RBC folate concentration [15].

Over a one-year period, our laboratory performed 6,136 plasma folate concentration measurements. The hemolysis index followed a skewed distribution with a range of 0–201 $\mu\text{mol/L}$ and a median (IQR) of 4 (2–5) $\mu\text{mol/L}$ (Fig. 2). In 3,979 (65%) of the samples, the hemolysis index exceeded the hemolysis threshold of 2 $\mu\text{mol/L}$ and, accordingly, the folate concentration was flagged. When a hemolysis threshold of 42 $\mu\text{mol/L}$ was applied to the hemolysis index distribution, the flagging rate decreased to 0.01% (Fig. 2). The practical implications of the suggested approach may differ across laboratories, because they will depend on the current protocol used to assess and report the folate concentrations.

This study has several limitations. First, we only assessed plasma samples. Therefore, the suggested approach for calculating a hemolysis threshold should be used only when routine folate concentration is measured in plasma. Second, our data are based on the assumption that hemolysis assays represent everyday conditions of hemolytic samples transported from clinical units. Despite the swift preparation of hemolysates with a dose–response series and a single freeze–thaw cycle, we cannot fully exclude the possibility that a certain loss of reduced folates or incomplete dissociation of folates from cellular binding proteins

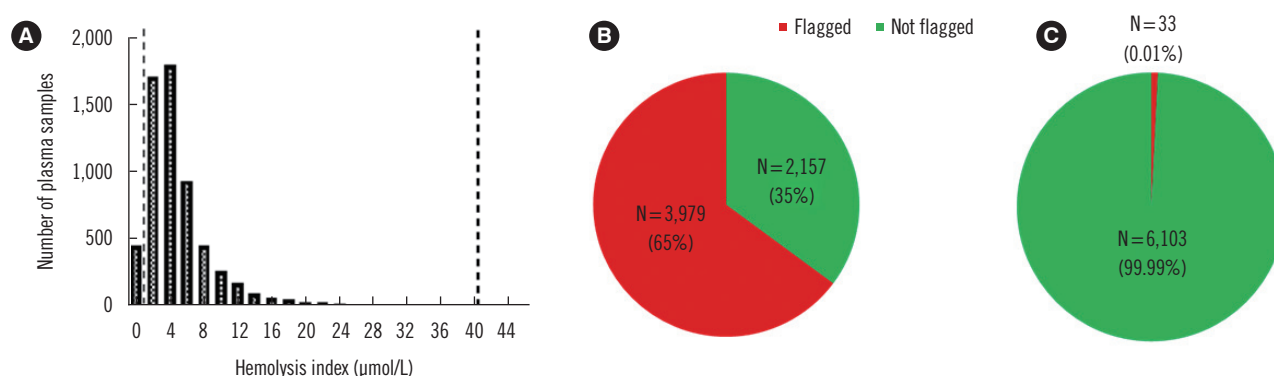


Fig. 2. Measured hemolysis indices and flagged folate concentrations. In the hemolysis index frequency distribution (A), the left and right dashed lines indicate hemolysis thresholds of 2 $\mu\text{mol/L}$ and 42 $\mu\text{mol/L}$, respectively. The pie charts show the proportions of flagged folate concentrations in our laboratory based on hemolysis thresholds of 2 $\mu\text{mol/L}$ (B) and 42 $\mu\text{mol/L}$ (C).

may have occurred during preparation of the hemolysates [16]. However, both situations would also hold true in the case of *in vitro* hemolysis occurring during the day-to-day transport of plasma samples. Thus, the hemolysis assays performed in this study are likely a good reflection of the sample conditions in routine practice. Third, we did not have information on RBC folate concentrations because RBC folate is not a routine diagnostic modality in the Netherlands. However, this parameter may be useful when plasma and RBC concentrations are discordant or when patients consistently produce hemolytic plasma samples [17].

In conclusion, the relationship between the degree of hemolysis and change in plasma folate concentration can be approximated with the equation $y = 1.86x + 1.56$, where x and y represent the laboratory-specific CD_{folate} and hemolysis threshold, respectively. The calculated hemolysis threshold can be used independent of the patient's folate status.

ACKNOWLEDGEMENTS

None.

AUTHOR CONTRIBUTIONS

Minović I, Vos MJ, and Kootstra-Ros JE designed the study. Minović I acquired the data, performed the statistical analyses, interpreted the data, and wrote the manuscript. Dikkeschei LD, Vos MJ, and Kootstra-Ros JE critically reviewed the manuscript. All authors have approved the final version of the manuscript and have agreed to be accountable for all aspects of the work.

CONFLICTS OF INTEREST

No potential conflicts of interest relevant to this article were reported.

RESEARCH FUNDING

None declared.

ORCID

Isidor Minović <https://orcid.org/0000-0002-5439-3781>
Lambert D. Dikkeschei <https://orcid.org/0000-0002-6171-9938>
Michel J. Vos <https://orcid.org/0000-0001-9379-2219>

Jenny E. Kootstra-Ros <https://orcid.org/0000-0002-1394-513X>

REFERENCES

1. Bailey LB, Stover PJ, McNulty H, Fenech MF, Gregory JFG, Mills JL, et al. Biomarkers of nutrition for development-folate review. *J Nutr* 2015; 145:1636S-80S.
2. Sobczyńska-Malefora A and Harrington DJ. Laboratory assessment of folate (vitamin B9) status. *J Clin Pathol* 2018;71:949-56.
3. Farrell CJ, Kirsch SH, Herrmann M. Red cell or serum folate: what to do in clinical practice? *Clin Chem Lab Med* 2013;51:555-69.
4. Thelen MHM, Jansen RTP, Weykamp CW, Steigstra H, Meijer R, Cobbaert CM. Expressing analytical performance from multisample evaluation in laboratory EQA. *Clin Chem Lab Med* 2017; 55:1509-16.
5. WHO. Serum and red blood cell folate concentrations for assessing folate status in populations. https://www.who.int/nutrition/publications/micronutrients/indicators_serum_RBC_folate/en/ (Updated in 2015).
6. CLSI. Interference testing in clinical chemistry: approved Guideline. 2nd ed. CLSI ep7-A2. Wayne, PA: Clinical and Laboratory Standards Institute. 2005.
7. CLSI. Hemolysis, icterus, and lipemia/turbidity indices as indicators of interference in Clinical Laboratory Analysis; approved guideline. CLSI ep56. Wayne, PA: Clinical and Laboratory Standards Institute, 2012.
8. Grzych G, Roland E, Beauvais D, Maboudou P, Brousseau T. Benefit of point of care testing in patient with major hyperleukocytosis. *Clin Biochem* 2019;65:55-7.
9. Swendseid ME, Bethell FH, Bird OD. The concentration of folic acid in leukocytes; observations on normal subjects and persons with leukemia. *Cancer Res* 1951;11:864-7.
10. Rana OB, Lagerlöf B, Einhorn J, Reizenstein PG. Folic acid activity in leukemia and cancer. *Cancer Res* 1965;25:221-4.
11. Monneret D, Mestari F, Atlan G, Corlouer C, Ramani Z, Jaffre J, et al. Hemolysis indexes for biochemical tests and immunoassays on Roche analyzers: determination of allowable interference limits according to different calculation methods. *Scand J Clin Lab Invest* 2015;75:162-9.
12. Coskun A, Serteser M, Karpuzoglu HF, Unsal I. How can we evaluate differences between serial measurements on the same sample? A new approach based on within-subject biological variation. *Clin Chem Lab Med* 2017;55:e44-6.
13. Borel MJ, Smith SM, Derr J, Beard JL. Day-to-day variation in iron-status indices in healthy men and women. *Am J Clin Nutr* 1991;54:729-35.
14. Pineda-Tenor D, Laserna-Mendieta EJ, Timón-Zapata J, Rodelgo-Jiménez L, Ramos-Corral R, Recio-Montealegre A, et al. Biological variation and reference change values of common clinical chemistry and haematologic laboratory analytes in the elderly population. *Clin Chem Lab Med* 2013;51:851-62.
15. Lacher DA, Hughes JP, Carroll MD. Biological variation of laboratory analytes based on the 1999-2002 National Health and Nutrition Examination Survey. *Natl Health Stat Report* 2010;21:1-7.
16. Pfeiffer CM and Gregory JF 3rd. Enzymatic deconjugation of erythrocyte polyglutamyl folates during preparation for folate assay: investigation with reversed-phase liquid chromatography. *Clin Chem* 1996;42:1847-54.
17. Galloway M and Rushworth L. Red cell or serum folate? Results from the National Pathology Alliance benchmarking review. *J Clin Pathol* 2003;56:924-6.