

University of Groningen

An adaptive hybrid control architecture for an active transfemoral prosthesis

Mazumder, Aniket; Hekman, Edsko E.G. ; Carloni, Raffaella

Published in:
IEEE Access

DOI:
[10.1109/ACCESS.2022.3173348](https://doi.org/10.1109/ACCESS.2022.3173348)

IMPORTANT NOTE: You are advised to consult the publisher's version (publisher's PDF) if you wish to cite from it. Please check the document version below.

Document Version
Publisher's PDF, also known as Version of record

Publication date:
2022

[Link to publication in University of Groningen/UMCG research database](#)

Citation for published version (APA):

Mazumder, A., Hekman, E. E. G., & Carloni, R. (2022). An adaptive hybrid control architecture for an active transfemoral prosthesis. *IEEE Access*, 10, 52008-52019. <https://doi.org/10.1109/ACCESS.2022.3173348>

Copyright

Other than for strictly personal use, it is not permitted to download or to forward/distribute the text or part of it without the consent of the author(s) and/or copyright holder(s), unless the work is under an open content license (like Creative Commons).

The publication may also be distributed here under the terms of Article 25fa of the Dutch Copyright Act, indicated by the "Taverne" license. More information can be found on the University of Groningen website: <https://www.rug.nl/library/open-access/self-archiving-pure/taverne-amendment>.

Take-down policy

If you believe that this document breaches copyright please contact us providing details, and we will remove access to the work immediately and investigate your claim.

Downloaded from the University of Groningen/UMCG research database (Pure): <http://www.rug.nl/research/portal>. For technical reasons the number of authors shown on this cover page is limited to 10 maximum.

Received March 10, 2022, accepted April 11, 2022, date of publication May 9, 2022, date of current version May 19, 2022.

Digital Object Identifier 10.1109/ACCESS.2022.3173348

An Adaptive Hybrid Control Architecture for an Active Transfemoral Prosthesis

ANIKET MAZUMDER¹, EDSKO E. G. HEKMAN², (Member, IEEE),
AND RAFFAELLA CARLONI¹, (Member, IEEE)

¹Faculty of Science and Engineering, Bernoulli Institute for Mathematics, Computer Science and Artificial Intelligence, University of Groningen, 9747 AG Groningen, The Netherlands

²Department of Biomechanical Engineering, Faculty of Engineering Technology, University of Twente, 7522 NB Enschede, The Netherlands

Corresponding author: Aniket Mazumder (a.mazumder@rug.nl)

This work was supported by the European Commission's Horizon 2020 Program as part of the Project MyLeg under Grant 780871.

ABSTRACT The daily usage of a prosthesis for people with an amputation consists of phases of intermittent and continuous walking patterns. Based on this observation, this paper introduces a novel hybrid architecture to control a transfemoral prosthesis, where separate algorithms are used depending on these two different types of movement. For intermittent walking, an interpolation-based algorithm generates control signals for the ankle and knee joints, whereas, for continuous walking, the control signals are generated utilizing an adaptive frequency oscillator. A switching strategy that allows for smooth transitioning from one controller to another is also presented in the design of the architecture. The individual algorithms for the generation of the joints angles' references, along with the switching strategy were experimentally validated on a pilot test with a healthy subject wearing an able-bodied adapter and a designed transfemoral prosthesis. The results demonstrate the capability of the individual algorithms to generate the required control signals while undergoing smooth transitions when required. Through the use of a combination of interpolation and adaptive frequency oscillator-based methods, the controller also demonstrates its response adaptation capability to various walking speeds.

INDEX TERMS Prosthetics, rehabilitation robotics, control design.

I. INTRODUCTION

The restoration of mobility for people with transfemoral amputation is essential to improve their quality of life. However, through the use of passive prostheses, only a partial restoration may be achieved. This is primarily due to their limited adaptation capability to different activities of daily living. To ease ambulation, the development of active transfemoral prostheses is considered an important area of research, as they provide suitable actuation to the joints thanks to the control strategies designed to achieve the desired system behavior.

In literature, various architectures have been proposed for the control of active transfemoral prostheses, as summarized in Table 1. In [1], [18], a multi-modal intent recognizer for a transfemoral prosthesis is proposed and designed for different locomotion modes, comprising level-ground walking and stair/ramp climbing, while two supplementary modes of stand-still and stumble are added to improve the safety

The associate editor coordinating the review of this manuscript and approving it for publication was Nasim Ullah¹.

of the system. A similar state machine is designed for the transfemoral prostheses in [2]–[4] and [5] were, based on gait events (i.e., heel-strike, flat-foot, and toe-off), the phases of walking are classified into different states (i.e., controlled plantarflexion, controlled dorsiflexion, powered plantarflexion, and knee swing). Inspired by [1], an echo control strategy running atop the previously mentioned state machine is discussed in [6], [7] and [8], where a modified motion of the healthy leg is played back on the contralateral side, while [2], [9] and [11] discuss a state machine-based impedance control. There are also methods found in the literature that allow for speed adaptation and obstacle crossing over by the use of joint torque regulation through the generation of quasi-stiffness torque profiles [19] and use of heuristic techniques [20]. Apart from the state machine and echo control strategies, in the past few years, significant efforts have also been made using electromyography (EMG) from residual-limb muscles to classify user intent and then impose a pre-determined gait trajectory. Progress using this method has been demonstrated in [12], [21]–[23] and [17]. Furthermore, in recent times with the improvement in processing power of onboard

TABLE 1. Relevant research on the control architectures of lower-limb prostheses.

[Ref.] Year	Research focus	Type	Control Strategy
[1] 1982	Multi-mode above-knee prosthesis controller	Ankle/Foot	Multi-mode state machine
[2] 2009	Powered ankle-foot prosthesis improves walking metabolic economy	Knee/Ankle	Gait event-based state machine
[3] 2013	Ankle/knee prosthesis with powered ankle energy transfer (CYBERLEGS- α)	Knee	Gait event-based state machine
[4] 2011	Metabolic cost of walking comparison	Knee	Gait event-based state machine
[5] 2014	CYBERLEGS: A user-oriented robotic transfemoral prosthesis	Knee/Ankle	Gait event-based state machine
[6] 2008	Design and control of an active electrical knee and ankle prosthesis	Knee/Ankle	Echo control
[7] 2008	Design and control of powered transfemoral prosthesis	Knee/Ankle	Echo control
[8] 2009	A powered self-contained knee and ankle prosthesis for near normal gait	Knee/Ankle	Echo control
[9] 2014	WalkMECHadapt	Knee	Iterative learning control
[10] 2014	Virtual constraint based control of powered leg	Knee/Ankle	Virtual constraint defining joint patterns
[11] 2015	A powered prosthesis intervention for bilateral transfemoral amputee	Knee/Ankle	State machine with impedance control
[12] 2015	Intuitive control of powered prosthetic leg during ambulation	Knee/Ankle	EMG-based control
[13] 2012	Cybernetic knee prosthesis	Knee/Ankle	AFO-based control
[14] 2019	Phase variable approach for rhythmic & non-rhythmic human locomotion	Knee/Ankle	Knee angle phase variable control
[15] 2020	Online estimation of continuous gait phase for transtibial prosthesis	Ankle/Foot	AFO-based control
[16] 2020	Compliant control of transfemoral prosthesis	Knee/Ankle	AFO-based control
[17] 2021	Stand, squat, lunge, walk with knee/ankle prosthesis with Neural Control	Knee/Ankle	EMG-based control

computers, computer vision and range sensors, have also been proposed to improve classification accuracy, as shown in [24], [25] and [26].

A phase variable control approach, wherein a single variable can parameterize the entire gait cycle of the prosthetic leg, is often used to determine motion trajectories as an alternate to EMG and state machine methods. In [10] the progression of the center of pressure was used as a phase variable for gait tracking, while [27] and [28] showed the existence of multiple angles associated with the hip joint that might be used as phase variable candidates in gait tracking for multiple activities.

An extension of the phase-variable approach to prosthesis control is the controller design based on central pattern generators or Adaptive Frequency Oscillators (AFOs) [29], [30], wherein virtual joint angle references are generated to guarantee continuous control of prosthetic limbs by coupling the gait frequency with the frequency of the oscillators, as shown in prosthesis [13], [15], [16] and orthotic devices [31]–[33]. This is achieved by using a mathematical periodic function with an initial starting frequency on which the frequency of the gait cycle is dependent. Over the course of multiple gait cycles, a change in gait frequency causes a change in the period of the function. Although AFOs are capable of allowing for continuous trajectory generation for repetitive tasks, usually in applications, their allowable frequency variance is fixed between maximum and minimum limits. Beyond these limits the performance of oscillators for gait tracking becomes unsatisfactory.

In this study, we contemplated upon the observation that the natural human gait in everyday life is a combination of cyclic and acyclic phases [34], [35]. For example, movements inside closed/confined spaces (e.g., indoors, such as living-room, kitchen, etc.) are generally intermittent in nature, whereas, outdoor walking is generally more repetitive with a maintained gait speed. Building upon this observation, we propose a hybrid control architecture in which periods of continuous movement (i.e., level ground walking at

different velocities) are controlled by AFOs, while the aperiodic phases (i.e., start and stop walking) are controlled by using interpolation techniques through the detection of gait events (i.e., heel strike and toe-off). Throughout the operation of the system, the AFO algorithm runs in parallel to the state machine, while the hybrid nature of the controller ensures smooth transitioning between the two control modes.

The significance of using such an approach is twofold. Firstly, in the case of a singular state-machine-based system, the walking speeds of the subject for slow, normal, and fast walking are usually determined experimentally, followed by which, joint-angular velocities are used as a reference for various walking efforts. On the other hand, in a system supplemented with an oscillator-based speed adaptive algorithm, this is not necessary as the AFO automatically and continuously adapts the joints' reference angles according to the walking speed, estimated using inertial measurement units (IMUs). Moreover, in a singular state machine approach, the speed change is discrete and the extent of change is predetermined through experiments. On the other hand, AFO adaptations have the inherent benefit of having a continuous speed change. Secondly, an AFO algorithm running in parallel to the state machine might act as a fallback method for reference generation for the system during emergencies, such as the failure of onboard sensors (force, pressure sensors). Usually, a sudden failure of onboard sensors in a prosthetic system results in the system becoming unusable. On the another hand by supplementing the control system with a gait tracking algorithm that depends on inputs from a single IMU only, a limited operation of the prosthesis might still be possible. Finally, when the only IMU in the system fails, the safety of the user must be ensured by locking the joint positions to a neutral position for the ankle and a hyper-extended knee.

The adaptive hybrid control architecture proposed in this study has been implemented and tested in a custom-made transfemoral prosthesis that has been designed for level ground walking at different velocities, with an eye on mechanical simplicity and lightness in weight.

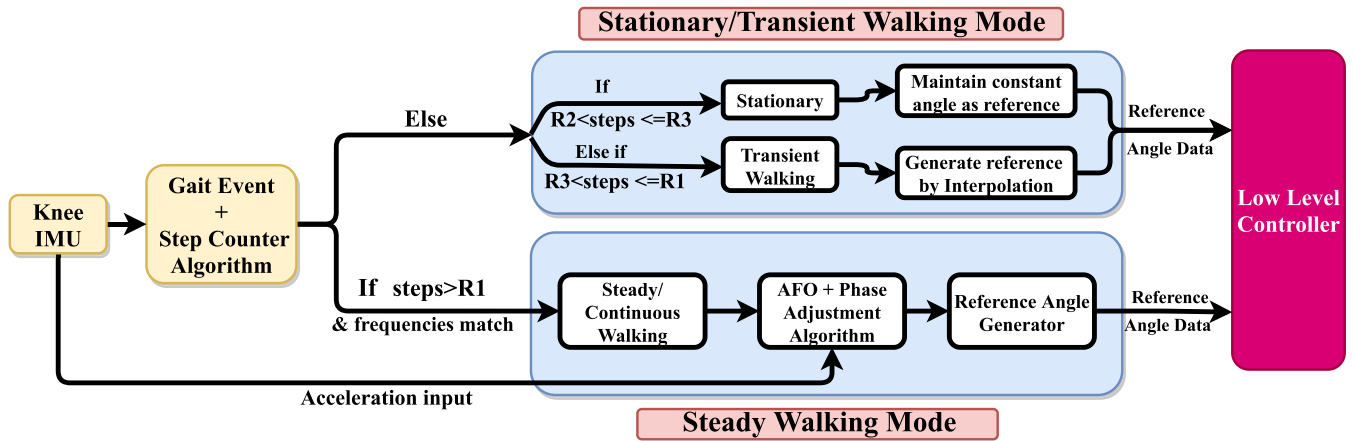


FIGURE 1. The high-level control of the transfemoral prosthesis. $R1 = 6$, $R2 = 0$, and $R3 = 2$ represent the threshold of step count for mode change. When the step count is between $R2$ and $R3$, the prosthesis is stationary, and, when the step count is between $R3$ and $R1$, the prosthesis is in transient walking. Whenever the number of steps goes beyond $R1$, the prosthesis is in steady-state walking. In the stationary/transient mode, the references are generated directly by a state machine, while in the steady-state walking mode, the AFO adapts the prosthesis response to vary its walking speeds.

Experiments with the prosthesis using an able-bodied adapter show that the control architecture is capable of generating reference angles for the ankle and knee joints, in both start/stop walking (using the state machine-based control) and continuous walking at different speeds (using the AFO-based control).

The remainder of the paper is organized as follows. The hybrid control architecture for a transfemoral prosthesis is presented in Section II. Section III describes the mechatronic design of the transfemoral prosthesis that has been realized to validate the control architecture. The experimental results are presented and discussed in Sections IV and V, respectively. Finally, concluding remarks are drawn in Section VI.

II. HYBRID CONTROL ARCHITECTURE

The proposed adaptive hybrid control architecture, as shown in Figure 1, is responsible for the detection of the mode of the prosthesis (namely whether the user is stationary, starts/stops walking, or walks continuously), along with the generation of the reference angles for the knee/ankle joints. A low-level motor controller, then, tracks these reference angles while monitoring the peak torque and current limits.

The controller receives the vertical acceleration data from a single IMU (MPU 9250-9 DOF, Sparkfun USA, www.sparkfun.com) placed above the knee joint. These data are then used to detect heel strike gait events and to keep a count of the number of steps taken by the prosthesis' user. The flowchart of the gait event detection function used in the prosthesis is shown in Figure 2. The algorithm uses the vertical component of the filtered accelerometer data sourced at 200Hz to detect gait events. At any given time, two data points (latest and previous) are compared against a set threshold to set/unset a flag for a gait event. The threshold is determined experimentally based on the chosen sensitivity, measurement ranges, placement/orientation, and data filtration bandwidth of the IMU. For the current application with

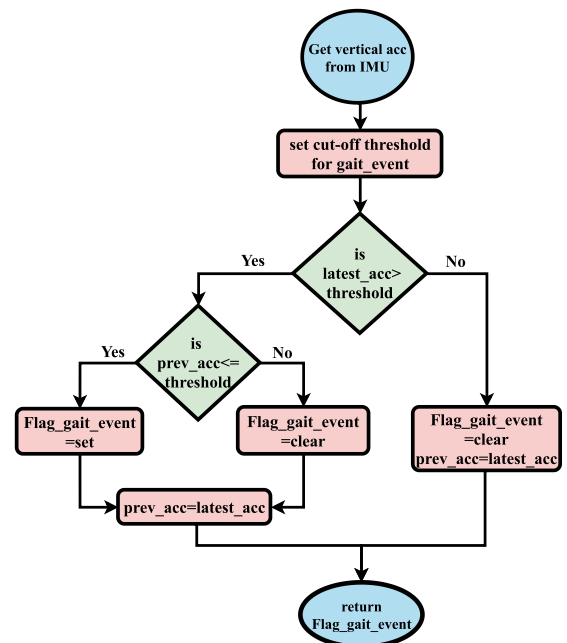


FIGURE 2. Flowchart showing the gait event detection function, which uses accelerometer data to set/unset the gait-event flag. This information is then sent to the step counter algorithm for counting steps.

an IMU sensitivity of 4 G, a cut-off of 1.2 G proved to be a reliable threshold for comparison. The output of this algorithm is then sent to the step counter algorithm for counting the number of steps and classifying whether the prosthesis is in motion or stationary.

The flowchart of the step counter algorithm is shown in Figure 3. The algorithm takes the flag of the gait event from the gait-event detection algorithm along with a record of the system time during the last detected positive gait event as input and compares the time duration between two successive gait events. In the case where this time difference lies between

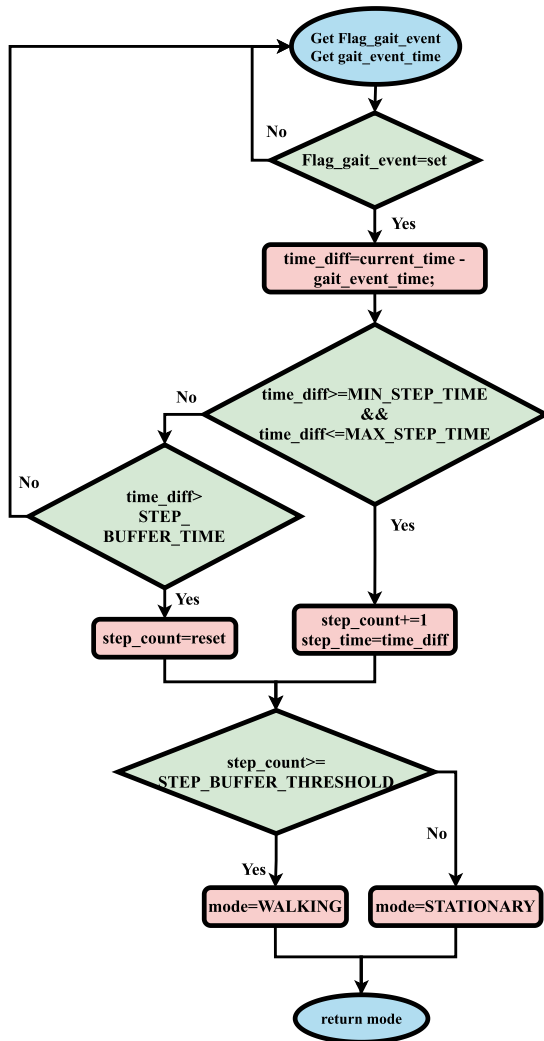


FIGURE 3. Flowchart for the step counter algorithm. It uses event data from the gait event detection algorithm and uses them to count the number of steps taken by the prosthesis. This information is then used to determine the mode of the prosthesis.

a minimum and maximum of allowed step time, the event is considered a valid step, and the step count increases. For the current application, the minimum and maximum limits to be considered a step were set at 250 ms and 2200 ms, respectively. In the cases where it lies outside these limits, a further check is made by comparing it to the allowed step buffer time. If the time difference is greater than the step buffer time, the step counter is reset. For the current application, the step buffer time was selected to be 2800 ms. In this way, the two algorithms working together can keep track of gait events and step counts. Once more than 2 steps are detected by the algorithm, the prosthesis is considered to be in motion, while for a step count lesser than 2 the prosthesis is considered to be stationary.

Formally, both algorithms process the data and generate an angle reference pattern, but only one is actually used/activated while the other one is suppressed. Herein lies

the hybrid nature of the controller, which is capable of switching from one mode to the other.

A. STATIONARY AND TRANSIENT WALKING MODE

In the stationary and transient walking mode, two different reference angles are generated. When the prosthesis is detected to be stationary, fixed values of angles are maintained at the joints. On the other hand, when the prosthesis is detected to be in transition walk, predetermined reference angles are imposed on the joints. The reference angles are computed starting from a vector $y(n)$, with $n \leq N$, containing the angular kinematics of one gait-cycle of healthy subjects during normal level ground walking [36]. Here N is the number of data points in one gait cycle determined at normal walking speed and fixed frequency determined by the system's frequency (200Hz in this case), whereas $y(n)$ is the vector determined by resampling the reference data at the same frequency and walking speed. Starting from this, a new vector $\bar{y}(\bar{n})$ is generated by using the step time information from the heel strike gait events. Specifically, the reference angles $\bar{y}(\bar{n})$, with $\bar{n} \leq \bar{N}$, are computed in real-time by using a linear interpolation technique. The total number of reference angle points \bar{N} in one footstep is given by:

$$\bar{N} = N \cdot (\text{latest_st} / \text{ref_st})$$

where ref_st is the step time in the reference data [36] and latest_st is the step time of the latest gait-cycle. For every new step, the reference angles $\bar{y}(\bar{n})$ is given by:

$$\bar{y}(\bar{n}) = y(p) + q \cdot (y(p+1) - y(p))$$

with $p = \lfloor n \cdot N / (\bar{N} - 1) \rfloor$ and $q = \{ n \cdot N / (\bar{N} - 1) \}$, where $\lfloor \cdot \rfloor$ indicates the floor function and $\{ \cdot \}$ the fractional function.

Following this for every footstep, a single value of reference angle is used as output, based on the prosthesis state, and time as input. In this way, varied references are generated from a fixed-speed system. This method of reference generation is active when the subject is undergoing start/stop and transient walking (e.g., walking in confined spaces), and is yet to cross the step threshold R1. This mode is also active when the number of steps taken by the subject crosses R1 and yet the frequency and angles of the gait cycle detected using the AFO and the interpolation techniques are not close enough for a switch. Thus, in the stationary mode fixed values of angles are maintained, while in the transient mode, time-varying angles corresponding to variable walking speeds are generated.

B. CONTINUOUS WALKING MODE

The continuous walking mode is active when the number of steps taken by the user goes beyond the step threshold R1 and a gait frequency and angle match happen between the AFO and interpolation methods [29], [30]. In this mode, the phase of an adaptive oscillator is used to generate the reference angles for the joints. The adaptive oscillator based algorithm as shown in Algorithm 1, consists of M sinusoidal

Algorithm 1 Gait Adaptation Algorithm

Input: *mode_IMU*, *no_of_steps*, *current_acc*
Output: *gaitPhase*

1 Initialize: $M \leftarrow 3$; $v \leftarrow 6$; $\epsilon \leftarrow 10$; $f_{min} \leftarrow 0.4$; *temp_step_count* $\leftarrow 0$
2

$$\text{ZeroValues} : Y_0 \leftarrow \begin{bmatrix} \phi_0 \\ \omega_0 \\ \alpha_0 \\ \beta_0 \end{bmatrix} = \begin{bmatrix} 0_{M \times 1} \\ 2\pi f_{min} \\ 0_{M \times 1} \\ 0_{1 \times 1} \end{bmatrix}_{(2M+2) \times 1}$$

/* get vertical acceleration from IMU */
3 $a_z \leftarrow \text{IMU}$
/* remove acceleration due to gravity */
4 $A_{des}(t) \leftarrow a_z - 9.8$
/* estimate acceleration */
5 $A_{est}(t) \leftarrow \beta_{t-1} + \sum_{i=1}^M \alpha_{t-1}(i) \sin(\phi_{t-1}(i))$
/* formulate teaching signal */
6 $T(t) \leftarrow (A_{des} - A_{est})$

$$\begin{bmatrix} \dot{Y}_t(i) \\ \dot{Y}_t(M+1) \\ \dot{Y}_t(M+1+i) \\ \dot{Y}_t(2M+2) \end{bmatrix} = \begin{bmatrix} iY_{t-1}(M+1) + \epsilon T(t) \cos(Y_{t-1}(i)) \\ \epsilon T(t) \cos(Y_{t-1}(1)) \\ vT(t) \sin(Y_{t-1}(i)) \\ vT(t) \end{bmatrix}$$

/* integrate */
7 $Y_t \leftarrow \int \dot{Y}_t$
/* Adjust phase based on prosthesis state */
8 **if** *mode* = *STATIONARY* **then**
| /* reset AFO array */
9 | $Y_t(\text{CHOSEN_OSC}) \leftarrow 2\pi f_{min}$
10 **end**
11 **else**
| /* get phase from oscillator */
12 | $Y_t(\text{CHOSEN_OSC}) \leftarrow f_{mod}(Y_t(1), 4\pi)$
13 **end**
/* Prevent Oscillator frequency from falling below minimum frequency */
14 **if** $Y_t(M) < 2\pi f_{min}$ **then**
15 | $Y_t(M) = 2\pi f_{min}$
16 **end**
17 $\text{gaitPhase} \leftarrow (\text{CHOSEN_OSC} * 100) / (4\pi)$
/* Return gait phase */
18 **return** *gaitPhase*

oscillators (see line 5), with parameters α , β , ω , that control their amplitude, offset, and angular frequency, respectively, which are used to generate an estimated acceleration A_{est} . The A_{est} is an estimate of the gravity removed actual acceleration of the knee as it moves through space (see line 4). In the current implementation of the algorithm, M is the minimum

number of oscillators chosen to give a Fourier representation of the desired signal A_{des} obtained from the IMU. A teaching signal T as shown in line 6, is then generated as a difference between the actual/desired and the Fourier estimated acceleration. This teaching signal is used to alter the frequency of the oscillators in real-time by solving the differential equations using Euler's technique with a constant time step as shown in line 7 after initialization of \dot{Y} to Y_0 . For the AFO, ϵ , v , and f_{min} form the parameters that control the coupling strength, learning factor, and the minimum frequency limit. At any point in time, the phase of the first oscillator (*CHOSEN_OSC*) estimated the gait phase. A minimum frequency limit of 0.4 Hz was chosen to prevent the frequency of the oscillators from falling too low while staying close enough to the frequency of level-ground walking for amputees (line 14). Using the above-mentioned technique, it is possible to automatically monitor and adjust the frequency of the oscillators using feedback from the acceleration signals of the IMU. Since the walking frequency is coupled to the frequency of one of the three oscillators (*CHOSEN_OSC*), it is possible to generate continuously varying reference signals following the changing gait speed. This was done through trials by calculating the frequency of walking beforehand using a stopwatch and using a value smaller than this as an initial estimated minimum frequency for the oscillators, while the coupling strength and learning factors were chosen to smoothen out the high-frequency noise in the vertical accelerations but still able to adapt to the low frequency of the gait cycle. For the current experiments, the number of oscillators was fixed at 3 while setting the coupling strength and learning factor to 6 and 10 respectively resulted in adaptation within 6-8 steps. Finally, the phase of the oscillators was reset whenever a stationary state was detected. During the subsequent restart of walking, the frequency of the oscillators begins adaptation from the minimum frequency limit.

C. SWITCH

The switch between the two mentioned control modes, is done by keeping a count of the number of steps taken by the prosthesis, along with the frequencies at which the references are generated by the interpolation and AFO methods, as shown in Figure 1. In the current experiments, R1 is chosen as 6 steps, R2 as 0, and R3 as 2. In our current implementation we have assumed that indoor distances (living-room/kitchen etc.) can be covered in less than 6 steps, while outdoor distances require a step count greater than 6. Hence there is no requirement of switch for the indoor distances. While for outdoors, we begin with interpolation, find a suitable match and switch over to the continuous method. These assumptions on the choices of the step-counts associated with the R values may be changed based on application as required in future. Thus the chosen 6 step mark is only a pointer to a user performing multiple steps without stopping. Henceforth, for reference, the associated step count is mentioned along with the R identifier for easier understanding. When the number of steps taken by the prosthesis is between R2 (0) and R3 (2),

the prosthesis is considered stationary, and a constant angle value is used as a reference for the joints. When the step count reaches between R3 (2) and R1 (6) the prosthesis is considered to be in a transient walking mode. In this mode, the references are generated using the interpolation technique. Beyond R1 (6), a switch for reference method change is enabled (although the switching does not happen yet, and the references are still generated using interpolation). As further steps are taken, the search for a match in the frequencies and angles of the gait-references continues. The moment a match is detected, and the prosthesis is found to undergo swing extension, the AFO method takes over the function of reference generation. At this point, the subject is considered to be walking steadily. To have a smooth transition from the interpolation method to AFO, the frequencies are continuously monitored while the phase information from the AFO is adapted in the transient walking mode between step count of R3 (2) and R1 (6) by constantly updating the phase of the oscillator using heel strike gait events. These checks ensure that switching happens only when the user is truly in a state of continuous walking [34], [35].

Once the source of reference angle is chosen, the angles are generated using respective angle generator functions. The angle generator functions then provide input to the low-level motor controller for motion generation. In this way, through the use of this hybrid architecture, it is possible to monitor the gait independently of the number of steps taken by the subject by using vertical acceleration information from one IMU only. Tricky situations, such as intermittent walking or walking in confined spaces allowing limited mobility, are handled mostly through the state machine by employing the interpolation method, while stretches of continuous walking with limited variation in walking speeds are handled solely by the adaptive oscillator.

III. MECHATRONIC DESIGN

This Section presents the mechatronic design of the transfemoral prosthetic leg realized for this study to validate the hybrid control architecture. The requirements and specifications of the mechanical design are described, and the choices of the sensors and electronics are explained.

A. REQUIREMENTS

The requirements for the mechanical design of the transfemoral prosthesis have been derived from the biomechanical data of healthy human subjects for level ground walking [36] specifically, from the ranges of motion and the joint power that should be (partially) provided by the artificial limb at the ankle and knee joints respectively.

Figure 4 shows the plots of the knee and ankle joint angles (top) and power (bottom) over a gait cycle at a self-selected speed. From the figure (top), it may be noted that the ankle joint angle ranges from 7° (dorsiflexion) to 20° (plantarflexion), while the knee joint angle ranges from a minimum of 0° (full extension) to a maximum of 65° (full flexion). The figure (bottom) shows that to perform level ground walking

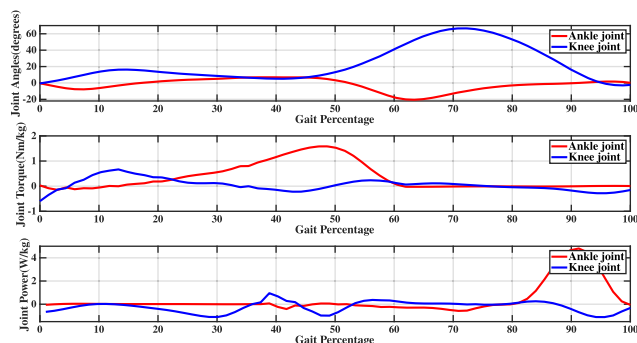



FIGURE 4. The knee and ankle joints angles (top) and the joint torque's scaled on body weight(center) and the joint power(bottom) over a gait cycle during level ground walking of a healthy subject [36].

at a preferred speed, the peak power required at the ankle is of the order of 4.5 W/kg, while it is around 0.8 W/kg at the knee joint. Besides the above-mentioned requirements on the range of motion and the joints' power, a transfemoral prosthesis should be lightweight while its height should be adjusted according to the comfort of the amputee.


B. MECHANICAL DESIGN

The transfemoral prosthesis has been designed with two degrees of freedom, one at each knee and ankle joint [37].

Functionality with simplicity was emphasized, hence the ankle was designed to allow at least 10° of dorsiflexion and 7° of plantarflexion. The ankle joint has a relatively small range of motion, as the idea here is to only provide a part of the push-off effort as assistance while walking [36]. On the other hand, the dorsiflexion angle was maintained at 10° to allow for a smooth rollover. The knee has been designed keeping in mind a range of motion of at least 100° allowing for knee flexion during the sit-to-stand transition. An extra -5° of knee hyperextension was implemented to guarantee the locking of the knee in the stance rollover phase. The hyperextension also helps stabilize the knee during the standing weight-bearing phase. The axis of the knee joint was strategically placed behind the load line of the knee to assist in the stance hyperextension phase of the gait cycle like a conventional passive prosthesis [38]. For the ankle joint, the range of motion of the joint was limited by placing end-stops to the ankle joint coupler. These end-stops restricted the motion of the foot blade and only allowed joint motion between desired angular limits. Figure 5 shows the 3D rendering of the complete lower limb prosthesis and the details of the bevel gear mechanism at the knee and ankle joints. The 3D drawings for all parts were made using SolidWorks (Dassault Systèmes, France, www.solidworks.com) prototyping software. The height of the prosthesis was limited to 420mm corresponding to a subject of height 175cm. The current implementation includes a size 28 ready-made foot blade of the Ossur's Proflex® (Össur hf., Iceland, www.ossur.com), the attachment of which to the ankle joint was done utilizing a custom-made connector to complete the foot design.

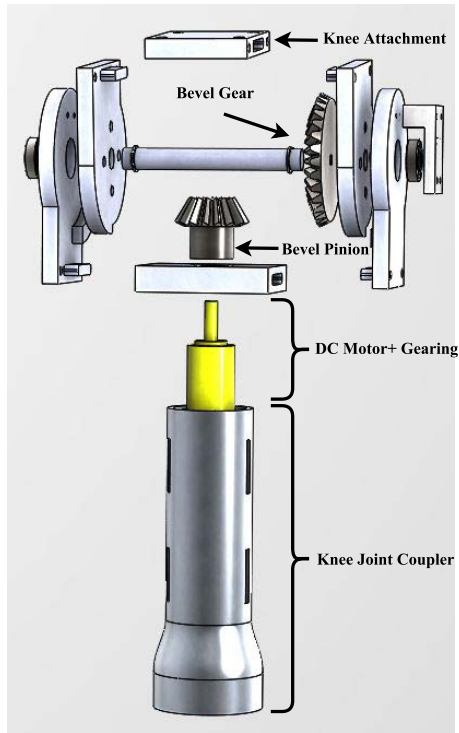

(a) Knee joint section

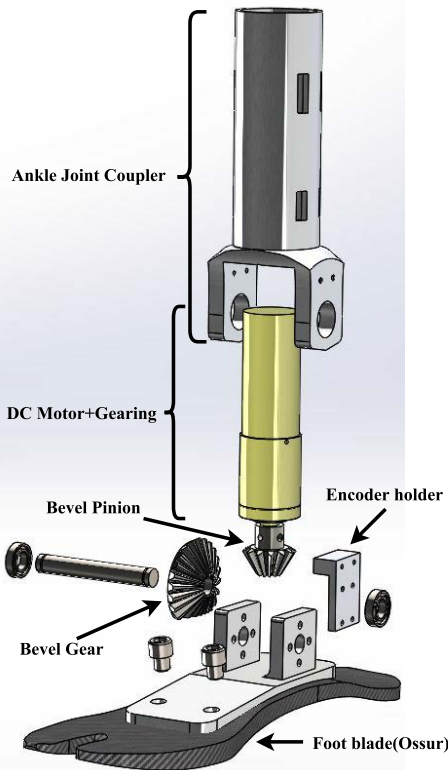

(b) Ankle joint section

FIGURE 5. CAD rendering of the sections of the knee (top) and ankle (bottom) joints, detailing the inner parts of the prosthesis. Both joints contain sets of bevel gears mounted on the respective motor shafts that enable perpendicular power transmission to the joints. The attachment of the prosthesis to a subject can be done using an adapter connected atop the knee attachment.

C. HARDWARE ARCHITECTURE DESIGN

The control system hardware for the transfemoral prosthesis consists of a PIC32 microcontroller running at 200 MHz, which acts as the backbone of the control architecture with all sensors connected to the mainboard using the I2C protocol.

The sensors are one MPU 9250-9 DOFs IMU (SparkFun, USA, www.sparkfun.com) for the knee joint and one for the ankle joint, mounted proximally to the body above the respective joints, and two magnetic encoders AS5600L (AMS AG, Austria, www.ams.com), mounted at custom-designed encoder mounts for contact-less absolute joint-angle sensing. This placement is chosen to get a better estimate of the movement of the upper leg and the lower leg, which in turn can give a better estimate of the tendency of motion of the amputee. This placement also avoids noise that can be introduced when IMUs are placed more distal to the knee joint during ground contact.

The DC motors for the system are directly coupled to the ankle and knee joints and are powered using high-power motor drivers from Pololu (Pololu Corporation, USA, www.pololu.com). The motor for the ankle is a Maxon RE30 60 W (Maxon Motor AG, Switzerland, maxongroup.com), and the knee motor is a Maxon DCX 10 W. Since the operation of the device is intermittent, i.e., positive power pulses are provided mainly during push-off phase, the ankle motor was set for operation at a maximum torque of 0.8 Nm. Coupled with the overall transmission ratio of $2 \times 67 : 1$, from the motor gear head and bevel gear-pinion set, the peak torque that can be supplied is around 107 Nm. A low-power knee motor was selected as its functionality was limited to dampening the leg at the end of the swing phase only. Support to the body weight was provided by the end stops at both joints. The selection of the powering elements was done keeping in mind the objective of minimal strategic power injection at joints to provide an assistive push-off only. The detailed specifications of the motors are reported in Table 2. The movements in both joints are achieved by the use of a bevel gear mechanism which allows the concealment of the ankle and knee actuators within the shank of the prosthesis.

TABLE 2. Specifications for the motors and gears of the ankle/knee joints.

Parameter	Ankle Joint	Knee Joint
Motor Power (W)	60	10
Motor Voltage (V)	24	24
Motor Coil Inductance (mH)	0.119	1.32
Motor Torque(Stall) (mNm)	1020	37.5
Motor Rotor Inertia (gcm^3)	33.5	2.72
Mechanical Time Constant (ms)	3.05	4.89
Gear Ratio	67:1	243:1

Data from the position sensors and IMU are sampled at a frequency of 200 Hz while motor current sensors are sampled at a frequency of 2 kHz. Power to the system is provided by using a 24V Base Tech, BT-305 lab bench power supply.

The IMU on the prosthesis records the accelerations of the upper and lower leg. The IMU includes an onboard signal processor that allows for real-time data filtration using a low-pass filter with a cut-off frequency of 10 Hz. This enables getting the filtered data directly from the IMU, thereby freeing up the microcontroller from data filtration tasks. The filtered data is then directly fed into the microcontroller for gait characterization. The collection of processed data from the transfemoral prosthesis is done using a UART protocol. For this purpose, a circular data buffer of 16-bit unsigned integers was implemented where data was added synchronously at the speed of 200 Hz. The accumulated data is then sent to a PC asynchronously over a standard USB connection. Floating point data was limited by truncating float values to two significant digits by multiplying it by 100 followed by integer typecasting. The structural framework of the manufactured prosthesis along with the mounted electronics is shown in Figure 6.

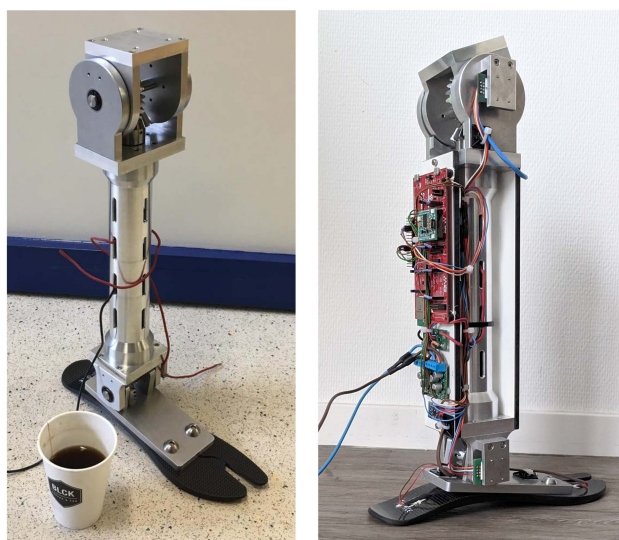


FIGURE 6. The structural framework of the prosthesis (left) along with the mounted electronics (right).

IV. EXPERIMENTS AND RESULTS

A. EXPERIMENTS

The sole motive of the experiments performed using the prosthesis was to ascertain the working of the hybrid control strategy for the transfemoral system. In this regard, the designed prosthesis serves as the mechanical backbone on which the validations of the reference generation capability of the control strategy were made. The initial experiment consisted of multiple trials ranging from 30 seconds to 1 minute where a healthy subject walked on level ground with an IMU placed close to the knee joint.¹ This was done to get estimates of peaks and thresholds of accelerations recorded by the IMU

¹The study, under protocol number M22.296628, was evaluated and received a waiver by the Medical Ethics Review Committee of the University Medical Center Groningen (Groningen, The Netherlands) on May 2, 2022.



FIGURE 7. The experimental testing process for the control system of the current implementation of the prosthesis. An able-bodied adapter on a healthy subject was used for the test pilot.

during level-ground walking for the algorithms. An average of the peaks and thresholds were taken and programmed for the trials with the prosthesis. Experiments with the prosthesis were done on a treadmill to simulate level ground walking a healthy subject wearing an able-bodied adapter during a pilot test. In our experience, the initially programmed thresholds were found to not accurately capture the heel strike using the prosthesis. Hence a separate experiment was performed with the prosthesis to record and then reprogram the thresholds. The speed of operation for the prosthesis was varied between 1 to 1.5 kmph, to simulate speed variations between slow and medium walking speeds. Data generated from the microcontroller consisting of vertical accelerations of the knee from the IMU, number of steps taken, ankle and knee joint references, gait phase and detected mode of the prosthesis were collected in real-time using a serial console and saved to PC.

B. RESULTS

Figure 8(a) shows the accelerations as recorded by the IMU placed above the knee. While the IMU continues to record the vertical accelerations of the prosthesis in the sagittal plane, the high-level control algorithm counts the number of footsteps by processing the acceleration data. The number of steps taken (blue line) along with the currently detected condition of the prosthesis (stationary, transient walking, or steady-state walking) can be observed in Figure 8(b) in red, green, and yellow patches, respectively. Figures 8(c) and (d) show the

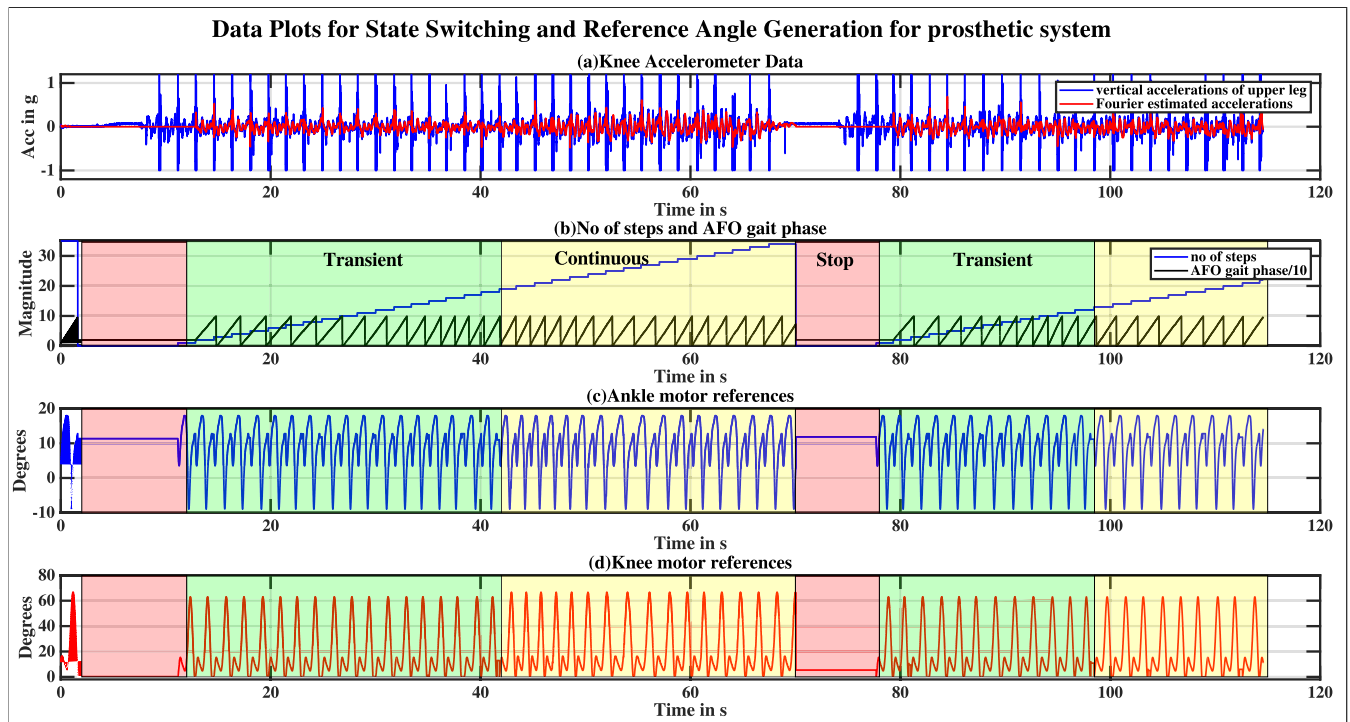


FIGURE 8. State switching capability of the transfemoral prosthesis while undergoing an intermittent/start-stop walking pattern. (a) Knee accelerometer data along with the Fourier estimated accelerations are used to generate the gait phase by the AFO; (b) Step count as calculated using the gait-event detection and step-counter algorithms. The gait phase as detected by the AFO algorithm along with the source of reference is also shown in the plot. When the references are generated using interpolation, the source is 0, while when a switch over to AFO happens the source is 20. (c) and (d) Reference angles generated for the ankle and knee joints, respectively, as a result of the switching of the algorithms. The yellow areas represent a continuous walk and are governed by references from the AFO algorithm, while the green areas represent transient phases of the walk which are governed by the interpolation technique. The red areas represent stationary instances when constant angles at the knee and ankle joints are maintained.

final references to the ankle and knee joints using the selected methods during the experiment.

Figure 9(a) shows the varying accelerations from the IMU for multiple gait cycles with varying speeds, while Figures 9(b) and (c) present the reference angles and oscillator phase varying with walking speed for both joints. The plot areas covered in green represent slow walking, while the areas in red represent normal speed walking. The capability of the algorithm to respond to changing walking speeds is shown in this figure.

V. DISCUSSION

The results reported in Figure 8 show the capability of the control architecture to smoothly transition from one method of reference generation to another during walking. The regions in green show the period in which the transfemoral prosthesis is controlled by the state and gait-event-based interpolation method, while the regions in yellow show the time spans for which the system is controlled by the AFO. With each step detected, the value shown by the blue line in Figure 8b increases accordingly. The first acceleration spike is always used as an indication of motion only, with the step counter remaining unchanged. Beyond this, the step counter begins to increment as shown by the blue line in the subplot. Once a certain number of steps have been detected

(i.e., $R1 = 6$), the mode change flag is set. Following this, the system continues to check for a suitable match in reference generation frequencies. Once a match is found, the switchover takes place during the swing phase of the subsequent gait cycle. The transitioning phenomenon can be observed in the plot around the 40 and 100 s mark. In either of these instances, the references are provided through interpolation for at least 6 steps before switching. The number 6 has been chosen based on the movement by a user within confined spaces, for example indoors where usually only a limited number of steps may be taken. As the step counts increase and a suitable match is found in the gait reference generation frequency, a switchover takes place. Thus, the areas in yellow may be considered analogous to steady walking. The saw tooth profile in figure 8(b) represents the gait phase of walking as estimated from the acceleration data of the knee IMU. The gait phase represented in black has been divided by 10 to bring it to scale with the rest of the plots. The AFO-based gait phase estimation algorithm starts running whenever the prosthesis is detected to be in motion and is reset whenever the prosthesis is stationary. Figures 8(c) and 8(d) show the reference angles for the ankle and knee joints through the phases of intermittent and steady walking. Through the use of the above-mentioned technique of frequency match detection, a smooth transition between the two reference generation

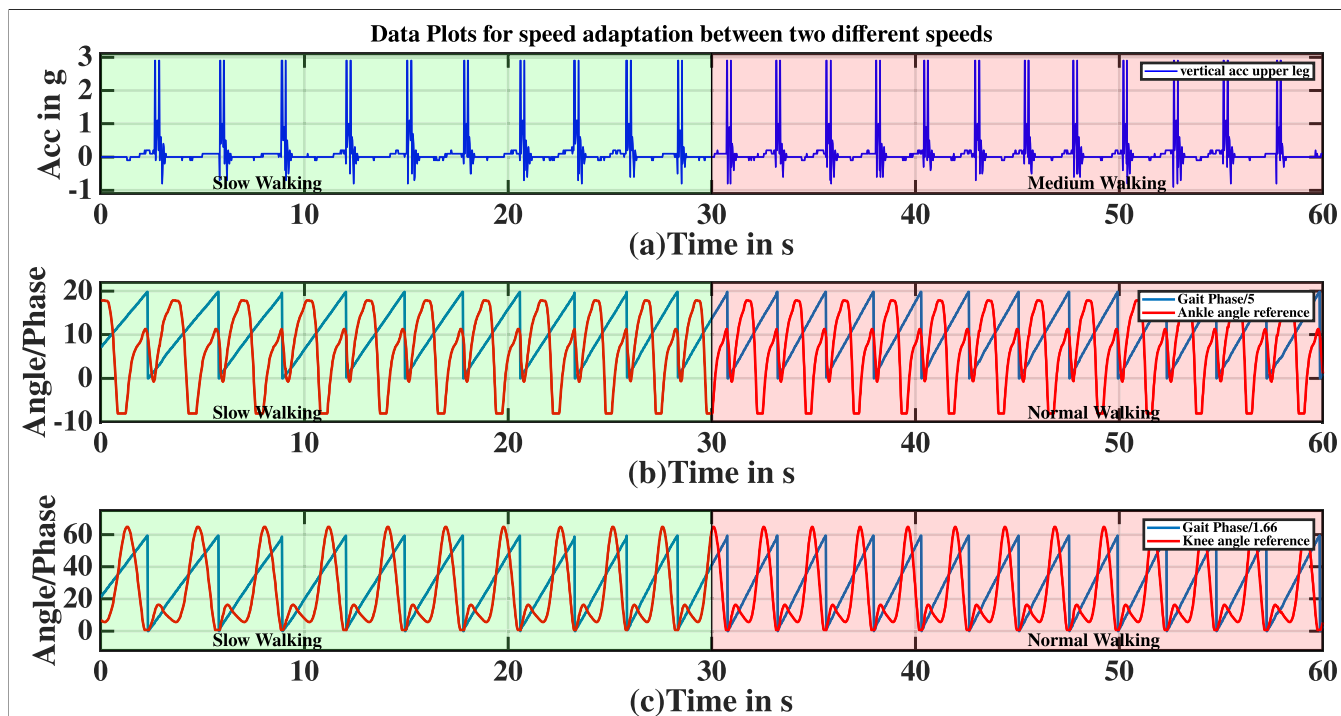


FIGURE 9. The adaptation capability to changing walking speeds. The areas in green are slow speed walking while those in red represent normal walking speeds.

methods is ensured. It must be mentioned that whenever the prosthesis is detected to be in motion, both the reference generation techniques continue to run in the background, while at any point in time, only one is chosen to supply the references to the motor while the other is kept suppressed.

Figure 9 shows the ability of the system to adapt its response to changing gait speeds. The regions shown in green in the figure are areas of slow walking speeds, whereas the region in red are areas where normal speed walking takes place. This is also evident from the acceleration plot in the figure, where the frequency of spikes in accelerations increases in the higher speed region. As the walking speed changes, the joint angle references generated by the algorithms alter their frequencies accordingly. In this way, continuously varying references for joint angles are generated in real-time.

There are several benefits of using this hybrid control algorithm of joint angle referencing. Firstly, the tracking of the angular velocities can be done based on the gait phase information obtained from the AFO alone. Since the gait phase keeps track of the changing gait velocities, there is no requirement of pre-determining the velocities for various speeds of walking. This saves time and effort as prior experiments to determine velocities from the amputee subject may be avoided. A second benefit is that the memory of the micro-controller used in controlling the prosthesis, which is often extremely limited, can be used for alternate processing tasks. Thirdly, since in this approach the prosthesis response can be made independent of the amputee, the same control system can be used for various amputees with minor tuning without

the need for extensive personalization. Finally, having a pre-determined set of velocities for the control instead of allowing for self-selected velocities, causes the user to adapt his/her response to the response of the prosthesis. This might not be totally in line with the desired comfort level of the amputee where ideally it is desired that the prosthesis should adjust its response to the response to that of the amputee. By removing this forced kinematic control, the current approach gives a choice of speed back to the prosthesis user to an extent. For all the above-mentioned reasons, the significance of supplementing control algorithms using oscillator-based gait tracking systems can be observed. Thus, using this hybrid control implementation of the high-level controller, where the prosthesis works at velocities generated through interpolation for a fixed number of steps, and subsequently switches over to an adaptive control scheme, some limitations related to singular state machine-based methods may be circumvented.

A. LIMITATIONS AND FUTURE OUTLOOK

Although the above technique has its benefits, certain limitations can be observed in the current implementation. Since in the current implementation, references generated when the interpolation method is active depend on the information of gait-events and step time from the previous step, the reference velocity to the joints using this method is always dependent on the gait cycle time of the previous step. As a result of this, the reference velocities and angles are always one step behind the actual occurrence in steps. While this may not cause issues when the walking speed is constant, sudden

variation in walking speed need at least one step before matching the phases of walking. This issue may be solved either by using data from pressure sensors to further subdivide the walking pattern. Allowing for further subdivisions such as mid-stance, flat-foot, late-stance shall allow for further points of phase correction. Another way would be to use the IMU to detect more points of one cycle. For instance, changing from upswing of the lower leg to forward swing can be detected. Another area that might need improvement is the knee design. Since a low-power knee actuator has been selected to minimize the weight of the system, the entirety of knee torque required for the stance roll-over phase is not available directly. The second issue may be solved by altering the reference knee joint trajectory to provide a hyper-extended knee between 0 and 50% of the gait cycle which is in accordance with how passive prostheses are aligned in practice. By doing so, the holding torque to support the body weight during stance rollover may be provided using the end stop. Once these improvements are implemented, the test of the performance of the algorithms with the prosthesis in use by an amputee subject needs to be performed to ensure validity and better tuning of parameters. In the process of development of this hybrid control architecture, there was a discussion on whether there should be a switchover again to the transient mode following the continuous mode of walking before coming to a complete halt. For the current iteration of the control system, this was not included mainly due to two reasons. Firstly, it is difficult to estimate, the exact number of steps, that the user would require to reach a complete halt, and secondly, the adaptive oscillator whose frequency may go down to 0.4Hz is still capable of keeping track of the slowing down the process. As the gait frequency falls below this limit, the subject is assumed to have stopped for all practical walking tasks. However, still, a switchover may be designed based on a minimum frequency limit that allows the interpolation technique to take over once the walking frequency falls below this limit. An implementation of this technique and whether a switchover to a transient walk where references are generated through interpolation makes a significant difference in usability or not are topics that shall be addressed through further research in the future.

VI. CONCLUSION

In this paper, we proposed a hybrid control architecture for an active transfemoral prosthesis by combining a state and gait event-based interpolation technique with an adaptive frequency oscillator using information from a single IMU only. The hybrid nature of the controller allows for gait characterization in stationary/transient and steady walking. The experimental results on a transfemoral prosthesis with an able-bodied adapter show that the technique of combining two different methods of reference generation can generate references both for periodic and aperiodic phases of gait cycles. Along with reference generation, through the use of adaptive oscillators, the algorithm was able to continuously adjust its response to changing velocities of walking.

The obtained results show that this technique of combining two methods can be used as a hybrid control method for active transfemoral prostheses.

ACKNOWLEDGMENT

The authors would like to thank Ossur[®] (Össur hf., Iceland, www.ossur.com) for providing the foot blade of the prosthesis and also would like to thank Vera G. M. Kooiman (doctoral candidate) and Ruud Leijendekkers (a Postdoctoral Researcher and a physical therapist) within the Orthopedic Research Laboratory, Radboud University Medical Center, Nijmegen, The Netherlands, for their support during the test pilot.

REFERENCES

- [1] D. Grimes and W. Flowers, "Multi-mode above-knee prosthesis controller," in *Proc. IFAC Symp.*, vol. 15, no. 2, 1982, pp. 43–53.
- [2] S. K. Au, J. Weber, and H. Herr, "Powered ankle-foot prosthesis improves walking metabolic economy," *IEEE Trans. Robot.*, vol. 25, no. 1, pp. 51–66, Feb. 2009.
- [3] J. Geeroms, L. Flynn, R. Jimenez-Fabian, B. Vanderborcht, and D. Lefeber, "Ankle-Knee prosthesis with powered ankle and energy transfer for CYBERLEGS α -prototype," in *Proc. IEEE Int. Conf. Rehabil. Robot.*, Jun. 2013, pp. 1–6.
- [4] E. C. Martinez-Villalpando, L. Mooney, G. Elliott, and H. Herr, "Antagonistic active knee prosthesis. A metabolic cost of walking comparison with a variable-damping prosthetic knee," in *Proc. Annu. Int. Conf. IEEE Eng. Med. Biol. Soc.*, Aug. 2011, pp. 8519–8522.
- [5] L. Ambrozic, M. Gorsic, J. Geeroms, L. Flynn, R. M. Lova, R. Kannik, M. Munih, and N. Vitiello, "CYBERLEGS: A user-oriented robotic transfemoral prosthesis with whole-body awareness control," *IEEE Robot. Autom. Mag.*, vol. 21, no. 4, pp. 82–93, Dec. 2014.
- [6] F. Sup, H. Varol, J. Mitchell, T. Withrow, and M. Goldfarb, "Design and control of an active electrical knee and ankle prosthesis," in *Proc. IEEE RAS/EMBS Int. Conf. Biomed. Robot. Biomechatronics*, Oct. 2008, pp. 523–528.
- [7] F. C. Sup, A. Bohara, and M. Goldfarb, "Design and control of powered transfemoral prosthesis," *Int. J. Robot. Res.*, vol. 27, pp. 263–273, Feb. 2008.
- [8] F. Sup, "A powered self-contained knee and ankle prosthesis for near normal gait in transfemoral amputees," Ph.D. dissertation, Vanderbilt Univ., 2009.
- [9] R. Unal, F. Klijnstra, S. M. Behrens, E. E. G. Hekman, S. Stramigioli, H. F. J. M. Koopman, and R. Carloni, "The control of recycling energy storage capacity for WalkMECHadapt," in *Proc. 23rd IEEE Int. Symp. Robot Hum. Interact. Commun.*, Aug. 2014, pp. 720–725.
- [10] R. D. Gregg, T. Lenzi, L. J. Hargrove, and J. W. Sensinger, "Virtual constraint control of a powered prosthetic leg: From simulation to experiments with transfemoral amputees," *IEEE Trans. Robot.*, vol. 30, no. 6, pp. 1455–1471, Dec. 2014.
- [11] B. E. Lawson, B. Ruhe, A. Shultz, and M. Goldfarb, "A powered prosthetic intervention for bilateral transfemoral amputees," *IEEE Trans. Biomed. Eng.*, vol. 62, no. 4, pp. 1042–1050, Apr. 2015.
- [12] L. J. Hargrove, A. J. Young, A. M. Simon, N. P. Fey, R. D. Lipschutz, S. B. Finucane, E. G. Halsne, K. A. Ingraham, and T. A. Kuiken, "Intuitive control of a powered prosthetic leg during ambulation: A randomized clinical trial," *J. Amer. Med. Assoc.*, vol. 313, no. 22, pp. 2244–2252, 2015.
- [13] R. R. Torrealba, J. Cappelletto, L. Fermín, G. Fernández-López, and J. C. Grieco, "Cybernetic knee prosthesis: Application of an adaptive central pattern generator," *Kybernetes*, vol. 41, no. 1/2, pp. 192–205, Mar. 2012.
- [14] S. Rezaadeh, D. Quintero, N. Divekar, E. Reznick, L. Gray, and R. D. Gregg, "A phase variable approach for improved rhythmic and non-rhythmic control of a powered knee-ankle prosthesis," *IEEE Access*, vol. 7, pp. 109840–109855, 2019.
- [15] D. Xu, S. Crea, N. Vitiello, and Q. Wang, "Online estimation of continuous gait phase for robotic transtibial prostheses based on adaptive oscillators," in *Proc. IEEE/ASME Int. Conf. Adv. Intell. Mechatronics (AIM)*, Jul. 2020, pp. 1890–1895.

- [16] S. Heins, L. Flynn, H. Laloyaux, J. Geeroms, D. Lefeber, and R. Ronsse, "Compliant control of a transfemoral prosthesis by combining feed-forward and feedback," in *Proc. IEEE RAS EMBS Int. Conf. Biomed. Robot. Biomechatronics*, Nov. 2020, pp. 452–458.
- [17] G. Hunt, S. Hood, and T. Lenzi, "Stand-up, squat, lunge, and walk with a robotic knee and ankle prosthesis under shared neural control," *IEEE Open J. Eng. Med. Biol.*, vol. 2, pp. 267–277, 2021.
- [18] A. H. Shultz, B. E. Lawson, and M. Goldfarb, "Variable cadence walking and ground adaptive standing with a powered ankle prosthesis," *IEEE Trans. Neural Syst. Rehabil. Eng.*, vol. 24, no. 4, pp. 495–505, Apr. 2016.
- [19] T. Lenzi, L. Hargrove, and J. Sensinger, "Speed-adaptation mechanism: Robotic prostheses can actively regulate joint torque," *IEEE Robot. Autom. Mag.*, vol. 21, no. 4, pp. 94–107, Dec. 2014.
- [20] J. Mendez, S. Hood, A. Gunnell, and T. Lenzi, "Powered knee and ankle prosthesis with indirect volitional swing control enables level-ground walking and crossing over obstacles," *Sci. Robot.*, vol. 5, no. 44, Jul. 2020, Art. no. eaba6635.
- [21] H. Huang, F. Zhang, L. J. Hargrove, Z. Dou, D. R. Rogers, and K. B. Englehart, "Continuous locomotion-mode identification for prosthetic legs based on neuromuscular-mechanical fusion," *IEEE Trans. Biomed. Eng.*, vol. 58, no. 10, pp. 2867–2875, Oct. 2011.
- [22] F. Zhang and H. Huang, "Source selection for real-time user intent recognition toward volitional control of artificial legs," *IEEE J. Biomed. Health Informat.*, vol. 17, no. 5, pp. 907–914, Sep. 2013.
- [23] L. J. Hargrove, A. M. Simon, R. D. Lipschutz, S. B. Finucane, and T. A. Kuiken, "Real-time myoelectric control of knee and ankle motions for transfemoral amputees," *J. Amer. Med. Assoc.*, vol. 305, no. 15, pp. 1542–1544, Apr. 2011.
- [24] N. E. Krausz, T. Lenzi, and L. J. Hargrove, "Depth sensing for improved control of lower limb prostheses," *IEEE Trans. Biomed. Eng.*, vol. 62, no. 11, pp. 2576–2587, Nov. 2015.
- [25] M. Liu, D. Wang, and H. H. Huang, "Development of an environment-aware locomotion mode recognition system for powered lower limb prostheses," *IEEE Trans. Neural Syst. Rehabil. Eng.*, vol. 24, no. 4, pp. 434–443, Apr. 2016.
- [26] N. Thatte, N. Srinivasan, and H. Geyer, "Real-time reactive trip avoidance for powered transfemoral prostheses," in *Proceedings of Robotics: Science and Systems*. 2019.
- [27] R. D. Gregg, E. J. Rouse, L. J. Hargrove, and J. W. Sensinger, "Evidence for a time-invariant phase variable in human ankle control," *PLoS ONE*, vol. 9, no. 2, Feb. 2014, Art. no. e89163.
- [28] D. J. Villarreal and R. D. Gregg, "A survey of phase variable candidates of human locomotion," in *Proc. Int. Conf. IEEE Eng. Med. Biol. Soc.*, Aug. 2014, pp. 4017–4021.
- [29] L. Righetti, J. Buchli, and A. J. Ijspeert, "Dynamic Hebbian learning in adaptive frequency oscillators," *Phys. D, Nonlinear Phenomena*, vol. 216, no. 2, pp. 269–281, 2006.
- [30] L. Righetti, "Control of legged locomotion using dynamical systems: Design methods and adaptive frequency oscillators," Ph.D. dissertation, École Polytechnique Fédérale de Lausanne, Lausanne, Switzerland, 2008.
- [31] V. Vashista, M. Khan, and S. K. Agrawal, "A novel approach to apply gait synchronized external forces on the pelvis using A-TPAD to reduce walking effort," *IEEE Robot. Autom. Lett.*, vol. 1, no. 2, pp. 1118–1124, Jul. 2016.
- [32] D. Zanutto, P. Stegall, and S. K. Agrawal, "Adaptive assist-as-needed controller to improve gait symmetry in robot-assisted gait training," in *Proc. IEEE Int. Conf. Robot. Autom. (ICRA)*, May 2014, pp. 724–729.
- [33] R. Ronsse, N. Vitiello, T. Lenzi, J. Van Den Kieboom, M. C. Carrozza, and J. A. Ijspeert, "Adaptive oscillators with human-in-the-loop: Proof of concept for assistance and rehabilitation," in *Proc. 3rd IEEE RAS EMBS Int. Conf. Biomed. Robot. Biomechatronics*, Sep. 2010, pp. 668–674.
- [34] B. Stansfield, K. Hawkins, S. Adams, and D. Church, "Spatiotemporal and kinematic characteristics of gait initiation across a wide speed range," *Gait Posture*, vol. 61, pp. 331–338, Mar. 2018.
- [35] S. C. Miff, D. S. Childress, S. A. Gard, M. R. Meier, and A. H. Hansen, "Temporal symmetries during gait initiation and termination in nondisabled ambulators and in people with unilateral transtibial limb loss," *J. Rehabil. Res. Develop.*, vol. 42, no. 2, pp. 175–182, 2005.
- [36] D. A. Winter, *Biomechanics and Motor Control of Human Movement*. Hoboken, NJ, USA: Wiley, 1990.
- [37] A. Mazumder and R. Carloni, "Mechatronic design adaptive control of a lower limb prosthesis," in *Proc. 8th IEEE RAS/EMBS Int. Conf. Biomed. Robot. Biomechatronics (BioRob)*, Nov. 2020, pp. 446–451.
- [38] R. Unal, R. Carloni, S. M. Behrens, E. E. G. Hekman, S. Stramigioli, and H. F. J. M. Koopman, "Towards a fully passive transfemoral prosthesis for normal walking," in *Proc. 4th IEEE RAS EMBS Int. Conf. Biomed. Robot. Biomechatronics (BioRob)*, Jun. 2012, pp. 1949–1954.



ANIKET MAZUMDER received the B.Tech. degree in mechanical engineering from the West Bengal University of Technology (WBUT) and the M.Tech. degree in mechanical engineering from the Indian Institute of Technology (IIT), Gandhinagar, India, in 2017. He is currently pursuing the Ph.D. degree with the Faculty of Science and Engineering, Bernoulli Institute of Mathematics, Computer Science and Artificial Intelligence, University of Groningen. His research interests

include the characterization of human gait and the design and control of prosthetic systems.



EDSKO E. G. HEKMAN (Member, IEEE) received the B.Sc. degree in liberal arts and engineering from the Calvin College, Grand Rapids, MI, USA, and the Master of Science degree (Ingenieur) from the Delft University of Technology, in 1986. After completing the Atheneum Edsko went to Calvin College. From there, he went to the Delft University of Technology. After some years of developing instrumentation for research with the Radboud University of Nijmegen, he accepted

a position as an Assistant Professor with the Department of Biomechanical Engineering, University of Twente. His research interests include the development of assistive devices (orthotics, prosthetics, and exoskeletons) and endoprosthesis for the spine.



RAFFAELLA CARLONI (Member, IEEE) received the M.Sc. degree in electronic engineering from the University of Bologna, Italy, and the Ph.D. degree from the Department of Electronics, Computer Science and Systems, University of Bologna. She was an Assistant Professor and an Associate Professor with the University of Twente, Enschede, The Netherlands, from 2008 to 2017. She joined the University of Groningen, The Netherlands, in 2017. She is currently an Associate

Professor with the Bernoulli Institute for Mathematics, Computer Science, and Artificial Intelligence, Faculty of Science and Engineering, University of Groningen. Her research interests include the design, modeling, control of compliant robotic systems, novel (soft) actuators, and prosthetic devices.

...