



Design of a stepwise safety protocol for lower limb prosthetic risk management in a clinical investigation

Downloaded from: <https://research.chalmers.se>, 2022-07-02 09:29 UTC

Citation for the original published paper (version of record):

Thesleff, A., Ahkami, B., Anderson, J. et al (2021). Design of a stepwise safety protocol for lower limb prosthetic risk management in a clinical investigation. 2021 43rd Annual International Conference of the IEEE Engineering in Medicine & Biology Society (EMBC): 4600-4604. <http://dx.doi.org/10.1109/EMBC46164.2021.9629989>

N.B. When citing this work, cite the original published paper.

Design of a stepwise safety protocol for lower limb prosthetic risk management in a clinical investigation

Alexander Thesleff, *Graduate Student Member, IEEE*, Bahareh Ahkami, *Student Member, IEEE*, Jenna Anderson, Kerstin Hagberg and Max Ortiz-Catalan, *Senior Member, IEEE*

Abstract—In research on lower limb prostheses, safety during testing and training is paramount. Lower limb prosthesis users risk unintentional loss of balance that can result in injury, fear of falling, and overall decreased confidence in their prosthetic leg. Here, we present a protocol for managing the risks during evaluation of active prosthetic legs with modifiable control systems. We propose graded safety levels, each of which must be achieved before advancing to the next one, from laboratory bench testing to independent ambulation in real-world environments.

I. INTRODUCTION

Most lower limb prostheses are either entirely passive mechanical devices or microprocessor-controlled devices which are energetically passive, meaning that they do not provide net positive power to the user. This lack of compensation for the lost musculature in the missing limb limits the ambulatory ability and leads to compensatory movements with increased reliance on the biological limb [1]–[3]. Only few energetically active prosthetic devices are commercially available, of which the Össur PowerKnee and the Ottobock Empower are two examples. However, extensive research efforts are directed to this field and a range of active devices have previously been, or currently are, being developed and tested in research settings [4]–[10].

Adding active joints to the prosthesis increases the number of achievable ambulatory modes and the complexity of the prosthesis control scheme. Embedded or added sensors on the prosthesis, the contralateral limb, or electromyography (EMG) sensors placed on/in the residual limb may be used to infer ambulation mode, gait phase, and ambulation mode transitions to allow smooth locomotion for the user [11]–[17]. By combining these sources of information, the ambition is to enable increased prosthesis function with increased safety for the users. However, as the complexity of sensor integration

and control schemes increase, so does the work required to test and verify function. Much of this work requires physical testing during actual prosthesis usage, and adequate safety precautions must be in place to avoid hazardous situations.

In contrast to individuals using upper limb prostheses, lower limb prosthesis users risk unintentional loss of balance due to intrinsic and extrinsic factors related to tripping, slipping or collision, all of which can lead to injury such as fractures [18]. Fear of falling and decreased confidence in the prosthetic leg can lead to a reduction of prosthesis use and to social withdrawal [19], [20]. Some lower limb prosthesis users report a need to concentrate while walking that has been associated with a fear of falling [19]. To minimize the risks, safety precautions should rely on well-designed rehabilitation and evaluation protocols in combination with the combined experience of healthcare and research professionals. To this end we are proposing a stepwise safety protocol for managing the risk when active prosthetic legs, with modifiable control systems, are used by individuals with a lower limb amputation. This protocol was designed owing to the need of our group to evaluate neuromusculoskeletal prostheses for the lower limb, (the neuromusculoskeletal interface is further described in [21], [22]), but it can be applied to any new leg prostheses and control strategies. The protocol is developed with focus on individuals with transfemoral amputation due to their increased risk of falling, but it is also applicable for the transtibial amputation level [19].

II. STRUCTURE OF THE PROTOCOL

As per Good Clinical Practice guidelines a risk management plan (RMP) should be maintained throughout a clinical investigation [23]. This stepwise safety protocol can be seen as a part of the RMP and comprises prosthetic evaluations and mobility from the laboratory bench (without a

* Research supported by the Promobilia Foundation, the IngaBritt and Arne Lundbergs Foundation, the Swedish Innovation Agency (VINNOVA), the Swedish Research Council (Vetenskapsrådet), and the Swedish state under the agreement between the Swedish government and the county councils, the ALF agreement (ALFGBG-76480 and ALFGBG-725641).

A. Thesleff is with the Center for Bionics and Pain Research, Sweden, with the Department of Electrical Engineering, Chalmers University of Technology, Sweden and with Integrum AB, Sweden (e-mail: thesleff@chalmers.se).

B. Ahkami is with the Center for Bionics and Pain Research, Sweden, with the Department of Electrical Engineering, and with Chalmers University of Technology (e-mail: ahkami@chalmers.se).

J. Anderson is with the Center for Bionics and Pain Research, Gothenburg, Sweden, and with the Centre for Advanced Reconstruction of Extremities,

Sahlgrenska University Hospital, Sweden (e-mail: jenna.anderson@vgregion.se).

K. Hagberg is with the Department of Orthopaedics, Sahlgrenska University Hospital, Gothenburg, Sweden, and Department of Orthopaedics, Institute of Clinical Sciences, Sahlgrenska Academy, University of Gothenburg, Sahlgrenska University Hospital, Gothenburg, Sweden (e-mail: kerstin.hagberg@vgregion.se).

M. Ortiz-Catalan is with the Center for Bionics and Pain Research, Sweden, with the Department of Electrical Engineering, Chalmers University of Technology, Sweden, with the Operational Area 3, Sahlgrenska University Hospital, Sweden, and with the Department of Orthopaedics, Institute of Clinical Sciences, Sahlgrenska Academy, University of Gothenburg, Sweden (e-mail: maxo@chalmers.se).

Physical environments are also defined in the safety protocol. The test bench is where the prosthesis can be mounted and tested, disconnected from the participant. The mounting and placement of the prosthesis should be done in a manner by which the safety of the research staff is ensured, preferably inside a cage or in an otherwise shielded-off environment. Laboratory environments include ambulation on a treadmill or in a small circuit in a clinical laboratory room, with minimal distractions and even surfaces. Outside lab environments are separated into “real-world” and “real-world +” environments where the latter is defined as environments which are challenging to navigate with a lower limb prosthesis, for example due to uneven terrain, slippery surfaces, or crowds. Examples of real-world and real-world + environments are shown in Fig. 3.



Figure 3. Examples of real-world environments (a and b) and real-world + environments (c and d).

Lower limb prosthesis users report the need to concentrate during ambulation [19], [24]. This is incorporated in the safety protocol by including dual-task paradigms such as serial subtraction, in which the participant is asked to count backwards by threes or sevens from a random starting number while performing another task such as standing or walking [25]. Advancing from a less to more challenging environment, for example from the small circuit in the laboratory setting to the larger circuit in the real-world setting, also considers the cognitive workload of the individual as an important safety component.

B. Requirements for transition to lower safety level

In order to transition to a lower safety level, one or more tests must be completed to a specified outcome, as detailed in

Fig. 1. A transition can only be made from one safety level at a time and both the research participant and the responsible professional must agree to make the transition to the lower safety level.

To confirm the reliability of active prosthetic devices with modifiable control systems, outcomes are categorized depending on the use of the prosthesis:

- For no user (bench testing), all joint torque and angles must be within safe limits.
- For ambulation on a treadmill with safety harness, the user must ambulate safely without stumbling or falling for 2 minutes per activity (defined below).
- For ambulation in a circuit, the user must complete the circuit (Fig. 4) without stumbling or falling a specified

number of times (four times for the small circuit and two times for the large circuit), divided per direction, to confirm fluency using the device. For users who want to use a preferred walking aid such as a crutch, cane, or a walking stick, in the real-world environment a slight adaptation of the safety levels is made. These users will not be required to walk without support in the ambulatory circuits, but may use the preferred walking aid for transition to a lower safety level. To verify the ability of safe ambulation without excessive cognitive effort, the last trials in the circuit before transitioning to a lower safety level must be completed while performing a dual task, such as serial subtraction.

- Users who would like to use their device in real-world + environments, must first exhibit safe ambulation in real-world environments (minimum 1 week, with more than 1000 steps/day on average) without any stumbles and/or falls. The user must also have a high confidence in ambulation with the prosthesis, to maximize research participant safety in a variety of physical settings.

Activities for ambulation on a treadmill include gait initiation/termination, level ground walking and ramp/descent at two different speeds. Activities for ambulation in a circuit start from a seated position at the starting point, continues to level walking, ramp ascent/descent, stairs ascent/descent, and transitions between level walking, before finishing the circuit by sitting on a comfortable chair at the end point.

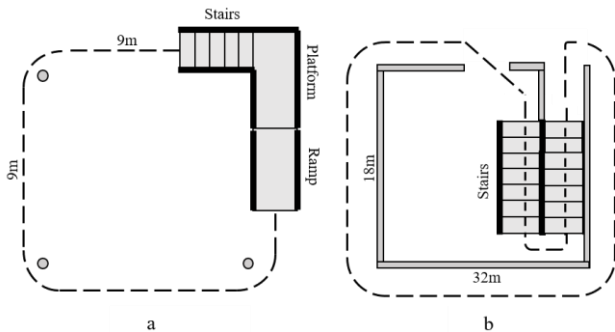


Figure 4. Example of walking circuits. a) Small circuit, b) Large circuit

IV. CONCLUSION

Employing a stepwise safety structure aims to minimize the risk to participants and research staff, thus maximizing the safety during testing and training to use active, prosthetic legs with modifiable control systems in individuals with lower limb amputations. In the proposed protocol the prosthesis must undergo bench testing and weight-bearing ambulation assessment by able-bodied users before research participants with lower limb amputation may begin testing such prosthetic devices. If a user is unable to achieve the specified tasks of a safety level, they will not be allowed to advance to the next safety level, thus minimizing the risk of potential injury. The protocol design requires that the safety level structure is followed to maximize safety for participants.

REFERENCES

- [1] R. E. Seroussi, A. Gitter, J. M. Czerniecki, and K. Weaver, "Mechanical work adaptations of above-knee amputee ambulation," *Arch. Phys. Med. Rehabil.*, 1996.
- [2] V. J. Harandi *et al.*, "Gait compensatory mechanisms in unilateral transfemoral amputees," *Med. Eng. Phys.*, 2020.
- [3] C. M. Powers, L. A. Boyd, L. Torburn, and J. Perry, "Stair ambulation in persons with transtibial amputation: An analysis of the Seattle LightFoot(TM)," *J. Rehabil. Res. Dev.*, 1997.
- [4] A. F. Azocar, L. M. Mooney, J. F. Duval, A. M. Simon, L. J. Hargrove, and E. J. Rouse, "Design and clinical implementation of an open-source bionic leg," *Nat. Biomed. Eng.*, 2020.
- [5] L. Flynn, J. Geeroms, R. Jimenez-Fabian, B. Vanderborght, N. Vitiello, and D. Lefeber, "Ankle-knee prosthesis with active ankle and energy transfer: Development of the CYBERLEGs Alpha-Prosthesis," in *Robotics and Autonomous Systems*, 2015.
- [6] L. Flynn *et al.*, "The Challenges and Achievements of Experimental Implementation of an Active Transfemoral Prosthesis Based on Biological Quasi-Stiffness: The CYBERLEGs Beta-Prosthesis," *Front. Neurobot.*, 2018.
- [7] F. Sup, H. A. Varol, J. Mitchell, T. J. Withrow, and M. Goldfarb, "Self-contained powered knee and ankle prosthesis: Initial evaluation on a transfemoral amputee," in *2009 IEEE International Conference on Rehabilitation Robotics, ICORR 2009*, 2009.
- [8] A. H. Shultz, J. E. Mitchell, D. Truex, B. E. Lawson, and M. Goldfarb, "Preliminary evaluation of a walking controller for a powered ankle prosthesis," in *Proceedings - IEEE International Conference on Robotics and Automation*, 2013.
- [9] T. Lenzi, M. Cempini, L. Hargrove, and T. Kuiken, "Hybrid actuation systems for lightweight transfemoral prostheses," in *Frontiers in Biomedical Devices, BIOMED - 2017 Design of Medical Devices Conference, DMD 2017*, 2017.
- [10] E. C. Martinez-Villalpando and H. Herr, "Agonist-antagonist active knee prosthesis: A preliminary study in level-ground walking," *J. Rehabil. Res. Dev.*, 2009.
- [11] L. J. Hargrove *et al.*, "Robotic Leg Control with EMG Decoding in an Amputee with Nerve Transfers," *N. Engl. J. Med.*, 2013.
- [12] L. J. Hargrove *et al.*, "Intuitive control of a powered prosthetic leg during ambulation: A randomized clinical trial," *JAMA - J. Am. Med. Assoc.*, vol. 313, no. 22, pp. 2244–2252, 2015.
- [13] H. Huang, F. Zhang, L. J. Hargrove, Z. Dou, D. R. Rogers, and K. B. Englehart, "Continuous locomotion-mode identification for prosthetic legs based on neuromuscular - Mechanical fusion," *IEEE Trans. Biomed. Eng.*, 2011.
- [14] H. Huang, T. A. Kuiken, and R. D. Lipschutz, "A strategy for identifying locomotion modes using surface electromyography," *IEEE Trans. Biomed. Eng.*, 2009.
- [15] R. Borjjan, M. B. Khamesee, and W. Melek, "Feasibility study on echo control of a prosthetic knee: Sensors and wireless communication," in *Microsystem Technologies*, 2010.
- [16] M. G. Bernal-Torres, H. I. Medellin-Castillo, and J. C. Arellano-González, "Design and Control of a New Biomimetic Transfemoral Knee Prosthesis Using an Echo-Control Scheme," *J. Healthc. Eng.*, 2018.
- [17] J. A. Spanias, A. M. Simon, S. B. Finucane, E. J. Perreault, and L. J. Hargrove, "Online adaptive neural control of a robotic lower limb prosthesis," *J. Neural Eng.*, 2018.
- [18] J. Kim, M. J. Major, B. Hafner, and A. Sawers, "Frequency and Circumstances of Falls Reported by Ambulatory Unilateral Lower Limb Prosthesis Users: A Secondary Analysis," *PM R*, vol. 11, no. 4, pp. 344–353, Apr. 2019.
- [19] W. C. Miller, M. Speechley, and B. Deathe, "The prevalence and risk factors of falling and fear of falling among lower extremity amputees," *Arch. Phys. Med. Rehabil.*, vol. 82, no. 8, pp. 1031–1037, Aug. 2001.
- [20] W. C. Miller and A. B. Deathe, "The influence of balance confidence on social activity after discharge from prosthetic rehabilitation for first lower limb amputation," *Prosthet. Orthot. Int.*, vol. 35, no. 4, pp. 379–385, Dec. 2011.
- [21] M. Ortiz-Catalan, B. Hakansson, and R. Branemark, "An osseointegrated human-machine gateway for long-term sensory feedback and motor control of artificial limbs," *Sci. Transl. Med.*, 2014.
- [22] M. Ortiz-Catalan, E. Mastinu, P. Sassu, O. Aszmann, and R. Brånemark, "Self-Contained Neuromusculoskeletal Arm

Prostheses,” *N. Engl. J. Med.*, vol. 382, no. 18, pp. 1732–1738, 2020.

- [23] “ISO 14155:2020(en), Clinical investigation of medical devices for human subjects — Good clinical practice.” .
- [24] C. Gauthier-Gagnon, M. C. Grisé, and D. Potvin, “Enabling factors related to prosthetic use by people with transtibial and transfemoral amputation,” *Arch. Phys. Med. Rehabil.*, 1999.
- [25] T. Bristow, C.-S. Jih, A. Slabich, and J. Gunn, “Standardization and adult norms for the sequential subtracting tasks of serial 3’s and 7’s,” *Appl. Neuropsychol. Adult*, vol. 23, no. 5, pp. 372–378, Sep. 2016.