

Application of Dielectric Resonator Antenna in Implantable Medical Devices

*Original*

Application of Dielectric Resonator Antenna in Implantable Medical Devices / Singhwal, Sumer Singh; Matekovits, Ladislau; Peter, Ildiko; Kanaujia, Binod Kumar. - ELETTRONICO. - (2021), pp. 80-81. ((Intervento presentato al convegno 2021 IEEE International Symposium on Antennas and Propagation and USNC-URSI Radio Science Meeting (APS/URSI) tenutosi a Singapore, Singapore nel 4-10 Dec. 2021 [10.1109/APS/URSI47566.2021.9704756]).

*Availability:*

This version is available at: 11583/2957157 since: 2022-03-04T10:38:17Z

*Publisher:*

IEEE

*Published*

DOI:10.1109/APS/URSI47566.2021.9704756

*Terms of use:*

openAccess

This article is made available under terms and conditions as specified in the corresponding bibliographic description in the repository

*Publisher copyright*

IEEE postprint/Author's Accepted Manuscript

©2021 IEEE. Personal use of this material is permitted. Permission from IEEE must be obtained for all other uses, in any current or future media, including reprinting/republishing this material for advertising or promotional purposes, creating new collecting works, for resale or lists, or reuse of any copyrighted component of this work in other works.

(Article begins on next page)

# Application of Dielectric Resonator Antenna in Implantable Medical Devices

Sumer Singh Singhwala *Member, IEEE*<sup>1</sup>, Ladislau Matekovits, *Senior Member, IEEE*<sup>2\*</sup>, Ildiko Peter<sup>3</sup> and Binod Kumar Kanaujia, *Senior Member, IEEE*<sup>4</sup>

<sup>1,2</sup>Department of Electronics and Telecommunications, Politecnico di Torino, 10129 Torino, Italy

<sup>2</sup>Istituto di Elettronica e di Ingegneria dell' Informazione e delle Telecomunicazioni, National Research Council of Italy, 10129 Turin, Italy

<sup>2</sup>Department of Measurements and Optical Electronics, Politehnica University Timisoara, 300223 Timisoara, Romania

<sup>2,3</sup>Faculty of Engineering and Information Technology, University of Medicine, Pharmacy, Science and Technology, 540088, Mures, Romania

<sup>4</sup>School of Computational and Integrative Science, Jawaharlal Nehru University, Delhi 110067, India

**Abstract**—Wireless biomedical telemetry through Implantable Medical Devices (IMD) has been one of the major interest of human kind in present times due to life supporting advantages. As sensors, actuators, battery and antenna comprises the IMD and role of efficient radiator describes the quality of implantable device. However, Dielectric Resonator Antennas (DRA) have been proved more efficient in comparison to their contemporaries in different applications due to its inherent properties, but application of DRA in implantable devices is not proposed yet. In this paper, a rectangular DRA resonating at 2.45 GHz excited by coplanar waveguide feed has been proposed for in depth implantable applications.

**Index Terms**—Dielectric resonator antenna (DRA), implant antennas, SAR, IMD.

## I. INTRODUCTION

An exponential growth has been experienced by wireless technologies in the past few decades due to rapid development in the field of antennas. Transition from wired to wireless communications has been distinguished in outer space communication but it is in growing phase when looked into in-body communication for biomedical applications. There are two operating bands reserved for biomedical applications which are Medical Implant Communication Service (MICS) band (402-405 MHz) to Industrial, Scientific and Medical (ISM) band (902-928 MHz, 2400-2483.5 MHz and 5.725 - 5.875 GHz). If looked electrically, human body is combination of dielectric materials with varied minor conductivity like skin, muscle, fat are equivalently represented as dielectric material with conductivity, in [1].

In [2], [3] authors reviewed significant microstrip patch antennas proposed in recent times for ingestible and implantable body antennas. Microstrip patch antennas have been preferred choice by researchers due to its various advantages like low profile and possible miniaturization.

But human body is very lossy in nature and metallic patch antenna experience low gain and high loss there. DRAs have advantages like high gain and design flexibility which may be a better choice in dielectric environment of human body. An Ultra Wide Band (UWB) frequency band 3.1-10.6 GHz hemispherical Dielectric Resonator Antenna (DRA) for medical capsule endoscope applications has been proposed in [4].

In this paper, a novel concept of using DRA in implantable application such as in human arm, has been proposed. To the author's knowledge, no other muscle implantable DRA work has been reported in the literature yet.

## II. ANTENNA DESIGN

Designing an implantable antennas requires biocompatibility and body radiation condition to be met with existing standards. Taking biocompatibility into considerations, DRA is made up of  $TiO_2$  with  $\epsilon_r=80$  which is a biocompatible ceramic. This DRA with dimensions 23.5mm×23.5mm×5 mm has been placed on biocompatible substrate made up of PVC plastic  $\epsilon_r=2.7$  with dimensions 40mm × 40mm × 0.5mm. Initial dimensions of DRA has been calculated using Marcatili's approximation method [5], [6] at 2.45 GHz for  $TE_{11\delta}$  mode, which were further optimized by EM simulator. Overall thickness of antenna is 5.5 mm which is considerable for implantable antenna applications. The microstrip feedline dimension are 25.3 mm×2.2mm with 0.5mm gap between ground and feedline. To avoid ground plane at the bottom side of substrate which can lead to losses and high power requirement to achieve desired results inside body environment, a CPW (Coplanar Waveguide) feed is used to excite RDRA. Geometry of antenna is shown in Fig. 1.

## III. RESULT ANALYSIS

A simulation analysis has been performed on 3D Canonical right arm tissue model in HFSS EM simulator. Upper

\*Corresponding author email: ladislau.matekovits@polito.it

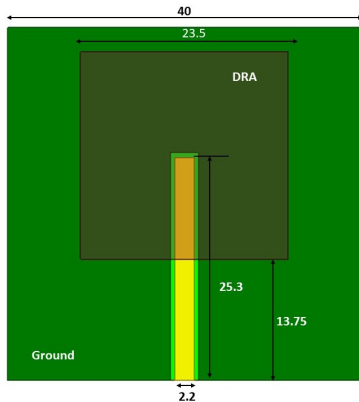


Fig. 1: Geometry of the Antenna

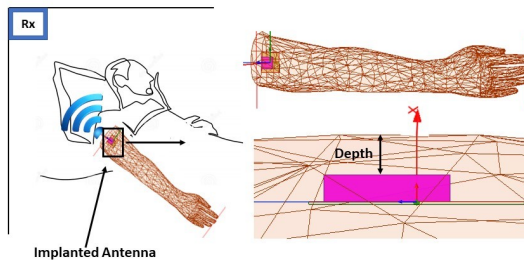


Fig. 2: 3D Canonical right arm tissue model in HFSS

human arm was chosen because it has thick muscle and fat which resembles chest and thighs. Simulation time per iteration heavily depends upon configuration of computer so a 16 GB RAM computer with 3.2 GHz processor was used in the analysis.

$S_{11}$  parameters and simulated gain at 2.45 GHz,  $\phi = 0$  are shown in Fig. 3 and Fig. 4 for two implant antenna depths i.e. 4.5 mm and 4.7 mm. Simulated gain for these two implant depths is shown in Fig. 4. Maximum gain of  $-29.5$  dB is achieved in the broadside direction (here at  $\theta = 90^\circ$  and  $\phi = 0$ ) due to change in inclination of human arm model in HFSS. Inside body radiation is majorly characterize by surface absorption rate (SAR). The IEEE C95.1-1999 standard restricts the SAR averaged over any 1 g of tissue to be less than 1.6 W/kg [7], and the IEEE C95.1-2005 SAR averaged over any 10 g of the tissue be less than 2 W/kg [8]. Maximum value of SAR field are 388.38 W/kg and 53.97 W/Kg for 1-g avg and 10-g avg cases. Maximum allowed net input power of proposed DRA for both the standards are 2.25 mW and 37 mW which are more than required when input power is less than 1 mW provided by internal battery. A link budget analysis revealed that this antenna can be useful for upto 5 meters out-body communication with data rate of 1 Mbps when base station antenna is considered as omnidirectional dipole antenna with gain of 2.45 dBi.

#### IV. CONCLUSION

In this paper, a novel concept of application of DRA in implantable devices has been presented. Exploiting advantages of DRA over microstrip patch antenna in the in-body to out-body communication is possible and demonstrated with the help of biocompatible rectangular DRA excited

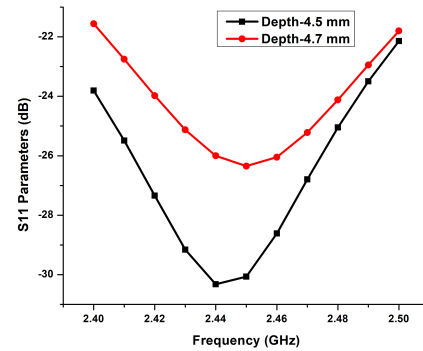


Fig. 3:  $S_{11}$  Parameters of RDRA in 3D Canonical right arm tissue model in HFSS

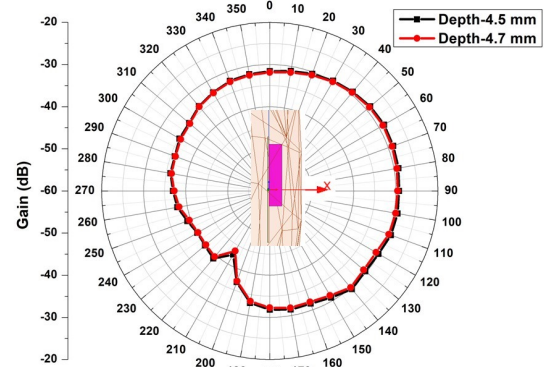


Fig. 4: Simulated gain of RDRA in 3D Canonical right arm tissue model in HFSS at 2.45 GHz and  $\phi = 0$ , here broadside is  $\theta = 90^\circ$  for Human Arm Model

by coplanar waveguide feed. SAR and link budget analysis supports its candidature for high data rate biomedical telemetry applications.

#### REFERENCES

- [1] S. Gabriel, R. W. Lau, and C. Gabriel, "The dielectric properties of biological tissues: II. Measurements in the frequency range 10 Hz to 20 GHz," *Phys. Med. Biol.*, vol. 41, no. 11, p. 2251, 1996. [Online].
- [2] A. Kiourti and K. S. Nikita, "A Review of Implantable Patch Antennas for Biomedical Telemetry: Challenges and Solutions [Wireless Corner]," in *IEEE Antennas and Propagation Magazine*, vol. 54, no. 3, pp. 210-228, June 2012.
- [3] A. Kiourti and K. S. Nikita, "A Review of In-Body Biotelemetry Devices: Implantables, Ingestibles, and Injectables," in *IEEE Transactions on Biomedical Engineering*, vol. 64, no. 7, pp. 1422-1430, July 2017.
- [4] Q. Wang, K. Wolf and D. Plettemeier, "An UWB capsule endoscope antenna design for biomedical communications," 2010 3rd International Symposium on Applied Sciences in Biomedical and Communication Technologies (ISABEL 2010), pp. 1-6, 2010.
- [5] E. A. J. Marcatili, "Dielectric rectangular waveguide and directional coupler for integrated optics," *Bell Syst. Tech. J.*, vol. 48, pp. 2071-2102, 1969.
- [6] R. K. Mongia and P. Bhartia, "Dielectric resonator antennas - A review and general design relations for resonant frequency and bandwidth," *Int. J. RF Microw. Millim. Comput.-Aided Eng.*, vol. 4, no. 3, pp. 230-247, 1994.
- [7] IEEE Standard for Safety Levels With Respect to Human Exposure to Radio Frequency Electromagnetic Fields, 3 KHz to 300 GHz, IEEE Standard C95.1-1991, 1999.
- [8] IEEE Standard for Safety Levels With Respect to Human Exposure to Radio Frequency Electromagnetic Fields, 3 KHz to 300 GHz, IEEE Standard C95.1-2005, 2005.