

Analytical and Bioanalytical Chemistry

Electronic Supplementary Material

Zinc oxide nanoparticles based microfluidic immunosensor applied in congenital hypothyroidism screening

Marco A. Seia, Sirley V. Pereira, Martin A. Fernández-Baldo, Irma E. De Vito, Julio Raba, Germán A. Messina

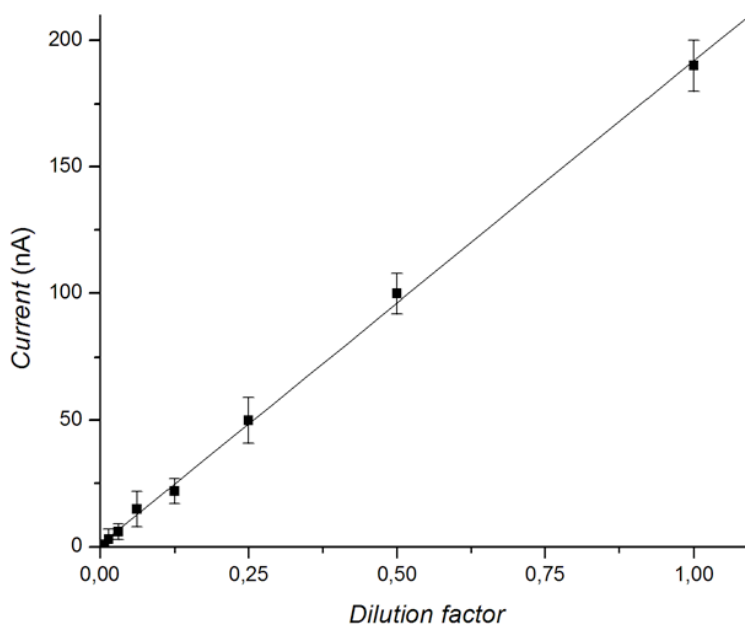


Fig. S1. Dilution test results for $5 \mu\text{U mL}^{-1}$ TSH serum control. Each value of current (nA) is based on five determinations