



Dynamic study of blood-brain barrier closure after its disruption using ultrasound: a quantitative analysis.

Benjamin Marty, Benoit Larrat, Maxime Van Landeghem, Caroline Robic, Philippe Robert, Marc Port, Denis Le Bihan, Mathieu Pernot, Mickael Tanter, Franck Lethimonnier, et al.

► **To cite this version:**

Benjamin Marty, Benoit Larrat, Maxime Van Landeghem, Caroline Robic, Philippe Robert, et al.. Dynamic study of blood-brain barrier closure after its disruption using ultrasound: a quantitative analysis.. Journal of Cerebral Blood Flow and Metabolism, Nature Publishing Group, 2012, 32 (10), pp.1948-58. <10.1038/jcbfm.2012.100>. <cea-00739117>

HAL Id: cea-00739117

<https://hal-cea.archives-ouvertes.fr/cea-00739117>

Submitted on 5 Oct 2012

HAL is a multi-disciplinary open access archive for the deposit and dissemination of scientific research documents, whether they are published or not. The documents may come from teaching and research institutions in France or abroad, or from public or private research centers.

L'archive ouverte pluridisciplinaire **HAL**, est destinée au dépôt et à la diffusion de documents scientifiques de niveau recherche, publiés ou non, émanant des établissements d'enseignement et de recherche français ou étrangers, des laboratoires publics ou privés.

Dynamic study of blood brain barrier closure after its disruption using ultrasound: a quantitative analysis.

Journal:	<i>Journal of Cerebral Blood Flow and Metabolism</i>
Manuscript ID:	Draft
Manuscript Type:	Original Articles
Date Submitted by the Author:	n/a
Complete List of Authors:	Marty, Benjamin; CEA/DSV/I2BM/NeuroSpin, LRMN Larrat, Benoit; CEA/DSV/I2BM/NeuroSpin, LRMN Van Landeghem, Maxime; PPMD, ESPCI ParisTech, CNRS UMR 7615 Robic, Caroline; Guerbet, Research Department Robert, Philippe; Guerbet, Research Department Port, Marc; Guerbet, Research Department Le Bihan, Denis; CEA/DSV/I2BM/NeuroSpin, LRMN Pernot, Mathieu; Institut Langevin, ESPCI ParisTech, CNRS UMR 7587, INSERM U979 Tanter, Mickael; Institut Langevin, ESPCI ParisTech, CNRS UMR 7587, INSERM U979 Lethimonnier, Franck; CEA/DSV/I2BM/NeuroSpin, LRMN Mériaux, Sébastien; CEA/DSV/I2BM/NeuroSpin, LRMN
Keywords:	MRI, Molecular imaging, Pharmacology, Ultrasound, Blood brain barrier

1
2
3 **Dynamic study of blood brain barrier closure after its disruption using**
4
5 **ultrasound: a quantitative analysis.**
6
7

8
9
10 Benjamin Marty¹ (MSc), Benoit Larrat^{1,2} (PhD), Maxime Van Landeghem³ (PhD), Caroline
11 Robic⁴ (PhD), Philippe Robert⁴ (PhD), Marc Port⁴ (PhD), Denis Le Bihan¹ (MD, PhD),
12 Mathieu Pernot² (PhD), Mickael Tanter² (PhD), Franck Lethimonnier¹ (PhD) and
13 Sébastien Mériaux¹ (PhD)
14

15
16 ¹NeuroSpin, I²BM, Commissariat à l'Énergie Atomique, Gif-sur-Yvette, France

17 ²Institut Langevin, ESPCI ParisTech, CNRS UMR 7587, INSERM U979, Paris, France

18 ³PPMD, ESPCI ParisTech, CNRS UMR 7615, Paris, France

19 ⁴Guerbet Research Division, Roissy-Charles de Gaulle, France
20
21

22
23 **Running title:** Study of BBB closure US-induced disruption
24
25
26

27 **Corresponding author:**
28

29 Sébastien Mériaux, sebastien.meriaux@cea.fr
30

31 CEA Saclay, DSV/I²BM/NeuroSpin, Bâtiment 145 – Point courrier 156
32

33 91191 Gif-Sur-Yvette CEDEX
34

35
36 Phone : +33169089423
37

38 Fax : +33169087980
39
40
41

42
43 **Grant sponsor:**
44

45 Iseult/Inumac French-German project.
46
47
48
49
50
51
52
53
54
55
56
57
58
59
60

Abstract

Delivery of therapeutic or diagnostic agents to the brain is majorly hindered by the blood-brain barrier (BBB). Recently, many studies have demonstrated local and transient disruption of the BBB using low power ultrasound sonication combined with intravascular microbubbles. However, BBB opening and closure mechanisms are properly understood, especially the maximum gap that may be safely generated between endothelial cells and the duration of opening of the BBB. Here we studied BBB opening and closure under MR guidance in a rat model. First, MR contrast agents (CA) of different hydrodynamic diameters (1 – 65 nm) were employed to estimate the largest molecular size permissible across the cerebral tissues. Secondly, to estimate the duration of the BBB opening, the CA were injected at various times post-BBB disruption (12 min – 24 h). A T_1 mapping strategy was developed to assess CA concentration at the US focal point. Based on our experimental data and BBB closure modeling, a calibration curve was obtained to compute the half closure time as a function of CA hydrodynamic diameter. These findings and the model provide an invaluable basis for optimal design and delivery of nanoparticles to the brain.

Key words: *BBB disruption, MR contrast agent, MRI, T_1 mapping, ultrasound, nanoparticles*

Introduction

Cerebral tissues are isolated from circulating blood by the blood brain barrier (BBB) (Rubin and Staddon 1999). This physiological barrier consists of a lining of tightly packed vascular endothelial cells, different from the peripheral blood vessels (Hawkins and Davis 2005). The tight junctions between these cells restrict the diffusion of microscopic objects (e.g. bacteria) and of large, hydrophilic molecules (>400 Da) from blood to brain parenchyma, while allowing the passage of small, hydrophobic molecules such as O₂, CO₂, proteins, and metabolites (Pardridge 2005). Because of the neuroprotective nature of the BBB, delivery of potentially important diagnostic and therapeutic agents is a major challenge in the treatment of most brain disorders. Strategies to design specific drugs targeted to the brain involve finding an efficient mode of drug delivery across the BBB.

Recently, it has been demonstrated that the use of low power focused ultrasound combined with a systemic injection of lipid- (or polymer-) shelled microbubbles enables a non-invasive, local and transient disruption of the BBB (Hynynen *et al* 2001). Many studies were then carried out to (i) establish optimal ultrasound parameters that permit adequate tissular penetration without causing tissue damage (Choi *et al* 2006; Hynynen *et al* 2005; O'Reilly *et al* 2010; O'Reilly *et al* 2011a; O'Reilly *et al* 2011b; Sheikov *et al* 2008), (ii) quantify permeability of the disrupted brain tissue (Vlachos *et al* 2010; Vlachos *et al* 2011), and (iii) evaluate responses to treatments of particular brain disorders including tumors (Chen *et al* 2010; Liu *et al* 2010; Treat *et al* 2009) and Alzheimer's disease (Jordao *et al* 2010; Raymond *et al* 2008). Most of these studies used magnetic resonance contrast agents (MR-CA) for monitoring the processes.

Despite a rapidly growing number of studies, the mechanism of ultrasound-induced BBB opening is understood only poorly. In particular, the maximum space that can be safely generated (ensuring reversibility) between endothelial cells, and the duration for which this

1
2
3 opening lasts, have not been measured. The knowledge of these parameters is crucial for the
4
5 current development of brain targeted nanoparticles. Functionalized MR-CA for instance, are
6
7 available in a wide range of hydrodynamic diameters: gadolinium chelates, a few nm
8
9 (Wadghiri *et al* 2003), iron nanoparticles, 25-100 nm (Mendonca Dias and Lauterbur 1986;
10
11 Renshaw *et al* 1986), gadolinium based emulsions or liposomes, 200-300 nm (Devoisselle *et*
12
13 *al* 1988), and have very different vascular remanences, ranging from a few minutes to tens of
14
15 hours. An estimate of the time window during which a molecule of a given size may be
16
17 delivered across the BBB would be useful to monitor the amount of drug released to cerebral
18
19 tissue and to adjust the dosage. For example, it has been shown that 3 – 8 nm wide particles
20
21 are able to cross BBB 20 min after its ultrasound-induced disruption, but not particles of size
22
23 50 nm (Choi *et al* 2010). Additionally, as the brain is unprotected while the BBB is open, it is
24
25 important to know the time-to-recovery to limit any possible brain damages induced by
26
27 tissular penetration of pathogenic agents.
28
29
30

31
32 The quantification of the amount of MR-CA crossing the BBB requires development
33
34 of molecular imaging sequences via imaging techniques that are sensitive (high field MRI)
35
36 and provide outputs that can be correlated with the MR-CA concentration. Contrast agent
37
38 (CA) quantification is one of the principal challenges for MR molecular imaging. Unlike
39
40 other techniques such as fluorescence or nuclear imaging where the received signal comes
41
42 directly from the CA, MR signal comes from the surrounding water protons and is therefore
43
44 indirectly related to the presence of an exogenous probe. To quantify the CA concentration
45
46 using MRI, it is necessary to model its interaction with the surrounding water molecules.
47
48 Paramagnetic complexes interact with the surrounding water protons by decreasing their
49
50 relaxation times (Swift and Connick 1962). CA concentration can be linked to the T_1 or T_2
51
52 relaxation time decrease (in ms). In this study, we adapted a T_1 mapping sequence proposed
53
54 by Deichmann and colleagues (Deichmann and Haase 1992; Deichmann *et al* 1999) that
55
56
57
58
59
60

permitted estimation of a wide range of T_1 values with a good accuracy, and high spatial and temporal resolutions.

In this study, a calibrated BBB opening procedure was performed in healthy young adult rats under MR guidance. Five MR-CA were used (3 paramagnetic and 2 superparamagnetic) with different hydrodynamic diameters (from 1 to 65 nm) to investigate the maximum permissible size of the gaps induced in the endothelial wall under safe conditions. Then, using the T_1 mapping strategy for the 3 paramagnetic CA we quantified the amount of particles crossing the BBB when injected at different times after ultrasound-induced BBB disruption. This enabled quantitative monitoring of the dynamics of BBB closure for each given molecular size. Lastly, we present a theoretical model to fit the experimental data and derive a calibration curve to predict duration of BBB opening as a function of the hydrodynamic diameter of a given CA.

Materials and Methods

Animal Preparation

All experiments were performed in accordance with the recommendations of the European Community (86/609/EEC) and the French legislation (decree no. 87/848) for use and care of laboratory animals. A total of 36 Sprague Dawley male rats (80-100 g, Janvier, France) were used. Their head was shaved to ensure proper coupling of the ultrasound beam to the brain. Rats were anesthetized with 1.5% isoflurane in a mixture of air and oxygen and placed in a cradle in prone position. A catheter (25 G needle) was positioned in the caudal vein to inject microbubbles and MR-CA from outside the scanner with minimal dead volume. 10% heparin was added to all injected solutions to avoid clot formation in the catheter. Body temperature and respiration rate were continuously monitored during the experiments.

MR-CA

MR-CA of different hydrodynamic diameters were provided by Guerbet Research (France). Main characteristics and injected doses of these nanoparticles are summarized in Table 1. After each MR-CA injection, the bolus was flushed by injection of 100 μ l of saline solution. Three of the five MR-CA were paramagnetic Gd-chelates (Dotarem®, P846, and P792) and were detected and quantified using T_1 strategies (Kang *et al* 2010; Protti *et al* 2010; Yankeelov *et al* 2006). The other two CA (P904 and P03680) were USPIO. A T_2 -weighted sequence was used to detect them in cerebral tissues (Hyodo *et al* 2009; Philippens *et al* 2004). Longitudinal r_1 and transverse r_2 relaxivities were measured *in vitro* at 7T using galleries of tubes containing different concentrations of CA diluted in a 0.3% agar matrix, and maintained at 37°C.

Ultrasound equipment

A MR-compatible focalized transducer (central frequency 1.5 MHz, diameter 30 mm, focal depth 20 mm, Imasonic, France) driven by a programmable function generator was used to produce ultrasound waves. It was coupled to the rat skull using a latex balloon filled with deionized and degassed water. Electrical power sent to the transducer was monitored during the BBB opening session. Main characteristics of the transducer (focal point size 0.6×0.6×3 mm³, transcranial acoustic transmission factor 52 ± 5 %) were estimated in a previous study [40].

BBB opening

BBB disruption was performed during MR imaging session thanks to a dedicated holder maintaining the ultrasound transducer above rat head. Its position was monitored using the ARFI sequence and the right thalamus in the brain was chosen as a target for BBB

1
2
3 disruption. Sonovue® microbubbles (Bracco, Italy) were administrated via a bolus (1.5×10^8
4 bubbles/ml, 200 μ l, 2 s) approximately 5 s before the beginning of ultrasound session. The
5 bolus was flushed by injection of 100 μ l of saline solution. Sonication was performed with
6 3 ms bursts every 100 ms for one minute (Choi *et al* 2011). The peak negative acoustic
7 pressure at the ultrasound focal point was calibrated to 0.45 MPa, a level sufficiently low to
8 ensure safe and reversible BBB opening (Larrat *et al* 2011; Chopra *et al* 2010). Anatomical
9 images were acquired at the end of each MRI session to verify integrity of the brain tissues.
10
11
12
13
14
15
16
17
18
19
20
21
22

23 **MRI acquisitions**

24
25 MRI was performed on a 7T/90 mm Pharmascan scanner (Bruker, Germany). A saddle
26 coil was specially designed in-house for excitation and signal reception. The geometry and
27 size of the resonator (diameter 30 mm) were optimized to maximize the overall signal-to-
28 noise ratio over the whole brain while allowing the ultrasound beam to propagate from the
29 transducer to the rat brain.
30
31
32
33
34
35

36 A multislice spin-echo sequence was modified to include additional motion-sensitizing
37 gradients, and synchronized to ultrasonic bursts so that the phase signal was proportional to
38 local acoustic intensity (Larrat *et al* 2010; McDannold and Maier 2008). This ARFI sequence
39 was acquired with the following parameters: TE/TR = 40/1700 ms, $T_{acq} = 4$ min,
40 $R = 0.5 \times 0.5 \times 1$ mm³, duration of the motion encoding gradients = 13.3 ms, duration of the
41 sonication = 3 ms.
42
43
44
45
46
47
48

49 A high spatial resolution T₂-weighted RARE sequence ($TE_{eff}/TR = 32/4200$ ms, $R =$
50 $0.125 \times 0.125 \times 0.3$ mm³) was used to detect the presence of USPIOs, and also for acquiring
51 images at the end of every experiment to confirm lack of haemorrhages or edema due to
52
53
54
55
56
57
58
59
60

ultrasound. T_1 -weighted MSME sequence ($TE/TR = 8/300$ ms, $R = 0.250 \times 0.250 \times 1$ mm³) was acquired to detect paramagnetic Gd-chelates.

To measure concentration of Gd-chelates, a T_1 mapping sequence was acquired before and after MR-CA injection. It consisted in a segmented series of fast gradient echo (FGE) images acquired at different time points after magnetization inversion in order to follow the entire T_1 recovery curve [24, 25]. Sequence parameters were: TR_1 , 5 ms, TE, 2.5 s, 6 segments, 60 inversion times (from 64 to 5800 ms), flip angle, 5°, and $R = 0.2 \times 0.2 \times 1$ mm³. Repetition time between the acquisitions of two segments, TR_2 , was 9 s, and total acquisition time is 12.5 min. A centric encoding of the k-space was chosen in order to avoid T_2 effects during echo trains at the acquisition of central lines.

Data analysis

Data were analyzed using dedicated codes written in Matlab software (MathWorks, USA). Maps of acoustic pressure index (IP_{ac}) were deduced from ARFI sequence using the following equation:

$$IP_{ac} \propto \frac{\sqrt{\varphi_{ON} - \varphi_{OFF}}}{P_{th}} \quad (1)$$

where φ_{ON} (respectively φ_{OFF}) is the phase of ARFI signal acquired with ultrasound (respectively without ultrasound), and P_{th} is the expected acoustic pressure at the focal point in case of an ideal ultrasound coupling. In a previous study (Larrat *et al* 2010), we verified the linearity between acoustic intensity and MR-ARFI phase signal using the same setup. In another study (Larrat *et al* 2011), we also characterized and verified the linearity between acoustic pressure and the amount of MR-CA crossing the BBB in the range of acoustic pressure values applied here.

To generate T_1 maps, the MRI signal measured with the FGE sequence was fitted as a function of the inversion time pixel by pixel as proposed by Deichmann and colleagues [24, 25]. MR-CA concentration maps (C) were then calculated from the T_{10} and the T_1 maps after MR-CA injection using the following equation (Swift and Connick 1962), considering that relaxivities r_1 measured *in vitro* in agar matrix hardly differ from the ones in rat brain tissues:

$$C = \frac{1}{r_1} \left(\frac{1}{T_1} - \frac{1}{T_{10}} \right) \quad (2)$$

Signals from different manually drawn ROIs were analyzed. A ROI_{spot} of $0.6 \times 0.6 \times 3 \text{ mm}^3$ corresponding to the transducer focal point size was drawn in the right thalamus. To analyze the effect of BBB disruption, a similar ROI_{contra} was taken in the corresponding contralateral (left thalamus) region of the brain. This enabled correction for the residual vascular concentration of MR-CA during imaging. Another control ROI was drawn in an extracerebral region in the cheek muscles (ROI_{muscle}). For each rat, a corrected MR-CA concentration at the focal point (C^* without unit) was calculated as given below, based on the concentration measured at the ROI_{spot} ($C_{ROI_{spot}}$) and that at the control spots ($C_{ROI_{contra}}$ and $C_{ROI_{muscle}}$), and the index of deposited acoustic pressure (IP_{ac}):

$$C^* = \frac{C_{ROI_{spot}} - C_{ROI_{contra}}}{C_{ROI_{muscle}} \cdot IP_{ac}} \quad (3)$$

This processing step was mandatory to ensure the correction of the bias introduced by unequal injected volumes (unequal plasmatic concentrations) and the bias introduced by variations in acoustic wave penetration through the skull. These corrections allowed comparing MR-CA concentrations among animals.

Results

Low power, pulsed, ultrasound for localized disruption of BBB

1
2
3 In a rat model, BBB was opened transiently with the use of ultrasound, immediately
4 followed by intravenous injection of Dotarem® (gadolinium (Gd)-chelate) and measurement
5 of the amount of the MR-CA delivered across the BBB (Figure 1). Before the ultrasound
6 sonication, acoustic radiation force imaging (ARFI) was performed to obtain the acoustic
7 pressure map in the brain (Figure 1-A). This sequence was used to verify that the ultrasound
8 beam was focused at the desired point in the right thalamus, and to estimate the acoustic
9 pressure at this focal point prior to microbubbles injection, ensuring that the acoustic pressure
10 remains below a predetermined safety threshold (Chopra *et al* 2010; Larrat *et al* 2011). Once
11 the transducer was set at the desired position, Sonovue® microbubbles were injected
12 intravenously via a catheter positioned in the caudal vein, and the BBB was disrupted by
13 pulsed sonication for one minute. Dotarem® was then injected using the same catheter. To
14 measure the concentration of Dotarem® delivered, T₁ maps were acquired before and after
15 MR-CA injection (Figure 1-B). There was high tissue perfusion of the CA (strong T₁
16 decrease) in the cheek and neck muscles, but not in the brain tissue due to the BBB. As
17 expected, the ultrasound focal point (red arrow) was the only area of the brain exhibiting a
18 strong T₁ decrease indicating BBB disruption. Based on T₁ mapping, CA concentration maps
19 were obtained at the three selected regions of interest (ROIs): ultrasound focal point, ROI_{spot}
20 (n°1), a control region contralateral to the ultrasound focal point, ROI_{contra} (n°2) and a region
21 in cheek muscles ROI_{checks} (n°3) (Figure 1-C).

22 23 24 25 26 27 28 29 30 31 32 33 34 35 36 37 38 39 40 41 42 43 44 45 46 47 **Maximum gap between endothelial cells after reversible ultrasound-induced disruption** 48 **of the BBB** 49

50
51
52 In order to determine the size of gaps generated after ultrasound-induced disruption of
53 the BBB, we chose five different MR-CA of varying hydrodynamic diameters (Table 1) and
54 verified their passage across BBB at the ultrasound focal point. The CA were intravenously
55
56
57
58
59
60

1
2
3 injected (n=1 rat for each CA) directly after ultrasound-induced BBB disruption. T₁-weighted
4 (T_{1w}) images were obtained for the 3 paramagnetic CA and T₂-weighted (T_{2w}) images for the
5 two ultrasmall superparamagnetic iron oxide (USPIO) CA (Figure 2). For all three Gd-
6 chelates, a positive contrast was clearly visible on T_{1w} images at the ultrasound focal point,
7 revealing the presence of the CA. Student's *t*-test performed on the measured MR signals
8 confirmed that signal differences between ROI_{spot} and ROI_{contra} were significant (p < 0.01).
9 For the 25 nm USPIO, a negative contrast appeared on T_{2w} images after its injection
10 suggesting that BBB was permeable to molecules of this size. Signal differences with
11 contralateral region were also significant (p < 0.01). However, the largest USPIO (65 nm) was
12 detected only at the very focal point of the transducer as its penetration was significantly
13 hindered compared to the smaller USPIO. The signal differences between ROI_{spot} and
14 ROI_{contra} for this USPIO were not significant (p > 0.01) if the ROI was of the standard size
15 (0.6×0.6×3 mm³), but the differences became significant (p < 0.01) if the size of the ROI_{spot}
16 was decreased to 0.2×0.2×1 mm³ around the focal point. These results suggest that 65 nm is
17 close to the maximal gap between endothelial cells that is attainable after BBB disruption
18 with this protocol.
19
20
21
22
23
24
25
26
27
28
29
30
31
32
33
34
35
36
37
38
39
40

41 **Quantification of MR-CA concentration**

42
43 Rats were injected with Dotarem® at increasing doses (375, 750 and 1500 μmol/kg,
44 n=1 rat per dose) following BBB disruption. Concentration maps acquired by T₁ mapping
45 were overlaid on the anatomical T_{2w} images (Figure 3-A). Additionally, a T₁-weighted
46 MSME sequence was also acquired. The estimated CA concentration at the ultrasound focal
47 point was found to be proportional to the injected dose (C₃₇₅ < C₇₅₀ < C₁₅₀₀) (Figure 3-B). In
48 contrast, the T_{1w} signals did not exhibit the same behavior and even saturated at high CA
49 injected doses (Figure 3-C). These observations confirm the high interest of our protocol to
50
51
52
53
54
55
56
57
58
59
60

1
2
3 precisely quantify small variations of CA concentration, and that quantitative analysis based
4
5 on T_{1w} signals alone can be misleading. Hence, results presented in the following sections of
6
7 this study were all derived from quantitative data obtained using the T_1 mapping sequence
8
9 (Equation 3).
10

14 **Quantitative study of BBB closure dynamics**

16 The BBB closure dynamics was assessed using paramagnetic CA of different
17
18 molecular sizes, administrated at different times after ultrasound-induced disruption. Rats
19
20 were injected with the following CA: Dotarem® (n=10 rats), P846 (n=10 rats) and P792 (n=8
21
22 rats) from 0 to 24 hours after ultrasound sonication. The reproducibility of CA delivery was
23
24 verified by measuring both the injected dose and the acoustic power deposited at the
25
26 ultrasound focal point. CA concentrations measured in the cheek muscles in each animal were
27
28 directly correlated with the injected dose since no permeability barrier like BBB exists in
29
30 muscles (Figure 4-A). Mean values were: 0.345 ± 0.034 mM for Dotarem® group,
31
32 0.061 ± 0.008 mM for P846 group and 0.040 ± 0.002 mM for P792 group. Variabilities
33
34 observed within the above three groups (10%, 13% and 5%, respectively) could be explained
35
36 by experimental errors during injection and also by slight variations in the weight or
37
38 metabolism of the animals. An index of the acoustic pressure (IP_{ac}) deposited at the focal
39
40 point was estimated from ARFI sequence (Figure 4-B) and was 1.13 ± 0.06 for Dotarem®
41
42 group, 1.00 ± 0.05 for P846 group and 0.97 ± 0.13 for P792 group. Variabilities observed
43
44 within the above three groups (5%, 5% and 13%, respectively) was mainly explained by slight
45
46 differences in the placement of the transducer on the heads. Variations in the incidence angle
47
48 of the ultrasound beam or in the thickness of the skull could have a significant impact on
49
50 attenuation of the beam during its passage through the skull and lead to variations of the peak-
51
52 negative acoustic pressure at the focal point.
53
54
55
56
57
58
59
60

1
2
3 Corrected CA concentrations (C^*) measured at the ultrasound focal point were plotted
4
5 as a function of the time elapsed between BBB disruption and MR-CA injection (Figure 4-C).
6
7 For Dotarem® (1 nm particle), the BBB was permeable for several hours post-BBB
8
9 disruption. A significant amount of CA was detectable in the brain even when injected 8 or 9
10
11 hours after disruption. Around 24 h post-disruption, the BBB had apparently recovered its
12
13 whole integrity, as very few CA were detectable in brain tissues. P846 (4 nm particle) was
14
15 delivered across the BBB only if injected within 2 hours post-BBB disruption. For P792
16
17 (7 nm particle), the duration of CA delivery to the brain was even shorter than for P846. One
18
19 hour post-BBB disruption, the amount of CA crossing the BBB was about 30% of its initial
20
21 value and dropped to undetectable levels after 90 minutes.
22
23

24
25 These findings confirmed that the duration of BBB crossing decreases when
26
27 increasing CA hydrodynamic diameter. Secondly, it appears from the shape of the time-
28
29 dependent concentration curve (Figure 4-C) that the BBB permeability decreased at a faster
30
31 rate initially and at a lesser rate later on.
32
33

34 35 36 **A model for BBB closure dynamics**

37
38 Based on the experimental observations, the BBB closure dynamics was modelled as
39
40 follows. First, it was assumed that each individual gap generated in the BBB by ultrasound
41
42 returns to its equilibrium position (i.e. closed) as a harmonic oscillator damped by fluid
43
44 friction. The gap diameter as a function of the time was therefore expressed as $d(t) = d_0 e^{-kt}$,
45
46 where d_0 is the gap diameter just after BBB disruption and k a time constant representative of
47
48 individual gap closure speed.
49
50

51
52 Next, the initial size distribution of gaps was assumed to be a hemi-Gaussian function
53
54 centered on 0 with a standard deviation σ_0 . These two conditions imply a distribution of gap
55
56 sizes as a function of time expressed as follows:
57
58
59
60

$$N(x,t) \propto \frac{1}{\sigma_0 e^{-kt}} e^{-\frac{x^2}{2\sigma_0^2 e^{-2kt}}} \quad (4)$$

For each time t , the amount $Q_{CA}(t)$ of CA of hydrodynamic diameter d_H crossing the BBB in a unit volume post-disruption is proportional to the inflow flux only, since the outflow of CA from brain to blood is assumed to be negligible due to high concentration in the blood compartment. Assuming a hard sphere behavior for CA molecules, $Q_{CA}(t)$ can be expressed as follows:

$$Q_{CA}(t) \propto \int_{d_H}^{+\infty} N(x,t) \cdot \frac{x^2}{d_H} dx \quad (5)$$

The CA diffusion in brain outside of the BBB disrupted region is also neglected since the CA tissular concentration is quantified within a few minutes after CA intravenous injection. A previous study from our team (Marty *et al* 2010) showed that the Gd-chelates used in this study do not diffuse fast enough in brain parenchyma to make this effect significant: for example, the diffusion coefficient of Dotarem® (1 nm particle) was estimated around $46 \mu\text{m}^2 \cdot \text{s}^{-1}$ (Table 1).

Integration of equation 5 gives:

$$Q_{CA}(t) \propto \frac{\sigma_0^2 e^{-2kt}}{d_H} \left(\sqrt{\frac{\pi}{2}} \left(1 - \text{erf} \left(\frac{d_H}{\sqrt{2}\sigma_0 e^{-kt}} \right) \right) + \frac{d_H}{\sigma_0 e^{-kt}} e^{-\frac{d_H^2}{2\sigma_0^2 e^{-2kt}}} \right) \quad (6)$$

All experimental data (n=28 rats) were used to fit this theoretical BBB closure model and determine the two parameters: a characteristic gap diameter $\sigma_0 = 1.54 \text{ nm}$, and BBB closure rate $k = 1.54 \times 10^{-5} \text{ s}^{-1}$.

The half closure time ($t_{1/2}$) was then defined as the time after disruption when the concentration of CA crossing the BBB was 50% of the maximal concentration obtained immediately after disruption. $t_{1/2}$ was then calculated as the numerical solution of the following equation:

$$\frac{1}{2} \left(\sqrt{\frac{\pi}{2}} \left(1 - \operatorname{erf} \left(\frac{d_H}{\sqrt{2}\sigma_0} \right) \right) + \frac{d_H}{\sigma_0} e^{-\frac{d_H^2}{2\sigma_0^2}} \right) = e^{-2kt_{1/2}} \left(\sqrt{\frac{\pi}{2}} \left(1 - \operatorname{erf} \left(\frac{d_H}{\sqrt{2}\sigma_0 e^{-kt_{1/2}}} \right) \right) + \frac{d_H}{\sigma_0 e^{-kt_{1/2}}} e^{-\frac{d_H^2}{2\sigma_0^2 e^{-2kt_{1/2}}}} \right) \quad (7)$$

From the fitted parameters (σ_0 and k), half closure times could be estimated as a function of hydrodynamic diameters of the molecules by numerically solving equation 7 (Figure 5, black circles). The calculated half closure time was ~ 5.5 h for a 1 nm particle; ~ 1.5 h for a 4 nm particle and about 30 min for a 7 nm particle. These values were close to those estimated experimentally for Dotarem®, P846 and P792, which were 5.2 h, 1.2 h and 45 min, respectively (Figure 5, red crosses).

For larger molecules, half closure times were greatly reduced (around 3 min for a 25 nm particle and only few seconds for a 65 nm particle). These results match the qualitative results obtained with USPIOs (Figure 2). Therefore, to deliver a significant amount of larger molecular size CA across the BBB their intravenous circulation should coincide with the end of ultrasound sonication.

Lastly, it appears that the following analytical formula fits reasonably well the numerical solution of equation 7, enabling to directly estimate half closure time as a function of hydrodynamic diameter:

$$t_{1/2} = \frac{A}{1 + B \cdot d_H^2} \quad (8)$$

with $A = 2.35 \times 10^4$ s and $B = 0.2106 \text{ nm}^{-2}$ (Figure 5, solid line).

Discussion

Ultrasound-induced BBB disruption

Drug delivery to the brain remains a major challenge for the treatment of most brain diseases. Although pathologies such as cancer degrade BBB integrity (Liu *et al* 2012), it was proven that endothelial wall permeability is still poorer in these regions than in vessels of

1
2
3 other organs. Recently, ultrasound-induced BBB disruption was demonstrated to be an
4
5 effective method of significantly increasing permeability of the blood-tumor barrier in a
6
7 controlled manner (Chen *et al* 2010). Another study reported that vessel wall permeability
8
9 after ultrasound-induced BBB disruption was comparable to permeability values for
10
11 unprotected organs (Vlachos *et al* 2010). Our study further demonstrates that ultrasound
12
13 combined with intravenous injection of microbubbles is a reliable, reproducible and non-
14
15 invasive technique to deliver nanoparticles with hydrodynamic diameters up to 65 nm.
16
17 Moreover, in our protocol, no edema or hemorrhages were detected on T_{2w} images following
18
19 ultrasound sonication. Animals kept alive for several weeks after undergoing BBB disruption
20
21 showed no adverse effects. The observation of a return to basal permeability within 24 hours
22
23 for the smallest available CA (1 nm) further proved that the disruption was transient and
24
25 reversible.
26
27
28
29
30

31 **MR guidance**

32
33
34 The ultrasound-induced BBB disruption described here was performed entirely under
35
36 high-field MRI guidance. This is a challenge as it requires integrating a stereotactic frame, a
37
38 MR-compatible ultrasound transducer adapted to the geometry of the rodent head and a
39
40 dedicated radiofrequency (RF) coil fitted into the 8.5 cm bore of a preclinical MRI scanner.
41
42 The optimized RF coil allowed the quantification of Gd MR-CA at a micromolar range, with
43
44 sufficient signal homogeneity over the whole brain and the ability for the ultrasound beam to
45
46 propagate through the coil.
47
48

49
50 The anesthetized animal was placed inside the MRI scanner just before the start of the
51
52 BBB disruption procedure till recovery. Thus, it was possible to obtain an acoustic intensity
53
54 map before BBB disruption. This ensured a proper positioning of the ultrasound focal spot in
55
56 the right thalamus and a precise *in situ* calibration of the acoustic pressure to avoid
57
58
59
60

1
2
3 irreversible tissue damage. Furthermore, microbubbles were injected to cause ultrasound-
4 induced BBB disruption followed by injection of MR-CA via the same the catheter, which
5 allowed imaging of the early events post-BBB disruption.
6
7
8

9 10 11 **Maximum gap obtained between endothelial cells**

12
13
14 CA of increasing hydrodynamic sizes were tested, and the maximum gap width
15 generated between endothelial cells after BBB disruption was estimated with our acoustic
16 parameters. Gaps slightly above 65 nm could be generated safely, and the BBB recovered full
17 integrity within 24 h. The mechanical index of our set-up was 0.37 which is below the
18 standard value proposed by other studies for reversible BBB opening (McDannold *et al*
19 2008). This result is particularly interesting from the view of development of targeted CA.
20 Using a similar sonoporation protocol, it would be possible to deliver nanoparticles such as
21 USPIOs, functionalized to target tissular biomarkers. In contrast, larger objects like emulsions
22 or liposomes that typically have hydrodynamic diameters >100 nm, would be difficult to
23 deliver to the brain using this technique, assuming a purely paracellular pathway. In general,
24 an estimate of the maximum possible gap diameter would be helpful when the technique is
25 applied to deliver therapeutic molecules. Several therapeutic drugs could benefit from this
26 information: for instance chemotherapeutic drugs such as Avastin® ($d_H \sim 10$ nm),
27 recombinant adeno-associated virus (rAAV) vectors for gene therapy ($d_H \sim 20$ nm),
28 monoclonal antibodies such as anti- β -amyloid (d_H of few nm), and vectorized short interfering
29 RNA (siRNA) used for gene expression modulation ($d_H \sim 50$ nm).
30
31
32
33
34
35
36
37
38
39
40
41
42
43
44
45
46
47
48

49
50 The maximum gap diameter measured in this study is probably dependent of the
51 sonication parameters, in particular ultrasound frequency, pulse duration and duty cycle, total
52 sonication time and size distribution of injected microbubbles (Sonovue® has a broad
53 distribution between 1-8 μ m). Here, we chose well established parameters that have been
54
55
56
57
58
59
60

1
2
3 proposed by others (Choi *et al* 2011). Several groups have studied the influence of acoustic
4
5 parameters (O'Reilly *et al* 2011a) and microbubbles size (Samiotaki 2011) on BBB opening.
6
7 An optimization of parameters based on the knowledge gained from these studies may allow
8
9 generation of pores larger than 65 nm wide.
10

11 12 13 14 **BBB closure dynamics**

15
16 In this study, the concentration of paramagnetic CA delivered at the ultrasound focal
17
18 point was quantitatively measured, based on which, the duration of passage across the BBB
19
20 was estimated for molecules of different sizes. This duration decreased rapidly as a function
21
22 of hydrodynamic diameter of the CA. For instance, small molecules (around 1 nm) continued
23
24 to cross the BBB for more than 10 h, whereas large iron oxide particles (around 25 nm) had a
25
26 time window of only a few minutes. Therefore, to maximize the amount of extravasation in
27
28 the brain, large molecules should be injected right after or even during ultrasound sonication.
29
30

31
32 The results presented here also suggest a closure of the BBB at a progressively
33
34 decreasing rate. We present a simple, damped, elastic model assuming an exponential decay
35
36 of individual gap sizes to semi-quantitatively describe the observed dynamics of BBB closure.
37
38 The experimental data were fed in the model to derive important physiological parameters,
39
40 such as the typical closure time constant k that was estimated to be $1.54 \times 10^{-5} \text{ s}^{-1}$. This
41
42 parameter is an indirect measurement of rate of endothelial cell relaxation after contraction. It
43
44 could be used as a physio-pathological index of vessel integrity.
45
46

47
48 This model assumes a paracellular passage of injected molecules with an inflow
49
50 limited by the size of the molecule relative to the size of the pores. Our results support the
51
52 notion that most of the crossing happens between endothelial cells rather than through them.
53
54 This reinforces the hypothesis that during ultrasound-induced BBB opening sonicated
55
56
57
58
59
60

1
2
3 microbubbles exert a mechanical stress on endothelial cells which makes them contract on
4 themselves and loosen the junctions between them creating gaps (Vykhodtseva *et al* 2008).
5
6
7

8 9 **Limitations of the study**

10 The proposed BBB closure model has certain limitations. It does not take into account
11 potential increased permeability of endothelial cell membranes (transcellular BBB crossing).
12 It does not distinguish between hydrophilic and lipophilic molecules although it is known that
13 lipophilic agents present an increased ability to cross the BBB via transcytosis (Pardridge
14 2005). This concurrent release pathway could explain the observed differences between
15 experimental data of P846 and P792 and predictions from the theoretical model.
16
17
18
19
20
21
22
23
24

25 The three Gd-chelates compared in this study have similar but not equal vascular
26 remanences (Table 1). The tissular concentrations were measured within 12.5 minutes after
27 CA injection, which is not a negligible time delay as the plasmatic half-life of the CA are
28 between 26 and 51 min (Fries *et al* 2009). Although during data processing the differences in
29 overall injected plasmatic concentration were corrected for each CA (Equation 3), temporal
30 variations of vascular concentrations during the T₁ mapping acquisition could be different
31 from one CA to the other, none of them remaining strictly steady. The impact of these
32 variations may be low since the MRI mapping acquisition was performed with a centric
33 encoding scheme. Nevertheless, it may explain the differences between the theoretical model
34 and the experimentally measured closure dynamics for the different molecules.
35
36
37
38
39
40
41
42
43
44
45
46
47
48

49 **Conclusion**

50 In this study, we developed a complete methodology for noninvasive, reversible and
51 controlled ultrasound-induced BBB disruption under MR-guidance that permitted precise
52 quantification of the amount of MR-CA delivered to brain parenchyma in a rat model. The
53
54
55
56
57
58
59
60

1
2
3 two key parameters in designing drug delivery across the BBB, namely, the largest
4
5 deliverable molecular size of the agent, and the time window for delivery of an agent of a
6
7 given molecular size, were estimated for the first time.
8
9

10 11 **Acknowledgements**

12
13
14 Authors would like to thank M. Leopoldie for providing animal care, B. Bresson for
15
16 RF coil support and Dr. A. Alahari for editing this manuscript.
17
18

19 20 21 **Disclosure/Conflict of interest**

22
23 Authors declare no conflict of interest.
24
25
26
27
28
29
30
31
32
33
34
35
36
37
38
39
40
41
42
43
44
45
46
47
48
49
50
51
52
53
54
55
56
57
58
59
60

References

Chen P-Y, Liu H-L, Hua M-Y, Yang H-W, Huang C-Y, Chu P-C, Lyu L-A, Tseng IC, Feng L-Y, Tsai H-C, Chen S-M, Lu Y-J, Wang J-J, Yen T-C, Ma Y-H, Wu T, Chen J-P, Chuang J-I, Shin J-W, Hsueh C, Wei K-C (2010) Novel magnetic/ultrasound focusing system enhances nanoparticle drug delivery for glioma treatment. *Neuro-Oncology* 12:1050-60

Choi JJ, Small SA, Konofagou EE (2006) Optimization of blood-brain barrier opening in mice using focused ultrasound. *2006 IEEE Ultrasonics Symposium (IEEE Cat No06CH37777)*

Choi JJ, Wang S, Tung Y-S, Morrison B, III, Konofagou EE (2010) Molecules of various pharmacologically-relevant sizes can cross the ultrasound-induced Blood-Brain Barrier opening in vivo. *Ultrasound Med Biol* 36:58-67

Choi JJ, Selert K, Gao Z, Samiotaki G, Baseri B, Konofagou EE (2011) Noninvasive and localized blood-brain barrier disruption using focused ultrasound can be achieved at short pulse lengths and low pulse repetition frequencies. *J Cereb Blood Flow Metab* 31:725-37

Chopra R, Vykhodtseva N, Hynynen K (2010) Influence of exposure time and pressure amplitude on blood-brain-barrier opening using transcranial ultrasound exposures, vol. 1(5): *ACS Chem Neurosci*, 391-8

Deichmann R, Haase A (1992) Quantification of T1 values by Snapshot-Flash NMR imaging. *J Mag Reson* 96:608-12

Deichmann R, Hahn D, Haase A (1999) Fast T1 mapping on a whole-body scanner. *Magn Reson Med* 42:206-9

Devoisselle JM, Viondury J, Galons JP, Confortgouny S, Coustaut D, Canioni P, Cozzone PJ (1988) Entrapment of Gadolinium-DTPA in liposomes - Characterization of vesicles by P-31 NMR-Spectroscopy. *Invest Radiol* 23:719-24

Fries P, Runge VM, Bucker A, Schurholz H, Reith W, Robert P, Jackson C, Lanz T, Schneider G (2009) Brain Tumor Enhancement in Magnetic Resonance Imaging at 3 Tesla Intraindividual Comparison of Two High Relaxivity Macromolecular Contrast Media With a Standard Extracellular Gd-Chelate in a Rat Brain Tumor Model. *Invest Radiol* 44:200-6

Hawkins BT, Davis TP (2005) The blood-brain barrier/neurovascular unit in health and disease. *Pharmacol Rev* 57:173-85

Hynynen K, McDannold N, Vykhodtseva N, Jolesz FA (2001) Noninvasive MR imaging-guided focal opening of the blood-brain barrier in rabbits. *Radiology* 220:640-6

Hynynen K, McDannold N, Sheikov NA, Jolesz FA, Vykhodtseva N (2005) Local and reversible blood-brain barrier disruption by noninvasive focused ultrasound at frequencies suitable for trans-skull sonications. *Neuroimage* 24:12-20

1
2
3 Hyodo F, Chandramouli GVR, Matsumoto S, Matsumoto K-I, Mitchell JB, Krishna MC,
4 Munasinghe JP (2009) Estimation of tumor microvessel density by MRI using a blood pool
5 contrast agent. *Int J Oncol* 35:797-804
6

7 Jordao JF, Ayala-Grosso CA, Markham K, Huang Y, Chopra R, McLaurin J, Hynynen K,
8 Aubert I (2010) Antibodies targeted to the brain with image-guided focused ultrasound
9 reduces amyloid-beta plaque load in the TgCRND8 mouse model of Alzheimer's disease.
10 *PLoS one* 5:e10549
11

12 Kang C-K, Park C-A, Kim K-N, Hong S-M, Park C-W, Kim Y-B, Cho Z-H (2010) Non-
13 Invasive Visualization of Basilar Artery Perforators With 7T MR Angiography. *J Magn*
14 *Reson Imaging* 32:544-50
15

16 Larrat B, Pernot M, Aubry JF, Dervishi E, Sinkus R, Seilhean D, Marie Y, Boch AL, Fink M,
17 Tanter M (2010) MR-guided transcranial brain HIFU in small animal models. *Phys Med Biol*
18 55:365-88
19

20 Larrat B, Marty B, Pernot M, Tanter M, Lethimonnier F, Mériaux S (2011) MR-Acoustic
21 Radiation Force Mapping can Quantitatively Predict Drug Delivery following Ultrasound-
22 Induced Blood Brain Barrier Disruption in Rats at High Field). ISMRM, Montreal, Canada
23

24 Liu H-L, Hua M-Y, Chen P-Y, Chu P-C, Pan C-H, Yang H-W, Huang C-Y, Wang J-J, Yen T-
25 C, Wei K-C (2010) Blood-Brain Barrier Disruption with Focused Ultrasound Enhances
26 Delivery of Chemotherapeutic Drugs for Glioblastoma Treatment. *Radiology* 255:415-25
27

28 Liu H-L, Yang H-W, Hua M-Y, Wei K-C (2012) Enhanced therapeutic agent delivery
29 through magnetic resonance imaging-monitored focused ultrasound blood-brain barrier
30 disruption for brain tumor treatment: an overview of the current preclinical status. *Neurosurg*
31 *focus* 32:E4
32

33 Marty B, Flament J, Giraudeau C, Robic C, Port M, Lethimonnier F, Boumezbeur F, Valette
34 J, Le Bihan D, Mériaux S (2010) Apparent diffusion coefficient of Gd-based contrast agents
35 assessed in vivo in the rat brain using dynamic T1 mapping). ISMRM, Stockholm, Sweden
36

37 McDannold N, Maier SE (2008) Magnetic resonance acoustic radiation force imaging. *Med*
38 *Phys* 35:3748-58
39

40 McDannold N, Vykhodtseva N, Hynynen K (2008) Blood-brain barrier disruption induced by
41 focused ultrasound and circulating preformed microbubbles appears to be characterized by the
42 mechanical index. *Ultrasound Med Biol* 34:834-40
43

44 Mendonca Dias MH, Lauterbur PC (1986) Ferromagnetic particles as contrast agents for
45 magnetic resonance imaging of liver and spleen. *Magnetic resonance in medicine : official*
46 *journal of the Society of Magnetic Resonance in Medicine / Society of Magnetic Resonance in*
47 *Medicine* 3:328-30
48

49 O'Reilly MA, Huang Y, Hynynen K (2010) The impact of standing wave effects on
50 transcranial focused ultrasound disruption of the blood-brain barrier in a rat model. *Phys Med*
51 *Biol* 55:5251-67
52
53
54
55
56
57
58
59
60

1
2
3 O'Reilly MA, Waspe AC, Ganguly M, Hynynen K (2011a) Focused-Ultrasound disruption of
4 the Blood-Brain Barrier using closely-timed short pulses: Influence of sonication parameters
5 and injection rate. *Ultrasound Med Biol* 37:587-94
6

7 O'Reilly MA, Yuexi H, Hynynen K (2011b) Standing Waves in Small Animal Models
8 Investigating Ultrasound Disruption of the Blood-Brain Barrier. *AIP Conference Proceedings*
9 1359
10

11 Pardridge WM (2005) The blood-brain barrier: bottleneck in brain drug development.
12 *NeuroRx : the journal of the American Society for Experimental NeuroTherapeutics* 2:3-14
13

14 Philippens MEP, Garnbarota G, Pikkemaat JA, Peeters WJM, van der Kogel AJ, Heerschap A
15 (2004) Characterization of late radiation effects in the rat thoracolumbar spinal cord by MR
16 imaging using USPIO. *MAGMA* 17:303-12
17

18 Protti A, Sirker A, Shah AM, Botnar R (2010) Late Gadolinium Enhancement of Acute
19 Myocardial Infarction in Mice at 7T: Cine-FLASH Versus Inversion Recovery. *J Magn Reson*
20 *Imaging* 32:878-86
21

22 Raymond SB, Treat LH, Dewey JD, McDannold NJ, Hynynen K, Bacskai BJ (2008)
23 Ultrasound Enhanced Delivery of Molecular Imaging and Therapeutic Agents in Alzheimer's
24 Disease Mouse Models. *Plos One* 3
25

26 Renshaw PF, Owen CS, McLaughlin AC, Frey TG, Leigh JS (1986) Ferromagnetic contrast
27 agents - A new approach. *Magn Reson Med* 3:217-25
28

29 Rubin LL, Staddon JM (1999) The cell biology of the blood-brain barrier. *Annual Review of*
30 *Neuroscience* 22:11-28
31

32 Samiotaki G, Vlachos, F., Tung, Y.-S. and Konofagou, E. E. (2011) A quantitative pressure
33 and microbubble-size dependence study of focused ultrasound-induced blood-brain barrier
34 opening reversibility in vivo using MRI: *Magn Reson Med*
35

36 Sheikov N, McDannold N, Sharma S, Hynynen K (2008) Effect of focused ultrasound applied
37 with an ultrasound contrast agent on the tight junctional integrity of the brain microvascular
38 endothelium. *Ultrasound Med Biol* 34:1093-104
39

40 Swift TJ, Connick RE (1962) NMR-Relaxation mechanisms of ^{17}O in aqueous solutions of
41 paramagnetic cations and lifetime of water molecules in first coordination sphere. *J Chem*
42 *Phys* 37:307-&
43

44 Treat LH, Zhang Y, McDannold N, Hynynen K (2009) Impact of Focused Ultrasound-
45 enhanced Drug Delivery on Survival in Rats with Glioma. In: *8th International Symposium on*
46 *Therapeutic Ultrasound* (Ebbini ES, ed), vol. 1113, 443-7
47

48 Vlachos F, Tung YS, Konofagou EE (2010) Permeability assessment of the focused
49 ultrasound-induced blood-brain barrier opening using dynamic contrast-enhanced MRI. *Phys*
50 *Med Biol* 55:5451-66
51

1
2
3 Vlachos F, Tung Y-S, Konofagou E (2011) Permeability Dependence Study of the Focused
4 Ultrasound-Induced Blood-Brain Barrier Opening at Distinct Pressures and Microbubble
5 Diameters Using DCE-MRI. *Magn Reson Med* 66:821-30
6

7 Vykhodtseva N, McDannold N, Hynynen K (2008) Progress and problems in the application
8 of focused ultrasound for blood-brain barrier disruption. *Ultrasonics* 48:279-96
9

10 Wadghiri YZ, Sigurdsson EM, Sadowski M, Elliott JI, Li YS, Scholtzova H, Tang CY,
11 Aguinaldo G, Pappolla M, Duff K, Wisniewski T, Turnbull DH (2003) Detection of
12 Alzheimer's amyloid in Transgenic mice using magnetic resonance microimaging. *Magn*
13 *Reson Med* 50:293-302
14

15
16 Yankeelov TE, DeBusk LM, Billheimer DD, Luci JJ, Lin PC, Price RR, Gore JC (2006)
17 Repeatability of a reference region model for analysis of murine DCE-MRI data at 7T. *J*
18 *Magn Reson Imaging* 24:1140-7
19

Titles and legends to figures

Figure 1: Different steps of MRI-guided ultrasound-induced disruption of blood-brain barrier (BBB). BBB disruption was achieved by intravenous injection of microbubbles via a catheter in the tail vein, in conjunction with transcranial ultrasound sonication. This was followed by injection of MRI contrast agent (CA) via the same catheter. The entire procedure was performed inside a 7T MRI scanner. A. Index of deposited acoustic pressure map derived from ARFI images acquired before injection of microbubbles revealed the ultrasound focal point. B. T_1 maps (in ms) acquired before (Baseline) and after MR-CA injection. C. MR-CA concentration map (in mM) derived from corresponding T_1 maps. Concentrations from three regions of interest (ROIs) were analyzed: ultrasound focal point ($n^{\circ}1$), contralateral control region ($n^{\circ}2$) and extra-cerebral control region in the cheek muscles ($n^{\circ}3$).

Figure 2: Ultrasound-induced localized delivery in rat brain of MRI contrast agents (CA) with different hydrodynamic diameters. Paramagnetic CA (Dotarem®, P846 and P792) or ultrasmall superparamagnetic iron oxide (USPIO) CA (P904 and P03680) were injected in rats immediately after ultrasound-induced BBB disruption, and the signal intensities were measured within 5 minutes at the ultrasound focal point. T_{1w} images of the paramagnetic CA (A, B and C) revealed a positive contrast, while T_{2w} images of the USPIO revealed a negative contrast (D and E). Comparison of the signal enhancement in arbitrary units (a.u.) in the region of interest of ultrasound focal point (ROI_{spot} , $n^{\circ}1$) and that in the control contralateral region (ROI_{contra} , $n^{\circ}2$) is given next to the scan corresponding to each CA ($n = 1$ rat for each CA). Differences between the two regions were considered significant for p -values < 0.01 (*) using a Student's t -test.

1
2
3 **Figure 3: Comparison of T_{1w} -weighted (T_{1w}) and T_1 mapping strategies to assess the**
4 **amount of Gadolinium (Gd)-chelate crossing the BBB.** Dotarem® was injected at different
5 doses just after ultrasound-induced BBB disruption in the right thalamus, followed by the
6 acquisition of one T_1 mapping sequence (to produce a concentration map) and one T_{1w}
7 sequence. A. Overlay of CA concentration maps on the corresponding anatomical T_{2w} images
8 after injection of increasing doses of Dotarem® (375 , 750 and 1500 $\mu\text{mol/kg}$, $n = 1$ rat per
9 dose). Purple arrows indicate the ultrasound focal spot where the BBB was disrupted. B. CA
10 concentration as estimated using T_1 mapping strategy at the ultrasound focal point showing
11 linear dependence on the injected dose. C. T_{1w} signal of the CA at the ultrasound focal point
12 as a function of the injected dose showing a saturation effect.
13
14
15
16
17
18
19
20
21
22
23
24
25
26

27 **Figure 4: BBB closure dynamics after ultrasound induced disruption for MR-CA of**
28 **different molecular sizes.** Paramagnetic CA were injected at different times (0 to 24h) after
29 BBB disruption. A. Concentrations of the three paramagnetic CA in the region of interest in
30 the cheek muscles $C_{ROI\text{muscle}}$ were measured. B. Index of delivered acoustic pressure at the
31 ultrasound focal point in the right thalamus in the brain. The maximum variability within each
32 group (CA) for these two parameters was 13 %. C. Corrected concentration (C^*) of the CA at
33 the ultrasound focal point in the brain was plotted as a function of the time elapsed between
34 ultrasound-induced BBB opening and the MR-CA injection ($n = 1$ rat per time point). All
35 experimental data ($n=28$ rats) were used to fit the theoretical BBB closure model and
36 determine the two parameters ($\sigma_0 = 1.54$ nm, $k = 1.54 \times 10^{-5} \text{ s}^{-1}$) (Equation 6); dashed lines
37 correspond to the fitted data for each MR-CA.
38
39
40
41
42
43
44
45
46
47
48
49
50
51
52
53
54


55 **Figure 5: Prediction of the time window of BBB passage for a given nanoparticle size.**

56 Based on the theoretical model proposed here, half closure time, $t_{1/2}$ (the time after
57
58
59
60

1
2
3 ultrasound-induced BBB disruption that is required for the delivery of 50% of the maximal
4
5 dose to the predetermined ultrasound focal point in the brain) was calculated as a function of
6
7 the hydrodynamic diameter of the nanoparticle (Equation 7) (black circles). Red crosses
8
9 correspond to experimental data on the paramagnetic nanoparticle contrast agents used here
10
11 (Dotarem® 1 nm; P846 4 nm; and P792 7 nm) and the solid line represents the best fit with
12
13 analytical function: $t_{1/2} = A / (1 + B \cdot d_H^2)$, where d_H is the hydrodynamic diameter of the
14
15 injected CA (in nm) and A and B are constants, $A = 2.35 \times 10^4$ s and $B = 0.2106 \text{ nm}^{-2}$.
16
17
18
19
20
21
22
23
24
25
26
27
28
29
30
31
32
33
34
35
36
37
38
39
40
41
42
43
44
45
46
47
48
49
50
51
52
53
54
55
56
57
58
59
60

	d_H (nm)	r_1 ($\text{mM}^{-1} \cdot \text{s}^{-1}$)	r_2 ($\text{mM}^{-1} \cdot \text{s}^{-1}$)	Dose ($\mu\text{mol/kg}$ body weight)	Vascular remenance (min)	Diffusion coefficient (\times $10^{-11} \text{ m}^2 \cdot \text{s}^{-1}$)
Paramagnetic MR-CA						
Dotarem®	<1	3.4	4.8	1500	26	4.6
P846	4	10.3	37	95	51	1.4
P792	7	4.9	42	210	32	0.8
Superparamagnetic MR-CA						
P904	21	1.4	88	1030	-	-
P03680	65	2.0	80	258	-	-


Table 1: Principal features of the paramagnetic and superparamagnetic nanoparticle contrast agents (CA) used in this study. Hydrodynamic diameters (d_H) were measured by light scattering, longitudinal (r_1) and transverse (r_2) relaxivities were estimated at 7T in 0.3% agar gels maintained at 37°C, vascular remanences were taken from literature (34) and diffusion coefficients in brain parenchyma were estimated in a previous work (28). The paramagnetic CA were imaged using T_{1w}/T_1 mapping sequences, while the superparamagnetic using T_{2w} sequences.

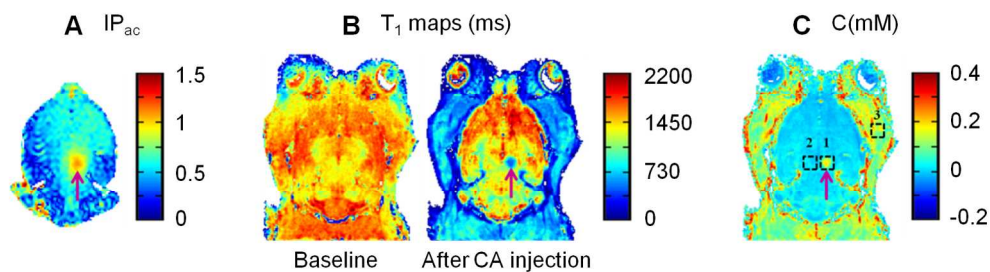

Different steps of MRI-guided ultrasound-induced disruption of blood-brain barrier (BBB). BBB disruption was achieved by intravenous injection of microbubbles via a catheter in the tail vein, in conjunction with transcranial ultrasound sonication. This was followed by injection of MRI contrast agent (CA) via the same catheter. The entire procedure was performed inside a 7T MRI scanner. A. Index of deposited acoustic pressure map derived from ARFI images acquired before injection of microbubbles revealed the ultrasound focal point. B. T_1 maps (in ms) acquired before (Baseline) and after MR-CA injection. C. MR-CA concentration map (in mM) derived from corresponding T_1 maps. Concentrations from three regions of interest (ROIs) were analyzed: ultrasound focal point ($n^{\circ}1$), contralateral control region ($n^{\circ}2$) and extra-cerebral control region in the cheek muscles ($n^{\circ}3$).

160x46mm (300 x 300 DPI)

For Review Only

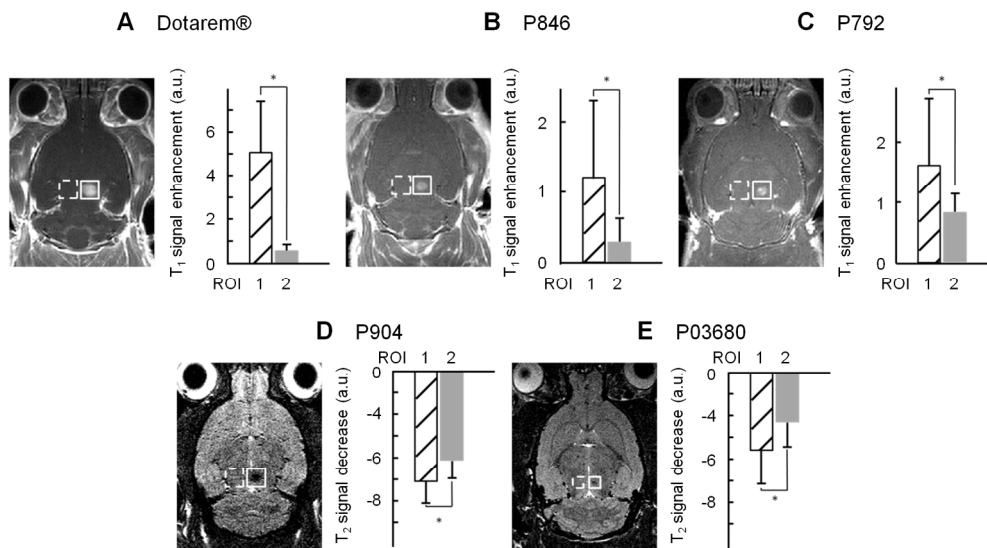

Ultrasound-induced localized delivery in rat brain of MRI contrast agents (CA) with different hydrodynamic diameters. Paramagnetic CA (Dotarem®, P846 and P792) or ultrasmall superparamagnetic iron oxide (USPIO) CA (P904 and P03680) were injected in rats immediately after ultrasound-induced BBB disruption, and the signal intensities were measured within 5 minutes at the ultrasound focal point. T_{1w} images of the paramagnetic CA (A, B and C) revealed a positive contrast, while T_{2w} images of the USPIO revealed a negative contrast (D and E). Comparison of the signal enhancement in arbitrary units (a.u.) in the region of interest of ultrasound focal point (ROI_{spot} , $n^{\circ}1$) and that in the control contralateral region (ROI_{contra} , $n^{\circ}2$) is given next to the scan corresponding to each CA ($n = 1$ rat for each CA). Differences between the two regions were considered significant for p-values < 0.01 (*) using a Student's t -test.

172x97mm (300 x 300 DPI)

Review Only

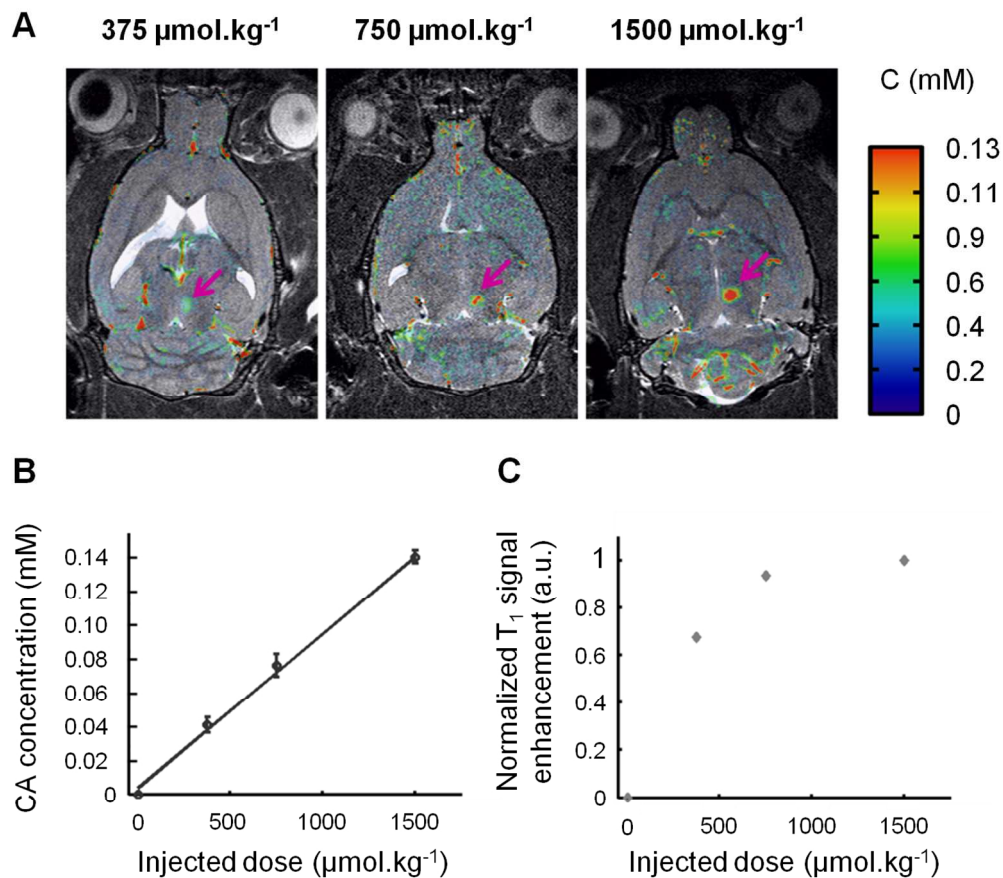


Figure 3: Comparison of T_1 -weighted (T_{1w}) and T_1 mapping strategies to assess the amount of Gadolinium (Gd)-chelate crossing the BBB. Dotarem® was injected at different doses just after ultrasound-induced BBB disruption in the right thalamus, followed by the acquisition of one T_1 mapping sequence (to produce a concentration map) and one T_{1w} sequence. A. Overlay of CA concentration maps on the corresponding anatomical T_{2w} images after injection of increasing doses of Dotarem® (375, 750 and 1500 $\mu\text{mol/kg}$, $n = 1$ rat per dose). Purple arrows indicate the ultrasound focal spot where the BBB was disrupted. B. CA concentration as estimated using T_1 mapping strategy at the ultrasound focal point showing linear dependence on the injected dose. C. T_{1w} signal of the CA at the ultrasound focal point as a function of the injected dose showing a saturation effect.

124x112mm (300 x 300 DPI)

Only





Figure 4: BBB closure dynamics after ultrasound induced disruption for MR-CA of different molecular sizes. Paramagnetic CA were injected at different times (0 to 24h) after BBB disruption. A. Concentrations of the three paramagnetic CA in the region of interest in the cheek muscles $C_{ROI\text{muscle}}$ were measured. B. Index of delivered acoustic pressure at the ultrasound focal point in the right thalamus in the brain. The maximum variability within each group (CA) for these two parameters was 13 %. C. Corrected concentration (C^*) of the CA at the ultrasound focal point in the brain was plotted as a function of the time elapsed between ultrasound-induced BBB opening and the MR-CA injection ($n = 1$ rat per time point). All experimental data ($n = 28$ rats) were used to fit the theoretical BBB closure model and determine the two parameters ($\sigma_0 = 1.54 \text{ nm}$, $k = 1.54 \times 10^{-5} \text{ s}^{-1}$) (Equation 6); dashed lines correspond to the fitted data for each MR-CA.

172x162mm (300 x 300 DPI)

Only



Prediction of the time window of BBB passage for a given nanoparticle size. Based on the theoretical model proposed here, half closure time, $t_{1/2}$ (the time after ultrasound-induced BBB disruption that is required for the delivery of 50 % of the maximal dose to the predetermined ultrasound focal point in the brain) was calculated as a function of the hydrodynamic diameter of the nanoparticle (Equation 7) (black circles). Red crosses correspond to experimental data on the paramagnetic nanoparticle contrast agents used here (Dotarem® 1 nm; P846 4 nm; and P792 7 nm) and the solid line represents the best fit with analytical function: $t_{1/2} = A / (1 + B \cdot d_H^2)$, where d_H is the hydrodynamic diameter of the injected CA (in nm) and A and B are constants, $A = 2.35 \times 10^4$ s and $B = 0.2106 \text{ nm}^{-2}$.

80x68mm (300 x 300 DPI)

www.Only