






Pulse Oximetry Sensor Decision Tree

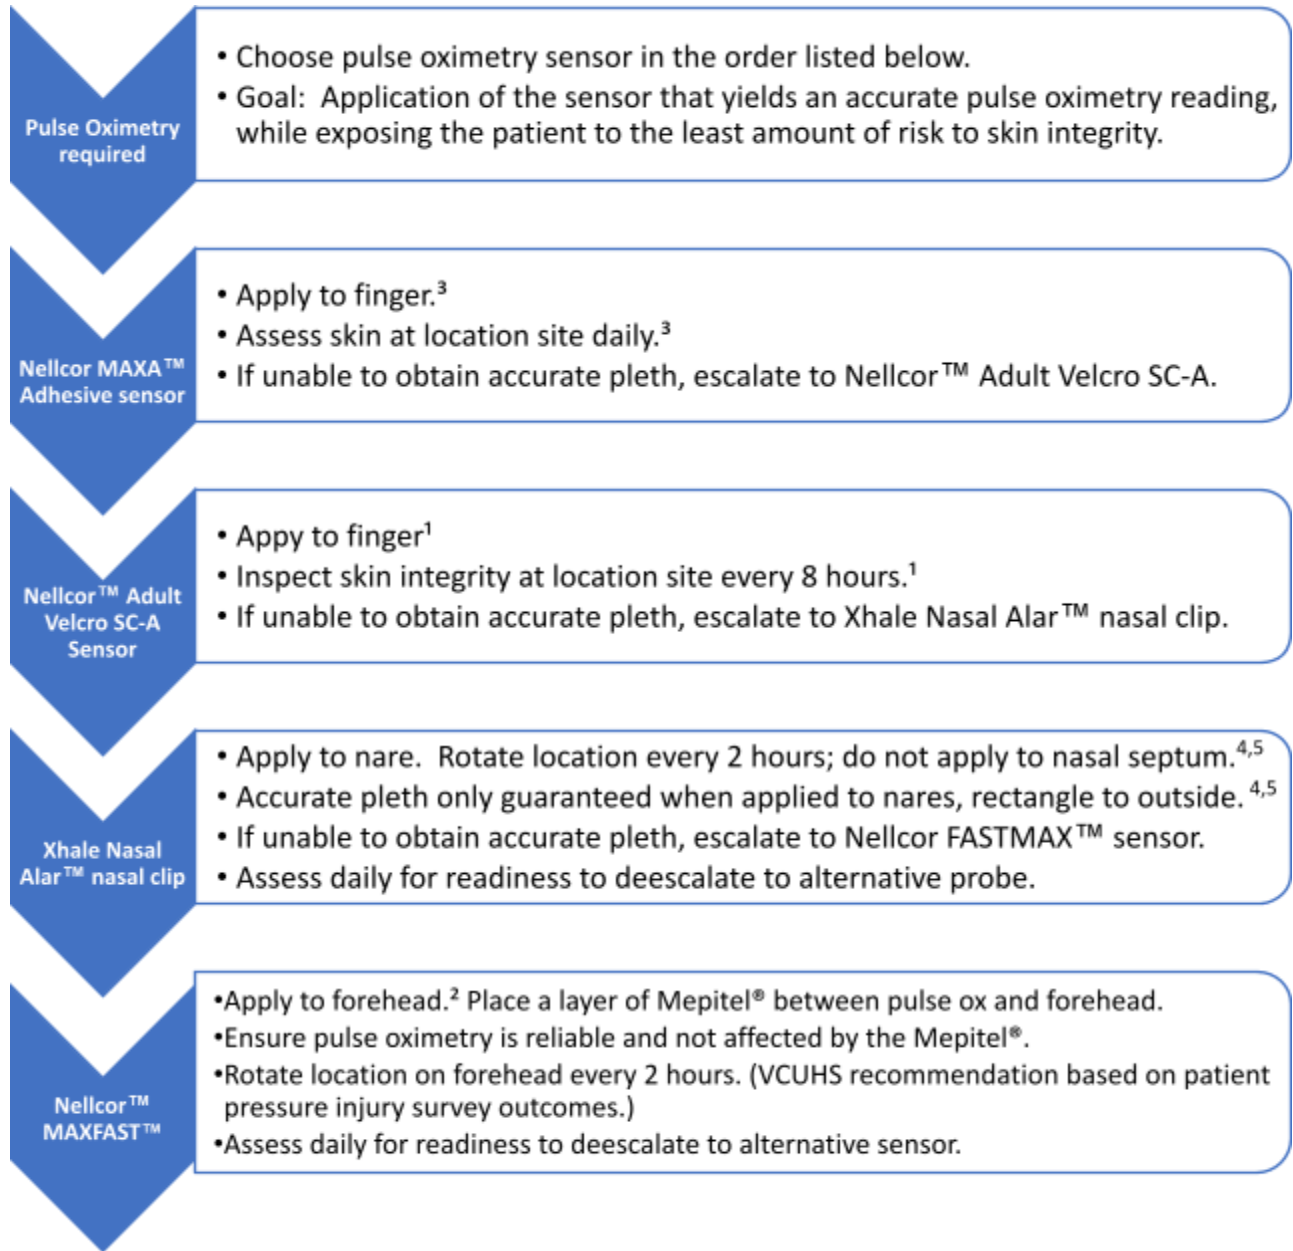

Nellcor MAXA™ Adhesive SpO2 Sensor	Nellcor™ Adult SC-A Velcro SpO2 Sensor	XHale Nasal Alar™ Clip SpO2 sensor	Nellcor MAXFAST™ Forehead SpO2 sensor
			

Pulse Oximetry Sensor Decision Tree

References:

¹Nellcor™ Adult SC-A Velcro Pulse Oximetry

http://www.medtronic.com/content/dam/covidien/library/global/multi/product/pulse-oximetry/Softcar eSensorAdult_Manual_Multi_10088256B00.pdf

²Nellcor MAXFAST™ Forehead SpO2 Sensor Instructions for Use Manual

http://www.medtronic.com/content/dam/covidien/library/global/multi/product/pulse-oximetry/MaxFas tSensor_Manual_Multi_10088259C00.pdf

³Nellcor MAXA™ Adhesive Pulse Oximetry Instructions for Use Manual

http://www.medtronic.com/content/dam/covidien/library/global/multi/product/pulse-oximetry/AdultO 2_Manual_Multi_10049951B00.pdf

⁴Xhale Nasal Alar SpO2™ Sensor Directions for Use

http://xhale.com/cms2014/wp-content/uploads/2018/02/10412_7-Alar-Sensor-Instructions-for-Use-Eng lish.pdf

⁵Xhale Alar Sensor™ Application & Rotate Guidelines

<http://xhale.com/cms2014/wp-content/uploads/2018/03/Alar-sensor-application-check-and-rotate-guid elines.pdf>