

1 **A microplate adaptation of the thiobarbituric acid reactive substances assay to determine lipid**
2 **peroxidation fluorometrically in small sample volumes**

3 Short version of title: **Miniaturization of the TBARS technique**

4 Espín S.^{1,2 a*}, Sánchez-Virosta P.^{1,2 a}, García-Fernández A.J.², Eeva T.¹

5 ¹*Department of Biology, University of Turku, 20014 Turku, Finland.*

6 ²*Area of Toxicology, Department of Health Sciences, University of Murcia, Campus de Espinardo,*
7 *30100 Murcia, Spain.*

8 **Note: S. Espín and P. Sánchez-Virosta have equal contribution to the article*

9 **Corresponding author: silvia.espin@um.es / +34868884317*

10 **Abstract**

11 A simple, fast, reproducible and low-cost assay for thiobarbituric acid reactive substances (TBARS)
12 has been adapted for use with a microplate spectrofluorometer. The technique allows rapid analysis
13 of multiple samples and requires a very small sample volume (50 µl of red cell homogenates from
14 passerine birds at protein concentrations of 3.4-8.9 mg/ml in this study), what is of special interest
15 for biomonitoring studies working with small-sized animals from which a limited amount of sample
16 can be obtained. The TBARS test involves the reaction of thiobarbituric acid (TBA) with
17 malondialdehyde (MDA) under heating (90°C), leading to the formation of products that can be
18 measured fluorometrically using black 384-well plates at excitation/emission wavelength of 532/553
19 nm. The concentrations of peroxidized lipids in samples were determined by extrapolation from a
20 MDA standard curve. Two different excitation/emission combinations (532/553 and 530/550 nm)
21 were used and both pairs were suitable for this technique. Intra- and inter-plate variability was < 20%

22 and a good linearity of the standard curve was observed ($R^2 > 0.99$). The research use of this
23 microplate adaptation of the TBARS assay will provide further data and understanding of lipid
24 peroxidation reducing the limitation of small sample volume.

25 **Resumen**

26 El presente trabajo adapta un ensayo sencillo, rápido, reproducible y económico de sustancias
27 reactivas al ácido tiobarbitúrico (TBARS) para su uso en espectrofluorómetro para microplacas. La
28 técnica permite un análisis rápido de múltiples muestras y requiere un mínimo volumen de muestra
29 (50 μ l de un homogeneizado de eritrocitos de aves paseriformes a una concentración proteica de 3.4-
30 8.9 mg/ml en este estudio), lo cual resulta de especial interés en estudios de biomonitorización que
31 trabajan con animales de pequeño tamaño de los que se puede obtener una cantidad de muestra
32 limitada. El ensayo TBARS consiste en la reacción del ácido tiobarbitúrico (TBA) con
33 malondialdehído (MDA) en condiciones de calor (90°C), formando productos que pueden medirse
34 fluorométricamente usando microplacas negras de 384 pocillos a 532/553 nm de excitación/emisión.
35 La concentración de peróxidos lipídicos en la muestra se determinó por extrapolación de una curva
36 de MDA. Se utilizaron dos combinaciones diferentes de excitación/emisión (532/553 and 530/550
37 nm) y ambas fueron apropiadas para la técnica. La variabilidad intra- e inter-placa fue $< 20\%$ y se
38 observó una buena linealidad de la curva estándar ($R^2 > 0.99$). El uso científico de la adaptación a
39 microplaca del ensayo TBARS proporcionará más datos y comprensión sobre la peroxidación lipídica
40 reduciendo la limitación que supone los pequeños volúmenes de muestra.

41 **Keywords:** lipid peroxidation; TBARS; malondialdehyde; oxidative stress; erythrocytes

42 **Palabras clave:** peroxidación lipídica; TBARS; malondialdehído; estrés oxidativo; eritrocitos

43 **1. Introduction**

44 Oxidative processes and the subsequent generation of free radicals are normal in the cellular
45 metabolism (Finkel and Holbrook, 2000). In response to this processes, organisms are equipped with
46 an antioxidant defense system able to inhibit the generation of reactive oxygen species (ROS) and
47 reduce the oxidation and the consequent cellular damage (McGraw, 2011). However, different
48 exogenous factors such as the exposure to environmental pollutants, radiation or infections can
49 deplete the major antioxidants of cells and induce ROS generation leading to oxidative stress
50 (imbalance between the antioxidant and pro-oxidant levels in favor of the latter; Halliwell and
51 Gutteridge, 2007), which may cause oxidative damage to membrane lipids (Ahmad, 1995; Schwarz,
52 1996; Bayoumi et al., 2001; Ercal et al., 2001; García-Fernández et al., 2002; Azzam et al., 2012).

53 Lipids are essential to maintain the structure of cell membranes and control the function of cells, and
54 they are the primary targets of the attack by ROS (Yin et al., 2011). The process in which oxidants
55 attack lipids containing carbon-carbon double bond(s), especially polyunsaturated fatty acids
56 (PUFAs), is called lipid peroxidation (Ayala et al., 2014). This process results in a wide variety of
57 oxidation products, the main primary products being the lipid hydroperoxides (LOOH), and two
58 secondary products extensively studied the aldehydes malondialdehyde (MDA) and 4-
59 hydroxynonenal (4-HNE) (see references in Ayala et al., 2014). Malondialdehyde and thiobarbituric
60 acid reactive substances (TBARS) have been widely used as standard biomarkers of lipid
61 peroxidation for many years because of its reaction with thiobarbituric acid (TBA) and its simplicity
62 and low cost (Ayala et al., 2014; Niki, 2014). The TBARS test involves the reaction of MDA with
63 TBA under acidic condition and heating, leading to the formation of pink-colored and fluorescent
64 products that can be measured by colorimetric and fluorometric methods. Although originally it was
65 accepted that the TBARS assay measured MDA, it is not exclusively measuring MDA, but also other
66 aldehydes and decomposition products from hydroperoxides. However, even though there remains a

67 controversy regarding the specificity of TBARS and artefactual production during analytical
68 processes, it still remains among the most popular and commonly applied assays to determine lipid
69 peroxidation (Niki, 2014).

70 In the field of toxicology, numerous studies have observed an increase in TBARS values as a
71 response to pollutant-related oxidative stress in different organisms (e.g. Howlett and Avery, 1997;
72 Oakes and Van Der Kraak, 2003; Stepić et al., 2012; Espín et al., 2014a; Osičková et al., 2014).
73 Particularly in avian ecotoxicology, the number of studies evaluating the effects of pollutants such as
74 metals on oxidative stress biomarkers (including TBARS) has significantly increased in the last years
75 (Mateo and Hoffman, 2001; Mateo et al., 2003; Koivula and Eeva, 2010; Martínez-Haro et al., 2011;
76 López-Antia et al., 2013; Espín et al., 2014a; 2014b; Ortiz-Santaliestra et al., 2015; Espín et al.,
77 2016a), and results suggest that TBARS is a convenient, simple and low-cost method that may
78 function as a useful biomarker of pollutant-induced lipid peroxidation in birds. When working with
79 wild species and particularly with small animals (e.g. passerine birds), only minimal volumes of
80 sample are available for the analysis of a battery of biomarkers. Therefore, adaptations of techniques
81 to minimize the sample volume are needed in order to be able to evaluate those biomarkers in a wide
82 range of species (Koivula et al., 2011; Espín et al., 2016b). The main aim of this study is to describe
83 a microplate TBARS assay to determine lipid peroxidation in small sample volumes using red blood
84 cells (RBC) from nestlings of a passerine bird species (great tit, *Parus major*). For this purpose, we
85 developed an adaptation of the TBARS technique described by Alonso-Álvarez et al. (2008)
86 following the technique by Aust (1985) with different modifications to minimize the sample volume
87 and by using fluorometry. The principle of the assay is based on the fact that different tissues contain
88 a mixture of TBARS, including lipid hydroperoxides and aldehydes, and their concentrations increase
89 due to oxidative stress (Alonso-Álvarez et al., 2008).

90 **2. Reagent preparation**

91 The sodium chloride (NaCl, 0.9%) was prepared by dissolving 0.9 g NaCl (27810.295, PROLABO,
92 VWR Chemicals™) in 100 ml milliQ-water. For TBARS reagent preparation (15% trichloroacetic
93 acid, TCA; 0.25 N hydrochloric acid, HCl; 0.375% 2-thiobarbituric acid, TBA), 7.5 g TCA
94 (1.00807.0100, EMSURE, Merck™), 0.1875 g TBA (T-5500, Sigma™) and 1.035 ml HCl (37%;
95 30721, Riedel-de Haën™) were dissolved in 50 ml milliQ-water. The butylated hydroxytoluene
96 (BHT, 2%) was prepared by dissolving 0.2 g BHT (B-1378, Sigma™) in 10 ml ethanol (99.5%,
97 ALTIA Oyj™). Finally, the stock malonaldehyde solution (MDA, 417 µM) for the standard curve
98 was prepared by dissolving 17.25µl MDA (malonaldehyde bis (dimethyl acetal) or 1,1,3,3-
99 Tetramethoxypropan 99%; 10,838-3, Aldrich™) in 250 ml ethanol. All the reagents were stored at
100 4°C.

101 **3. Method procedure**

102 **3.1. Sample collection**

103 This method is described for bird erythrocytes, but it can be applicable to other biological sample
104 types. Blood samples from great tit nestlings (14 days old) were collected during the breeding season
105 2015 in southwestern Finland. Blood samples (approximately 75 µl) were collected by venipuncture
106 of the brachial vein with a needle and using sodium-heparinized microhematocrit capillary tubes (80
107 iu/ml, Marienfeld™). Tubes were centrifuged in the field (4400 g, 5 min) and RBCs were split in
108 200-µl microcentrifuge tubes and kept in liquid nitrogen and then conserved at -80°C in the
109 laboratory. A total of 100 RBC samples were used in this study.

110 **3.2. *Sample and MDA standard curve preparation***

111 RBC were homogenized in 0.9% NaCl to maximize the volume and to get protein concentrations
112 between 3.4 and 8.9 mg/ml, working on ice to avoid oxidation. The protein concentration (mg/ml)
113 was measured using the Pierce™ BCA Protein Assay Kit from ThermoFisher Scientific, Waltham,
114 Massachusetts, USA. In brief, the BCA reaction mix is made according to the kit instructions (50:1,
115 BCA Reagent A:B). A serial dilution of bovine serum albumin (BSA, 10 mg/ml) is used as protein
116 standard. One μ l of each BSA standard dilution, control (salmon liver) or sample is pipetted in a
117 transparent 384-well plate in triplicate. Then, 50 μ l of BCA reaction mix are added to each well with
118 a multichannel pipette and briefly mixed using a plate shaker. Then the plate is incubated at 37 °C for
119 30 min. Finally, the protein concentration is measured spectrophotometrically at an absorbance of
120 562 nm.

121 Fifty μ l of each homogenate was split in a 1.5-ml microcentrifuge tube for TBARS assay, and
122 the remaining was divided into different microcentrifuge tubes for other oxidative stress
123 measurements. For 5 of the samples, 250 μ l of homogenate was divided in 5 tubes (50 μ l per tube) in
124 order to use them as controls in the different plates and evaluate the inter-assay precision. All
125 measurements (standards, controls and samples) were done in triplicate in each plate to evaluate the
126 intra-assay variability.

127 Seven standard dilutions of MDA (from 0 to 0.5 nmol/ml) were prepared using the stock MDA
128 solution (417 μ M) and milliQ-water according to the instructions provided in Table 1. Firstly, 100 μ l
129 from the stock MDA solution were dissolved in 900 μ l of milliQ-water to prepare solution C, 100 μ l
130 from solution C were dissolved in 900 μ l of milliQ-water to prepare solution B, and 149.9 μ l from
131 solution B were dissolved in 850.1 μ l of milliQ-water to prepare solution A. The standard point
132 number 7 was prepared by dissolving 800 μ l from solution A in 200 μ l of milliQ-water, the standard
133 point number 6 was prepared by dissolving 500 μ l from standard 7 in 500 μ l of milliQ-water, etc.,
134 following the process shown in Table 1.

135 [Table 1 near here]

136 3.3. *TBARS assay description*

137 This method is described to work in sets of 19 different unknown samples, 5 control samples and a
138 standard curve of 7 points. Therefore, 95 unknown samples were analyzed in 5 different assays, and
139 the other 5 unknown samples were used as control samples in all the assays. Several sets can be done
140 the same day, and a standard curve should always be included in each assay in order to calculate the
141 final MDA concentration.

142 Before starting the assay, a set of 1.5-ml microcentrifuge tubes containing 500 μ l of water is
143 prepared (31 tubes in total, one per standard point, sample and control). Tubes are labelled with the
144 standard number or sample identification code and a glass insert (with conical base and plastic bottom
145 spring, 6 x 29 mm) is introduced inside each tube (the water will facilitate the heat transfer to the
146 sample that will be inside the glass insert). The standard curve and a 1:100 mix of BHT 2% and
147 TBARS reagent (a mix of 40 μ l BHT and 4 ml TBARS reagent will be needed for each set of 19
148 samples, 5 controls and the standard curve) are prepared daily. All reagents except samples, controls
149 and standards must be equilibrated to room temperature before beginning the assay.

150 A diagram summarizing the assay protocol is shown in Figure 1.

151 [Figure 1 near here]

152 The tubes with 50 μ l of the RBC homogenates and 7 tubes with 50 μ l of each standard point
153 are kept on ice and mixed with 100 μ l of the mix TBARS reagent plus BHT. The whole mix is
154 transferred to glass inserts kept inside appropriately labelled 1.5-ml microcentrifuge tubes with 500
155 μ l of water, and then warmed for 30 min at 90°C in a thermoblock. During the incubation in the
156 thermoblock, keep the microcentrifuge tubes open and place stainless steel balls (6 mm) covering all
157 the glass inserts. The steel balls prevent the sample evaporation but allow the escape of excess gas.
158 After the incubation, the steel balls are removed, the tubes are closed carefully with the inserts inside,

159 and the samples are cooled in ice-water for 10 min to stop the reaction. The tubes are centrifuged for
160 15 min at 6°C and 2100 g. Subsequently, the 7 standard points, samples and controls are pipetted in
161 the microplate in triplicate (a total of 93 wells are used). A volume of 30 µl of supernatant in triplicate
162 (30 µl per well) is pipetted in black 384-well plates (OptiPlate, PerkinElmer), keeping the plate on
163 ice while pipetting. There is no specific pattern for using the wells on the microplate and it is not
164 necessary to use all the wells on the microplate at one time. Supernatant has to be taken with caution
165 while pipetting it in the microplate to avoid the pellet-supernatant mixture after centrifugation. Glass
166 inserts with conical base and plastic bottom spring (6 x 29 mm) are recommended since the conical
167 base will help to keep the pellet at the bottom of the insert after centrifugation. Some trials were done
168 using glass inserts with flat base and there were pellet-supernatant mixture problems. It is also
169 possible to filter the sample before pipetting. However, part of the sample can be lost during this
170 process and it should be done carefully in order to have enough volume for the triplicates (90 µl in
171 total).

172 Finally, the fluorescence intensity (FI) is measured at an excitation/emission wavelength of
173 532/553 and 530/550 nm with the microplate spectrofluorometer (EnSpire 2300 Multilabel Reader,
174 PerkinElmer™).

175 **3.4. Calculations**

176 After calculating the mean fluorescence for triplicate measurements of each standard, control and
177 sample, the coefficient of variability (CV) for triplicates is determined as follows (equation 1):

$$178 \quad \text{CV (\%)} = (\text{SD}/\text{M}) \times 100 \quad (1)$$

179 where SD is the standard deviation and M is the arithmetic mean value for the repeated measurements.
180 If a high dispersion of triplicates is observed (CV values > 20%), this may be due to pipetting errors
181 or presence of bubbles in the well. A meticulous pipetting is recommended to prevent sample splash

182 from the wells and the plate can be carefully tapped with the fingers to remove bubbles before the FI
183 measurement.

184 The fluorescence values of each standard are plotted as a function of the MDA concentration
185 by linear regression analysis [$y = (\text{slope})x + y\text{-intercept}$]. The concentrations of peroxidized lipids in
186 samples and controls are determined by extrapolation from the MDA standard curve from each assay.
187 This way, we will obtain the nmol of MDA per ml of homogenate (equation 2).

$$188 \quad \text{MDA (nmol/ml homogenate)} = [(\text{FI} - y\text{-intercept}) / \text{slope}] \quad (2)$$

189 If MDA is not detected in the samples, this may be due to a low MDA concentration or the
190 sample being too diluted, thus a lower RBC dilution in order to have a more concentrated homogenate
191 may help to detect MDA.

192 As explained before, the total protein concentrations were analyzed in the same homogenates
193 and were expressed as mg per ml of homogenate. The final MDA concentration can be expressed in
194 relation to the mg of protein in RBC homogenates (nmol of MDA per mg of protein). Alternatively,
195 the final MDA concentration can be expressed in relation to the amount or volume of the original
196 tissue (e.g. nmol of MDA per mg of RBC, nmol of MDA per ml of blood). In this case, the sample
197 values must be corrected for any dilutions performed during sample preparation, and the original
198 sample amount/volume must be recorded.

199 **4. Fluorescence measurement (excitation and emission wavelengths)**

200 In fluorometric determination of TBARS, discrepant data for excitation and emission wavelengths
201 have been reported in literature (Yin, 1995). Although TBARS assay can be measured by colorimetric
202 methods (absorbance at 535 nm), higher volumes of sample are needed to obtain reliable data.
203 However, fluorometric assays may be more sensitive and, therefore, more suitable for small amount
204 of sample and samples containing low lipid peroxidation products (Yagi, 1976; Jo and Ahn, 1998).

205 According to Yagi (1976), the excitation/emission maxima of the MDA-TBA reaction product were
206 observed at 532/553 nm, while Yin (1995) found an excitation/emission maxima of the MDA-TBA
207 product at 536/549 nm. The latter recommends excitation/emission wavelengths as close as possible
208 to these values in order to obtain the greatest sensitivity.

209 In the present study, the fluorescence excitation/emission spectrum was studied on a
210 microplate spectrofluorometer (EnSpire 2300 Multilabel Reader, PerkinElmer™) by scanning
211 wavelengths of an excitation light while a wavelength in the emission detector was fixed and vice
212 versa, and the highest fluorescence intensity was observed at an excitation wavelength of 530-535
213 nm and an emission wavelength of 550-555 nm. Therefore, the fluorometric measurement at
214 excitation/emission wavelengths of 532/553 nm reported by Yagi (1976) was used. This was possible
215 because of the ability of our instrument to select any specific wavelength; however, some instruments
216 do not have this flexibility. Therefore, all the plates were also measured at 530/550 nm according to
217 other methods described in the literature. The excitation/emission wavelength of 536/549 nm could
218 not be tested since a minimum distance of 20 nm between excitation and emission wavelengths is
219 needed in our instrument. Figure 2 shows the mean standard curves plotting fluorescence and MDA
220 concentration (nmol/ml) obtained at 532/553 nm and 530/550 nm. Measurements at
221 excitation/emission wavelengths of 532/553 nm and 530/550 nm provided very similar intra- and
222 inter-assay CV and fluorescence intensity for control samples and standards, and the linearity of the
223 standard curve showed R^2 values > 0.99 (Table 2), thus both excitation/emission pairs seem to be
224 suitable for this technique.

225 [Table 2 near here]

226 [Figure 2 near here]

227 **5. Method validation**

228 The precision of an assay can be described using repeatability and reproducibility tests. Repeatability

229 is used to prove the ability to provide similar results when the measurement is repeated in the same
230 sample under the same operating conditions and by the same operator. It is also called intra-assay
231 precision. Reproducibility expresses the ability to provide similar results when the technique is
232 repeated in the same sample but by different operators or different laboratories. The effect of random
233 events on the precision of the assay can be also tested, and a typical variation to be studied is the
234 inter-assay precision in different days. The precision of the analytical procedure is usually expressed
235 as the CV of a series of measurements. Repeatability and reproducibility acceptance criterion was set
236 at $CV \leq 20\%$. To validate the repeatability and reproducibility of the method, standards, samples and
237 aliquots of a subset of 5 different samples (control samples) were analyzed in the 5 assays developed
238 by 2 different researchers (S.E. and P.S-V.) in 2 different days. All measurements (standards, samples
239 and controls) in each plate were done in triplicates to evaluate the intra-assay precision, reflecting the
240 variability among triplicate determinations within the same assay run. The intra-assay CV was $< 10\%$
241 for the 100 samples/controls and the standards analyzed. The inter-assay variation when comparing
242 assays done at different days was $< 20\%$ for both the standard curve and the control samples, and the
243 variation when the standards and control samples were analyzed by different researchers was $< 10\%$
244 (Table 2). These results indicate that the method can be considered acceptable for the analysis of
245 TBARS.

246 The linearity of the standard curve is evaluated to determine the proportionality between the
247 concentration of MDA in the standard points and the FI. In the present study, the linearity was
248 calculated using 7 different standard points (from 0 to 0.5 nmol MDA/ml, Table 1). Each standard
249 point was analyzed in triplicate and a different standard curve was analyzed in each assay. Linear
250 regression of data to a calibration curve was performed, and the linearity was accepted when $R^2 >$
251 0.95. A good linearity was found in all the assays, since R^2 was above 0.99 (Table 2).

252 **6. Conclusions**

253 The microplate assay herein described is a simple, fast, reproducible and economical fluorometric
254 method for TBARS determination in small sample volumes. Only 50 µl of diluted RBC homogenates
255 are needed, what is of special interest for biomonitoring studies working with animals of small size
256 from which a limited amount of sample can be obtained non-destructively. In addition, multiple
257 samples may be analyzed simultaneously. This TBARS microplate assay format may be easily
258 adapted to measure TBARS in different sample types and species using the appropriate concentrations
259 in the standard curve. The research use of this microplate adaptation of the TBARS assay will provide
260 further data and understanding of lipid peroxidation in different organisms reducing the limitation of
261 small sample volumes.

262

263 **Acknowledgments**

264 This work was supported by the Academy of Finland under project 265859 to T. Eeva and by Séneca
265 Foundation (CARM) under MASCA'2014 Project (19481/PI/14) to A.J. García-Fernández. S. Espín
266 is financially supported by the Academy of Finland and by the *Consejería de Educación y*
267 *Universidades de la CARM* through *Fundación Séneca-Agencia de Ciencia y Tecnología de la Región*
268 *de Murcia* (Project 20031/SF/16 to S. Espín). P. Sánchez-Virosta is funded by the University of Turku
269 Graduate School – UTUGS. Thanks to M.P. Aldeguer and A. Salas for their help during the first trials
270 of the technique, M. Kanerva for her help with the fluorometric measurements, and S. Ruiz, L.
271 Winder, M. Rainio, and J. Nurmi for their help during sample collection. Special thanks to R. Mateo,
272 M.E. Ortiz-Santaliestra and M. Martínez-Haro for their collaboration in teaching the original
273 technique for higher sample volumes.

274 **Declaration of interest statement**

275 The authors declare that they have no conflict of interest.

276 **References**

- 277 Ahmad S. Oxidative Stress from Environmental Pollutants. *Arch. Insect Biochem. Physiol.* 1995; 29
278 (2), 135–157.
- 279 Alonso-Álvarez C, Pérez-Rodríguez L, Mateo R, Chastel O, Viñuela J. The Oxidation Handicap
280 Hypothesis and the Carotenoid Allocation Trade-Off. *J. Evol. Biol.* 2008; 21 (6), 1789–1797.
- 281 Aust SD. Lipid peroxidation. *Handbook of Methods for Oxygen Radical Research.* R.A. Greenwald.
282 CRC Press, Boca Raton, FL. 1985. p. 203–207.
- 283 Ayala A, Muñoz MF, Argüelles S. Lipid Peroxidation: Production, Metabolism, and Signaling
284 Mechanisms of Malondialdehyde and 4-Hydroxy-2-Nonenal. *Oxid. Med. Cell. Longev.* 2014.
285 e360438.
- 286 Azzam EI, Jay-Gerin J-P, Pain D. Ionizing radiation-induced metabolic oxidative stress and
287 prolonged cell injury. *Cancer. Lett.* 2012; 327, 48–60.
- 288 Bayoumi AE, García-Fernández AJ, Ordóñez C, Pérez-Pertejo Y, Cubría JC, Reguera RM, Balaña-
289 Fouce R, Ordóñez D. Cyclodiene Organochlorine Insecticide-Induced Alterations in the
290 Sulfur-Redox Cycle in CHO-K1 Cells. *Comp. Biochem. Physiol. C.* 2001; 130, 315–323.
- 291 Ercal N, Gurer-Orhan H, Aykin-Burns N. Toxic Metals and Oxidative Stress Part I: Mechanisms
292 Involved in Metal-Induced Oxidative Damage. *Curr. Top. Med. Chem.* 2001; 1 (6), 529–539.
- 293 Espín S, Martínez-López E, Jiménez P, María-Mojica P, García-Fernández AJ. Effects of Heavy
294 Metals on Biomarkers for Oxidative Stress in Griffon Vulture (*Gyps Fulvus*). *Environ. Res.*
295 2014a; 129, 59–68.
- 296 Espín S, Martínez-López E, Jiménez P, María-Mojica P, García-Fernández AJ. Interspecific
297 Differences in the Antioxidant Capacity of Two Laridae Species Exposed to Metals. *Environ.*
298 *Res.* 2016a; 147, 115–124.

299 Espín S, Martínez-López E, León-Ortega M, Martínez JE, García-Fernández AJ. Oxidative Stress
300 Biomarkers in Eurasian Eagle Owls (*Bubo Bubo*) in Three Different Scenarios of Heavy Metal
301 Exposure. *Environ. Res.* 2014b; 131, 134–144.

302 Espín S, Ruiz S, Sánchez-Virosta P, Eeva T. Effects of Calcium Supplementation on Growth and
303 Biochemistry in Two Passerine Species Breeding in a Ca-Poor and Metal-Polluted Area.
304 *Environ. Sci. Pollut. Res.* 2016b; 23, 9809-9821.

305 Finkel T, Holbrook N.J. Oxidants, Oxidative Stress and the Biology of Ageing. *Nature* 2000; 408
306 (6809), 239–247.

307 García-Fernández AJ, Bayoumi AE, Pérez-Pertejo Y, Romero D, Ordóñez C, Reguera RM, Balaña-
308 Fouce R, Ordóñez D. Changes in Glutathione-Redox Balance Induced by
309 Hexachlorocyclohexane and Lindane in CHO-K1 Cells. *Xenobiotica* 2002; 32, 1007–1016.

310 Halliwell B, Gutteridge J. *Free Radicals in Biology and Medicine*. 4th ed. Oxford University Press,
311 USA. 2007.

312 Howlett NG, Avery SV. Induction of Lipid Peroxidation during Heavy Metal Stress in
313 *Saccharomyces Cerevisiae* and Influence of Plasma Membrane Fatty Acid Unsaturation.
314 *Appl. Environ. Microbiol.* 1997; 63 (8), 2971–2976.

315 Jo C, Ahn DU. Fluorometric Analysis of 2-Thiobarbituric Acid Reactive Substances in Turkey. *Poult.*
316 *Sci.* 1998; 77 (3), 475–480.

317 Koivula MJ, Eeva T. Metal-Related Oxidative Stress in Birds. *Environ. Pollut.* 2010; 158 (7), 2359–
318 2370.

319 Koivula MJ, Kanerva M, Salminen J-P, Nikinmaa M, Eeva T. Metal Pollution Indirectly Increases
320 Oxidative Stress in Great Tit (*Parus Major*) Nestlings. *Environ. Res.* 2011; 111 (3), 362–370.

321 López-Antia A., Ortiz-Santaliestra ME, Mougeot F, Mateo R. Experimental Exposure of Red-Legged
322 Partridges (*Alectoris Rufa*) to Seeds Coated with Imidacloprid, Thiram and Difenoconazole.
323 *Ecotoxicology* 2013; 22 (1), 125–138.

324 Martínez-Haro M, Green AJ, Mateo R. Effects of Lead Exposure on Oxidative Stress Biomarkers and
325 Plasma Biochemistry in Waterbirds in the Field. *Environ. Res.* 2011; 111 (4), 530–538.

326 Mateo R, Hoffman DJ. Differences in Oxidative Stress between Young Canada Geese and Mallards
327 Exposed to Lead-Contaminated Sediment. *J. Toxicol. Environ. Health. A.* 2001; 64 (7), 531–
328 545.

329 Mateo R, Beyer WN, Spann JW, Hoffman DJ, Ramis A. Relationship between Oxidative Stress,
330 Pathology, and Behavioral Signs of Lead Poisoning in Mallards. *J. Toxicol. Environ. Health.*
331 *A.* 2003; 66 (14), 1371–1389.

332 McGraw KJ. Avian Antioxidants and Oxidative Stress: Highlights from Studies of Food, Physiology,
333 and Feathers. In Mandelker L, Vajdovich P (Eds.), *Studies on Veterinary Medicine*. 2011. p.
334 161–174.

335 Niki E. Biomarkers of Lipid Peroxidation in Clinical Material. *Biochim. Biophys. Acta BBA – Gen.*
336 *Subj.* 2014; 1840 (2), 809–817.

337 Oakes KD, Van Der Kraak GJ. Utility of the TBARS Assay in Detecting Oxidative Stress in White
338 Sucker (*Catostomus Commersoni*) Populations Exposed to Pulp Mill Effluent. *Aquat.*
339 *Toxicol.* 2003; 63 (4), 447–463.

340 Ortiz-Santaliestra ME, Resano-Mayor J, Hernández-Matías A, Rodríguez-Estival J, Camarero PR,
341 Moleón M, Real J, Mateo R. Pollutant Accumulation Patterns in Nestlings of an Avian Top
342 Predator: Biochemical and Metabolic Effects. *Sci. Total. Environ.* 2015; 538, 692–702.

343 Osičková J, Band'ouchová H, Kováčová V, Král J, Novotný L, Ondráček K, Pohanka M, et al.
344 Oxidative Stress and Liver Damage in Birds Exposed to Diclofenac and Lead. *Acta. Vet.*
345 *Brno.* 2014; 83 (4), 299–304.

346 Schwarz KB. Oxidative Stress during Viral Infection: A Review. *Free. Radic. Biol. Med.* 1996; 21
347 (5), 641–649.

- 348 Stepić S, Hackenberger BK, Hackenberger DK, Velki M, Lončarić Ž. Impact of Oxidative Stress
349 Indicated by Thiobarbituric Acid Reactive Substances (TBARS) and Protein Carbonyl Levels
350 (PC) on Ethoxyresorufin-O-Deethylase (EROD) Induction in Common Carp (*Cyprinus*
351 *Carpio*). *Water. Air. Soil. Pollut.* 2012; 223 (8), 4785–4793.
- 352 Yagi K. A Simple Fluorometric Assay for Lipoperoxide in Blood Plasma. *Biochem. Med.* 1976; 15
353 (2), 212–216.
- 354 Yin D. Appropriate Excitation/emission Wavelengths for Fluorometric Determination of
355 Thiobarbituric Acid-Reactive Substances. *Clin. Chem.* 1995; 41 (2), 329–330.
- 356 Yin H, Xu L, Porter NA. Free Radical Lipid Peroxidation: Mechanisms and Analysis. *Chem. Rev.*
357 2011; 111 (10), 5944–5972.

Table 1. Standard curve preparation (7 points) for a microplate adaptation of the TBARS assay

MDA concentration (nmol/ml)	0	0.03125	0.0625	0.09375	0.125	0.25	0.5	0.625	4.17	41.7	417
Standard number	1	2	3	4	5	6	7	A	B	C	Stock
MilliQ-water (μl)	1000	500	500	977.52	500	500	200	850.1	900	900	
MDA (μl)	0	500	500	22,48	500	500	800	149.9	100	100 from	
		from 3	from 5	from B	from 6	from 7	from A	from B	from C	Stock	

358 MDA: malondialdehyde
 359 Table reading: 100 μl from the stock MDA solution were dissolved in 900 μl of milliQ-water to prepare solution C, 100 μl from
 360 solution C were dissolved in 900 μl of milliQ-water to prepare solution B, and 149.9 μl from solution B were dissolved in 850.1 μl of
 361 milliQ-water to prepare solution A. The standard points (1-7) were prepared by dissolving X μl from solution X in X μl of milliQ-
 362 water as shown in the table.

Table 2. Validation parameters (i.e. intra/inter-assay coefficient of variability and linearity of the standard curve) for a microplate adaptation of the TBARS assay

Excitation/emission wavelength	Sample type	Intra-assay CV (%) ^a	Inter-assay CV (% global) ^b	Inter-assay CV (% different days) ^c	Inter-assay CV (% different researchers) ^d	Linearity (R ²) ^e
532/553 nm	Control	2.73 (1.78-4.02)	15.95 (11.66-19.36)	14.38 (13.34-16.05)	5.89 (1.67-8.59)	-
	Standard curve	4.13 (2.70-5.35)	12.03 (3.34-27.03)	4.85 (0.53-16.19)	8.40 (0.76-26.00)	0.995 (0.991-0.999)
530/550 nm	Control	2.66 (1.86-3.15)	15.38 (10.94-20.24)	13.99 (10.80-17.04)	4.98 (0.55-7.99)	-
	Standard curve	4.13 (3.29-5.44)	11.03 (1.31-22.51)	3.87 (0.06-15.04)	7.30 (0.72-21.65)	0.994 (0.991-0.998)

^a Intra-assay precision reflects variability among triplicates within the same assay run (same microplate) (mean, min and max CV for 5 control samples or 7 standard points in the 5 plates)

^b Inter-assay precision (global) reflects variability among microplates for the same sample/standard (mean, min and max CV for 5 control samples or 7 standard points)


^c Inter-assay precision (different days) reflects variability with time (mean, min and max CV for 5 control samples or 7 standard points)

^d Inter-assay precision (different researchers) reflects variability among researchers (mean, min and max CV for 5 control samples or 7 standard points)


^e Linearity calculated using 7 different standard points from 0 to 0.5 nmol MDA/ml (mean, min and max R² for 5 standard curves)

364 **Legends of figures**

365 Figure 1. Diagram summarizing the microplate TBARS assay protocol.

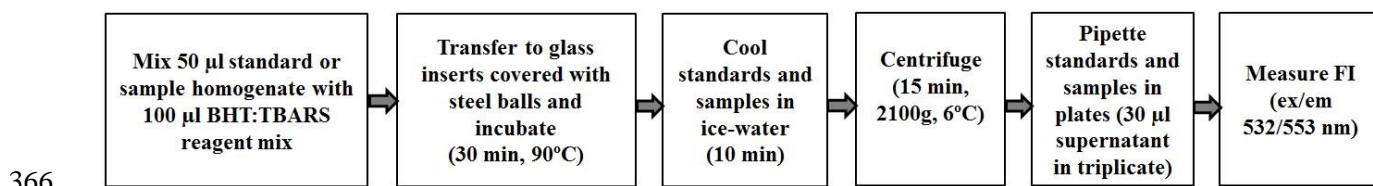

367 Figure 2. Standard curves plotting fluorescence intensity (FI) and MDA concentration (nmol/ml) at
368 532/553 nm and 530/550 nm of excitation/emission wavelengths. Each standard point corresponds to
369 the mean value \pm SD of 5 different curves (in each curve all the standard points were measured in
370 triplicate).

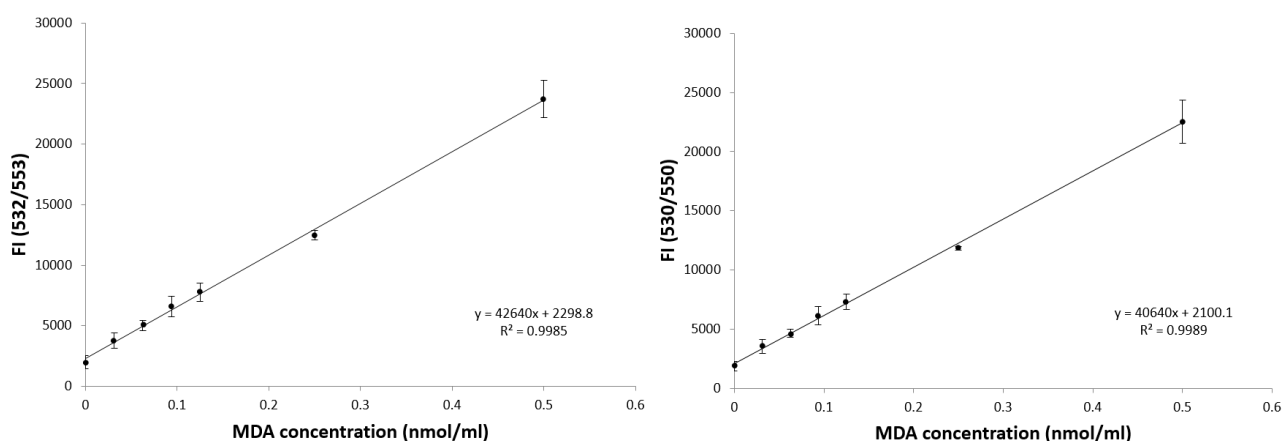

371