



**Manchester
Metropolitan
University**

Garcia-Miranda Ferrari, A ORCID logoORCID: <https://orcid.org/0000-0003-1797-1519>, Crapnell, RD, Adarakatti, PS, Suma, BP and Banks, CE (2022) Electroanalytical overview: The detection of chromium. *Sensors and Actuators Reports*, 4. p. 100116.

Downloaded from: <https://e-space.mmu.ac.uk/630839/>

Version: Published Version

Publisher: Elsevier

DOI: <https://doi.org/10.1016/j.snr.2022.100116>

Usage rights: Creative Commons: Attribution-Noncommercial-No Derivative Works 4.0

Please cite the published version

<https://e-space.mmu.ac.uk>



Electroanalytical overview: The detection of chromium

Alejandro Garcia-Miranda Ferrari ^a, Robert D. Crapnell ^a, Prashanth S. Adarakatti ^{a,b}, B P Suma ^c,
Craig E. Banks ^{a,*}

^a Faculty of Science and Engineering, Manchester Metropolitan University, Chester Street, Manchester M1 5GD, UK

^b Department of Chemistry, SVM Arts, Science and Commerce College, Ilkal 587125, India

^c Department of Chemistry, Central College, Bangalore University, Bengaluru 560001, India

ARTICLE INFO

Keywords:

Chromium (Cr(III), Cr(VI))
Electroanalytical
Sensing
Electroanalysis
Sensor
Electrochemistry
Screen-printed electrode (SPE)

ABSTRACT

Chromium exerts serious damage to human beings and to aquatic life and is one of the most common environmental contaminant and possess toxicity when present above threshold limits. In comparison with the traditional quantification methods such as atomic absorption spectroscopy (AAS), inductively coupled plasma mass spectrometry, UV-Vis or high-performance liquid chromatography, electrochemical methods towards monitoring chromium ions have the advantages of being portable, rapid, cost effective, simple, sensitive and selective enough to meet regulatory limits. This review presents the recent progress in the field of electroanalysis using different electrode platforms such as solid or screen-printed electrode (SPE) and various functional materials towards chromium determination. The fabrication strategy and the analytical performance of carbon nanomaterials (such as carbon nanotubes and graphene), metal and metal oxide nanomaterials enabled sensors for electrochemical determination of chromium (III) and chromium (VI) ions are summarized systematically. In addition, method validation and the application of these sensors in real samples for the analysis of chromium ions is discussed and future developments in this domain are provided.

1. Introduction

Chromium (Cr) is a d-block transition metal that can exist in various oxidation states, ranging from (0) up to (+6). Despite this plethora of oxidation states, it is predominantly only the trivalent (+3) and hexavalent (+6) forms of chromium that are stable enough to be routinely found in the environment [1]. The physiological effect on human life that these two species have could not be more different. Chromium (III) is classed as an essential micronutrient for living organisms, with the UK's National Health Service recommending approximately 25 mg per day for adults [2]. Additionally, studies have shown reduced risk of type 2 diabetes for adults taking chromium containing supplements [3]. On the other hand, chromium (VI) is highly toxic [4] and classed as group 1 carcinogen [5]. It has been shown to penetrate cell walls, followed by a reduction to chromium (III), forming reactive oxygen species (ROS) as a by-product. This process exerts an oxidative potential on the cell, leading to inhibition of the metallo-enzyme system [5,6]. As such, in 2003 the World Health Organisation (WHO) set a guideline value for chromium within drinking water at 50 µg/L, which has been upheld as valid in 2020 [7]. The presence of Cr in the environment is attributed to the

rapid industrialization of cities and urban areas due to chromium's wide usage in a variety of industrial advancements such as electroplating, tanning of leather, in wood polishing and preservation and use as a pigment in the manufacturing of artificial gems and jewels. The effluent released from these metal plating industries further adds up to the increased content of chromium in biosystems. Due to the potential consequences of ingestion, and varied exposure limits set out by different countries worldwide [8], monitoring of the concentration levels of Cr (VI) present in natural waters is vital for global human health. Due to the critical health implications of Cr (VI), the majority of work found throughout the literature is aimed toward detecting and quantifying the presence of this species.

In this review we focus on the electrochemical approaches for the detection of chromium using various modified electrodes. We highlight detection strategies for Cr(III) and Cr(VI) species from various sample matrices and recent advances in fabrication of diverse modified electrodes towards chromium sensing are discussed.

* Corresponding author.

E-mail address: c.banks@mmu.ac.uk (C.E. Banks).

<https://doi.org/10.1016/j.snr.2022.100116>

Received 19 February 2022; Received in revised form 23 July 2022; Accepted 26 July 2022

Available online 28 July 2022

2666-0539/© 2022 The Author(s). Published by Elsevier B.V. This is an open access article under the CC BY-NC-ND license (<http://creativecommons.org/licenses/by-nc-nd/4.0/>).

2. Detection of chromium

Work on the identification of chromium using diphenylcarbazide can be traced back to the early 1900's where Brandt [9] took the earlier observations from Cazeneuve [10] and used the violet to green colour change as an indicator for the end-point of the bichromate iron titration. This turned out to have significantly greater sensitivity compared to other methods at the time such as the ether-hydrogen peroxide method [11]. Diphenylcarbazide has been utilised for the detection of chromium ions ever since in conjunction with various methodologies, such as spot tests [12] and solid-phase spectrophotometry [13]. The latter is an example of conventional laboratory-based analytical methodologies commonly used for chromium detection, among many other analytes, throughout the world. Numerous analytical techniques considered as fundamental analytical methods are accessible for analysing chromium in variety of samples such as high performance liquid chromatography (HPLC) [14], capillary electrophoresis, capillary chromatography, atomic adsorption spectrophotometry (AAS), inductively coupled plasma mass spectrometry (ICP-MS), spectro-fluorimetry, spectrophotometry and chemiluminescence (CL) [15–17].




To enhance detection capabilities, the combination of two or more analytical techniques has been utilised in various sectors aimed at speciation and trace element analysis [18]. These conventional hyphenated techniques are powerful tools in solving various problems encountered in qualitative and quantitative elemental analysis and offer an attractive method to investigate oxidation and reduction processes. In this regard, Spanu et al. proposed a highly selective method by coupling frontal chromatography (FC) with Inductively Coupled Plasma – Mass Spectrometry (ICP-MS) for the fast determination of Cr(VI) ultra-traces in a minute. However, a common disadvantage of ICP-MS methods is the requirement of acidifying the sample prior Cr(VI) measurement [19]. Pechancová et al. proposed the foremost study which focusses on soluble Cr(III), total Cr(VI) and total bound Cr species in living tissues. Herein alkaline EDTA extraction was followed by their separation using ion-exchange high-performance liquid chromatography inductively coupled plasma mass spectrometry (IE-HPLC-ICP-MS) was used towards the determination of total Cr(VI) and soluble Cr(III) species [20]. Monika et al. reported the use of hyphenation for elemental speciation analysis of mixture of metals such as arsenite – As(III), arsenate – As(V) and hexavalent chromium – Cr(VI) in water using high performance liquid chromatography inductively coupled plasma mass spectrometry (HPLC/ICP-MS). The method was successfully applied to real water samples with limit of detection (LODs) below the ppb levels [21]. Zou and co-workers developed a method for the non-chromatographic speciation of Cr(VI) and Cr(III) and selective determination of Cr(VI) which involves chemical vapor generation (CVG) in KBH_4 -acid system for introduction sample into an inductively coupled plasma mass spectrometer (ICP-MS) for Cr(VI) detection. Non-chromatographic speciation analysis of Cr(III) and Cr(VI) can be achieved via the oxidation of Cr(III) to Cr(VI) supported by KMnO_4 . The CVG of Cr(VI), rather than Cr(III), was reported to be enhanced in the presence of sodium diethylaminodithioformate. Under optimal conditions, the LOD of Cr(VI) was found to be 0.2 ng/mL and their method was successfully applied to the determination of Cr(VI) in real water samples [22]. Saraiva et al. reported a new analytical approach for the real-time speciation analysis of both Cr(III) and Cr(VI) by coupling high-performance liquid chromatography (HPLC) to inductively coupled plasma mass spectrometry (ICP-MS) and double spike species specific-isotope dilution (SS-ID) [23]. The selective extraction was achieved by sequential complexation of Cr(III) with ethylenediamine tetraacetic acid (EDTA) and of Cr(VI) with 1,5-diphenylcarbazide (DPC) in the same analytical run. The quantification limit was 0.013 $\mu\text{g}/\text{kg}$ for Cr(III) and 0.049 $\mu\text{g}/\text{kg}$ for Cr(VI), respectively. The authors concluded that the developed method is a powerful analytical tool for precise and specific quantification of Cr(III) and Cr(VI) at trace levels. The method was successfully applied to the analysis of meat and dairy products such

as baby and semi-skimmed milk and steak beef samples.

Electrochemical techniques have also been used in hyphenated setups as the detection methodology, commonly alongside HPLC. [24] In 1982 Bond [25] reported the simultaneous detection of Cu, Ni, Co, Cr (III) and Cr (VI) using HPLC to separate metal dithiocarbamate complexes, followed by well-defined oxidations to detect below nanogram levels for the target metal ions. However, these methods are time consuming, require sample pretreatment prior to analysis, experienced experimentalists, are highly sophisticated and require expensive equipment maintenance. Environmental monitoring of Cr (VI) is one of the most pressing reasons for the development of suitable analytical techniques. The majority of environmental contamination for industrial applications will be in water sources, without easy access to the laboratory setting required to use these analytical techniques. Hence the drive for the development of rapid, portable, low-cost, simple to use sensing platforms that be performed on-site to obtain immediate results; electrochemical sensors can meet these specific criteria and that is where our focus of this review turns to.




3. Electrochemistry of chromium (III) and (VI)

When designing electrochemical sensing platforms, it is important for researchers to consider the different species that could be present and stable at their specific conditions. This can be obtained by consulting the Pourbaix diagrams specific for that element, in this case chromium as shown in Fig. 1. Pourbaix diagrams plot the potential (E) against the pH of the solution for a certain temperature and indicate the thermodynamically stable phases that are possible in an aqueous electrochemical system. The lines forming boundaries between species represent the 50/50 boundaries, where the two species will be in equilibrium. The electrochemical oxidation of Cr(III) has been studied at platinum [26], metal oxide electrode [27], glassy carbon electrode (GCE), boron-doped diamond electrode (BDDE) and gold electrodes [28]. In this latter study combining GCE, BDDE and gold (Au) electrodes, it was seen that trivalent Cr was electroactive in only very alkaline media ($\text{pH} > 12$) at an Au electrode surface, due to the formation of an oxide film. The oxidation occurs through a multi-step mechanism, where the first step is an electrochemically irreversible electron transfer and is rate determining. The full mechanism was proposed to be:



where RDS is “rate-determining step”, the second and third steps represent two fast electron transfer steps or disproportionation steps. Key to the rate determining step is the transfer of a hydroxide anion, highlighted by the fact that at a KOH supporting electrolyte concentration of 1 M compared to 0.1 M, the oxidation potential of Cr(III) shifts by approximately 88 mV toward more negative values.

There are predominantly five Cr (VI) species that exist in equilibrium and impact the electrochemical detection: H_2CrO_4 , HCrO_4^- , CrO_4^{2-} , HCr_2O_7^- and $\text{Cr}_2\text{O}_7^{2-}$ according to the following equilibrium [31];



The speciation of Cr (VI) is dependent upon pH and concentration of the different forms of species, an indication in aqueous media is


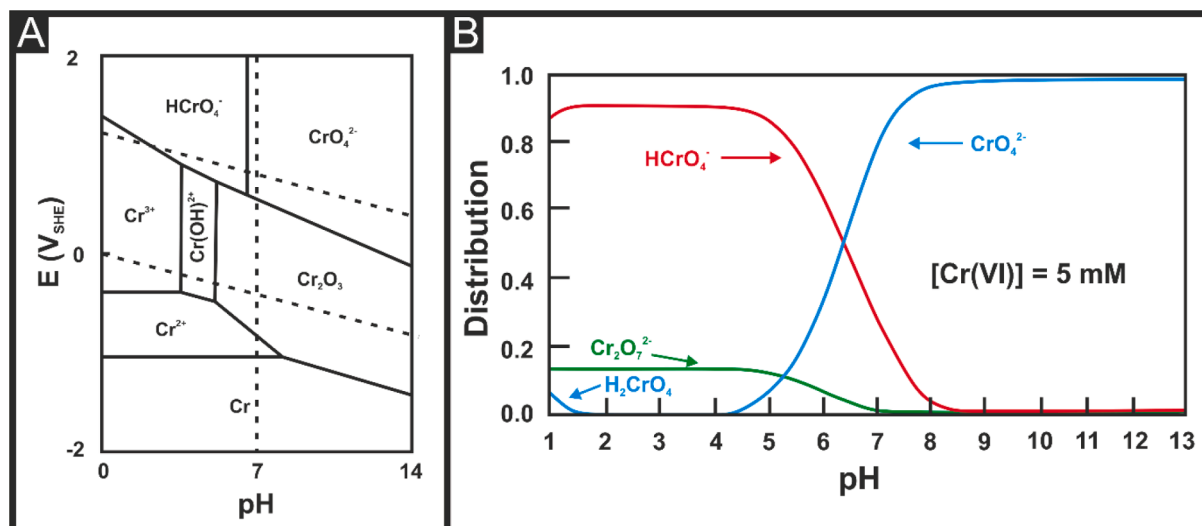




Fig. 1. A) Pourbaix diagram for chromium and $[\text{Cr}_{(\text{aq})\text{tot}}] = 10^{-6}$ M at 25°C . Reproduced and adapted with permission from reference [29]. Copyright Elsevier 1997. B) The distribution diagram for Cr (VI) at different pH values, corresponding to a Cr (VI) concentration of 5 mM. Reproduced and adapted with permission from reference [30]. Copyright Elsevier 2013.

presented in Fig. 1B. At alkaline pH values, the major species in solution are chromates, CrO_4^{2-} and as the pH shifts to more acidic range, protonation is expected which results in the formation of HCrO_4^- and H_2CrO_4 species in aqueous solution. It has been reported that at low pH values, HCrO_4^- is the dominant and electrochemically active species whereas H_2CrO_4 and complex species present no significant voltammetry [32]. It is important to note that the concentrations of the specific species in acidic media can vary depending on the concentration of Cr. At low Cr concentrations ($< 50 \mu\text{M}$), H_2CrO_4 is expected to be present in larger quantities than $\text{Cr}_2\text{O}_7^{2-}$ [33].


The electrochemical detection of Cr (VI) is commonly achieved through the reduction at the electrode's surface and, as with a vast majority of electrochemical work, this was first noted using polarography. In 1953, McElroy and Laitinen reported a two-step reduction using a mercury dropping electrode with tetrabutylammonium iodide or ammonium iodide as the supporting electrolyte [34]. More recently, Welch et al. [32] have extensively explored the electrochemical reduction of hexavalent chromium at gold, glassy carbon and boron-doped diamond electrodes in acidic media. At a glassy carbon electrode (GCE), an electrochemically irreversible single reduction peak was observed, confirmed through Tafel analysis of approximately 300 mV/decade. The authors rationalised this as the one-step reduction of Cr (VI) to Cr(III) at low concentrations ($< 200 \mu\text{M}$), with a pre-shoulder occurring above this concentration, thought to be due to the reduction of Cr(VI) to Cr(V). Due to the poor reproducibility using a GCE and the corrosive environment, they recommend not using a GCE for analytical purposes. For the boron-doped diamond (BDD) electrode, a single diffusion-controlled irreversible reduction peak at ~ -0.27 V (vs. SCE) shifting to more negative values with scan rate was observed, indicating a highly electrochemically irreversible reaction. They report the significantly improved voltammetric profile for the reduction of Cr(VI) at a solid Au macroelectrode compared to that seen at a GCE or BDD electrode. It was observed that a 1 mM solution of Cr(VI) exhibited a well-defined, diffusion-controlled reduction peak at $+0.27$ V (vs. SCE) that does not change significantly with scan rate, indicating an electrochemically reversible system, with the absence of a corresponding oxidative peak signalling toward a chemically irreversible reaction. Upon analysis in solutions of different pH they suggest the following proton-dependant mechanism for the reduction of the Cr(VI) monochromate species:



followed by:



or



where the monochromate species undergoes a one-electron reduction, one-proton reaction, followed by disproportionation. At high concentrations of H^+ , disproportionation from Cr(V) to Cr(III) can occur rapidly, whilst in dilute solutions further direct electrochemical reduction is most likely observed. Compton and co-workers used this understanding of the two species to explore the basis of Cr(III) and Cr(VI) electroanalytical sensing in this, and future work. Examples of how they and other groups have achieved this is where our attention turns next.

4. Electroanalytical detection of chromium (III) and (VI)

Table 1 chronologically summarizes the various accomplishments directed toward the sensing of chromium III and VI; consequently, below we explore this history, current electroanalytical approaches and offer insights into possible future trends in the field.

The first report of polarography for the determination of chromium was in 1954 of the insoluble residue remaining from dissolving calcium metal in hydrochloric acid, with a detection limit of $0.25 \mu\text{g}/\text{mL}$ [195, 35]. In 1975, differential pulse polarography and a hanging mercury drop electrode (HDME) were used to determine the concentration of Cr (VI) in natural water by buffering the water to a pH of 7 using ammonium acetate and ethylenediamine [36]. This achieved detection in the range of $0.035 - 2.0 \mu\text{g}/\text{mL}$, a LOD of $0.01 \mu\text{g}/\text{mL}$ and showed no interference from the presence of Cu (III) or Fe (III). As can be seen from Table 1, this was the beginning of a plethora of publications using mercury electrodes for the detection of Cr in different mediums, from specific natural waters [65] to plants [49,50,57], coolant [44], concrete [46,52] and wine [67]. Most of these works then deviated away from

Table 1

A comprehensive summary of the electroanalytical methods reported in the literature for the detection of Cr (III) and (VI); highlighting the electrode used alongside any electrode modifications, the key analytical parameters of dynamic range and limit of detection, and the real sample composition tested.

| Cr Ion | Electrode Material | Electrode Modification | Electroanalytical Technique | Dynamic Range | Limit of Detection | Real Sample Composition | Reference |
|--------|--------------------|------------------------------|-----------------------------|--|--|---|-----------|
| - | MDE | N/A | Polarography | - | 0.25 µg/mL | Calcium Metal | [35] |
| VI | MDE | N/A | Polarography | 0.035-2 µg/mL | 0.01 µg/mL | Natural Waters | [36] |
| VI | GCE | N/A | HPLC-EC | - | < 1ng | Wastewater | [25] |
| VI | MDE | DTPA complex | Polarography | - | 100 ng/g | Gallium Arsenide | [37] |
| VI | Pt | Iodine | ISE | 0.006-2 mM | 2 µM | - | [38] |
| VI | Pt | Poly(4-vinylpyridine) | CV | 0.01-1 µM | 10 nM | - | [39] |
| VI | MDE | N/A | Polarography | 0.06-1.2 µM | 16 nM | Lake Water | [40] |
| III | MDE | DTPA complex | DPAdSV | 20-2000 ng/L | 20 ng/L | River, Lake, Sea Water | [41] |
| VI | MDE | Diphenylcarbazide complex | Polarography | 0.2-60 µM | 200 nM | Waste Solids | [42] |
| VI | Pd | N/A | FI-AMP | - | - | - | [43] |
| III | MDE | DTPA complex | AdSV | - | 23 ng/L | PWR Coolant | [44] |
| VI | Pt | N/A | Polarography | 0.05-17.2 ppm | 0.02 ppm | Wastewater | [45] |
| VI | MFE | N/A | Polarography | 1-10 ppb | 0.3 ppm | Cement | [46] |
| VI | Pt | Poly-3-methylthiophene | LSV | - | 100 ppb | Acidic Media | [47] |
| III | MDE | TTHA complex | DPAdSV | - | 0.3 ng/L | Aluminium Samples | [48] |
| VI | MDE | NaPipDTC | Polarography | - | 0.01 ppm | <i>Ocimum sanctum</i> , stainless steel | [49] |
| III | MDE | 5-Br-PADAP complex | LSV | 3-90 nM | 0.9 nM | Millet, Rice | [50] |
| VI | CFE | DTPA complex | AdSV | - | 10 nM | - | [51] |
| VI | MDE | N/A | Polarography | - | 1 µM | Concrete | [52] |
| VI | MDE | Diphenylcarbazide complex | AdSV | 0-10 nM | 0.02 µg/L | Mineral Water | [53] |
| III | CPE | Diphenylcarbazide | LSV | 0.013-100 µM | 13 nM | Soil Samples | [54] |
| VI | MDE | EDTA complex | DPV | - | - | Plating Bath Water | [55] |
| III | MDE | DTPA complex | AdSV | - | 5 µM | - | [56] |
| III | MDE | BPY complex | CSV | 0.02-50 nM | 20 pM | Natural Water, Soil, Plants | [57] |
| VI | MDE | N/A | DPAdSV | 1-100 nM | 1 nM | Aqueous Samples | [58] |
| III | MDE | Surfactant additions | Polarography | - | - | - | [59] |
| VI | MDE | DTPA complex | AdSV | - | 0.51 nM | Estuarine Waters | [60] |
| III | MDE | Pyrocatechol Violet complex | AdSV | 15-100 nM | 3 nM | Lake Water | [61] |
| VI | MDE | Xylenol Orange complex | CSV | - | 1.2 ng/L | Sea Water | [62] |
| VI | MDE | TTHA complex | AdSV | - | 1.8 ng/L | Gallium | [63] |
| III | MFM | DTPA complex | CSV | 9.62-170 nM | 0.28 nM | Cell Culture | [64] |
| VI | MDE | N/A | DPV | - | - | Louisiana Water | [65] |
| VI | MDE | DTPA complex | DPAdSV | 0.1-10 nM | 30 pM | Natural Water | [66] |
| III | MDE | DTPA complex | DPAdSV | - | 0.47 nM | Wine | [67] |
| VI | MDE | N/A | DPV | 0.1-100 µM | 0.3 µM | Alkaline solutions | [68] |
| III VI | MDE | HEDTA, PCV complexes | DPAdSV | 4.85-105 nM | 30 nM | Mineral, Tap Water | [69] |
| VI | GCE | Hg Film | SWAdSV | 0.01-0.6 µM | 32.3 nM | Drinking Water | [70] |
| VI | DPE | Natural or synthetic diamond | DPV | 10 ⁻¹¹ -10 ⁻⁹ 10 ⁻¹⁰ -10 ⁻⁷ 10 ⁻⁶ -10 ⁻³ | 10 ⁻¹² 10 ⁻¹¹ 10 ⁻⁸ | Vitamin Tablets | [71] |
| III | DPE | Natural or synthetic diamond | DPV | 10 ⁻¹⁰ -10 ⁻⁸ | 10 ⁻¹² | Vitamin Tablets | [72] |
| VI | Pt | PANI/Glucose Oxidase | Amp | 0.49-95.73 µg/L, 0.096-8.05 mg/L | 0.49 µg/L | Soil Samples | [73] |
| VI | GCE | PPy/tyrosinase | Amp | 0.5-100 µM | 0.5 µM | Urine, Waste and River Water | [74] |
| VI | Hg | N/A | DPCAdSV | 0.10 nM | 40 pM | Tap, River Water | [75] |
| III | BFE | N/A | AdSV | 0.5-40 µg/L | 100 ng/L | Soil/Tobacco | [76] |
| VI | CPE | N/A | DPCSV | 0.5-50 µM | 50 nM | Tea | [77] |
| VI | Gold | N/A | CV | 20-200 µM | 4.3 µM | N/A | [32] |
| VI | CPE | Bentonite/DPCI | DPV | 0.03-0.5 mg/L | 17 µg/L | Sea Water | [78] |
| VI | GCE | Bi | CAdSV | 0-50 nM | 0.3 nM | River Water | [79] |
| VI | GCE | Pyridine-Sol Gel Films | SWV | 0-400 ppb | 4.6 ppb | N/A | [80] |
| III | GCE | N/A | FIA-SPS | - | 14 ng/L | River Water | [81] |
| III | Hg | N/A | CAdSV | 0.5-50 nM | 80 pM | Tea Leaves, Mixed Herbs, Rain/ Estuarine Water | [82] |
| VI | SPCE | AuNPs | SWV | 10-5000 µg/L | 5 µg/L | River Water | [83] |
| III | GCE | Stannum film | DPASV | 10-110 µg/L | 2 µg/L | Tap Water | [84] |
| VI | GCE | Porous | CT | 5-500 µg/L | 1.9 µg/L | Tap, Mineral, River Water | [85] |
| VI | SPCE | Poly-L-histidine | LSV | 0.1-150 µM | 0.046 µM | Waste Water | [86] |
| III | Ni-BPE | N/A | FIA | 0.3-1000 µM | 0.3 µM | Water | [87] |
| VI | GCE | Au _{nano} | SWV | 0.13-45 µg/L | 0.01 µg/L | Tap/Sewage Water | [88] |
| VI | SPCE | AuNP | DPV | 0.4-30 µM | 0.4 µM | Tap/Sea Water | [89] |
| VI | ITO | AgNP | SWV | 0.5-38 µM | 0.85 µM | Tap, Stream, Sea Water | [90] |
| VI | Gold | silicate/nanoAuNPs | Amp | 0.5-50 µM | 0.1 µM | Tap, River Water | [91] |
| VI | GCE | Bi Film | SWASV | 0.2-3 ppb | 0.1 ppb | Polypropylene | [92] |
| VI | GCE | Prussian Blue | Amp | 10-70 ppb | 5.27 ppb | Polypropylene | [93] |
| VI | CPE | Triethylamine | Amp | 0.5-200 ppb | 0.15 ppb | Waste Water | [93] |
| VI | CPE | Triethylamine | CSV | 500 nM-1 mM | 3.4 nM | Electronic Materials | [94] |

(continued on next page)

Table 1 (continued)

| Cr Ion | Electrode Material | Electrode Modification | Electroanalytical Technique | Dynamic Range | Limit of Detection | Real Sample Composition | Reference |
|--------|---------------------|--|-----------------------------|---------------------------------------|----------------------|-----------------------------|-----------|
| III | SPCE | Hg | DPV | 30-300 μM | 39 μM | Waste Water | [95] |
| VI | | AuNPs | | 4.9-40 μM | 0.5 μM | | |
| III | Bi Film | Rotating Disc Electrode/DTPA | SWAdSV | 1-10 nM | 0.336 nM | River Water | [96] |
| VI | | | | | 0.414 nM | | |
| VI | SPCE | N/A | Amp | 100-1000 $\mu\text{g/L}$ | 19 $\mu\text{g/L}$ | Canal Water | [16] |
| III | SPCE | L-DOPA | Amp | 10-125 $\mu\text{g/L}$ | 6.01 $\mu\text{g/L}$ | Wastewater | [97] |
| III | GCE | Polycarbonate/IrO ₂ nanotubes | DPV | 1-10 μM | 0.2 μM | N/A | [98] |
| VI | GCE | Al ₂ O ₃ / μNP -Bi Film | AdSV | 50-300 ng/L | 0.12 ng/L | N/A | [99] |
| VI | Gold | AgNPs | Amp | 2-370 ppb | 0.65 ppb | Wastewater | [100] |
| VI | GCE | AgNPs/Nafion film | Amp | 2-230 ppb | 0.67 ppb | Wastewater | [101] |
| VI | GCE | AuNPs/MPPTS/AuNP/PET | SWCSV | 10-1200 ng/L | 2.9 ng/L | Blood | [102] |
| III | GCE | Fe ₃ O ₄ /rGO | CV | 0.2-2 nM | N/A | N/A | [103] |
| VI | BDD | - | LSV | 0.01-5 ppm | 3 ppb | N/A | [104] |
| VI | GCE | Bi Film/SWCNT/DTPA | AdCSV | 0-25 nM | 0.036 nM | River Water | [105] |
| VI | Gold | - | ASV | 2-200 μM | 0.9 μM | Tap/Sewage/Industrial Water | [106] |
| VI | GCE | TiO ₂ /quercetin | PEC | 1-10, 20-140 nM | 0.24 nM | Drinking Water | [107] |
| VI | SPCE | quercetin | ASV | 1-200 μM | 0.3 μM | Drinking Water | [108] |
| VI | Ti | TiO ₂ NT/AuNP | Amp | 0.1-105 μM | 0.03 μM | Tap/Lake Water | [109] |
| VI | Gold | Graphene/AuNPs/chitosan | CV | 5-800 μM | N/A | N/A | [110] |
| VI | SPCE | DTPA | Amp | 0.003-40 nM | 1 μM | N/A | [111] |
| III | CFE | Poly(natural red)/HRP | Amp | 0.2-5.1 μM | 0.27 μM | N/A | [112] |
| VI | | | | 0.05-0.35 μM | 0.09 μM | | |
| III | SPCE | Tetrathiafulvalene | Amp | 1.8-15.8 μM | 2 μM | Wastewater | [113] |
| VI | SPC _{Pt} E | Glucose oxidase | Amp | 89-769 nM | 90.5 nM | | |
| VI | BD-Si | SWCNT/PA | Amp | 0.01-10 ppb | 0.01 ppb | Wastewater | [114] |
| VI | SPCE | DTPA | Amp | 3-3000 μM | 1 μM | N/A | [115] |
| VI | GCE | Ag@TiO ₂ NPs | Amp | 0.1-3.1 μM | 0.01 μM | Tap/Lake Water | [116] |
| VI | Gold | 6-mercapto-1-hexanol/methylene blue | CV | 0.5-10 μM | 500 nM | Synthetic Aquifer | [117] |
| III | GCE | CNT/chitosan/MnO nanoflakes | Amp | 3-200 μM | 0.3 μM | Drinking Water | [118] |
| VI | MCE | Bi Film | ASV | 1-25 $\mu\text{g/L}$ | 0.05 $\mu\text{g/L}$ | N/A | [119] |
| VI | SPCE | AuNPs | LSASV | 0.7-3.5, 3.5-35 ng/mL | 1.6 pg/mL | Tap/Sea Water | [120] |
| VI | ITO | Agar/PANI | CV | 2.48-50 μM | 2.48 μM | N/A | [121] |
| VI | GCE | rGO | DPSV | 0.2-1000 μM | 150 nM | Tap Water | [122] |
| VI | FTO | TiO ₂ /AuNPs | PEC | 0.01-100 μM | 4 nM | Tap/River Water | [123] |
| VI | Gold | Azacrown Monolayer | EIS | 1-100 ppb | 1.4 ppt | River Water | [124] |
| III | GCE | AuNPs | DPSV | 0.5-75 ppb | 10 ppt | Wastewater | [125] |
| VI | Pt | GQD/S ₂ O ₈ ²⁻ | ECL | 0.05-60 μM | 20 nM | River Water | [126] |
| VI | ITO | PVS/PANI | SWV | 14.6-60 μM | 4.83 μM | Tap Water | [127] |
| VI | GCE | MWCNTs/PEI | Amp | 0.002-20 μM | 0.6 nM | Tap/Lake/Wastewater | [128] |
| VI | Gold | B-galactosidase | EIS | 10 ⁻¹⁰ -10 ⁻⁴ M | 0.312 nM | River Water | [129] |
| VI | GCE | SWCNTs/pyridine-solgel | SWV | 5-300 $\mu\text{g/L}$ | 0.8 $\mu\text{g/L}$ | Swine Blood | [130] |
| VI | GCE | Fe ₃ O ₄ /MoS ₂ | Amp | 1-2360 μM | 0.5 μM | N/A | [131] |
| VI | CTE | Gold | Amp | 1-50 $\mu\text{g/L}$ | 0.7 $\mu\text{g/L}$ | Tap/Lake Water, Plastics | [132] |
| III | GCE | Electrochemical Activation | DPV | 0.05-6 μM | 0.015 μM | N/A | [133] |
| VI | | | | 0.4-250 μM | 0.12 μM | | |
| VI | SPCE | CNT | Amp | 20-1000 ppb | 5 ppb | Power Plant Water | [134] |
| VI | GCE | POT/PVC | ASV | 30-1300 nM | 12 nM | Tap Water | [135] |
| III | SPCE | Chitosan/Au | DPSV | 1-100 μM | 0.4 μM | Industrial Wastewater | [136] |
| VI | FTO | IIP/F-g-C ₃ N ₄ | PEC | 0.01-100 ppb | 0.006 ppb | River Water | [137] |
| VI | SPCE | PANI/GQD | FIA-LSV | 0.1-10 mg/L | 0.097 mg/L | Drinking Water | [138] |
| VI | GCE | Au/TiO ₂ | Amp | 0.1-3.1 μM | 0.01 μM | Tap/Wastewater | [139] |
| VI | PET | Gold | CAdSV | 0.5-100 $\mu\text{g/L}$ | 0.5 $\mu\text{g/L}$ | Textile/River Water | [140] |
| III | CPE | IIP (itaconic acid based) | DPV | 0.1-10 μM | 17.6 nM | River/Sea Water, Urine | [141] |
| III | CPE | <i>C. freudentii</i> | DPCSV | 10 ⁻⁶ -10 ⁻² M | 100 nM | Mine Water | [142] |
| VI | | | | 10 ⁻⁷ -10 ⁻⁴ M | 1 nM | | |
| VI | GCE | CB | Amp | 0.025-483 μM | 10 nM | N/A | [143] |
| VI | GCE | NiFeNPs | Amp | 0.025-98.3 μM | 10 nM | Ground Water | [144] |
| VI | SPCE | AuNPs | LSV | 20-200 $\mu\text{g/L}$ | 5.4 $\mu\text{g/L}$ | River Water | [145] |
| VI | GCE | AuNPs/Graphene | CV | 0-20 μM | 10 nM | River Water | [146] |
| VI | Ni Foam | PANI | DPV | 0-4528 nM | 0.396 pM | N/A | [147] |
| III | GCE | CNF/chitosan/AuNPs | FIA-DECD | 0.1-100 ppm | 0.69 ppb | Industrial Waste Water | [148] |
| VI | | | | 0.1-100 ppm | 0.32 ppb | | |
| VI | Gold | IIP-S | DPV | 0.009-10 μM | 0.64 nM | Tap/River Water | [147] |
| VI | CPE | AuNPs | DPV | 40-3000 $\mu\text{g/L}$ | 7 $\mu\text{g/L}$ | Tap Water | [149] |
| VI | GCE | Ag plating | ASV | 0.35-40 μM | 0.1 μM | Tap Water | [150] |
| VI | GCE | AuPdNPs/rGO | DPV | 0.05-5, 5-1000 μM | 13 nM | Lake/River Water | [151] |
| III | Pt | AgNP-LE | DPV | 10-90 μM | 0.804 μM | Lake/Waste Water | [152] |
| VI | GCE | Bi Film/Zn | CAdSV | 0.2-1.25 pM | 5.8 fM | Sea/Estuarine/Rain Water | [153] |
| VI | GCE | AuNPs/rGO | SWV | 0.1-30 μM | 46 nM | Lake/River Water | [154] |
| VI | Gold | AuNPs/PANI-co-PoT/GO | SWV | 5-500 μM | 21.5 nM | Tap Water | [155] |

(continued on next page)

Table 1 (continued)

| Cr Ion | Electrode Material | Electrode Modification | Electroanalytical Technique | Dynamic Range | Limit of Detection | Real Sample Composition | Reference |
|-----------|--------------------|---|-----------------------------|--|----------------------|--|-----------|
| VI | FTO | NiO | CV | N/A | N/A | N/A | [156] |
| III | SPCE | AuNPs | LSV | 0.5–10 μM | 0.01 μM | Tea, coffee and mineral water | [157] |
| VI | Gold | Ox-MWCNT/Au _{nano} | AMP/RDE | 0–0.2 mM | 720 nM | “Real Water” | [158] |
| III | Gold | Nick-HCR nanostructure | I-V | 200 fM–20 nM | 200 fM | N/A | [159] |
| VI | SPCE | $\alpha\text{-Fe}_2\text{O}_3$ | LSV | 5–3000 $\mu\text{g/L}$ | 1.17 $\mu\text{g/L}$ | Tap Water | [160] |
| III | GCE | Bi film | FSV | 10^{-12} – 10^{-7} M | 0.3 pM | Tap Water | [161] |
| VI | SPCE | BIVO ₄ | AMP | 0.01–264.5 μM | 3.5 nM | N/A | [162] |
| VI | GCE | Pyridine/AuNPs/rGO | ASV | 25–300 $\mu\text{g/L}$ | 1.16 $\mu\text{g/L}$ | Wastewater | [163] |
| VI | ITO | Bi/BiOI-3 | PEC | 1–230 μM | 0.3 μM | Tap/Lake Water | [164] |
| VI | Gold | Mn ₃ O ₄ /Nafion | CV | 50–400 ppb | 9.5 ppb | Canal/Sewage Water | [165] |
| VI | GCE | Ni-dealloyed AuNi/pPAT | SWV | 1 ppb – 10 ppm | 0.25 ppb | Hard/Soft/Waste Water | [166] |
| VI | GPE | AgNPs/BP/BPQ NRs | DPV | 0.08–10 nM, 0.01–1 μM , 1–100 μM | 2 pM | Tap/River/Waste Water | [167] |
| VI | GCE | PcIrCl | Amp | 50–2500 nM | 18 nM | Tap/Bore Well Water | [168] |
| VI | SPCE | MWCNT/Neutral red/AuNPs | LSV | 0.4–80 μM | 25 nM | Tea/Milk Mineral Water | [169] |
| VI | GCE | Nafion/AgM/g-C ₃ N ₄ | Amp | 0.1–0.7 μM | 1.6 nM | Drinking/Tap/River/Industrial Water | [170] |
| VI | GCE | [HC ₅ H ₆ N ₂] ₆ (Co[Mo ₆ O ₁₂ (OH) ₅ (HPO ₄) ₂].3H ₂ O | Amp | 0.5–378 μM | 26 nM | Lake Water | [171] |
| VI | BDD | AuNPs | CSV | 10–1000 $\mu\text{g/L}$ | 1.19 $\mu\text{g/L}$ | Tap Water | [172] |
| VI | GCE | (H ₂ bpp) ₂ [Na ₄ Fe(H ₂ O) ₇] [Fe(P ₄ Mo ₆ O ₃₁ H ₆) ₂].2H ₂ O/CB | Amp | 2–2610 μM | 0.174 μM | Lake Water | [173] |
| III VI | CPE | <i>S. macrogoltabida</i> | DPCSV | 0.1–1 mM 0.01–10 μM | 100 nM 1 nM | Sukinda Valley Water | [174] |
| VI | GCE | N/A | CV | 25 μM –1 mM | N/A | Tap/Lake/River Water | [175] |
| VI | GCE | (H ₂ bpp) ₆ [GdMo ₂ Mo ₁₆ O ₄₉ (HPO ₄)(PO ₄) ₅] ₂ .11H ₂ O | Amp | 5–510 μM | 0.202 μM | Lake Water | [173] |
| III | GCE | 4-BBBSH | I-V | 100 pM–100 mM | 95.5 pM | Coal/Red Sea/Tap/Well Water, Industrial Effluent | [176] |
| III | ITO | AuNPs/MSA/MSA/AgNPs | ASV | 0.1–10 nM | 0.05 nM | Tap/Pond/Lake Water | [177] |
| VI | ITO | MoS ₂ /BiOI | PEC | 0.05–160 μM | 0.01 μM | Tap/Lake Water | [178] |
| VI | ITO | 0.05-Bi-BiPO ₄ /BiOI-6% | PEC | 0.5–180 μM | 0.3 μM | Tap/Lake Water | [179] |
| VI | GCE | TPBS-C | ECL | 10^{-12} – 10^{-4} M | 0.83 pM | Lake Water | [180] |
| VI | SPCE | Melanin NPs | Amp | 0.1–5 μM | 0.03 μM | Tap/Lake Water | [179] |
| VI | gold | PDDA/Graphene/TiO ₂ | PEC | 1.4–2592.3 ppb | 0.44 ppb | N/A | [181] |
| VI | CPE | chitosan@Fe ₃ O ₄ | SWV | 0.01–0.3 $\mu\text{g/L}$ 0.5–30 $\mu\text{g/L}$ | 6.1 ng/L 78 ng/L | Drinking/Sea Water | [182] |
| VI | ITO | BiOI/CN-34% | PEC | 0.5–190 μM | 0.1 μM | Tap/Lake Water | [183] |
| VI | ITO | 5%-CuS/BW | PEC | 0.5–230 μM | 0.12 μM | Tap/Lake water | [184] |
| III VI | SPCE | AuAgNPs | DPV | 0.05–1 ppm 0.05–5 ppm | 0.1 ppb 0.1 ppb | Artificial saliva/sweat, tap water, wastewater | [185] |
| III | ITO | AuNP/3-mpa/Cr(III)/3-mpa/ AuNP | SWV | 200–500 ppb | 278 ppb | Pond Water | [186] |
| III VI | CPE | MNPZ | EIS | 1 nM–1 μM 1 nM–50 μM | 69 pM 0.45 nM | N/A | [187] |
| VI | GCE | Au/mpg-C ₃ N ₄ | LSV | 100–1000 ppb | 14.7 ppb | Tannery Wastewater | [188] |
| VI | CPE | [Co ₂ (4-dptb) ₂ (1,3-BDC) ₂].2H ₂ O | Amp | 10–1000 μM | 6.51 μM | Tap Water | [189] |
| VI | PL | Au | CV | 5–100 μM | 2.3 μM | N/A | [190] |
| VI | GCE | rGO/NiS/AuNCs | SWASV | 2–14 $\mu\text{g/L}$ | 0.09 $\mu\text{g/L}$ | Ground Water | [191] |
| VI | MGCE | PANI/Hep/MTA | DPV | 10^{-7} – 10^{-4} ppm | 0.0358 ppm | Whole Blood | [192] |
| VI | GCE | PANI@ZrO ₂ -SO ₄ ²⁻ @MWCNT | DPV | 0.55–39.5 μM | 64.3 nM | Industrial Wastewater | [193] |
| VI | GCE | [Cu ^I (BBTZ)] ₄ [Mn ^{II} (H ₂ O) ₃] ₂ [Cu ^{II} (P ₄ Mo ₆ O ₃₁ H ₇) ₂]. H ₃ PO ₄ .3H ₂ O | DPV | 0.1–1 μM | 1.59 nM | Lake Water | [194] |

Key: MDE: mercury dropping electrode; MFM: mercury film microelectrode; MGCE: magnetic glassy carbon electrode; MCE: mesoporous carbon electrode; GCE: glassy carbon electrode; DPE: diamond paste electrode; Ni-BPE: Nickel barrel plating electrode; CTE: carbon tape electrode; CPE: carbon paste electrode; BDD: boron-doped diamond; PL: pencil lead; SPCE: screen-printed carbon electrode; GPE: graphite paste electrode; PET: poly(ethylene terephthalate); ITO: indium-doped tin oxide; FTO: fluorine-doped tin oxide; BD-Si: boron doped silicon; NaPipDTC: sodium pentamethylenedithiocarbamate; 5-Br-PADAP: 2-(5'-bromo-2'-pyridylazo)-5-diethylamino-phenol; BPY: 2,3-bipyridine; TTHA: triethylene tetramine-N,N,N',N'',N''',N''''-hexaacetic acid; HEDTA: N-(2-hydroxyethyl)ethylenediamine-N,N',N'-triacetic acid; PCV: pyrocatechol violet; TiO₂NT: titania nanotubes; SWCNT-PA: single walled carbon nanotubes – bis(2,4,4-trimethylpentyl)phosphonic acid; AuNP: gold nanoparticles; MPTS: 3-mercaptopropyltrimethoxysilane; DPCI: 1,5-diphenylcarbide; DTPA: diethylenetriamine-pentaacetic acid; GQD: graphene quantum dots; CNT: carbon nanotube; CNF: carbon nanofibers; PVS: poly(vinyl sulfonic acid); POT: poly(3-octylthiophene); PVC: poly(vinyl chloride); F-g-C₃N₄: formate anion incorporated graphitic carbon nitride; IIP: ion-imprinted polymer; IIP-S: ion-imprinted chitosan-graphene nanocomposite; pPAT: poly[3'-(2-aminopyrimidyl)-2,2':5',2''-tertiophene]; AgNPs: silver nanoparticles; AgNPs-LE: silver nanoparticles from *Lycopodium esculentum*; PANI-co-PoT: poly(aniline)-co-poly(o-toluidine); Nick-HCR: nick hybridization chain reaction; BP: biphenol; BPQ NRs: biphenolquinone nanoribbons; PcIrCl: iridium phthalocyanine; AgM: silver molybdate; g-C₃N₄: graphitic carbon nitride; CB: carbon black; 4-BBBSH: (E)-N'-(4-bromobenzylidene)-4-benzenesulfonohydrazine; MSA: mercapto succinic acid; TPBS-C: 2,3-bis(4-cyanophenyl)-1,1-diphenyl-benzosilole; PDPA: poly(diallyldiamine chloride); BiOI: bismuth oxyiodide; CN: carbon nitride; BW: Bi₂WO₆ (180 °C); 3-mpa: 3-mercaptopropionic acid;

MNPZ: ZnO₂ modified-Fe₃O₄ magnetic nanoparticles; mgp-C₃N₄: mesoporous graphitic carbon nitride; rGO: reduced graphene oxide; AuNCs: gold nanocubes; Hep: heparin; MTA: magnetic tannin-modified adsorbent; PANI: poly(aniline); MWCNT: multi-walled carbon nanotube; BBTZ: bis(1,2,4-triazol-1-ylmethyl)benzene); CV: cyclic voltammetry; PEC: photoelectrochemistry; LSV: linear sweep voltammetry; DPV: differential pulse voltammetry; EIS: electrochemical impedance spectroscopy; AMP: amperometric; ECL: electrochemiluminescence; SPS: Solid-Phase Spectrophotometry; FSV: fast scan voltammetry; FIA: flow-injection analysis; RDE: rotating disc electrode; SWASV: square-wave adsorptive stripping voltammetry; CT: coulometric titration; CSV: cathodic stripping voltammetry; CAdSV: catalytic adsorptive stripping voltammetry; LSASV: linear sweep anodic stripping voltammetry; ASV: anodic stripping voltammetry; FIA-DECD: flow injection analysis coupled dual-electrochemical detectors; DPSV: differential pulse stripping voltammetry; DPCSV: differential pulse cathodic stripping voltammetry; I-V: current voltage.

differential pulse polarography toward stripping voltammetry, whilst still using a mercury electrode.

Adsorptive cathodic stripping voltammetry (AdCSV), when applied to chromium detection, exhibits the benefit of allowing direct redox speciation with no separation step. This process has been widely reported within the last four decades of literature for the determination of chromium in water samples at trace levels [32,44,41,196–200]. Fig. 2 shows the principles of voltammetric (A) and amperometric (B) techniques and, although stripping voltammetry is the most common electrochemical method for heavy metal sensing, differential pulse voltammetry (DPV), square wave voltammetry (SWV) and chronoamperometry (CA) are often applied as well. As shown in Fig. 2C, stripping analysis starts with a pre-concentration method that accumulates the heavy metal in question onto the working electrode's surface, followed by a stripping step that allows the direct quantification of the analyte (by measuring the directly proportional associated current) [201]. Stripping analysis is generally expressed by $i = K C t_{pre-concentration}^{\nu}$ [202]; where K , is a constant that includes the electrode (geometric) area (A), scan rate (ν), diffusion coefficient (D), number of electrons transferred in the electrochemical process (n) and convection rate (usually applied using the deposition step). Electroanalytical metal stripping offers ppb-grade detection limits, multi-elemental determination and *in-situ* analysis of the free heavy metal at the pH of the sample

(unlike other techniques that require the ions to be forced into free-state) [202,203].

For the ideal electroanalytical determination of heavy metals, the working electrode should be highly reproducible, exhibit low background currents and exhibit large potential ranges [202]. Jin and collaborators elegantly summarised the chronological use of different types of mercury electrodes (dropping mercury electrode (DME), hanging dropping mercury electrode (HDME), solid and mercury film electrode (MFE) with potentiostatic techniques towards chromium sensing [204, 205]. Clearly due to the potential dangers of working with mercury electrodes [202], these have been replaced by solid substrates such as precious metals (Au, Ag and Pt) and carbon electrodes, which exhibit low background current, wide potential range and chemical inertness [206,207]. It is because of the advances in electrode materials and progress replacing these classic solid electrodes, a plethora of electrode materials and modification strategies have been reported since and this is where our focus turns for the majority of this review.

5. Working electrode composition

The electrochemical signature of analytes is critically influenced by the working electrode material. Usually, electrochemistry and material science go hand-in-hand to achieve a material that exhibits good

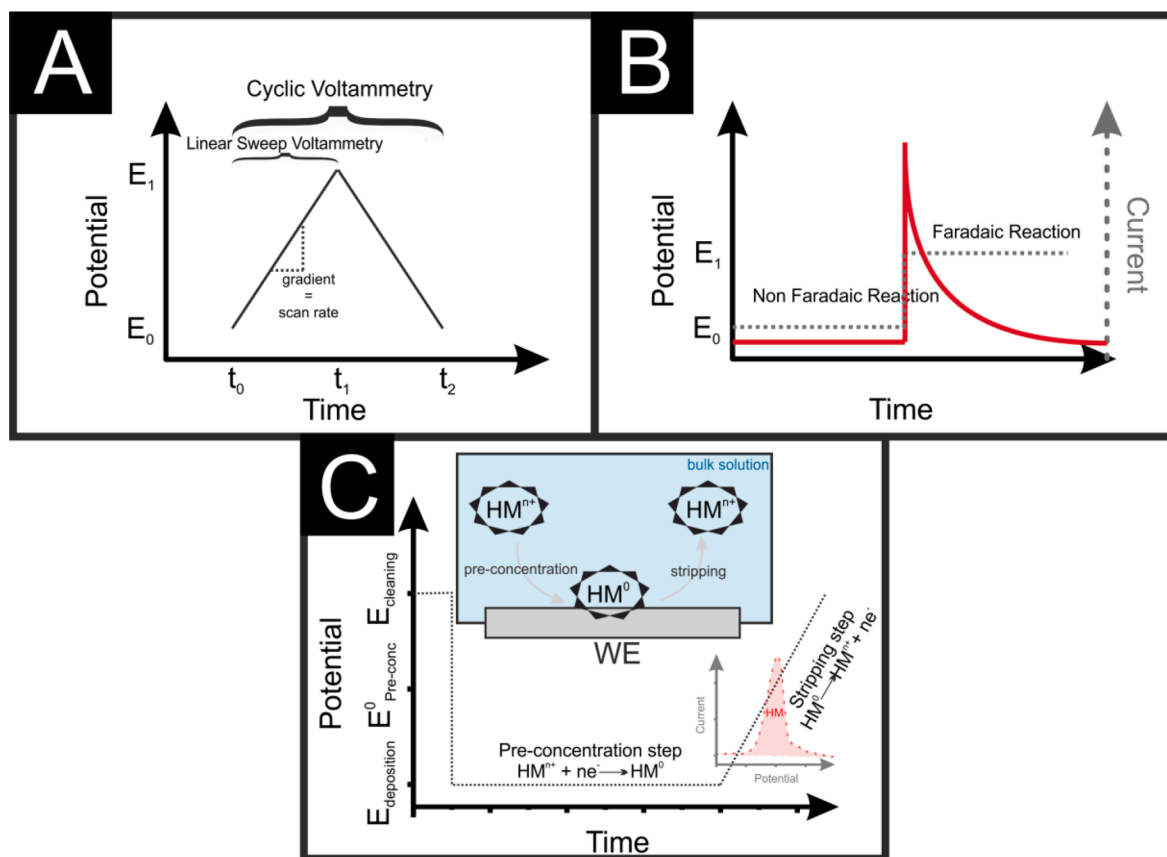


Fig. 2. Schematic diagram of voltammetric (A), amperometric (B) and stripping voltammetric (C) methods. C is reproduced and adapted with permission from reference [201] and with permission of Royal Society of Chemistry 2020.

electron transport, large electrochemically active surface area and offers a wide stable potential window with low background currents and chemical stability [208,209]. Conventional solid electrodes have been reported, extensively, towards the direct oxidation of trivalent chromium, with examples such as platinised platinum microelectrodes [210], metal oxide electrodes [211], synthetic diamond paste electrodes [212], boron doped diamond, glassy carbon and gold electrodes [28]. Brett and collaborators applied their batch injection analysis (BIA) with adsorptive stripping voltammetry (AdSV) for the detection and quantification of chromium [213]. BIA allows the injection of a small sample volume (< mL) of analyte to be added directly perpendicular to the working electrode, while all is immersed within the electrolyte. They reported the use of a mercury thin film electrode in conjunction with DTPA and cupferron as ligands for their BIA-SWAdSV, achieving an optimal LOD of 32.3 nM using cupferron complexes and a mercury electrode. O'Mahony and collaborators reported the transfer of Cr(VI) across two immiscible electrolyte solutions (ITIES) when NeoTT ionophore was used in the organic phase, achieving a LOD of 0.25 ppm Cr(VI) when using square wave voltammetry (SWV) [214].

Platinum (Pt) and Gold (Au) electrodes are often used within electroanalysis due to their excellent potential stability and electrolyte compatibility while exhibiting fast electron transfer kinetics [215,216]. Gold solid electrodes were initially used as a substitute to mercury ones due to their wide polarization range [28,217], and are still widely reported nowadays in the form of gold nanoparticles (AuNPs), thin films and other types of decorations. However, it is well known that Au(I/III) oxides are unstable, which can be easily reduced to elemental gold by electrode treatments (such as heat, UV light or reducing agents) [218–220]. It is because of this that obtaining stable Au(I/III) is considered a priority for sensor developers, and often experimentalists design combinations of several forms of gold with other metals (such as Ag-Au NPs [218] or other Au alloys such as AuCu, AuCo, and AuNi

[166], graphitic materials (graphene oxide (GO) [163], nanotubes (CNTs) [158,169]) and others forms of gold [221] towards chromium determination. Burke et al. published a comprehensive study comparing the electrochemical reduction behaviour of Cr(VI) between platinum and gold disk electrodes, reporting that the reduction of Cr(VI) occurred rapidly at lower overpotentials when using gold electrodes, compared to platinum [222]. The authors rationalised this on the basis of the pre-monolayer Cr(VI) oxidation or the hydrous oxide electrochemistry of both gold and platinum. Later on, Welch reported the direct detection of Cr(VI) at polycrystalline gold disk electrode by cyclic voltammetry, reporting good interference resistance when Cr^{3+} , Ni^{2+} , Cu^{2+} , Fe^{3+} and other surfactants were present [28]. In more recent times, and with the trend of applying the attractive physicochemical and electroanalytical properties of noble metal nanoparticles (NPs), gold NPs (AuNPs) have been widely applied to Cr(VI) determination [223]. Jin et al. [224], as shown in Fig. 3, combined the use of TiO_2 nanotubes (TiO_2NTs) with AuNPs reporting a 23-fold improvement in the electrochemical performance towards Cr(VI) detection due to the enhanced electron conductivity and increased surface-to-volume ratio of the AuNPs- TiO_2NTs . Their system achieved a LOD of 0.03 μM via chronoamperometry and exhibited good anti-interference resistance against Cr(III) and Fe(III). Stefan et al. [212] reported the use of monocrystalline (natural and synthetic) diamond paste electrodes for the determination of Cr(III) and (VI) in pharmaceutical compounds in the 2000s. They reported excellent analytical performance when interfering species (Fe^{2+} , Mg^{2+} , Cr^{6+} , Mn^{2+} , Cu^{2+} and Zn^{2+}) were present, being the natural diamond-based electrode the one exhibiting the highest sensitivity due to its higher conductivity when compared to synthetic diamonds. This was assumed to be due to the uncontrolled development of the monocrystals, causing more structural defects that hinder the electron transfer.

Following the use of solid precious metals, glassy carbon became apparent as a graphitic alternative for electrochemists. A simple

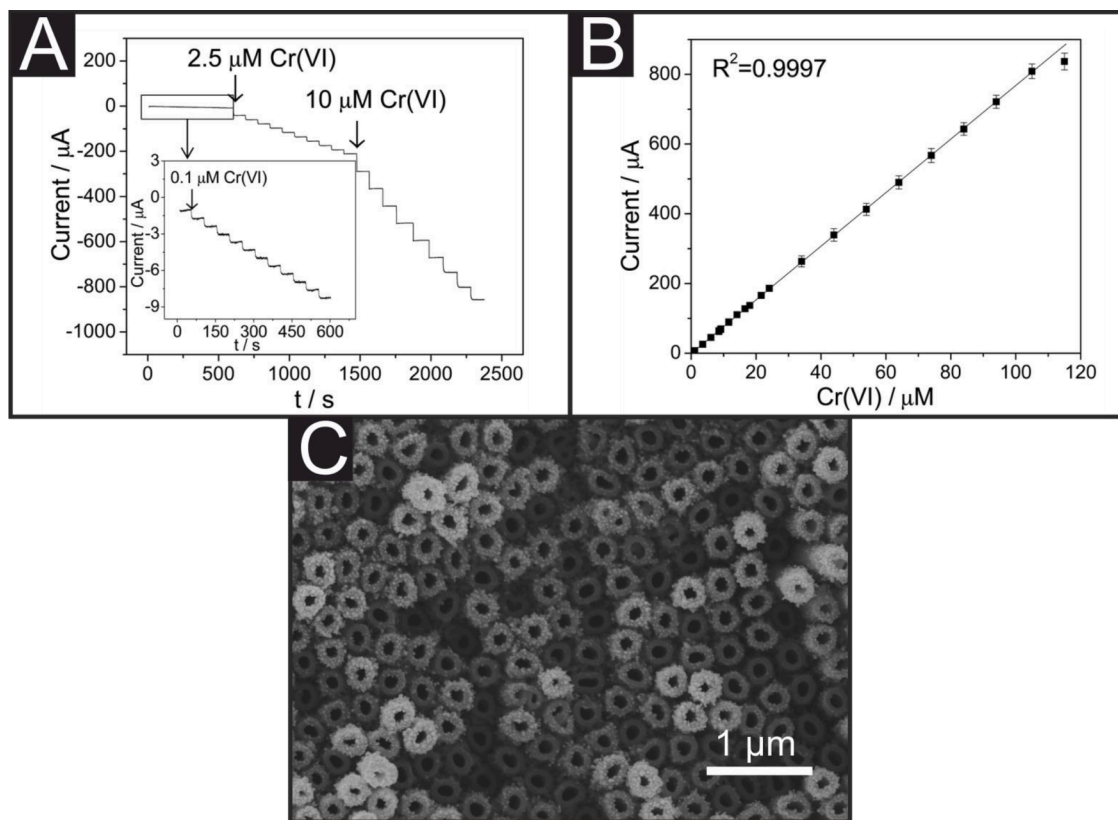


Fig. 3. (A) Amperometric current signals of the $\text{TiO}_2\text{NT-AuNPs}$ electrodes with the addition of Cr(VI) at a fixed 0.28 V potential. (B) Calibration plot of the current responses from (A) against the Cr(VI) concentration ($n=3$). (C) SEM image of the as prepared Au NPs decorated TiO_2 nanotube electrode. Reproduced and adapted with permission from reference [224].

approach was the one performed by Stern et al. [175] who reported the use of glassy carbon as an effective electrode material for the reduction and detection of hexavalent chromium in water. Fig. 4A shows their (200 μM) potassium chromate sensing with bare glassy carbon electrodes with increased concentrations of citric acid (0.05 mM (dark blue), 0.1 mM (light blue), 0.15 mM (cyan), 0.2 mM (green), 0.3 mM (yellow), 0.4 mM (orange), and 0.5 mM (red)). Fig. 4B summarises the changes in the oxidation peak of potassium chromate at different pHs. Ouyang et al., in a combined approach, reported the fabrication of a flower-like assembly of AuNPs on GC for the ultratrace detection of Cr(VI) [102]. They reported the use of two AuNP layers, where the first one is electroplated onto the GC surface as anchors, to which a thiol sol-gel film would bind to. The second AuNP layer was a self-assembled layer on top of the sol-gel, creating a flower-like AuNP nanoelectrode, expanding the electroactive area of the electrode. Finally, the surface was functionalised by a thiol pyridinium, which allowed for an enhanced preconcentration of the Cr(VI). Their proposed sensor exhibited a linear range between 10–1200 ng/L and a LOD of 2.9 ng/L towards the Cr(VI) determination.

A different electrochemical strategy of using glassy carbon (GC) was the one proposed and reported by Manova et al. [225], where they used an in-electrode coulometric titration with a porous GC electrodes. They reported the use of a coulometric method for the direct determination of Cr(VI) in water samples. The coulometry applied a constant current that will reduce the chromate ions to Cr(III) at the porous surface of the GC, where the potential of the electrode is monitored during the reduction process, indicating the end of the titration. The use of a porous GC electrodes allowed for in-electrode coulometric titration, which are based on the direct electrolysis of the chromium in the bulk of the porous electrode by the applied constant current. On the contrary to classical coulometric titrations, here the measurements were in a thin-layer solution around the three-dimensional area of the electrode. Herein, the analyte was titrated directly by electrical charge and the potential of the electrode was controlled by the oxidation-reduction couple engaged in the process. By using this clever approach, the authors reported a reproducible Cr(VI) sensor with 1.9 and 6.0 ppb as LOD and LOQ respectively. The authors also reported recoveries of around 100% for real tap, mineral and river water samples. It is important to note from their work that the use of porous electrodes might be clogged by complicated matrix samples with colloidal and solid particles. Also based on GC electrodes, Xing and collaborators reported the use of the Everitts/Prussian Blue (PB) redox couple as a mediator for the Cr(VI) reduction [226]. Under optimal conditions, their PB/GCE sensor provided a wide linear response for Cr(VI) from 0.5 to 200 ppb with a LOD of 0.15 ppb; testing it in real world waste water samples with satisfactory results. They applied an amperometric method for the Cr(VI) determination, with interference studies in the presence of metal ions (40 ppm Bi^{3+} , 2.5 ppm Co^{2+} , 1 ppm Cd^{2+} , 6 ppm Ni^{2+} , 2 ppm Sb^{2+} , 1

ppm Zn^{2+}) to solutions containing 10.0 ppb Cr(VI) which induced a less than 5.0% current deviation. Although Prussian Blue was reported as a redox mediator in catalysis and electroanalysis [227–230], the PB film was not reported until then as an electron-transfer mediator for Cr(VI).

Using a different approach, Domínguez Renedo and collaborators [231] reported the use of a Polypyrrole (PPy)-tyrosinase modified glassy carbon electrode for the indirect chromium determination in urine, waste and river waters. They used an enzymatic amperometric approach to measure Cr(III) based on the inhibitive action of this chromium on tyrosinase enzyme activity. They used electrodeposited PPy-tyrosinase membrane on the GC electrode, where the tyrosinase catalysed the oxidation of o-diphenols to o-quinones. Afterwards, the o-quinones are reduced back to catechols, which is directly influenced by the presence of Cr(III) in the sample, where the tyrosinase activity is inhibited by the chromium presence. Sánchez-Fernández et al. [232] reported the use of a bentodine-modified carbon paste electrode towards the determination of Cr(III) as shown in Fig. 5. Their procedure was based on the electrochemical response of Cr(VI)/1,5-diphenylcarbazide (DPCI) complex, measured by differential pulse voltammetry and cyclic voltammetry. The use of the DPCI complex avoided the usual interferences of other heavy metal reduction procedures and exhibited successful quantification of Cr(III) in spiked seawater. An interesting approach was the one reported by Svancara et al. [77] where they applied the synergistic pre-concentration effect of the chromate anion at the carbon paste electrode, which was *in-situ* modified with quaternary ammonium salts. They reported the successful determination of Cr(VI) in either certified reference materials and CRM black tea samples achieving a limit of detection of about 5×10^{-8} M CrO_4^{2-} . Interference studies were also explored and successful towards TlCl_4^- , AuCl_4^- , PdCl_4^{2-} , PtCl_6^{2-} , VO_4^{3-} , MnO_4^- and I^- .

More recently and following the miniaturisation trend, screen-printed electrodes (SPEs) have also been applied towards chromium detection. SPEs offer disposable and decentralised analysis with high specificity and little requirements to achieve tailored mass-producible sensors at low-cost [201,233]. Screen-printed technologies also offer the versatility of design, modification, and material composition such as graphite [111,234], carbon nanotubes (CNTs) [158,134] or gold macro-electrodes [15], which have all been successfully applied towards chromium electroanalytical determination. We note that recent work has shown that the connection length of graphitic SPEs can have a profound effect on the electrochemical and electroanalytical performance of the electrode, something which should be considered by experimentalists before undertaking work [235]. Hallam et al. demonstrated the successful use of graphite screen-printed macro-electrodes to Cr(VI) with LOD at the ppb level in canal water samples [234]. They reported that the underlying electrochemical mechanism follows an indirect process involving surface oxygenated species, suggesting that the use of HCl as a model solution might affect those species.

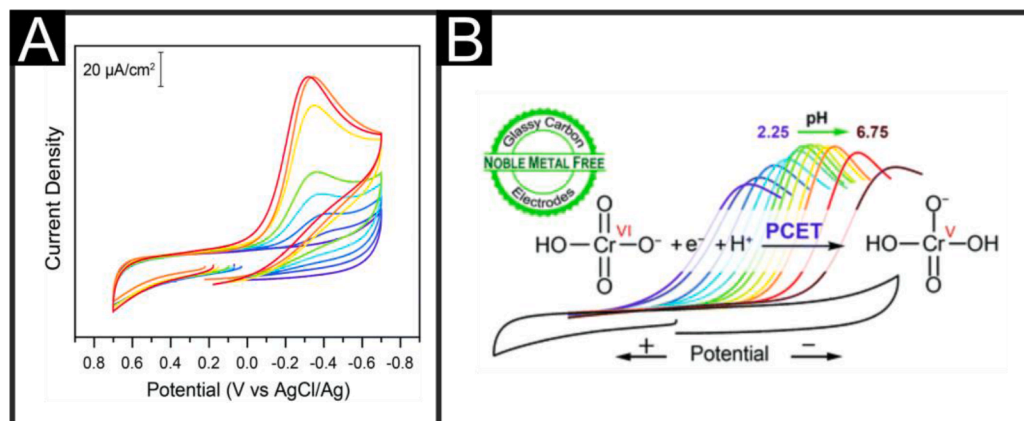


Fig. 4. (A) Cyclic voltammograms on glassy carbon electrodes of a 200 μM solution of potassium chromate in water in the absence (purple) and presence of increasing concentrations of citric acid: 0.05 mM (dark blue), 0.1 mM (light blue), 0.15 mM (cyan), 0.2 mM (green), 0.3 mM (yellow), 0.4 mM (orange), and 0.5 mM (red). Data recorded at 100 mV s^{-1} . (B) Peak current comparison of the potassium chromate oxidation at different pHs. Reproduced and adapted with permission from reference [175]. (For interpretation of the references to colour in this figure legend, the reader is referred to the web version of this article.)

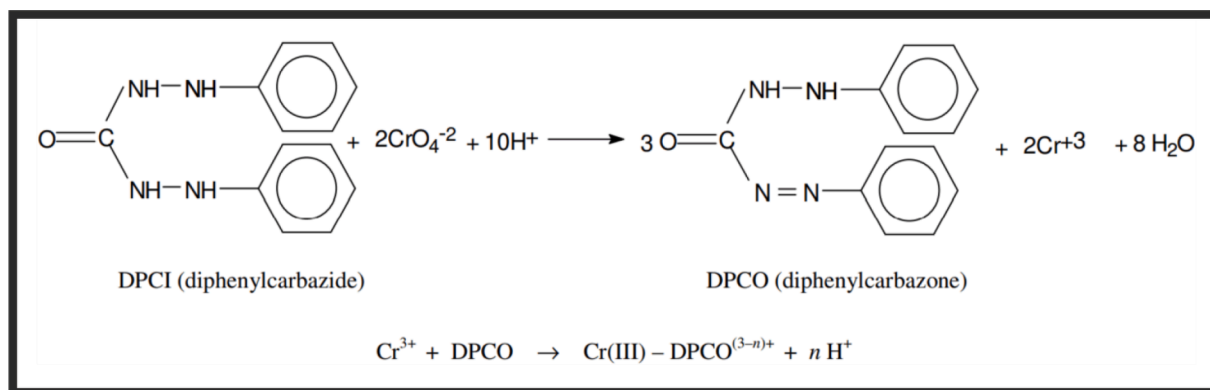


Fig. 5. Complexation of the DPCI and CrO_4^{2-} for the following electrochemical determination of Cr^{3+} . Reproduced and adapted with permission from reference [232].

Their system exhibited a simplified methodology capable of achieving a LOD of 19 ppb Cr(VI). Sánchez-Moreno et al. [236], reported the use of a BIA-SPE system targeting the chromium determination with a graphite-epoxy composite for the selective potentiometric response in batch and flow analysis, achieving LODs of 0.21 and 0.94 μM respectively. The authors also tested their sensor against Cr(VI) in mineral, tap, river waters and in leachates from municipal solid waste landfills with successful results. Metters and collaborators later explored the use of gold screen-printed macro-electrodes (AuSPEs), towards the speciation of Cr(III) and Cr(VI) [15]. They reported that the AuSPEs have electrode kinetics of at least one order of magnitude lower than polycrystalline gold macroelectrodes, however the AuSPEs mimic the analytical performance of the solid gold electrode towards sensing Cr(III) and Cr(VI). The AuSPEs however, are capable of disposable one-shot measurements and offer ease of manufacture. In terms of enhancing the electrochemical performance of working electrodes, surface modifications are a common solution that many experimentalists explore. Surface modifications such as adsorption (coatings such as dip coating or drop-casting), covalent bonding, electro-polymerisation and/or electrochemical

depositions are often utilised towards electroanalytical applications [201,237].

Domínguez-Renedo et al. [238] also applied carbon screen-printed electrodes (CSPE) towards Cr(VI) sensing, but this time with metallic silver and gold nanoparticle surface electrodeposition. As shown in Fig. 6, their newly created silver (Fig. 6A) and gold (B) nanoparticles were deposited in aggregated forms on the graphite flakes. They report that the use of bare carbon screen-printed electrodes (CSPEs) exhibited no Cr(VI) electrochemical DPV signal, however the use of silver and gold nanoparticles produced a reduction peak of Cr(VI) to Cr(III) as shown in Fig. 6C and D respectively. Their system exhibited LODs of 8.5 and 4.0×10^{-7} M for the silver- and gold-modified CSPEs, with high selectivity towards the analysis of Cr(VI) in the presence of foreign ions, including Cr(III). The same group took their CSPE modification strategy one step forward, using a two-working electrode CSPE to be the base of a Hg film and AuNP-modified bi-CSPE for the determination of Cr(III) and Cr(VI) [239]. The determination of Cr(III) was carried out by DPV using the Hg-SPEs and analogously, the Cr(VI) analysis was performed using the AuNPs-CSPEs by DPV too. The choice of an array of two working

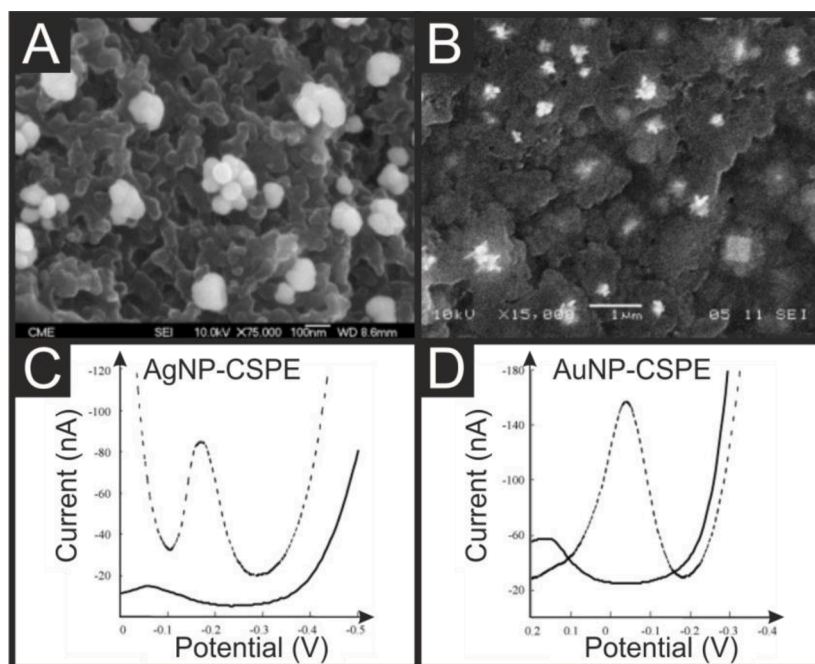


Fig. 6. SEM images of silver- (A) and gold-nanoparticle (B) modified CSPE modified by electrodeposition. Differential pulse voltammograms for Cr(VI) using silver- (A) and gold-nanoparticle (B) modified CSPEs, where solid lines represent the blank and the dotted lines are in presence of 1 μM Cr(VI); potentials vs Ag/AgCl. Reproduced and adapted with permission from reference [238].

electrodes allows for the simultaneous determination of Cr(III) and (VI) by DPV, exhibiting LODs of 1.4×10^{-4} and 4.8×10^{-6} M for Cr(III) and (VI) respectively (in the presence of each other). The authors also demonstrated its analytical application in sewage wastewater from tanning industries. Filik et al. reported the use of a neutral red inter-linked AuNPs/MWCNT modified screen-printed carbon electrode for the successful simultaneous speciation of Cr(VI) and V(V), exhibiting high sensitivity for both due to the synergistic effect of AuNPs and graphite to facilitate electron transfer, reporting a 100 fold improvement over polycrystalline gold electrode when detecting Cr(VI) [169]. Filik and Avan [157] reported a new analytical approach for the speciation analysis of both Cr(III) and Cr(VI). A simple and fast solid phase microextraction method using magnetic dextran (Sephadex G-150) as a sorbent was developed for the extraction, separation and speciation analysis of chromium ions. The retained Cr(VI) ions on the magnetic dextran sorbents were eluted and detected by linear sweep voltammetry at the gold nanoparticles modified screen- printed carbon electrode.

Another example of using AuNPs and CNTs towards Cr(VI) electroanalysis was the one reported by Breslin et al. who functionalised a gold disc electrode with multi-walled carbon nanotubes, Ox-MWCNT-Au_{nano} [158]. Their sensor showed good selectivity for the detection of Cr(VI) in the presence of Cu(II), chloride and nitrates and in a real water sample, which was attributed to the electropositive reduction potentials of Cr(VI) and the acid (H₂SO₄) supporting electrolyte that provided a clean gold surface to deposit the AuNPs without agglomeration [158].

Another successful attempt of using gold nanoparticles on screen-printed carbon electrodes (AuNPs-CSPE) was the one reported by Tu et al. [240], where they developed an *in-situ* miniaturised system for Cr(VI) determination. Their electrochemical deposition of chloroauric

acid on the CSPEs generated AuNPs, which were later activated by a voltammetric cycling step in sulfuric acid to expose more active sites. Fig. 7A shows a photograph of their CSPE before and after the gold decoration and Fig. 7B shows a series of SEM images before (above) and after (below) the gold decoration at different magnifications. Fig. 7C shows the recorded voltammograms for increasing concentrations of Cr(VI) and its corresponding calibration curve (Fig. 7D). Their disposable and portable solution exhibited reproducibility of around 5% RSD and the electrodes maintained a LOD of 5.4 ppb with long-term stability when vacuumed and tested their performance in river water samples from the Tiesha River in Hangzhou. The authors confirmed to achieve the development of a portable Cr(VI) sensor, capable of challenging AAS at a much lower cost (\$2 for the AuNP-CSPE vs \$350 for the AAS samples).

The use of Ag nanoparticles was also explored by Xu et al. [241], with the use of gold nanoporous films on gold substrates (AgGNF) towards the amperometric detection for trace Cr(VI). Their solid gold electrode (SGE) was directly anodized at +5 V to be then reduced to obtain the gold nanoporous film (AuNF) by freshly prepared ascorbic acid. Afterwards the AgNPs were grown via electrodeposition. Their multi-step AgGNF electrode exhibited higher electrocatalytic performance than those of AuNF and SGE, exhibiting a LOD of 0.65 ppb for Cr(VI) and successful anti-interference effects from other heavy metals (Cr³⁺, Cu²⁺, Pb²⁺, As³⁺ and Hg²⁺).

These are some examples of recent uses of SPEs towards chromium sensing, often with surface modifications. However, recently there is a new trend in electrode methodology, where the introduction of nano-materials [242], composites and metal-organic frameworks (MOFs) into the field of electroanalysis has promoted the advances of environmental

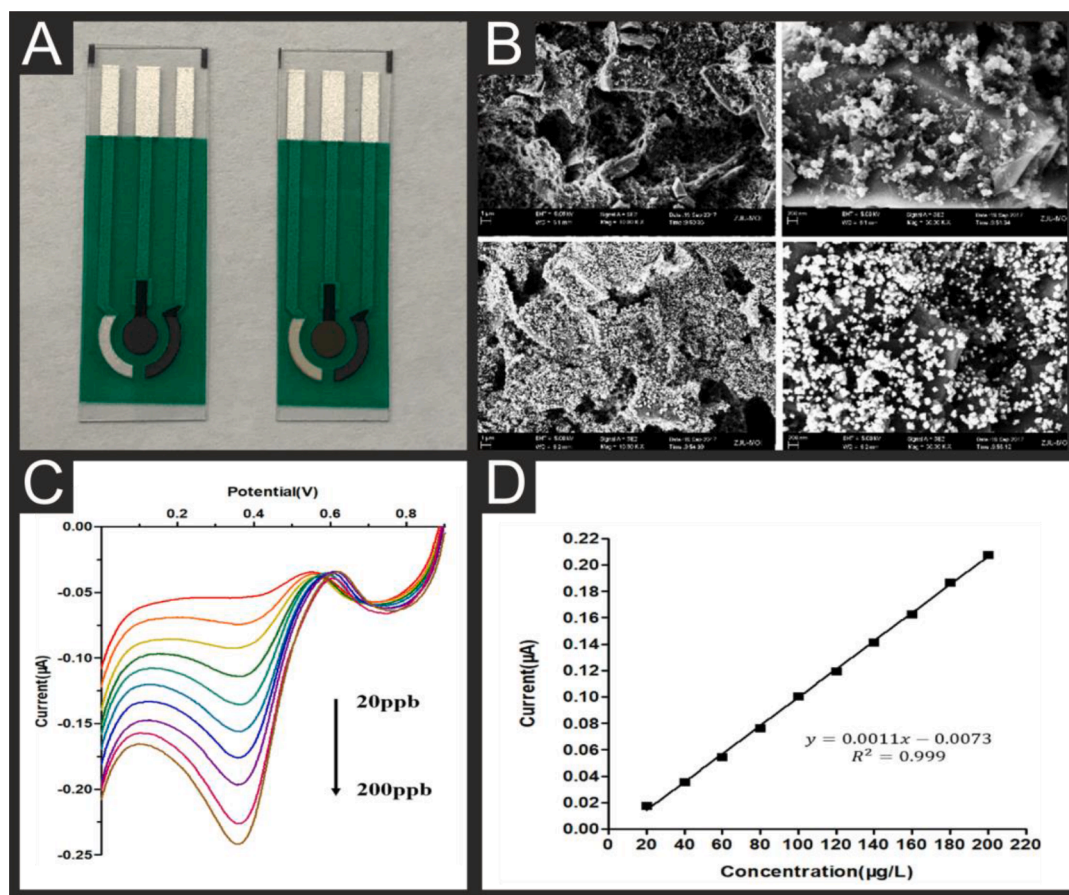


Fig. 7. Photograph of the CSPEs before (left) and after (right) the AuNPs decoration. SEM images of CSPEs before (above) and after (below) the decoration at 10K (left) and 50K (right) magnifications. C) Voltammograms for increasing Cr(VI) concentrations and D) its corresponding calibration curve. Reproduced and adapted with permission from reference [240].

monitoring solutions. Although recent, the application of MOFs to electroanalysis offers a precise and open-pore structure for surface functionalization, allowing the improvement of charge transfer and electron conductivity. One example of MOF surface modification of SPEs is by Fu et al. [160], who decorated α -Fe₂O₃ on SPEs. They produced iron nanostructures in the presence of glycerol by hydrothermal conditions, as shown in Fig. 8. Their urchin-like α -Fe₂O₃ with restricted (001) plane exposure was deposited onto SPEs, exhibiting a successful Cr(VI) sensor in tap water, with a LOD of ca. 1 ppb. The iron nanostructure had mostly exposed (001) planes, which have a higher density of coordinated hydroxyl groups that allowed a high Cr(VI) adsorption.

A graphene carbon nitride immobilisation using a nafion-modified glassy carbon electrode and coated with silver molybdate (g-C₃N₄/AgM/Nf/GCE) was proposed by Karthika et al. [170]. The nanocomposite was created *via* a sonochemical approach, as shown in Fig. 9, and showed high electrocatalytic activity towards the amperometric reduction of Cr(VI). The use of g-C₃N₄/AgM nanorods exhibited a large surface area and an enhanced electron transfer when immobilised with nafion. The use of an amperometric technique at fixed 0.29 V allowed the Cr(VI) determination in 3 seconds, which exhibited a limit of detection of 0.0016 μ M. No interference effects were detected with Fe²⁺, Ca²⁺, Mg²⁺ and Mn²⁺ (at 4x the concentration against Cr(VI)). The authors also tested their systems in real tap, bottled, river and industrial waste waters, which averaged recovery percentages >95% among them. A functionalised three-dimensional graphene electrode with AuNPs was reported by Xu et al. [163] towards Cr(VI) sensing in water samples. The use of 3D graphene alleviated the self-aggregation issue of graphene, which often hinders electrochemical performance. The three-dimensional reduced graphene oxide structure offered a porous and interconnected framework for fast electron transfer, enhanced mass transfer and large surface area. This, when coupled with AuNPs, exhibited synergistic cooperation for Cr(VI) determination. In this work, the authors used a self-assembled pyridine groups on the AuNPs through a S-Au bond as shown in Fig. 10, which exhibited LOD of ca. 1 ppb and recoveries in the range of 96-104%.

6. Future prospects

Numerous research groups have reported the use of additive manufacturing (AM) to achieve electrodes and microfluidic detection systems for heavy metal monitoring [243–247]. These are portable and cost-effective alternatives to conventional desktop detection methods, which can be fully printed modularly [248] or all-in-one [249] for their electrochemical application. However, these have their own challenges and have not been reported towards chromium detection in water yet. The use of 3D printed/additive manufactured electrodes towards electroanalytical applications depends on the effectiveness of the surface of the electrode to transport electrons, pre-accumulate the metal on its surface, and then to strip it back to the solution. Further research in material science and electrochemical detection methods is necessary to allow these AM electroanalytical devices to be fully developed. In addition, challenges such as the determination in complex water matrices and variable matrix conditions need to be addressed. Microfluidic-based systems are often used within the literature, however their use within the water industry is still limited due to biofouling, gas bubbles and irregular flow rates, although, current manufacturing techniques are advancing at a high pace, this might allow these issues to be sorted out in the near future. The introduction of filtration systems, highly selective recognition elements, multi-array electrode systems and internal standards might allow these challenges to be a thing of the past soon. Despite rapid advances and research outcomes towards on-site low-cost heavy metal analysis in water, these are often only applicable to laboratory conditions. Only a handful of systems that comply with water quality regulations, whilst being developed and proven as portable and mass-producible chromium devices.

7. Conclusions and outlook

In this review, we remind the reader the importance of Chromium contamination in drinking water. Herein, we have explored and analysed the historical use of electroanalytical methods towards Cr determination as an alternative robust, sensitive and rapid methodology to bench-top instruments. Due to the introduction of stricter limits for

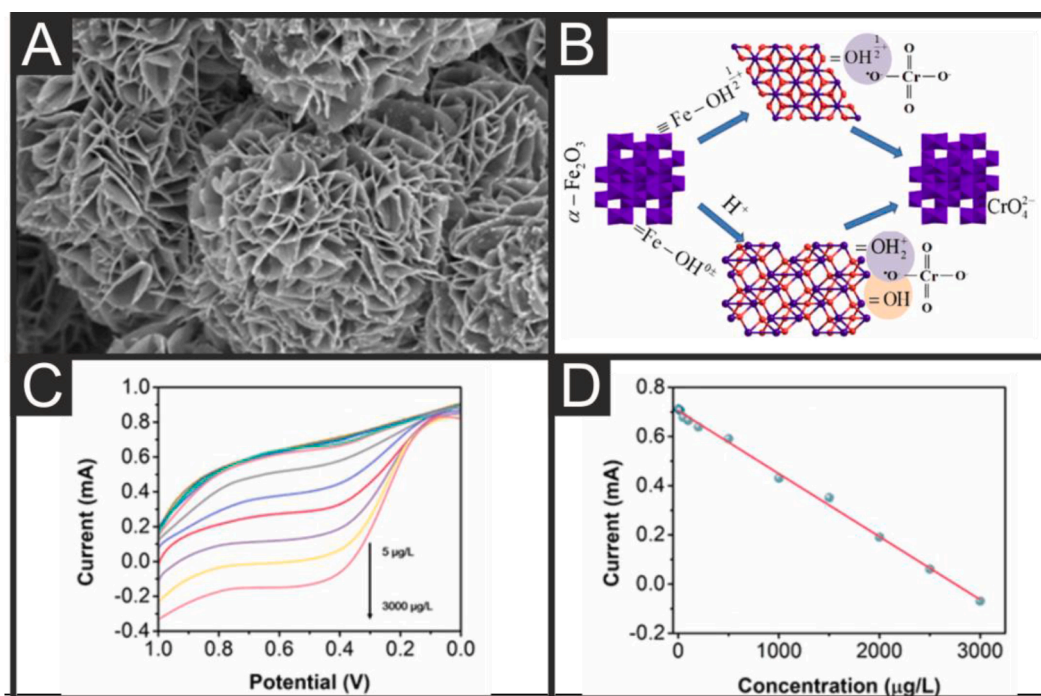


Fig. 8. SEM image of urchin-like α -Fe₂O₃, adsorption mechanism of Cr(VI) on α -Fe₂O₃ (B), linear sweep voltammetry of the α -Fe₂O₃/SPE electrochemical signals with increasing amounts of Cr(VI) were present (C) and its corresponding calibration curve (D). Reproduced and adapted with permission from reference [160].

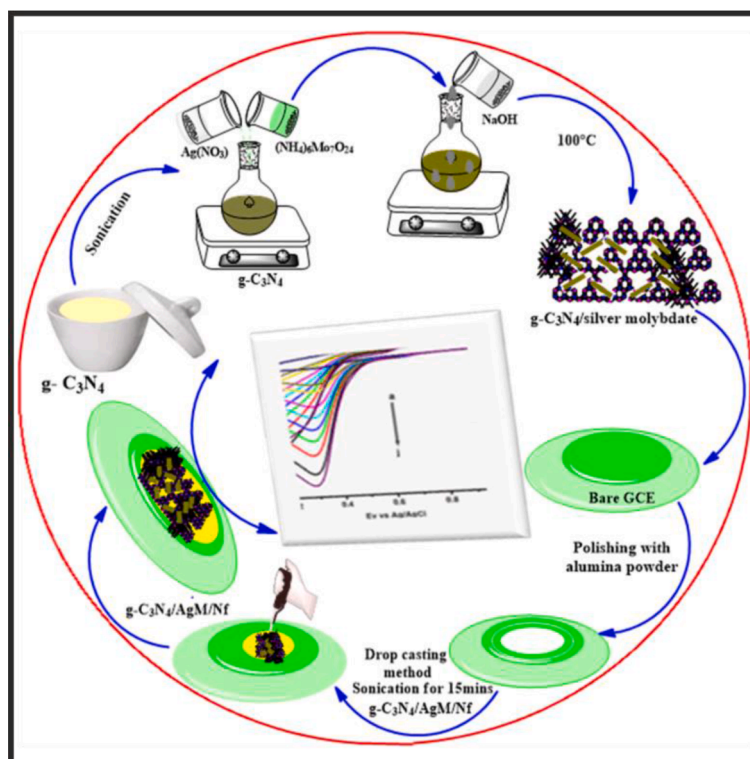


Fig. 9. Step-by-step schematic representation of the fabrication of g-C₃N₄/AgM/Nf modified glassy carbon electrode for Cr(VI) electrochemical determination. Reproduced and adapted with permission from reference [170].

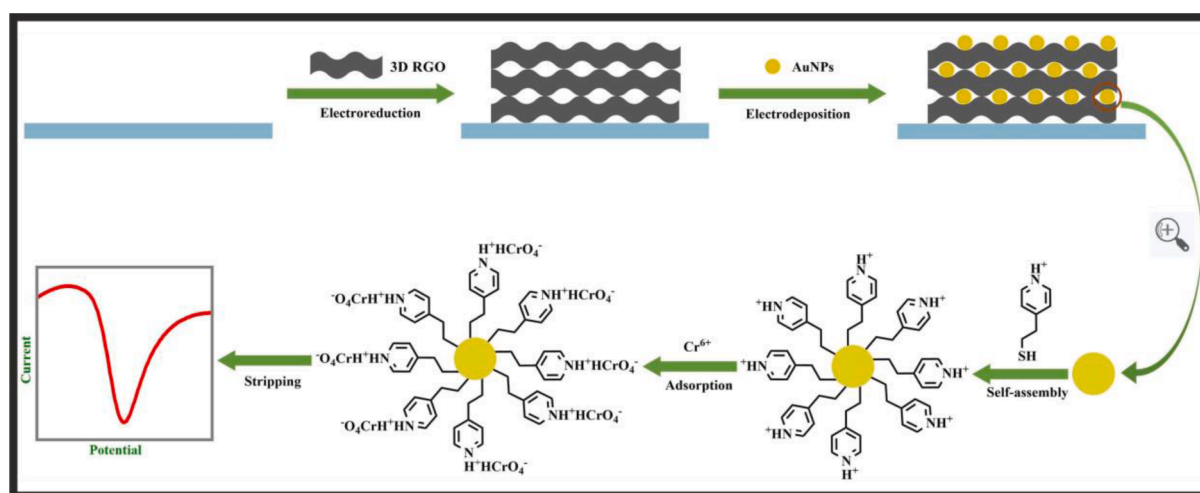


Fig. 10. Schematic illustration of the pyridine preparation and functionalisation on AuNPs/3D graphene/GCE and an analytical Cr(VI) response. Reproduced and adapted with permission from reference [163].

drinking water and environmental pollutants, there is a need for alternative solutions that can create large-scale environmental monitoring at an affordable cost. This review showcases and explains some of the recent advances in nanomaterials and electrochemistry and their application to Cr analysis, with particular attention to screen-printed electrochemical platforms. However, more efforts are needed to target multi-analyte speciation, unknown matrices or on-line sensors for screen-printed electrode platforms to become a dominant instrument in the environmental monitoring market. As material science grows, more materials will likely be reported towards electroanalytical purposes, however it is clear that this is an emerging and exciting field utilising previously well-known methodologies.

Declaration of Competing Interest

There are no conflict of interest to declare.

Acknowledgments

Innovate UK (KTP Reference: 11606) is acknowledged.

References

- [1] M.B. Arain, I. Ali, E. Yilmaz, M. Soylyak, Nanomaterial's based chromium speciation in environmental samples: a review, *TrAC Trends Anal. Chem.* 103 (2018) 44–55.

- [2] N. England, *Vitamins and Minerals* (2020). <https://www.nhs.uk/conditions/vitamins-and-minerals/others/#chromium>. Accessed 01/10/2021 2021.
- [3] D.J. McIver, A.M. Grizales, J.S. Brownstein, A.B. Goldfine, Risk of type 2 diabetes is lower in US adults taking chromium-containing supplements, *J. Nutr.* 145 (12) (2015) 2675–2682.
- [4] A.M. Standeven, K.E. Wetterhahn, Chromium (VI) toxicity: uptake, reduction, and DNA damage, *J. Am. College Toxicol.* 8 (7) (1989) 1275–1283.
- [5] H. Yao, L. Guo, B.-H. Jiang, J. Luo, X. Shi, Oxidative stress and chromium (VI) carcinogenesis, *J. Environ. Pathol.* 27 (2) (2008). Toxicology and Oncology.
- [6] M. Costa, Potential hazards of hexavalent chromate in our drinking water, *Toxicol. Appl. Pharmacol.* 188 (1) (2003) 1–5.
- [7] W.H. Organization, Chromium in Drinking-water, World Health Organization, 2020.
- [8] E. Vaioopoulou, P. Gikas, Regulations for chromium emissions to the aquatic environment in Europe and elsewhere, *Chemosphere* 254 (2020), 126876.
- [9] Z. Brandt, *Anal. Chem.* 45 (95) (1906).
- [10] Cazeneuve, *Bull. Soc. Chim.* 23 (592) (1900).
- [11] N.M. Stover, Diphenylcarbazide as a test for chromium, *J. Am. Chem. Soc.* 50 (9) (1928) 2363–2366.
- [12] D. Bregnbak, J.D. Johansen, M.S. Jellesen, C. Zachariae, J.P. Thyssen, Chromium (VI) release from leather and metals can be detected with a diphenylcarbazide spot test, *Contact Dermatitis* 73 (5) (2015) 281–288.
- [13] M. Noroozifard, M. Khorasani-Modlagh, Specific extraction of chromium as tetrabutylammonium-chromate and spectrophotometric determination by diphenylcarbazide: speciation of chromium in effluent streams, *Anal. Sci.* 19 (5) (2003) 705–708.
- [14] J.-F. Jen, G.-L. Ou-Yang, C.-S. Chen, S.-M. Yang, Simultaneous determination of chromium (III) and chromium (VI) with reversed-phase ion-pair high-performance liquid chromatography, *Analyst* 118 (10) (1993) 1281–1284.
- [15] J.P. Metters, R.O. Kadara, C.E. Banks, Electroanalytical sensing of chromium(III) and (VI) utilising gold screen printed macro electrodes, *Analyst* 137 (4) (2012) 896–902.
- [16] P.M. Hallam, D.K. Kampouris, R.O. Kadara, C.E. Banks, Graphite screen printed electrodes for the electrochemical sensing of chromium (VI), *Analyst* 135 (8) (2010) 1947–1952.
- [17] S.J. Hood, D.K. Kampouris, R.O. Kadara, N. Jenkinson, F.J. Del Campo, F. X. Muñoz, C.E. Banks, Why ‘the bigger the better’ is not always the case when utilising microelectrode arrays: high density vs. low density arrays for the electroanalytical sensing of chromium (VI), *Analyst* 134 (11) (2009) 2301–2305.
- [18] M.R. Letsoalo, M.A. Mamo, A.A. Ambushe, Synchronous Extraction and Quantitative Speciation of Arsenic and Chromium in Sediments by High-Performance Liquid Chromatography–Inductively Coupled Plasma–Mass Spectrometry (HPLC-ICP-MS), *Anal. Lett.* 54 (12) (2021) 1943–1967.
- [19] D. Spanu, D. Monticelli, G. Binda, C. Dossi, L. Rampazzi, S. Recchia, One-minute highly selective Cr (VI) determination at ultra-trace levels: An ICP-MS method based on the on-line trapping of Cr (III), *J. Hazard. Mater.* 412 (2021), 125280.
- [20] R. Pechancová, J. Gallo, D. Milde, T. Pluháček, Ion-exchange HPLC-ICP-MS: a new window to chromium speciation in biological tissues, *Talanta* 218 (2020), 121150.
- [21] M. Marcinkowska, I. Komorowicz, D. Barakiewicz, Study on multielemental speciation analysis of Cr (VI), As (III) and As (V) in water by advanced hyphenated technique HPLC/ICP-DRC-MS. Fast and reliable procedures, *Talanta* 144 (2015) 233–240.
- [22] W. Zou, C. Li, J. Hu, X. Hou, Selective determination of Cr (VI) and non-chromatographic speciation analysis of inorganic chromium by chemical vapor generation-inductively coupled plasma mass spectrometry, *Talanta* 218 (2020), 121128.
- [23] M. Saraiva, R. Chekri, T. Guérin, J.J. Sloat, P. Jitaru, Chromium speciation analysis in raw and cooked milk and meat samples by species-specific isotope dilution and HPLC-ICP-MS, *Food Addit. Contamin.* 38 (2) (2021) 304–314.
- [24] N. Hilali, H. Mohammadi, A. Amine, N. Zine, A. Errachid, Recent Advances in Electrochemical Monitoring of Chromium, *Sensors* (2020) 5153.
- [25] A. Bond, G. Wallace, Simultaneous determination of copper, nickel, cobalt, chromium (VI), and chromium (III) by liquid chromatography with electrochemical detection, *Anal. Chem.* 54 (11) (1982) 1706–1712.
- [26] G. Kelsall, C. House, F. Gudyanga, Chemical and electrochemical equilibria and kinetics in aqueous Cr (III)/Cr (II) chloride solutions, *J. Electroanal. Chem. Interfacial Electrochem.* 244 (1–2) (1988) 179–202.
- [27] F. Danilov, A. Velichenko, Electrocatalytic activity of anodes in reference to Cr (III) oxidation reaction, *Electrochim. Acta* 38 (2–3) (1993) 437–440.
- [28] C.M. Welch, M.E. Hyde, O. Nekrassova, R.G. Compton, The oxidation of trivalent chromium at polycrystalline gold electrodes, *Phys. Chem. Chem. Phys.* 6 (12) (2004) 3153–3159.
- [29] B. Beverskog, I. Puigdomenech, Revised pourbaix diagrams for chromium at 25–300 C, *Corros. Sci.* 39 (1) (1997) 43–57.
- [30] R.T. Kachosangi, R.G. Compton, Voltammetric determination of Chromium (VI) using a gold film modified carbon composite electrode, *Sens. Actuators B* 178 (2013) 555–562.
- [31] C. Ni, S. Liu, L. Cui, Z. Han, L. Wang, R. Chen, H. Liu, Adsorption performance of Cr (VI) onto Al-free and Al-substituted ferrihydrites, *RSC Adv.* 6 (71) (2016) 66412–66419.
- [32] C.M. Welch, O. Nekrassova, R.G. Compton, Reduction of hexavalent chromium at solid electrodes in acidic media: reaction mechanism and analytical applications, *Talanta* 65 (1) (2005) 74–80.
- [33] C.-H. Weng, Y.-T. Lin, T. Lin, C. Kao, Enhancement of electrokinetic remediation of hyper-Cr (VI) contaminated clay by zero-valent iron, *J. Hazard. Mater.* 149 (2) (2007) 292–302.
- [34] A. McElroy, H. Laitinen, Polarography in Liquid Ammonia. V. The Polarography of Lead, Cadmium, Zinc, Nickel, Cobalt, Chromium and Aluminum Ions, *J. Phys. Chem.* 57 (6) (1953) 564–567.
- [35] G. Reynolds, H. Shalgowsky, The polarographic determination of manganese, copper, chromium and iron in the insoluble residue remaining after the solution of calcium metal in hydro, *Anal. Chim. Acta* 10 (1954) 273–280.
- [36] S.T. Crosman, T.R. Mueller, The determination of chromium (VI) in natural waters by differential pulse polarography, *Anal. Chim. Acta* 75 (1) (1975) 199–205.
- [37] D. Ferri, F. Zignani, P. Buldini, Differential pulse polarographic determination of chromium in gallium arsenide, *Fresenius' Zeitschrift für analytische Chemie* 313 (7) (1982) 539–541.
- [38] J.A. Cox, P.J. Kulesza, M.A. Mbugwa, Voltammetric ion-selective electrode for chromium (VI), *Anal. Chem.* 54 (4) (1982) 787–789.
- [39] J.A. Cox, P.J. Kulesza, Stripping voltammetry of chromium (VI) at a poly (4-vinylpyridine)-coated platinum electrode, *Anal. Chim. Acta* 154 (1983) 71–78.
- [40] J.A. Cox, J.L. West, P.J. Kulesza, Determination of chromium (VI) by differential-pulse polarography with a sodium fluoride supporting electrolyte, *Analyst* 109 (7) (1984) 927–930.
- [41] J. Golimowski, P. Valenta, H.W. Nürnberg, Trace determination of chromium in various water types by adsorption differential pulse voltammetry, *Fresenius' Zeitschrift für analytische Chemie* 322 (3) (1985) 315–322.
- [42] J. Mocač, M. Vančková, J. Labuda, Determination of extractable chromium (VI) in the presence of large excess of chromium (III) in solid materials, *Microchim. Acta* 86 (3) (1985) 231–246.
- [43] K.W. Pratt, W.F. Koch, Determination of trace-level chromium (VI) in the presence of chromium (III) and iron (III) by flow-injection amperometry, *Anal. Chem.* 58 (1) (1986) 124–127.
- [44] K. Torrance, C. Gatford, Determination of soluble chromium in simulated PWR coolant by differential-pulse adsorptive stripping voltammetry, *Talanta* 34 (11) (1987) 939–944.
- [45] P. Sharma, R. Kapoor, Polarographic determination of chromium in aqueous matrices at micro levels, *Int. J. Environ. Anal. Chem.* 30 (1–2) (1987) 51–57.
- [46] J. Vandenbalck, G. Patriarche, Electrochemical micro-determinations of thallium (I) and chromium (VI) ions using DPASV and DP polarography, *Sci. Total Environ.* 60 (1987) 97–104.
- [47] P.R. Teasdale, M.J. Spencer, G.G. Wallace, Selective determination of Cr (VI) oxyanions using a poly-3-methylthiophene-modified electrode, *Electroanalysis* 1 (6) (1989) 541–547.
- [48] K. Sarmaik, M. Palrecha, R. Dhaneshwar, Differential pulse adsorptive voltammetric determination of chromium in aluminum, *Electroanalysis* 1 (5) (1989) 469–471.
- [49] K. Saraswathi, K. Santha, K. Meenakumari, Specific and sensitive method for the determination of trace amounts of chromium using the catalytic current at a dropping mercury electrode, *Analyst* 115 (4) (1990) 465–466.
- [50] J. Lu, W. Jin, S. Wang, T. Sun, Determination of trace chromium (III) by linear sweep adsorption voltammetry, *J. Electroanal. Chem. Interfacial Electrochem.* 291 (1–2) (1990) 49–57.
- [51] C. Hua, K.A. Sagar, K. McLaughlin, M. Jorge, M.P. Meaney, M.R. Smyth, Development of a micro-electrochemical flow cell using carbon or gold fibres for voltammetric and amperometric analyses, *Analyst* 116 (11) (1991) 1117–1120.
- [52] A. Yamada, K. Hodouchi, A. Yanagisawa, Electrochemical Determination of Chromate in Fresh Concrete, *Denki Kagaku Oyobi Kogyo Butsuri Kagaku* 59 (6) (1991) 519–520.
- [53] C. Elleouet, F. Quentel, C. Madec, Determination of trace amounts of chromium (VI) in water by electrochemical methods, *Anal. Chim. Acta* 257 (2) (1992) 301–308.
- [54] A. Paniagua, M. Vazquez, M. Tascon, P.S. Batanero, Determination of chromium (VI) and chromium (III) by using a diphenylcarbazide-modified carbon paste electrode, *Electroanalysis* 5 (2) (1993) 155–163.
- [55] J. Golimowski, B. Krasnodębska, E. Najdeker, Voltammetric determination of Cr (III) in plating baths containing Cr (III) salts as the main component, *Fresenius. J. Anal. Chem.* 352 (6) (1995) 544–546.
- [56] Z. Filipovic-Kovacevic, I. Kruhac, B. Borovnjak-Zlataric, S. Milardovic, Simultaneous determination of chromium, nickel and selenium by voltammetric techniques, *Anal. Lett.* 29 (3) (1996) 451–461.
- [57] Z. Gao, K.S. Siow, Catalytic-adsorptive stripping voltammetric determination of chromium in environmental materials, *Electroanalysis* 8 (6) (1996) 602–606.
- [58] M.A. Ghandour, S.A. El-Shatoury, A.M. Aly, S.M. Ahmed, Adsorptive cathodic stripping voltammetric determination of hexavalent chromium, *Anal. Lett.* 29 (8) (1996) 1431–1445.
- [59] A. Ibrahim, M.I. Ismail, Polarographic determination of Pb (II), Sb (II), U (VI), Bi (III), Cu (II), Cd (II), In (III), Cr (III) and Ti (IV) in the presence of TI (I) using ionisable and non-ionisable surfactants, (1996).
- [60] E.M. de Souza, A.D.L.R. Wagener, P. Farias, Voltammetric Determination of Cr (III) and Cr (VI) in Tropical Estuarine Waters: advantages and Limitations, *Croat. Chem. Acta* 70 (1) (1997) 259–269.
- [61] D.V. Vukomanovic, K. Nakatsu, D.E. Zoutman, Determination of chromium (VI) and (III) by adsorptive stripping voltammetry with pyrocatechol violet, *Microchim. J.* 57 (1) (1997) 86–95.
- [62] R. Ramjuttun, The chemical speciation of chromium in seawater by cathodic stripping voltammetry, Memorial University of Newfoundland, 1997.

- [63] M. Palrecha, P. Mathur, Adsorptive stripping voltammetric determination of chromium in gallium, *Talanta* 45 (2) (1997) 433–436.
- [64] S. Morais, G.S. De Carvalho, J. Sousa, Chromium determination in osteoblast-like cell culture medium by catalytic cathodic stripping voltammetry with a mercury microelectrode, *J. Trace Elem. Med. Biol.* 12 (2) (1998) 101–108.
- [65] K.J. Bundy, D. Berzins, Differential pulse polarographic analysis of lead and chromium content in Louisiana waters, *Environ. Geochem. Health* 20 (2) (1998) 45–51.
- [66] M. Korolczuk, M. Grabarczyk, Voltammetric determination of Cr (VI) in a flow system in the presence of diethylenetriaminepentaacetic acid (DTPA) following its deposition in the metallic state, *Anal. Chim. Acta* 387 (1) (1999) 97–102.
- [67] O. Domínguez, S. Sanlloriente, M.J. Arcos, Application of an optimization procedure of adsorptive stripping voltammetry for the determination of chromium in wine, *Electroanalysis* 11 (17) (1999) 1273–1279.
- [68] V. Sladkov, V. Peretroukhina, A. Maslennikov, F. David, Differential pulse voltammetric determination of U (VI)-Tc (VII) and U (VI)-Cr (VI) in alkaline solutions, *Radiochim. Acta* 89 (3) (2001) 139–144.
- [69] O. Domínguez, M.J. Arcos, Simultaneous determination of chromium (VI) and chromium (III) at trace levels by adsorptive stripping voltammetry, *Anal. Chim. Acta* 470 (2) (2002) 241–252.
- [70] C.M. Brett, O.M. Filipe, C.S. Neves, Determination of chromium (VI) by batch injection analysis and adsorptive stripping voltammetry, *Anal. Lett.* 36 (5) (2003) 955–969.
- [71] R.I. Stefan, S.G. Bairu, Diamond paste based electrodes for the determination of Cr (VI) at trace levels, *Instrum. Sci. Technol.* 31 (3) (2003) 261–267.
- [72] R.-I. Stefan, S.G. Bairu, J.F. van Staden, Diamond paste-based electrodes for determination of Cr (III) in pharmaceutical compounds, *Anal. Bioanal. Chem.* 376 (6) (2003) 844–847.
- [73] G.-M. Zeng, L. Tang, G.-L. Shen, G.-H. Huang, C.-G. Niu, Determination of trace chromium (VI) by an inhibition-based enzyme biosensor incorporating an electropolymerized aniline membrane and ferrocene as electron transfer mediator, *Int. J. Environ. Anal. Chem.* 84 (10) (2004) 761–774.
- [74] O.D.n. Renedo, M.A. Lomillo, M.A. Martínez, Optimisation procedure for the inhibitive determination of chromium (III) using an amperometric tyrosinase biosensor, *Anal. Chim. Acta* 521 (2) (2004) 215–221.
- [75] M. Grabarczyk, L. Kaczmarek, M. Korolczuk, Determination of Cr (VI) by catalytic adsorptive stripping voltammetry with application of nitrilotriacetic acid as a masking agent, *Electroanalysis* 16 (18) (2004) 1503–1507.
- [76] E. Chatzitheodorou, A. Economou, A. Voulgaropoulos, Trace Determination of Chromium by Square-Wave Adsorptive Stripping Voltammetry on Bismuth Film Electrodes, *Electroanalysis* 16 (21) (2004) 1745–1754.
- [77] I. Svancara, P. Foret, K. Vytras, A study on the determination of chromium as chromate at a carbon paste electrode modified with surfactants, *Talanta* 64 (4) (2004) 844–852.
- [78] M. Sanchez-Fernandez, L. Cubillana-Aguilera, J. Palacios-Santander, I. Naranjo-Rodríguez, J. de Cisneros, An oxidative procedure for the electrochemical determination of chromium (VI) using modified carbon paste electrodes, *Bull. Electrochem.* 21 (12) (2005) 529.
- [79] L. Lin, N.S. Lawrence, S. Thonggamdee, J. Wang, Y. Lin, Catalytic adsorptive stripping determination of trace chromium (VI) at the bismuth film electrode, *Talanta* 65 (1) (2005) 144–148.
- [80] N.A. Carrington, L. Yong, Z.-L. Xue, Electrochemical deposition of sol-gel films for enhanced chromium (VI) determination in aqueous solutions, *Anal. Chim. Acta* 572 (1) (2006) 17–24.
- [81] S. Matsuoka, Y. Nakatsu, K. Takehara, S. Saputro, K. Yoshimura, On-line electrochemical oxidation of Cr (III) for the determination of total Cr by flow injection-solid phase spectrophotometry, *Anal. Sci.* 22 (12) (2006) 1519–1524.
- [82] M. Grabarczyk, K. Tyszczyk, M. Korolczuk, Catalytic adsorptive stripping voltammetric procedure for determination of total chromium in environmental materials, *Electroanalysis* 18 (12) (2006) 1223–1226.
- [83] G. Liu, Y.-Y. Lin, H. Wu, Y. Lin, Voltammetric detection of Cr (VI) with disposable screen-printed electrode modified with gold nanoparticles, *Environ. Sci. Technol.* 41 (23) (2007) 8129–8134.
- [84] W.W. Zhu, N.B. Li, H.Q. Luo, Simultaneous determination of chromium (III) and cadmium (II) by differential pulse anodic stripping voltammetry on a stannum film electrode, *Talanta* 72 (5) (2007) 1733–1737.
- [85] A. Manova, S. Humenikova, M. Strelec, E. Beinrohr, Determination of chromium (VI) and total chromium in water by in-electrode coulometric titration in a porous glassy carbon electrode, *Microchim. Acta* 159 (1–2) (2007) 41–47.
- [86] M.F. Bergamini, D.P. dos Santos, M.V.B. Zanon, Development of a voltammetric sensor for chromium (VI) determination in wastewater sample, *Sens. Actuators B* 123 (2) (2007) 902–908.
- [87] J.-W. Sue, C.-Y. Tai, W.-L. Cheng, J.-M. Zen, Disposable barrel plating nickel electrodes for use in flow injection analysis of trivalent chromium, *Electrochem. Commun.* 10 (2) (2008) 277–282.
- [88] B. Liu, L. Lu, M. Wang, Y. Zi, A study of nanostructured gold modified glassy carbon electrode for the determination of trace Cr (VI), *J. Chem. Sci.* 120 (5) (2008) 493–498.
- [89] O. Domínguez-Renedo, L. Ruiz-Espelt, N. García-Astorgano, M.J. Arcos-Martínez, Electrochemical determination of chromium (VI) using metallic nanoparticle-modified carbon screen-printed electrodes, *Talanta* 76 (4) (2008) 854–858.
- [90] M.-C. Tsai, P.-Y. Chen, Voltammetric study and electrochemical detection of hexavalent chromium at gold nanoparticle-electrodeposited indium tin oxide (ITO) electrodes in acidic media, *Talanta* 76 (3) (2008) 533–539.
- [91] B.K. Jena, C.R. Raj, Highly sensitive and selective electrochemical detection of sub-ppb level chromium (VI) using nano-sized gold particle, *Talanta* 76 (1) (2008) 161–165.
- [92] J. Li, J. Zhang, H. Wei, E. Wang, Combining chemical reduction with an electrochemical technique for the simultaneous detection of Cr (VI), Pb (II) and Cd (II), *Analyst* 134 (2) (2009) 273–277.
- [93] S. Xing, H. Xu, G. Shi, J. Chen, L. Zeng, L. Jin, A simple and sensitive method for the amperometric detection of trace chromium (VI) based on prussian blue modified glassy carbon electrode, *Electroanalysis* 21 (15) (2009) 1678–1684.
- [94] J. Xu, Y. Kong, W. Wang, Z. Chen, S. Yao, Determination of chromium (VI) in electronics materials using triethylamine modified carbon paste electrode, *Anal. Sci.* 25 (12) (2009) 1427–1430.
- [95] A. Calvo-Pérez, O. Domínguez-Renedo, M.A. Alonso-Lomillo, M.J. Arcos-Martínez, Simultaneous Determination of Cr (III) and Cr (VI) by Differential Pulse Voltammetry Using Modified Screen-Printed Carbon Electrodes in Array Mode, *Electroanalysis* 22 (24) (2010) 2924–2930.
- [96] E. Jorge, M. Rocha, I. Fonseca, M. Neto, Studies on the stripping voltammetric determination and speciation of chromium at a rotating-disc bismuth film electrode, *Talanta* 81 (1–2) (2010) 556–564.
- [97] S. Banerjee, P. Sarkar, Amperometric detection of hexavalent chromium with L-DOPA modified screen printed electrode, *Sens. Lett.* 9 (4) (2011) 1370–1375.
- [98] E. Mafakheri, A. Salimi, R. Hallaj, A. Ramazani, M.A. Kashi, Synthesis of iridium oxide nanotubes by electrodeposition into polycarbonate template: fabrication of chromium (III) and arsenic (III) electrochemical sensor, *Electroanalysis* 23 (10) (2011) 2429–2437.
- [99] J. Saturno, D. Valera, H. Carrero, L. Fernández, Electroanalytical detection of Pb, Cd and traces of Cr at micro/nano-structured bismuth film electrodes, *Sens. Actuators B* 159 (1) (2011) 92–96.
- [100] H. Xu, Q. Zheng, P. Yang, J. Liu, S. Xing, L. Jin, Electrochemical synthesis of silver nanoparticles-coated gold nanoporous film electrode and its application to amperometric detection for trace Cr (VI), *Sci. China Chem.* 54 (6) (2011) 1004–1010.
- [101] S. Xing, H. Xu, J. Chen, G. Shi, L. Jin, Nafion stabilized silver nanoparticles modified electrode and its application to Cr (VI) detection, *J. Electroanal. Chem.* 652 (1–2) (2011) 60–65.
- [102] R. Ouyang, S.A. Bragg, J.Q. Chambers, Z.-L. Xue, Flower-like self-assembly of gold nanoparticles for highly sensitive electrochemical detection of chromium (VI), *Anal. Chim. Acta* 722 (2012) 1–7.
- [103] A. Prakash, S. Chandra, D. Bahadur, Structural, magnetic, and textural properties of iron oxide-reduced graphene oxide hybrids and their use for the electrochemical detection of chromium, *Carbon* 50 (11) (2012) 4209–4219.
- [104] S. Fierro, T. Watanabe, K. Akai, Y. Einaga, Highly sensitive detection of Cr⁶⁺ on boron doped diamond electrodes, *Electrochim. Acta* 82 (2012) 9–11.
- [105] R. Ouyang, W. Zhang, S. Zhou, Z.-L. Xue, L. Xu, Y. Gu, Y. Miao, Improved Bi film wrapped single walled carbon nanotubes for ultrasensitive electrochemical detection of trace Cr (VI), *Electrochim. Acta* 113 (2013) 686–693.
- [106] D. Li, J. Li, X. Jia, Y. Xia, X. Zhang, E. Wang, A novel Au–Ag–Pt three-electrode microchip sensing platform for chromium (VI) determination, *Anal. Chim. Acta* 804 (2013) 98–103.
- [107] H. Li, J. Li, W. Wang, Z. Yang, Q. Xu, X. Hu, A subnanomole level photoelectrochemical sensing platform for hexavalent chromium based on its selective inhibition of quercetin oxidation, *Analyst* 138 (4) (2013) 1167–1173.
- [108] S. Sadeghi, A. Garmroodi, A highly sensitive and selective electrochemical sensor for determination of Cr (VI) in the presence of Cr (III) using modified multi-walled carbon nanotubes/quercetin screen-printed electrode, *Mater. Sci. Eng.* 33 (8) (2013) 4972–4977.
- [109] W. Jin, G. Wu, A. Chen, Sensitive and selective electrochemical detection of chromium (VI) based on gold nanoparticle-decorated titania nanotube arrays, *Analyst* 139 (1) (2014) 235–241.
- [110] C. Santhosh, M. Saranya, R. Ramachandran, S. Felix, V. Velmurugan, A. Nirmala Grace, Graphene/gold nanocomposites-based thin films as an enhanced sensing platform for voltammetric detection of Cr (VI) ions, *J. Nanotechnol.* 2014 (2014).
- [111] S.A. Miscoria, C. Jacq, T. Maeder, R.M. Negri, Screen-printed electrodes for electroanalytical sensing, of chromium VI in strong acid media, *Sens. Actuators B* 195 (2014) 294–302.
- [112] A. Attar, M.E. Ghica, A. Amine, C.M. Brett, Poly (neutral red) based hydrogen peroxide biosensor for chromium determination by inhibition measurements, *J. Hazard. Mater.* 279 (2014) 348–355.
- [113] A. Calvo-Pérez, O. Domínguez-Renedo, M. Alonso-Lomillo, M. Arcos-Martínez, Speciation of chromium using chronoamperometric biosensors based on screen-printed electrodes, *Anal. Chim. Acta* 833 (2014) 15–21.
- [114] A. Deep, A.L. Sharma, S.K. Tuteja, A. Paul, Phosphonic acid functionalized carbon nanotubes for sensitive and selective sensing of chromium (VI), *J. Hazard. Mater.* 278 (2014) 559–565.
- [115] S.A. Miscoria, C. Jacq, T. Maeder, R.M. Negri, Screen-printed electrochemical chromium (VI) sensing electrodes for effluent bioremediation monitoring, *Sens. Actuators B* 195 (ARTICLE) (2014) 294–302.
- [116] T. Ravishankar, S. Muralikrishna, G. Nagaraju, T. Ramakrishnapa, Electrochemical detection and photochemical detoxification of hexavalent chromium (Cr (vi)) by Ag doped TiO₂ nanoparticles, *Anal. Methods* 7 (8) (2015) 3493–3499.
- [117] L.E. Korshoj, A.J. Zaitouna, R.Y. Lai, Methylene blue-mediated electrocatalytic detection of hexavalent chromium, *Anal. Chem.* 87 (5) (2015) 2560–2564.
- [118] A. Salimi, B. Pourbahram, S. Mansouri-Majd, R. Hallaj, Manganese oxide nanoflakes/multi-walled carbon nanotubes/chitosan nanocomposite modified

- glassy carbon electrode as a novel electrochemical sensor for chromium (III) detection, *Electrochim. Acta* 156 (2015) 207–215.
- [119] S. Xu, X. Wang, C. Zhou, A micro electrochemical sensor based on bismuth-modified mesoporous carbon for hexavalent chromium detection. 2015 IEEE SENSORS, IEEE, 2015, pp. 1–4.
- [120] S.A. Tukur, N.A. Yusuf, R. Hajian, Linear sweep anodic stripping voltammetry: determination of Chromium (VI) using synthesized gold nanoparticles modified screen-printed electrode, *J. Chem. Sci.* 127 (6) (2015) 1075–1081.
- [121] E.A. de Oliveira Farias, M.C. dos Santos, N. de Araujo Dionisio, P.V. Quelemes, J. R.D.S.A. Leite, P. Eaton, D.A. da Silva, C. Eiras, Layer-by-Layer films based on biopolymers extracted from red seaweeds and polyaniline for applications in electrochemical sensors of chromium VI, *Mater. Sci. Eng.* 200 (2015) 9–21.
- [122] C. Liu, C. He, T. Xie, J. Yang, Reduction of graphite oxide using ammonia solution and detection Cr (VI) with graphene-modified electrode, Fullerenes, Nanotubes and Carbon Nanostruct. 23 (2) (2015) 125–130.
- [123] R.S. Moakhar, G.K.L. Goh, A. Dolati, M. Ghorbani, A novel screen-printed TiO₂ photoelectrochemical sensor for direct determination and reduction of hexavalent chromium, *Electrochem. Commun.* 61 (2015) 110–113.
- [124] J. Wei, Z. Guo, X. Chen, D.-D. Han, X.-K. Wang, X.-J. Huang, Ultrasensitive and ultrasensitive impedimetric detection of Cr (VI) using crown ethers as high-affinity targeting receptors, *Anal. Chem.* 87 (3) (2015) 1991–1998.
- [125] S. Wyantuti, Y.W. Hartati, M.L. Firdaus, C. Panatarani, R. Tjokronegoro, Fabrication of gold nanoparticles-modified glassy carbon electrode and its application for voltammetric detection of Cr (III), *Int. J. Sci. Technol. Res.* 4 (1) (2015) 135–139.
- [126] Y. Chen, Y. Dong, H. Wu, C. Chen, Y. Chi, G. Chen, Electrochemiluminescence sensor for hexavalent chromium based on the graphene quantum dots/peroxodisulfate system, *Electrochim. Acta* 151 (2015) 552–557.
- [127] P.R.S. Teixeira, A.S. do Nascimento Marreiro, E.A. de Oliveira Farias, N. A. Dionisio, E.C. Silva Filho, C. Eiras, Layer-by-layer hybrid films of phosphate cellulose and electroactive polymer as chromium (VI) sensors, *J. Solid State Electrochem.* 19 (7) (2015) 2129–2139.
- [128] Y. Peng, Y. Wang, Y. Li, X. He, Polyethyleneimine Functionalized Multi-walled Carbon Nanotubes for Electrochemical Detection of Chromium (VI), *Electroanalysis* 28 (9) (2016) 2029–2036.
- [129] H. Fourou, A. Zazoua, M. Braiek, N. Jaffrezic-Renault, An enzyme biosensor based on beta-galactosidase inhibition for electrochemical detection of cadmium (II) and chromium (VI), *Int. J. Environ. Anal. Chem.* 96 (9) (2016) 872–885.
- [130] S.M. Rosolina, S.A. Bragg, R. Ouyang, J.Q. Chambers, Z.-L. Xue, Highly sensitive detection of hexavalent chromium utilizing a sol-gel/carbon nanotube modified electrode, *J. Electroanal. Chem.* 781 (2016) 120–125.
- [131] Y. Zhang, P. Chen, F. Wen, B. Yuan, H. Wang, Fe₃O₄ nanospheres on MoS₂ nanoflake: electrocatalysis and detection of Cr (VI) and nitrite, *J. Electroanal. Chem.* 761 (2016) 14–20.
- [132] W. Wang, H. Bai, H. Li, Q. Lv, Q. Zhang, N. Bao, Carbon tape coated with gold film as stickers for bulk fabrication of disposable gold electrodes to detect Cr (VI), *Sens. Actuators B* 236 (2016) 218–225.
- [133] L. Richtera, H.V. Nguyen, D. Hynek, J. Kudr, V. Adam, Electrochemical speciation analysis for simultaneous determination of Cr (III) and Cr (VI) using an activated glassy carbon electrode, *Analyst* 141 (19) (2016) 5577–5585.
- [134] C. Wang, C.K. Chan, Carbon nanotube-based electrodes for detection of low-ppb level hexavalent chromium using amperometry, *ECS J. Solid State Sci. Technol.* 5 (8) (2016) M3026.
- [135] A. Izadyar, F. Al-Amoody, D.R. Arachchige, Ion transfer stripping voltammetry to detect nanomolar concentrations of Cr (VI) in drinking water, *J. Electroanal. Chem.* 782 (2016) 43–49.
- [136] S. Wu, N.C. Sekar, S.N. Tan, H. Xie, S.H. Ng, Determination of chromium (III) by differential pulse stripping voltammetry at a chitosan-gold nanocomposite modified screen printed electrode, *Anal. Methods* 8 (5) (2016) 962–967.
- [137] T. Fang, X. Yang, L. Zhang, J. Gong, Ultrasensitive photoelectrochemical determination of chromium (VI) in water samples by ion-imprinted/formate anion-incorporated graphitic carbon nitride nanostructured hybrid, *J. Hazard. Mater.* 312 (2016) 106–113.
- [138] E. Punrat, C. Maksuk, S. Chuanuwatanakul, W. Wonsawat, O. Chailapakul, Polyaniline/graphene quantum dot-modified screen-printed carbon electrode for the rapid determination of Cr (VI) using stopped-flow analysis coupled with voltammetric technique, *Talanta* 150 (2016) 198–205.
- [139] T.N. Ravishankar, M.D.O. Vaz, T. Ramakrishnappa, S.R. Teixeira, J. Dupont, Ionic liquid assisted hydrothermal syntheses of Au doped TiO₂ 2 NPs for efficient visible-light photocatalytic hydrogen production from water, electrochemical detection and photochemical detoxification of hexavalent chromium (Cr 6+), *RSC Adv.* 7 (68) (2017) 43233–43244.
- [140] W. Wang, H. Bai, H. Li, Q. Lv, Z. Wang, Q. Zhang, Disposable plastic electrode for electrochemical determination of total chromium and hexavalent chromium, *J. Electroanal. Chem.* 794 (2017) 148–155.
- [141] T. Alizadeh, F. Rafiei, N. Hamidi, M.R. Ganjali, A new electrochemical sensing platform for Cr (III) determination based on nano-structured Cr (III)-imprinted polymer-modified carbon composite electrode, *Electrochim. Acta* 247 (2017) 812–819.
- [142] D.C. Prabhakaran, J. Riotte, Y. Sivry, S. Subramanian, Electroanalytical detection of Cr (VI) and Cr (III) ions using a novel microbial sensor, *Electroanalysis* 29 (5) (2017) 1222–1231.
- [143] D. Liu, L. Ji, Y. Ding, X. Weng, F. Yang, X. Zhang, Mesoporous carbon black as a metal-free electrocatalyst for highly effective determination of chromium (VI), *J. Electroanal. Chem.* 803 (2017) 58–64.
- [144] J. Liu, Y. Ding, L. Ji, X. Zhang, F. Yang, J. Wang, W. Kang, Highly sensitive detection of Cr (VI) in groundwater by bimetallic NiFe nanoparticles, *Anal. Methods* 9 (6) (2017) 1031–1037.
- [145] J. Tu, Y. Gan, T. Liang, H. Wan, P. Wang, A miniaturized electrochemical system for high sensitive determination of chromium (VI) by screen-printed carbon electrode with gold nanoparticles modification, *Sens. Actuators B* 272 (2018) 582–588.
- [146] T.K. Sari, F. Takahashi, J. Jin, R. Zein, E. Munaf, Electrochemical determination of chromium (VI) in river water with gold nanoparticles-graphene nanocomposites modified electrodes, *Anal. Sci.* 34 (2) (2018) 155–160.
- [147] S. Wu, X. Dai, T. Cheng, S. Li, Highly sensitive and selective ion-imprinted polymers based on one-step electrodeposition of chitosan-graphene nanocomposites for the determination of Cr (VI), *Carbohydr. Polym.* 195 (2018) 199–206.
- [148] S. Nellaippan, A.S. Kumar, A bipotentiostat based separation-free method for simultaneous flow injection analysis of chromium (III) and (VI) species, *Electrochim. Acta* 273 (2018) 248–256.
- [149] N. Hilali, A. Ghanam, H. Mohammadi, A. Amine, J.J. García-Guzmán, L. Cubillana-Aguilera, J.M. Palacios-Santander, Comparison between modified and unmodified carbon paste electrodes for hexavalent chromium determination, *Electroanalysis* 30 (11) (2018) 2750–2759.
- [150] Z. Stojanović, Z. Koudelkova, E. Sedláčková, D. Hynek, L. Richtera, V. Adam, Determination of chromium (VI) by anodic stripping voltammetry using a silver-plated glassy carbon electrode, *Anal. Methods* 10 (24) (2018) 2917–2923.
- [151] J. Hu, Y. Liu, G. Gao, X. Zou, One-step synthesis of AuPdNPs/ERGO nanocomposite for enhanced electrochemical sensing of Cr (VI) in water, *J. Electrochem. Soc.* 165 (16) (2018) B893.
- [152] A. Aravind, M. Sebastian, B. Mathew, Green synthesized unmodified silver nanoparticles as a multi-sensor for Cr (iii) ions, *Environ. Sci.* 4 (10) (2018) 1531–1542.
- [153] K. Tyszczuk-Rotko, K. Madejska, K. Domańska, Ultrasensitive hexavalent chromium determination at bismuth film electrode prepared with mediator, *Talanta* 182 (2018) 62–68.
- [154] Y. Liu, G. Gao, J. Hu, X. Zou, Electrodeposited AuNPs/rGO nanocomposite as sensor for Cr (VI) determination in water, *Int. J. Electrochem. Sci.* 13 (2018) 11853–11866.
- [155] M.A. Hussein, A.A. Ganash, S.A. Alqarni, Electrochemical sensor-based gold nanoparticle/poly (aniline-co-o-toluidine)/graphene oxide nanocomposite modified electrode for hexavalent chromium detection: a real test sample, *Polym.-Plast. Technol. Mater.* 58 (13) (2019) 1423–1436.
- [156] B. Kowsalya, V.A. Thampi, V. Sivakumar, B. Subramanian, Electrochemical detection of Chromium (VI) using NiO nanoparticles, *J. Mater. Sci. Mater. Electron.* 30 (15) (2019) 14755–14761.
- [157] H. Filik, A.A. Avan, Dextran modified magnetic nanoparticles based solid phase extraction coupled with linear sweep voltammetry for the speciation of Cr(VI) and Cr(III) in tea, coffee, and mineral water samples, *Food Chem.* 292 (2019) 151–159.
- [158] C.B. Breslin, D. Branagan, L.M. Garry, Electrochemical detection of Cr (VI) with carbon nanotubes decorated with gold nanoparticles, *J. Appl. Electrochem.* 49 (2) (2019) 195–205.
- [159] L. Zhu, M. Miao, X. Shao, Z. Du, K. Huang, Y. Luo, W. Xu, A universal electrochemical biosensor using nick-HCR nanostructure as molecular gate of nanochannel for detecting Chromium (III) ions and microRNA, *Anal. Chem.* 91 (23) (2019) 14992–14999.
- [160] L. Fu, Z. Liu, J. Ge, M. Guo, H. Zhang, F. Chen, W. Su, A. Yu, 001) plan manipulation of α -Fe₂O₃ nanostructures for enhanced electrochemical Cr (VI) sensing, *J. Electroanal. Chem.* 841 (2019) 142–147.
- [161] G. Chen, J. Xie, Z. Zhang, W. Meng, C. Zhang, K. Kang, Y. Wu, Z. Guo, A portable digital-control electrochemical system with automatic ohmic drop compensation for fast scan voltammetry and its application to ultrasensitive detection of chromium (III), *Sens. Actuators B* 301 (2019), 127135.
- [162] D.P. Jaihindh, B. Thirumalraj, S.-M. Chen, P. Balasubramanian, Y.-P. Fu, Facile synthesis of hierarchically nanostructured bismuth vanadate: an efficient photocatalyst for degradation and detection of hexavalent chromium, *J. Hazard. Mater.* 367 (2019) 647–657.
- [163] Y. Xu, W. Zhang, X. Huang, J. Shi, X. Zou, Z. Li, X. Cui, Adsorptive stripping voltammetry determination of hexavalent chromium by a pyridine functionalized gold nanoparticles/three-dimensional graphene electrode, *Microchem. J.* 149 (2019), 104022.
- [164] M. Li, R. He, S. Wang, C. Feng, H. Wu, H. Mei, Visible light driven photoelectrochemical sensor for chromium (VI) by using BiOI microspheres decorated with metallic bismuth, *Microchim. Acta* 186 (6) (2019) 345.
- [165] G. Bhanjana, P. Rana, G.R. Chaudhary, N. Dilbaghi, K.-H. Kim, S. Kumar, Manganese oxide nanochips as a novel electrocatalyst for direct redox sensing of hexavalent chromium, *Sci. Rep.* 9 (1) (2019) 1–10.
- [166] M.-O. Park, K.-D. Seo, Y.-B. Shim, J.-H. Yoon, D.-S. Park, Chromium (VI) sensor based on catalytic reduction using the nanoporous layer of poly (aminopyrimidyl-terthiophene) and AuNi composite, *Sens. Actuators B* 301 (2019), 127151.
- [167] M. Shahbakhsh, M. Noroozifar, Ultra-trace determination of hexavalent chromium by novel two dimensional biphenol-biphenolquinone nanoribbons/silver nanoparticles, *Sens. Actuators B* 281 (2019) 1023–1033.
- [168] S. Aralekallu, M. Palanna, S. Hadimani, K.P. CP, V.A. Sajjan, M.O. Thotiyl, L. K. Sanegowda, Biologically inspired catalyst for electrochemical reduction of hazardous hexavalent chromium, *Dalton Trans.* 49 (42) (2020) 15061–15071.
- [169] H. Filik, A.A. Avan, Neutral red interlinked gold nanoparticles/multiwalled carbon nanotubes modified electrochemical sensor for simultaneous speciation

- and detection of chromium (VI) and vanadium (V) in water samples, *Microchem. J.* 158 (2020), 105242.
- [170] A. Karthika, S. Nikhil, A. Suganthi, M. Rajarajan, A facile sonochemical approach based on graphene carbon nitride doped silver molybdate immobilized nafion for selective and sensitive electrochemical detection of chromium (VI) in real sample, *Adv. Powder Technol.* 31 (5) (2020) 1879–1890.
- [171] X. Xin, N. Hu, Y. Ma, Y. Wang, L. Hou, H. Zhang, Z. Han, Polyoxometalate-based crystalline materials as a highly sensitive electrochemical sensor for detecting trace Cr (vi), *Dalton Trans.* 49 (14) (2020) 4570–4577.
- [172] Y. Xu, C. Xiong, C. Gao, Y. Li, C. Bian, S. Xia, Cathodically Pretreated AuNPs-BDD Electrode for Detection of Hexavalent Chromium, *Micromachines* 11 (12) (2020) 1095.
- [173] J.-Q. Niu, Y.-Y. Ma, X. Xin, Z.-G. Han, Rare Earth Ion Encapsulated Basket-like {GdC P6MoV2MoVI16O73} Cage as Efficient Electrochemical Sensor and Fluorescent Probe for Cr (VI), *Cryst. Growth Des.* 20 (6) (2020) 3584–3589.
- [174] D.C. Prabhakaran, P.C. Ramamurthy, Y. Sivry, S. Subramanian, Electrochemical detection of Cr (VI) and Cr (III) ions present in aqueous solutions using bio-modified carbon paste electrode: a voltammetric study, *Int. J. Environ. Anal. Chem.* (2020) 1–21.
- [175] C.M. Stern, D.W. Hayes, L.O. Kgoadi, N. Elgrishi, Emerging investigator series: carbon electrodes are effective for the detection and reduction of hexavalent chromium in water, *Environ. Sci.* 6 (5) (2020) 1256–1261.
- [176] M.M. Hussain, A.M. Asiri, M.N. Arshad, M.M. Rahman, Synthesis, characterization, and crystal structure of (E)-N-(4-Bromobenzylidene)-benzenesulfonohydrazide and its application as a sensor of chromium ion detection from environmental samples, *J. Mol. Struct.* 1207 (2020), 127810.
- [177] Y. Gao, B. Feng, L. Miao, Y. Chen, J. Di, Determination of Cr (III) ions based on plasmonic sensing and anodic stripping voltammetry with amplification of Ag nanoparticles, *Microchem. J.* 157 (2020), 104995.
- [178] R. Chen, R. Tang, C. Chen, Photoelectrochemical detection of chromium (VI) using layered MoS₂ modified BiOI, *J. Chem. Sci.* 132 (1) (2020) 1–9.
- [179] G. Kaleli-Can, B. Ozlu, H.F. Özgüzar, B. Onal-Ulusoy, G. Kabay, T. Eom, B.S. Shim, M. Mutlu, Natural Melanin Nanoparticle-decorated Screen-printed Carbon Electrode: performance Test for Amperometric Determination of Hexavalent Chromium as Model Trace, *Electroanalysis* 32 (8) (2020) 1696–1706.
- [180] J. Guo, W. Feng, P. Du, R. Zhang, J. Liu, Y. Liu, Z. Wang, X. Lu, Aggregation-induced electrochemiluminescence of tetraphenylbenzosilole derivatives in an aqueous phase system for ultrasensitive detection of hexavalent chromium, *Anal. Chem.* 92 (21) (2020) 14838–14845.
- [181] Q. Liu, J. Kim, T. Cui, A highly sensitive photoelectrochemical sensor with polarity-switchable photocurrent for detection of trace hexavalent chromium, *Sens. Actuators B* 317 (2020), 128181.
- [182] P. Sanchayanukun, S. Muncharoen, Chitosan coated magnetite nanoparticle as a working electrode for determination of Cr (VI) using square wave adsorptive cathodic stripping voltammetry, *Talanta* 217 (2020), 121027.
- [183] D. Cheng, H. Wu, C. Feng, Y. Zhang, Y. Ding, H. Mei, Highly sensitive detection of chromium (VI) by photoelectrochemical sensor based on pn heterojunction of carbon nitride-modified BiOI, *J. Alloys Compd.* (2021), 160690.
- [184] G. Zhang, D. Cheng, M. Li, C. Feng, H. Wu, H. Mei, Enhanced the photoelectrochemical performance of Bi₂XO₆ (X= W, Mo) for detecting hexavalent chromium by modification of CuS, *J. Environ. Sci.* 103 (2021) 185–195.
- [185] K. Zhao, L. Ge, T.I. Wong, X. Zhou, G. Lisak, Gold-silver nanoparticles modified electrochemical sensor array for simultaneous determination of chromium (III) and chromium (VI) in wastewater samples, *Chemosphere* 281 (2021), 130880.
- [186] S.Y. Ejeta, T. Imae, Selective colorimetric and electrochemical detections of Cr (III) pollutant in water on 3-mercaptopropionic acid-functionalized gold plasmon nanoparticles, *Anal. Chim. Acta* 1152 (2021), 338272.
- [187] M. Bagherzadeh, Z. Hadizadeh, Z. Akrami, Z.S. Ghahfarokhi, Electrochemical detection of Cr (III) and Cr (VI) in solution by using ZrO₂ modified magnetic nanoparticles by redox probes, *Mater. Sci. Semicond. Process.* 131 (2021), 105840.
- [188] X. Chen, X.-X. Ke, Y. Liu, R. Weerasooriya, H. Li, Y.-C. Wu, Photocatalytically induced Au/mpg-C₃N₄ nanocomposites for robust electrochemical detection of Cr (VI) in tannery wastewater, *J. Environ. Chem. Eng.* 9 (1) (2021), 104642.
- [189] Y. Wang, J.-X. Ma, Y. Zhang, N. Xu, X.-L. Wang, A Series of Cobalt-Based Coordination Polymer Crystalline Materials as Highly Sensitive Electrochemical Sensors for Detecting Trace Cr (VI), Fe (III) Ions, and Ascorbic Acid, *Cryst. Growth Des.* 21 (8) (2021) 4390–4397.
- [190] T.K. Sari, R. Riga, M. Zubir, Pencil Lead Electrode Modified with Gold Thin Layer for Voltammetric Detection of Chromium (VI), *Eksakta: Berkala Ilmiah Bidang MIPA (E-ISSN: 2549-7464)* 22 (2) (2021) 145–153.
- [191] S. Sahoo, A. Satpati, Fabrication of rGO/NiS/AuNCs ternary nanocomposite modified electrode for electrochemical sensing of Cr (VI) at ultra-trace level, *Surf. Interfaces* 24 (2021), 101096.
- [192] D. Fang, T. Xu, L. Fang, H. Chen, Y. Huang, H. Zhang, Z. Miao, C. Mao, B. Chi, H. Xu, A blood compatible, high-efficient sensor for detection of Cr (VI) in whole blood, *Sens. Actuators B* 329 (2021), 129219.
- [193] M.H. Motaghefard, S.M. Pourmortazavi, S. Mirsadeghi, Selective and sensitive detection of Cr (VI) pollution in waste water via polyaniline/sulfated zirconium dioxide/multi walled carbon nanotubes nanocomposite based electrochemical sensor, *Sens. Actuators B* 327 (2021), 128882.
- [194] J.-Q. Niu, W.-T. An, X.-J. Zhang, Y.-Y. Ma, Z.-G. Han, Ultra-trace determination of hexavalent chromium in a wide pH range triggered by heterometallic Cu-Mn centers modified reduced phosphomolybdate hybrids, *Chem. Eng. J.* 418 (2021), 129408.
- [195] G. Reynolds, H. Shalgosky, T. Webber, The polarographic behaviour of some elements in concentrated calcium chloride solution: the development of a method for the determination of metallic impurities in calcium metal, *Anal. Chim. Acta* 10 (1954) 192–200.
- [196] F. Scholz, B. Lange, M. Draheim, J. Pelzer, The catalytic adsorptive stripping voltammetric determination of chromium with DTPA and nitrate, *Fresenius. J. Anal. Chem.* 338 (5) (1990) 627–629.
- [197] M. Boussemart, C.M.G. van den Berg, M. Ghaddaf, The determination of the chromium speciation in sea water using catalytic cathodic stripping voltammetry, *Anal. Chim. Acta* 262 (1) (1992) 103–115.
- [198] A.M. Dobney, G.M. Greenway, On-line determination of chromium by adsorptive cathodic stripping voltammetry, *Analyst* 119 (2) (1994) 293–297.
- [199] J. Wang, J. Wang, J. Lu, B. Tian, D. MacDonald, K. Olsen, Flow probe for in situ electrochemical monitoring of trace chromium, *Analyst* 124 (3) (1999) 349–352.
- [200] S. Sander, T. Navrátil, L. Novotný, Study of the Complexation, Adsorption and Electrode Reaction Mechanisms of Chromium(VI) and (III) with DTPA under Adsorptive Stripping Voltammetric Conditions, *Electroanalysis* 15 (19) (2003) 1513–1521.
- [201] A. García-Miranda Ferrari, P. Carrington, S.J. Rowley-Neale, C.E. Banks, Recent advances in portable heavy metal electrochemical sensing platforms, *Environ. Sci.* 6 (10) (2020) 2676–2690.
- [202] J. Wang, *Stripping Analysis, Encyclopedia of Electrochemistry* 2007.
- [203] A.J. Borrill, N.E. Reily, J.V. Macpherson, Addressing the practicalities of anodic stripping voltammetry for heavy metal detection: a tutorial review, *Analyst* 144 (23) (2019) 6834–6849.
- [204] W. Jin, K. Yan, Recent advances in electrochemical detection of toxic Cr(vi), *RSC Adv.* 5 (47) (2015) 37440–37450.
- [205] J. Wang, *Analytical electrochemistry*, 2006.
- [206] A. Hayat, J.L. Marty, Disposable Screen Printed Electrochemical Sensors: tools for Environmental Monitoring, *Sensors* 14 (6) (2014) 10432–10453.
- [207] R.W. Murray, A.G. Ewing, R.A. Durst, Chemically modified electrodes. Molecular design for electroanalysis, *Anal. Chem.* 59 (5) (1987) 379A–390A.
- [208] U. Yogeswaran, S.-M. Chen, A Review on the Electrochemical Sensors and Biosensors Composed of Nanowires as Sensing Material, *Sensors* 8 (1) (2008) 290–313.
- [209] I. Moldoveanu, R.-I. van Stefan-Staden, J.F. van Staden, Electrochemical Sensors Based on Nanostructured Materials, in: M. Aliofkhaezrai, A.S.H. Makhlof (Eds.), *Handbook of Nanoelectrochemistry: Electrochemical Synthesis Methods, Properties and Characterization Techniques*, Springer International Publishing, Cham, 2016, pp. 1–15.
- [210] P. Zanello, G. Raspi, Electrooxidation of chromium(III) in alkaline hydroxide solution at a platinum electrode, *Anal. Chim. Acta* 88 (2) (1977) 237–243.
- [211] F.I. Danilov, A.B. Velichenko, Electrocatalytic activity of anodes in reference to Cr (III) oxidation reaction, *Electrochim. Acta* 38 (2) (1993) 437–440.
- [212] R.-I. Stefan, S.G. Bairu, J.F. van Staden, Diamond paste-based electrodes for determination of Cr(III) in pharmaceutical compounds, *Anal. Bioanal. Chem.* 376 (6) (2003) 844–847.
- [213] C.M.A. Brett, O.M.S. Filipe, C.S. Neves, Determination of Chromium(VI) by Batch Injection Analysis and Adsorptive Stripping Voltammetry, *Anal. Lett.* 36 (5) (2003) 955–969.
- [214] A.M. O'Mahony, M.D. Scanlon, A. Berduque, V. Beni, D.W.M. Arrigan, E. Faggi, A. Bencini, Voltammetry of chromium(VI) at the liquid|liquid interface, *Electrochem. Commun.* 7 (10) (2005) 976–982.
- [215] V.S. Bagotsky, *Fundamentals of Electrochemistry*, 2005.
- [216] J. Wang, *Analytical electrochemistry /Joseph Wang*, 2006.
- [217] A. Economou, Screen-Printed Electrodes Modified with "Green" Metals for Electrochemical Stripping Analysis of Toxic Elements, *Sensors (Basel)* 18 (4) (2018) 1032.
- [218] K. Zhao, L. Ge, T.I. Wong, X. Zhou, G. Lisak, Gold-silver nanoparticles modified electrochemical sensor array for simultaneous determination of chromium(III) and chromium(VI) in wastewater samples, *Chemosphere* 281 (2021), 130880.
- [219] L. Alves, B. Ballesteros, M. Boronat, J.R. Cabrero-Antonino, P. Concepción, A. Corma, M.A. Correa-Duarte, E. Mendoza, Synthesis and Stabilization of Subnanometric Gold Oxide Nanoparticles on Multiwalled Carbon Nanotubes and Their Catalytic Activity, *J. Am. Chem. Soc.* 133 (26) (2011) 10251–10261.
- [220] M. Yang, L.F. Allard, M. Flytzani-Stephanopoulos, Atomically Dispersed Au-(OH) x Species Bound on Titania Catalyze the Low-Temperature Water-Gas Shift Reaction, *J. Am. Chem. Soc.* 135 (10) (2013) 3768–3771.
- [221] S. Dutta, G. Strack, P. Kurup, Gold nanostar-based voltammetric sensor for chromium (VI), *Microchim. Acta* 186 (11) (2019) 1–7.
- [222] L.D. Burke, P.F. Nugent, Dichromate reduction on gold and platinum electrodes in aqueous acid solutions, *Electrochim. Acta* 42 (3) (1997) 399–411.
- [223] K. Sohn, F. Kim, K.C. Pradel, J. Wu, Y. Peng, F. Zhou, J. Huang, Construction of Evolutionary Tree for Morphological Engineering of Nanoparticles, *ACS Nano* 3 (8) (2009) 2191–2198.
- [224] W. Jin, G. Wu, A. Chen, Sensitive and selective electrochemical detection of chromium(vi) based on gold nanoparticle-decorated titania nanotube arrays, *Analyst* 139 (1) (2014) 235–241.
- [225] A. Manova, S. Humenikova, M. Strelec, B. Ernest, Determination of chromium(VI) and total chromium in water by in-electrode coulometric titration in a porous glassy carbon electrode, *Microchim. Acta* 159 (2007) 41–47.
- [226] S. Xing, H. Xu, G. Shi, J. Chen, L. Zeng, L. Jin, A Simple and Sensitive Method for the Amperometric Detection of Trace Chromium(VI) Based on Prussian Blue Modified Glassy Carbon Electrode, *Electroanalysis* 21 (2009) 1678–1684.
- [227] D. Zhang, K. Zhang, Y.L. Yao, X.H. Xia, H.Y. Chen, Multilayer Assembly of Prussian Blue Nanoclusters and Enzyme-Immobilized Poly(toluidine blue) Films

- and Its Application in Glucose Biosensor Construction, *Langmuir* 20 (17) (2004) 7303–7307.
- [228] S. Han, Y. Chen, R. Pang, P. Wan, M. Fan, Fabrication of Prussian Blue/Multiwalled Carbon Nanotubes/Glass Carbon Electrode through Sequential Deposition, *Ind. Eng. Chem. Res.* 46 (21) (2007) 6847–6851.
- [229] S.K.S. M, K. Pillai, A kinetic study of the electrocatalytic oxidation of reduced glutathione at Prussian blue film-modified electrode using rotating-disc electrode voltammetry, *Electrochim. Acta* 54 (2009) 7374–7381.
- [230] G.L. de Lara González, H. Kahlert, F. Scholz, Catalytic reduction of hydrogen peroxide at metal hexacyanoferrate composite electrodes and applications in enzymatic analysis, *Electrochim. Acta* 52 (5) (2007) 1968–1974.
- [231] O. Domínguez Renedo, M.A. Alonso Lomillo, M.J. Arcos Martínez, Optimisation procedure for the inhibitive determination of chromium(III) using an amperometric tyrosinase biosensor, *Anal. Chim. Acta* 521 (2) (2004) 215–221.
- [232] M.E. Sánchez-Fernández, L. Cubillana-Aguilera, J. Palacios Santander, I. Naranjo-Rodríguez, J.L. Cisneros, An oxidative procedure for the electrochemical determination of chromium(VI) using modified carbon paste electrodes, *Bull. Electrochem.* 21 (2005) 529–535.
- [233] A. García-Miranda Ferrari, O. Amor-Gutiérrez, E. Costa-Rama, M.T. Fernández-Abedul, Batch injection electroanalysis with stainless-steel pins as electrodes in single and multiplexed configurations, *Sens. Actuators B* 253 (2017) 1207–1213.
- [234] P.M. Hallam, D.K. Kampouris, R.O. Kadara, C.E. Banks, Graphite screen printed electrodes for the electrochemical sensing of chromium(vi), *Analyst* 135 (8) (2010) 1947–1952.
- [235] M.J. Whittingham, N.J. Hurst, R.D. Crapnell, A. García-Miranda Ferrari, E. Blanco, T.J. Davies, C.E. Banks, Electrochemical Improvements Can Be Realized via Shortening the Length of Screen-Printed Electrochemical Platforms, *Anal. Chem.* 93 (49) (2021) 16481–16488.
- [236] R.A. Sánchez-Moreno, M.J. Gismera, M.T. Sevilla, J.R. Procopio, Screen-printed sensor for batch and flow injection potentiometric chromium(VI) monitoring, *Anal. Bioanal. Chem.* 397 (1) (2010) 331–338.
- [237] A.J. Bard, Chemical modification of electrodes, *J. Chem. Educ.* 60 (4) (1983) 302.
- [238] O. Domínguez-Renedo, L. Ruiz-Espelt, N. García-Astorgano, M.J. Arcos-Martínez, Electrochemical determination of chromium(VI) using metallic nanoparticle-modified carbon screen-printed electrodes, *Talanta* 76 (4) (2008) 854–858.
- [239] A. Calvo-Pérez, O. Domínguez-Renedo, M.A. Alonso-Lomillo, M.J. Arcos-Martínez, Simultaneous Determination of Cr(III) and Cr(VI) by Differential Pulse Voltammetry Using Modified Screen-Printed Carbon Electrodes in Array Mode, *Electroanalysis* 22 (24) (2010) 2924–2930.
- [240] J. Tu, Y. Gan, T. Liang, H. Wan, P. Wang, A miniaturized electrochemical system for high sensitive determination of chromium(VI) by screen-printed carbon electrode with gold nanoparticles modification, *Sens. Actuators B* 272 (2018) 582–588.
- [241] H. Xu, Q. Zheng, P. Yang, J. Liu, S. Xing, L. Jin, Electrochemical synthesis of silver nanoparticles-coated gold nanoporous film electrode and its application to amperometric detection for trace Cr(VI), *Sci. China-Chem. - SCI CHINA-CHEM* 54 (2011) 1004–1010.
- [242] R.D. Crapnell, C.E. Banks, Electroanalytical overview: utilising micro-and nano-dimensional sized materials in electrochemical-based biosensing platforms, *Microchim. Acta* 188 (8) (2021) 1–23.
- [243] K. Lee, A. Ambrosi, M. Pumera, 3D-Printed metal electrodes for heavy metals detection by anodic stripping voltammetry, *Electroanalysis* 29 (2017).
- [244] J.G. Walters, S. Ahmed, I.M. Terrero Rodríguez, G.D. O’Neil, Trace Analysis of Heavy Metals (Cd, Pb, Hg) Using Native and Modified 3D Printed Graphene/Poly (Lactic Acid) Composite Electrodes, *Electroanalysis* 32 (4) (2020) 859–866.
- [245] D.P. Rocha, A.L. Squizzato, S.M. da Silva, E.M. Richter, R.A. Munoz, Improved electrochemical detection of metals in biological samples using 3D-printed electrode: chemical/electrochemical treatment exposes carbon-black conductive sites, *Electrochim. Acta* 335 (2020), 135688.
- [246] C. Kokkinos, A. Economou, A. Pournara, M. Manos, I. Spanopoulos, M. Kanatzidis, T. Tziotzi, V. Petkov, A. Margariti, P. Oikonomopoulos, G.S. Papaefstathiou, 3D-printed lab-in-a-syringe voltammetric cell based on a working electrode modified with a highly efficient Ca-MOF sorbent for the determination of Hg(II), *Sens. Actuators B* 321 (2020), 128508.
- [247] C.W. Foster, H.M. Elbardisy, M.P. Down, E.M. Keefe, G.C. Smith, C.E. Banks, Additively manufactured graphitic electrochemical sensing platforms, *Chem. Eng. J.* 381 (2020), 122343.
- [248] E.M. Richter, D.P. Rocha, R.M. Cardoso, E.M. Keefe, C.W. Foster, R.A.A. Munoz, C.E. Banks, Complete Additively Manufactured (3D-Printed) Electrochemical Sensing Platform, *Anal. Chem.* 91 (20) (2019) 12844–12851.
- [249] R.D. Crapnell, E. Bernalte, A.G.-M. Ferrari, M.J. Whittingham, R.J. Williams, N. J. Hurst, C.E. Banks, All-in-One Single-Print Additively Manufactured Electroanalytical Sensing Platforms, *ACS Meas. Sci. Au* (2021).