

Federation University ResearchOnline

<https://researchonline.federation.edu.au>

Copyright Notice

This is the published version of:

Unsworth, Chua, J., & Gudimetla, P. (2020). A 3D Measurement and Computerized Meshing Study to Promote Bus Ridership Among People Using Powered Mobility Aids. *Frontiers in Built Environment*, 6.

Available online: <https://doi.org/10.3389/fbuil.2020.00090>

Copyright © 2020 Unsworth, Chua and Gudimetla. This is an open-access article distributed under the terms of the Creative Commons Attribution License (CC BY 4.0) (<https://creativecommons.org/licenses/by/4.0/>). The use, distribution or reproduction in other forums is permitted, provided the original author(s) or licensor are credited and that the original publication in this journal is cited, in accordance with accepted academic practice. No use, distribution or reproduction is permitted which does not comply with these terms.

See this record in Federation ResearchOnline at:

<http://researchonline.federation.edu.au/vital/access/HandleResolver/1959.17/184153>



A 3D Measurement and Computerized Meshing Study to Promote Bus Ridership Among People Using Powered Mobility Aids

Carolyn A. Unsworth^{1,2*}, Julian Chua¹ and Prasad Gudimetla³

¹ Department of Exercise and Health Sciences, School of Health Medical and Applied Sciences, CQUniversity, Melbourne, VIC, Australia, ² Department of Rehabilitation, School of Health and Welfare, Jönköping University, Jönköping, Sweden, ³ School of Engineering and Technology, CQUniversity, Bundaberg, QLD, Australia

OPEN ACCESS

Edited by:

Richard Tay,
RMIT University, Australia

Reviewed by:

Amiruddin Bin Ismail,
Universiti Kebangsaan
Malaysia, Malaysia
Jonathan M. Bunker,
Queensland University of
Technology, Australia

*Correspondence:

Carolyn A. Unsworth
c.unsworth@cqu.edu.au

Specialty section:

This article was submitted to
Transportation and Transit Systems,
a section of the journal
Frontiers in Built Environment

Received: 28 March 2020

Accepted: 18 May 2020

Published: 17 June 2020

Citation:

Unsworth CA, Chua J and
Gudimetla P (2020) A 3D
Measurement and Computerized
Meshing Study to Promote Bus
Ridership Among People Using
Powered Mobility Aids.
Front. Built Environ. 6:90.
doi: 10.3389/fbuil.2020.00090

People who use powered mobility aids such as wheelchairs and scooters need and want to use public transport. Buses are the most affordable and efficient form of public transport, capable of connecting people across local communities. However, with curbside rather than platform boarding and internal space limitations, buses also present many accessibility challenges for people using mobility aids during ingress, egress, and interior maneuverability. In Australia, people using mobility aids board low floor buses that are required to comply with the national bus accessibility standard, using the front doors. A new standard was recently created to provide a Blue Label identification for powered mobility aids suitable to access public transport. The accuracy of this standard to identify mobility aids suitable to use on buses has not been verified. This research used a world-first methodology that included 3-Dimensional (3D) scanning of 35 mobility aids and 21 buses. The resulting 735 scan combinations were efficiently meshed using Meshlab, an open-source software. The research demonstrated that (i) although none of the buses were compliant with the relevant standard in 3D, many could still facilitate the boarding of a variety of mobility aids, and (ii) the Blue Label, while a valuable guide, did not accurately identifying all mobility aids that would and would not be able to board buses. This research has shortlisted nine mobility aids that can be recommended to consumers as being able to fit all the full-size buses tested. The dimensions of mobility aids that appear to enable access on most buses were also identified for consumers to consider when purchasing a mobility aid. The novel 3D meshing methodology used in this research also revealed that most collision points between mobility aids and buses occur in the curved-corridor entry of the buses. To minimize this entry problem, future bus boarding designs should consider the option of double-door entry/exit in the middle of the bus, which is common in many other countries. Adoption of this strategy would mitigate some of the challenges that people using mobility aids encounter when accessing buses, thereby increasing public transport ridership among this group.

Keywords: public transport, wheelchair, mobility scooter, disability, 3D scanning, accessibility

INTRODUCTION



Conservative estimates suggest that over 1 million Australians use a 3- or 4-wheeled powered or unpowered wheelchair or mobility scooter (Australian Bureau of Statistics (ABS), 2016), and that every day, ~4.3 million people in the UK (Office of Fair Trading, 2011) and 7.8 million people in the USA use wheelchairs or scooters or other mobility aids including walking sticks (also called canes), crutches or walkers (La Plante and Kaye, 2010). The number of people using any of these mobility aids internationally is expected to rise as the population ages and an increasing number of people turn to these devices to maintaining community mobility, and age in place (Grimmer et al., 2015). Given the affordability and efficiency of public transport, many people using mobility aids need and want to use this method of transport to access services, participate in community activities and spend time with friends and family (Pyer and Tucker, 2014; Steinfeld et al., 2018). However, increasing public transport ridership for this large and growing group relies people being able to use their mobility aid to safely board and maneuver within the conveyance.

Buses are an affordable and convenient form of public transport that have wide reach into the heart of local communities, yet they present many access challenges for people using mobility aids (May et al., 2010; Park and Chowdhury, 2018). A survey undertaken with 67 people who use mobility aids identified that the most important features when choosing a mobility aid were reliability and turning ability, both of which are essential attributes for accessibility on buses (Unsworth et al., 2019a). Survey participants identified that getting their mobility aid in and out of the bus and using the aid within the bus were particularly problematic due to the size of the mobility aid and accessories such as shopping baskets, and the interior space of the bus. This finding was reinforced by a systematic review of public transport access for people using mobility aids (Unsworth et al., 2019b). Of the 26 studies included in the review, 24 included information on buses, and while 14 studies investigated user experiences, five specifically examined bus formats and floor layouts and a further five focused on bus ramps and optimal ramp designs. D'Souza et al. (2017a,b) investigated the effect of low-floor bus interior configuration and passenger crowding on boarding and disembarking efficiency and safety, as well as determining the effect of seating configuration and passenger load on physical accessibility. They reported that ramp ascent was the most difficult task for manual wheelchair users, while interior circulation was most difficult for powered mobility device users. They noted that interior configurations with boarding and disembarking from mid/rear doorways were preferred by users. Bharathy and D'Souza (2018) developed an algorithm to determine the dimensions of the clear floor area required to best accommodate people in their mobility devices in buses. This team used 3D coordinates from participants to derive estimates of width, height and depth of persons and their mobility aids, and clear floor space required. They reported that only 59.4% of people and their mobility devices could fit into current floor spaces. Frost et al. (2015) investigated factors that contributed to ramp related incidents during bus boarding/alighting of people

using mobility aids. Of their 414 participants, 4.6% ($n = 35$) had experienced a ramp-related accident. These accidents were more common when; boarding (6.3%) compared to alighting (2.2%), the ramp slope was greater than the maximum of 9.5° proposed Americans with Disabilities Act (1990), and when the ramp was deployed to street level as opposed to the sidewalk.

In Australia, access difficulties for people using mobility devices on buses continue to occur, despite the use of local access standards including the Disability Standards for Accessible Public Transport (DSAPT) (Department of Infrastructure Regional Development Australian Government, 2011; Department of Infrastructure Regional Development, 2013), AS/NZS3695 for mobility aids (Standards Australia, 2013), and AS/NZS ISO10865 for buses. Anecdotal evidence suggests that bus access problems may persist because the DSAPT reports two-dimensional (2D) measurements of floor space on vehicles for mobility aids that are driven by skilled drivers of average weight. Two dimensional measures don't account for access interference from the positioning of fare reading devices, support rails at chest height, and seat cushioning that may protrude and block what otherwise appears to be a wider clearance space for wheelchair access at 2D floor level. The DSAPT (Department of Infrastructure Regional Development Australian Government, 2011) specifies the width of a bus entrance and access corridor as 800 mm, the area designated for travel called Allocated Space as 850 mm wide minus clearance and 1,300 mm long minus clearance, with a height of 1,500 mm, and that a maneuvering area comprising a space that is that is not $<2,070$ mm width by 1,540 mm length is available for turning. This is illustrated in the aerial view presented in **Figures 1, 2**. Unlike many other countries such as Sweden and Germany where all door bus boarding is possible and enables people using mobility aids to enter via a mid or rear double door that leads directly to an allocated space, in Australia, ramp access is usually limited to front door boarding.

A new Standards Australia–Technical Specification (AS–TS) has been developed to provide mobility aids with a White Label indicating suitability for use on footpaths and/or road-related areas, or a Blue Label indicating suitability for use on footpaths and/or road-related areas as well as meeting the criteria denoting suitability for use on public transport: AS–TS 3695.3:2018 (Standards Australia, 2018). The criteria for a Blue Label are: the aid measures ≤ 740 mm wide, is $\leq 1,500$ mm, weighs ≤ 170 kg and that the mobility aid can successfully (according to 2D illustrations with measurements provided): (1) access a Swept Path (believed to represent the curved entrance of a bus); (2) travel a Narrow Access Path (the corridor from the curved entrance at the front of the bus to the designated travel area); (3) access an Allocated Space (the designated travel area); (4) complete a 180° turn within an area $2,070$ mm \times $1,540$ mm area; and (5) traverse a Pavement Gap (believed to represent crossing a light rail or rail crossing gauge gap in a pavement or road surface). These illustrations with measures are available elsewhere (Unsworth et al., under review). Of note, the AS–TS make provision that mobility aids with a diagonal length of $\leq 1,200$ mm are exempt from undertaking the Allocated Space Test.

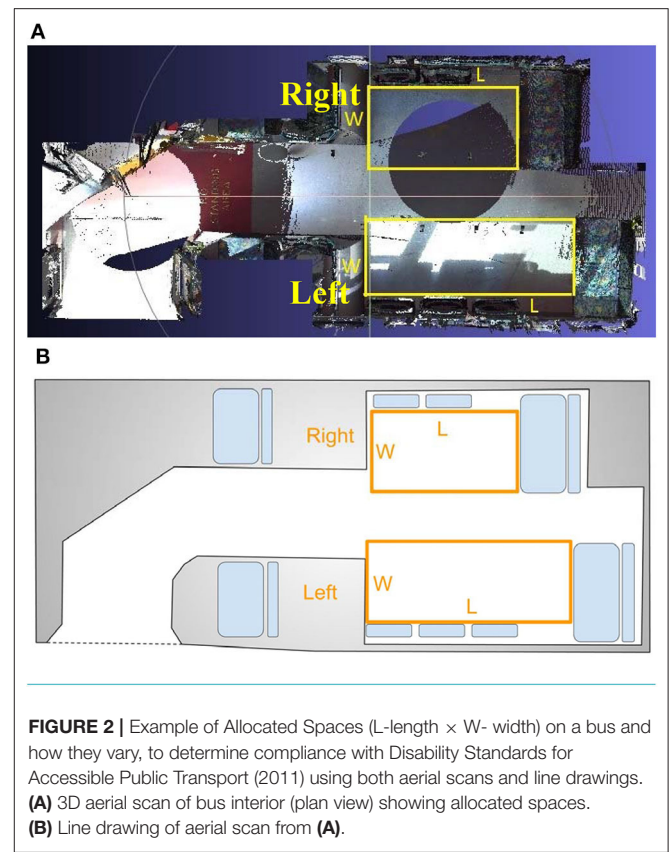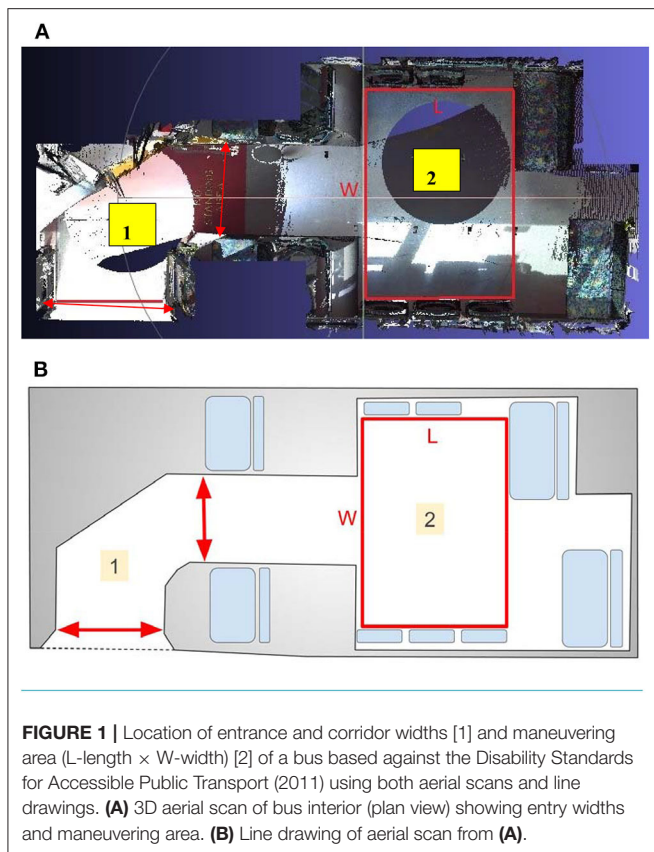

Previous research (Unsworth et al., under review) examined the validity and practical implications of AS-TS 3695.3:2018 Blue Label. This study measured a sample of 35 mobility aids and tested them in five rigs built according to the 2D measures specified in the AS-TS to identify the measurements of mobility aids that are most likely to be awarded a Blue Label, as well as which of the 35 mobility aids tested would be awarded a Blue Label denoting suitability for use on public transport. The 35 mobility aids were tested by three real-world mobility aid users, as well as research team members. It was found that nine of 35 mobility aids would not be awarded a Blue Label, and the Allocated Space test presented the most challenge for these mobility aids, followed by successful completion of the 180° turn test. The measurements of powered mobility aids that were most likely to comply with AS-TS 3695.3:2018 Blue Label for public transport access were those with a diagonal length (D) <1,280 mm, overall length (L) <1,110 mm, and a measured turn radius <760 mm.

Testing to determine the accuracy of AS-TS 3695.3:2018 against the real-world fit of mobility aids on buses (and other transport such as trams and trains in the future) is also required. For example, to what extent are buses compliant with DSAP measures, and can powered mobility aids that are, and are not awarded a Blue Label access and maneuver within these buses? One of the limitations of the current AS-TS is that it relies on manufacturer specifications. However, our previous research

identified that it was not possible to determine if mobility aids would be awarded a Blue Label based on these specifications alone (Unsworth et al., under review), and that building the test rigs was necessary. Anecdotally, it also seemed that there was limited consistency in the measures of the mobility aids that were and were not awarded a Blue Label. Therefore, research to determine the accuracy of the AS-TS 3695.3:2018 Blue Label to identify mobility aid access on buses that are and are not compliant with DSAPT is required, using either real word testing, or computer-generated simulations.

Testing real world access for the vast number of mobility aids on the market in the large number of bus formats in service would be an exhausting undertaking. However, the emergence of 3D scanning technology (Paquet and Feathers, 2004) and use of meshing software to develop accurate models for virtual examination is a convenient alternative to address this issue. We previously undertook a proof-of-principle study to demonstrate that 3D scans of mobility aids and buses could be accurately undertaken and meshed (Unsworth et al., 2018). The aims of the current paper were to use 3D scanning and meshing technology for the first time to help answer the following real-world accessibility questions: (i) which low floor transit buses that do and don't comply with the DSAPT standards, enable boarding for people using powered mobility aids that are or are not compliant with AS-TS 3695.3:2018 Blue Label measures, and (ii) what are the dimensions of mobility aids that fit

most buses? To answer these questions, the following objectives were undertaken:

- 1) generate 3D scans and calculate accurate measurements for a sample of 35 mobility aids, which previous research has shown 25 of which do, and 10 do not achieve a Blue Label,
- 2) generate 3D scans and calculate measurements for a sample of 21 low-floor transit buses, and identify how many are compliant with the Australian specifications for buses according to the Disability Standards for Accessible Public Transport (DSAPT; Department of Infrastructure Regional Development Australian Government, 2011),
- 3) use our previously validated meshing software technique to manipulate the 35 powered mobility aids through the 21 buses (using collision detection to determine a grid of positions that the mobility aid could occupy, and a path finding algorithm), to determine how many of the mobility aids (25 with Blue Label, and 10 without) are actually compatible to access the buses and if they are not compatible, which section/s of the bus caused most problems, and
- 4) identify the measurements of powered mobility aids most likely to access transit buses.

METHODS

Design

Three dimensional (3D) scanning has been widely used in the medical rehabilitation and engineering fields to aid design and fit processes such as in the design and customization of orthotics (Telfer and Woodburn, 2010) or for improving wheelchair seating design (Crytzer et al., 2016), as well as for mapping interiors to develop virtual environments (Henry et al., 2014). A proof of principle paper has previously demonstrated that 3D scanning and computerized meshing techniques can successfully identify the match or mis-match of mobility devices on public transport, and full details of the techniques used have been provided (Unsworth et al., 2018). A summary of these techniques to determine the match and mismatch between a sample of 35 mobility aids when maneuvered within 21 buses, is detailed below.

Bus and Mobility Aids Selected for Scanning

This research was undertaken in the large metropolitan city of Melbourne with a population of ~5 million people. Two large mobility aid suppliers were approached to provide access to a range of commonly used (and best-selling) 3- and 4- wheeled scooters as well as powered wheelchairs. A total of 35 mobility aids (16 powered wheelchairs and 19 scooters) were scanned in the time available for the research, which can be described as a convenience sample. These mobility aids have been previously described (Unsworth et al., under review) and four were classified as suitable for indoor use only (Class A) although several of these were sold as light-weight local and international travel aids, 27 were suitable for a mix of indoor and outdoor use (Class B) and four were suitable for outdoor use only (Class C).


The buses scanned in this research were similarly sourced from two of the largest providers of transit bus services in the city/suburban region (~25 km²). All buses were randomly pulled from service to suit the operational timetable on the days allocated for scanning. Twenty of the buses were standard low floor, two axel vehicles and the final conveyance was a low floor, two-axel miniature bus. The buses were from numerous chasses and body builders including MAN, Scania, Mercedes Benz, Volvo, Toyota, Optare, Designline, Denning, Gemilang, Iveco, and Volgren.

3D Scanning Technique

3D scanning collects data of interiors or objects and saves these in a digital format that can be converted into computer-aided design (CAD) models. These CAD models can then be used to take measurements or run computer simulations. Three-dimensional scanning of mobility aids has been successfully undertaken over the past 15 years (Paquet and Feathers, 2004). The scanner used in this research was a tripod-mounted Faro Focus X330 laser scanner (Faro, Lake Mary FL, USA). This scanner is capable of scanning the environment 360° in the horizontal (azimuthal) and vertical axes with a precision of ±2 millimeters at distances up to 10 meters. While the buses took approximately 45 min to scan, each mobility aid only took ~25 min. The primary output from a laser scanner is a “point cloud” of reflection positions. Poisson surface reconstruction (Kazhdan et al., 2006) can then be used to generate a tet-mesh of the point cloud, and render the required model. The positioning of the Faro Focus X330 laser scanner to scan both bus interiors as well as mobility aids is provided in **Figure 3**.

Data Analyses Using Meshing Software

On completion of scanning the mobility aids and bus interiors, meshes of the two were generated. Faro Scene LT (Faro, Lake Mary FL, USA) was used to convert the proprietary Faro Scan data of the mobility aids and bus interiors to a PTX file which is in an open format for point cloud data. Meshlab, an open-source 3D meshing tool (Cignoni et al., 2008), was then used to align the powered mobility aid scans with each bus scan to create meshes, and Poisson surface reconstruction was used for further processing. Collision detection was then applied, using a hierarchical mesh decomposition for computational efficiency, to determine a grid of positions that the mobility aid could occupy in the bus and determine the allowable orientations of the mobility aid at each position. Finally, a path finding algorithm was employed to compute the range of allowable paths of the mobility aid through the bus from the entry to the exit point, thus providing exact details of the match or mis-match of each mobility aid to maneuver through each bus. The Find Path simulation is completed using two steps. First, using the occupiable grid of positions, the simulation attempts to identify a “direct path” between every two points adjacent to each other. A “direct path” exists when the radius of the arc formed between the two points is larger than the turning radius of the mobility aid. All the points that have a “direct path” create a “full path” graph. Then from the “full path” graph, the simulation determines if there is a path the mobility aid can use to travel from the entry

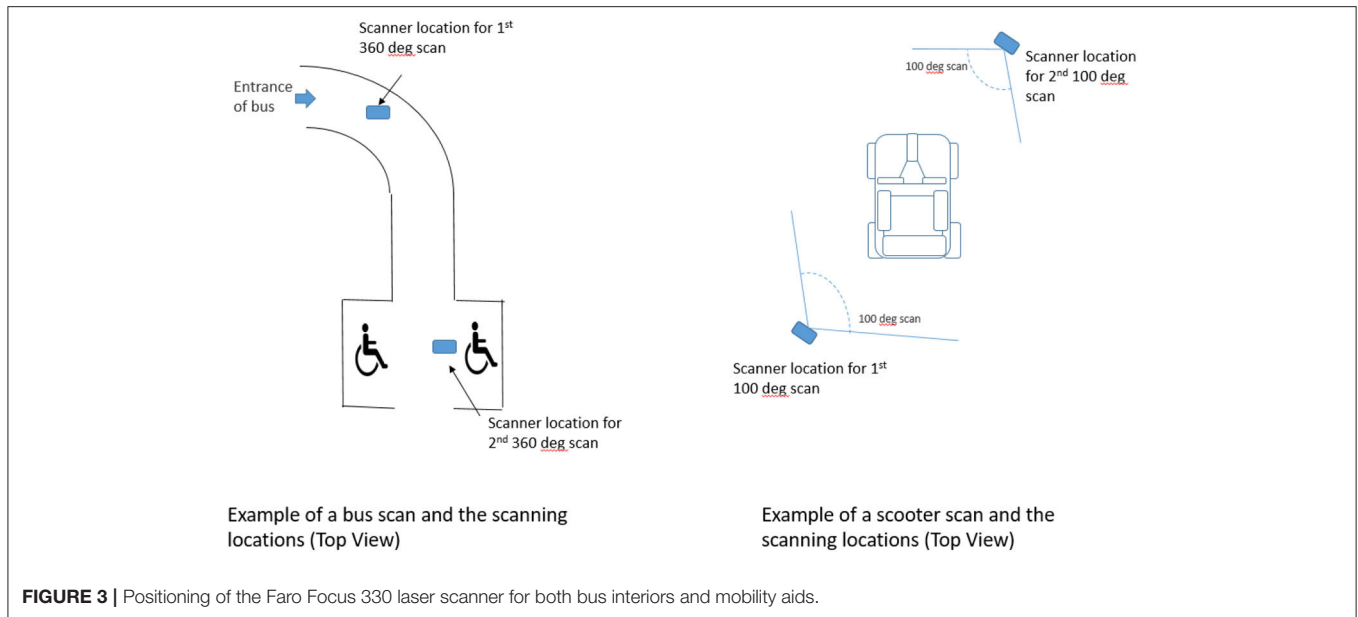

to the exit point. For this simulation, the entry to exit point includes the swept path, through the narrow entrance, to the allocated space. This method enabled the research team to detect the access or collision for large numbers of powered mobility aids on each bus in a time efficient manner. Data processing for each of the 375 meshes (35 mobility aids \times 21 buses) took \sim 30 min.

RESULTS

Measures of the 35 Mobility Aids Scanned in 3D

On completion of 3D scanning, the measurements of the 35 mobility aids were recorded and are presented in **Table 1**, which also shows if each mobility aid passed or failed the Blue Label 2D test when the test rigs were built in 3D and the mobility aid driven through as previously reported (Unsworth et al., under review). As noted above, the AS-TS makes provision that mobility aids with a diagonal length of 1,200 mm or less are exempt from undertaking the Allocated Space Test, presumably because all mobility aids with this dimension or less would pass this test. It was found that the Shoprider GK4 (diagonal length of 1,149 mm) did not pass this test, suggesting this criterion is not always valid. However, this mobility aid was also not able to complete the 180° turn test within a 2,070 mm \times 1,540 mm area and therefore failed to attain the criteria for a Blue Label anyway. As noted above, 25 of the mobility aids would have been allocated a Blue Label, and 10 would not.

Measures of the 21 Buses Scanned in 3D

Table 2 presents the measurements of the 20 of the buses scanned, while **Figure 4** presents the measures of the first bus scanned against an aerial image showing the location of where

measures were taken. The measures of the buses using both 2D as well as 3D data from the scans were compared against the Disability Standards for Accessible Public Transport (2011), and the findings reported in **Table 3**. The final column of **Table 3** demonstrates that while overall three of the 21 buses were DSAPT compliant when using 2D measures, none were compliant when using the 3D measures.

Compatibility of Mobility Aids on Buses and the Measures of Mobility Aids Most Likely to Fit

The 3D mobility aid and bus scans were meshed using collision detection to determine the grid of positions that the mobility aid could occupy, as well as a path finding algorithm. **Figure 5** demonstrates examples of the images generated from these meshing activities. **Figure 5A** provides an example of a Collision image (Left) and Find Path image (Right) of a mobility aid that was able to successfully navigate the Swept Path entry, Narrow Access corridor and Allocated Space for travel, and classified as a pass. **Figure 5B** provides an example of Find Path image (Left) of a mobility aid that could not enter the Swept Path of a bus (classified as fail), as well as a 3D Find Path image (Right) showing the mobility aid and the point of collision of the left rear wheel. **Table 4** then provides a summary of each of the mobility aids and the number of buses they can fit on. The mobility aids listed in bold all achieve AS-TS 3695.3:2018 Blue Label, theoretically denoting compatibility with public transport. Of note, three mobility aids that did not achieve a Blue Label could access 12 or 13 of the 21 buses tested. Specifically, the Heartway Puzzle (wheelchair) and Shoprider GK4 (scooter) could both access 12, and the Monarch Hybrid (scooter) could access 13 of the 21 buses. It was also important to note that four of the mobility aids that would be awarded a Blue Label, were not able to

TABLE 1 | Measures for mobility devices (**Bold italic** font indicating measure >1,200, and gray highlight indicates a failed Blue Label test).

No	Make	Model	Driver	Type (S/W)	Wheels	Drive	Class	Length (mm)	Width (mm)	Height (mm)	Diagonal (mm)	Weight (kg)	Turn radius (mm)	Rear (drive) wheel Dia (mm)	Front Wheel Dia (mm)	Rear wheel Dia (mm)	2D Blue Label Allocated Space	2D Blue Label Swept Path	2D Blue Label Narrow Access	2D Blue Label Pavement Gap 90 deg	2D Blue Label Pavement Gap 60 deg	2D Blue Label Area (2070 x 1540 mm)
1	Luggie	Chair	1	S	4	Rear	A	950	610	<1,500	1,129	34	780	199	178	Nil	Pass	Pass	Pass	Pass	Pass	Pass
2	Monarch	Hybrid 4	3	S	4	Rear	B	1,170	565	880	1,299	8	535	250	250	Nil	Fail Stuck at 2	Pass	Pass	Pass	Pass	Pass
3	Monarch	Buzz 3 wheel	1	S	3	Rear	B	1,010	550	<1,500	1,150	46	Not-ava	200	200	Nil	Pass	Pass	Pass	Pass	Pass	Pass
4	Luggie	standard	2	S	4	Rear	B	982	450	<1,500	1,080	26	1,040	177.8	152.4	Nil	Pass	Pass	Pass	Pass	Pass	Pass
5	Monarch	GC440	2	S	4	Rear	B	1,187	600	1,000	1,330	85	Not-ava	250	250	Nil	Fail	Pass	Pass	Pass	Pass	Fail
6	Monarch	Zener	2	S	4	Rear	B	1,190	600	<1,500	1,333	90	Not-ava	250	250	Nil	Fail Stuck at 2	Pass	Pass	Pass	Pass	Fail
7	Luggie	Elite	1	S	4	Rear	B	982	455	<1,500	1,082	26	900	177.8	152.4	Nil	Pass	Pass	Pass	Pass	Pass	Pass
8	Pride	Gogo LX	R	S	4	Rear	B	1,041	521	<1,500	1,164	53.4	1,162	203	178	Nil	Pass	Pass	Pass	Pass	Pass	Pass
9	Merits	Yoga	R	S	4	Rear	B	980	435	<1,500	1,072	25.7	960	178	153	Nil	Pass	Pass	Pass	Pass	Pass	Pass
10	Shoprider	GK4	R	S	4	Rear	B	1,030	510	850	1,149	42.5	940	203.2	177.8	Nil	Fail	Pass	Pass	Pass	Pass	Fail
11	Shoprider	GK9-3	R	S	3	Rear	B	1,020	560	<1,500	1,164	56	1,150	265	265	Nil	Pass	Pass	Pass	Pass	Pass	Pass
12	Invacare	Colibri	R	S	4	Rear	B	1,010	500	<1,500	1,127	48.9	1,100	210	210	Nil	Pass	Pass	Pass	Pass	Pass	Pass
13	Trek	SupaScoota SHd02	R	S	4	Rear	B	1,010	570	<1,500	1,160	27.9	910	200	200	Nil	Pass	Pass	Pass	Pass	Pass	Pass
14	Pride	Gogo Ultra X	R	S	4	Rear	B	1,010	495	<1,500	1,125	44.5	1,120	200	180	Nil	Pass	Pass	Pass	Pass	Pass	Pass
15	Trek	SupaScoota Sumo	R	S	4	Rear	B	1,110	630	<1,500	1,276	34.2	1,000	200	200	Nil	Pass	Pass	Pass	Pass	Pass	Pass
16	Shoprider	889SL	2	S	4	Rear	C	1,300	640	1,200	1,449	146	1,440	330	330	Nil	Fail Stuck at 2	Pass	Pass	Pass	Pass	Fail
17	Afikim	Breeze C3	R	S	3	Rear	C	1,300	670	1,260	1,462	102	1,280	Not-ava	Not-ava	Nil	Fail Stuck at 2	Pass	Pass	Pass	Pass	Fail
18	Trek	Evolution	R	S	4	Rear	C	1,270	620	<1,500	1,413	67	Not-ava	260	260	Nil	Fail Stuck at 2	Pass	Pass	Pass	Pass	Fail
19	Invacare	Metro	R	S	4	Rear	C	1,270	660	1078	1,431	110	1,300	279.4	279.4	Nil	Fail Stuck at 2	Fail	Pass	Pass	Pass	Fail
20	Shoprider	888SE	R	S	4	Rear	B	1,280	600	1,070	1,414	99	1,500	260	260	Nil	Fail Stuck at 2	Fail	Pass	Pass	Pass	Fail
21	Merits	Maverick 14	1	W	6	Mid	B	1,010	660	1,270	1,207	115	530	355.6	203.2	203.2	Pass	Pass	Pass	Pass	Pass	Pass
22	Monarch	GP650	1	W	6	Mid	B	960	610	<1,500	1,137	84	Not-ava	250	Not-ava	Not-ava	Pass	Pass	Pass	Pass	Pass	Pass
23	Pride	Jazzy Air	1	W	6	Mid	B	1,100	648	<1,500	1,277	125.6	571.5	254	152.4	152.4	Pass	Pass	Pass	Pass	Pass	Pass
24	Shoprider	Puma 14 HD	R	W	6	Mid	B	1,060	640	<1,500	1,238	126	545	350	175	175	Pass	Pass	Pass	Pass	Pass	Pass
25	Shoprider	Cougar Power Tilt	R	W	6	Mid	B	1,090	620	<1,500	1,254	100	600	250	125	100	Pass	Pass	Pass	Pass	Pass	Pass
26	Heartway	P3DXC	R	W	6	Mid	B	1,060	600	<1,500	1,218	98	500	360	155	155	Pass	Pass	Pass	Pass	Pass	Pass
27	Heartway	P3D	R	W	6	Mid	B	1,080	597	1,092	1,234	107	550	330	155	155	Pass	Pass	Pass	Pass	Pass	Pass
28	Monarch	Literider	3	W	4	Rear	A	825	562	<1,500	998.2	54	Not-ava	225	150	Nil	Pass	Pass	Pass	Pass	Pass	Pass
29	Shoprider	Venice	R	W	4	Rear	A	725	545	<1,500	907	37.8	400	200	155	Nil	Pass	Pass	Pass	Pass	Pass	Pass
30	Shoprider	Como	R	W	4	Rear	A	870	580	851	1,046	47.4	685	230	155	Nil	Pass	Pass	Pass	Pass	Pass	Pass
31	Pride	GoChair	R	W	4	Rear	B	825.5	483	<1,500	956.2	36.2	682.6	203.2	127	Nil	Pass	Pass	Pass	Pass	Pass	Pass
32	Invacare	Pronto Air	R	W	4	Rear	B	960	510	1,170	1,087	72.6	742	304.8	152.4	Nil	Pass	Pass	Pass	Pass	Pass	Pass
33	Pride	R40 Fusion	R	W	4	Rear	B	890	635	<1,500	1,093	64.84	965	355	228	76	Pass	Pass	Pass	Pass	Pass	Pass
34	Heartway	Puzzle 15	R	W	4	Rear	B	1,040	610	<1,500	1,206	38	720	320	180	Nil	Fail	Pass	Pass	Pass	Pass	Pass
35	Trek	Supachair (Safari)	R	W	4	Rear	B	870	600	840	1,057	36.5	700	200	178	Nil	Pass	Pass	Pass	Pass	Pass	Pass

Key: Driver 1,2,3,R, 1,2,3, Denotes drivers with lived experience, and R driven by a researcher.

S/W, Scooter/Wheelchair.

Class A,B,C, Class A indoor use, Class B mix of indoor and outdoor use and Class C outdoor use only.

Not-ava, Not available.

TABLE 2 | Measures for buses scanned (Bus No. 7 scan and indicative dimensions included in **Figure 1**).

Bus #	16	35	83	98	115	130	145	101	117	411	569	638	710	747	914	996	2,001	8,609	8,901	Mini
Bus Measure in millimeters																				
Entrance, A	968	1,033	1,012	857	941	898	1,005	1,097	1,041	1,002	1,090	1,084	972	1,012	960	1,010	1,000	917	910	808
Start corridor, B	838	793	824	820	852	820	849	856	870	844	839	832	880	865	882	840	891	857	865	852
Start allocated space, C	837	789	840	816	854	820	840	852	842	848	864	846	838	888	891	840	897	847	869	852
Length of allocated space, D	1,354	1,382	1,873	1,340	1,245	1,308	1,405	1,538	1,301	1,297	1,544	1,390	1,352	1,673	1,405	1,858	1,345	1,400	2,952	1,609
Width of allocated space, E	550	640	600	607	596	573	604	552	523	691	575	597	478	543	567	594	595	598	616	310
Width of allocated space, E2	727	830	740	NA	NA	NA	NA	626	538	785	748	767	675	772	757	714	796	724	NA	608
Length of allocated space, D (right)	893	1,550	1,300	1,730	1,274	1,304	1,838	1,998	1,502	1,230	1,953	1,917	1,619	1,637	1,820	1,600	1,479	1,844	1,408	1,729
Width of allocated space, E (right)	595	600	533	628	642	656	597	536	530	646	582	616	644	698	596	605	580	652	625	758
Width of allocated Space, E2 (right)	766	780	762	779	693	NA	753	669	621	690	720	748	796	774	763	737	742	760	730	758
End allocated space, F	615	474	454	789	909	1137	827	542	716	703	481	477	543	486	530	663	500	591	793	NA
Seat configuration: left	2 × 2 folded	3 × 1 folded 1 × 2 fixed	3 × 1 folded 1 × 2 fixed	3 × 1 folded	3 × 1 folded	3 × 1 folded	3 × 1 folded	3 × 1 folded	3 × 1 folded	2 × 2 folded	2 × 1 folded 1 × 2 folded	3 × 1 folded	1 × 1 folded 1 × 2 folded	1 × 1 folded 1 × 2 folded	3 × 1 folded	3 × 1 folded	3 × 1 folded	2 × 1 folded 1 × 2 folded	6 × 1 folded	3 × 1 folded
Seat configuration: right	1 × 2 folded 1 × 2 fixed	3 × 1 folded 1 × 2 fixed	2 × 1 folded 1 × 2 fixed	3 × 1 folded 1 × 2 fixed	3 × 1 folded	3 × 1 folded	3 × 1 folded 1 × 2 folded	4 × 1 folded	3 × 1 folded	3 × 1 folded	3 × 1 folded	3 × 1 folded	3 × 1 folded	3 × 1 folded	4 × 1 folded	3 × 1 folded	3 × 1 folded	3 × 1 folded 1 × 2 folded	2 × 1 folded 1 × 2 folded	3 × 1 folded

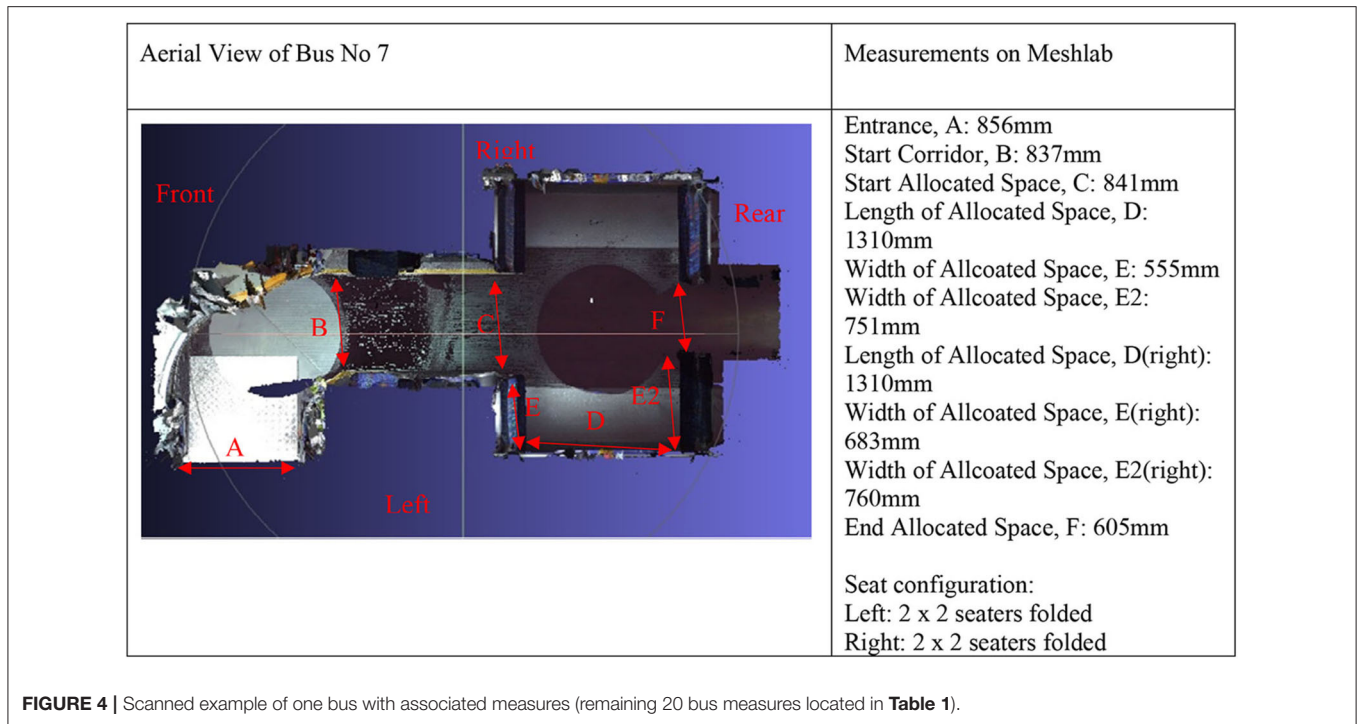


TABLE 3 | Results from 2D and 3D measures of buses in relation to Disability Standards for Accessible Public Transport (DSAPT) (Department of Infrastructure Regional Development Australian Government, 2011) compliance.

Bus DSAPT Compliance using 2D and 3D measures					
	Min width	Allocated space (left)	Allocated space (right)	Maneuvering area	Overall
No. 7	Pass	Fail	Fail	Fail	Fail
No. 16	Pass	Fail	Fail	Fail	Fail
No. 35	Pass	Pass	Pass 2D/Fail 3D	Fail	Fail
No. 83	Pass	Pass 2D/Fail 3D	Pass 2D/Fail 3D	Fail	Fail
No. 98	Pass	Fail	Pass 2D/Fail 3D	Fail	Fail
No. 115	Pass	Fail	Fail	Fail	Fail
No. 130	Pass	Fail	Fail	Fail	Fail
No. 145	Pass	Fail	Pass 2D/Fail 3D	Fail	Fail
No. 101	Pass	Pass 2D/Fail 3D	Pass 2D/Fail 3D	Fail	Fail
No. 117	Pass	Fail	Pass 2D/Fail 3D	Fail	Fail
No. 411	Pass	Pass 2D/Fail 3D	Fail	Fail	Fail
No. 569	Pass 2D/Fail 3D	Pass 2D/Fail 3D	Fail	Pass 2D/Fail 3D	Fail
No. 638	Pass 2D/Fail 3D	Fail	Fail	Fail	Fail
No. 710	Pass	Pass 2D/Fail 3D	Pass 2D/Fail 3D	Fail	Fail
No. 747	Pass 2D/Fail 3D	Pass 2D/Fail 3D	Pass 2D/Fail 3D	Pass	Pass 2D/Fail 3D
No. 914	Pass 2D/Fail 3D	Pass 2D/Fail 3D	Pass 2D/Fail 3D	Pass 2D/Fail 3D	Fail
No. 996	Pass	Fail	Fail	Pass 2D/Fail 3D	Pass 2D/Fail 3D
No. 2001	Pass	Pass 2D/Fail 3D	Pass 2D/Fail 3D	Fail	Fail
No. 8609	Pass	Fail	Pass 2D/Fail 3D	Fail	Fail
No. 8901	Pass	Fail	Pass 2D/Fail 3D	Fail	Fail
Mini	Pass	Fail	Pass 2D/Fail 3D	Pass 2D/Fail 3D	Pass 2D/Fail 3D

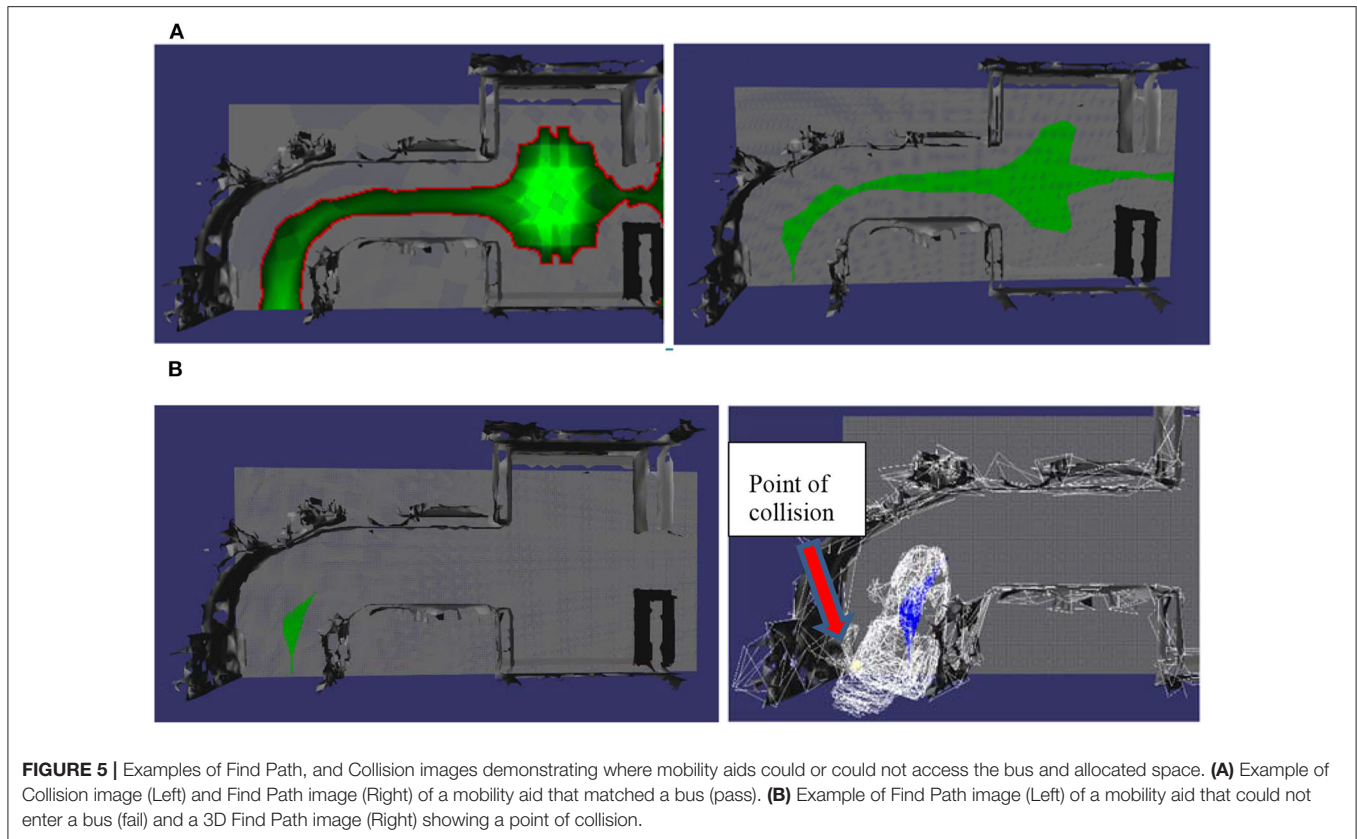


TABLE 4 | Number of buses that can fit the following 35 mobility aids that do (**bold font**) and don't (regular font) meet the AS-TS 3695.3:2018 for public transport access.

Fit 16 or more buses	Fit 11–15 buses	Fit 6–10 buses	Fit 5 buses or less
Monarch Buzz3 Luggie Std Luggie Elite Luggie Chair Merits Yoga Invacare Colibri Pride Gogo UltraX Trek SupaScootaSS	Trek Supa Scoota Sumo Monarch Literider Shopperider Cougar Tilt Shopperider Venice Shopperider Como Pride Gochair Trek Supachair	Heartway P3DX Shopperider GK93 Merits Maverick Pride Jazzy Air Pride Gogo LX Invacare Pronto Air Heartway Puzzle Monarch Hybrid Shopprider GK4	Heartway P3D Monarch GP650 Shopperider Puma14HD Pride R40Fusion Afikim Breeze 3 (fit on 0) Monarch GC440 (fit on 1) Monarch Zener (fit on 0) Shopprider 889SL (fit on 0) Trek Evolution (fit on 0) Invacare Metro (fit on 0) Shopprider 888 (fit on 0)

successfully navigate 11 or more buses (Heartway P3D, Monarch GP650, Shopprider Puma 14HD, and Pride R40Fusion).

The section of the bus that caused most problems when the mobility aid scans were meshed with the bus scans was the Swept Path entrance. The 735 meshing simulations were undertaken to determine each collision point, and then restart the simulation to identify any subsequent collision points. There were 286 (67%) collisions in the Swept Path, 0 collisions in the Narrow Path, and 141 (33%) collisions in the Allocated Space. The main features that contributed to the collision points in the Swept Path were protrusions from fare reading devices (many of which were located at approximately hip height of a standing person), cushioning from the first row of bus seats on either side of the entrance, and due to a small narrowing of the pathway that provides the transition between the Swept Path and the Narrow

Access Path. All these features essentially reduced the functional width of the Swept Path area and prevented many of the larger powered mobility aids or those with smaller turning radii to enter, often causing a collision in the entry point as shown in **Figure 5B**.

The final aim of this research was to identify the measurements of powered mobility aids most likely to access transit buses. The measures identified draw on the measures of the mobility aids that could access the most buses. Nine of the 35 powered mobility aids were able to fit at least the 20 full-size transit buses, and five of these could fit on the mini bus as well: five were scooters with turn radii ranging from 650 to 995 mm (Monarch Buzz 3, Luggie Standard, Luggie Elite, Merits Yoga, and Pride GoGo Ultra X) and 4 were powered wheelchairs with turn radii of 300–310 mm (Shopperider Venice, Shopprider Como, Trek Supachair, and Luggie Chair). Their length ranged from

TABLE 5 | Measures of mobility devices most suitable for bus access: Comparison of results from current research and AS–TS 3695.3:2018 Blue Label requirements.

Measure	Current research findings	Blue label requirements
Overall width	Not applicable	740 mm, plus meet requirements of Clause 5 [four tests which must be passed: Swept Path test, Narrow Access Path test, Allocated Space test and Pavement Gap test.]
Overall length	1,100 mm or less	Meet requirements of Clause 5 [as noted above]
Diagonal length	1,250 mm or less	Not applicable
180° turn	Measured turn radius of 750 mm or less	Within 2,070 mm × 1,540 mm area
Mass of mobility scooter (max)	Not applicable	170 kg

725 to 1,041 mm and their width range from 435 to 610 mm. However, it was the diagonal length (absorbing the width measure) that was most informative for determining guidelines for overall fit. **Table 5** provides the measures of mobility aids recommend for use on buses and compares these against the Blue Label measures.

DISCUSSION

This discussion examines the outcome of the computerized meshing task to examine the accuracy of AS–TS 3695.3:2018 Blue Label to identify mobility aids that will and will not fit on transit buses, measures of mobility aids most likely to access buses, limitations of the research, and areas for further study. While Bharathy and D’Souza (2018) developed an algorithm to determine the dimensions of the clear floor area required to best accommodate people in their mobility devices in buses, the current research approached the same access problem from a different perspective, viz., how to identify which, from a sample of mobility aids, are compatible to access and maneuver within all 3D spaces of existing buses, and the dimensions of mobility aids most suited to this purpose. Previous research (Unsworth et al., under review) examined whether a sample of 35 mobility aids tested in purpose-built rigs according to AS–TS 3695.3:2018 would achieve a Blue Label denoting compatibility with public transport. Twenty-five of the mobility aids were compliant, and it was demonstrated that the test rigs needed to be built in order to accurately determine the label award. The current study then used a novel computerized meshing approach (Unsworth et al., 2018) to generate both Collision and Find Path analyses to identify any points at which a mobility device might collide and become stuck when entering, maneuvering within and exiting a bus.

In the current study, the Swept Path entrance of the buses proved most challenging for the mobility aids to maneuver within. However, in the previous study validating the Blue Label

(Unsworth et al., under review), it was found that the Allocated Space caused most problems. In the previous study, eight of the 10 mobility aids that did not achieve Blue Label could not be positioned in the allocated space, and the final two aids could complete this task, but only with more than 5 min of small, skilled maneuvers. To maneuver into the Allocated Space, the mobility aids were driven to follow the specified pattern requiring the driver to make the following three moves: (1) drive forward down the bus corridor from front entrance, just past the allocated space (e.g., on the right), (2) reverse backwards using an elongated S into the allocated space, (3) exit the allocated space by driving forward while rotating 180° to exit from the front entrance. Seven of the 10 mobility aids encountered the collision point at turn number 2. reverse backwards using an elongated S into the allocated space. Research undertaken by Bharathy and D’Souza (2018) and D’Souza et al. (2017a,b) also focused on transit spaces as being most problematic for people using mobility aids. However, since the buses in these jurisdictions allow entry from mid doors, the need for curved swept entry, and any problems that generates were bypassed. The finding in the current study that the Swept Path is the main problem for accessibility for people using mobility devices also supports Australia to transition to positioning ramps at bifold mid bus doors and promote boarding for people using mobility aids from this point. Very few other studies have been conducted to compare the present study findings against. For example, while Koontz et al. (2010) also scanned mobility aids in 3D, their study aimed to then measure the minimum turning spaces for a wheelchair to maneuver in building corridor spaces.

Nine of the 35 powered mobility aids tested were identified as being able to fit at least 20 of the different transit buses. It is important to note that three of these are Class A mobility aids while the other six are Class B. Class A mobility aids are specified by manufacturers as suitable for indoor use such as in a home or shopping center. However, these devices are often lightweight and portable and therefore ideal to take on outings or use on domestic and international travel. In fact, many mobility aid retailers sell these devices to people wishing to travel, including navigating cobbled streets as found across Europe. It is also important to note that the simulations undertaken in this study assume that the bus has both left and right Allocated Spaces available for maneuverability. However, in reality one of the Allocated Spaces may already be occupied by someone who has a disability or by passengers with prams (Velho, 2019). This means that the potential space a mobility aid must maneuver within may be considerably smaller in real life than in simulations.

Several limitations of this research must be acknowledged. The computer simulations we undertook were very strict on determining a collision at any point of contact regardless of whether it was a soft (cushion) point of contact or hard (metal or plastic) contact which prevented further entry for the powered mobility aid. This has the advantage of “protecting” both mobility aids and buses against damage as well as wear and tear, but it is acknowledged that some mobility aids could potentially push past some collision points such as from seat cushioning, and gain access. In addition, the Find Path simulation we undertook does not currently have an automated method of testing all

the different starting points or different starting angles for a mobility aid entering a bus. We considered several options for start points and angles but acknowledge that there might be a small number of rare configurations that might improve the Find Path outcomes produced in this study. In practice, however, it is unlikely that a person using a mobility aid would be able to replicate unusual entry angles that might improve access. In addition, many people using mobility aids also affix accessories such as shopping baskets to the front or rear or attach a walking aid such as a rollator on the rear. The measures taken in this research do not account for the additional space requirements generated by attaching any of these accessories on a mobility aid. Finally, this research only investigated a sample of 35 mobility aids and 21 buses from one area in Australia. Therefore, further scanning and meshing of a greater number of mobility aids and buses is required to extend our understanding of the measures of mobility aids most likely to access buses, and how the AS-TS 3695.3:2018 Blue Label may need to be revised to ensure that the measures provided are accurate in determining if a mobility aid will be able to fit on public transport or not. As demonstrated in previous research, the maneuverability of powered mobility aids, even from the same class are very different (Pellegrini et al., 2010), and therefore the access requirements for each must be individually tested. In future, and as 3D scanning becomes more affordable and commonplace, a target could be set of scanning 50% of all new buses as they go into service, and 50% of new mobility aids as they come onto the market. As the dataset of compatibility meshes grows, it is possible that the dimensions of mobility aids that will fit on most buses may alter from those reported in this paper.

CONCLUSION

Ensuring access for people using powered mobility aids on our public transport network, particularly buses, is vital for both users and service providers. Buses reach far into the community to support people with limited resources to connect with essential health and retail services, as well as to support participation in family, sporting, and cultural activities. While Standards such as DSAPT (Department of Infrastructure Regional Development Australian Government, 2011) and AS-TS 3695.3:2018 Blue Label have been developed to support this goal, without research to test and validate their use, they may hinder rather than promote best practice. This research demonstrated that although none of the buses were compliant with all aspects of the DSAPT, the meshing of 3D scans indicated that many powered mobility aids could still successfully access many buses and 13/21 of the buses could actually accommodate at least 22/35 powered mobility aids. However, there were problems with the Blue Label system not accurately indicating if a powered mobility aid could fit on a bus, and 3/35 powered mobility aids that would not achieve a Blue Label could actually access up to 13 buses, and 4/25 powered mobility aids that would be awarded a Blue Label could not access 11 or more buses. Nine powered mobility aids that were able to fit on all 20 full-size buses tested in this research are recommended for users to consider purchasing to optimize

their access on buses. Furthermore, the length and diagonal length dimensions of mobility aids that appear to enable fit on most buses tested in this research were also identified for consumers to consider the use of mobility aids on buses beyond the 35 specifically measured in this research. Since the majority of mobility aids that could not gain entry on a bus experienced a collision point in the Swept Path entry, future bus design in Australia should investigate boarding people using powered mobility aids from double doors in the middle of the bus to a large adjacent allocated space, as occurs in bus boarding in other parts of the world. This research provides important information to support the decisions made by a range of end users including customers wishing to purchase a mobility aid as well as bus designers and commissioning teams. The findings from this research also serve to fill fundamental gaps and inconsistencies in statutory and policy obligations to ensure public transport is accessible for all, and thus increase ridership among the growing group of people who use mobility aids to access the community.

DATA AVAILABILITY STATEMENT

The raw data supporting the conclusions of this article will be made available by the authors, without undue reservation.

AUTHOR CONTRIBUTIONS

CU conceptualized the study. JC and CU collected the data, with discussion with PG. JC developed the data analysis technique and undertook all analyses. JC and CU interpreted the findings. CU, JC, and PG prepared the findings for publication, edited the manuscript, and approved the final manuscript submitted. All authors contributed to the article and approved the submitted version.

FUNDING

This research was funded from a grant from Department of Transport (formerly Public Transport Victoria), Victoria, Australia.

ACKNOWLEDGMENTS

Sincere thanks are extended to the bus companies for assisting with this research so enthusiastically and making the buses available for scanning, as well as Scooters Australia and Mobility Aids Australia for providing the mobility aids for testing. Thanks also to team in the Inclusive Public Transport Unit at Department of Transport for their great collaboration. We also acknowledge the input of Professor Drew Dawson and Associate Professor Anjum Naweed (CQUniversity), Professor Richard Tay (RMIT University) and Dr. Richard Huysmans (Raven Consulting) who were all involved in early discussions about the research and supported the initial funding applications. Sincere thanks are also extended to Dr. Toan Nguyen and Associate Professor David Barnes (Monash eResearch Centre, Monash University) who advised on the data processing.

REFERENCES

- Australian Bureau of Statistics (ABS) (2016). *4430.0 - Survey of Disability, Ageing and Carers 2015, Viewed 15 March 2020*. Available online at: <https://www.and.org.au/pages/disability-statistics.html>
- Bharathy, A., and D'Souza, C. (2018). Revisiting clear floor area requirement for wheeled mobility device users in public transportation. *Transp. Res. Rec.* 2672, 675–685. doi: 10.1177/0361198118787082
- Cignoni, P., Callieri, M., Corsini, M., Dellepiane, M., Ganovelli, F., and Ranzuglia, G. (2008). "MeshLab: an open-source mesh processing tool," in *Proceedings of the Sixth Eurographics Italian Chapter Conference* (Salerno), 129–136.
- Crytzer, T. M., Hong, E., Dicianno, B. E., Pearlman, J., Schmeler, M., and Cooper, R. A. (2016). Identifying characteristic back shapes from anatomical scans of wheelchair users to improve seating design. *Med. Eng. Phys.* 38, 999–1007. doi: 10.1016/j.medengphy.2016.06.017
- Department of Infrastructure and Regional Development (2013). *Review of the Disability Standards for Accessible Public Transport*. Canberra, ACT.
- Department of Infrastructure and Regional Development and Australian Government (2011). *Disability Standards for Accessible Public Transport*. Canberra, ACT.
- D'Souza, C., Paquet, V., Lenker, J. A., and Steinfeld, E. (2017a) Effects of transit bus interior configuration on performance of wheeled mobility users during simulated boarding and disembarking. *Appl. Ergon.* 62, 94–106. doi: 10.1016/j.apergo.2017.02.008
- D'Souza, C., Paquet, V., Lenker, J. A., and Steinfeld, E. (2017b) Self-reported difficulty and preferences of wheeled mobility device users for simulated low-floor bus boarding, interior circulation and disembarking. *Disabil. Rehab. Assis. Technol.* 14, 109–121. doi: 10.1080/17483107.2017.1401128
- Frost, K. L., Bertocci, G., and Smalley, C. (2015). Ramp-related incidents involving wheeled mobility device users during transit bus boarding/alighting. *Arch. Phys. Med. Rehabil.* 96, 928–933. doi: 10.1016/j.apmr.2014.12.013
- Grimmer, K., Kay, D., Foot, J., and Pastakia, K. (2015). Consumer views about ageing-in-place. *Clin. Intervent. Aging.* 10, 1803–1811. doi: 10.2147/CIA.S90672
- Henry, P., Krainin, M., Herbst, E., Ren, X., and Fox, D. (2014). "RGB-D mapping: using depth cameras for dense 3D modeling of indoor environments," in *Experimental Robotics Springer Tracts in Advanced Robotics, Vol. 79*, eds O. Khatib, V. Kumar, and G. Sukhatme (Berlin: Springer), 647–663.
- Kazhdan, M., Bolitho, M., and Hoppe, H. (2006). "Poisson surface reconstruction," in *Proceedings of the 2006 Eurographics Symposium on Geometry Processing*, eds K. Polthier and A. Sheffer (Cagliari), 61–70.
- Koontz, A. M., Brindle, E. D., Kankipati, P., Feathers, D., and Cooper, R. A. (2010). Design features that affect the maneuverability of wheelchairs and scooters. *Arch. Phys. Med. Rehabil.* 91, 759–764. doi: 10.1016/j.apmr.2010.01.009
- La Plante, M. P., and Kaye, H. S. (2010). Demographics and trends in wheeled mobility equipment use and accessibility in the community. *Assis. Technol.* 22, 3–17. doi: 10.1080/10400430903501413
- May, E., Garrett, R., and Ballantyne, A. (2010). Being mobile: electric mobility-scooters and their use by older people. *Ageing Soc.* 30, 1219–1237. doi: 10.1017/S0144686X10000334
- Office of Fair Trading (2011). *Mobility Aids: An Office of Fair Trading Market Study (OFT1374)*. London: UK Government.
- Paquet, V., and Feathers, D. (2004). An anthropometric study of manual and powered wheelchair users. *Int. J. Indus. Ergono.* 33, 191–204. doi: 10.1016/j.ergon.2003.10.003
- Park, K., and Chowdhury, S. (2018). Investigating the barriers in a typical journey by public transport users with disabilities. *J. Transport Health* 10, 361–368. doi: 10.1016/j.jth.2018.05.008
- Pellegrini, N., Bouche, S., Barbot, F., Figère, M., Guillon, B., and Lofaso, F. (2010). Comparative evaluation of electric wheelchair maneuverability. *J. Rehab. Med.* 42, 605–607. doi: 10.2340/16501977-0562
- Pyer, T., and Tucker, F. (2014). With us, we like, physically can't: transport, mobility and the leisure experiences of teenage wheelchair users. *Mobilities* 12, 36–52. doi: 10.1080/17450101.2014.970390
- Standards Australia (2013). *AS/NZS 3695.2:2013 Wheelchair Requirements and Test Methods for Electrically Powered Wheelchairs Including Electric Mobility Scooters*. Sydney, NSW: SAI Global Limited.
- Standards Australia (2015). *AS/NZS ISO 10865.1:2015 Wheelchair Containment and Occupant Retention Systems for Accessible Transport Vehicles Designed for Use by Both Sitting and Standing Passenger Systems for Rearward-Facing Wheelchair-Seated Passengers*. Sydney, NSW: SAI Global Limited.
- Standards Australia (2018). *SA TS 3695.3:2018 Wheelchairs Requirements for Designation of Powered Wheelchairs and Mobility Scooters for Public Transport and/or Road-Related Area Use*. Sydney, NSW: SAI Global Limited.
- Steinfeld, A., Maisel, J. L., and Steinfeld, E. (2018). *Accessible Public Transportation*. New York, NY: Routledge.
- Telfer, S., and Woodburn, J. (2010). The use of 3D surface scanning for the measurement and assessment of the human foot. *J. Foot Ankle Res.* 3, 1–19. doi: 10.1186/1757-1146-3-19
- Unsworth, C. A., Chua, J., Naweed, A., Gudimetla, P., Nguyen, T. D., and Barnes, D. G. (2018). Use of 3D scanning technology to determine bus access for people using powered mobility aids. *J. Transport Health* 10, 350–360. doi: 10.1016/j.jth.2018.07.002
- Unsworth, C. A., Rawat, V., Sullivan, J., Tay, R., Naweed, A., and Gudimetla, P. (2019a). "I'm very visible but seldom seen": consumer choice and use of mobility aids on public transport. *Disab. Rehab. Assis. Technol.* 14, 122–132. doi: 10.1080/17483107.2017.1407829
- Unsworth, C. A., So, M. H., Chua, J., Gudimetla, P., and Naweed, A. (2019b). A systematic review of what is known about public transport accessibility for people using mobility aids. *Disab. Rehab.* 4, 1–15. doi: 10.1080/09638288.2019.1697382
- Velho, R. (2019). Transport accessibility for wheelchair users: a qualitative analysis of inclusion and health. *Int. J. Transp. Sci. Technol.* 8, 103–115. doi: 10.1016/j.ijst.2018.04.005

Conflict of Interest: The authors declare that the research was conducted in the absence of any commercial or financial relationships that could be construed as a potential conflict of interest.

Copyright © 2020 Unsworth, Chua and Gudimetla. This is an open-access article distributed under the terms of the Creative Commons Attribution License (CC BY). The use, distribution or reproduction in other forums is permitted, provided the original author(s) and the copyright owner(s) are credited and that the original publication in this journal is cited, in accordance with accepted academic practice. No use, distribution or reproduction is permitted which does not comply with these terms.