

IMAGES IN INTERVENTION

# TAVR in a Patient With Quadricuspid Aortic Stenosis



## The Role of Patient-Specific Computer Simulation in Treatment Planning and Outcome Prediction

Yu Han, MD,<sup>a</sup> Joana Maria Ribeiro, MD, MSc,<sup>b,c</sup> Peter P.T. de Jaegere, MD,<sup>b</sup> Gejun Zhang, MD<sup>a</sup>

A 70-year-old man with symptomatic aortic stenosis and regurgitation was referred for transcatheter aortic valve replacement. Pre-procedural computed tomography showed a quadricuspid aortic valve (QAV) (**Figure 1**). The annular

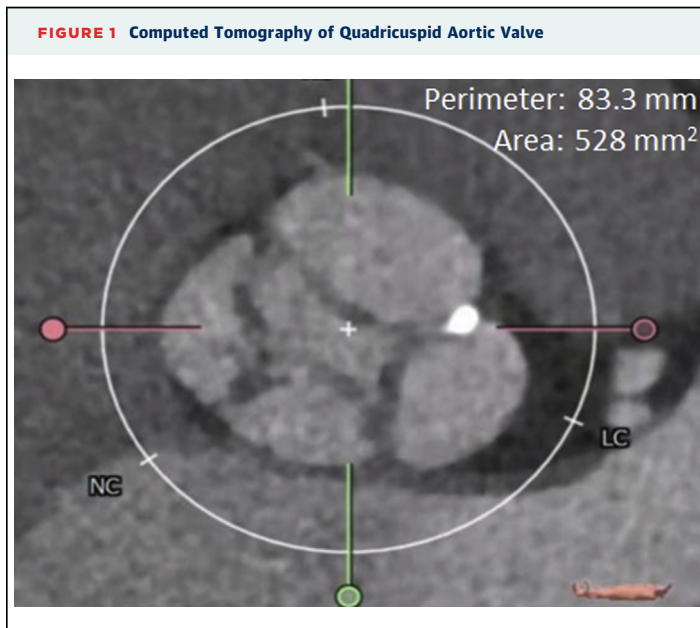
perimeter and area were 83.3 mm and 527.7 mm<sup>2</sup>, respectively.

The sizing chart (for tricuspid aortic valve) proposed a 29-mm Venus A-valve (Venus Medtech, Hangzhou, China). Nevertheless, a 26-mm valve was chosen given unfamiliarity with QAV plus uncertainty regarding annular measurements.

After pre-dilatation with a 23-mm balloon, the implantation of the 26-mm valve (deeper than anticipated) was associated with severe paravalvular leak (PVL) (**Figures 2A and 2B, Video 1**). Another 26-mm valve was implanted 10 mm higher, reducing PVL from severe to moderate (**Figure 2C, Video 1**).

To learn from this procedure and sizing in the setting of QAV, we retrospectively performed patient-specific computer simulation (FEops HEARTguide, FEops, Ghent, Belgium) (1). Briefly, a computed tomography-derived 3-dimensional model of the aortic root and valve was first created (segmentation), followed by the generation of high-quality meshes of the aortic root and valve. Finite-element computer modeling and computational fluid dynamics were used for simulation of valve implantation and quantification of PVL (1,2).

All steps of the actual implantation were respected during simulation, including the implantation depths of both valves (1). Simulation of the first valve confirmed

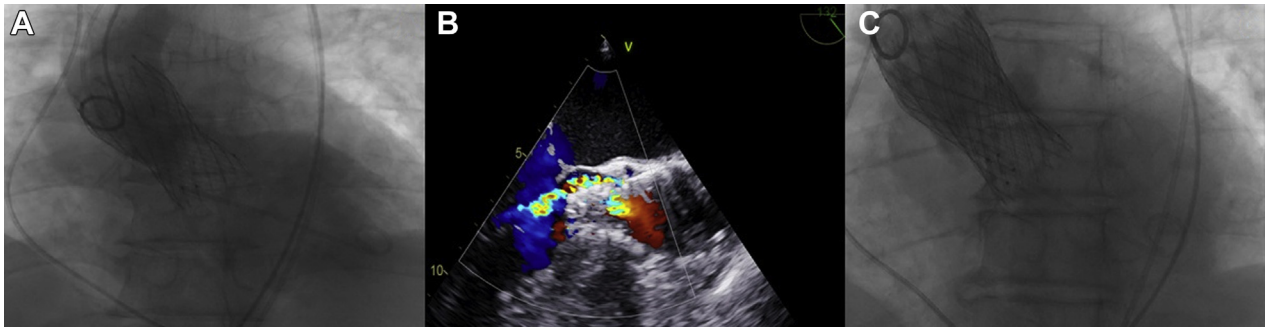


**FIGURE 1** Computed Tomography of Quadricuspid Aortic Valve

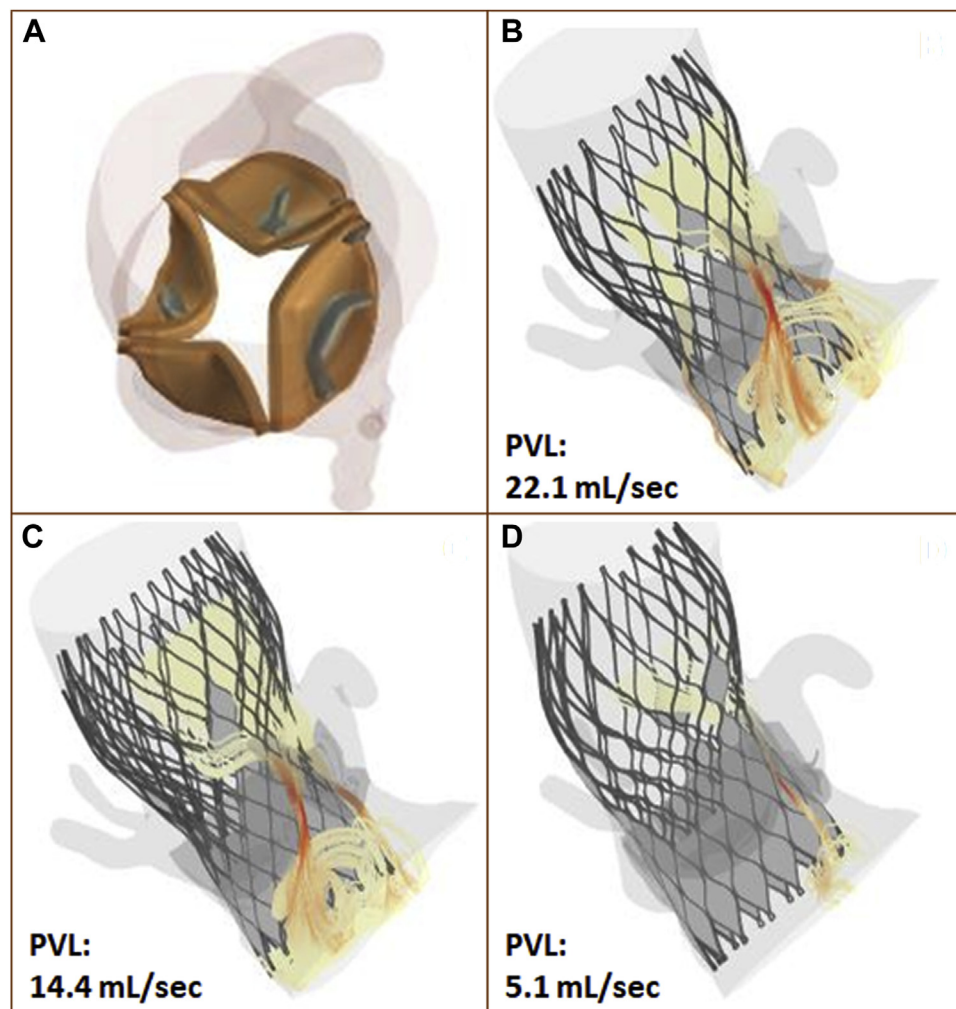
From the <sup>a</sup>Department of Cardiology, Fuwai Hospital Chinese Academy of Medical Sciences, Zhengzhou, China; <sup>b</sup>Department of Cardiology, Erasmus Medical Center, Rotterdam, the Netherlands; and the <sup>c</sup>Department of Cardiology, Centro Hospitalar de Entre o Douro e Vouga, Santa Maria da Feira, Portugal.

The authors attest they are in compliance with human studies committees and animal welfare regulations of the authors' institutions and Food and Drug Administration guidelines, including patient consent where appropriate. For more information, visit the [Author Center](#).

Manuscript received November 24, 2020; revised manuscript received December 17, 2020, accepted January 5, 2021.

**FIGURE 2** Aortic Regurgitation Severity After Valve Implantation

(A,B) Severe aortic regurgitation after first valve implantation. (C) Moderate aortic regurgitation after second valve implantation.

**FIGURE 3** Computer Modeling and Simulation TAVR

Quadricuspid valve (A), computational fluid dynamics; significant paravalvular leak (PVL) (22.1 mL/c) after first 26-mm valve implantation (B) and mild PVL (14.4 mL/s) after second 26-mm valve implantation (C). Mild PVL (5.1 mL/s) after 29-mm valve implantation (D). TAVR = transcatheter aortic valve replacement.

severe PVL (22.1 ml/s), reduced to 14.0 ml/s after the second valve, consistent with angiography (**Figures 3A to 3C, Video 1**) (2). Given PVL of 14.0 ml/l (<16.25 ml/s, which defines mild PVL), the decision not to perform dilatation after the implantation of the second valve proved correct in hindsight (2). Simulation with a 29-mm Venus valve (the size selected by the independent computed tomographic analyst at FEops) predicted mild PVL even at a lower depth (**Figure 3D, Video 2**), confirming that this was the optimal valve size.

This case highlights the role of patient-specific computer simulation in the planning of transcatheter aortic valve replacement for patients with rare or complex aortic root pathology, with implications in valve size selection and depth of implantation.

## FUNDING SUPPORT AND AUTHOR DISCLOSURES

This study is part of a project that has received funding from the European Union's Horizon 2020 research and innovation program under grant agreement no. 945698. Prof. Dr. de Jaegere is a medical adviser to FEops. All other authors have reported that they have no relationships relevant to the contents of this paper to disclose.

**ADDRESS FOR CORRESPONDENCE:** Dr. Gejun Zhang, Department of Cardiology, Fuwai Hospital Chinese Academy of Medical Sciences, Zhengzhou 100037, China. E-mail: [gjzhang212@163.com](mailto:gjzhang212@163.com). OR Prof. Peter de Jaegere, Department of Cardiology, Erasmus MC, PB Dr Molewaterplein 40, 3015 GD, Rotterdam, the Netherlands. E-mail: [p.dejaegere@erasmusmc.nl](mailto:p.dejaegere@erasmusmc.nl).

## REFERENCES

1. De Jaegere PPT, Rocatello G, Prendergast BD, et al. Patient-specific computer-simulation for transcatheter-cardiac-interventions. *Heart* 2019; 105 suppl 2:s21-7.
2. de Jaegere P, De Santis G, Rodriguez Olivares R, et al. Patient-specific computer-modeling to predict aortic regurgitation after transcatheter aortic valve replacement. *J Am Coll Cardiol Intv* 2016;9:508-12.

**KEY WORDS** aortic stenosis, computer modeling, TAVR

**APPENDIX** For supplemental videos, please see the online version of this paper.