

4-19-2023

Head-to-head comparison of 10 plasma phospho-tau assays in prodromal Alzheimer's disease

Shorena Janelidze
Lund University

Nicolas R Barthélemy
Washington University School of Medicine in St. Louis

Yingxin He
Washington University School of Medicine in St. Louis

Randall J Bateman
Washington University School of Medicine in St. Louis
et al.

Follow this and additional works at: https://digitalcommons.wustl.edu/oa_4



Part of the [Medicine and Health Sciences Commons](#)

Please let us know how this document benefits you.

Recommended Citation

Janelidze, Shorena; Barthélemy, Nicolas R; He, Yingxin; Bateman, Randall J; and et al., "Head-to-head comparison of 10 plasma phospho-tau assays in prodromal Alzheimer's disease." *Brain*. 146, 4. 1592 - 1601. (2023).

https://digitalcommons.wustl.edu/oa_4/1578

This Open Access Publication is brought to you for free and open access by the Open Access Publications at Digital Commons@Becker. It has been accepted for inclusion in 2020-Current year OA Pubs by an authorized administrator of Digital Commons@Becker. For more information, please contact vanam@wustl.edu.



Head-to-head comparison of 10 plasma phospho-tau assays in prodromal Alzheimer's disease

Shorena Janelidze,¹ Divya Bali,¹ Nicholas J. Ashton,^{2,3,4,5} Nicolas R Barthélemy,^{6,7} Jeroen Vanbrabant,⁸ Erik Stoops,⁸ Eugene Vanmechelen,⁸ Yingxin He,^{6,7} Anna Orduña Dolado,¹ Gallen Triana-Baltzer,⁹ Michael J. Pontecorvo,^{10,11} Henrik Zetterberg,^{2,12,13,14,15} Hartmuth Kolb,⁹ Manu Vandijck,¹⁶ Kaj Blennow,^{2,12} Randall J. Bateman^{6,7} and Oskar Hansson^{1,17}

Plasma phospho-tau (p-tau) species have emerged as the most promising blood-based biomarkers of Alzheimer's disease. Here, we performed a head-to-head comparison of p-tau181, p-tau217 and p-tau231 measured using 10 assays to detect abnormal brain amyloid- β ($A\beta$) status and predict future progression to Alzheimer's dementia. The study included 135 patients with baseline diagnosis of mild cognitive impairment (mean age 72.4 years; 60.7% women) who were followed for an average of 4.9 years. Seventy-one participants had abnormal $A\beta$ -status (i.e. abnormal CSF $A\beta_{42/40}$) at baseline; and 45 of these $A\beta$ -positive participants progressed to Alzheimer's dementia during follow-up. P-tau concentrations were determined in baseline plasma and CSF. P-tau217 and p-tau181 were both measured using immunoassays developed by Lilly Research Laboratories (Lilly) and mass spectrometry assays developed at Washington University (WashU). P-tau217 was also analysed using Simoa immunoassay developed by Janssen Research and Development (Janss). P-tau181 was measured using Simoa immunoassay from ADxNeurosciences (ADx), Lumipulse immunoassay from Fujirebio (Fuji) and Splex immunoassay from Mesoscale Discovery (Splex). Both p-tau181 and p-tau231 were quantified using Simoa immunoassay developed at the University of Gothenburg (UGOT). We found that the mass spectrometry-based p-tau217 (p-tau217^{WashU}) exhibited significantly better performance than all other plasma p-tau biomarkers when detecting abnormal $A\beta$ status [area under curve (AUC) = 0.947; $P_{diff} < 0.015$] or progression to Alzheimer's dementia (AUC = 0.932; $P_{diff} < 0.027$). Among immunoassays, p-tau217^{Lilly} had the highest AUCs (0.886–0.889), which was not significantly different from the AUCs of p-tau217^{Janss}, p-tau181^{ADx} and p-tau181^{WashU} (AUC_{range} 0.835–0.872; $P_{diff} > 0.09$), but higher compared with AUC of p-tau231^{UGOT}, p-tau181^{Lilly}, p-tau181^{UGOT}, p-tau181^{Fuji} and p-tau181^{Splex} (AUC_{range} 0.642–0.813; $P_{diff} \leq 0.029$). Correlations between plasma and CSF values were strongest for p-tau217^{WashU} ($R = 0.891$) followed by p-tau217^{Lilly} ($R = 0.755$; $P_{diff} = 0.003$ versus p-tau217^{WashU}) and weak to moderate for the rest of the p-tau biomarkers (R_{range} 0.320–0.669). In conclusion, our findings suggest that among all tested plasma p-tau assays, mass spectrometry-based measures of p-tau217 perform best when identifying mild cognitive impairment patients with abnormal brain $A\beta$ or those who will subsequently progress to Alzheimer's dementia. Several other assays (p-tau217^{Lilly}, p-tau217^{Janss}, p-tau181^{ADx} and p-tau181^{WashU}) showed relatively high and consistent accuracy across both outcomes. The results further indicate that the highest performing assays have performance metrics that rival the gold standards of $A\beta$ -PET and CSF. If further validated, our findings will have significant impacts in diagnosis, screening and treatment for Alzheimer's dementia in the future.

Received June 27, 2022. Revised August 01, 2022. Accepted August 20, 2022. Advance access publication September 10, 2022

© The Author(s) 2022. Published by Oxford University Press on behalf of the Guarantors of Brain.

This is an Open Access article distributed under the terms of the Creative Commons Attribution-NonCommercial License (<https://creativecommons.org/licenses/by-nc/4.0/>), which permits non-commercial re-use, distribution, and reproduction in any medium, provided the original work is properly cited. For commercial re-use, please contact journals.permissions@oup.com

- 1 Clinical Memory Research Unit, Lund University, Lund, Sweden
- 2 Department of Psychiatry and Neurochemistry, Institute of Neuroscience and Physiology, Sahlgrenska Academy, University of Gothenburg, Mölndal, Sweden
- 3 Institute of Psychiatry, Psychology and Neuroscience, Maurice Wohl Clinical Neuroscience Institute, King's College London, London, UK
- 4 NIHR Biomedical Research Centre for Mental Health and Biomedical Research Unit for Dementia at South London and Maudsley NHS Foundation, London, UK
- 5 Centre for Age-Related Medicine, Stavanger University Hospital, Stavanger, Norway
- 6 Department of Neurology, Washington University School of Medicine, St Louis, MO, USA
- 7 The Tracy Family SILQ Center, St Louis, MO, USA
- 8 ADx NeuroSciences, Gent, Belgium
- 9 Neuroscience Biomarkers, Janssen Research & Development, La Jolla, CA, USA
- 10 Avid Radiopharmaceuticals, Philadelphia, PA, USA
- 11 Eli Lilly and Company, Indianapolis, IN, USA
- 12 Clinical Neurochemistry Laboratory, Sahlgrenska University Hospital, Mölndal, Sweden
- 13 Department of Neurodegenerative Disease, UCL Institute of Neurology, Queen Square, London, UK
- 14 UK Dementia Research Institute at UCL, London, UK
- 15 Hong Kong Center for Neurodegenerative Diseases, Hong Kong, Hong Kong SAR, China
- 16 Fujirebio Europe N.V., Gent, Belgium
- 17 Memory Clinic, Skåne University Hospital, Malmö, Sweden

Correspondence to: Oskar Hansson
Memory Clinic, Skåne University Hospital, SE-20502 Malmö, Sweden
E-mail: Oskar.Hansson@med.lu.se

Keywords: blood p-tau; Alzheimer's disease; amyloid- β ; dementia

Introduction

Alzheimer's disease neuropathologic changes in the brain, i.e. accumulation amyloid- β (A β) plaques and neurofibrillary tangles containing hyperphosphorylated tau (p-tau), can be detected in living people using PET scanning or quantification of A β and p-tau proteins levels in CSF.¹ Although A β - and tau-PET as well as CSF A β _{42/40} and p-tau are highly accurate and validated diagnostic and prognostic biomarkers of Alzheimer's disease^{2–4} that have been widely used in research settings, blood-based tests are needed for implementation in clinical practice globally and to facilitate patient screening and selection in clinical trials.^{3,5}

In CSF, soluble p-tau species change in different stages and progression of Alzheimer's disease.⁶ A growing number of studies have demonstrated that three variants of p-tau, p-tau181, p-tau217 and p-tau231, measured in blood plasma hold great promise as biomarkers of Alzheimer's disease-related A β and tau pathologies.^{7–11} At the same time, there are reported differences in the performance of different plasma p-tau species and assays. For example, p-tau217 [measured using either mass spectrometry (MS) or immunoassays] has consistently shown higher accuracy for detecting abnormal CSF and PET biomarker status and differentiating Alzheimer's disease from other neurodegenerative disorders (in both clinical and neuropathological cohorts) and controls than p-tau181, even though the effect sizes were in many cases relatively small.^{7,10,12,13} Some data also suggest that while plasma p-tau231 and p-tau181 perform equally well as diagnostic biomarkers in later dementia phase of Alzheimer's disease, p-tau231 starts to increase earlier than p-tau181 and is more strongly associated with A β and tau PET measures in preclinical disease stages.^{14–16} However, it is at present unclear how much varying performance of the plasma p-tau biomarkers is attributable to analytical measurement methods. Several immunoassays¹⁷ and an MS-based method⁷ have been developed for determination of different p-tau

species in plasma and used across different studies making their interpretation challenging. MS is considered to be the 'gold standard' for protein identification and analysis and, although published work shows that MS-based plasma A β measures might more accurately reflect brain A β pathology in Alzheimer's disease than immunoassays,¹⁸ a direct comparison of these methods for blood p-tau quantification is currently lacking. Some studies, on the other hand, compared several of the available plasma p-tau immunoassays. P-tau217 measured with two different immunoassays developed by Lilly Research Laboratories and Janssen Research and Development have both been shown to accurately predict abnormal CSF A β status and future conversion to Alzheimer's disease dementia (ADD) in patients with mild cognitive impairment (MCI).¹⁹ In contrast, a certain degree of variability has been found in performance of different p-tau181 immunoassays.^{12,20} Interestingly, differences in the performance between plasma p-tau217 and p-tau181 appears much smaller when both biomarkers are measured with Lilly immunoassays that only differ in phospho-specific capture antibodies compared to the differences between Lilly p-tau217 and other p-tau181 immunoassays.^{10,12,13} Collectively, these findings suggest that immunoassay components (e.g. antibodies, other reagents, detection systems) may affect the performance of p-tau biomarkers and illustrate the importance of conducting head-to-head comparisons of different plasma p-tau immunoassays. On the other hand, MS measurement of tau peptides generated by trypsinization or other enzymatic digestions may be confounded by the presence of various endogenously produced tau truncated species.²¹ Expanding on previous preliminary studies, with the additional aim to compare MS-based methods and immunoassays, we analysed p-tau181, p-tau217 and p-tau231 using 10 assays in plasma samples from a cohort of MCI patients who were followed for up to 9.5 years to monitor progression of clinical symptoms. We tested the ability of p-tau biomarkers to identify participants with abnormal CSF A β status and to predict future progression from MCI to ADD.

Materials and methods

Participants

The study was approved by the Ethics Committee at the University of Lund and the patients and/or their relatives gave their informed consent (for research). We included 135 individuals with clinical diagnosis of MCI at baseline who were recruited at the Memory Clinic at Skåne University Hospital in Malmö, Sweden.^{19,22,23} All participants underwent a thorough physical, neurological and psychiatric examination, as well as a clinical interview focusing on cognitive symptoms and activities of daily living function by physicians with an expertise in cognitive disorders. Patients with MCI at baseline had to fulfill the criteria by Petersen,²⁴ including (i) memory complaint, preferably corroborated by an informant; (ii) objective memory impairment adjusted for age and education, as judged by the physician; (iii) preservation of general cognitive functioning, as determined by the clinician's judgement based on a structured interview with the patient and a Mini-Mental Status Examination (MMSE) score ≥ 24 ; (iv) zero or minimal impairment of daily life activities; and (v) not fulfilling the DSM-III-R criteria for dementia. The exclusion criteria were (i) significant unstable systemic illness or organ failure; (ii) current significant alcohol or substance misuse; and (iii) cognitive impairment that could be explained by other specific non-neurodegenerative disorders such as brain tumour or subdural haematoma. Study participants were followed for an average of 4.9 (SD = 2.1) years. The MCI-ADD group included participants who progressed to ADD during follow-up. Patients who received a diagnosis of Alzheimer's disease were required to meet the DSM-III-R criteria for dementia and the criteria of probable Alzheimer's disease defined by NINCDS-ADRDA²⁵ and have abnormal CSF $A\beta_{42/40}$ ratio.¹⁹ The criteria for non-ADD diagnosis in this MCI cohort have been previously described.^{22,23} Stable MCI patients and MCI who progressed to non-ADD were classified as non-progressors and further stratified into $A\beta$ -negative (A-) and $A\beta$ -positive (A+) groups based on the CSF $A\beta_{42/40}$ ratio status. The characteristics of the study participants are given in Table 1.

CSF and plasma sampling and analysis

CSF and blood sample were drawn in the morning while participants were not necessarily non-fasting. Blood was collected in six K2-EDTA-plasma tubes and centrifuged at 2000g, +4°C for 10 min. Following centrifugation plasma was aliquoted into 1.5-ml polypropylene tubes (1 ml per tube) and stored at -80°C. CSF was obtained by lumbar puncture and stored at -80°C in polypropylene tubes following the Alzheimer's Association flow chart for lumbar puncture and CSF sample processing.²⁶ All samples went through one freeze-thaw cycle before the analysis when 0.2–0.5ml were further aliquoted into LoBind tubes. P-tau217 was measured as phosphorylation occupancy at Thr217 using MS assay developed at Washington University (p-tau217^{WashU}),⁷ Meso Scale Discovery (MSD) immunoassay developed by Lilly Research Laboratories (p-tau217^{Lilly})^{10,27} and Single molecule arrays (Simoa) immunoassay developed by Janssen Research and Development (p-tau217^{Janss}).^{19,28,29} P-tau181 was measured as phosphorylation occupancy at Thr181 using MS-WashU assays (p-tau181^{WashU}),⁷ MSD immunoassay developed by Lilly Research Laboratories (p-tau181^{Lilly}),^{8,30} Simoa immunoassay developed at the University of Gothenburg (p-tau181^{UGOT}),⁹ Simoa immunoassay developed by ADx Neurosciences (p-tau181^{ADx}),^{20,31} Lumipulse immunoassay developed by Fujirebio (p-tau181^{Fuji}) and Splex immunoassay from MSD (p-tau181^{Splex}). P-tau231 was measured using in-house Simoa immunoassay developed at the

University of Gothenburg (p-tau231^{UGOT}).¹⁴ We also tested a p-tau231^{Splex} assay from MSD. However, this assay failed to detect any measurable p-tau231 in a pilot study of eight plasma samples (four from $A\beta$ -negative and the other four from $A\beta$ -positive individuals) analysed across two runs, and therefore was not included in the present study. P-tau217^{Lilly} and p-tau217^{Janss} data in overlapping sample have been reported previously.¹⁹ CSF samples ($n = 78$) were analysed using p-tau217^{WashU}, p-tau217^{Lilly}, p-tau217^{Janss}, p-tau181^{WashU}, p-tau181^{ADx}, p-tau181^{UGOT}, p-tau181^{Fuji} and p-tau231^{UGOT} assays. CSF $A\beta_{40}$ and $A\beta_{42}$ levels were assessed using commercially available MSD immunoassays. Amyloid positivity was defined based on CSF $A\beta_{42/40}$ and a previously described threshold of 0.07.^{22,23} All samples were analysed by staff blinded to the clinical data. Further details of the p-tau analyses are described in the [Supplementary material](#) and data on assay performance are shown in [Table 2](#) and [Supplementary Fig. 1](#).

Statistical analysis

SPSS (version 28, IBM, Armonk, NY, US) and R (version 4.1.2) in RStudio³² were used for statistical analysis. Demographic and clinical data were compared with Mann-Whitney U, Kruskal-Wallis and χ^2 (sex and APOE $\epsilon 4$ positivity) tests. Group differences in the log₁₀-transformed biomarker levels were assessed with univariate general linear models adjusting for age and sex and additionally for duration of follow-up when comparing MCI participants who progressed to ADD with those who did not. In figures, fold changes relative to the mean of the A- stable MCI group are presented to aid interpretation of biomarker levels across comparisons. Correlations between CSF and plasma were examined using the Spearman test, and we used bootstrapping ($n = 2000$ iterations) to test differences in the correlation coefficients. Diagnostic accuracies of CSF biomarkers were assessed using receiver operating characteristic (ROC) curve analysis. The Youden index with bootstrapping ($n = 2000$ iterations) was used to determine sensitivity, specificity and accuracy with 95% confidence interval (CI) at optimal thresholds. Area under the curve (AUC) of two ROC curves were compared with a DeLong test with adjustment for multiple comparisons using the Benjamini-Hochberg false discovery rate method.³³ For p-tau181^{UGOT} and p-tau181^{Splex} assays, plasma samples from 124 and 101 participants, respectively, were analysed and included in the main analysis. However, we performed a sensitivity analysis in subsamples where all plasma p-tau measures were available. Two-sided $P < 0.05$ was considered statistically significant.

Data availability

Anonymized data will be shared by request from a qualified academic investigator for the sole purpose of replicating procedures and results presented in the article and as long as data transfer is in agreement with EU legislation on the general data protection regulation and decisions by the Ethical Review Board of Sweden and Region Skåne, which should be regulated in a material transfer agreement.

Results

Participants

The study included 45 MCI patients who progressed to ADD (MCI-ADD), 64 non-progressors with normal $A\beta$ - status (A-) and 26 A+ non-progressors (Table 1). There were differences in age [$H(2) = 19.0$, $P < 0.001$], sex [$\chi^2(2) = 8.1$, $P = 0.018$], MMSE [$H(2) = 30.1$, $P < 0.001$], APOE $\epsilon 4$ carriership [$\chi^2(2) = 33.0$, $P < 0.001$] and follow-up

Table 1 Demographic and clinical characteristics

	Overall	Non-progressors A– ^a	Non-progressors A+ ^a	MCI-ADD
n	135	64	26	45
Age, years	74.0 (66.0–79.0)	70.5 (63.0–76.8)	72.0 (65.0–76.0)	78.0 (73.5–81.0)
Female, n (%)	82 (60.7)	37 (57.8)	11 (42.3)	34 (75.6)
MMSE	28.0 (26.0–29.0)	28.0 (27.0–29.0)	28.0 (27.0–29.3)	26.0 (25.0–27.0)
APOE ε4 positivity, n (%)	75 (55.6)	19 (29.7)	20 (76.9)	36 (80.0)
Follow-up time, years	4.6 (3.3–6.6)	6.21 (4.02–7.21)	5.16 (3.90–6.64)	3.64 (2.68–4.65)
Plasma p-tau				
p-tau217 ^{WashU} , %	1.36 (0.742–3.25)	0.753 (0.614–0.951)	1.88 (1.27–2.73)	3.49 (2.91–4.73)
p-tau217 ^{Lilly} , pg/ml ^b	0.247 (0.170–0.404)	0.177 (0.146–0.201)	0.275 (0.200–0.359)	0.442 (0.330–0.532)
p-tau217 ^{Janss} , pg/ml ^b	0.055 (0.030–0.105)	0.034 (0.020–0.049)	0.066 (0.036–0.104)	0.109 (0.077–0.173)
p-tau181 ^{ADx} , pg/ml	29.7 (19.3–46.3)	19.5 (10.4–27.3)	30.0 (22.8–45.0)	46.3 (38.8–63.7)
p-tau181 ^{WashU} , %	23.5 (19.8–28.7)	20.3 (18.2–22.7)	24.5 (20.7–29.0)	28.4 (25.7–32.1)
p-tau231 ^{UGOT} , pg/ml	20.9 (15.7–27.3)	16.8 (12.7–21.4)	22.0 (17.6–27.2)	26.9 (22.6–33.1)
p-tau181 ^{Lilly} , pg/ml	1.90 (1.42–2.59)	1.57 (1.20–1.90)	1.77 (1.49–2.26)	2.59 (2.04–3.30)
p-tau181 ^{UGOT} , pg/ml ^c	2.46 (1.72–3.55)	1.88 (1.49–2.58)	2.43 (1.89–3.45)	3.38 (2.58–4.07)
p-tau181 ^{Fuji} , pg/ml	4.80 (3.64–5.75)	3.83 (3.01–5.14)	4.73 (3.74–5.57)	5.61 (4.77–6.25)
p-tau181 ^{Splex} , pg/ml ^b	1.07 (0.859–1.55)	0.999 (0.792–1.22)	0.927 (0.754–1.73)	1.28 (1.05–2.16)

Data are shown as median (interquartile range) unless otherwise specified.

^aAβ status was defined using the CSF Aβ_{42/40} cutoff (0.07) as described in the 'Materials and methods' section

^bp-tau217^{Lilly} and p-tau217^{Janss} data in overlapping sample have been reported previously.¹⁹

^cp-tau181-UGOT and p-tau181-Splex data were available for 124 and 101 participants, respectively.

Table 2 Analytical performance of plasma p-tau assays

Plasma biomarkers	Required plasma volume, ml	Intra-assay CV, %	Inter-assay CV, %	Samples below LLOD, %	LLOD, pg/ml
p-tau217 ^{WashU}	1 ^a	3.3 ^b	3.5 ^b	0	NA ^c
p-tau217 ^{Lilly}	0.07	6.8	10.1	15.6	0.150
p-tau217 ^{Janss}	0.2	23.7	12.4	0	0.013
p-tau181 ^{ADx}	0.1	11.1	3.8	16.3	2.312
p-tau181 ^{WashU}	1 ^a	3.7 ^b	0.4 ^b	0	NA ^c
p-tau231 ^{UGOT}	0.08	7.6	8.5	0	1
p-tau181 ^{Lilly}	0.07	6.0	11.2	0	0.864
p-tau181 ^{UGOT}	0.08	8.2	10.9	0	0.5
p-tau181 ^{Fuji}	0.13	NA ^d	NA ^d	0	0.052
p-tau181 ^{Splex}	0.06	4.8	13.5	0	0.190

CV = coefficient of variation; LLOD = lower limit of detection.

^aOne millilitre was required for the entire multiplex assay.

^bCVs were estimated using quality control samples; study samples were tested in singlicate.

^cNot applicable for phosphorylation occupancy measures.

^dNot applicable, samples in this study were tested in singlicate in one run.

duration [H(2) = 23.3, $P < 0.001$] between the groups. The MCI-ADD group was on average older, had lower MMSE and shorter follow-up time than both non-progressor groups ($P < 0.001$). There were more women among MCI-ADD compared with A+ non-progressors ($P = 0.005$) and A– non-progressors ($P = 0.056$), whereas APOE ε4 positivity rate was lower in A– non-progressors than both A+ non-progressors and MCI-ADD ($P < 0.001$).

Associations with Aβ pathology

We first assessed how well plasma p-tau species measured with different assays identified individuals with abnormal baseline Aβ status among all study participants with baseline diagnosis of MCI (Fig. 1A and Table 3). In the ROC curve analysis, the MS-based p-tau217 assay (p-tau217^{WashU}) performed significantly better than all other p-tau biomarkers with an AUC of 0.947 (95% CI, 0.907–0.987; $P_{diff} < 0.015$). Among immunoassays, p-tau217^{Lilly} had the highest AUC (AUC = 0.886; CI, 0.827–0.944), which was not

significantly different from the AUCs of p-tau217^{Janss} (AUC = 0.858; 95% CI, 0.795–0.920; $P_{diff} = 0.38$), p-tau181^{ADx} (AUC = 0.841; 95% CI, 0.768–0.913; $P_{diff} = 0.24$) and p-tau181^{WashU} (AUC = 0.835; 95% CI, 0.765–0.906; $P_{diff} = 0.20$), but higher compared with AUC of p-tau231^{UGOT}, p-tau181^{Lilly}, p-tau181^{UGOT}, p-tau181^{Fuji} and p-tau181^{Splex} (AUC_{range} 0.642–0.784; $P_{diff} \leq 0.029$). For comparison, the AUCs of the best performing CSF p-tau assays in a subsample of 78 participants with CSF measures available ranged between 0.948 and 0.975 (p-tau217^{WashU}, AUC = 0.975; p-tau181^{ADx}, AUC = 0.961; p-tau181^{WashU}, AUC = 0.954; p-tau217^{Lilly}, AUC = 0.952; p-tau217^{Janss}, AUC = 0.948). CSF p-tau showed significantly higher AUCs than corresponding plasma p-tau for most assays (Supplementary Table 1).

When testing differences in plasma p-tau levels between A+ and A– groups, we found that all 10 p-tau biomarkers were significantly higher in A+ MCI than A– MCI (Fig. 2). However, the fold increase in the A+ group compared with the A– group was largest for the p-tau217^{WashU} (mean = 3.6, SD = 1.9), followed by p-tau217^{Janss}





A A- MCI vs A+ MCI**B Non-progressors vs progressors**

Figure 1 ROC curve analysis for abnormal CSF $A\beta_{42/40}$ status and progression to ADD. ROC curve analysis for differentiating (A) MCI participants with abnormal CSF $A\beta_{42/40}$ from those with normal CSF $A\beta_{42/40}$ and (B) MCI patients who progressed to ADD during follow-up from those who did not (stable MCI patients and MCI patients who progressed to other types of dementia).

(mean = 2.7, SD = 1.8), p-tau217^{Lilly} (mean = 2.0, SD = 1.0) and p-tau181^{ADx} (mean = 1.8, SD = 0.8), and ranged between 1.2 and 1.4 for the rest of the biomarkers.

Prediction of future progression to Alzheimer's disease dementia

We next studied the performance of the plasma p-tau biomarkers to predict future clinical progression to ADD (Fig. 1B and Table 4). When distinguishing MCI patients who progressed to ADD during follow-up from those who did not, p-tau217^{WashU} again showed significantly higher AUC than all other p-tau biomarkers (AUC = 0.932; 95% CI, 0.891–0.974; $P_{diff} < 0.027$), followed by p-tau217^{Lilly} (AUC = 0.889; 95% CI, 0.833–0.946). P-tau217^{Janss} (AUC = 0.872; 95% CI,

0.814–0.931; $P_{diff} = 0.53$), p-tau181^{ADx} (AUC = 0.846; 95% CI, 0.777–0.916; $P_{diff} = 0.16$) and p-tau181^{WashU} (AUC = 0.835; 95% CI, 0.764–0.906; $P_{diff} = 0.09$) were non-inferior to p-tau217^{Lilly}, whereas p-tau231^{UGOT}, p-tau181^{Lilly}, p-tau181^{UGOT}, p-tau181^{Fuji} and p-tau181^{Splex} all had significantly lower AUCs (AUC_{range} 0.688–0.813; $P_{diff} \leq 0.013$). For comparison, the AUCs of the best performing CSF p-tau assays in a subsample of 78 participants with CSF measures available ranged between 0.907 and 0.943 (p-tau217^{WashU}, AUC = 0.943; p-tau217^{Janss}, AUC = 0.928; p-tau217^{Lilly}, AUC = 0.926; p-tau181^{ADx}, AUC = 0.924; p-tau181^{Fuji}, AUC = 0.907). The differences in AUCs between CSF and corresponding plasma p-tau assays were not significant (Supplementary Table 1).

We also found differences in plasma concentrations of all p-tau biomarkers except p-tau181^{Fuji} between the A– non-progressor, A+

Table 3 Associations of plasma p-tau with CSF A β _{42/40}

Plasma p-tau	AUC (95% CI)	P-value versus p-tau217 ^{WashU}	P-value versus p-tau217 ^{Lilly}	Specificity (95% CI)	Sensitivity (95% CI)	Accuracy (95% CI)
p-tau217 ^{WashU}	0.947 (0.907–0.987)	NA	0.015	90.6 (82.8–98.4)	94.4 (84.5–98.6)	92.6 (88.1–96.3)
p-tau217 ^{Lilly}	0.886 (0.827–0.944)	0.015	NA	84.4 (71.9–96.9)	85.9 (67.6–95.8)	84.4 (78.5–90.4)
p-tau217 ^{Janss}	0.858 (0.795–0.920)	0.004	0.38	87.5 (65.6–95.3)	74.6 (60.6–91.5)	80.0 (73.3–86.7)
p-tau181 ^{ADx}	0.841 (0.768–0.913)	<0.001	0.24	85.9 (68.8–95.3)	77.5 (66.2–93.0)	81.5 (74.8–87.4)
p-tau181 ^{WashU}	0.835 (0.765–0.906)	<0.001	0.20	87.5 (73.4–95.3)	76.1 (64.8–88.7)	81.5 (74.8–87.4)
p-tau231 ^{UGOT}	0.784 (0.703–0.864)	<0.001	0.029	73.4 (46.9–87.5)	78.9 (64.8–98.6)	76.3 (69.6–82.2)
p-tau181 ^{Lilly}	0.759 (0.676–0.841)	<0.001	<0.001	78.1 (65.6–89.1)	71.8 (60.6–84.5)	75.6 (68.1–82.2)
p-tau181 ^{UGOT} ^a	0.743 (0.652–0.833)	<0.001	0.005	70.2 (50.9–86.0)	79.1 (59.7–92.5)	74.2 (66.9–81.5)
p-tau181 ^{Fuji}	0.694 (0.604–0.784)	<0.001	<0.001	56.3 (40.6–85.9)	84.5 (50.7–93.0)	69.6 (62.2–76.3)
p-tau181 ^{Splex} ^a	0.642 (0.533–0.751)	<0.001	<0.001	79.6 (22.4–98.0)	53.8 (26.9–100.0)	65.3 (58.4–73.3)

Data are from ROC curve analysis. MCI participants were classified as amyloid-negative (n = 64) or as amyloid-positive (n = 71) using CSF A β _{42/40} as described in the methods. ^ap-tau181-UGOT and p-tau181-Splex data were available for 124 (57 amyloid-negative, 67 amyloid-positive) and 101 (49 amyloid-negative, 52 amyloid-positive) participants, respectively.

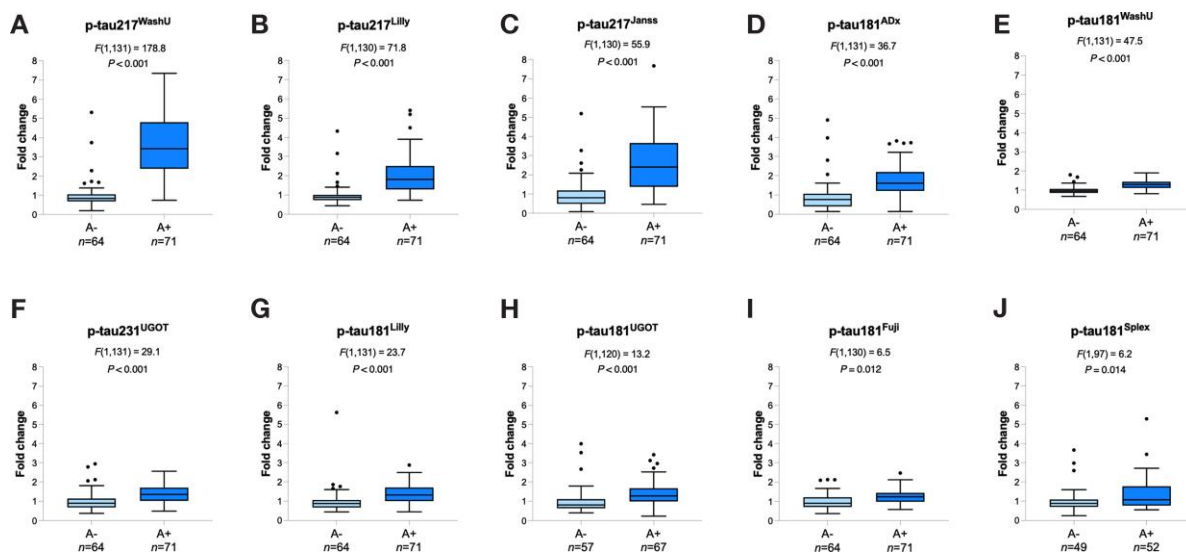


Figure 2 Plasma p-tau biomarkers in amyloid-negative and -positive MCI patients. Plasma levels of p-tau217 (A–C), p-tau181 (D–E and G–J) and p-tau231 (F) measured using different assays in the A– and A+ MCI groups. A β status was defined based on the CSF A β _{42/40} ratio. Data are presented as a fold change from the mean of the A– MCI group. Two p-tau217^{WashU} and p-tau217^{Janss} outliers in the A+ group and one p-tau181^{ADx} outlier in the A– group are not shown in A, C and D, but these data were included in the statistical analysis. F-values and P-values are from univariate general linear models adjusted for age and sex. Boxes show interquartile range, the horizontal lines are medians and the whiskers and outliers were plotted using the Tukey method.

non-progressor and MCI-ADD groups (Fig. 3). Post hoc analysis revealed that plasma levels of p-tau217 (when measured with three different assays), but not p-tau181 or p-tau231, were higher in MCI-ADD than A+ non-progressors (P < 0.002). At the same time, the three p-tau217 biomarkers as well as the best performing p-tau181 biomarkers (p-tau181^{WashU} and p-tau181^{ADx}) were increased in both A+ non-progressors and MCI-ADD compared with A– non-progressors (P ≤ 0.001). P-tau217^{WashU} showed the largest fold increase in both MCI-ADD (mean = 4.3, SD = 1.7) and A+ non-progressors (mean = 2.5, SD = 1.4) compared with A– non-progressors. Fold increase was also larger in MCI-ADD (mean_{range} 2.0–3.2) than in A+ non-progressors (mean_{range} 1.4–1.9) for p-tau217^{Lilly}, p-tau217^{Janss} and p-tau181^{ADx}.

Correlations between plasma and CSF p-tau

Finally, we examined associations between plasma and CSF p-tau biomarkers (Fig. 4). CSF p-tau concentrations are presented in

Supplementary Table 2. In line with other results of this study, the strongest correlations between CSF and plasma were seen for p-tau217^{WashU} (R = 0.891; 95% CI, 0.832–0.930), followed by p-tau217^{Lilly} (R = 0.755; 95% CI, 0.635–0.839) with significant difference in correlation coefficients between the two biomarkers (P = 0.003). The correlations were weak to moderate for the rest of the biomarkers (R_{range} 0.320–0.669).

Plasma p-tau217^{WashU} correlated strongly with plasma p-tau217^{Lilly}, p-tau217^{Janss}, p-tau181^{ADx} and p-tau181^{WashU} (R_{range} 0.712–0.862; Supplementary Fig. 2), while correlations with other plasma p-tau biomarkers were weak to moderate (R_{range} 0.376–0.619; Supplementary Fig. 2).

Sensitivity analysis

The results were similar when statistical analysis was performed in smaller sub-samples where p-tau181^{UGOT} and p-tau181^{Splex} data were available (Supplementary Tables 3–6). Briefly, plasma

Table 4 Associations of plasma p-tau with future progression to ADD

Plasma p-tau	AUC (95% CI)	P-value versus p-tau217 ^{WashU}	P-value versus p-tau217 ^{Lilly}	Specificity (95% CI)	Sensitivity (95% CI)	Accuracy (95% CI)
p-tau217 ^{WashU}	0.932 (0.891–0.974)	NA	0.027	86.7 (77.8–93.3)	95.6 (84.4–100.0)	88.9 (83.7–94.1)
p-tau217 ^{Lilly}	0.889 (0.833–0.946)	0.027	NA	83.3 (65.6–93.3)	88.9 (73.3–100.0)	84.4 (75.6–90.4)
p-tau217 ^{Janss}	0.872 (0.814–0.931)	0.027	0.53	74.4 (61.1–91.1)	91.1 (71.1–100.0)	80.0 (71.9–87.4)
p-tau181 ^{ADx}	0.846 (0.777–0.916)	0.007	0.16	81.1 (72.2–88.9)	91.1 (80.0–97.8)	84.4 (77.8–90.4)
p-tau181 ^{WashU}	0.835 (0.764–0.906)	0.001	0.09	76.7 (64.4–86.7)	88.9 (77.8–97.8)	80.7 (72.6–86.7)
p-tau181 ^{Lilly}	0.813 (0.734–0.892)	0.002	0.013	74.4 (60.0–86.7)	86.7 (71.1–97.8)	77.8 (70.4–85.2)
p-tau231 ^{UGOT}	0.777 (0.699–0.856)	<0.001	0.009	68.9 (57.8–81.1)	86.7 (73.3–95.6)	74.8 (67.4–81.5)
p-tau181 ^{UGOT a}	0.775 (0.692–0.858)	<0.001	0.014	65.9 (52.4–82.9)	88.1 (69.0–97.6)	73.4 (64.5–81.5)
p-tau181 ^{Fuji}	0.735 (0.649–0.821)	<0.001	0.002	70.0 (40.0–86.7)	75.6 (53.3–97.8)	71.1 (57.8–79.3)
p-tau181 ^{Splex a}	0.688 (0.579–0.796)	<0.001	<0.001	66.7 (50.0–90.9)	74.3 (42.9–91.4)	69.3 (59.4–78.2)

Data are from a ROC curve analysis. Forty-five MCI participants progressed to ADD during follow-up and 90 remained stable or progressed to non-ADD.

^ap-tau181-UGOT and p-tau181-Splex data were available for 124 (82 non-progressors, 42 MCI-ADD) and 101 (66 non-progressors, 35 MCI-ADD) participants, respectively.

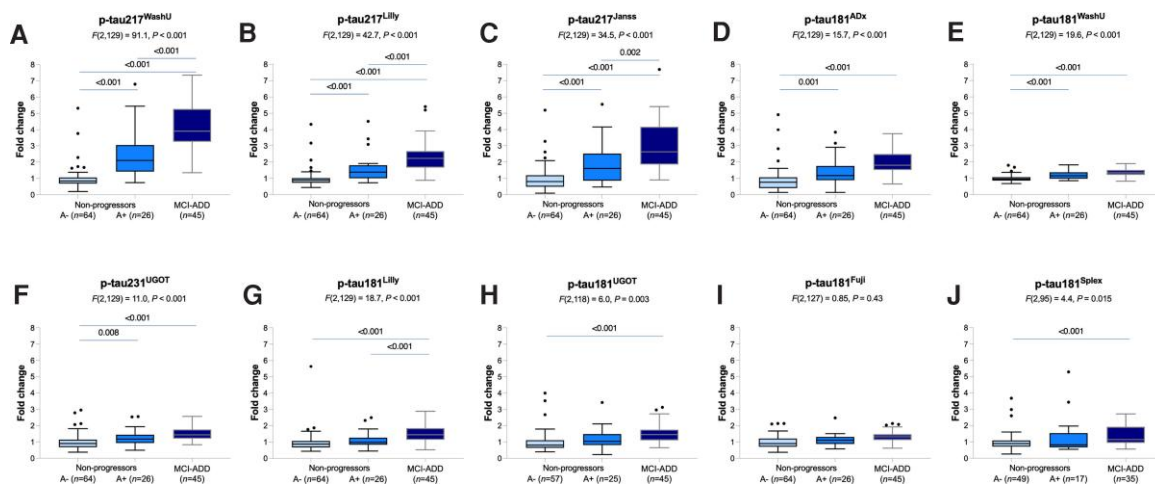


Figure 3 Plasma p-tau biomarkers in MCI participants who progressed to ADD during follow-up and amyloid-negative and -positive non-progressors. Plasma levels of p-tau217 (A–C), p-tau181 (D–E and G–J) and p-tau231 (F) measured using different assays in patients with MCI who progressed to ADD during follow-up (MCI-ADD), A– and A+ non-progressor MCI patients. A β status was defined based on the CSF A β _{42/40} ratio. Data are presented as a fold change from the mean of the A– MCI group. Two p-tau217^{WashU} and p-tau217^{Janss} outliers in the MCI-ADD group and one p-tau181^{ADx} outlier in the A– group are not shown in A, C and D, but these data were included in the statistical analysis. F-values and P-values are from univariate general linear models adjusted for age, sex and follow-up time. Boxes show interquartile range, the horizontal lines are medians and the whiskers and outliers were plotted using the Tukey method.

p-tau217^{WashU} showed the best performance when detecting both abnormal A β status and progression to ADD (AUC_{range} 0.927–0.955), followed by p-tau217^{Lilly} (AUC_{range} 0.878–0.900), p-tau217^{Janss} (AUC_{range} 0.860–0.870), p-tau181^{ADx} (AUC_{range} 0.832–0.860) and p-tau181^{WashU} (AUC_{range} 0.809–0.827). None of the AUCs of p-tau231^{UGOT}, p-tau181^{Lilly}, p-tau181^{UGOT}, p-tau181^{Fuji} or p-tau181^{Splex} were consistently above 0.800.

Discussion

Recently developed blood tests for A β and p-tau are anticipated to transform Alzheimer's disease research and care. Here we sought to directly compare currently available methods for determinations of p-tau in blood in order to establish which of these methods are accurate enough to be useful for implementation in clinical practice or drug trials. In this study including patients with MCI, plasma p-tau217 quantified using MS-based assay showed very high accuracy when both identifying participants with abnormal A β status and those who progress to ADD during follow-up with AUCs >

0.93, which was higher than for the other p-tau biomarkers. Furthermore, this assay exhibited significantly higher correlations with p-tau levels in CSF than the other p-tau assays. However, p-tau217^{Lilly}, p-tau217^{Janss}, p-tau181^{ADx} and p-tau181^{WashU} all displayed relatively high and consistent accuracy across both outcomes (AUC_{range} 0.835–0.889), whereas the performance of other biomarkers (p-tau231^{UGOT}, p-tau181^{Lilly}, p-tau181^{UGOT}, p-tau181^{Fuji}, p-tau181^{Splex}) was significantly inferior (AUC_{range} 0.642–0.813). Of note, there was no added value of combining different plasma p-tau species (p-tau217^{WashU}, p-tau181^{ADx} and p-tau231^{UGOT}) when either distinguishing normal from abnormal A β status or predicting future progression to ADD (data not shown).

MS-based measure of plasma p-tau217 has previously shown very good accuracy to detect A β pathology in two mixed cohorts of cognitively healthy controls, MCI participants and patients at different stages of Alzheimer's disease.⁷ Using an improved version of the same MS assay (now requiring lower volume of plasma) we demonstrate that p-tau217^{WashU} accurately predicted abnormal A β status as well as future progression to ADD in a sample of MCI patients. One novel finding of the present study is that MS




Figure 4 Correlations between CSF and plasma p-tau. Heat map showing Spearman coefficients for correlations between CSF and plasma p-tau measured using different assays (p-tau181^{UGOT}, n = 72; p-tau181^{SpIex}, n = 52; all other biomarkers n = 78). Correlations between plasma and CSF p-tau measured with the same assay are highlighted in orange except plasma p-tau181^{Lilly} and p-tau181^{SpIex} for which corresponding CSF assay data were not available.

p-tau217^{WashU} performed significantly better than p-tau217 quantified with immunoassays. A possible explanation for this may be that MS-based detection methods are highly accurate and potentially more so than immunoassays, and therefore could more reliably quantify low abundance proteins in protein-rich matrices such as blood as was seen for plasma Aβ.¹⁸

We also found that p-tau217^{WashU} performed better than p-tau181^{WashU} corroborating the results of an earlier MS-based study.⁷ The higher performance of p-tau217 over p-tau181 has been shown for immunoassays-based p-tau measures^{10,12,13} as well as for CSF p-tau217 and p-tau181^{34,35} and could be due to the specificity of p-tau217 for Alzheimer’s disease (this biomarker is found at considerably lower levels in people without Alzheimer’s disease compared to p-tau181) and to a greater dynamic range of p-tau217, i.e. larger fold increase in relation to developing Aβ and tau pathologies. Among eight immunoassays tested in the present study, p-tau217^{Lilly} displayed numerically highest AUCs which were significantly different from the AUCs of several p-tau181 biomarkers. However, p-tau217^{Lilly}, p-tau217^{Janss} and p-tau181^{ADx} all exhibited comparable accuracies for both abnormal Aβ status and progression to ADD indicating substantial variability in the performance of p-tau181 that is most likely caused by the differences in antibodies and analytical procedures used across the assays.

Our study has several limitations. The overall sample size was moderate with a relatively small number of A+ non-progressors and participants with CSF data, which might have affected the analysis. The cohort was restricted to MCI participants, and it is possible that the performance of the plasma p-tau assays varies across disease stages, warranting future investigations in individuals with preclinical Alzheimer’s disease. Nevertheless, our findings in MCI patients are very relevant given that this patient group represents the most likely target population to receive

disease-modifying therapies in the clinical setting in the coming years. Replication in more heterogeneous and ethnically diverse population-based cohorts is also needed. Finally, future larger studies should establish if combining individual plasma p-tau biomarkers with other accessible demographic and clinical measures could further improve their diagnostic and prognostic accuracy as has previously been shown for plasma p-tau217.³⁶

In conclusion, we show that there are significant and meaningful differences in the performance of plasma p-tau assays that have to be taken into account when interpreting results from published work. Our data support superior performance of MS p-tau217 to detect abnormal Aβ status and progression to ADD in MCI patients. In addition, we report relatively high and consistent accuracy for several p-tau immunoassays for both outcomes. Overall, our findings indicate that certain MS-based methods and immunoassays might be suitable for implementation in drug trials and clinical practice whereas others require substantial improvement. An important consideration is that compared with immunoassays, currently available research-based MS analytical technologies are more labour intensive and time consuming with less throughput. However, with the development of commercial fully automated MS platforms which have already increased capacity and speed with automated systems, MS platforms can provide reasonable clinical access.

Acknowledgements

We would like to thank Nele Dewit, a former employee of ADx NeuroSciences, for performing the plasma p-tau181ADx assays.

Funding

Work at the authors’ research centre was supported by the Swedish Research Council (2016-00906), the Knut and Alice Wallenberg foundation (2017-0383), the Marianne and Marcus Wallenberg Foundation (2015.0125), the Strategic Research Area MultiPark (Multidisciplinary Research in Parkinson’s disease) at Lund University, the Swedish Alzheimer Foundation (AF-939932), the Swedish Brain Foundation (FO2021-0293), The Parkinson Foundation of Sweden (1280/20), the Konung Gustaf V:s och Drottning Victorias Frimurarestiftelse, the Skåne University Hospital Foundation (2020-O00028), Regionalt Forskningsstöd (2020-0314) and the Swedish federal government under the ALF agreement (2018-Projekt0279). H.Z. is a Wallenberg Scholar supported by grants from the Swedish Research Council (#2018-02532), the European Research Council (#681712 and #101053962), Swedish State Support for Clinical Research (#ALFGBG-71320), the Alzheimer Drug Discovery Foundation (ADDF), USA (#201809-2016862), the AD Strategic Fund and the Alzheimer’s Association (#ADSF-21-831376-C, #ADSF-21-831381-C and #ADSF-21-831377-C), the Olav Thon Foundation, the Erling-Persson Family Foundation, Stiftelsen för Gamla Tjänarinnor, Hjärfonden, Sweden (#FO2019-0228), the European Union’s Horizon 2020 research and innovation programme under the Marie Skłodowska-Curie grant agreement No 860197 (MIRIADE), the European Union Joint Programme – Neurodegenerative Disease Research (PN2021-00694), and the UK Dementia Research Institute at UCL (UKDRI-1003). K.B. is supported by the Swedish Research Council (#2017-00915), the Alzheimer Drug Discovery Foundation (ADDF), USA (#RDAPB-201809-2016615), the Swedish Alzheimer Foundation (#AF-930351, #AF-939721 and #AF-968270), Hjärfonden, Sweden (#FO2017-0243 and #ALZ2022-0006), the Swedish state under the agreement between the Swedish government and the County

Councils, the ALF-agreement (#ALFGBG-715986 and #ALFGBG-965240), the European Union Joint Program for Neurodegenerative Disorders (JPND2019-466-236), the National Institutes of Health (NIH), USA, (grant #1R01AG068398-01), and the Alzheimer's Association 2021 Zenith Award (ZEN-21-848495). This study was supported by Coins for Alzheimer's Research Trust (PI N.R.B.), The Tracy Family SILQ Center (PI R.J.B.) and Pilot Grant (PI N.R.B.), and the NIH NINDS R01NS095773 (PI RJB). The funding sources had no role in the design and conduct of the study; in the collection, analysis, interpretation of the data; or in the preparation, review, or approval of the manuscript.

Competing interests

H.Z. has served at scientific advisory boards and/or as a consultant for Abbvie, Alector, ALZPath, Annexon, Apellis, Artery Therapeutics, AZTherapies, CogRx, Denali, Eisai, Nervgen, Novo Nordisk, Pinteon Therapeutics, Red Abbey Labs, reMYND, Passage Bio, Roche, Samumed, Siemens Healthineers, Triplet Therapeutics and Wave, has given lectures in symposia sponsored by Cellectricon, Fujirebio, Alzecure, Biogen and Roche, and is a co-founder of Brain Biomarker Solutions in Gothenburg AB (BBS), which is a part of the GU Ventures Incubator Program (outside submitted work). K.B. has served as a consultant, at advisory boards, or at data monitoring committees for Abcam, Axon, BioArctic, Biogen, JOMDD/Shimadzu, Julius Clinical, Lilly, MagQu, Novartis, Ono Pharma, Pharmatrophix, Prothena, Roche Diagnostics and Siemens Healthineers, and is a co-founder of Brain Biomarker Solutions in Gothenburg AB (BBS), which is a part of the GU Ventures Incubator Program (outside submitted work). R.J.B. has received research funding from Avid Radiopharmaceuticals, Janssen, Roche/Genentech, Eli Lilly, Eisai, Biogen, AbbVie, Bristol Myers Squibb and Novartis. Washington University and R.J.B. have equity ownership interest in C2N Diagnostics. R.J.B. and N.R.B. receive income based on technology (blood plasma assay, and methods of diagnosing Alzheimer's disease with phosphorylation changes) licensed by Washington University to C2N Diagnostics. R.J.B. receives income from C2N Diagnostics for serving on the scientific advisory board. R.J.B. serves on the Roche Gantenerumab Steering Committee as an unpaid member. M.J.P. is an employee of Avid radiopharmaceuticals, a wholly owned subsidiary of Eli Lilly and Company, and is a minor stockholder in Eli Lilly. O.H. has acquired research support (for the institution) from ADx, AVID Radiopharmaceuticals, Biogen, Eli Lilly, Eisai, Fujirebio, GE Healthcare, Pfizer and Roche. In the past 2 years, he has received consultancy/speaker fees from AC Immune, Amylyx, Alzpath, BioArctic, Biogen, Cerveau, Fujirebio, Genentech, Novartis, Roche and Siemens. The rest of authors do not report any disclosures. G.T.B. and H.K. are employees of Janssen Research and Development. J.V. and E.S. are employees of ADx NeuroSciences. E.V.M. is a co-founder of ADx NeuroSciences. M.V. is an employee of Fujirebio Europe N.V.

Supplementary material

Supplementary material is available at *Brain* online.

References

- Scheltens P, Blennow K, Breteler MM, et al. Alzheimer's disease. *Lancet*. 2016;388:505–517.
- Blennow K, Mattsson N, Scholl M, Hansson O, Zetterberg H. Amyloid biomarkers in Alzheimer's disease. *Trends Pharmacol Sci*. 2015;36:297–309.
- Hansson O. Biomarkers for neurodegenerative diseases. *Nat Med*. 2021;27:954–963.
- Ossenkoppele R, van der Kant R, Hansson O. Tau biomarkers in Alzheimer's disease: towards implementation in clinical practice and trials. *Rapid Review. Lancet Neurol*. 2022;21:726–734.
- Blennow K. Phenotyping Alzheimer's disease with blood tests. *Science*. 2021;373:626–628.
- Barthelemy NR, Li Y, Joseph-Mathurin N, et al. A soluble phosphorylated tau signature links tau, amyloid and the evolution of stages of dominantly inherited Alzheimer's disease. *Nat Med*. 2020;26:398–407.
- Barthelemy NR, Horie K, Sato C, Bateman RJ. Blood plasma phosphorylated-tau isoforms track CNS change in Alzheimer's disease. *J Exp Med*. 2020;217.
- Janelidze S, Mattsson N, Palmqvist S, et al. Plasma P-tau181 in Alzheimer's disease: relationship to other biomarkers, differential diagnosis, neuropathology and longitudinal progression to Alzheimer's dementia. *Nature Medicine*. 2020;26:379–386.
- Karikari TK, Pascoal TA, Ashton NJ, et al. Blood phosphorylated tau 181 as a biomarker for Alzheimer's disease: a diagnostic performance and prediction modelling study using data from four prospective cohorts. *Lancet Neurol*. 2020;19:422–433.
- Palmqvist S, Janelidze S, Quiroz YT, et al. Discriminative Accuracy of Plasma Phospho-tau217 for Alzheimer Disease vs Other Neurodegenerative Disorders. *JAMA*. 2020.
- Thijssen EH, La Joie R, Wolf A, et al. Diagnostic value of plasma phosphorylated tau181 in Alzheimer's disease and frontotemporal lobar degeneration. *Nature Medicine*. 2020;26:387–397.
- Mielke MM, Frank RD, Dage JL, et al. Comparison of plasma phosphorylated tau species with amyloid and tau positron emission tomography, neurodegeneration, vascular pathology, and cognitive outcomes. *JAMA Neurol*. 2021;78:1108–1117.
- Thijssen EH, La Joie R, Strom A, et al. Plasma phosphorylated tau 217 and phosphorylated tau 181 as biomarkers in Alzheimer's disease and frontotemporal lobar degeneration: a retrospective diagnostic performance study. *Lancet Neurol*. 2021;20:739–752.
- Ashton NJ, Pascoal TA, Karikari TK, et al. Plasma p-tau231: a new biomarker for incipient Alzheimer's disease pathology. *Acta Neuropathol*. 2021;141:709–724.
- Meyer PF, Ashton NJ, Karikari TK, et al. Plasma p-tau231, p-tau181, PET biomarkers, and cognitive change in older adults. *Ann Neurol*. 2022;91:548–560.
- Smirnov DS, Ashton NJ, Blennow K, et al. Plasma biomarkers for Alzheimer's disease in relation to neuropathology and cognitive change. *Acta Neuropathol*. 2022;143:487–503.
- Leuzy A, Mattsson-Carlgren N, Palmqvist S, Janelidze S, Dage JL, Hansson O. Blood-based biomarkers for Alzheimer's disease. *EMBO Mol Med*. 2022;14:e14408.
- Janelidze S, Teunissen CE, Zetterberg H, et al. Head-to-head comparison of 8 plasma amyloid-beta 42/40 assays in Alzheimer disease. *JAMA Neurol*. 2021; 78:1375–1382.
- Groot C, Cicognola C, Bali D, et al. Diagnostic and prognostic performance to detect Alzheimer's disease and clinical progression of a novel assay for plasma p-tau217. *Alzheimers Res Ther*. 2022;14:67.
- Bayoumy S, Verberk IMW, den Dulk B, et al. Clinical and analytical comparison of six Simoa assays for plasma P-tau isoforms P-tau181, P-tau217, and P-tau231. *Alzheimers Res Ther*. 2021;13:198.
- Hansson K, Dahlen R, Hansson O, et al. Use of the tau protein-to-peptide ratio in CSF to improve diagnostic classification of Alzheimer's disease. *Clin Mass Spectrom*. 2019;14:74–82.
- Cicognola C, Janelidze S, Hertze J, et al. Plasma glial fibrillary acidic protein detects Alzheimer pathology and predicts future

- conversion to Alzheimer dementia in patients with mild cognitive impairment. *Alzheimers Res Ther.* 2021;13:68.
23. Hertze J, Minthon L, Zetterberg H, Vanmechelen E, Blennow K, Hansson O. Evaluation of CSF biomarkers as predictors of Alzheimer's disease: a clinical follow-up study of 4.7 years. *J Alzheimers Dis.* 2010;21:1119–1128.
 24. Petersen RC. Mild cognitive impairment as a diagnostic entity. *J Intern Med.* 2004;256:183–194.
 25. McKhann GM, Knopman DS, Chertkow H, et al. The diagnosis of dementia due to Alzheimer's disease: recommendations from the National Institute on Aging-Alzheimer's Association workgroups on diagnostic guidelines for Alzheimer's disease. *Alzheimers Dement.* 2011;7:263–269.
 26. Blennow K, Hampel H, Weiner M, Zetterberg H. Cerebrospinal fluid and plasma biomarkers in Alzheimer disease. *Nat Rev Neurol.* 2010;6:131–44.
 27. Janelidze S, Palmqvist S, Leuzy A, et al. Detecting amyloid positivity in early Alzheimer's disease using combinations of plasma A β 42/A β 40 and P-tau. *Alzheimers Dement.* 2022;18:283–293.
 28. Dore V, Doecke JD, Saad ZS, et al. Plasma p217 + tau versus NAV4694 amyloid and MK6240 tau PET across the Alzheimer's continuum. *Alzheimers Dement (Amst).* 2022;14:e12307.
 29. Triana-Baltzer G, Moughadam S, Slemmon R, et al. Development and validation of a high-sensitivity assay for measuring p217 + tau in plasma. *Alzheimers Dement (Amst).* 2021;13:e12204.
 30. Mielke MM, Hagen CE, Xu J, et al. Plasma phospho-tau181 increases with Alzheimer's disease clinical severity and is associated with tau- and amyloid-positron emission tomography. *Alzheimers Dement.* 2018;14:989–997.
 31. De Meyer S, Vanbrabant J, Schaevebeke JM, et al. Phospho-specific plasma p-tau181 assay detects clinical as well as asymptomatic Alzheimer's disease. *Ann Clin Transl Neurol.* 2022;9:734–746.
 32. Team RC. R: A Language and Environment for Statistical Computing. R Foundation for Statistical Computing, Vienna, Austria. 2014; <http://www.R-project.org/>
 33. Robin X, Turck N, Hainard A, et al. pROC: an open-source package for R and S+ to analyze and compare ROC curves. *BMC Bioinform.* 2011;12:77.
 34. Barthelemy NR, Bateman RJ, Hirtz C, et al. Cerebrospinal fluid phospho-tau T217 outperforms T181 as a biomarker for the differential diagnosis of Alzheimer's disease and PET amyloid-positive patient identification. *Alzheimers Res Ther.* 2020;12:26.
 35. Janelidze S, Stomrud E, Smith R, et al. Cerebrospinal fluid p-tau217 performs better than p-tau181 as a biomarker of Alzheimer's disease. *Nat Commun.* 2020;11:1683.
 36. Palmqvist S, Tideman P, Cullen N, et al. Prediction of future Alzheimer's disease dementia using plasma phospho-tau combined with other accessible measures. *Nat Med.* 2021;27:1034–1042.