



Available online at www.sciencedirect.com

ScienceDirect

journal homepage: www.elsevier.com/locate/gie



ORIGINAL ARTICLE/ARTICOLO ORIGINALE

Evaluation of cyclic fatigue resistance of modern Nickel–Titanium rotary instruments with continuous rotation



Valutazione della resistenza alla fatica ciclica di strumenti rotanti a rotazione continua prodotti con moderne leghe Nickel-Titanio

Massimo Amato^{a,d}, Giuseppe Pantaleo^{b,d}, Dina Abdellatif^{c,d},
Andrea Blasi^{b,d}, Roberto Lo Giudice^{c,d}, Alfredo Iandolo^{b,d,*}

^a Department of Medicine and Surgery, University of Salerno, Salerno, Italy

^b Department of Neurosciences, Reproductive and Odontostomatological Sciences, University of Naples Federico II, Naples, Italy

^c University of Alexandria, Egypt

^d Medical Sciences and Stomatology Department, School of Dentistry, University of Messina, Messina, Italy

Received 4 February 2017; accepted 6 September 2017

Available online 28 September 2017

KEYWORDS

Cyclic fatigue;
Nickel-Titanium;
Continuous rotation;
Rotary instruments.

Abstract

Aim: The aim of present study was to compare cyclic fatigue resistance of three modern Ni–Ti instruments used with continuous rotation.

Materials and methods: For this study 3 groups of rotating instruments with continuous rotation (HyFlex EDM, Twisted File Adaptive, Revo S SU) have been used, each group consisted of 20 files. The various groups were subjected to cyclic fatigue testing through an artificial metal device. A statistical analysis with Kruskal–Wallis test and Mann–Whitney test was performed.

Results: There were statistically significant differences between the three groups. The HyFlex EDM instruments have a fracture resistance slightly higher than the Twisted file and far higher than Revo S SU.

* Corresponding author at: University of Naples Federico II, via S.Pansini 5, 80131 Naples, Italy.

E-mail: iandoloalfredo@libero.it (A. Iandolo).

Peer review under responsibility of Società Italiana di Endodonzia.



Production and hosting by Elsevier

<http://dx.doi.org/10.1016/j.gien.2017.09.002>

1121-4171/© 2017 Società Italiana di Endodonzia. Production and hosting by Elsevier B.V. This is an open access article under the CC BY-NC-ND license (<http://creativecommons.org/licenses/by-nc-nd/4.0/>).

PAROLE CHIAVE

Fatica ciclica;
Nickel-Titanio;
Rotazione continua;
Strumenti rotanti.

Conclusions: Modern Ni–Ti alloys increase resistance of the rotating instruments to cyclic fatigue.

© 2017 Società Italiana di Endodonzia. Production and hosting by Elsevier B.V. This is an open access article under the CC BY-NC-ND license (<http://creativecommons.org/licenses/by-nc-nd/4.0/>).

Riassunto

Obiettivo: Lo scopo di questa ricerca è stato valutare la resistenza alla fatica ciclica di tre differenti Files rotanti prodotti con nuove leghe Ni-Ti con movimento di rotazione continua.

Materiali e Metodi: Per la verifica di questo studio sono stati utilizzati 3 gruppi di strumenti rotanti a rotazione continua (HyFlex EDM, Twisted File Adaptive, Revo S SU), ogni gruppo comprendeva 20 files. I vari gruppi sono stati sottoposti a test di fatica ciclica attraverso un dispositivo metallico artificiale. È stata effettuata una analisi statistica con test di Kruskal-Wallis e test di Mann-Whitney.

Risultati: Sono state rilevate differenze statisticamente significative tra i vari gruppi. Gli strumenti HyFlex EDM hanno mostrato una resistenza alla frattura leggermente superiore ai Twisted file e nettamente superiore ai Revo S Su.

Conclusioni: Le moderne leghe Ni-Ti determinano una maggiore resistenza dello strumento rotante alla fatica ciclica.

© 2017 Società Italiana di Endodonzia. Production and hosting by Elsevier B.V. Cet article est publié en Open Access sous licence CC BY-NC-ND (<http://creativecommons.org/licenses/by-nc-nd/4.0/>)

Introduction

The use of Ni-Ti represented a turning point in the history of Endodontics, in fact it allowed the production of new endodontic instruments both manual and rotating with higher features than stainless steel one, achieving more effective and reproducible results.^{1–3}

Ni–Ti alloys used in dentistry have a fair atomic composition of Ni and Ti, corresponding to 55% of Ni and 45% of Ti.^{4,5}

In the past the only way to improve performance of Ni–Ti instruments was to change their dimensions, tip, cross-sectional and flutes design.^{6,7} With the development of M-wire and Twisted File technology the instruments have been commercialized aiming at improving safety.⁸ The movement kinematics is another important factor.⁹ Ni–Ti instruments have been traditionally used with a continuous motion, but in the last years a reciprocating movement has been introduced.^{10,11}

Some authors demonstrated that the reciprocating motion can extend cyclic fatigue resistance of Ni–Ti instruments when compared to continuous rotation, but these are only preliminary results.^{12,13}

Although the use of Ni–Ti alloy involves a series of advantages, the use of these rotating instruments in Endodontics involves a possible and increased risk of fracture compared to steel files use.^{14–16}

Cyclic fatigue occurs when a metal is subjected to repeated cycles of tension and compression that causes its structure to break down, ultimately leading to fracture.¹⁷ Torsional fatigue is the twisting of a metal about its longitudinal axis at one end, while the other end is in a fixed position.^{18,19}

The resistance to cyclic fatigue of Ni–Ti rotary instruments can be increased via improvements in the manufacturing process or by the use of new alloys with superior mechanical properties.^{20,21} There have been many studies

on the cyclic resistance of different Ni–Ti rotary instruments with different designs or compositions.^{22–24}

Therefore, the aim of this study was to compare cyclic fatigue resistance of new rotating files produced with modified Ni–Ti alloys with rotating files produced with common Ni–Ti alloy.

Materials and methods

Three Ni–Ti rotary instruments – HyFlex EDM (Coltene/Whaledent, Langenau, Germany), Twisted file Adaptive (Kerr, Orange, CA, USA), Revo S SU (Micro-Mega, Besancon Cedex, France) – were selected for the cyclic resistance test. Each group included 20 unused instruments, the size of instruments in Group 1 and 2 was 25/08 and 25/06 for Group 3.

Group 1 was composed by HyFlex EDM Ni–Ti, instruments with complete new properties due to their innovative manufacturing process using electric discharge machining that create unique surface of the new Ni–Ti files and makes the HyFlex EDM files stronger and more fracture resistant.²⁵ Group 2 was composed by Twisted Files Adaptive, these are formed by twisting a triangular blank in combination with heat treatment and special surface conditioning, which conserves the natural grain structure.²⁶ Group 3 was composed by Revo S SU, Ni–Ti instruments with asymmetrical cross-section that provides less stress on the instrument and more flexibility.²⁷

To evaluate the resistance to cyclic fatigue testing of all instruments, a metal device has been created. The device was composed by a support base to which a rigid locking system for the handpiece was connected. At the head of the handpiece cubes with artificial canals have been set. The entrance of the cubes artificial canal was set in axis with the tools inserted in the handpiece head (Fig. 1).



Figure 1 Device created for the cyclic fatigue resistance tests of the rotary instruments.

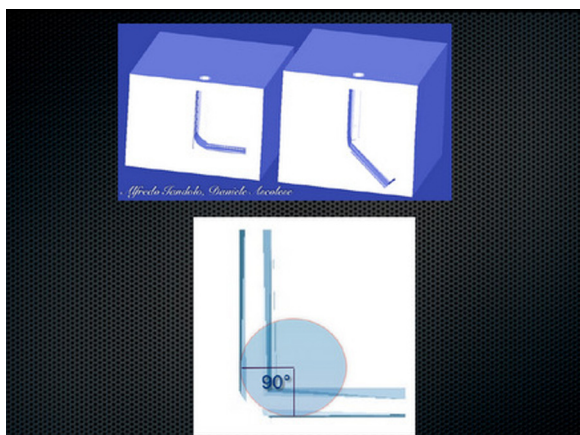


Figure 2 The artificial canal had an angle of 90° and an arch of 5 mm.

The cubes were created through 3D printing (precision 0.1 mm) with a material similar to dentin, to simulate conditions similar to a true root canal during the test. The artificial canal had an angle of 90° and an arch of 5 mm (Fig. 2).

To avoid variables, for each instrument a new artificial canal has been used. Each instrument was rotated within the artificial canal for a length of 13 mm.

The endodontic motor used was the Elements Motor (Sybron Endo) with Sybron Endo 8:1 contra-angle. Continuous rotation at 300 rpm has been used and the maximum torque delivered by the device.

Each instrument was rotated until fracture occurrence, easily detectable because the device allowed the complete visibility of the working part of the instrument during the test. The times from start of the rotation to the point of fracture, were recorded using a digital stopwatch 1/1000 s.

Mean and standard deviation were calculated (Table 1). All data were recorded and subjected to statistical evalua-

Table 1 Mean and standard deviation of tested Ni–Ti instruments expressed in milliseconds.

	Mean ± standard deviation
HyFlex EDM	93385,00 ± 2088,635
Twisted file	80020,00 ± 3095,770
Revo S Su	31935,00 ± 2077,011

tion with Kruskal–Wallis and Mann–Whitney tests. Statistical significance was set at $p < 0.05$.

Results

Kruskal–Wallis test indicated significant differences among the tested instruments with $p = <0.001$. Mann–Whitney significance test was set at $p < 0.05$, it showed that HyFlex EDM had a very similar fracture resistance but slightly above to the Twisted File and higher than Revo S Su.

Discussion

In the literature, there is still a debate regarding the impact of torsional stress and metal fatigue on the fracturing of Ni–Ti rotary instruments.²⁸ A number of studies have stated that fatigue is the predominant mechanism in material failure.^{29,30} Different types of rotary files exhibit differences in resistance to fatigue failure due to differences in various determinants such as their manufacturing process, structural characteristics and geometric designs, surface texture.^{31–33}

It has been clearly shown that multiple factors contribute to file separation, and cyclic fatigue is one of the leading causes. Fatigue failure usually occurs by the formation of micro crack at the surface of the file that starts from surface irregularities.^{34,35} During each loading cycle micro cracks develop, getting deeper in material, until complete separation of the file.³⁶

Gambarini et al.³⁷ also concluded that instruments made of M-wire alloy did not show higher resistance to fatigue when compared to instruments produced by the traditional Ni–Ti. Further research is required regarding the different factors involved in this matter.

All tested instruments fractured at the point of the maximum flexure within the curved part of the artificial canal where the stress concentrates.

Recent literature show that reciprocating motion can extend cyclic fatigue life when compared to continuous rotation.^{12,13,38} However, the term reciprocating motion includes several possible movements and angles, each of which may influence performance and strength of the nickel titanium instruments. All the reciprocating instruments have been commercialized with motors allowing a rotating reciprocation, but angles are not clearly disclosed by manufacturers; however, all studies showed increased lifespan of the instruments, mainly related to the reduction of instrumentation stress by using a reciprocating motion.^{39,40} This reduction of instrumentation stress is the main advantage of reciprocating movements, even if it has been shown that a lot of different reciprocating movements can be used, each one affecting performance and safety of the Ni–Ti instruments.^{41,42}

In this study HyFlex EDM showed the best characteristics in terms of cyclic fatigue resistance than Twisted Files and Revo S Su.

Finally it should be noted that in clinical conditions, rotary files are used in a dynamic mode, endure torsional stresses and cyclic fatigue at the same time and are bind to the root canal walls; therefore, their fatigue resistance may be different from the results of this study. Further research is required.

Conclusions

This study showed how modern Ni–Ti alloys increase resistance of the rotating instruments to cyclic fatigue. HyFlex EDM and Twisted Files showed the best characteristics. However, further studies investigating the different factors which can affect the instruments cyclic fatigue resistance are necessary.

Conflict of interest

The authors have no conflict of interest to declare.

References

- Pettiette MT, Metzger Z, Phillips C, Trope M. Endodontic complications of root canal therapy performed by dental students with stainless-steel K-files and nickel-titanium hand files. *J Endod* 1999;25:230–4.
- Sonntag D, Guntermann A, Kim SK, Stachniss V. Root canal shaping with manual stainless steel files and rotary NiTi files performed by students. *Int Endod J* 2003;36:248–55.
- Cantatore G, Ceci A. L' Endodonzia verso il duemila. Preparazione canalare con strumenti Ni-Ti Evoluzione delle tecniche. *Dent Cadm* 1996;2:21–8.
- Silvani M, Brambilla E, Cerutti A, Amato M, Gagliani M. Root canal treatment quality in undergraduate program: a preliminary report on NiTi reciprocating files. *G Ital Endod* 2013;27:33–7.
- Ferreira F, Adeodato C, Barbosa I, Aboud L, Scelza P, Zaccaro Scelza M. Movement kinematics and cyclic fatigue of NiTi rotary instruments: a systematic review. *Int Endod J* 2017;50:143–52.
- Carratù P, Amato M, Riccitiello F, Rengo S. Evaluation of leakage of bacteria and endotoxins in teeth treated endodontically by two different techniques. *J Endod* 2002;28:272–5.
- Ametrano G, Riccitiello F, Amato M, Formisano A, Muto M, Grassi R, et al. μ CT analysis of mandibular molars before and after instrumentation by Reciproc files. *Recent Prog Med* 2013;104:420–4.
- Varghese NO, Pillai R, Sujathen UN, Sainudeen S, Antony A, Paul S. Resistance to torsional failure and cyclic fatigue resistance of ProTaper Next, WaveOne, and Mtwo files in continuous and reciprocating motion: an in vitro study. *J Conserv Dent* 2016;19:225–30.
- Iandolo A, Iandolo G, Malvano M, Pantaleo G, Simeone M. Modern technologies in endodontics. *G Ital Endod* 2016;30:2–9.
- Suter B, Lussi A, Sequeira P. Probability of removing fractured instruments from root canals. *Int Endod J* 2005;38:114–23.
- Vadhana S, SaravanaKarthikeyan B, Nandini S, Velmurugan N. Cyclic fatigue resistance of RaCe and Mtwo rotary files in continuous rotation and reciprocating motion. *J Endod* 2014;40:995–9.
- Testarelli L, Putorti E, Staffoli S, Valenti Obino F, Di Nardo D, Miccoli G. Cyclic fatigue of NiTi instruments used in complex curvatures with continuous or reciprocating rotation. *G Ital Endod* 2014;28:87–90.
- Aminsobhani M, Meraji N, Sadri E. Comparison of cyclic fatigue resistance of five nickel titanium rotary file systems with different manufacturing techniques. *J Dent (Tehran)* 2015;12:636–46.
- Spagnuolo G, Ametrano G, D'Antò V, Formisano A, Simeone M, Riccitiello F, et al. Microcomputed tomography analysis of mesio-buccal orifices and major apical foramen in first maxillary molars. *Open Dent J* 2012;6:118–1125.
- Pedullà E, Grande NM, Plotino G, Gambarini G, Rapisarda E. Influence of continuous or reciprocating motion on cyclic fatigue resistance of 4 different nickel-titanium rotary instruments. *J Endod* 2013;39:258–61.
- Ahn SY, Kim HC, Kim E. Kinematic effects of nickel–titanium instruments with reciprocating or continuous rotation motion: a systematic review of in vitro studies. *J Endod* 2016;42:1009–17.
- Paduano S, Uomo R, Amato M, Riccitiello F, Simeone M, Valletta R. Cyst-like periapical lesion healing in an orthodontic patient: a case report with five-year follow-up. *G Ital Endod* 2013;27:95–104.
- Di Lorenzo P, Niola M, Pantaleo G, Buccelli C, Amato M. On the comparison of age determination methods based on dental development radiographic studies in a sample of Italian population. *Dent Cadm* 2015;83:38–45.
- Karataş E, Arslan H, Bükler M, Seçkin F, Çapar ID. Effect of movement kinematics on the cyclic fatigue resistance of nickel–titanium instruments. *Int Endod J* 2016;49:361–4.
- Riccitiello F, Stabile P, Amato M, Rengo S, D'Ambrosio C. The treatment of the large periradicular endodontic injury. *Minerva Stomatol* 2011;60:417–26.
- Iandolo A, Pantaleo G, Malvano M, Simeone M, Amato M. Non-surgical management of complex endodontic cases with several periapical lesions: a case series. *G Ital Endod* 2016;30:101–10.
- Kaval ME, Çapar ID, Ertas H. Evaluation of the cyclic fatigue and torsional resistance of novel nickel–titanium rotary files with various alloy properties. *J Endod* 2016;42:1840–3.
- Simeone M, Valletta A, Giudice A, Di Lorenzo P, Iandolo A. The activation of irrigation solutions in endodontics: a perfected technique. *G Ital Endod* 2015;29:65–9.
- Spagnuolo G, Desiderio C, Riviaccio V, Amato M, Rossetti DV, D'Antò V, et al. In vitro cellular detoxification of triethylene glycol dimethacrylate by adduct formation with N-acetylcysteine. *G Dent Mater* 2013;29:e153–60.
- Pirani C, Iacono F, Generali L, Sassatelli P, Nucci C, Lusvarghi L, et al. HyFlex EDM: superficial features, metallurgical analysis and fatigue resistance of innovative electro discharge machined NiTi rotary instruments. *Int Endod J* 2016;49:483–93.
- Gambarini G, Grande NM, Plotino G, Somma F, Garala M, De Luca M, et al. Fatigue resistance of engine-driven rotary nickel–titanium instruments produced by new manufacturing methods. *J Endod* 2008;34:1003–5.
- Basrani B, Roth K, Geoffrey S, Kishen A, Peters OA. Torsional profiles of new and used Revo-S™ rotary instruments: an in vitro study. *J Endod* 2001;37:989–92.
- Kiefner P, Ban M, De-Deus G. Is the reciprocating movement per se able to improve the cyclic fatigue resistance of instruments? *Int Endod J* 2014;47:430–6.
- Di Lorenzo P, Niola M, Buccelli C, Re D, Cortese A, Pantaleo G, et al. Professional responsibility in dentistry: analysis of an interdepartmental case study. *Dent Cadm* 2015;83:324–40.
- Riccitiello F, Maddaloni G, D'Ambrosio C, Amato M, Rengo S, Simeone M. Operating microscope: diffusion and limits. *G Ital Endod* 2012;26:67–72.
- Arslan H, Karataş E, Çapar ID, Ozsu D, Doğanay E. Effect of ProTaper Universal, Endoflare, Revo-S, HyFlex coronal flaring instruments, and Gates Glidden drills on crack formation. *J Endod* 2014;40:1681–3.

32. Amato M, Scaravilli MS, Farella M, Riccitiello F. Bleaching teeth treated endodontically: long-term evaluation of a case series. *J Endod* 2006;**32**:376–8.
33. Iacono F, Pirani C, Generali L, Bolelli G, Sassatelli P, Lusvarghi L, et al. Structural analysis of HyFlex EDM instruments. *Int Endod J* 2017;**50**:303–13.
34. D'Antò V, Valletta R, Amato M, Schweikl H, Simeone M, Paduano S, et al. Effect of nickel chloride on cell proliferation. *Open Dent J* 2012;**6**:177–81.
35. Peng C, Hui WU, Wang L, Xin HU, Deng S, Li C, et al. Cyclic fatigue resistance of two nickel–titanium instruments in different curving angles: a comparative study. *Braz Oral Res* 2015;**29**:1–7.
36. Iandolo A, Ametrano G, Amato M, Rengo S, Simeone M. IG-File: un nuovo strumento per l'ottimizzazione della detersione canale e per la misurazione del diametro apicale. *G Ital Endod* 2011;**25**:72–81.
37. Gambarini G, Grande NM, Plotino G, Somma F, Garala M, De Luca M, et al. Fatigue resistance of engine-driven rotary nickel-titanium instruments produced by new manufacturing methods. *J Endod* 2008;**34**:1003–5.
38. Sekar V, Kumar R, Nandini S, Ballal S, Velmurugan N. Assessment of the role of cross section on fatigue resistance of rotary files when used in reciprocation. *Eur J Dent* 2016;**10**:541–5.
39. Spagnuolo G, Ametrano G, D'Antò V, Rengo C, Simeone M, Riccitiello F, et al. Effect of autoclaving on the surfaces of TiN-coated and conventional nickel–titanium rotary instruments. *Int Endod J* 2012;**45**:1148–55.
40. Scolari G, Lazzarin F, Fornaseri C, Rengo S, Amato M, Cicciù D, et al. A comparison of nimesulide beta cyclodextrin and nimesulide in postoperative dental pain. *Int J Clin Pract* 1999;**53**:345–8.
41. Lo Giudice R, Pantaleo G, Lizio A, Romeo U, Castiello G, Spagnuolo G, et al. Clinical and spectrophotometric evaluation of LED and laser activated teeth bleaching. *Open Dent J* 2016;**10**:242–50.
42. Çapar ID, Ertas H, Arslan H. Comparison of cyclic fatigue resistance of nickel–titanium coronal flaring instruments. *J Endod* 2014;**40**:1182–5.