

Production and measurement of line standards in Eindhoven University of Technology

Citation for published version (APA):

Koning, J., Schellekens, P. H. J., & Veenstra, P. C. (1971). Production and measurement of line standards in Eindhoven University of Technology. *Annals of the ICRP*, 20(1), 85-86.

Document status and date:

Published: 01/01/1971

Document Version:

Publisher's PDF, also known as Version of Record (includes final page, issue and volume numbers)

Please check the document version of this publication:

- A submitted manuscript is the version of the article upon submission and before peer-review. There can be important differences between the submitted version and the official published version of record. People interested in the research are advised to contact the author for the final version of the publication, or visit the DOI to the publisher's website.
- The final author version and the galley proof are versions of the publication after peer review.
- The final published version features the final layout of the paper including the volume, issue and page numbers.

[Link to publication](#)

General rights

Copyright and moral rights for the publications made accessible in the public portal are retained by the authors and/or other copyright owners and it is a condition of accessing publications that users recognise and abide by the legal requirements associated with these rights.

- Users may download and print one copy of any publication from the public portal for the purpose of private study or research.
- You may not further distribute the material or use it for any profit-making activity or commercial gain
- You may freely distribute the URL identifying the publication in the public portal.

If the publication is distributed under the terms of Article 25fa of the Dutch Copyright Act, indicated by the "Taverne" license above, please follow below link for the End User Agreement:

www.tue.nl/taverne

Take down policy

If you believe that this document breaches copyright please contact us at:

openaccess@tue.nl

providing details and we will investigate your claim.

Production and Measurement of Line Standards in Eindhoven University of Technology

J. Koning, P. H. J. Schellekens, University of Technology, Eindhoven, presented by P. C. Veenstra

Aim

The object of the work described here was the production of line standards of reasonable quality, i.e. of 1 m length and errors within 1 μm .

Principle

All dividing machines use some sort of standard which is copied on to the object to be divided; in many machines this standard is a lead screw. Generally, there is some correcting system to eliminate the errors of the standard. In view of the possibilities of the laboratory, combined with a personal dislike of the leadscrew-nut-combination, a line standard was chosen as the standard to be copied. Therefore the most conspicuous part of the dividing machine is a rather long carriage supporting both the standard to be copied and the standard to be divided, arranged in line. A photoelectric microscope is used to observe the lines of the first standard and to control the position of the carriage. Corrections for the errors of the standard are entered into the system in digital form.

Prerequisites

Two essential starting points in building a machine of this kind are (1) a suitable line standard and (2) a measuring instrument of sufficient range and accuracy to determine the corrections to be applied to the standard and to measure the products. The first point will be dealt with later in this paper. For measuring line standards a universal length measuring machine (Carl Zeiss, Jena) of 3 m range was available; in this instrument the well-known Eppenstein compensation system is used to eliminate tilting errors. Thus, the instrument behaves as a longitudinal comparator. The accuracy of the instrument was not quite sufficient when the quality of the standards produced approached our aim and the measurements took too much time. Therefore, at a later stage, a line standard interferometer was built for the purpose; a description of this instrument was presented at the CIRP meeting of September 1970.

Construction Elements Common to Dividing Machines and Comparators

In both instruments a line standard has to be positioned according to the lines engraved. The lines are observed by a simple photo-electric microscope using a vibrating slit. The slit is moved sinusoidally by means of an electro-mechanical exciter, which resembles a small loudspeaker without a cone. The surface of the standard is imaged by the objective lens on to this slit; light passing through this slit is collected on a photo-sensitive transistor. The properties of a microscope of this kind are such that the position of the lines of the standard can be observed on an oscilloscope and that the output voltage can—after suitable amplification—control the position of the standard by means of a servo-system. The net result is that the line is positioned on the axis of the microscope within a second and with an accuracy of better than 0.1 μm . In this context the axis of the microscope is defined as the line joining the centre of the objective lens and the central position of the slit.

As the mechanical construction of both instruments is similar, two identical beds were made with dimensions $4 \times 0.4 \times 0.5 \text{ m}^3$ and with a mass about 1000 kg. Because in this case only one standard has to be accommodated, the range of the interferometer is much greater than that of the dividing machine.

Coarse Control System

In both instruments the displacement of the carriage over long distances is done by means of a lead screw and a special kinematical nut. In the dividing machine the leadscrew is turned by a stepping motor; the motor can be switched off at mm intervals by means of a slotted disc and a photo-diode. In the interferometer a d.c. motor is used which is switched off by means of an auxiliary counter counting an appropriate number of interference fringes. Thus there are no limitations set to the pitch of the standard to be measured.

Correction System

The corrections are punched in a tape using a BCD code. The tape is read by a conventional tape reader, the corrections are processed by a combined relay memory and digital-to-analogue converter. Net result is a direct current proportional to the correction. This current is introduced into the moving coil of the exciter, causing this coil and the slit which is coupled to it to oscillate around a new central position. Therefore the axis of the microscope is shifted an amount proportional to the correction inserted, and the standard is displaced over a corresponding distance by the servo-system.

Secondary Quality Considerations

The quality of a line standard—given an accurate division—is determined to a large extent by the state of the surface and of the lines engraved. At the moment steel standards of a conventional H-profile are used. The surface to be divided is lapped, nickel plated and fine lapped, successively.

A simple, yet adequate, lapping machine was built for the purpose, the tracing is done with a diamond tool. The tracing mechanism uses spring strip pivots throughout. Movement of the tool is governed by two adjustable eccentrics in such a way that the "free" path of the tool is a narrow ellipse. If the tracelet is lowered, the tool rests on the surface during part of the cycle; in that case the force can be adjusted by means of a counterpoise. Normally the force is around 0.9 N (90 gf) resulting in a line width of 3 μm .

The eccentrics mentioned are mounted on a shaft rotated by a small d.c. motor by means of a gear train. By changing the voltage on the motor the time cycle can be adjusted from a few seconds to more than a minute.

Just after the tool is lifted off the surface, a micro-switch is actuated; this causes the coarse control, correction tape, etc. to advance.

Measuring System of the Interferometer

The interferometer was described earlier (loc cit.). Therefore it may be sufficient to mention here that a single mode, frequency stabilised laser is used, that the electronic system registers a pulse for a displacement of $\lambda/8 \cong 0.08 \mu\text{m}$ and that, consequently, displacements of the carriage are punched in tape in units of $\cong 0.08 \mu\text{m}$. Measurements are performed at a rate of between 2 and 3 seconds per line, somewhat dependent on the line quality of the standard.

Recently a quartz thermometer (Hewlett Packard model 2801 A) was added to the instrument to measure the temperature of the standard and of the air path in the interferometer. By means of a separate interface temperatures can be punched into the output tape at time intervals chosen according to the rate of change of the temperature.

The computer programme used to evaluate the measurements causes a new value of $\lambda/8$ to be calculated every time a new value of a temperature is offered.

Generation of Standards

It is not considered acceptable to make copies of commercially available high quality line standards. It is not necessary either, because in principle every standard can be used, provided its errors are within the range of the correcting system. Therefore the procedure adopted was as follows:

1. a brass bar of 250 mm length was divided using a small shaper. The feed of the table could be adjusted to 1 mm, and a crude tracing mechanism was mounted on the ram. The line quality was rather bad.
2. a brass bar of 250 mm length was copied from (1).
3. a steel strip of 550 mm length was divided. It was necessary to displace bar (2) two times over 200 mm, using gauge

blocks. Next a copy of (3) was made and mounted end to end with (3).

4. the combination was used to make a steel standard of 1100 mm length, of H-profile, and divided over a length of 1030 mm. The error curves of these four standards are represented in Fig. 1.

Some more blanks were divided to gain insight into the properties of the machine. The standard denoted (5) in Fig. 1 is the last one made to date (March 10, '71). The accuracy of this standard is $1.5 \mu\text{m}$, that is: the error of the distance of any pair of lines is within that value. This accuracy is still somewhat outside its original aim. There is good reason to assume that it is not an optimal result, and that the machine can produce standards of slightly better quality with only minor re-adjustments.

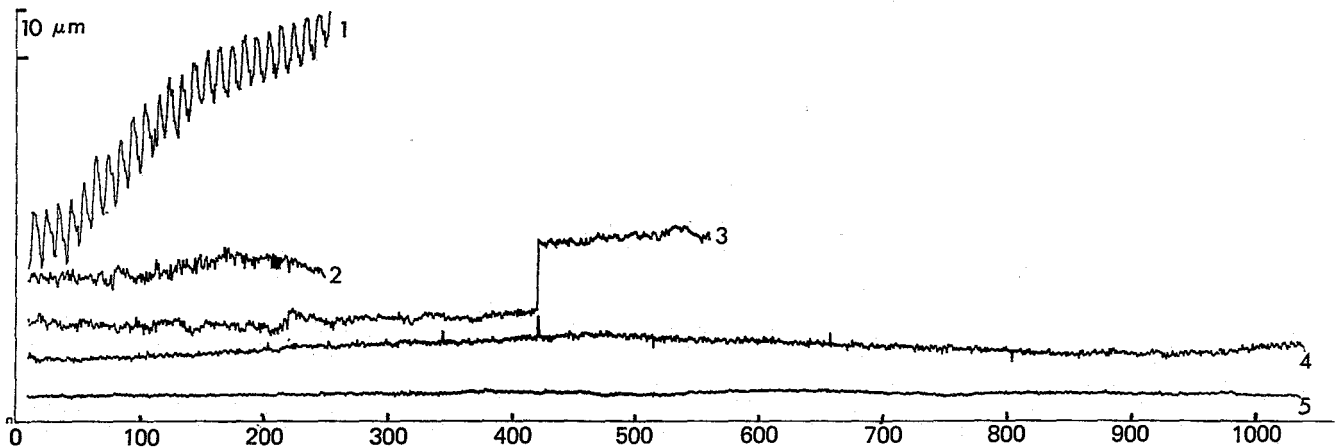


Fig. 1.