

Continuum Emission Spectroscopy on a Plasmaline Microwave Discharge Source

Citation for published version (APA):

Hubner, S., Carbone, E. A. D., Rijke, A. J., & Mullen, van der, J. J. A. M. (2010). Continuum Emission Spectroscopy on a Plasmaline Microwave Discharge Source. In *Proceedings of the XX European Conference on the Atomic and Molecular Physics of Ionized Gases (20th ESCAMPIG, Novi Sad, Serbia, July 13-17, 2010)* (pp. P2.13-)

Document status and date:

Published: 01/01/2010

Document Version:

Publisher's PDF, also known as Version of Record (includes final page, issue and volume numbers)

Please check the document version of this publication:

- A submitted manuscript is the version of the article upon submission and before peer-review. There can be important differences between the submitted version and the official published version of record. People interested in the research are advised to contact the author for the final version of the publication, or visit the DOI to the publisher's website.
- The final author version and the galley proof are versions of the publication after peer review.
- The final published version features the final layout of the paper including the volume, issue and page numbers.

[Link to publication](#)

General rights

Copyright and moral rights for the publications made accessible in the public portal are retained by the authors and/or other copyright owners and it is a condition of accessing publications that users recognise and abide by the legal requirements associated with these rights.

- Users may download and print one copy of any publication from the public portal for the purpose of private study or research.
- You may not further distribute the material or use it for any profit-making activity or commercial gain
- You may freely distribute the URL identifying the publication in the public portal.

If the publication is distributed under the terms of Article 25fa of the Dutch Copyright Act, indicated by the "Taverne" license above, please follow below link for the End User Agreement:

www.tue.nl/taverne

Take down policy

If you believe that this document breaches copyright please contact us at:

openaccess@tue.nl

providing details and we will investigate your claim.

Continuum Emission Spectroscopy on a Plasmaline Microwave Discharge Source

S. Hübner^(1*), E.A.D. Carbone⁽¹⁾, A.J. Rijke⁽¹⁾, J.J.A.M. van der Mullen⁽¹⁾

⁽¹⁾ Department of Applied Physics, Technische Universiteit Eindhoven, P.O. Box 513

5600 MB Eindhoven

^(*) s.huebner@tue.nl

The visible range of radiation is the most often studied one. Essential plasma properties could be obtained by passive diagnostics of optical emission in this spectral region of a discharge. Because of the large errors in the usual determination of plasma properties it is convenient to apply multiple diagnostic methods. This so-called poly diagnostic approach can decrease the uncertainties a lot.

In this study absolute bremsstrahlung continuum measurements were carried out. This straightforward technique was already used in the past⁽¹⁾. From which we learned that accurate calibration is an important issue. In order to do so, one needs an absolute calibrated radiation source. Here a deuterium lamp and a tungsten ribbon lamp were used. As a validation the results of electron density were compared to Thomson Scattering measurements. The latter, active laser diagnostic method, is more reliable than continuum emission, but also more demanding. The complete setup for this diagnostic, including a triple grating spectrograph (TGS) for blocking the intense Rayleigh scattered light, is described elsewhere in detail^(2,3).

The experiment was conducted on a plasmaline discharge setup. That means a discharge sustained by an inner conductor which is surrounded by a quartz tube. On the outside of this containment a vacuum vessel is situated with a low variable pressure of 1 to 20 mbar of argon gas. The input power at a fixed frequency of 2.45 GHz is about 100 to 300 W. A monochromator equipped with an CCD-camera for long-term light exposure was used. It should be mentioned here that line radiation of the plasma close to the wavelength of interest for continuum measurements has, depending on the resolution of the monochromator, a very strong influence on the measured continuum radiation. For that reason an additional set of interference filters was used to narrow the spectral range of the incoming light. Due to the low power densities only a low ionization degree is reached. Therefore here is only the electron-atom bremsstrahlung of importance and the contributions of electron-ion scattering and recombination were calculated to be negligible.

From the theoretical point of view it is also important to evaluate an accurate emission coefficient in the case of the continuum radiation. This is needed to determine an absolute electron density. In other experiments and simulations it was proved that the continuum emission is described quite good in the infrared by the classical calculations, which basically integrates the convolution of the momentum transfer cross section with the electron energy distribution function over the incoming energy of the electrons⁽⁴⁾. A different approach is the scattering of a electron on an atom in the quantum mechanical description. But in fact here assumptions regarding the potential of the atom have to be made.

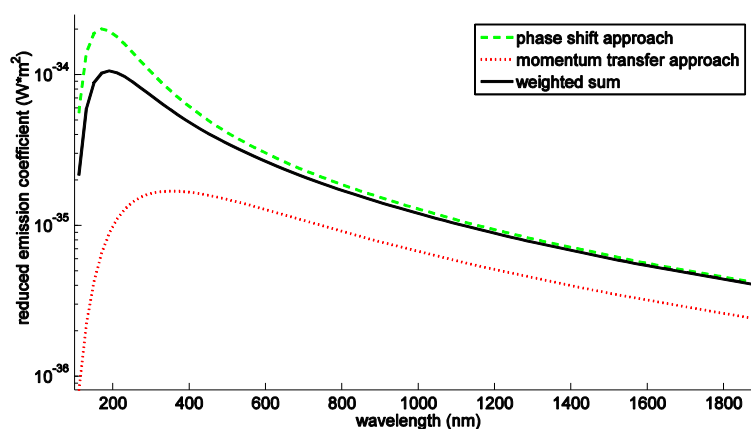


Figure 1: Comparison of reduced emission coefficient $\varepsilon = j/(n_e n_a)$ for $T_e = 1.3$ eV, in argon gas at $T_h = 600$ °K.

Therefore a combination of the phase shift approximation and the classical momentum transfer approach was used. The weighting of the sum of this two contributions is a function of the temperature. In this way this two different approaches lead to a good estimation for the emission coefficient⁽⁵⁾. Generally the phase shift approximation gives somewhat higher emission coefficients but this is even more true for small wavelength of $\lambda < 400$ nm. Whereas the classical momentum transfer approach gives an underestimation of the emission coefficient. Under our plasma conditions of low gas pressure and small ionization degree the weighting is shifted in favor of the phase shift approximation.

The empirical validation of the weighting factor was done by the experiment and the above mentioned laser scattering method.

Reference

- [1] E Iordanova, N Vries, M Guillemier and J J A M van der Mullen, 2007 *J. Phys. D: Applied Physics* **41** 015208
- [2] J.M. Palomares, et al., submitted to *Spectrochim. Acta B* (2010)
- [3] N Vries, J M Palomares, W J van Harskamp, E Iordanova, G M W Kroesen, J J A M van der Mullen, 2008 *J. Phys. D: Applied Physics* **41** 105209
- [4] J. Chapelle et F. Cabanne , 1969 *J. Q. S. R. T.* **9** 889-919
- [5] J E Lawler, 2004 *J. Phys. D: Applied Physics* **37** 1532