

Virtual reality simulation as a training tool for perfusionists in extracorporeal circulation: Establishing face and content validity

Zaheer U. D. Babar, BSc, EKP, ECCP,^a Samuel A. Max, BM, Bch(Oxon),^a Bryan G. Martina, MD,^b Rodney A. Rosalia, PhD, MBA,^a Jette J. Peek, MSc,^a Antony van Dijk, BSc, EKP,^a Amir H. Sadeghi, MD, PhD,^a and Edris A. F. Mahtab, MD, PhD^a


ABSTRACT

Objective: We conducted a prospective study to assess the face and content validity of a new virtual reality (VR) extracorporeal circulation simulator (ECC) developed for perfusionists to facilitate training and practice. We evaluated the opinions of students and staff members about the feasibility of the simulation. The 2 groups consisted of experts (qualified perfusionists) and novices (trainee perfusionists).

Methods: Perfusionists ($n = 12$ experts and $n = 11$ trainees) received instructions on how to use the VR simulator and then proceeded to perform the start of cardiopulmonary bypass in the VR environment. Participants then completed a Usefulness, Satisfaction, and Ease of Use Questionnaire. The questions were rated on a 5-point Likert scale, ranging from 1 (fully disagree) to 5 (fully agree), to assess the face validity and content validity of this simulator.

Results: Participants reported a predominantly positive experience with the VR-ECC simulator, with 96% ($n = 22$) agreeing that the simulator was a useful way of training ECC scenarios. All participants found it easy to interact with the software (100%, $n = 23$), and 82% of students ($n = 9$) believed it helped them remember the steps involved with initiating ECC. Finally, (87% [$n = 20$]) of participants believed the image quality and depth perception were good.

Conclusions: Our next-generation simulator was valid for face and content constructs, and almost all participants found it to be a useful way of training for ECC scenarios. This simulator represents a first step toward truly blended digital learning and a new interactive, flexible, and innovative modality for perfusion training. (JTCVS Techniques 2023; ■:1-14)



Virtual reality extracorporeal circulation simulator image and questionnaire results.

CENTRAL MESSAGE

Participants found the virtual reality extracorporeal circulation simulator to be useful to train on, realistic, easy to use, and contain high-fidelity visual models.

PERSPECTIVE

Our realistic virtual reality extracorporeal circulation simulator affords new training opportunities for perfusionists of all levels. It will increasingly form part of future curricula to enable perfusionists to better prepare for the challenges of their profession. Our simulation will enable unlimited practice to master complex perfusion operations or prepare for unexpected disaster scenarios.

See Commentary on page XXX.

From the ^aDepartment of Cardiothoracic Surgery, University Medical Center, Erasmus MC, Rotterdam, The Netherlands; and the ^bDepartment of Cardiothoracic Surgery, Medisch Spectrum Twente, Enschede, The Netherlands.

This research and software development is funded by an Erasmus+ grant (No. 2022-1-NL01-KA220-HED-000087770).

Institutional Review Board Statement: The Institutional Review Board (IRB) of the Erasmus MC University Medical Center approved the study protocol and publication of data with reference MEC-2023-0210. The participants provided informed written consent for the publication of the study data.

Mr Babar and Dr Max contributed equally to this article.

Received for publication Feb 8, 2023; revisions received May 11, 2023; accepted for publication May 30, 2023.

Address for reprints: Edris A. F. Mahtab, MD, PhD, Department of Cardiothoracic Surgery, University Medical Center, Erasmus MC, Dr Molewaterplein 40, 3015GD Rotterdam, The Netherlands (E-mail: e.mahtab@erasmusmc.nl).

2666-2507

Copyright © 2023 The Author(s). Published by Elsevier Inc. on behalf of The American Association for Thoracic Surgery. This is an open access article under the CC BY license (<http://creativecommons.org/licenses/by/4.0/>).

<https://doi.org/10.1016/j.xjtc.2023.06.004>

Abbreviations and Acronyms

ECC = extracorporeal circulation
 HLM = heart-lung machine
 VR = virtual reality

▶ Video clip is available online.

For trainee perfusionists, knowledge of physiology and the interaction between a patient's hemodynamic state and the heart-lung machine (HLM) is essential to prepare them for their clinical practice. A substantial part of a perfusionist's training process is dedicated to transferring this theoretical knowledge into practical skills. Providing this training presents logistical and financial challenges, not least during times of social distancing, travel restrictions, and health care budget constraints. The high cost of equipment and supplies puts considerable pressure on the training program budget, making it challenging to allocate enough resources for repetitive practice of complex procedures or emergency scenarios.

Virtual Reality (VR) simulation training may help to ameliorate these issues, and simultaneously provide equitable access to training across the globe. VR can provide fully immersive, interactive, and realistic scenarios in which the user can repeatedly train and acquire skills without the need to travel long distances or being present physically at a specific location. Other advantages of VR training for health care professionals include its convenience, flexibility, and cost-effectiveness.¹ The efficacy of the VR modality in training (surgical) skills has previously been demonstrated.²⁻⁴


The application of a VR simulator in the education of perfusionists appears to be promising but remains to be fully investigated.⁵ The initial experience with augmented reality training of perfusion students demonstrated the significant value of this modality, although as of yet does not include a full HLM simulation.¹ To the best of our knowledge, a fully virtual simulation has not yet been implemented in clinical perfusion training. VR can recreate fully immersive 360° interactive and realistic scenarios, enabling users to hone their skills without the need for expensive physical simulation equipment. Users can make mistakes without fear of consequences. Moreover, VR can be used in a multiuser setting, allowing different users to be present in the same scenario while physically distanced.⁵ Multiple studies have shown that simulation training effectively improves knowledge, confidence, motivation, and satisfaction with training versus standard

training methods.⁶⁻⁹ Creating an accurate virtual environment is essential to successfully transfer knowledge and skills, especially as an alternative conventional training method.¹⁰

To that end, we developed the VR extracorporeal circulation simulator (VR-ECC sim). In this simulator, we have recreated the process of preparing and building an HLM, the procedure for initiating cardiopulmonary bypass, the management of the patient while on bypass, and the procedure for weaning from bypass.

Once built, such a VR training tool requires validation to demonstrate its educational utility.^{11,12} This validation comprises different subtypes, including face validity and content validity.¹³ Face validity considers how realistic the simulator is, and how closely it resembles the look and feel of a physical HLM. This is judged by experts (qualified perfusionists) and nonexperts alike (novices/trainees).¹¹ Content validity refers to the degree to which the content of a simulator precisely portrays the intended medical construct, in terms of knowledge or skills that it aims to impart through education.¹³ It is therefore assessed by examining the ratings that experts give in the usefulness and satisfaction sections of the questionnaire.

We performed a prospective study to assess the feasibility and to establish the face and content validity of the VR-ECC sim in a group of novice and expert perfusionists.



VIDEO 1. A video captured from the virtual reality-extracorporeal circulation (VR-ECC) simulator showing a beta version of the simulator, where participants prepare the heart-lung machine and go on bypass. Video available at: [https://www.jtcvs.org/article/S2666-2507\(23\)00198-0/fulltext](https://www.jtcvs.org/article/S2666-2507(23)00198-0/fulltext).

METHODS

Study Design

Software development. We developed a vendor-agnostic VR simulation that recreates the perioperative steps, preparation, initiation, and termination of cardiopulmonary bypass using an HLM. Unreal Engine 4 (Epic Games) software was used for the simulation development, with visual modeling being performed in Autodesk Maya (Autodesk Inc).

The VR-ECC sim was designed by a multidisciplinary team consisting of perfusionists, VR software developers, digital transformation experts, and cardiothoracic surgeons from the cardiothoracic surgery departments at Erasmus Medical Centre, Distant Point LTD, and Medisch Spectrum Twente. Still images captured from the simulator can be found in [Figures 1 and 2](#), and [Video 1](#) shows the simulator.

The software used for this study was an alpha version of the simulator. One limitation of this early version was that users were not able to make mistakes. This feature will be included in future iterations of the simulator.

Hardware. A Meta Quest 2 (Meta Platforms Inc) head-mounted display, in combination with 2 VR controllers was used to run the VR-ECC sim in a standalone setup, without requiring the use of external computer hardware.

Interventions. Participants were recruited through the Dutch national perfusion educational institute and through clinical perfusion departments in the Netherlands. The Institutional Review Board of the Erasmus MC University Medical Center approved the study protocol and publication of data with reference MEC-2023 to 0210 (April 28, 2023). As seen in [Figure 3](#), a total of 11 novices (58% of the current national cohort of trainee perfusionists) and 12 experts were included and provided informed consent. A copy of the informed consent form can be found in [Appendix E1](#). Before running the simulation, each participant was given a short briefing on the scenario, how to use the VR head-mounted display, and how to interact with the controls and software to perform the VR ECC sim. Participants then entered the simulation and were placed into the virtual operating theatre environment. They completed the “initiating cardiopulmonary bypass” scenario, which is interactive and contained a list of steps to be performed.

Data collection. Data was gathered through means of questionnaires given to participants that were completed after they completed the simulation. The validated Usefulness, Satisfaction, and Ease of Use Questionnaire format was employed to assess face validity and content validity specifically.¹⁴ This questionnaire employs four different themes to evaluate the reliability of new technologies and innovations on the subjects of Usefulness, Satisfaction, Ease of use, and Immersion. These questions were rated on a five-point Likert scale, ranging from 1 (fully disagree) to 5 (fully agree). In addition to the Usefulness, Satisfaction, and Ease of Use Questionnaire, demographic information and experience with ECC and digital learning platforms were gathered through a supplementary questionnaire.

The end of the questionnaire contained three free text questions, where participants were asked to list the advantages and disadvantages of using VR-ECC sim as a training tool and to leave any comments they had about the experience of using the simulator. The questionnaire can be found in [Appendix E2](#), and the raw data from the completed questionnaires can be found in the [Online Data Supplement](#).

To examine face validity, we used questionnaire results from all participants on the ease of use and immersiveness. When assessing content validity, the results from the expert group were considered, specifically regarding usefulness and satisfaction.

Statistical Analysis

Statistical analysis was performed using IBM SPSS Statistics for Windows, version 28.0 (IBM Corp). The χ^2 test was used to perform statistical analyses of categorical data such as the participant characteristics. Continuous data are presented as mean \pm SD, and categorical data, including Likert scales, are presented as percentages.

RESULTS

Demographic Data

All participants ($n = 23$) who were enrolled in the study completed a questionnaire after completing the VR scenario. The baseline characteristics did not differ significantly between the two groups, with the exception of the group's exposure to digital learning or serious games, where the expert group had significantly more experience than the novice group. The breakdown of baseline characteristics and experience with virtual reality-related technologies can be found in [Table 1](#).

Novices

[Figure 4](#) shows the data collected from novice perfusionists after they completed the VR-ECC sim. Concerning the face validity, this group believed that the simulator was realistic, including 10 (91%) participants agreeing that the depth perception and image quality was good, 7 participants (63%) stating that they were not distracted from the simulation, and a further 7 participants (63%) believed they were actively involved in the ECC scenario. Most novice participants were interested in the progress of the simulation ($n = 7$ [63%]). Concerning content validity, novice participants

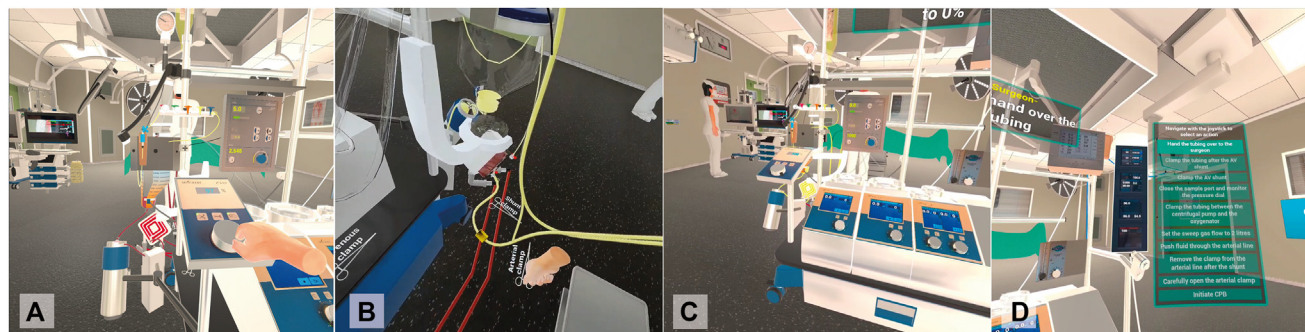


FIGURE 1. Screen captures from the virtual reality-extracorporeal circulation (VR-ECC) simulator, featuring from left-to-right: adjustment of the venous occluder (A), removal of a clamp from the arterial line (B), an overview of the heart-lung machine (C), and the menu system by which users navigate through the simulation (D).




FIGURE 2. The central picture of this manuscript, displaying selected metrics from the use questionnaires, completed by experts and novices, and a screen capture from the virtual reality-extracorporeal circulation (VR-ECC) simulator.


believed the simulator was useful: the whole group ($n = 11$ [100%]) agreed that the VR-ECC sim was a useful training tool for perfusionists, 9 participants (82%) reported that the simulation helped them to remember the steps in performing an ECC, and 6 participants (60%) said that they learned a lot from performing the simulation. With respect to satisfaction, all novice participants ($n = 11$ [100%]) liked taking part in the VR-ECC sim and enjoyed using VR for learning purposes. Ten participants (91%) suggested that they would find the VR simulation useful in addition to conventional classroom training and 7 participants (63%) agreed that they would prefer VR simulation instead of conventional classroom training. Almost all novice participants ($n = 10$ [91%]) would recommend the VR-ECC sim to colleagues for training purposes. Regarding ease of use, all novice participants found it easy to interact with software ($n = 11$ [100%]), and 8 participants (73%) found it easy to move around the virtual environment. Most of the novice participants ($n = 9$ [90%]) agreed that their head and hand movements were sufficiently mirrored by the simulation. Finally, only 1 participant (10%) agreed that communication felt natural, which represents an area that should be addressed in future iterations of the simulator.

Experts

Figure 5 shows the data collected from expert perfusionists after they completed the simulation. The results obtained from the experts broadly mirrored those of the less experienced group. In terms of face validity, experts believed that the simulator was realistic, including 10 (83%) participants agreeing that the depth perception and image quality was

good, 75% ($n = 9$) were not distracted from the simulation, and 66% ($n = 8$) believed they were actively involved in the patient scenario. The majority of expert participants were interested in the progress of the simulation ($n = 9$ [75%]). When considering content validity, the expert participants agreed with novice participants and believed the simulator was useful; almost the whole group ($n = 10$ [91%]) agreed that the VR-ECC sim was a useful training tool for perfusionists. Experts learned relatively little from the simulation, which is not unsurprising given their level of experience. Three participants (30%) reported that the simulation helped them to remember the steps in performing an ECC, and 2 participants (20%) said that they learned a lot from performing the simulation. Experts were satisfied with the VR-ECC sim, and all participants ($n = 12$ [100%]) liked taking part in the VR-ECC sim, and enjoyed using VR for learning purposes. Eleven participants (92%) suggested that they would find the VR simulation useful in addition to conventional Microsoft PowerPoint training and 5 participants (42%) agreed that they would prefer VR simulation instead of conventional PowerPoint training. Almost all expert participants ($n = 11$ [91%]) would recommend the VR-ECC sim to colleagues for training purposes. Regarding ease of use, all expert participants found it easy to interact with software ($n = 11$ [100%]), and 75% ($n = 9$) found it easy to move around the virtual environment. All experts ($n = 12$ [100%]) agreed that their head and hand movements were mirrored by the simulation. Only 25% ($n = 3$) agreed that communication felt natural.

All participants were asked to complete a free text section of the questionnaire addressing the advantages and

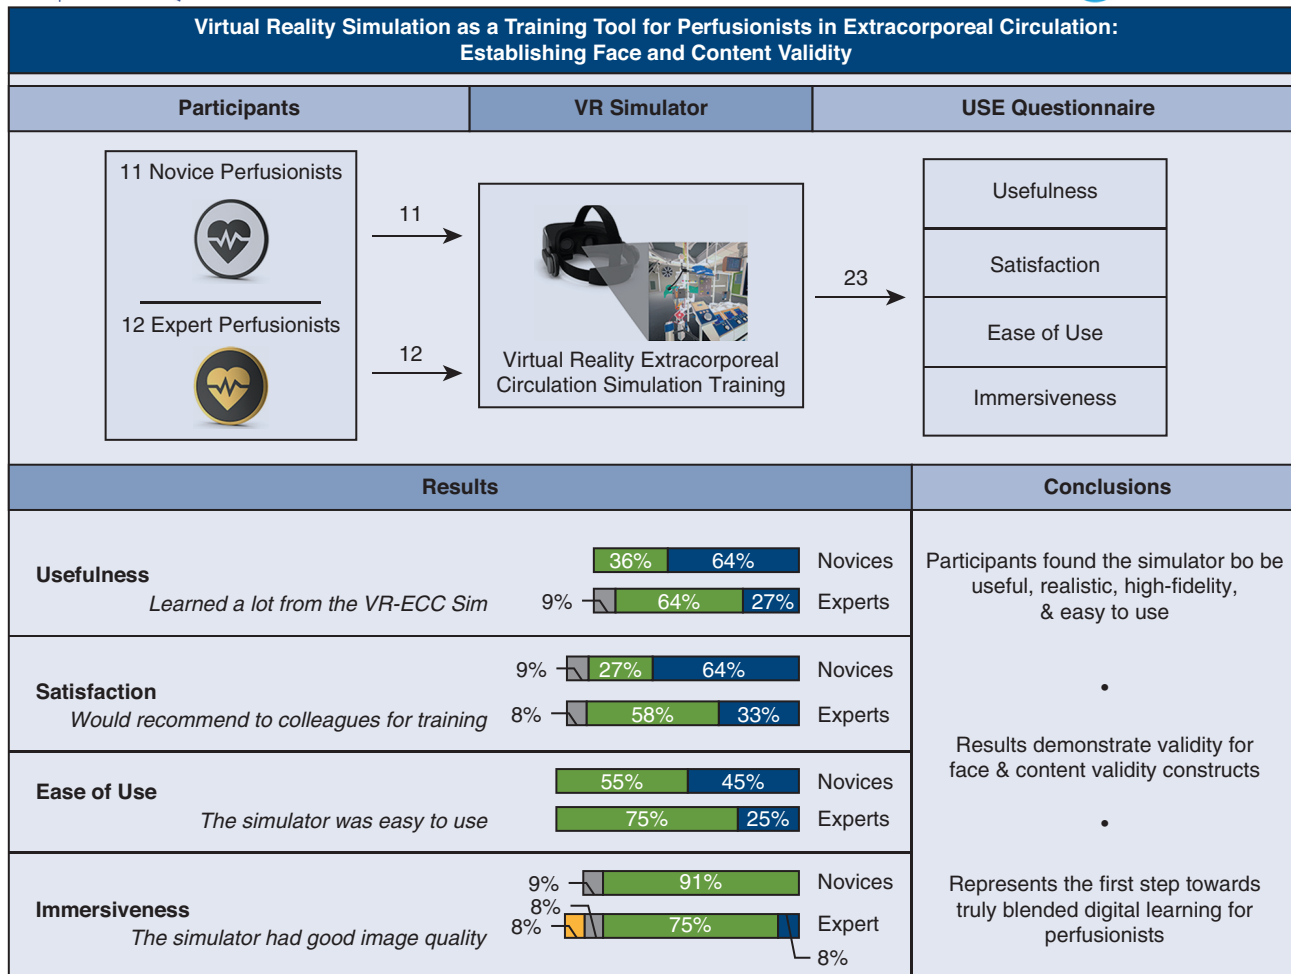

■ Strongly Disagree
 ■ Disagree
 ■ Neutral
 ■ Agree
 ■ Strongly Agree

FIGURE 3. Graphical abstract showing a summary of the study design, as well as a sample of the results from each section of the Usefulness, Satisfaction, and Ease of Use Questionnaire. VR, Virtual reality; VR-ECC, virtual reality-extracorporeal circulation.

disadvantages of the VR-ECC sim. Full results of this and the Usefulness, Satisfaction, Ease of Use Questionnaire data can be found in the [Online Data Supplement](#). Common themes among the reported advantages included high image quality, a realistic simulation, the ability to practice procedure steps, establish a good routine, gain experience, practice with different systems, the ability to make mistakes without consequences, and to be able to troubleshoot difficult situations. Disadvantages included a (current) inflexibility in the order of steps, an unfamiliar HLM type in the simulation, and the slow progression of the simulation.

DISCUSSION

We present the results of this prospective feasibility study, which aimed to demonstrate the face and content

validity of our prototype VR-ECC sim. The participants broadly agreed with all of the statements presented in the various categories of the USE Questionnaire (Usefulness, Satisfaction, Ease of Use, and Immersiveness). Therefore, this constitutes face validity, demonstrating that our simulator is realistic and that the simulated HLM looks and feels like a physical HLM.

Experts and novices alike felt immersed in the virtual environment, with only communication standing out as an area that should be improved in future iterations of the simulator. They also believed that the depth perception was good and were not distracted when performing the simulation. Almost all participants unanimously agreed that our VR-ECC simulation is a useful way to train for ECC scenarios and were very satisfied with the simulation

TABLE 1. Baseline characteristics table showing the baseline characteristics of the participants in both groups, and statistical comparisons and their significance for each question

| Baseline Characteristic | Novice perfusionists (n = 11) | | Expert perfusionists (n = 12) | | P value | Statistical test |
|---|-------------------------------|------|-------------------------------|-------|---------|------------------|
| Sex | | | | | 0.37 | χ^2 |
| Female | 6 | 54.5 | 5 | 41.7 | | |
| Male | 4 | 36.3 | 3 | 25.0 | | |
| N/A | 1 | 9.0 | 4 | 33.3 | | |
| Age | 29.5 ± 6.46 | | 36.8 ± 11.5 | | .11 | t test |
| Period as a trainee/expert (y) | 1.35 ± 1.09 | | 11.2 ± 13.0 | | .21 | χ^2 |
| How many ECC operations have you participated in? | | | | | 0.22 | Fisher exact |
| 1-5 times | 2 | 18.2 | 0 | 0 | | |
| More than 10 times | 9 | 81.8 | 12 | 100.0 | | |
| Do you have experience with gaming consoles (eg, computer gaming, Xbox, PlayStation)? | | | | | 0.10 | χ^2 |
| I have never used a gaming console | 0 | 0 | 4 | 33.3 | | |
| I have used a gaming console a few times before | 8 | 72.7 | 5 | 41.7 | | |
| I am gaming on a regular basis (at least once a month) | 3 | 27.3 | 3 | 25.0 | | |
| How often do you use VR hardware/software (eg, VR gaming, simulations, consoles, entertainment etc.)? | | | | | 0.16 | Fisher exact |
| I have never had a VR experience until today | 7 | 63.6 | 11 | 91.7 | | |
| I have used VR a few times before | 4 | 36.4 | 1 | 8.3 | | |
| Do you have experience with physical simulation trainings in skills labs? | | | | | 0.67 | Fisher exact |
| I have never had simulation training before | 4 | 36.4 | 3 | 25.0 | | |
| I have had simulation trainings multiple times before | 7 | 63.6 | 9 | 75.0 | | |
| Do you have experience with digital training (eg, e-learning or serious games)? | | | | | 0.02* | χ^2 |
| I have never had such training before | 7 | 63.6 | 2 | 16.7 | | |
| I have had a digital training a few times before | 1 | 9.1 | 8 | 66.7 | | |
| I have had digital trainings multiple times before | 3 | 27.3 | 2 | 16.7 | | |
| Do you have experience with a simulation training in VR? | | | | | | N/A |
| Yes | 0 | 0.0 | 0 | 0 | | |
| No | 11 | 100 | 12 | 100 | | |

Values are presented as n (%) or mean ± SD. N/A, Not available; ECC, extracorporeal circulation; VR, virtual reality. *Result is statistically significant where $P < .05$.

experience. Experts and students alike found the simulator easy to use, with prior gaming/digital learning experience appearing not to be a factor in this regard. The study was conducted with an alpha version of the simulator. Future iterations of our simulator will contain more in-depth simulations allowing for mistakes with physiological consequences and troubleshooting scenarios with equipment failures and patients with challenging requirements. These scenarios will additionally be useful for surgeons to practice, especially for emergency situations requiring intense cooperation and communication between surgeons and perfusionists. We envision a multiuser simulator whereby a surgeon, scrub nurse, and perfusionist can practice in the same virtual operating theatre, creating a cohesive team before performing real cardiothoracic procedures.

When assessing content validity, we specifically considered the results from the expert group regarding the usefulness and satisfaction. The principal finding in this regard was whether or not experts believed that our simulator would be a useful way to train perfusionists, which they almost unanimously agreed that it was. Experts reported that they did not learn much from the simulation.

This outcome is not surprising, considering the high level of expertise of the expert group and the current aim of our simulator, which is to assist trainees in becoming familiar with the HLM and the operational environment of the operating theatre. In terms of satisfaction, experts rated the simulator highly, with a strong majority agreeing with every statement, with the exception of replacing conventional classroom/PowerPoint training with VR training, where



FIGURE 4. Stacked bar charts of the Usefulness, Satisfaction, Ease of Use Questionnaire data completed by novice perfusionists. *VR-ECC*, Virtual reality-extracorporeal circulation; *HMD*, head mounted displays.

42% agreed. This may be in part due to the early stage of the simulator, and the current lack of theoretical knowledge imparted during such a training scenario. This is a feature that will be implemented in the future, such that a blended experience of simulation and theoretical learning can be produced, whilst leveraging the gold standard spaced repetition learning strategy.¹⁵

We envision that this training tool will form a part of blended learning curriculum in combination with traditional classroom learning, and hands-on clinical practice. Additionally, it will contribute to more radical educational transformation, including standardization, decentralization, and flexible learning strategies that can be performed at the

convenience of the user. In this way, it can be used to increase and maintain competency. Evaluating user performance in the simulator will be key in this regard, such that users and supervisors alike can track progress and demonstrate competency in a proficiency-based curriculum.¹⁶

Creating such a curriculum will require a simulator that is flexible and can adapt to local practice in terms of equipment and standard operating procedure. Modeling different systems will require a visual component that is currently being produced, but also a physical model. Our aim is through use of real-life perfusion data, to build virtual models from a variety of equipment and clinical scenarios such that the simulator looks and responds like it would in a given

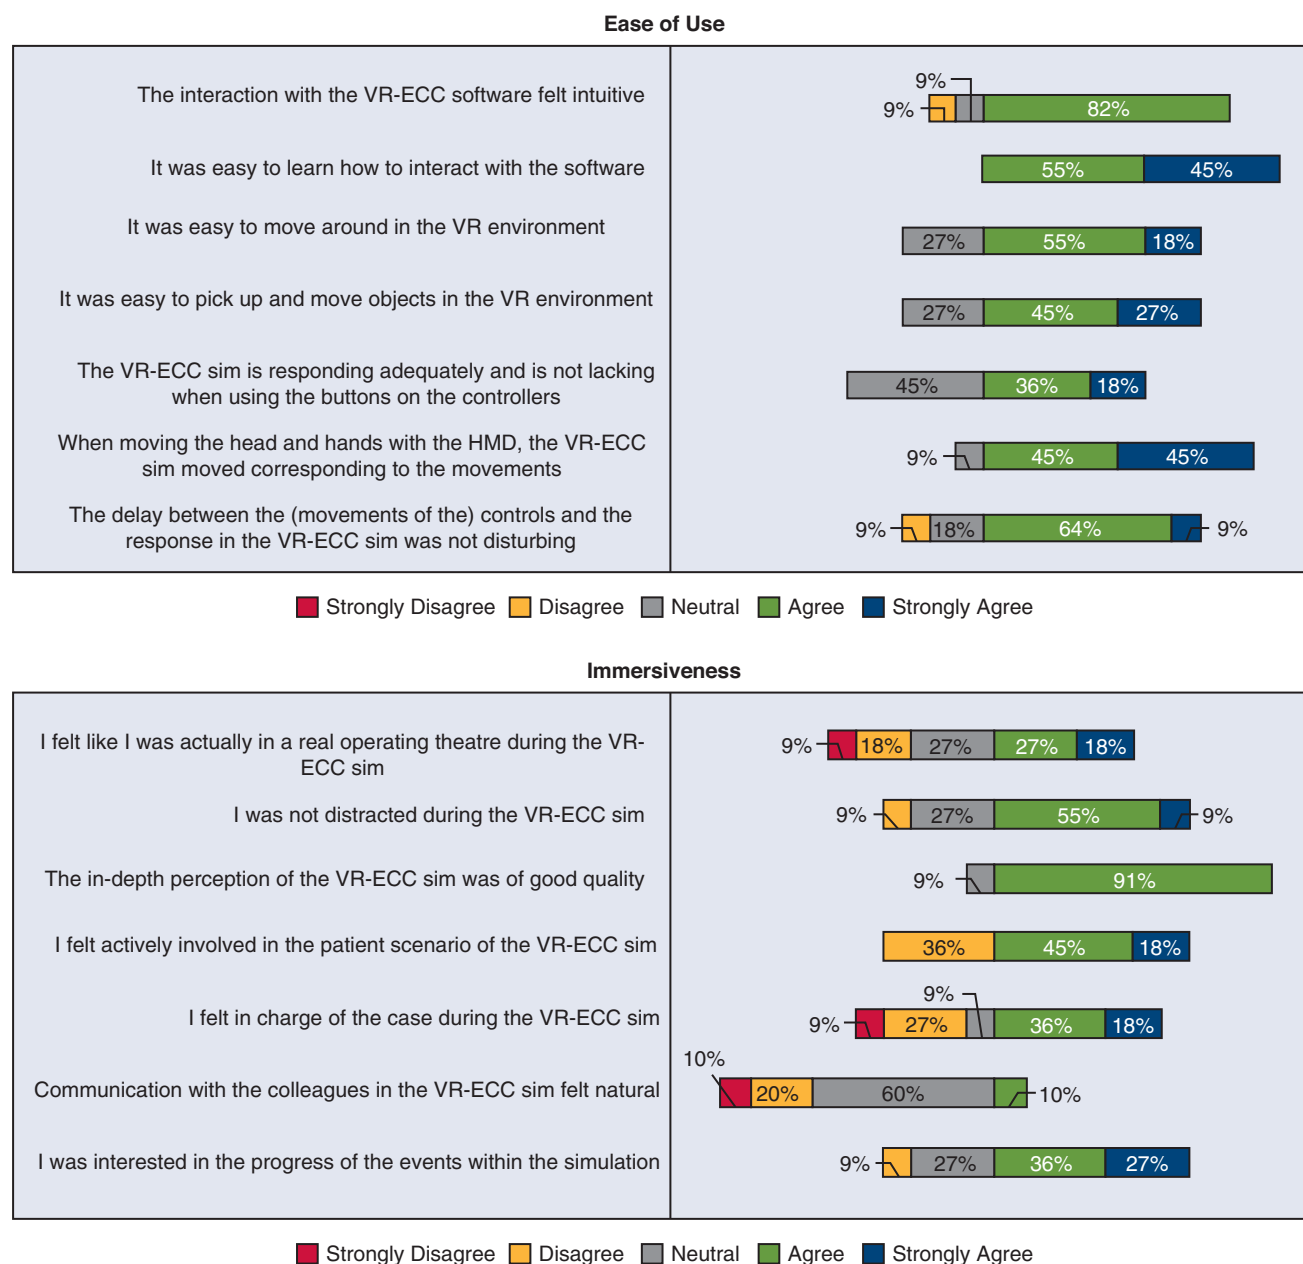


FIGURE 4. Continued.

clinical situation. With a realistic mechano-physiological HLM model, perfusionists can transition to new equipment and practice in a sandbox environment.

The multiplayer, multirole design of this simulator streamlines the learning of new center-specific protocols and the utilization of unfamiliar equipment, particularly in troubleshooting scenarios. It enables interaction between mentors and students within a simulated setting, allowing students to execute crucial tasks in a secure environment under expert supervision. Our VR simulation also helps strike

a balance between theoretical knowledge and hands-on practical experience to ensure students are well prepared for real-life clinical situations.

The field of clinical perfusion is constantly evolving, with increasing complexity of clinical cases and ongoing advancements in technology. Although previous this study and previous studies have demonstrated the value of simulation in training perfusionists, the decision regarding which modality to choose—physical, augmented reality, or VR—is less clear. Equipment cost is likely to be a



FIGURE 5. Stacked bar chart of the Usefulness, Satisfaction, Ease of Use Questionnaire data completed by expert perfusionists. *VR-ECC*, Virtual reality-extracorporeal circulation.

significant factor in this decision-making process. Current physical simulators, including the Califia Patient Simulator (Biomed Simulations) and ECCSIM (Senko Medical Instrument Mfg Co Ltd) cost in excess of 5 figures, with the latter cited as costing \$40,000.¹ Augmented reality is an order of magnitude less expensive, costing around \$2100, but as of yet is not a complete simulation of an HLM.¹


The start-up costs for the VR-ECC sim are estimated at \$400 associated with the purchase of the VR headset. Our software will be provided as a software as a service, with setup, user licenses, and customer support covered via monthly subscriptions. Therefore, VR-ECC sim represents the most cost-effective option to our knowledge to provide

spaced repetition learning of basic skills, as well as simulation training of novel techniques, enabling trainees to stay up to date with innovation in the field.

Software development costs often remain prohibitively high across the various platforms currently available, which represents an issue that should be addressed in future to ensure access to the benefits of next generation simulators is equitable. To that end, our subscription model and geographical pricing strategy greatly lowers entry barriers and accessibility to both individuals and organizations.

With this feasibility study, we demonstrate the VR-ECC sim fulfills the criteria for face and content validity. To validate the simulator, we will compare its educational

Ease of Use

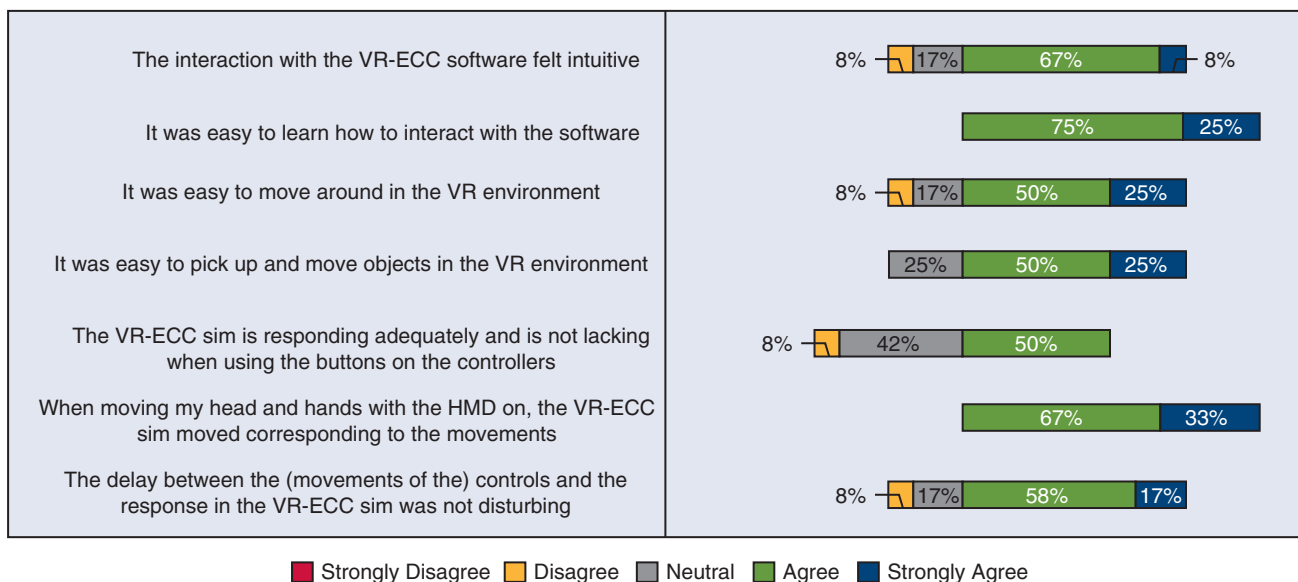

Immersiveness

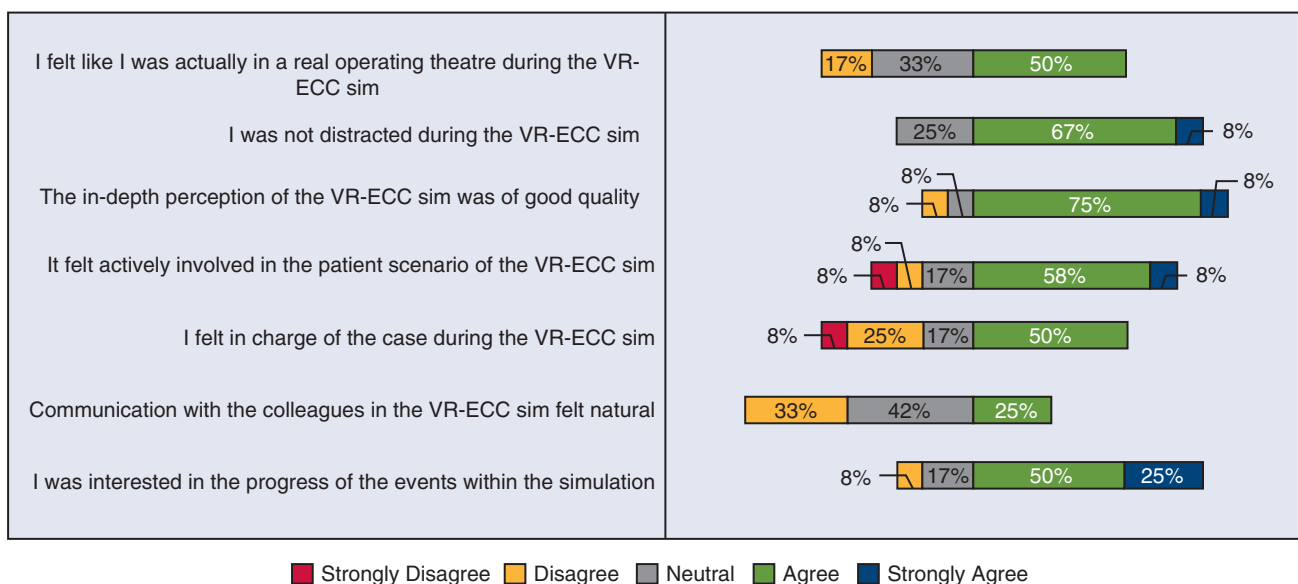


FIGURE 5. Continued.

performance to traditional training methods in terms of preparing perfusionists for disaster scenarios. This comparison will occur through a physical moulage scenario, and the outcomes measured will include time, accuracy, and safety, which will evaluate the simulator’s construct validity. Once an intermediate difficulty version of the simulator is available, we will be able to assess participants’ performance in the simulator with the aforementioned metrics. This will be rated by experts through a video made of the participant’s test scenario in VR and thresholds for expert competency for each of these targets will be determined in

advance. Finally, predictive validity, or the ability of the simulator to discriminate between novices and experts should be compared against the gold standard assessment’s predictive ability. There is little consensus as to what is the gold standard of practical ECC assessment, making it difficult at this moment to produce such evidence.

Limitations

Our limitations include a small group of participants because this was a feasibility study. We did not perform comparative statistics for the outcomes measured because

there would not be sufficient data to do so, nor would this produce meaningful data. The simulator was still in the alpha stage of development and thus the versions tested by participants varied slightly with minor bug fixes implemented over the course of this study. Limitations of the simulator as reported by users included an inflexibility in the order of steps, an unfamiliar HLM type in the simulation, and slow progression through the simulation. These issues have largely been ameliorated in the new beta version of the simulator.

CONCLUSIONS

To the best of our knowledge, this is the first VR simulator that recreates the setup and operation of an HLM for cardiopulmonary bypass. The results demonstrate that this simulator is valid in terms of face and content validity. Participants reported finding it useful, realistic, enjoyable, and easy to use. Future research should include a randomized controlled trial whereby the VR-ECC sim is compared with the gold standard classroom equivalent before performing a physical skills assessment where the time to completion and number of mistakes are assessed by an independent expert. With further development and testing, this high-fidelity simulator has the potential to become an essential part of the next generation of educational tools for perfusionists around the world.

Conflict of Interest Statement

Drs Mahtab, Sadeghi, Babar, Max, Martina, Rosalia, and van Dijk and Ms Peek are co-developers of the VR-ECC sim.

The *Journal* policy requires editors and reviewers to disclose conflicts of interest and to decline handling or reviewing manuscripts for which they have a conflict of interest. The editors and reviewers of this article have no conflicts of interest.

The authors thank Aleksandar Trifunovski, Ivo Matevski, Tomi Jurukovski, Simona Manoleva, and Kristina Kerkez for their work in developing the VR-ECC sim. The VR-ECC sim team also thank Wouter de Wilde and Denise Hoogzaad for their work in translating and providing voiceover media, and to all participants for their time and efforts for this study.

References

1. Yamada Y, Nakamura T, Yamada M, Maruyama J, Maruyama K, Azuma E. Use of augmented reality to assist teaching for future perfusionists in extracorporeal technology. *J Extra Corpor Technol.* 2019;51:244-7.
2. Mao RQ, Lan L, Kay J, Lohre R, Ayeni OR, Goel DP, et al. Immersive virtual reality for surgical training: a systematic review. *J Surg Res.* 2021;268:40-58. <https://doi.org/10.1016/j.jss.2021.06.045>
3. Schmidt MW, Köppinger KF, Fan C, Kowalewski K-F, Schmidt LP, Vey J, et al. Virtual reality simulation in robot-assisted surgery: meta-analysis of skill transfer and predictability of skill. *BJS Open.* 2021;5:zraa066. <https://doi.org/10.1093/bjsopen/zraa066>
4. Palter VN, Grantcharov TP. Virtual reality in surgical skills training. *Surg Clin North Am.* 2010;90:605-17. <https://doi.org/10.1016/j.suc.2010.02.005>
5. Wolff G, Bruno RR, Reiter M, Kantzow B, Kelm M, Jung C. Virtual reality device training for extracorporeal membrane oxygenation. *Crit Care.* 2020;24:390. <https://doi.org/10.1186/s13054-020-03095-y>
6. Graafland M, Schraagen JM, Schijven MP. Systematic review of serious games for medical education and surgical skills training. *Br J Surg.* 2012;99:1322-30. <https://doi.org/10.1002/bjs.8819>
7. Nichols S, Haldane C, Wilson JR. Measurement of presence and its consequences in virtual environments. *Int J Hum Comput Stud.* 2000;52:471-91. <https://doi.org/10.1006/ijhc.1999.0343>
8. Dankbaar MEW, Roozeboom MB, Oprins EAPB, Rutten F, van Merriënboer JIG, van Saase JLCM, et al. Preparing residents effectively in emergency skills training with a serious game. *Simul Healthc.* 2017;12:9-16. <https://doi.org/10.1097/SIH.0000000000000194>
9. Dankbaar MEW, Richters O, Kalkman CJ, Prins G, ten Cate OTJ, van Merriënboer JIG, et al. Comparative effectiveness of a serious game and an e-module to support patient safety knowledge and awareness. *BMC Med Educ.* 2017;17:1-10. <https://doi.org/10.1186/s12909-016-0836-5>
10. Carter FJ, Schijven MP, Aggarwal R, Grantcharov T, Francis NK, Hanna GB, et al. Consensus guidelines for validation of virtual reality surgical simulators. *Surg Endosc.* 2005;19:1523-32. <https://doi.org/10.1007/s00464-005-0384-2>
11. Harris DJ, Bird JM, Smart PA, Wilson MR, Vine SJ. A framework for the testing and validation of simulated environments in experimentation and training. *Front Psychol.* 2020;11:605. <https://doi.org/10.3389/fpsyg.2020.00605>
12. Sadeghi AH, Peek JJ, Max SA, Smit LL, Martina BG, Roalia RA, et al. Virtual reality simulation training for cardiopulmonary resuscitation after cardiac surgery: face and content validity study. *JMIR Serious Games.* 2022;10:e30456. <https://doi.org/10.2196/30456>
13. Izard SG, Juanes JA, García Peñalvo FJ, Estella JMG, Ledesma MJS, Ruisoto P. Virtual reality as an educational and training tool for medicine. *J Med Syst.* 2018;42:50. <https://doi.org/10.1007/s10916-018-0900-2>
14. Gao M, Kortum P, Oswald F. Psychometric evaluation of the USE (usefulness, satisfaction, and ease of use) questionnaire for reliability and validity. *Proc Hum Factors Ergon Soc.* 2018;3:1414-8. <https://doi.org/10.1177/1541931218621322>
15. Jape D, Zhou J, Bullock S. A spaced-repetition approach to enhance medical student learning and engagement in medical pharmacology. *BMC Med Educ.* 2022;22:1-11. <https://doi.org/10.1186/s12909-022-03324-8>
16. Seymour NE, Gallagher AG, Roman SA, O'Brien MK, Bansal VK, Andersen DK, et al. Virtual reality training improves operating room performance results of a randomized, double-blinded study. *Ann Surg.* 2002;236:458-64. <https://doi.org/10.1097/0000658-200210000-00008>

Key Words: virtual reality, extracorporeal circulation, simulator

APPENDIX E1. INFORMED CONSENT FORM FOR PARTICIPATING IN SCIENTIFIC RESEARCH

Participant Information: VR-ECC Face and Content Validity

General information and objectives

Operating a heart lung machine (HLM) in order to perform Extracorporeal Circulation (ECC) is a complex and multifaceted task, requiring a knowledge of protocols for operating both under normal conditions, and more extreme deviations occurring with an equipment malfunction for example. The VR-ECC sim aims to recreate an HLM in a virtual environment, where perfusionists can learn and practice their skills. Over the past years emerging virtual reality (VR) applications have quickly gained broad attention in the medical field, including cardiology and cardiothoracic surgery, as well as medical education and communication. Combining VR technology with head mounted displays (HMD) (eg, Oculus), enables the design of a realistic, custom made simulation in a 3-dimensional and fully immersive environment. Such a VR simulation enables the user to train themselves repeatedly, without the need for other supplies or instructor-led training sessions. In this study, we will investigate the face and content validity of the VR-ECC sim, or how realistic this simulator is for the purposes of education.

1. What participation involves

If you participate in this study, you will first fill in a short questionnaire, about experience as a perfusionist/perfusion student, and experience with digital training methods such as e-learning and Virtual Reality. You will then be asked to complete a training scenario from the VR-ECC sim, and afterwards complete a Usefulness, Satisfaction, Ease of Use (USE) questionnaire about your experience in the simulator. No follow up is required. There is a minor risk of nausea or dizziness that may occur during the simulation associated with virtual reality. If this occurs, please notify a research assistant who will help you remove the goggles.

2. If you don't want to participate and/or stop participating in the study

Participation is voluntary, so you decide whether to participate or not in this study. You can decide to stop participating at any point. Your participation ends if you choose to stop or when all measurements are completed.

3. Usage and storage of data

Your personal data will be collected, used, and stored securely for this study. This concerns data such as your

age, experience as a perfusionist, VR and e-learning. The collection, use, and storage of this data is necessary to answer the questions asked in this research and to publish the results. When data is collected, your data will be assigned a study code, and the data is anonymized. Only with a key the data is traceable, this key is safely stored in the Erasmus MC. Data will be stored on an Erasmus MC local network drive with automatic overnight backup. Stored data regarding anonymous data sets and personnel included in this study can only be accessed by the investigators, the Erasmus MC ethics committee, Erasmus MC auditors and Erasmus MC monitors and any person or agency required by Dutch law such as the "Inspectie voor de Gezondheidszorg". All data will be treated according to the "Wet Bescherming Persoonsgegevens" and the Erasmus MC privacy regulations. Any information from this study, if published in scientific journals or presented at scientific meetings, will not reveal participant identity. Data will be stored for a maximum of 15 years after ending the study.

Title of the research: **Virtual Reality Simulation as a Tool for Training of Perfusionists in Extra Corporeal Circulation; a Feasibility Study.**

I declare that I read the consent form. I had the opportunity to ask additional questions which are answered to my satisfaction.

- I had sufficient time to consider my participation.
- I am aware that participation is voluntary and that I may decide at any time not to participate or withdraw from the study. I do not need to give a reason for this.
- I give permission for collection and use of my data to answer the research question of this study.
- I am aware that appointed persons may have access to my data in order to verify the study. These people are listed in the information sheet. I give consent for the inspection by them.
 - I wish to participate in this study and I give consent for my data to be used for this study.
 - I **do not** wish to participate in this study and I do not give consent for my data to be used for this study.

Name of Participant:

Signature: Date: __/__/__

I hereby declare that I have fully informed this study subject about this study.

Name of investigator (or his/her representative):

Signature: Date: __/__/__

APPENDIX E2. USER EXPERIENCE QUESTIONNAIRE FOR THE EXTRACORPOREAL CIRCULATION-VIRTUAL REALITY (ECC VR) SIMULATOR

Please complete the following:

Male/female/other Age: _____ Profession: _____

1. How many years of work experience do you have in thoracic surgery working as a perfusionist or trainee perfusionist?

2. How many ECC operations have you participated in?
 - I have never participated in an ECC operation.
 - 1 to 5 times.
 - 5 to 10 times.
 - More than 10 times.
3. Do you have experience with gaming consoles (eg computer gaming, Xbox, PlayStation)?
 - I have never used a gaming console.
 - I have used a gaming console a few times before.
 - I game on a regular basis (at least once a month).

4. How often do you use VR hardware/software (eg VR gaming, simulations, consoles, entertainment etc.)?
 - I have never had a VR experience until today.
 - I have used VR a few times before.
 - I am experienced and use VR on a regular basis (at least once a month)
 - I am an VR expert (have a VR console and applications myself)
5. Do you have experience with physical simulation trainings in skills labs?
 - I have never had simulation training before.
 - I have had simulation trainings multiple times before.
 - I am a certified simulation trainer.
6. Do you have experience with digital training (eg e-learning or serious games)?
 - I have never had such training before.
 - I have had a digital training a few times before.
 - I have had digital trainings multiple times before.
7. Do you have experience with a simulation training in VR?
 - Yes.
 - No.

| | 1. Fully disagree | 2. Disagree | 3. Neutral | 4. Agree | 5. Fully agree | N/A |
|---------------------|--|-------------|------------|----------|----------------|-----|
| Usefulness | | | | | | |
| 1 | I learned a lot about ECC in the VR-ECC simulation | | | | | |
| 2 | The VR-ECC simulation helped me being more confident in taking the lead as a future operator of ECC | | | | | |
| 3 | The VR-ECC simulation helped me remember the steps in performing ECC | | | | | |
| 4 | After the VR-ECC simulation, I have enough knowledge to take the lead of a future ECC operation | | | | | |
| 5 | CPVR simulation is a useful way to train ECC scenarios | | | | | |
| Satisfaction | | | | | | |
| 6 | I liked participating in the VR-ECC simulation | | | | | |
| 7 | I enjoy using VR for learning purposes | | | | | |
| 8 | I would recommend using VR for training purposes to other colleagues | | | | | |
| 9 | I would prefer VR training <u>instead of</u> conventional training (in-classroom training with PowerPoint and a simulation with multiple participants) | | | | | |
| 10 | I would prefer VR training <u>instead of</u> digital training (eg e-learning or serious game) | | | | | |
| 11 | I would prefer VR training <u>additionally to</u> conventional training (in-classroom training with PowerPoint and a simulation with multiple participants)? | | | | | |
| 11 | I would prefer VR training <u>additionally to</u> digital training (eg e-learning or serious game) | | | | | |
| Ease of use | | | | | | |
| 12 | The interaction with the VR-ECC software felt intuitive | | | | | |
| 13 | It was easy to learn how to interact with the software | | | | | |

(Continued)

. Continued

| | | 1. Fully disagree | 2. Disagree | 3. Neutral | 4. Agree | 5. Fully agree | N/A |
|----------------------|---|-------------------|-------------|------------|----------|----------------|-----|
| 14 | It was easy to move around in the VR environment | | | | | | |
| 15 | It was easy to pick up and move objects in the VR environment | | | | | | |
| 16 | The VR-ECC simulation responds adequately and is not lacking when using the buttons on the controllers | | | | | | |
| 17 | When moving the head and hands with the HMD, the VR-ECC simulation moved corresponding to the movements | | | | | | |
| 18 | There delay between the (movements of the) controls and the response in the VR-ECC simulation was <u>not</u> disturbing | | | | | | |
| Immersiveness | | | | | | | |
| 19 | I felt like I was actually in a real operating theatre during the VR-ECC simulation | | | | | | |
| 20 | I was <u>not</u> distracted during the VR-ECC simulation | | | | | | |
| 21 | The in-depth perception of the VR-ECC simulation was of good quality | | | | | | |
| 22 | I felt actively involved in the patient scenario of the VR-ECC simulation | | | | | | |
| 23 | I felt in charge of the case during the VR-ECC simulation | | | | | | |
| 24 | Communication with the colleagues in the VR-ECC simulation felt natural | | | | | | |
| 25 | I was interested in the progress of the events within the simulation | | | | | | |

Write down the advantages and disadvantages of the VR-ECC simulation training, rank them in order of importance, from most important (1) to least important (3).

Advantages:

- 1.
- 2.
- 3.

Disadvantages:

- 1.
- 2.
- 3.

Do you have any comments or did you miss something in the simulation?

Thank you for participating!