



LAWRENCE
LIVERMORE
NATIONAL
LABORATORY

UCRL-TR-235948

LCLS soft x-ray imager mirrors and their performance

S. Bajt

October 30, 2007

Disclaimer

This document was prepared as an account of work sponsored by an agency of the United States government. Neither the United States government nor Lawrence Livermore National Security, LLC, nor any of their employees makes any warranty, expressed or implied, or assumes any legal liability or responsibility for the accuracy, completeness, or usefulness of any information, apparatus, product, or process disclosed, or represents that its use would not infringe privately owned rights. Reference herein to any specific commercial product, process, or service by trade name, trademark, manufacturer, or otherwise does not necessarily constitute or imply its endorsement, recommendation, or favoring by the United States government or Lawrence Livermore National Security, LLC. The views and opinions of authors expressed herein do not necessarily state or reflect those of the United States government or Lawrence Livermore National Security, LLC, and shall not be used for advertising or product endorsement purposes.

This work performed under the auspices of the U.S. Department of Energy by Lawrence Livermore National Laboratory under Contract DE-AC52-07NA27344.

LCLS soft x-ray imager mirrors and their performance

Saša Bajt

Lawrence Livermore National Laboratory

October 19, 2007

Soft X-ray imager mirrors have been designed, calibrated and fabricated at Lawrence Livermore National Laboratory and characterized at the Advanced Light Source for their performance between 200 and 1300 eV.

The mirrors are coated with a multilayer coating consisting of 70 bilayers of W/ SiC. The mirrors are to reflect at 22.5 deg from grazing angle at 1.50 nm wavelength and the width of the reflectivity peak should be at least 1.3%. Also, the mirrors should be non-reflective elsewhere. Our multilayer design was optimized to satisfy these requirements. The coating is very challenging since the individual layer thicknesses need to be less than 1 nm thick and reproducibility from layer to layer is crucial. To minimize the second harmonic peak we designed a multilayer with $\Gamma = 0.5$ (W and SiC layer thicknesses are the same). This way we end up with a mirror that has only the 1st and 3rd harmonic peak as shown in Figure 1. To suppress reflectivity outside the first peak we used our novel approach, an antireflective coating. Modeling predicted substantial reduction in reflectivity, especially for lower energies as shown in Figure 1.

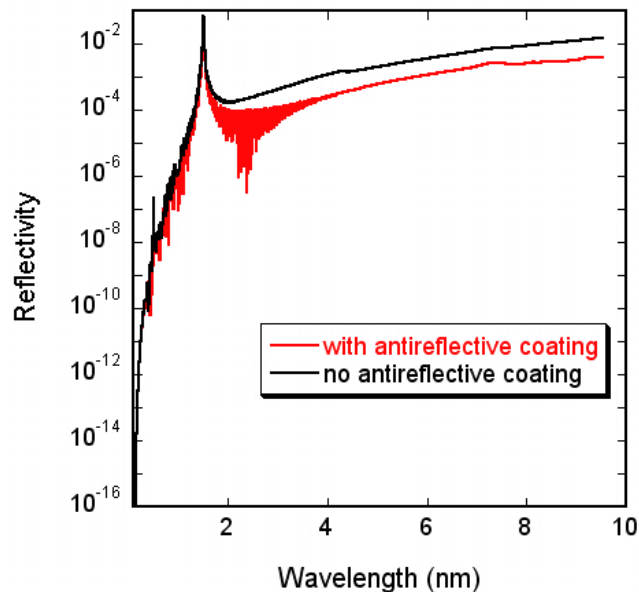


Figure 1: Modeled reflectivity shows complete suppression of the 2nd order harmonic peak at 0.76 nm and a very weak 3rd harmonic peak at 0.5 nm (10^{-7}) as an effect of the antireflective coating. The red curve is a mirror with antireflective coating and the black is the one without.

The experimental results of the soft x-ray imager mirror as measured at the ALS are shown in Figure 2 (log and linear scale). The energy range over which we measured the reflectivity is limited by the beamline hardware. This plot is a compilation of about six scans over different energy ranges using different gratings, filters and order sorter positions. The measured reflectivity of the peak at 1.505 nm is 4.3% with the peak width of 0.028 nm or 1.8%, satisfying the specs on the peak width.

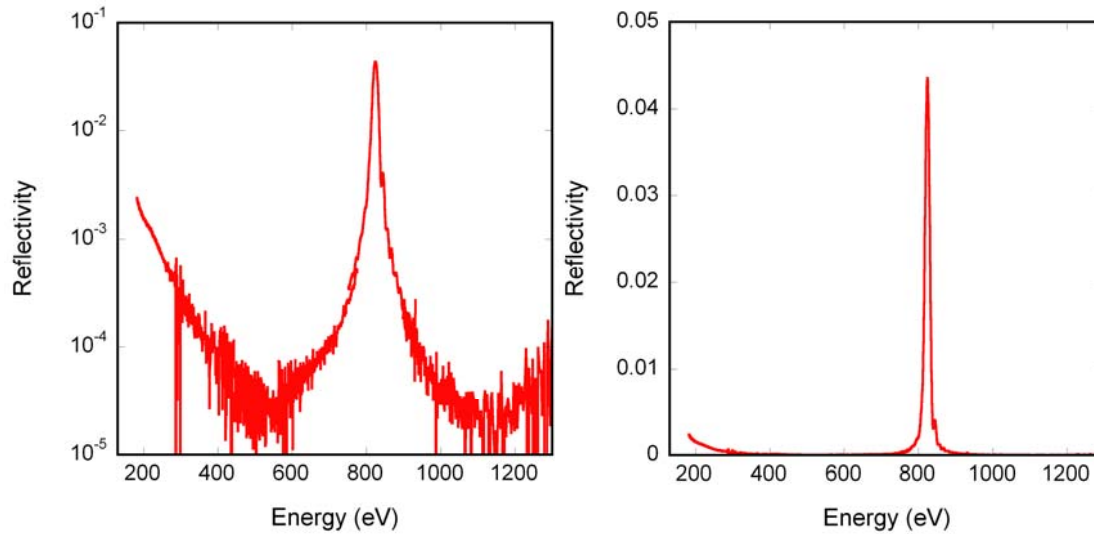


Figure 2: Measured reflectivity of the soft X-ray imager mirror for the LCLS between 200 and 1300 eV on a logarithmic (left) and linear (right) scale.

The other important specification was overall low reflectivity (except for 1st harmonic). We demonstrated this with the antireflective coating that is applied on these mirrors. The application of the antireflective coating also reduces the reflectivity of the 1st harmonic peak from 8.23% to 4.30%, which is in agreement with our modeling results. As shown in Figure 3 the antireflective coating substantially suppresses reflectivity in the energy range between 200 and 800 eV.

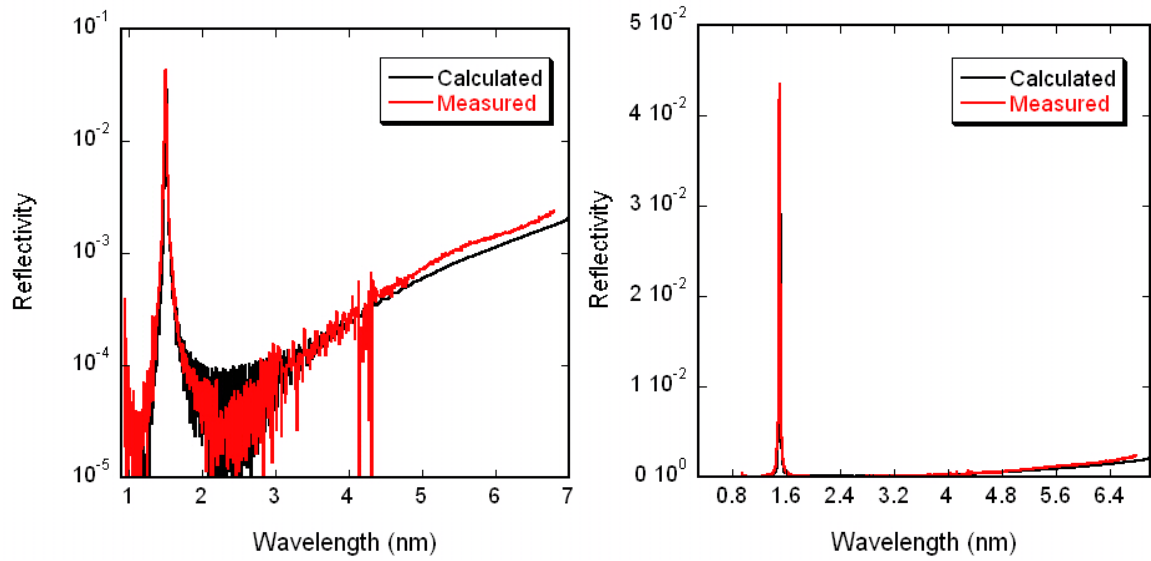


Figure 3: Measured (red) and calculated (black) reflectivity of soft x-ray imager mirror for the LCLS on a logarithmic (left) and linear (right) scale.

Considering the excellent agreement between modeled and measured data we then take a step further and extrapolate the calculation (Figure 1) up to 10 keV (0.12 nm). It is clear that the 2nd order harmonic is suppressed while the 3rd harmonic has reflectivity of only 10^{-7} . Finally, we also calculate the rocking curve of the 1st harmonic (Figure 4), which is of importance if a two bounce mirror system will be necessary.

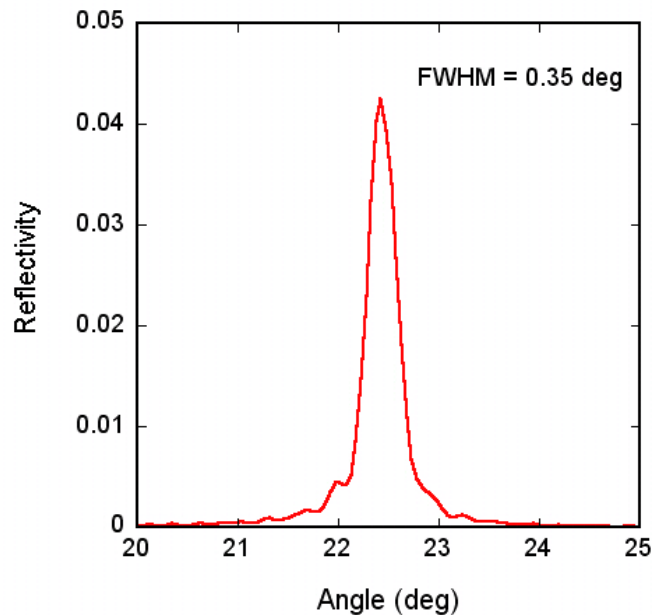


Figure 4: Calculated rocking curve for the 1st harmonic.

In summary, two 100 mm mirrors with >4% reflectivity at 1.50 nm and 1.8% FWHM for operation at 22.5 deg grazing angle were fabricated. Both mirrors are coated with antireflective coating that suppresses radiation outside the 1st harmonic. Experimental and modeling results are in excellent agreement indicating that we understand the physics of this multilayer system very well.

This work was performed under the auspices of the U.S. Department of Energy by Lawrence Livermore National Laboratory under Contract DE-AC52-07NA27344.