

## A novel electrochemical aptamer-antibody sandwich assay for lysozyme detection

Cristina Ocaña<sup>a,b</sup>, AkhtarHayat<sup>b,c</sup>, RupeshMishra<sup>b</sup>, Alina Vasilescu<sup>d</sup>, Manel del Valle<sup>a</sup>, Jean-Louis Marty<sup>b\*</sup>

<sup>a</sup>*Sensors and Biosensors Group, Department of Chemistry, Universitat Autònoma de Barcelona, 08193 Bellaterra, Spain*

<sup>b</sup>*Université de Perpignan, Laboratoire IMAGES, EA 4218, 52 avenue Paul Alduy, bât. S, Perpignan cedex 66860, France*

<sup>c</sup>*Interdisciplinary Research Centre in Biomedical Materials (IRCBM), COMSATS Institute of Information Technology (CIIT), Lahore, Pakistan*

<sup>d</sup>*International Centre of Biodynamics, 1B Intrarea Portocalelor, sector 6, 060101, Bucharest, Romania*

\*Corresponding author: jlmarty@univ-perp.fr

### Abstract

In this paper, we reported a novel electrochemical aptamer-antibody based sandwich biosensor for the detection of lysozyme. In the sensing strategy, Anti-lysozyme aptamer was immobilized onto the carbon electrode surface by covalent binding via diazonium salt chemistry. After incubating with the target protein (lysozyme), a biotinylated antibody was used to complete the sandwich format. The subsequent additions of avidin-alkaline phosphatase as enzyme label, and 1-naphthyl phosphate substrate (1-NPP) allowed to determine the concentration of lysozyme (Lys) via Differential Pulse Voltammetry (DPV) of the generated enzyme reaction product, 1-naphthol. Using this strategy, a wide detection range from 1 fM to 5 nM was obtained for target lysozyme, with a detection limit of 4.3 fM. The control experiments were also carried out by using albumin (BSA), cytochrome c and casein. The results showed that the proposed biosensor had good specificity, stability and reproducibility for lysozyme analysis. In addition, the biosensor was applied for detecting lysozyme in spiked wine samples, very good recovery rates were obtained in the range from 96.67 to 102% for lysozyme detection. This implies that the proposed sandwich biosensor is a promising analytical tool for the analysis of lysozyme in real samples.

**Keywords:** aptamer-antibody sandwich, biosensor, lysozyme detection, differential pulse voltammetry, wine sample

**Post-print of:** Ocaña, C. et al "A novel electrochemical aptamer-antibody sandwich assay for lysozyme detection" in The Analyst (Ed. RSC), vol. 140, issue 12 (June 2015), p. 4148-4153. **The final version is available at:** DOI 10.1039/c5an00243e

## 1. Introduction

Nowadays, use of biosensors for detection and quantification of proteins plays a vital role in research<sup>1</sup>, clinical applications<sup>2</sup> and food industry<sup>3</sup>. Biosensors are analytical devices which incorporate a biomolecule to provide specific recognition for an analyte together with transduction technology to detect and quantify the binding taking place between analyte and detector molecule<sup>4</sup>. Traditionally, enzymes, antibodies and proteins have been employed in biosensors as biorecognition species. Since their discovery in 1990<sup>5</sup>, aptamers have attracted considerable attention in biosensor development<sup>6</sup>. Aptamers are artificial DNA or RNA oligonucleotides selected *in vitro* which have the ability to bind to proteins, small molecules or even whole cells, with high affinity and specificity<sup>7</sup>. They offer many advantages over antibodies such as relatively easy production, highly affinity and specificity, easy chemical modification and high stability<sup>8</sup>. Thanks to these excellent properties, a number of aptamer-based sensors have been developed using different transducer techniques<sup>9, 10</sup>. Among different types of biosensors, electrochemical biosensing is of particular interest due to its remarkable sensitivity, simple instrumentation, fast response, low cost and portability<sup>11</sup>.

Lysozyme (Lys) is a relatively small protein (14.3 kDa) consisting of only 129 amino acid residues, and is widely distributed in the nature<sup>12</sup>. It has an isoelectric point of 11.0 and constitutes 3.5% of egg white protein. It is clear that lysozyme's relatively small size and simplicity makes it an excellent model analyte for novel methods in protein detection. This protein is also known as N-acetylmuramide glycan hydrolase due to its property to destroy bacterial cellular membranes by catalyzing the hydrolysis of glycosidic bonds between N-acetylmuramic acid and N-acetylglucosaminein peptidoglycan residues of Gram-positive bacteria cell walls<sup>13</sup>. Moreover, the monitoring of lysozyme level is used as a marker of some health problems such as

1  
2  
3 bronchopulmonary dysplasia in newborns<sup>14</sup>, conjunctivitis, kidney problems<sup>15</sup> and  
4  
5 leukemia<sup>16</sup>. Additionally, Lys has been widely used as an antimicrobial agent in the  
6  
7 production of wine<sup>17</sup>, cheese<sup>18</sup>, beers<sup>19</sup> and as well as to prolong the shelf-life of shrimp,  
8  
9 surimi products and sausages<sup>20</sup>. Specifically, in wine-making, Lys has been used since  
10  
11 1990 to prevent or mitigate heterolactic fermentation<sup>17</sup>. The maximum permitted level  
12  
13 of lysozyme in wine samples is 500 mg/L ( $\sim 35\mu\text{M}$ )<sup>21</sup>. Being an egg-protein, lysozyme  
14  
15 is considered as an allergen; therefore developing new, rapid, cheap and sensitive  
16  
17 methods for the detection of Lys is of great significance.  
18  
19

20  
21 Presently, the available analytical methods for the detection of lysozyme include  
22  
23 conventional methods like chromatographic or immunosensing techniques based on  
24  
25 ELISA, which have high sensitivity, but high cost and experimental complexity. Thus,  
26  
27 numerous sensors have been presented as alternatives to overcome these limitations  
28  
29 based on mainly electrochemical and optical detection<sup>22</sup>. In this work, we report a novel  
30  
31 electrochemical aptamer-antibody sandwich assay for the detection of Lys. Differential  
32  
33 Pulse Voltammetry (DPV) technique was used to detect Lys via 1-naphtol oxidation  
34  
35 signal changes. For this purpose, the aptamer was immobilized onto the electrode  
36  
37 surface by covalent binding via diazonium salt. After incubating with lysozyme, a  
38  
39 biotinylated antibody was used to form the sandwich format. The addition of avidin  
40  
41 modified alkaline phosphatase and the 1-NPP enzymatic substrate allowed to detect  
42  
43 lysozyme based on the electrochemical oxidation signals of 1-naphtol. Results showed  
44  
45 that this novel biosensor can be used for accurate quantification of the concentration of  
46  
47 Lys in spiked wine samples. The developed biosensor is simple, sensitive, specific and  
48  
49 fast for the detection of Lys.  
50  
51  
52  
53  
54

## 55 **2. Experimental**

### 56 *2.1. Chemicals and materials*

1 Potassium dihydrogen phosphate, sodium monophosphate, bovine serum alumina  
2 (BSA), lysozyme (Lys), avidin-labeled alkaline phosphatase (Av-ALP), casein, biotin-  
3 labeled rabbit anti-chicken Lys antibody (AbLysBio), magnesium chloride, potassium  
4 chloride, sodium chloride, ethanolamine, diethanolamine (DEA), N-  
5 hydroxysuccinimide (NHS), N-(3-dimethylaminopropyl)-N'-ethyl-carbodiimide  
6 hydrochloride (EDC), 4-aminobenzoic acid (ABA), 1-naphtyl phosphate (1-NP) and  
7 sodium nitrite were purchased from Sigma (St. Louis, MO, USA). All reagents were  
8 analytical reagent grade. The aptamer used was:

19 AptLys<sup>23</sup>

20  
21  
22  
23 5'-NH<sub>2</sub>-GCA GCT AAG CAG GCG GCT CAC AAA ACC ATT CGC ATG CGG C-3'  
24  
25 and was provided by Eurogenetic (France)

26  
27  
28 All solutions were made up using MilliQ water. The buffers employed were: binding  
29 buffer (BB) (1mM MgCl<sub>2</sub>, 2.7mMKCl, 140mMNaCl, 0.1mM Na<sub>2</sub>HPO<sub>4</sub> and  
30 1.8mMKH<sub>2</sub>PO<sub>4</sub> pH 7.4), 10% DEA buffer (pH 9.5) and 100mM MES buffer containing  
31 0.09%NaCl.

### 32 33 34 35 36 37 *2.2. Equipment*

38  
39  
40 The electrochemical measurements were performed using an Autolab PGSTAT100  
41 potentiostat/galvanostat (Eco Chimie, Netherlands) controlled by General Purpose  
42 Electrochemical System software (GPES) (4.9) for voltammetry. Screen printed carbon  
43 electrodes (SPCEs) were fabricated using a DEK 248 screen-printing system. The SPCE  
44 consists of conventional three electrode configuration with graphite as working (4-mm  
45 diameter disk) and counter (16 mm × 1.5 mm curved line) electrode, and Ag/AgCl (16  
46 mm × 1.5 mm straight line) as pseudo reference electrode.

### 47 48 49 50 51 52 53 54 55 56 57 *2.3. Experimental protocol*

### 2.3.1. Electrochemical SPE pretreatment

SPE was subjected to electrochemical pretreatment by 10 cyclic potential scans between 1.0 and -1.5V at scan rate of 0.2V/s in 0.5M H<sub>2</sub>SO<sub>4</sub> and 0.1M KCl. Then, the electrodes were rinsed with water.

### 2.3.2. Immobilization of AptLys onto the electrode surface

In detail, the diazonium cation was synthesized by in situ reaction of 2 $\mu$ L of 1M NaNO<sub>2</sub> and 1mL of 2mM ABA prepared in 0.5M HCl. The mixture was left to react for 5 min at room temperature. 100 $\mu$ L of this mixture and 100 $\mu$ L of 0.5M HCl were deposited onto the electrode surface and the electrochemical modification was performed by linear sweep voltammetry from 0.6 to -0.8V. After modification, the electrode was rinsed three times with distilled water. The carboxylic groups onto the electrode surface were activated with 100  $\mu$ L of 100mM EDC and 25mM NHS in 100mM MES buffer for 1 hour. After rinsing three times with distilled water, 30 $\mu$ L of 10 $\mu$ M solution of Apt were incubated onto the electrode surface for 1 hour. After that, the electrodes were washed three times with BB to remove the unbound aptamer. In order to deactivate the remaining succinimide groups, the electrodes were incubated with 30  $\mu$ L of 1M ethanolamine solution. After washing three times with BB, the electrodes were incubated with 30 $\mu$ L of 5% BSA solution for 1h to avoid nonspecific adsorption. The modified electrodes can be used directly or stored dry at 4°C for several days without decrease in the sensitivity.

### 2.3.3. Aptamer-antibody sandwich assay

The electrodes were incubated with different concentrations of Lys for 15 min. Then, the electrodes were washed three times with BB. In order to achieve the aptamer-antibody sandwich, the electrodes were incubated with 30  $\mu$ L of anti-Lys antibody from a 1/1500 dilution of the stock solution in BB buffer. The incubation took place for 1 h.

1  
2 This was followed by three washing steps using BB. Then, 30  $\mu\text{L}$  of av-ALP, from  
3  
4 1/12500 dilution from the stock solution of enzyme, were deposited on the electrodes  
5  
6 for 1 h. After that, the electrodes were washed three times with BB.  
7

#### 8 9 *2.3.4. Electrochemical detection*

10  
11 90  $\mu\text{L}$  of 10% DEA buffer and 10  $\mu\text{L}$  of 1-NPP  $5\text{mg}\cdot\text{mL}^{-1}$  were added on the electrode  
12  
13 surface and incubated for 2 min at room temperature. Electrochemical detection was  
14  
15 performed by DPV. A modulation time of 2s, interval time of 0.2 s, initial potential of  
16  
17 0.1V, end potential of 0.4V, step potential of 0.01V, modulation amplitude of 0.06V  
18  
19 and stand-by potential of 0 V were applied. The height of the resulting oxidation peak  
20  
21 was recorded and plotted against Lys concentration to give a calibration curve.  
22  
23

#### 24 25 *2.3.5. Wine samples preparation*

26  
27 Wine samples were prepared following a protocol from a previous study<sup>24</sup>. Briefly, 1  
28  
29 mL of wine sample was spiked with 200 $\mu\text{M}$  of Lys and allowed to stand for 3min. Next,  
30  
31 200 $\mu\text{L}$  of a 5M NaCl solution containing 5% Tween-20 surfactant were added to 200 $\mu\text{L}$   
32  
33 of lysozyme–wine mixture and diluted to a final volume of 1mL using 20mM MES  
34  
35 buffer pH 6 with 1mM  $\text{MgCl}_2$ . This mixture was further centrifuged at 5000rpm for  
36  
37 5min and diluted using the buffer aforesaid to obtain the desired concentration of Lys.  
38  
39

### 40 41 **3. Results and discussion**

#### 42 43 44 *3.1. Principle of the aptamer-antibody sandwich assay*

45  
46 Figure 1 illustrates the different steps involved in the fabrication of biosensor for the  
47  
48 detection of Lys based on its specific recognition by aptamer-antibody assay. As  
49  
50 described in Section 2.3, the aptamer was covalently immobilized through EDC/NHS  
51  
52 chemistry via diazonium salt on the SPE surface. This step was followed by a blocking  
53  
54 step with BSA to avoid non-specific adsorption on the transducer surface. Then, Anti-  
55  
56  
57  
58  
59  
60

1  
2  
3 Lys antibody was incubated on the sensing platform to obtain sandwich type detection.  
4  
5 Thereafter, a solution of avidin modified-ALP was deposited onto the electrode surface  
6  
7 to achieve coupling to the antibody through biotin-avidin affinity. Finally, the biosensor  
8  
9 was immersed in DEA buffer solution of pH 9.5 containing 1-NPP as ALP substrate,  
10  
11 and Lys was determined by differential pulse voltammetry of the generated 1-naphtol as  
12  
13 the enzyme reaction product.  
14  
15

16  
17 <Figure 1>  
18

### 19 20 3.2. Optimization of the working experimental conditions 21

22  
23 In order to achieve the improved analytical characteristics of a proposed biosensor, it is  
24  
25 of vital importance to optimize the different experimental parameters. In this context,  
26  
27 several parameters including concentrations of anti-Lys antibody and avidin modified  
28  
29 enzyme, and their incubation time with Lys were optimized prior to perform  
30  
31 concentration dependence response of the proposed sandwich assay. Figure 2a shows  
32  
33 the voltammetric peak response of *1-NPP* in the presence of different concentrations of  
34  
35 Anti-Lys antibody (1/3000 from to 1/500, dilutions from stock solution of antibody). As  
36  
37 can be observed, the current response increased rapidly with increasing concentration of  
38  
39 Anti-Lys antibody, with a maximal electrochemical output signal at 1/1500. Similarly,  
40  
41 Figure 2b shows that peak current increased with increasing concentration of avidin  
42  
43 modified ALP till 1/12500 (dilution from stock enzyme solution), which was followed  
44  
45 by a decrease in response for subsequent increasing concentration, indicating the  
46  
47 saturation point of enzyme label is reached. Thus, 1/1500 and 1/12500 were chosen as  
48  
49 the optimal dilutions for Anti-Lys antibody and avidin modified-ALP respectively.  
50  
51  
52  
53

54  
55 The effect of the incubation time of Lys on the current response of the biosensor  
56  
57 was also studied. As can be seen from Figure 2c, the maximum peak current of *1-NPP*  
58  
59  
60

1 was observed for an incubation period of 15 min. For longer incubation times, the peak  
2 current was decreased. Thus, according to the experimental results, an incubation time  
3 period of 15 min was selected to perform the further experiments.  
4  
5  
6  
7

8  
9 <Figure 2>

### 10 3.3. Analytical performance of the aptamer-antibody sandwich biosensor

11  
12  
13 In order to perform the quantitative analysis, the designed biosensor was incubated with  
14 different concentrations of Lys under the optimal conditions, and the DPV responses  
15 were recorded to draw a calibration curve. As shown in the Figure 3a, the oxidation  
16 peak current increased with the increasing concentration of Lys. The peak current was  
17 plotted against the concentration of Lys, and the calibration plots (Figure 3b) exhibited  
18 a good linear correlation between the peak current and the logarithm of Lys  
19 concentrations in the range from 5fM to 5nM with a correlation coefficient of 0.998.  
20 The calculated limit of detection (LOD) for Lys was 4.3fM. The reproducibility of the  
21 method showed a relative standard deviation (RSD) of 5.5%, obtained from a series of 3  
22 experiments carried out in a concentration of 5nM of Lys. Table 1 provides a  
23 comparison of different biosensors reported in the literature for Lys detection. The data  
24 in Table 1 indicates the lowest limit of detection of our proposed sandwich biosensor as  
25 compared to the LOD of previously reported biosensors for Lys detection. In addition,  
26 the linear range was greatly improved, being much wider than for other biosensors.  
27  
28  
29  
30  
31  
32  
33  
34  
35  
36  
37  
38  
39  
40  
41  
42  
43  
44

45 <Figure 3>

46  
47  
48 <Table 1>

### 49 3.4. Selectivity of the biosensor

50  
51  
52 In order to establish the specificity and selectivity of the designed biosensors, different  
53 proteins including casein, BSA and cytochrome c were incubated on the biosensor  
54  
55  
56  
57  
58  
59  
60



1  
2  
3 surface and DPV measurements were carried out under the same experimental  
4  
5 conditions as those described for Lys analysis. As shown in Figure 4, the presence of  
6  
7 these proteins exhibited a negligible response compared with that of Lys, even in the  
8  
9 case of cytochrome c which is structurally similar to Lys. Therefore, the results  
10  
11 demonstrated that the developed strategy could be used to identify Lys with high  
12  
13 specificity.  
14

15  
16 <Figure 5>  
17

### 18 *3.5. Application of the biosensor for the detection of Lys in spiked wine sample*

19  
20 In order to demonstrate the analytical reliability and applicability of the method for real  
21  
22 sample matrix, analysis of wine samples were performed by spiking at three different  
23  
24 concentrations of Lys (1.5 nM-5 pM). The recovery values were determined in  
25  
26 accordance with the calibration curve performed in buffer. The obtained Lys  
27  
28 concentrations were in consistent with the spiked values, indicating the suitability of  
29  
30 method for real sample analysis. The recovery results along with other analytical  
31  
32 characteristic for the proposed biosensors are presented in the table 2.  
33  
34  
35

36 <Table 2>  
37

### 38 **Conclusions**

39  
40 In conclusion, a novel electrochemical biosensor has been successfully developed for  
41  
42 the detection of lysozyme protein based on a hybrid sandwich protocol. Differential  
43  
44 Pulse Voltammetry was used to detect Lys via the changes in 1-naphthol oxidation  
45  
46 signals. The described biosensor showed a lower detection limit (4.3fM) as compared to  
47  
48 the previously reported biosensors for lysozyme detection (Table1), wide linear range  
49  
50 for lysozyme detection from 5 fM to 5nM, high sensitivity and selectivity. In addition,  
51  
52 the biosensor was used for detecting lysozyme in spiked wine samples and very  
53  
54  
55  
56  
57  
58  
59  
60

1  
2 promising recovery values were obtained, indicating the great potential of proposed  
3 methodology for detecting lysozyme in wines and possibly other food matrices.  
4  
5  
6

### 7 Acknowledgement

8  
9 Prof Dr Jean Louis Marty and Dr Alina Vasilescu would like to thanks BRANCUSI  
10 Project.  
11  
12  
13

### 14 References

- 15 1. T. F. McGrath, J. Buijs, A. C. Huet, P. Delahaut, C. T. Elliott and M. H.  
16 Mooney, *Sensors and Actuators B: Chemical*, 2013, **186**, 423-430.
- 17 2. P. D'Orazio, *Clinica Chimica Acta*, 2011, **412**, 1749-1761.
- 18 3. V. Scognamiglio, F. Arduini, G. Palleschi and G. Rea, *TrAC Trends in*  
19 *Analytical Chemistry*, 2014, **62**, 1-10.
- 20 4. G. D. Griffin, D. N. Stratis-Cullum and T. E. McKnight, in *Reference Module in*  
21 *Biomedical Sciences*, Elsevier, 2014.
- 22 5. A. D. Ellington and J. W. Szostak, *Nature*, 1990, **346**, 818-822.
- 23 6. E. Luzi, M. Minunni, S. Tombelli and M. Mascini, *TrAC Trends in Analytical*  
24 *Chemistry*, 2003, **22**, 810-818.
- 25 7. K. A. Davis, B. Abrams, Y. Lin and S. D. Jayasena, *Nucleic Acids Res.*, 1996,  
26 **24**, 702-706.
- 27 8. S. Tombelli, M. Minunni and M. Mascini, *Biomolecular Engineering*, 2007, **24**,  
28 191-200.
- 29 9. A. Hayat, A. Sassolas, J. L. Marty and A. E. Radi, *Talanta*, 2013, **103**, 14-19.
- 30 10. L. Zhang, P. Cui, B. Zhang and F. Gao, *Chemistry - A European Journal*, 2013,  
31 **19**, 9242-9250.
- 32 11. N. J. Ronkainen, H. B. Halsall and W. R. Heineman, *Chem. Soc. Rev.*, 2010, **39**,  
33 1747-1763.
- 34 12. M. Schindler, Y. Assaf, N. Sharon and D. M. Chipman, *Biochemistry*, 1977, **16**,  
35 423-431.
- 36 13. L. E. H. Smith, L. H. Mohr and M. A. Raftery, *Journal of the American*  
37 *Chemical Society*, 1973, **95**, 7497-7500.
- 38 14. M. E. Revenis and M. A. Kaliner, *The Journal of Pediatrics*, 1992, **121**, 262-  
39 270.
- 40 15. B. Porstmann, K. Jung, H. Schmechta, U. Evers, M. Pergande, T. Porstmann,  
41 H.-J. Kramm and H. Krause, *Clinical Biochemistry*, 1989, **22**, 349-355.
- 42 16. R. S. Pascual, J. B. L. Gee and S. C. Finch, *New England Journal of Medicine*,  
43 1973, **289**, 1074-1076.
- 44 17. C. Lasanta, A. Roldán, I. Caro, L. Pérez and V. Palacios, *Food Control*, 2010,  
45 **21**, 1442-1447.
- 46 18. M. Kondeková, V. Maier, P. Ginterová, J. Marák and J. Ševčík, *Food*  
47 *Chemistry*, 2014, **153**, 398-404.
- 48 19. C. Chen, X.-M. Sun and B.-H. Li, *Chinese Journal of Analytical Chemistry*,  
49 2011, **39**, 91-94.  
50  
51  
52  
53  
54  
55  
56  
57  
58  
59  
60

- 1
  - 2
  - 3
  - 4
  - 5
  - 6
  - 7
  - 8
  - 9
  - 10
  - 11
  - 12
  - 13
  - 14
  - 15
  - 16
  - 17
  - 18
  - 19
  - 20
  - 21
  - 22
  - 23
  - 24
  - 25
  - 26
  - 27
  - 28
  - 29
  - 30
  - 31
  - 32
  - 33
  - 34
  - 35
  - 36
  - 37
  - 38
  - 39
  - 40
  - 41
  - 42
  - 43
  - 44
  - 45
  - 46
  - 47
  - 48
  - 49
  - 50
  - 51
  - 52
  - 53
  - 54
  - 55
  - 56
  - 57
  - 58
  - 59
  - 60
20. R. Chander and N. Lewis, *European J. Appl. Microbiol. Biotechnol.*, 1980, **10**, 253-258.
21. I. O. o. V. a. Wine, 2013.
22. A. Vasilescu, S. Gaspar, I. Mihai, A. Tache and S. C. Litescu, *Analyst*, 2013, **138**, 3530-3537.
23. D. T. Tran, K. P. Janssen, J. Pollet, E. Lammertyn, J. Anne, A. Van Schepdael and J. Lammertyn, *Molecules (Basel, Switzerland)*, 2010, **15**, 1127-1140.
24. I. Mihai, A. Vezeanu, C. Polonschii, C. Albu, G.-L. Radu and A. Vasilescu, *Sensors and Actuators B: Chemical*, 2015, **206**, 198-204.
25. Y. Li, H. Qi, Q. Gao and C. Zhang, *Biosens. Bioelectron.*, 2011, **26**, 2733-2736.
26. H. Wang, W. Gong, Z. Tan, X. Yin and L. Wang, *Electrochim. Acta*, 2012, **76**, 416-423.
27. Y. Xiao, Y. Wang, M. Wu, X. Ma and X. Yang, *Journal of Electroanalytical Chemistry*, 2013, **702**, 49-55.
28. A. Erdem, E. Eksin and M. Muti, *Colloids and Surfaces B: Biointerfaces*, 2014, **115**, 205-211.
29. F. Rohrbach, H. Karadeniz, A. Erdem, M. Famulok and G. Mayer, *Anal. Biochem.*, 2012, **421**, 454-459.
30. Y. Peng, D. Zhang, Y. Li, H. Qi, Q. Gao and C. Zhang, *Biosens. Bioelectron.*, 2009, **25**, 94-99.
31. Y. Xia, S. Gan, Q. Xu, X. Qiu, P. Gao and S. Huang, *Biosens. Bioelectron.*, 2013, **39**, 250-254.
32. M. C. Rodríguez and G. A. Rivas, *Talanta*, 2009, **78**, 212-216.
33. Z. Chen and J. Guo, *Electrochim. Acta*, 2013, **111**, 916-920.
34. D. Xie, C. Li, L. Shangguan, H. Qi, D. Xue, Q. Gao and C. Zhang, *Sensors and Actuators B: Chemical*, 2014, **192**, 558-564.
35. Z. Chen, L. Li, Y. Tian, X. Mu and L. Guo, *Biosens. Bioelectron.*, 2012, **38**, 37-42.

1  
2  
3  
4  
5  
6  
7  
8  
9  
10 **Figures and Captions**  
11

12 **Figure 1.** Schematic representation of the developed sandwich biosensor.  
13

14 **Figure 2.** a) Optimization of the concentration of AbLys antibody. b) Optimization of the  
15 concentration of fav-ALP. c) Optimization of incubation time with Lys. Uncertainty  
16 values corresponding to replicate experiments (n = 3).  
17  
18

19 **Figure 3.** a) DPV curves for different concentrations of Lys; b) Calibration curve and  
20 regression plot of the biosensor. Uncertainty values corresponding to replicate  
21 experiments (n=3).  
22  
23  
24

25 **Figure 4** .Selectivity of the biosensor to casein, BSA and cytochrome Cat 5nM,  
26 respectively. Error bars are obtained based on three independent measurements.  
27  
28  
29  
30  
31  
32  
33  
34  
35  
36  
37  
38  
39  
40  
41  
42  
43  
44  
45  
46  
47  
48  
49  
50  
51  
52  
53  
54  
55  
56  
57  
58  
59  
60

## Tables

**Table 1.** Comparison of the proposed biosensor with other reported methodologies for lysozyme detection.

Analytical Technique	Detection Limit	Linear Range	Reference
Electroluminescence	120 pM	64pM-0.64μM	<sup>25</sup>
Electroluminescence	0.15ng·mL <sup>-1</sup> <sup>1</sup> (~10.4pM)	0.5nM-9nM	<sup>26</sup>
SPR	2.4nM	0.5-80μg·mL <sup>-1</sup>	<sup>24</sup>
Impedance	6fM	0.01-0.5pM	<sup>27</sup>
Impedance	28.53nM		<sup>28</sup>
Impedance	862nM	0-400μg·mL <sup>-1</sup>	<sup>29</sup>
Impedance	0.07nM	0.2nM-4nM	<sup>30</sup>
Square Wave Voltammetry	0.2nM	0.5nM-100nM	<sup>31</sup>
Square Wave Voltammetry	38/16nM	0-30mg·L <sup>-1</sup>	<sup>32</sup>
Square Wave Voltammetry	1nM	7-30nM	<sup>33</sup>
Square Wave Voltammetry	0.3pg·mL <sup>-1</sup> <sup>1</sup> (~20.8fM)	1-50pg·mL <sup>-1</sup>	<sup>34</sup>
Cyclic Voltammetry	0.1pM	5pM-1nM	<sup>35</sup>
Differential Pulse Voltammetry	4.3fM	5fM-5nM	Our work

**Table 2.** Recovery studies performed in spiked wine samples for applicability of biosensor (n=3).

Spiked [Lys] (M)	Found [Lys] (M)	R.S.D.%	Recovery %	Relative error %
$1.5 \cdot 10^{-9}$	$1.45 \cdot 10^{-9}$	3.1	96.67	3.33
$2.5 \cdot 10^{-11}$	$2.38 \cdot 10^{-11}$	4.2	95.2	4.8
$5 \cdot 10^{-12}$	$5.1 \cdot 10^{-12}$	5.1	102	1.96

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19

# Analyst

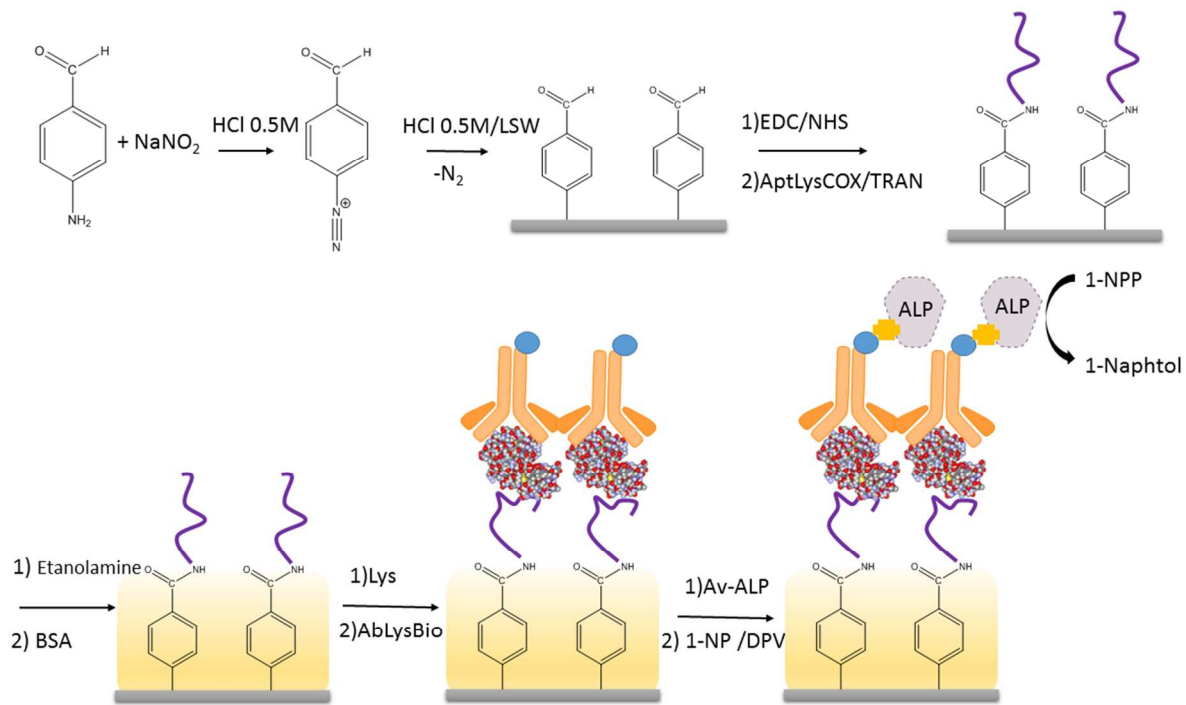


Figure 1

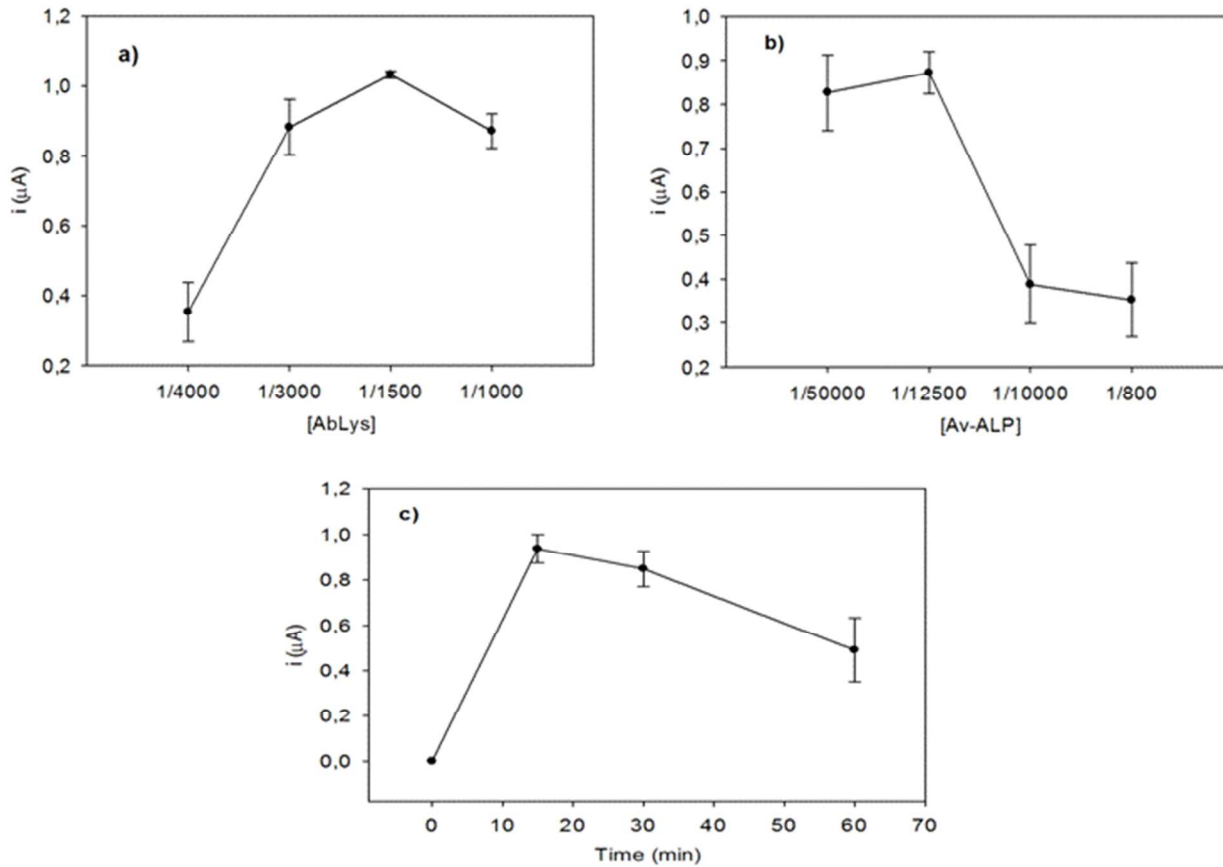


Figure 2

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20  
21  
22  
23  
24  
25  
26  
27  
28  
29  
30  
31  
32  
33  
34  
35  
36  
37  
38  
39  
40  
41  
42  
43  
44  
45  
46  
47  
48  
49  
50  
51  
52  
53  
54  
55  
56  
57  
58  
59  
60



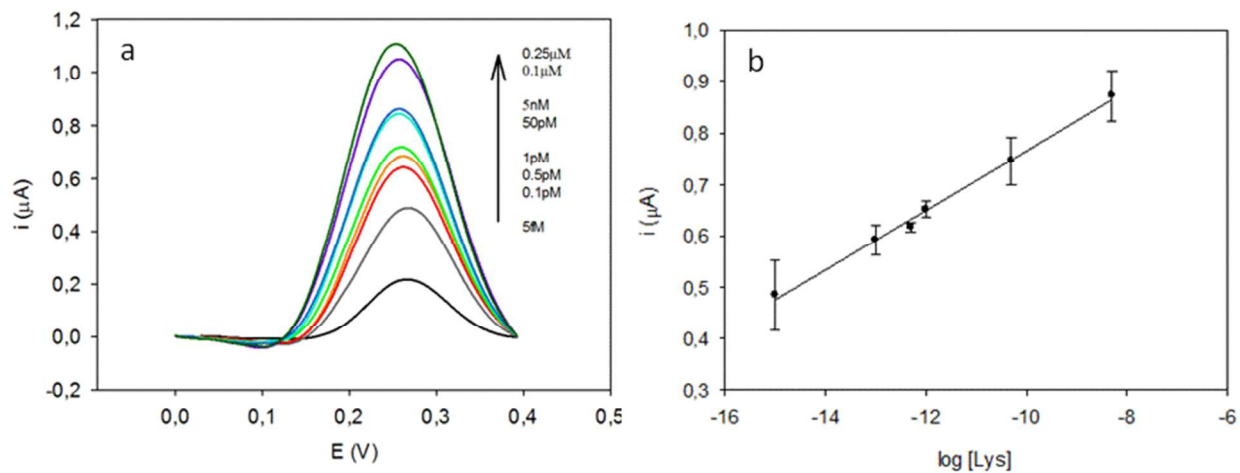


Figure 3

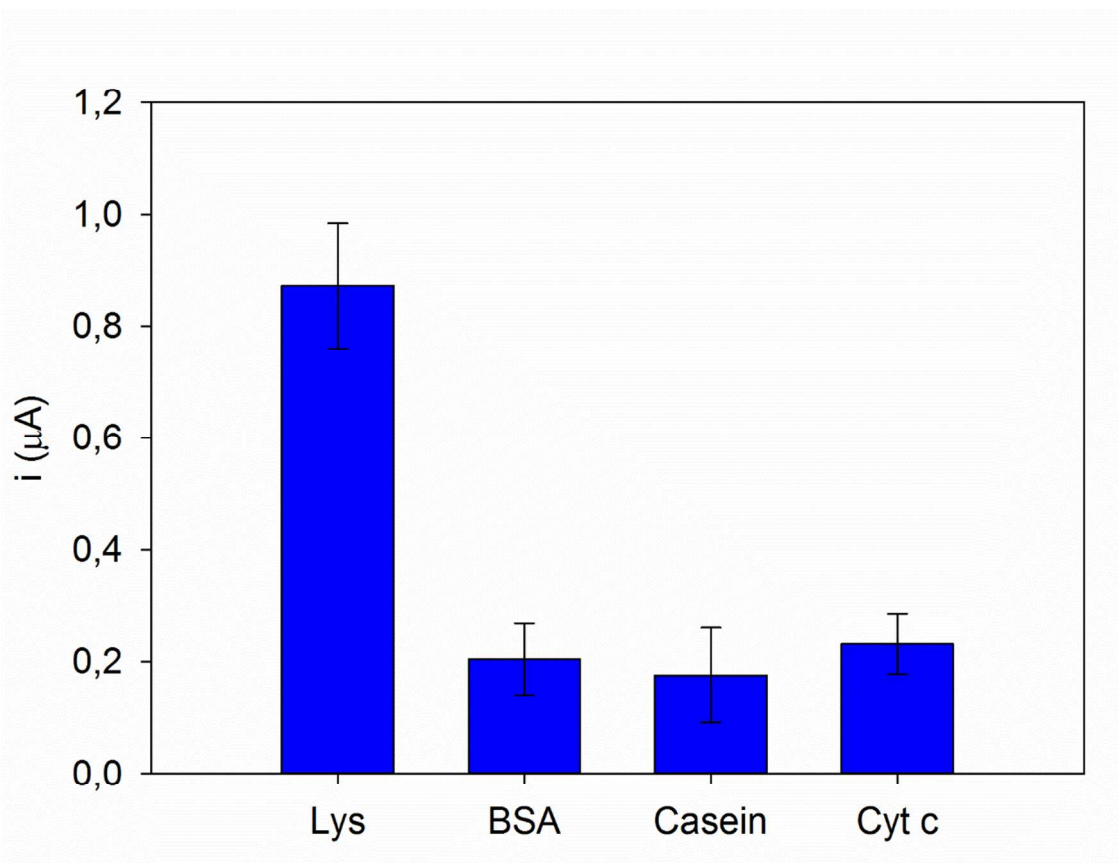


Figure 4