

MARGARITA KAGAN

Biosensing penicillins' residues
in milk flows



DISSERTATIONES CHIMICAE UNIVERSITATIS TARTUENSIS

156

MARGARITA KAGAN

Biosensing penicillins' residues
in milk flows



UNIVERSITY OF TARTU
Press

Institute of Chemistry, Faculty of Science and Technology, University of Tartu,
Estonia

Dissertation is accepted for commencement of the degree of Doctor of
Philosophy in Chemistry on June 30th, 2016 by Council of Institute of
Chemistry, University of Tartu

Supervisors: Toonika Rinke, PhD
Institute of Chemistry, University of Tartu, Estonia

Opponent: Assos. Prof. Elena Suchkova (Dr)
ITMO University, St. Petersburg, Russia

Commencement: August 23rd, 2016, 10.00
Ravila Street 14a, Tartu (Chemicum), auditorium 1021



European Union
Regional Development Fund



Investing in your future

ISSN 1406-0299
ISBN 978-9949-77-193-6 (print)
ISBN 978-9949-77-194-3 (pdf)

Copyright: Margarita Kagan, 2016

University of Tartu Press
www.tyk.ee

TABLE OF CONTENTS

LIST OF ORIGINAL PUBLICATIONS	6
ABBREVIATIONS AND SYMBOLS	7
INTRODUCTION.....	8
1. LITERATURE OVERVIEW	9
1.1. The use of antibiotics in dairy farming.....	9
1.2. Methods for the detection of antibiotics in milk.....	9
1.3. Biosensors for the detection of antibiotic residues in milk.....	10
1.4. Problems with practical biosensing of antibiotic residues.....	13
1.5. Data acquisition for obtaining rapid results.....	13
2. EXPERIMENTAL	14
2.1. Dual-optrode biosensor system and flow cell.....	14
2.2. Immobilisation of glucose oxidase and preparation of glucose bio-optrode.....	14
2.3. Measurement procedures and data acquisition	15
2.3.1. Measurements in flows	15
2.3.2. Assessment of enzyme activity in glass cell.....	15
2.4. Milk samples	16
3. RESULTS AND DISCUSSION	17
3.1. Modulation of the catalytic properties of glucose oxidase	17
3.1.1. Enhanced detection of glucose in cascaded lactose biosensor.....	19
3.2. Modelling the bio-optrode signal in flows	20
3.3. Fitting of the biosensor response to the model	23
3.4. Practical aspects of model application.....	24
3.5. Time required for data acquisition.....	26
3.6. Application of glucose dual-optrode biosensor for the determination of penicillins in milk.....	27
CONCLUSIONS.....	32
REFERENCES.....	33
SUMMARY IN ESTONIAN	40
ACKNOWLEDGEMENTS	42
PUBLICATIONS.....	43
CURRICULUM VITAE	121
ELULOOKIRJELDUS.....	122

LIST OF ORIGINAL PUBLICATIONS

The present thesis consists of four original research papers and a review, which are referred in the text by Roman numerals I–V.

- I. **Kagan, M.**, Kivirand, K., Rincken, T. Modulation of enzyme catalytic properties and biosensor calibration parameters with chlorides: Studies with glucose oxidase. *Enzyme and Microbial Technology*, 2013, 53, 278–282 (DOI: 10.1016/j.enzmictec.2013.02.011.)
- II. Kivirand, K., **Kagan, M.**, Rincken T. Calibrating Biosensors in Flow-Through Set-Ups: Studies with Glucose Optrodes. Published in: *State of the Art in Biosensors – General Aspects*, 2013, 331–351, Intech (DOI: 10.5772/54127)
- III. Kivirand, K., Floren, A., **Kagan, M.**, Avarmaa, T., Rincken, T., Jaaniso, R. Analyzing the Biosensor Signal in Flows: Studies with Glucose Optrodes. *Talanta*, 2015, 131, 74–80 (DOI: 10.1016/j.talanta.2014.07.061.)
- IV. Kivirand, K., **Kagan, M.**, Rincken, T. Biosensors for the detection of antibiotic residues in milk. Published in: *Biosensors – Micro and Nanoscale Applications*, 2015, 425–456, Intech (DOI: 10.5772/60464)
- V. **Kagan, M.**, Printsman, G., Kivirand, K., Rincken T. Determination of Penicillins in Milk by a Dual Optrode Biosensor. *Analytical Letters*, 2016, in press (DOI 10.1080/00032719.2016.1202957.)

Author's contribution

Paper I: Performed all the experimental work and calculations, responsible for the interpretation of results and writing of the paper.

Paper II: Performed the experimental work and calculations.

Paper III: Performed the experimental work and calculations.

Paper IV: Responsible for writing of the paper.

Paper V: Performed all the experimental work and calculations, responsible for the interpretation of results and writing of the paper.

ABBREVIATIONS AND SYMBOLS

<i>A</i>	the total signal change parameter
<i>B</i>	the kinetic parameter
DOC	dissolved oxygen concentration
GOD	glucose oxidase (EC 1.1.3.4)
HPLC	high-performance liquid chromatography
LOD	limit of detection
MIPs	molecularly imprinted polymer sensors
MRL	maximum residue limit
MS	mass spectrometry
PB	phosphate buffer
PPB	parts per billion ($\mu\text{g/L}$)
PPM	parts per million (mg/L)
SPR	surface plasmon resonance
β -gal	β -galactosidase (EC 3.2.1.23)
<i>c</i>	dissolved oxygen concentration
<i>s</i>	substrate concentration
<i>t</i>	time
K_S	Michaelis-Menten constant for substrate
K_{O_2}	Michaelis-Menten constant for oxygen
V_{MAX}	ultimate reaction speed
k_S	substrate mass transfer rate between the flowing liquid and sensor surface
k_{O_2}	oxygen mass transfer rate between the flowing liquid and sensor surface
k_R	reaction rate ($k_R = \frac{V_{MAX}}{K_S}$)
k_{SR}	rate parameter describing the reaction and mass transfer of substrate
R^2	coefficient of determination

INTRODUCTION

Milk and dairy products, generally considered to be healthy and nutritionally balanced natural food comprise essential nutrients for all age groups and are an important part of our everyday diet. However, the use of veterinary drugs, in particular antibiotics for the treatment of food-producing animals generates the risk to human health due to the transmission of the residues and metabolites of these compounds into food chain. In addition, scientists and health experts are also concerned that wide application of antimicrobial agents is contributing to the rise and spread of antibiotic-resistant bacteria. Penicillins, which belong to the group of β -lactam antibiotics, are bactericidal antibiotics and act by disrupting peptidoglycan synthesis in actively multiplying bacteria. Although penicillins have several clinical limitations, as instability in the presence of gastric acids and ineffectiveness against many Gram-negative bacteria, they are still considered to be the best antibiotics to use against most Gram-positive organisms. At present, strict regulations have been established for the levels of antibiotic residues and metabolites in food of animal origin.

Antibiotic residues in food are commonly determined chromatographically and with the help of special tests. The application of biosensors for the detection of antibiotic residues is a good alternative to traditional methods. The benefits of biosensors are their low cost, simplicity and possibility for rapid real-time analysis. Nowadays, the critical problems of biosensing antibiotic residues are the reliability of results and time required for analyses enabling automatic on-line control of production.

The main goal of the present work was to introduce a rapid method for real-time detection of penicillins' residues in milk, to propose a simple and effective model to describe the response of enzymatic bio-optrode operating in flow regime and to study the possibilities of amplifying the biosensor signal to reduce experimental noise and accelerate the acquisition of results. We used a dual-sensor system consisting of glucose and reference oxygen optrodes, enabling to eliminate the fluctuations in the initial dissolved oxygen concentration, temperature and fluidic flow as a robust standard system for model development. The modulation of the catalytic properties of glucose oxidase with different metal cations was studied to amplify the characteristic calibration parameters of glucose and cascaded lactose biosensors based on glucose oxidation in order to accelerate the rate and improve the quality of milk analysis. The effect of sample flow rate on different biosensor calibration parameters, calculated from the biosensor transient phase signal, was also studied. Finally, the dual optrode glucose biosensing system was used for the determination of the effect of penicillins on the biosensor signal in milk and the assessment of substandard milk, collected from cows undergoing treatment with penicillin antibiotics.

1. LITERATURE OVERVIEW

1.1. The use of antibiotics in dairy farming

The use of antibiotics in dairy farming includes not only the treatment of various inflammatory processes, but also the prophylaxis and addition of sub-therapeutic doses into feed to promote growth and improve production efficiency in some countries [1–3]. The occurrence of antibiotic residues in milk can lead to health problems in humans and risks of developing microbial resistance [2]. In addition, the presence of antibiotics in milk impairs fermentation processes during cheese and yoghurt production [4].

The overall sales of veterinary antibiotics, used in food-producing animals, including dairy farming, were 8 122 tonnes in EU and 13 600 tonnes in U.S., whereas in Estonia veterinary antibiotics sales number was 8.7 tonnes as of pure ingredients in 2013 [5,6]. The highest proportion of the sales constituted penicillins, which belong to the group of β -lactams; and tetracyclines; whereby the use of the first is prevailing in Nordic countries [5–8].

Due to their lipophilic properties, penicillins accumulate in milk. Taking into account the widespread consumption of milk and the high potential of accumulation of antibiotic residues in it, milk is one of the most heavily regulated food products [9]. In EU, the Maximum Residue Limits (MRLs), which are not to be exceeded in milk, are set to 4 $\mu\text{g/L}$ (ppb) for benzylpenicillin, amoxicillin and ampicillin and 30 $\mu\text{g/L}$ (ppb) for cloxacillin [10].

Since the introduction of EU regulations on MRLs of pharmacologically active substances in foodstuff of animal origin (Commission Regulation 37/2010), it has been clear that the concept of regulating MRL values in foods can be implemented successfully only if methods for quantification of these substances are available for on-site use for rapid monitoring and testing of production [10].

1.2. Methods for the detection of antibiotics in milk

At present, there are two major methods applied for the assessment of antibiotic residues in milk: various chromatography-based techniques and qualitative milk screening tests [11–14].

High-performance liquid chromatography in combination with mass spectrometry (HPLC/MS) is considered to be the most reliable technique for quantitative detection of antibiotic residues [11,14], and more than 80% of the analyses of veterinary drugs are carried out using this technique [14]. The detection limits for penicillins in milk with HPLC/MS are usually well below 1 ppb [14,15]. However, chromatography based methods require expensive equipment and trained personnel and therefore do not enable to discover the antibiotic residues in milk in farm, prior to the contamination of subsequent food chain with polluted milk. In addition, HPLC techniques demand laborious

pre-treatment of samples like extraction of the analyte from sample matrix and derivatization [11,14]. β -lactams can also degrade if methanol and/or 0.1% formic acid are present in the extraction solvent [15].

Qualitative microbial inhibition tests comprise spores of specific bacteria, sensitive to particular antibiotics on agar gel including nutrients for bacterial growth and a pH indicator. These commercial tests include Delvotest, BetaStar Plus, Charm Farm Test, Eclipse test, Arla test, Copan test, Disc assay, Diffusion test, Valio 101 test, etc [12,14–15]. The main advantages of these tests are their low cost, simple performance, and broad selection towards different antibiotics, e.g. Diffusion test and Delvotest for the determination of β -lactams, Lumac test for the determination of penicillins, Charm Farm Test for the determination of aminoglycosides and tetracyclines [12]. As a rule, the detection limits of these tests for specific compounds are in the range of the established MRL values [11,12,15,16]. Although microbial inhibition tests are considered to be rapid, they take 3 to 24 hours to perform in an incubator [12]. Another problem is that the bacterial strains (*Streptococcus thermophilus*, *Bacillus subtilis*, *Bacillus stearothermophilus* var. *calidolactis*, *Sarcina lutea*, *Escherichia coli*) used in tests should be constantly monitored to ensure that they have not become resistant to the analyzed antibiotics. The interpretation of test results is quite subjective and may lead to false negative or positive results. The presence of natural inhibitors in abnormal milk (e.g. milk of mastitic cows or colostrum) can be the cause of false positive results [11–13]. In addition to microbial inhibition tests; there are different rapid tests, based either on immunoassay or enzymatic operation, available for screening of a number of antibiotic residues in milk [15,17]. These tests can provide preliminary results within 15 minutes, although the reliability of these tests is not very high as several components in mastitic milk (e.g. somatic cells, lactoferrin, lysozyme, microbes, and free fatty acids) may have a major impact on the outcome of the test and cause elevated false non-compliant/compliant results [15,18].

In spite of detection limits in the range of established MRL values, none of the abovementioned technologies are suitable for on-line analytical arrangements.

1.3. Biosensors for the detection of antibiotic residues in milk

The application of biosensors for milk analyses is a good alternative to traditional methods, as biosensors enable the development of equipment for real-time analysis in complex matrixes, operating in fully automatic or manual mode. Biosensors are compact devices transferring selective biochemical recognition into a measurable physical signal. This signal can be translated into an indicator of the safety or quality of milk. Due to the large number of different principles used, biosensors can be classified according to the bio-recognition or signal transduction technologies employed [19].

The most common biosensors, developed for the detection of antibiotic residues in milk are immunosensors, based on immunochemical biorecognition reactions and electrochemical and optical signal transduction, the latter most often being a Surface Plasmon Resonance (SPR) biosensor. The application of SPR technology secures low detection limits even below the established MRL values [20–22]. The main drawbacks of SPR biosensors are high cost and time, required for the preparation of specific biorecognition chips and system regeneration [21]. Detection limits of the majority of current immunosensors [IV], which are, designed for the determination of β -lactam antibiotic residues, vary in a broad range: from 10^{-6} ppb to 14.6 ppb [22–30]; and the detection limits are in the similar range for other antibiotics [31,32]. Although immunosensors are very selective, the speed of analysis depends on the incubation time required to form antigen/antibody complex, which can be several hours [26,33].

The second most common group of biosensors is receptor or enzyme-based biosensors, where specific receptors or enzymes interact with the antibiotic molecules and the substrates or products of the bio-recognition reaction are determined directly with a suitable transducer [IV]. These biosensors have been designed for the determination of β -lactam residues with the limit of detection (LOD) ranging from 4×10^{-8} ppb to 9×10^3 ppb [21,34–46]. Receptor or enzyme-based biosensors like immunosensors usually employ optical (mainly SPR) or electrochemical signal detection principles [11,21,34,37,47].

There are a few biosensors for detecting antibiotic residues in milk based on the application of enzymatic activity of microorganisms [48–50]. These microbial biosensors are based on the measurement of the inhibition of bacterial growth due to the presence of antibiotics [11–14]. For instance, systems for the monitoring of β -lactams are based on similar principles as microbiological inhibition tests for milk [12,14] with the difference that the bio-recognition reaction signal is detected quantitatively or semi-quantitatively. Detection limits in both cases are at the MRLs levels [48].

During last years aptamer-based biosensors have been proposed for the detection of antibiotic residues in milk [51–55]. Aptamers are oligonucleotide or peptide molecules that bind to a specific target molecule. Specific three-dimensional aptamers, fold into well-defined structures, are produced using Systematic Evolution of Ligands by EXponential enrichment (SELEX) method [56,57]. Aptamers are quite stable and are not affected by reasonable temperature or pH fluctuations, at optimal conditions they can restore their original conformation. Aptamers are smaller in size compared to antibodies enabling to reach previously blocked or intracellular targets [58]. The detection limits of common aptasensors [IV] are varying in the range of 3.5×10^{-2} ppb to 350 ppb for the detection of β -lactam residues [53]. A serious disadvantage using aptamer-based biosensors for milk analyses is the presence of milk proteins and fat; and the non-transparency of the samples, which hamper the application of optical detection methods. Pre-treatment of milk samples is commonly required for the analyses with aptamer-based biosensors [54,55,59–64].

A recent development in the biosensing of antibiotic residues in milk is the application of molecularly imprinted polymer sensors (MIPs) for biorecognition [65–67]. Molecular imprinting is a technique for the creation of synthetic materials containing specific receptor sites having high affinity towards the target molecule [68]. MIPs are effective alternatives to the natural biorecognition compounds in biosensor assays. Unfortunately, so far there are no MIPs for the determination of β -lactam residues. Current MIP sensors have been mostly designed for the detection of aminoglycosides [IV]. These sensors are very sensitive with LOD varying in the range from ≤ 1 ppb to 6 ppb [66,69], which is far below of the allowed MRL values, so dilution of samples is required for their practical applications.

A condensed overview of currently available different biosensor platforms, used for the detection of β -lactam antibiotic residues in milk, is given in Table 1.

Table 1. Currently available biosensor platforms for the detection of β -lactam antibiotic residues in milk.

Biosensing principle	Detection range, ppb	Advantages	Disadvantages	Ref.
Immuno-sensors	10^{-6} –14.6	<ul style="list-style-type: none"> • High selectivity 	<ul style="list-style-type: none"> • High cost • Time consuming biosensor production • Slow regeneration 	[22–30]
Receptor or enzyme-based biosensors	4×10^{-8} – 9×10^3	<ul style="list-style-type: none"> • Low LOD 	<ul style="list-style-type: none"> • High cost • Possible non-specific binding • Long time required for analyses 	[21,34–46]
Microbial biosensors	At MRL levels	<ul style="list-style-type: none"> • Similar to microbiological tests 	<ul style="list-style-type: none"> • Low sensitivity • Semi-quantitative detection • Time of analysis over 120 min 	[48–50]
Aptamer-based biosensors	3.5×10^{-2} –350	<ul style="list-style-type: none"> • High affinity • Stable • Enabling to reach intracellular targets 	<ul style="list-style-type: none"> • Application of optical detection methods is problematic (non-transparency of the samples) • Pre-treatment of the samples is required 	[51–55]

1.4. Problems with practical biosensing of antibiotic residues

Concerning the practical application of biosensors, there are several problems to be solved. One of the major problems is time required to get reliable results, especially in case of on-site analyses. The average detection time (excl. pre-treatment) is usually 30–40 minutes or even up to 2 hours if a longer incubation period for bio-recognition is required [29,37,70]. Moreover, some complex biosensing systems require additional pre-treatment of milk samples to remove fat and proteins [54,55,60,62].

The other drawback is that most antibiotics' biosensors have been used for the “proof of concept” and the validation of the proposed technology has been carried out with only spiked milk samples. However, studies using real milk of animals undergoing antibiotic treatment are scarce, although this can be a key factor to indicate the applicability of biosensor technology, as “natural” samples can additionally contain different metabolites of antibiotic compounds, which have a major effect on the measured biosensor signal [15].

1.5. Data acquisition for obtaining rapid results

The crucial assignment of on-line measurements is to obtain reliable results as quickly as possible, which requires exact modelling of the processes taking place in the system and smart management of data. Commonly the only information used in obtaining results with biosensing systems, is the steady state output (or the presumed 95% of it) [71]. The main problems with measuring the experimental steady state signal is time, required to reach this state and the imprecision of estimating the attainment of steady state [71–73]. Therefore, for real-time measurements it is unavoidable to develop methods for the determination of the characteristic parameters of the biorecognition reaction from early pre-steady state signal.

Carrying out measurements in flow systems enables further reduction of analysis time allowing high sample throughput and the possibility to work with small volumes of analytes [72,74,75]. Flow arrangements present a wide response range and high sensitivity, but measurements in continuous flows require consideration of the flowing effects, both laminar and turbulent, in the biosensor output signal. Most modelling efforts dealing with biosensor performance in flow regime are made for amperometric signal transducers [76–81]. There is only very few information about detailed signal analyses of optical biosensors, which are working in continuous-flow or flow-through systems. For SPR biosensors, calculation of the two-compartment model had been used in order to determine accurate values of the rate constants and transport coefficients for data that are influenced by flow and diffusion [82]. In comparison with amperometric biosensors, optical biosensors have several advantages as they are resistant to electrical and electrochemical interferences, allow non-contact sensing or transmission of parallel sensor signals over optical fibres, and have relatively long service interval [83].

2. EXPERIMENTAL

2.1. Dual-optrode biosensor system and flow cell

The system comprises of flow cell, heater, opto-electronic unit, control unit and two oxygen optrodes, one of which is covered with biorecognition layer to form a biooptrode and the other forms a reference optrode [III]. The optrodes (30 mm long optical quartz fibres with diameter of 1 mm, dip-coated with oxygen-sensitive Pd-tetraphenylporphyrine-containing polymethylmethacrylate film) were placed into identical isolated flow channels ($l=50$ mm; $\varnothing=3$ mm) of the carefully thermostated at 37.0 ± 0.1 °C flow cell. To minimize the accidental forming of microbubbles in flow channels, the inflow was in the bottom and the outflow in the upper part of the cell (Fig. 1).

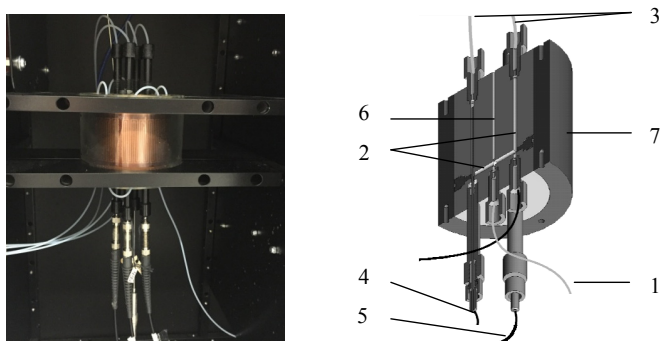


Figure 1. The dual-optrode biosensor system set up: 1–sample inflow; 2–flow channels; 3–outflows; 4–glucose bio-optrode; 5–reference oxygen optrode; 6–temperature sensor; 7–cylindrical stainless steel flow cell for the stabilization of temperature.

The opto-electronic unit provided optical excitation ($\lambda=405$ nm) as well as the detection and amplification of luminescence signals ($\lambda= 690$ nm). The control unit was connected to personal computer via USB interface and included analog-to-digital signal converter, input/output ports for switching the light-emitting diodes for luminescence excitation, and heater regulator.

2.2. Immobilisation of glucose oxidase and preparation of glucose bio-optrode

The glucose bio-optrode was produced by coiling 19 cm of nylon-6,6 thread with covalently immobilized glucose oxidase (GOD, EC1.1.3.4) [III] around the oxygen-sensitive surface of the oxygen optrode, where it formed a biorecognition layer for glucose [84–86]. The initial catalytic activity of the thread was 0.016 U/cm and this was tested before each series of measurements. If the

activity dropped below critical (80% of its initial value) during measurements [III], the GOD-containing thread was replaced. The reference oxygen optrode was covered with 19 cm of identical “blank” thread to eliminate diffusion effects.

2.3. Measurement procedures and data acquisition

2.3.1. Measurements in flows

All kinetic studies were carried out in air-saturated solutions at 37 °C varying the flow rate from 0.8 mL/min to 13.0 mL/min for model development [III] and using an optimal flow rate 3.3 mL/min for the studies with milk samples [V].

The output signals of optrodes were recorded with the interval of 1 second. Original software Oxysens 2.0 was developed for the automatic data acquisition and calculation of the dissolved oxygen concentration (DOC) using Stern-Volmer relationship; but also for the automatic control of the system's working parameters. The change of oxygen concentration due to glucose oxidation, catalyzed by glucose oxidase, was calculated as the DOC difference between glucose bio-optrode and reference optrode at every time moment measured, so minimizing the impact of experimental noise; and normalized to bring the data from different sensors onto common scale. Each experimental result was an average of at least 3 identical measurements and consisted of at least 300 data points. After each measurement the system was washed with 0.1 mol/L phosphate buffer (PB, pH 6.50) until the sensors' signals reached their initial values.

2.3.2. Assessment of enzyme activity in glass cell

The kinetic measurements for the assessment of modulating and inhibiting effects of different compounds on enzyme activity were performed in an airtight temperature regulated glass cell at constant stirring with an oxygen optrode [I,V]. The oxygen-sensitive film of the optrode was additionally covered with a thin black silicone coating to eliminate the effect of divergent light.

The oxygen optrode was plunged into air-saturated reaction medium, containing substrate or a definite amount of enzyme. The reaction was initiated by injecting soluble enzyme or substrate, initiating the decrease of DOC.

The reduction of DOC in the course of the biorecognition reaction was characterized using 2 independent parameters: the total signal change parameter (*A*) and the kinetic parameter (*B*), calculated from the biosensor transient signal using a modified dynamic biosensor model [87].

The activity of soluble β -galactosidase (β -gal, EC3.2.1.23) was determined also spectrophotometrically, following the formation of optically active product of the hydrolysis of glucoside bond in o-nitrophenol- β -D-galactoside [88].

2.4. Milk samples

Milk samples were collected in the Dairy Research Farm of the Estonian University of Life Sciences in Southern Estonia. The collected milk samples were kept under moderate stirring at room temperature. To prepare milk samples spiked with benzylpenicillin, this antibiotic was added to the milk of healthy cows.

The milk samples from two cows undergoing mastitis treatment with penicillin antibiotics (Norbrook® Lactaclox intramammary infusion, a single dose containing 75 mg of ampicillin and 200 mg of cloxacillin; or Bimoxyl intramuscular injections, a single dose containing 150 mg of amoxicillin per 10 kg animal bodyweight) were immediately frozen at $-20\text{ }^{\circ}\text{C}$ after collection and melted at $+4\text{ }^{\circ}\text{C}$ before testing. The treatment of cows with antibiotics was administered for 3 days followed by a 3-day withdrawal period.

Before injection into the flow cell, milk samples (5 mL) were diluted (1:4) with 0.1 mol/L PB (pH 6.50; 0.01% Tween 20) and aerated with air for 5 minutes at $37\text{ }^{\circ}\text{C}$.

3. RESULTS AND DISCUSSION

3.1. Modulation of the catalytic properties of glucose oxidase

First we studied the possibilities of modulating the glucose oxidase catalytic properties with metal cations: Na^+ , Mg^{2+} and Al^{3+} [1]. The enzymatic oxidation of glucose was characterized using two different signal parameters, calculated from the transient phase data of the reaction: total signal change parameter and kinetic parameter [89]. The values of these reaction parameters at different concentrations of different chlorides are shown on Figure 2 [1]. NaCl at concentrations below 0.5 mol/L increased the value of the total signal change parameter from its initial value of 0.82 in salt-free solutions to its limiting maximum value 1.00 (Fig. 2(A1)). Magnesium chloride (MgCl_2) caused a 1.3-fold essential increase of the total signal change parameter in concentration range from 0.1 to 0.4 mol/L. At lower concentrations, the value of parameter A was slightly reduced, and at concentrations above 0.4 mol/L, parameter A maintained its maximum value (Fig. 2(A2)). At MgCl_2 concentrations greater than 1 mol/L, the glucose oxidation reaction was slow; thus, although the maximum value for the signal change parameter was observed (meaning that at the reaction steady state DOC equals zero), the experimental determination and interpretation of steady state was problematic.

In the presence of aluminium chloride (AlCl_3) the total signal change parameter was decreased (Fig. 2(A3)).

As for the practical applications of biosensors, the slope and linear range of the calibration curves, based on biosensor signal parameters, determine the quality of the results – the amplification of the measured values of these parameters enables to increase the accuracy and sensitivity of the analysis. The modulation of the GOD-based biosensor signal parameters with NaCl and MgCl_2 at concentrations below 0.5 mol/L increased the calculated total signal change parameter and the slope of the calibration curve by nearly 20% compared to its initial value. At the same time, the kinetic parameter showed decrease in the presence of all three salts (Fig. 2(B1,B2,B3)), so it is not possible to amplify the modulation of this parameter in order to get rapid results with metal cations.

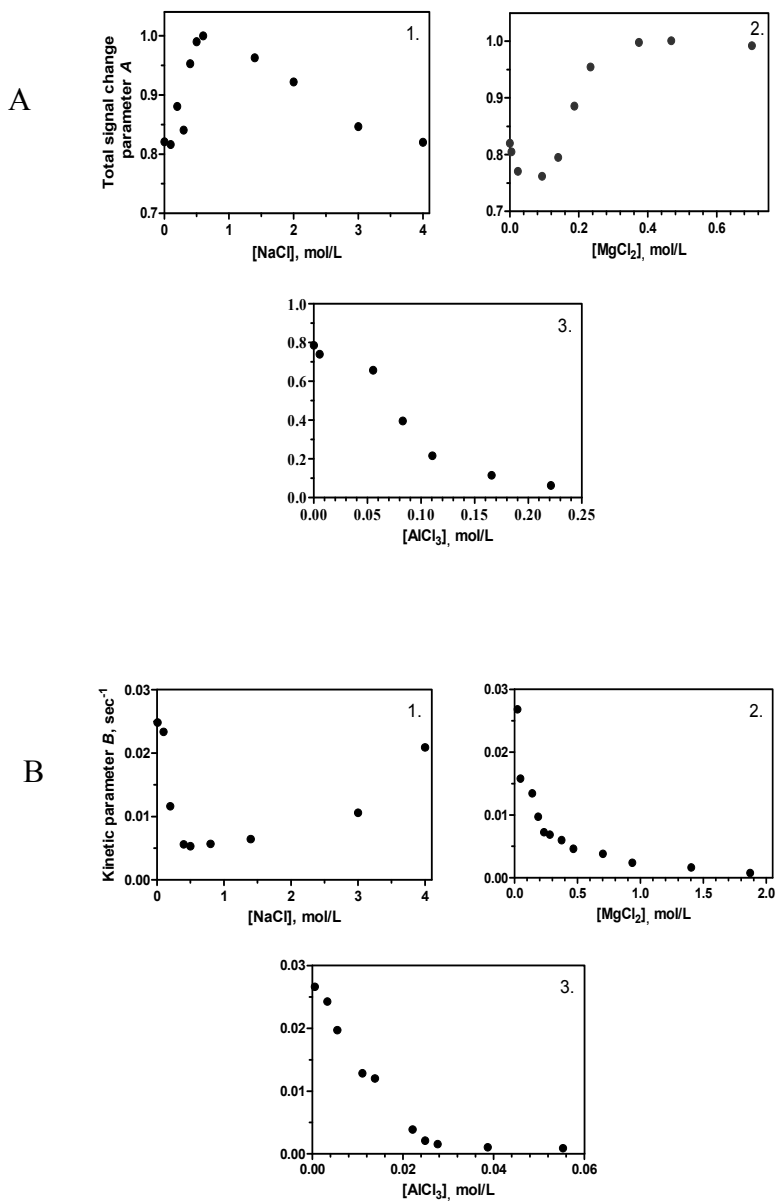


Figure 2. The dependence of biosensor signal parameters on the concentrations of different chlorides. (A) Total signal change parameter; (B) kinetic parameter. All measurements were carried out in air-saturated 0.1 mol/L acetic buffer (pH 5.60) at 25 °C; [glucose]=3mmol/L, [glucose oxidase]=1.3 U/mL.

3.1.1. Enhanced detection of glucose in cascaded lactose biosensor

Cascaded lactose biosensors usually integrate two consecutive catalytic processes: (1) the hydrolysis of lactose into galactose and glucose, catalyzed by β -gal and (2) the successive oxidation of the produced glucose, catalyzed by GOD [90]. These cascaded biosensors are commonly not applicable for quick analyses due to the relatively low speed of lactose hydrolysis [91]. However, it might be possible to detect smaller quantities of the produced glucose and obtain faster results if the sensitivity of glucose measurements is increased [1].

NaCl caused a similar modulation of the total signal change parameter in lactose cascaded biosensor as in glucose biosensor and as expected, this parameter increased for 20% compared to its initial value. $MgCl_2$ increased values of both parameters A and B , as Mg^{2+} is supposed to activate also β -gal [92,93]. Reaction parameters A and B for the detection of lactose were increased by 1.2 and 1.5 times, respectively, at $MgCl_2$ concentrations below 5 mmol/L (Fig. 3).


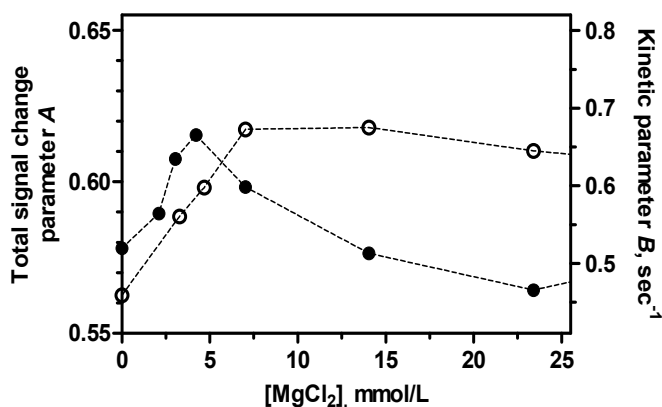


Figure 3. Lactose biosensor signal parameters at different $MgCl_2$ concentrations (● Total signal change parameter A ; ○ Kinetic parameter B). All measurements were carried out in air-saturated 0.1 mol/L phosphate buffer (pH 6,50) at 25 °C; [lactose]=0.14 mol/L, [β -galactosidase]=10.08 U/ml, [glucose oxidase]=1.3 U/ml.

The addition of 5 mmol/L $MgCl_2$ was optimal to achieve the highest amplification of the lactose biosensor calibration parameters, hence could be used for the acceleration of lactose analyses. The amplification of the signal parameters is vital for analyses conducted at low temperatures, like in cooled milk, where lactose hydrolysis and glucose production are slow.

3.2. Modelling the bio-optrode signal in flows

In order to develop a model, which enables to calculate relevant parameters of the bio-recognition reaction in flows from the pre-steady state biosensor signal and reduce the effect of side processes, we studied the oxidation of glucose by dissolved oxygen, catalyzed by glucose oxidase as a model reaction:



In flow cells, there are two general processes governing oxygen concentration at optrode surface:

- 1) enzyme-catalyzed reaction in the enzyme containing layer;
- 2) transport of oxygen and the second substrate into and in the flow cell.

The studied reaction (1) is of ping-pong type [94] and can be described in the quasi-steady state approximation as following:

$$\frac{ds(t)}{dt} = \frac{dc(t)}{dt} = -\frac{V_{MAX}}{1 + \frac{K_S}{s(t)} + \frac{K_{O_2}}{c(t)}}, \quad (2)$$

where $s(t)$ is the substrate concentration and $c(t)$ is DOC at time moment t ; K_S and K_{O_2} are Michaelis' constants for substrate and oxygen, respectively; and V_{MAX} is the ultimate reaction speed.

If the following condition is fulfilled:

$$\frac{K_S}{s} \gg 1 + \frac{K_{O_2}}{c}, \quad (3)$$

Eq. (2) can be simplified to:

$$\frac{ds(t)}{dt} = \frac{dc(t)}{dt} = -k_R s(t), \quad (4)$$

where

$$k_R = \frac{V_{MAX}}{K_S}. \quad (5)$$

For the reaction of glucose oxidation $K_S \gg K_{O_2}$ [94], and therefore condition (3) is fulfilled in a quite wide range of glucose and oxygen concentrations. The upper limit of oxygen concentration in water solutions is generally determined by its saturation value ($c_0 \sim 0.2\text{--}0.3$ mmol/L at temperatures 20–40 °C) and the reaction is described by first order kinetics (4).

Regarding the transport processes, the addition of substrate and oxygen into the vicinity of sensor surface is described with linear kinetic terms. Then the overall process can be modelled by two kinetic equations:

$$\frac{ds(t)}{dt} = -k_R s(t) + k_S [s_0 F(t) - s(t)] \quad (6)$$

$$\frac{dc(t)}{dt} = -k_R s(t) + k_{O_2} [c_0 - c(t)] \quad (7)$$

The rate constants k_S and k_{O_2} characterise the exchange speed of the concentrations of substrate and oxygen, respectively, between the flowing liquid and sensor surface (Fig. 4).

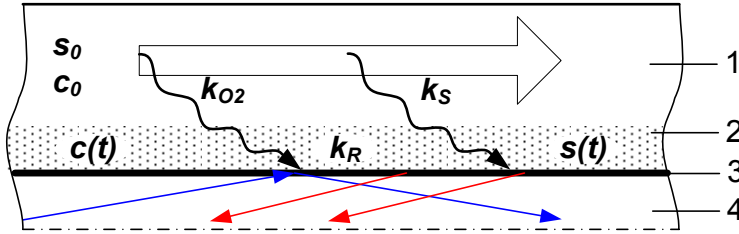


Figure 4. Cross-section of the flow cell and scheme of model processes. 1–flowing liquid; 2–flossy coating containing immobilized enzyme molecules; 3–oxygen sensitive coating; 4–core of optical fibre. The arrows inside the fibre represent the light involved in optical oxygen sensing.

Assuming that the oxygen concentration in the flowing liquid entering the cell is always c_0 , and after passing the initial front, the substrate carried by liquid flow has constant concentration s_0 . The function $F(t)$ describes the arrival front of the substrate into the cell. When the passage of the front is fast compared to the reaction and transport processes, then $F(t)$ can be approximated by Heaviside function:

$$F(t) = H(t) = \begin{cases} 0, & t < 0 \\ 1, & t \geq 0 \end{cases} \quad (8)$$

It is also assumed that there is no substrate present in the cell before $t=0$. Under these conditions the solutions of equations (6) and (7) are:

$$s(t) = s_0 k_S \int_0^t dt' \exp[(k_R + k_S)(t' - t)], \quad (9)$$

$$c(t) = c_0 - k_R \int_0^t dt' s(t') \exp[k_{O_2}(t' - t)]. \quad (10)$$

After inserting Eq. (9) into (10) and evaluating the integrals:

$$c(t) = c_0 - s_0 \frac{k_R k_S}{k_{SR} k_{O_2}} \left\{ 1 - \exp(-k_{O_2} t) + \frac{k_{O_2}}{k_{O_2} - k_{SR}} [1 - \exp(-k_{SR} t)] \right\}, \quad (11)$$

where

$$k_{SR} = k_S + k_R. \quad (12)$$

The stationary solution for DOC is:

$$c_f = \lim_{t \rightarrow \infty} c(t) = c_0 - s_0 \frac{k_R k_S}{k_{SR} k_{O_2}} \quad (13)$$

The Eq. (11) can be rewritten in a following form:

$$\frac{c(t)}{c_0} = 1 - A \cdot f(t), \quad (14)$$

where

$$f(t) = 1 - \frac{k_{SR}}{k_{SR} - k_{O_2}} \exp(-k_{O_2} t) + \frac{k_{O_2}}{k_{SR} - k_{O_2}} \exp(-k_{SR} t) \quad (15)$$

is the normalised function describing the temporal evolution of relative DOC. It is a monotonic function changing from zero to unity, i.e. $f(0) = 0$ and $\lim_{t \rightarrow \infty} f(t) = 1$.

Parameter A gives the relative difference between the initial (c_0) and final stationary (c_f) oxygen concentrations and can be easily determined experimentally as a normalized change of DOC between the initial and final steady states:

$$A = \frac{c_0 - c_f}{c_0} = \frac{s_0 k_R k_S}{c_0 (k_S + k_R) k_{O_2}}. \quad (16)$$

3.3. Fitting of the biosensor response to the model

Several series of glucose dual optrode responses were recorded at different glucose concentrations at flow rate 2.7 mL/min in order to compare the biosensor output response with the model [II, III]. Biosensor response at 5 different glucose concentrations (in duplicate) and recovery curves are shown in Figure 5. The arrows mark the time moments, when the substrate was added. The duration of substrate injection was 300 seconds and thereafter the signal was restored in the flow of pure buffer solution to the initial level.

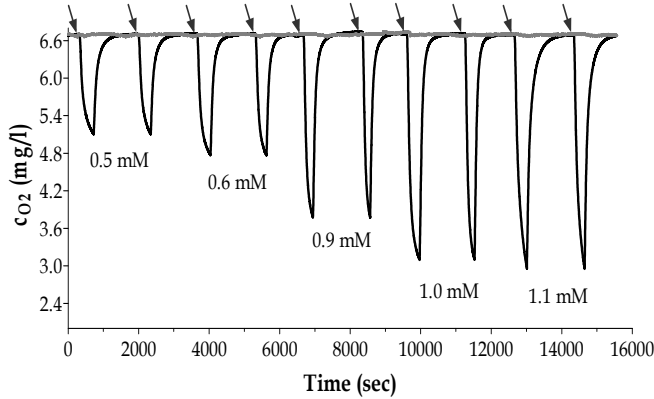


Figure 5. Response curves of glucose bio-optrode (black line) and the reference optrode (gray line) of consecutive measurements at different glucose concentrations (two at each concentration). Measurements were carried out at 37 °C in 0.1 mol/L phosphate buffer (pH 6.50) at flow rate 2.7 mL/min. Arrows indicate the time of adding the substrate solution.

The response of the reference sensor at constant saturated DOC was not dependent on glucose concentration. Its signal fluctuations did not exceed 1% of the working range of the sensor at any measured glucose concentration. The response of the glucose biosensor decreased due to consumption of oxygen

according to reaction (1). In order to eliminate all potential experimental noise, the difference between the signals of the reference and glucose sensor responses was used to determine the normalized output of the system.

Normalized response curves at four different glucose concentrations together with the model curves obtained by fitting with equations (14), (15) are shown in Figure 6.

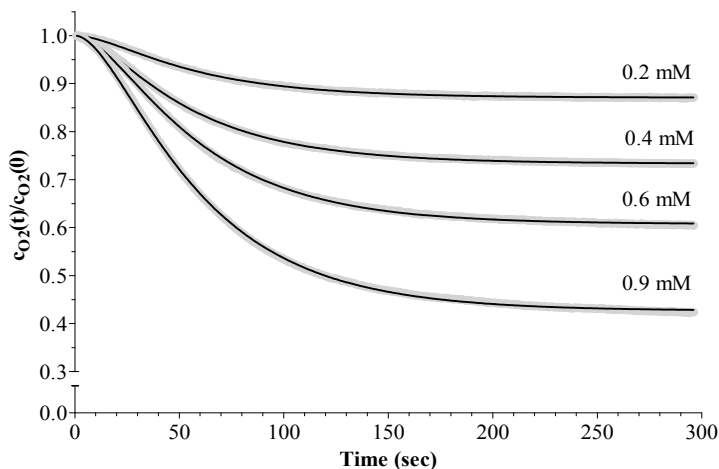


Figure 6. Fitting the experimental curves (gray) obtained at different glucose concentrations (0.2 mmol/L (mM); 0.4 mmol/L; 0.6 mmol/L; 0.9 mmol/L) with the proposed model. Theoretical approximations are shown as solid black lines. Measurements were carried out at 37 °C in 0.1 mol/L phosphate buffer (pH 6.50) at flow rate 2.7 mL/min.

Parameter A and two rate constants, k_{O_2} and k_{SR} , were determined for each curve. The application of the model for the characterization of the biosensor output signal resulted in good correlation (coefficient of determination–99%, standard deviations from the model–0.00077, $P < 0.0001$). The relatively slow signal decrease at the beginning of the response curves (Fig. 6) is caused by the lack of substrate in the enzyme-containing layer at the initial moment, what is accurately described by the model. The fitting of temporal response curves, as demonstrated in Fig. 6, provides not only more accurate way of determining parameter A , but also valuable information included in rate constants.

3.4. Practical aspects of model application

The important aspects of practical applications of biosensors are: i) the time required for the acquisition of the results – it should be as short as possible; ii) the repeatability of the experimental measurements; iii) quick regeneration of

bio-sensing system, what is of most importance in real-time analysis; and iv) operational stability and sensitivity of the biosensor system.

In continuous-flow biosensor set-ups the choice of optimal flow rate is an additional presumption of accurate and reliable results. The dependence of parameter A on flow rate at different glucose concentrations was studied in the range of flow rate varying from 0.8 to 13.0 mL/min (or 0.3–5.1 cm/sec) [II,III]. It was not possible to carry out experimental measurements at flow rates under 0.8 mL/min due to the accumulation of air bubbles in the flow cell. The value of parameter A was practically independent on the flow rate in the studied range of glucose concentrations (0.2 to 1.5 mmol/L), and was also indifferent towards the determination of time, at which the analyte front reaches the biosensor, as it is defined as a biosensor total signal change in steady state conditions ($t \rightarrow \infty$) [II,III]. This allows constructing the universal glucose calibration curves, not dependent on the flow rate in the system. The results obtained at a medium flow rate of 2.7 mL/min were used as examples of calibration parameters, as this flow rate offered acceptable response time and sufficient sensitivity [III].

The repeatability of the experimental measurements was studied at glucose concentration of 0.5 mmol/L (15 experiments per day and four days in a row) [II]. Repeatability of the measurements was very good considering that the standard deviation was 0.0051 and the coefficient of determination was 98%. The results showed that the biosensor exhibited a fairly analytical feature of repeatability [II].

Regeneration of bio-sensing continuous-flow system involves passing a background flow of fluid without reactive components through the flowing system. This was controlled by varying the flow rate between 0.8 to 13.0 mL/min. As expected, the washing of the flow system depended on the flow rate and slightly on the substrate concentration [II]. At lower flow rates (0.8 to 2.1 mL/min) the regeneration time of the system increased with the increase of the flow rate and substrate concentration. At higher flow rates the regeneration time did not depend on the substrate concentration and flow rate (because of the diffusion in the flow channels) any more [II]. The rate for GOD-based biosensor system regeneration should be at least 2.1 mL/min. At this flow rate the washing time is approximately 4.5–5 min.

The loss of sensitivity under operational conditions is one of the most serious limits of the practical utility of biosensors. Besides leaching of the bio-selective material, it can be ascribed to inactivation and denaturation of the bioactive compound. The operational stability of the present biosensor system was assessed by a continuous long-term experiment, in which a 0.5 mmol/L glucose solution was repeatedly analyzed [II]. The biosensor system was in everyday exploitation – used for about 15 measurements per day – after what it was washed with 0.1 mol/L PB (pH 6.50) and left overnight at 37°C. The initial activity of the sensor dropped for approximately 20% during the first 3 days; afterwards the biosensor response remained constant for over 35 days operation period with no significant loss of activity [II].

In addition, the actual design of the continuous-flow biosensor enables to prolong the effective lifetime of optrodes. For example, if the enzyme activity and accordingly the reaction rate decreases by 20%, the sensitivity and equally the slope of the calibration curve change just by 1%. Furthermore, the system sensitivity does not drop below 90% of the initial one even in case 30% of the initial enzymatic activity remaining [III].

3.5. Time required for data acquisition

The proposed biosensor model describes the sensor responses adequately and allows clear interpretation of underlying processes and relatively easy biosensor calibration from pre-steady state data.

The temporal responses (shown in Fig. 7) were fitted within different time intervals (the curves were fitted between $t=0$ and $t=t_F$, whereas t_F was varied from 300 sec to a minimal value of ~ 20 sec) [III]. This allowed simulating the situation, where the sensor output value is determined from shorter and shorter measurements. The results for parameter A , determined at three different substrate concentrations, are presented in Figure 7.

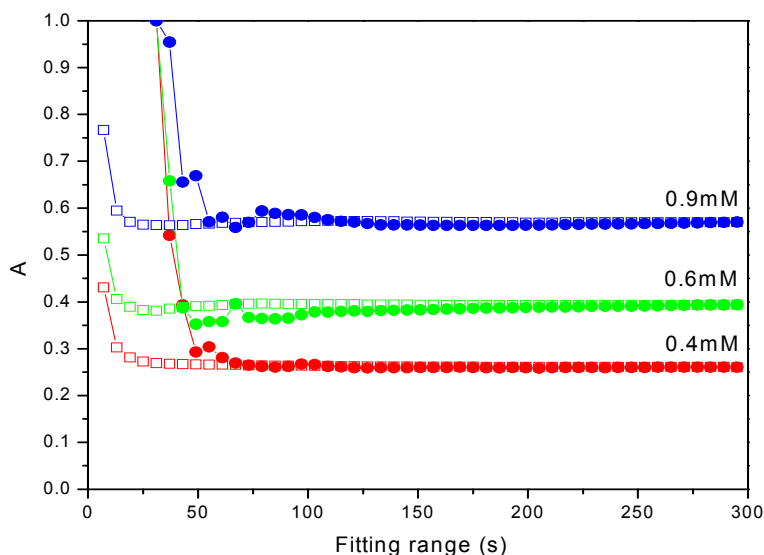


Figure 7. The dependence of the total signal change parameter A on the fitting range (measurement time). Measurements were carried out at 37 °C in 0.4 mmol/L, 0.6 mmol/L, and 0.9 mmol/L glucose solutions in 0.1 mol/L phosphate buffer (pH 6.50) at flow rate 2.7 mL/min. At fitting, all three reaction parameters (A , k_{SR} , and k_{O_2} ; filled dots) or only parameter A (open dots) was freely varied.

In all cases the value of parameter A was practically constant down to the fitting range (measurement time) $t_F \sim 60$ sec. In Figure 7, the data for two fitting procedures are presented: the filled dots present the data obtained when all parameters (A , k_{SR} , and k_{O_2}) in Eqs. (14, 15) were freely varied, whereas the empty dots present the data obtained when the pre-calibrated rate parameters were fixed and only parameter A was varied [III]. As a result, using the fixed set of pre-calibrated rate parameters, the measurement time can even be as short as 20 sec. In other words, for obtaining the value of parameter A , there is no need to record the signal up to 300 sec, but the recording time can be as short as 20 sec. These concrete time values are related to the parameters of concrete bio-optrodes and may hence vary between different systems, in particular, the optrodes with higher enzyme activity will have higher reaction rate and shorter measurement time as well. If we compare the fitting results in Figure 6 and the signal changes in Figure 7, more general criteria may be formulated. In Figure 7 we can see that the relative signal has dropped at 20 and 60 sec by $\sim 20\%$ and $\sim 50\%$, respectively. So, the substrate concentrations can be determined with relatively high accuracy by measuring the signal until it drops only by 20–50% of its maximal (steady state) change, and not waiting until the signal change has reached the 95% level of the presumed final change. This allows significant advantages in biosensor analysis speed, as the measurement time can be shortened more than by one order in magnitude.

3.6. Application of glucose dual-optrode biosensor for the determination of penicillins in milk

The main goal of the present work was to study the possibilities of rapid bio-sensing of penicillins' residues in milk and the application of the biosensor for the analyses of real milk samples of mastitic cows.

The excretion of penicillins via milk is dependent on different factors, e.g. an animal's individuality, milking interval etc., but as an average 30–40% of the total amount of penicillins applied are eliminated from the organism with milk as parent compound [15,95].

Milk is a complex colloid of fat globules within a water-based fluid that contains dissolved carbohydrates and protein aggregates with minerals [96]. The major carbohydrate in milk is lactose, which controls milk volume by maintaining its osmolarity [97]. Lactose concentration in raw bovine milk is very stable (around 140 mmol/L), exceeding the typical concentrations of glucose and galactose in milk more than 500 times [98,99]. Diet has no effect on lactose concentration in bovine milk and the regional and seasonal varieties are also very small [98]. As being a highly nutritious food, raw milk contains a diverse and complex microbiota, entering milk from contact with the animal and/or the surrounding environment [100,101]. Over 250 different bacterial species have been found in cows' raw milk [102]. The dominant microbial population in bovine milk are the lactic acid bacteria [103]. In addition, there

are also bacteria carrying the structural genes of *lac* operon, encoding the synthesis of β -gal, which is an enzyme required for the transport and metabolism of lactose and catalyzes the hydrolysis of lactose into glucose and galactose [102]. So, the amounts of soluble glucose and galactose in raw milk are dependent on the activity of β -gal. The presence of antibiotic residues in milk affects the production of β -gal by microorganisms leading to reduced glucose and galactose concentrations compared to high quality milk.

At first the effect of benzylpenicillin on the activity of β -gal was determined with amperometrical and spectrophotometrical methods [V]. It was found, that the catalytic activity of dissolved β -gal (0.1 mol/L PB; pH 6.50) did not change over a 48 hour period (Fig. 8). At the same time, the activity of β -gal decreased for 51% in 48 hours in case 3.3×10^3 ppb benzylpenicillin was added to the solution. This benzylpenicillin concentration corresponds to the average minimum concentration of benzylpenicillin in milk of dairy cows during their treatment with procaine-benzylpenicillin, although the actual concentration of benzylpenicillin residues in the milk of treated animals can be as high as 120×10^3 ppb [95]. Comparable results were obtained with both amperometrical and spectrophotometric methods [V].

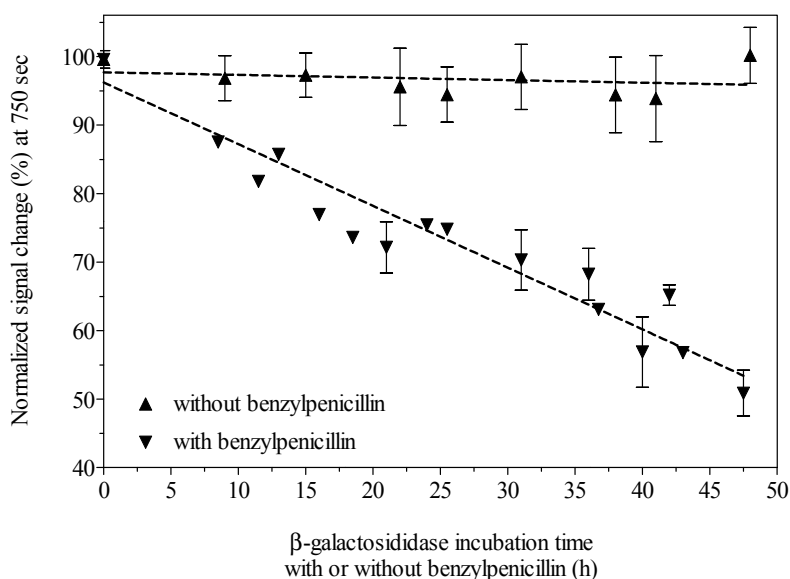


Figure 8. Inactivation of β -galactosidase during its incubation with benzylpenicillin. The measurements were carried out under constant stirring at 37 °C in 0.033 U/mL β -galactosidase solutions in 0.1 mol/L phosphate buffer (pH 6.50) with (3.3×10^3 μ g/L, ▼) or without benzylpenicillin (▲). Lactose concentration in the system was 140 mmol/L, the lactose incubation time with β -galactosidase was 480 sec and glucose oxidase concentration was 1 U/mL.

In order to imitate the conditions in cow's udder after administration of benzylpenicillin, we first studied the effect of benzylpenicillin on glucose concentration in milk during incubation, both in pure and spiked milk samples. We studied the effect of benzylpenicillin at concentrations 50 ppb and 50 ppm, which are quite high in comparison with MRL levels (4 ppb for benzylpenicillin in milk). These concentrations were chosen because the applied biosensing system enables to analyze the milk of single animals quickly within the early milking process and we could focus on analyzing the milk of the treated animals before it is "diluted" with the milk of other animals in milk collection tank. The determination of antibiotic residues in "undiluted" milk has an additional positive effect on the speed of analyses.

Changes of the glucose levels in milk due to the addition of benzylpenicillin were monitored during 5 hours (Fig. 9).

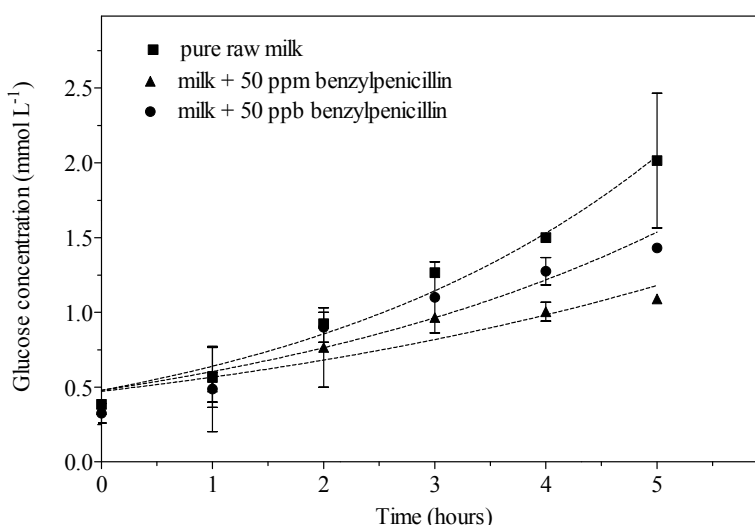


Figure 9. The change of glucose concentration in milk samples at different storage times. The measurements were carried out at 37 °C in pure milk (■), in milk spiked with 50 ppm (▲) and with 50 ppb of benzylpenicillin (●). The samples were stored at room temperature under constant stirring.

Immediately after the addition of benzylpenicillin, there was no detectable difference in the measured glucose concentrations (0.35 ± 0.065 mmol/L) in pure and in spiked milk samples (Fig. 9). In time course, the differences in glucose concentrations in spiked and pure raw milk samples increased and after 5 hours, the concentration of glucose had risen almost 7 times from its initial value in pure milk and only 3 times in milk spiked with 50 ppm of benzylpenicillin causing the deceleration of the increase of glucose concentration for approximately 66%. The addition of 50 ppb benzylpenicillin leads to rate deceleration for roughly 38% (Fig. 9).

Finally, the biosensor system was used for the measurement of glucose levels in raw milk of cows, which were administered penicillin antibiotics to cure mastitis, during the treatment and milk withdrawal periods. As expected, the measured glucose concentrations in the milk of the treated animals were considerably lower compared to the milk of healthy animals. The unpaired t-test indicated that this difference was significant ($P < 0,001$) (Fig. 10).

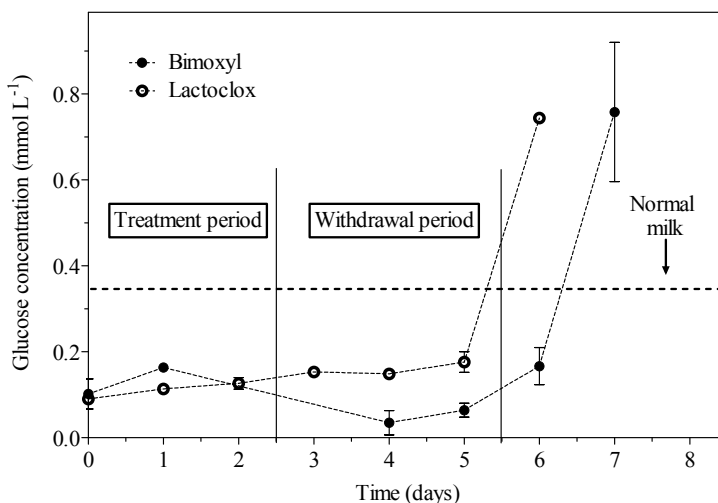


Figure 10. Glucose concentrations in the milk of cows, which had conducted mastitis and were treated with penicillin antibiotics. Milk samples were collected in the Dairy Research Farm of the Estonian University of Life Sciences in Southern Estonia. The milk samples from two cows undergoing mastitis treatment with Norbrook® Lactaclox or Bimoxyl LA were immediately frozen at $-20\text{ }^{\circ}\text{C}$ right after collection and melted at $+4\text{ }^{\circ}\text{C}$ just before testing. The treatment was administered for 3 days followed by a 3-day withdrawal period.

To validate the biosensor results, the presence of penicillin residues in the collected milk samples were analyzed also with Delvotest (DSM Food Specialties B.V.) The Delvotest analyses showed the presence of antibiotic residues above MRL levels in milk samples collected during the treatment and withdrawal periods, where the glucose levels were very low in comparison with glucose levels in pure milk (Fig. 10). Based on these results, the decreased glucose level can well serve as a qualitative indicator of the presence of antibiotic residues in raw milk similarly to Delvotest. The main advantage of using biosensing system for the detection of penicillin residues is time required for analyses – it is only 1 minute compared to 2–3 hours required for testing milk samples with Delvotest.

The output signals of reference oxygen optrode were also analyzed in the milk samples during the measurements, as the decrease of oxygen concentration in time indicates the oxygen demand of the total number of bacteria present in

milk samples. The oxygen demand in milk was low (around 15% of DOC in 5 minutes) and didn't change within days 1–4 counting from the beginning of treatment (slope=0; $P=0.17171$), but it increased by 5% per day from in days 5–9 (slope=0.005; $P<0.0001$). Based on the signal of the reference optrode, the total number of bacteria in samples decreased in the course of treatment and began to rise during the withdrawal period, indicating that the normal microbiota in udder began to recover.

CONCLUSIONS

As a result, a rapid method and a biosensor set-up have been proposed for the detection of penicillins' residues in milk flows.

A fibre-optical dual-channel glucose biosensor was used as a model set up for studying the processes during bio-recognition in flows on the example of glucose oxidase catalyzed glucose oxidation reaction. A mathematical model involving two-substrate reaction and mass transport of substrates was developed for describing the sensor signal. The model is based on a system of rate equations and has a relatively simple analytical solution. This facilitated the interpretation of the experimental data and allowed to develop a method for determining the biosensor output from early pre-steady state signals. It was demonstrated that the sensor reading could be obtained when the signal had changed only by 20% towards its final steady state value, which reduced the detection time about 10-fold as compared to standard procedures and gave significant advantage in analysis speed. It was found that the sensor parameters did not depend on the flow rate in a relatively wide range (0.8–13 mL/min or 0.3–5.1 cm/sec) [II, III]. The application of the model allowed to predict optimal biosensor parameters for obtaining maximal sensitivity and high stability on one hand, and to obtain fast results from the initial phase of the reaction on the other hand [III].

The modulation of the catalytic properties of glucose oxidase with the aim to amplify the characteristic calibration parameters of glucose and cascaded lactose biosensors was performed in the presence of different chlorides in order to accelerate the rate and improve the quality of milk analysis. It was found that sodium and magnesium chlorides at concentrations below 0.5 mol/L increased the total signal change parameter, used for the calibration of glucose biosensors, up to 20%. [I]. The addition of magnesium chloride gave further acceleration to the lactose measurements with bi-enzyme cascaded biosensors, as Mg^{2+} also activates β -galactosidase. The amplification was highest at a magnesium chloride concentration of 5 mmol/L [I].

The glucose dual-optrode biosensor was applied to detect penicillins' residues in the milk of cows with mastitis. The glucose concentration in their milk during treatment and withdrawal periods decreased significantly compared to glucose levels in high quality milk. This decrease was likely due to the decreased activity of β -galactosidase, which catalyzes the hydrolysis of lactose, enabling to use glucose concentration as an indicator of the presence of penicillins' residues in milk [V].

The studied biosensor set-up has a high potential to serve as a system for real-time automatic control of the quality of raw milk in milk production farms. The application of this system allows the separation of substandard milk from the milk flow prior to milk collection tank. The enzymatic oxidation of glucose, going on in the biosensor, can be further accelerated by adding metal chlorides for even more rapid analyses. The system can be upgraded by attaching additional biosensors to build up a more robust biosensor array, where the signals of individual biosensors form a typical pattern of milk sample, which changes in the presence of different antibiotics.

REFERENCES

- [1] Erman, M., Grow, B. Special Report: Powerful antibiotic for cows often misused by farmers, 2014. <http://www.reuters.com/article/us-farmaceuticals-ceftiofur-specialreport-idUSKCN0JJ03T20141206> last updated Dec 5, 2014.
- [2] Maureen, S. China's Overuse of Antibiotics in Livestock May Threaten Human Health, 2013. <http://health.usnews.com/health-news/news/articles/2013/02/11/chinas-overuse-of-antibiotics-in-livestock-may-threaten-human-health> last updated Feb 11, 2013.
- [3] Graham, J. P., Boland, J. J., Silbergeld, E. Growth Promoting Antibiotics in Food Animal Production: An Economic Analysis. *Public Health Reports*, 2007, 122(1), 79–87.
- [4] Grunwald, L., Petz, M. Food processing effects on residues: penicillins in milk and yoghurt. *Analytica Chimica Acta*, 2003, 483, 73–79.
- [5] Sales of veterinary antimicrobial agents in 26 EU/EEA countries in 2013 (EMA/387934/2015), 5th ESVAC Report, 2015.
- [6] Antimicrobials Sold or Distributed for Use in Food-Producing Animals, FDA Summary Report 2013. <http://www.fda.gov/downloads/ForIndustry/UserFees/AnimalDrugUserFeeActADUFA/UCM440584.pdf> last updated Apr, 2015.
- [7] Sales of veterinary antimicrobial agents in 19 EU/EEA countries in 2010 (EMA/88728/2012), European Medicines Agency, 2012.
- [8] Sales of veterinary antimicrobial agents in 26 EU/EEA countries in 2012 (EMA/333921/2014), 4th ESVAC Report, 2014.
- [9] Reder-Christ, K., Bendas, G. Biosensor Applications in the Field of Antibiotic Research – A Review of Recent Developments. *Sensors*, 2011, 11(10) 9450–9466.
- [10] Commission Regulation (European Union) 37/2010. Pharmacologically active substances and their classification regarding maximum residue limits in foodstuffs of animal origin.
- [11] Babington, R., Matas, S., Marco, M. P., Galve, R. Current bioanalytical methods for detection of penicillins. *Analytical and Bioanalytical Chemistry*, 2012, 403, 1549–1566.
- [12] Chafer-Pericas, C., Maquieira, A., Puchades, R. Fast screening methods to detect antibiotic residues in food samples. *TrAC Trends in Analytical Chemistry*, 2010, 29, 1038–1049.
- [13] Beltran, M.C., Berruga, M.I., Molina, A., Althaus, R.L., Molina, M.P. Performance of current microbial tests for screening antibiotics in sheep and goat milk. *International Dairy Journal*, 2015, 41, 13–15.
- [14] Kantiani, L., Farre, M., Damia, B. Analytical methodologies for the detection of [beta]-lactam antibiotics in milk and feed samples. *TrAC Trends in Analytical Chemistry*, 2009, 28, 729.
- [15] Wang, J., MacNeil, J.D., Kay, J.F. *Chemical Analysis of Antibiotic Residues in Food*. Hoboken, New Jersey: John Wiley & Sons, 2012.
- [16] DSM: Reliable antibiotic residue tests for milk. www.dsm.com/content/markets/foodandbeverages/en_US/solutions/responsible-food-delivery/reliable-antibiotic-residue-tests.html?wt.srch=1&wt.mc_id=GA-Branding last retrieved Jun 2015.
- [17] Adrian, J., Pinacho, D.G., Granier, B., Diserens, J.M., Sanchez-Baeza, F., Marco, M.P. A multianalyte ELISA for immunochemical screening of sulfonamide, fluoroquinolone and β -lactam antibiotics in milk samples using class-selective bioreceptors. *Analytical and Bioanalytical Chemistry*, 2008, 391, 1703–1712.

- [18] Andrew, S.M. Effect of fat and protein content of milk from individual cows on the specificity rates of antibiotic residue screening tests. *Journal of Dairy Science*, 2000, 83(12), 2992–2997.
- [19] Kivirand, K., Kagan, M., Rincken, T. Biosensors for the detection of antibiotic residues in milk. Published in: *Biosensors – Micro and Nanoscale Applications*, Intech, 2015, 425–456.
- [20] Cacciatore, G., Petz, M., Rachid, S., Hakenbeck, R., Bergwerff, A. Development of an optical biosensor assay for detection of beta-lactam antibiotics in milk using the penicillin-binding protein 2x*. *Analytica Chimica Acta*, 2004, 520, 105–115.
- [21] Gustavsson, E., Degelaen, J., Bjurling, P., Sternesjö, A. Determination of beta-Lactams in Milk Using a Surface Plasmon Resonance-Based Biosensor. *Journal of Agricultural and Food Chemistry*, 2004, 52, 2791–2796.
- [22] Gaudin, V., Fontaine, J., Maris, P. Screening of penicillin residues in milk by a surface plasmon resonance-based biosensor assay: Comparison of chemical and enzymatic sample pre-treatment. *Analytica Chimica Acta*, 2001, 436, 191–198.
- [23] Karaseva, N.A., Ermolaeva, T.N. Piezoelectric immunosensors for the detection of individual antibiotics and the total content of penicillin antibiotics in foodstuffs. *Talanta*, 2014, 120, 312–317.
- [24] Zhang, Z.F., Liu, J., Xu, K. X., Shi, T. Development of a miniature optical biosensor-based inhibition immunoassay for detection of ampicillin residues in milk. *Nanotechnology and Precision Engineering*, 2009, 7, 483–489.
- [25] Jiang, Z., Li, Y., Liang, A., Qin, A. A sensitive and selective immuno-nanogold resonance-scattering spectral method for the determination of trace penicillin G. *Luminescence*, 2008, 23, 157–162.
- [26] Thavarungkul, P., Dawan, S., Kanatharana, P., Asawatreratanakul, P. Detecting penicillin G in milk with impedimetric label-free immunosensor. *Biosensors and Bioelectronics*, 2007, 23, 688–694.
- [27] Kloth, K., Rye-Johnsen, M., Didier, A., Dietrich, R., Märtlbauer, E., Niessner, R., Seidel, M. A regenerable immunochip for the rapid determination of 13 different antibiotics in raw milk. *Analyst*, 2009, 134, 1433–1439.
- [28] Wu, H., Fuan, S., Zhang, W., Chen, H., Peng, L., Jin, X., Ma, J., Zhang, H. Amperometric immunosensor based on covalent immobilization of new methylene blue and penicillin polyclonal antibody for determination of penicillin G in milk. *Analytical Methods*, 2014, 6, 497–502.
- [29] Merola, G., Martini, E., Tomassetti, M., Campanella, L. Simple and suitable immunosensor for beta-lactam antibiotics analysis in real matrixes: Milk, serum, urine. *Journal of Pharmaceutical and Biomedical Analysis*, 2015, 106, 186–196.
- [30] Gruhl, F.J., Länge, K. Surface Acoustic Wave (SAW) Biosensor for Rapid and Label-Free Detection of Penicillin G in Milk. *Food Analytical Methods*, 2014, 7, 430–437.
- [31] Conzuelo, F., Gamella, M., Campuzano, S., Reviejo, A.J., Pingarrón J.M. Disposable amperometric magneto-immunosensor for direct detection of tetracyclines antibiotics residues in milk. *Analytica Chimica Acta*, 2012, 737, 29–36.
- [32] Adrian, J., Pasche, S. Voirin, G., Adrian, J., Pinacho, D.G., Font, H., Sánchez-Baeza, F., Marco, M.P., Diserens, J.M., Granier, B. Wavelength-interrogated optical biosensor for multi-analyte screening of sulfonamide, fluoroquinolone, beta-lactam and tetracycline antibiotics in milk. *TrAC Trends in Analytical Chemistry*, 2009, 28, 769–777.

- [33] Ionescu, R.E., Jaffrezic-Renault, E., Bouffier, L., Gondran, C., Cosnier, S., Pinacho, D.G., Marco, M.P., Sanchez-Baeza, F.J., Healy, T., Martelet, C. Impedimetric immunosensor for the specific label free detection of ciprofloxacin antibiotic. *Biosensors and Bioelectronics*, 2007, 23, 549–555.
- [34] Sternesjö, A., Gustavsson, E. Biosensor analysis of beta-lactams in milk using the carboxypeptidase activity of a bacterial penicillin binding protein. *Journal of AOAC International*, 2006, 89, 832–837.
- [35] Gustavsson, E., Bjurling, P., Degelaen, J., Sternesjö, A. Analysis of beta-lactam antibiotics using a microbial receptor protein-based biosensor assay. *Food and Agricultural Immunology*, 2002, 14, 121.
- [36] Drawz, S. M., Bonomo, R. A. Three decades of beta-lactamase inhibitors. *Clinical Microbiology Reviews*, 2010, 23, 160–201.
- [37] Lamar, J., Petz, M. Development of a receptor-based microplate assay for the detection of beta-lactam antibiotics in different food matrices. *Analytica Chimica Acta*, 2007, 586, 296–303.
- [38] Setford, S. J., Van Es, R. M., Blankwater, Y. J., Kröger, S. Receptor binding protein amperometric affinity sensor for rapid beta-lactam quantification in milk. *Analytica Chimica Acta*, 1999, 398, 13–22.
- [39] Gamella, M., Campuzano, S., Conzuelo, F., Esteban-Torres, M., de las Rivas, B., Reviejo, A.J., Muñoz, R., Pingarrón, J. M. An amperometric affinity penicillin-binding protein magnetosensor for the detection of beta-lactam antibiotics in milk. *Analyst*, 2013, 138, 2013–2022.
- [40] Conzuelo, F., Ruiz-Valdepenas Montiel, V., Campuzano, S., Gamella, M., Torrente-Rodríguez, R.M., Reviejo, A.J., Pingarrón, J.M. Rapid screening of multiple antibiotic residues in milk using disposable amperometric magnetosensors. *Analytica Chimica Acta*, 2014, 820, 32–38.
- [41] Chen, B., Ma, M., Su, X. An amperometric penicillin biosensor with enhanced sensitivity based on co-immobilization of carbon nanotubes, hematein, and beta-lactamase on glassy carbon electrode. *Analytica Chimica Acta*, 2010, 674, 89–95.
- [42] Wu, Y., Tang, L., Huang, L., Han, Z., Wang, J., Pan, H. A low detection limit penicillin biosensor based on single graphene nanosheets preadsorbed with hematein/ionic liquids/penicillinase. *Materials Science and Engineering: C*, 2014, 39, 92–99.
- [43] Healey, B. G., Walt, D. R. Improved fiber-optic chemical sensor for penicillin. *Analytical Chemistry*, 1995, 67, 4471–4476.
- [44] Goncalves, L. M., Callera, W. F. A., Sotomayor, M. D. P. T., Bueno P. R. Penicillinase-based amperometric biosensor for penicillin G. *Electrochemistry Communications*, 2014, 38, 131.
- [45] Ismail, F., Adeloju, S. B., Moline, A. N. Fabrication of a single layer and bilayer potentiometric biosensors for penicillin by galvanostatic entrapment of penicillinase into polypyrrole films. *Electroanalysis*, 2014, 26, 2607–2618.
- [46] Ismail, F., Adeloju, S. B. Galvanostatic entrapment of penicillinase into polytyramine films and its utilization for the potentiometric determination of penicillin. *Sensors*, 2010, 10, 2851–2868.
- [47] Narsaiah, K., Jha, S.N., Bhardwaj, R., Sharma, R., Kumar, R. Optical biosensors for food quality and safety assurance-A review. *Journal of Food Science and Technology*, 2012, 49, 383–406.

- [48] Ferrini, A. M., Mannoni, V., Carpico, G., Pellegrini, G. E. Detection and identification of beta-lactam residues in milk using a hybrid biosensor. *Journal of Agricultural and Food Chemistry*, 2008, 56, 784–788.
- [49] Das, S. Microbial based assay for specific detection of beta-lactam group of antibiotics in milk. *Journal of Food Science and Technology*, 2014, 51, 1161.
- [50] Pellegrini, G. E., Carpico, G., Coni, E. Electrochemical sensor for the detection and presumptive identification of quinolone and tetracycline residues in milk. *Analytica Chimica Acta*, 2004, 520, 13.
- [51] Ni, H., Zhang, S., Ding, X., Mi, T., Wang, Z., Liuet, M. Determination of Enrofloxacin in Bovine Milk by a Novel Single-Stranded DNA Aptamer Chemiluminescent Enzyme Immunoassay. *Analytical Letters*, 2014, 47, 2844–2856.
- [52] Berlina, A.N., Taranova, N.A., Zherdev, A.V., Vengerov, Y.Y, Dzantiev, B.B. Quantum dot-based lateral flow immunoassay for detection of chloramphenicol in milk. *Analytical and Bioanalytical Chemistry*, 2013, 405, 4997–5000.
- [53] Dapra, J., Lauridsen, L. H., Nielsen, A. T., Rozlosnik N. Comparative study on aptamers as recognition elements for antibiotics in a label-free all-polymer biosensor. *Biosensors and Bioelectronics*, 2013, 43, 315.
- [54] Wu, S., Zhang, H., Shi, Z., Duan, N., Fang, C., Dai, S., Wang, Z. Aptamer-based fluorescence biosensor for chloramphenicol determination using upconversion nanoparticles. *Food Control*, 2015, 50, 597–604.
- [55] Alibolandi, M., Hadizadeh, F., Vajhedin, F., Abnous, K., Ramezani M. Design and fabrication of an aptasensor for chloramphenicol based on energy transfer of CdTe quantum dots to graphene oxide sheet. *Materials Science and Engineering C*, 2015, 48, 611–619.
- [56] Famulok M., Mayer, G. Aptamer modules as sensors and detectors. *Accounts of Chemical Research*, 2011, 44, 1349.
- [57] Shangguan, D., Tang, Z., Mallikaratchy, P., Xiao, Z., Tan, W. Optimization and Modifications of Aptamers Selected from Live Cancer Cell Lines. *ChemBioChem*, 2007, 8, 603–606.
- [58] Toh, S. Y., Citartan, M., Gopinath, S. C. B., Tang, T. H. Aptamers as a replacement for antibodies in enzyme-linked immunosorbent assay. *Biosensors and Bioelectronics*, 2015, 64, 392.
- [59] He, L., Luo, Y., Zhi, W., Wu, Y., Zhou, P. A colorimetric aptamer biosensor based on gold nanoparticles for the ultrasensitive and specific detection of tetracycline in milk. *Australian Journal of Chemistry*, 2013, 66, 485–490.
- [60] Song, K. M., Jeong, E., Jeon, W., Cho, M., Ban, C. Aptasensor for ampicillin using gold nanoparticle based dual fluorescence-colorimetric methods. *Analytical and Bioanalytical Chemistry*, 2012, 402, 2153–2161.
- [61] Song, K.M., Jeong, E., Jeon, W., Jo, H., Ban, C. A coordination polymer nanobelt (CPNB)-based aptasensor for sulfadimethoxine. *Biosensors and Bioelectronics*, 2012, 33, 113–119.
- [62] Zhou, N., Zhang, J., Tian, Y. Aptamer-based spectrophotometric detection of kanamycin in milk. *Analytical Methods*, 2014, 6, 1569.
- [63] Kim, C.H., Lee, L.P., Min, J.R., Lim, M.W., Jeong, S.H. An indirect competitive assay-based aptasensor for detection of oxytetracycline in milk. *Biosensors and Bioelectronics*, 2014, 51, 426–430.
- [64] Luo, Y., He, L., Zhan, S., Wu, Y., Liu, L., Zhi, W., Zhou, P. Ultrasensitive resonance scattering (RS) spectral detection for trace tetracycline in milk using

- aptamer-coated nanogold (ACNG) as a catalyst. *Journal of Agricultural and Food Chemistry*, 2014, 62, 1032–1037.
- [65] Liu, B., Tang, D., Zhang, B., Que, X., Yang, H., Chen, G. Au(III)-promoted magnetic molecularly imprinted polymer nanospheres for electrochemical determination of streptomycin residues in food. *Biosensors and Bioelectronics*, 2013, 41, 551–556.
- [66] Yola, M. L., Uzun, L., Özaltın, N., Denizli, A. Development of molecular imprinted nanosensor for determination of tobramycin in pharmaceuticals and foods. *Talanta*, 2014, 120, 318.
- [67] Sadeghi, S., Motaharian, A. Voltammetric sensor based on carbon paste electrode modified with molecular imprinted polymer for determination of sulfadiazine in milk and human serum. *Materials Science and Engineering: C*, 2013, 33, 4884.
- [68] Turiel, E., Martín-Esteban, A. Molecularly imprinted polymers for sample preparation: A review. *Analytica Chimica Acta*, 2010, 668, 87.
- [69] Lian, W., Liu, S., Yu, J., Li, J., Cui, M., Xu, W., Huang, J. Electrochemical sensor using neomycin-imprinted film as recognition element based on chitosan-silver nanoparticles/graphene-multiwalled carbon nanotubes composites modified electrode. *Biosensors and Bioelectronics*, 2013, 44, 70.
- [70] Haasnoot, W., Loomans, E. E. M. G., Cazemier, G., Dietrich, R., Verheijen, R., Bergwerff A. A., Stephany, R. W. Direct versus competitive biosensor immunoassays for the detection of (Dihydro)streptomycin residues in milk. *Food and Agricultural Immunology*, 2002, 14, 15–27.
- [71] Baker, D.A., Gough, D.A. Dynamic Delay and Maximal Dynamic Error in Continuous Biosensors. *Analytical Chemistry*, 1996, 68, 1292–1297.
- [72] Baronas, D., Ivanauskas, F., Baronas, R. Mechanisms controlling the sensitivity of amperometric biosensors in flow injection analysis systems. *Journal of Mathematical Chemistry*, 2011, 49, 1521–1534.
- [73] Lammertyn, J., Verboven, P., Veraverbeke, E.A., Vermeir, S., Irudayaraj, J., Nicolai, B.M. Analysis of fluid flow and reaction kinetics in a flow injection analysis biosensor. *Sensors and Actuators, B: Chemical*, 2006, 114, 728–736.
- [74] Baronas, R., Ivanauskas, F., Kulys, J. Modelling dynamics of amperometric biosensors in batch and flow injection analysis. *Journal of Mathematical Chemistry*, 2002, 32, 225–237.
- [75] Bäcker, M., Rakowski, D., Poghossian, A., Biselli, M., Wagner, P., Schöning, M.J. Chip-based amperometric enzyme sensor system for monitoring of bioprocesses by flow-injection analysis. *Journal of Biotechnology*, 2013, 371–376.
- [76] Gooding, J.J. A simple model for an amperometric channel biosensor. *Electrochemistry Communications*, 1999, 119–123.
- [77] Ronkainen, N. J., Halsall, H. B., Heineman, W. R. Electrochemical biosensors. *Chemical Society Reviews*, 2010.
- [78] Bacha, S., Bergel, A., Comtat, M. Transient Response of Multilayer Electroenzymic Biosensors. *Analytical Chemistry*, 1995, 67, 1669–1678.
- [79] Flexer, V., Pratt, K.F.E., Garay, F., Bartlett, P.N., Calvo, E.J. Relaxation and Simplex mathematical algorithms applied to the study of steady-state electrochemical responses of immobilized enzyme biosensors: Comparison with experiments. *Journal of Electroanalytical Chemistry*, 2008, 87–98.
- [80] Leyboldt, J. K., Gough, D. A. Model of a two-substrate enzyme electrode for glucose. *Analytical Chemistry*, 1984, 56, 2896–2904.

- [81] Romero, M. R., Baruzzi, A. M., Garay, F. Mathematical modeling and experimental results of a sandwich-type amperometric biosensor, *Sensors and Actuators B: Chemical*, 2012, 284–291.
- [82] Myszka, D.G., He, X., Dembo, M., Morton, T. A., Goldstein, B. Extending the Range of Rate Constants Available from BIACORE: Interpreting Mass Transport-Influenced Binding Data. *Biophysical Journal*, 1998, 583–594.
- [83] Johnston, M.W., Williams, J.S. Field Comparison of Optical and Clark Cell Dissolved Oxygen Sensors in the Tualatin River, Oregon, 2005. *U.S. Geological Survey Open-File Report 2006–1047*, 2006, <http://pubs.usgs.gov/of/2006/1047/pdf/ofr2006-1047.pdf>
- [84] Kivirand, K., Rinken, T. Preparation and characterization of cadaverine sensitive nylon threads. *Sensor Letters*, 2009, 7, 580–585.
- [85] Rinken, T., Järv, J., Rinken, A. Production of Biosensors with Exchangeable Enzyme – Containing Threads. *Analytical Chemistry*, 2007, 79, 6042–6044.
- [86] Kivirand, K., Rebane, R., Rinken, T. A Simple Biosensor for Biogenic Diamines, Comprising Amine Oxidase – Containing Threads and Oxygen Sensor. *Sensor Letters*, 2011, 1794–1800.
- [87] Rinken, T., Tenno T. Dynamic model of amperometric biosensors. Characterisation of glucose biosensor output. *Biosensors and Bioelectronics*, 2001, 16, 53–59.
- [88] Held, P.G. Determination of beta-Galactosidase Activity using the PowerWave 200 Microplate Spectrophotometer. Creating Solutions for the Future of Science™. 2005. www.biotek.com.
- [89] Kivirand, K., Floren, A., Kagan, M., Avarmaa, T., Rinken, T., Jaaniso, R. Analyzing the Biosensor Signal in Flows: Studies with Glucose Optrodes. *Talanta*, 2015, 131, 74–80.
- [90] Adanyi, N., Szabo, E.E., Varadi, M. Multi-enzyme biosensors with amperometric detection for determination of lactose in milk and dairy products. *European Food Research and Technology*, 1999, 209, 220–226.
- [91] Gornischeff, A., Rinken, T. Calculating the output signal parameters of a lactose bienzymatic biosensing system from the transient phase response. *Proceedings of the Estonian Academy of Sciences*, 2011, 60, 136–140.
- [92] Sutendra, G., Wong, S., Fraser, M.E., Huber, R.E. β -galactosidase (*Escherichia coli*) has a second catalytically important Mg^{2+} site. *Biochemical and Biophysical Research Communications*, 2007, 352, 566–570.
- [93] Lo, S., Dugdale, M., Jeerh, N., Ku, T., Roth, N., Huber, R. Studies of Glu-416 variants of β -galactosidase (*E. coli*) show that the active site Mg^{2+} is not important for structure and indicate that the main role of Mg^{2+} is to mediate optimization of active site chemistry. *The Protein Journal*, 2010, 29, 26–31.
- [94] Gibson, Q.H., Swoboda, B.E.P., Massey, V. Kinetics And Mechanism Of Action Of Glucose Oxidase. *The Journal of Biological Chemistry*, 1964, 3927–3934.
- [95] Knappstein, K., Suhren, G., Walte, H.G. Influences of milking intervals and frequencies in automatic milking systems on excretion characteristics of different antibiotics in milk. *Project nr. QLK5-CT-2000-01006, Prevention of antibiotic residues*. 2003.
- [96] Jost, R. Milk and dairy products. In: *Ullmann's Encyclopedia of Industrial Chemistry*, Wiley, 2000.
- [97] Zhao, F.Q., Keating, A.F. Expression and regulation of glucose transporters in the bovine mammary gland. *Journal of Dairy Science*, 2007, 90, 76–86.

- [98] Meurant, G. *Handbook of Milk Composition*. Academic Press, 1995.
- [99] Faulkner, A., Chaiyabutr, N., Peaker, M., Carrick, D.T., Kuhn, N.J. Metabolic significance of milk glucose. *Journal of Dairy Research*, 1981, 48, 51–56.
- [100] Coorevits, A., De Jonghe, V., Vandroemme, J., Reekmans, R., Heyrman, J., Messens, W., De Vos, P., Heyndrickx, M. Comparative analysis of the diversity of aerobic spore-forming bacteria in raw milk from organic and conventional dairy farms. *Systematic and Applied Microbiology*, 2008, 31, 126–140.
- [101] Vacheyrou, M., Normand, A.C.C., Guyot, P., Cassagne, C., Piarroux, R., Bouton Y. Cultivable microbial communities in raw cow milk and potential transfers from stables of sixteen French farms. *International Journal of Food Microbiology*, 2011, 146, 253–262.
- [102] Masoud, W., Vogensen, F.K., Lillevang, S., Abu Al-Soud, W., Sorensen, A.J., Jakobsen, M. The fate of indigenous microbiota, starter cultures, *Escherichia coli*, *Listeria innocua* and *Staphylococcus aureus* in Danish raw milk and cheeses determined by pyrosequencing and quantitative real time (qRT)–PCR. *International Journal of Food Microbiology*, 2012, 153, 192–202.
- [103] Quigley, L., O'Sullivan, O., Beresford, T.P., Ross, R.P., Fitzgerald, G.F., Cotter P.D. Molecular approaches to analysing the microbial composition of raw milk and raw milk cheese. *International Journal of Food Microbiology*, 2011, 150, 81–94.

SUMMARY IN ESTONIAN

Penitsilliinide jääkide määramine piimas läbivoolulise biosensorsüsteemi abil

Käesoleva doktoritöö eesmärgiks oli välja töötada biosensorsüsteem penitsilliinide jääkide kiireks määramiseks toorpiimas, samuti pakkuda välja matemaatiline mudel läbivoolulistest mõõtesüsteemidest saadud eksperimentaalsete andmete kiireks analüüsiks ja biosensori kalibratsiooniparameetrite arvutamiseks ning uurida võimalusi biosensorites toimuvate äratundmisreaktsioonide kiirendamiseks. Töö praktiliseks eesmärgiks oli uurida võimalusi biosensori kasutamiseks penitsilliinide jääkide kiireks määramiseks antibiootikumiravil olevate lehmade piimas [I–III, V].

Penitsilliinid on beetalaktaamide hulka kuuluvad antibiootikumid, mida kasutatakse peamiselt Gram-positiivsete bakterite poolt tekitatud haiguste raviks. Penitsilliini ja teiste antibiootikumide jäägid piimas tekitavad inimestel allergilisi reaktsioone ning soodustavad resistentsete mikroobitüvede teket, mistõttu on antibiootikumide jääkide lubatud sisaldus toidus rangelt reguleeritud. Penitsilliinide jääkide maksimaalseks lubatud kontsentratsiooniks toorpiimas on bensüülpenitsilliini, ampitsilliini ja amoksitsilliini puhul 4 µg/L ning kloksatsilliini puhul 30 µg/L.

Tavaliselt kasutatakse antibiootikumide jääkide määramiseks piimas mitmesuguseid kromatograafial põhinevaid meetodeid ning erinevaid mikroobse inhibeerimise ja immuunoretseptor teste. Üheks võimalikuks alternatiiviks traditsioonilistele analüüsimeetoditele on biosensorite kasutamine. Biosensorite eeliseks on nende lihtsus, suhteline odavus ning kiirus, mis võimaldab nende kasutamist kiireteks analüüsideks reaalajas.

Voolavates süsteemides toimuvaid mõõtmisi iseloomustava mudeli väljatöötamiseks kasutati mõõtesüsteemi, mille keskseks osaks oli kahe voolukanaliga silindriline mõõterakk, millesse oli paigutatud glükoosi biooptrood ning hapniku võrdlusoptrood. Mõlemale optroodile, mis kujutavad endast hapnikutundliku materjaliga kaetud kvartsfiibrit, oli keritud niit, millele glükoosi optroodi puhul oli immobiliseeritud glükoosi oksüdaas. Mõlemad optroodid kokku moodustasid diferentsiaalse glükoosi biosensori, mis võimaldas eksperimentaalsete mürade mõju vähendamist biosensoris toimuva äratundmisreaktsiooni kirjeldamisel hapniku kontsentratsiooni vähenemise kaudu [III].

Väljapakutud läbivoolu mudeli ja eksperimentaalsete kõverate kokkulangevus oli väga hea ($R^2=0,99$). Leiti, et voolukiiruste vahemikus 0,8–13,0 mL/min signaali kogumuutuse parameetri väärtus voolu kiirusest ei sõltunud [II]. Võrreldes erinevate ajavahemike jooksul saadud andmetest arvutaud reaktsiooni parameetrite väärtusi leiti, et usaldusväärsete tulemuste saamiseks vajalik äratundmisreaktsiooni sügavus on ligikaudu 20%. Seega, uus läbivoolu biosensorite jaoks väljapakutud mudel võimaldab saada reprodutseeritavaid ja usaldusväärseid tulemusi 10-korda kiiremini kui varem [III]. Samuti selgus, et bio-

sensoris oleva ensüümi aktiivsuse vähenemine kuni 20% ei mõjuta oluliselt saadud tulemusi [III].

Piimas tehtavate analüüside kiirendamiseks uuriti ka glükoosi oksüdaasi aktiivsuse modulleerimise võimalusi erinevate metallide kationide abil nii glükoosi kui ka kaskaadses laktoosi biosensoris [I]. Signaali kogumuutuse parameetri väärtus suurenes kuni 20% naatrium- ja magneesiumioonide mõjul nende kontsentratsioonidel üle 5 mmol/L. Lisaks aktiveeris Mg^{2+} kaskaadses laktoosi biosensoris β -galaktosidaasi, suurendades veelgi mõõdetavat biosensori väljundsignaali [I].

Penitsilliini jääkide määramisel glükoosi biosensoriga selgus, et penitsilliiniga ravitavate lehmade piimas on glükoosi kontsentratsioon võrreldes tervetelt loomadelt saadava puhta piimaga väga madal ning see erinevus on statistiliselt oluline. Glükoosi madal kontsentratsioon on tõenäoliselt tingitud β -galaktosidaasi – ensüümi, mis katalüüsib laktoosi hüdrolyüsi piimas, vähenenud aktiivsusest. Töö tulemusena leiti, et glükoosi tase piimas on heaks indikaatoriks penitsilliini jääkide määramiseks toorpiimas [V].

Kasutatud biosensorsüsteem on rakendatav kiireks penitsillinide jääkide määramiseks toorpiimas piimafarmides. Kiire lüpstava piima analüüs võimaldab mittekvaliteetse piima õigeaegset eraldamist kvaliteetsest toodangust ning kogu toodetava piima kvaliteedi tõstmist. Kasutatud biosensorsüsteemi on erinevate antibiotikumide jääkide määramiseks toorpiimas võimalik tulevikus modifitseerida täiendavate biosensorite lisamisega.

ACKNOWLEDGEMENTS

In the first place, I would like to thank my supervisor Toonika Rinken for all her invaluable advice and continuous support throughout of my studies. I appreciate your guidance very much.

My warmest thanks to my colleagues and friends at the laboratory of the biosensors, at the Chair of Colloid and Environmental Chemistry at the University of Tartu, and especially for Kairi Kivirand who always helped and guided me during my studies.

I would like also to thank Dr. Raivo Jaaniso, Tea Avarmaa and Aare Floren for providing the oxygen optrodes and constructing the flow cell.

My very special thanks to my father and brother for their endless encouragement and support, and for my dearest Roman, being there for me and believing in me.

I am grateful to everyone who has supported and inspired me during my doctoral studies.

The financial support through funding from Estonian Science Foundation grants No7465 and No9061, Estonian Research Council Grant IUT 20–17, and the European Regional Development Fund Project “Mesosystems: theory and applications”; and from the graduate school “Functional Materials and Technologies” receiving funding from the European Social Fund (Project 1.2.0401.09-0079).

PUBLICATIONS

CURRICULUM VITAE

Margarita Kagan

Born: 09.03.1987
Citizenship: Estonian
Marital status: Single
Address: Institute of Chemistry, University of Tartu, Ravila 14a, 50411,
Tartu, Estonia
Phone: +372 556 06 697
e-mail: kaganmargarita@gmail.com

Education

2011–2016 University of Tartu, *PhD* student, supervisor Toonika Rincken
2008–2010 University of Tartu, *M.Sc* in environmental technology
2005–2008 University of Tartu, *B.Sc* in environmental technology

Professional employment

2013–2014 University of Tartu, Institute of Chemistry, chemist

Main scientific publications

- Kagan, M.**, Kivirand, K., Rincken, T. Modulation of enzyme catalytic properties and biosensor calibration parameters with chlorides: Studies with glucose oxidase. *Enzyme and Microbial Technology*, 2013, 53(4), 278–282.
- Kivirand, K., **Kagan, M.**, Rincken T. Calibrating Biosensors in Flow-Through Set-Ups: Studies with Glucose Optrodes. Published in: *State of the Art in Biosensors – General Aspects*, 2013, 331–351, Intech
- Kivirand, K., Floren, A., **Kagan, M.**, Avarmaa, T., Rincken, T., Jaaniso, R. Analyzing the Biosensor Signal in Flows: Studies with Glucose Optrodes. *Talanta*, 2015, 131, 74–80.
- Kivirand, K., **Kagan, M.**, Rincken, T. Biosensors for the detection of antibiotic residues in milk. Published in: *Biosensors – Micro and Nanoscale Applications*, 2015, 425–456, Intech
- Kagan, M.**, Printsman, G., Kivirand, K., Rincken T. Determination of Penicillins in Milk by a Dual Optrode Biosensor. *Analytical Letters*, 2016, In press.

ELULOOKIRJELDUS

Margarita Kagan

Sünniaeg ja koht: 09.03.1987, Tartu
Kodakondsus: Eesti
Perekonnaseis: Vallaline
Aadress: Tartu Ülikool, Keemia Instituut, Ravila 14a, 50411, Tartu, Estonia
Telefon: +372 556 06 697
e-mail: kaganmargarita@gmail.com

Haridus

2011–2016 Tartu Ülikool, doktoriõpe, juhendaja Toonika Rinke
2008–2010 Tartu Ülikool, *M.Sc.* keskkonnatehnoloogia
2005–2008 Tartu Ülikool, *B.Sc.* keskkonnatehnoloogia

Teenistuskäik

2013–2014 Tartu Ülikool, Keemia Instituut, keemik

Tähtsamad teaduspublikatsioonid

- Kagan, M.**, Kivirand, K., Rinke, T. Modulation of enzyme catalytic properties and biosensor calibration parameters with chlorides: Studies with glucose oxidase. *Enzyme and Microbial Technology*, 2013, 53(4), 278–282.
- Kivirand, K., **Kagan, M.**, Rinke, T. Calibrating Biosensors in Flow-Through Set-Ups: Studies with Glucose Optodes. Published in: *State of the Art in Biosensors – General Aspects*, 2013, 331–351, Intech
- Kivirand, K., Floren, A., **Kagan, M.**, Avarmaa, T., Rinke, T., Jaaniso, R. Analyzing the Biosensor Signal in Flows: Studies with Glucose Optodes. *Talanta*, 2015, 131, 74–80.
- Kivirand, K., **Kagan, M.**, Rinke, T. Biosensors for the detection of antibiotic residues in milk. Published in: *Biosensors – Micro and Nanoscale Applications*, 2015, 425–456, Intech
- Kagan, M.**, Printsman, G., Kivirand, K., Rinke, T. Determination of Penicillins in Milk by a Dual Optode Biosensor. *Analytical Letters*, 2016, In press.

DISSERTATIONES CHIMICAE UNIVERSITATIS TARTUENSIS

1. **Toomas Tamm.** Quantum-chemical simulation of solvent effects. Tartu, 1993, 110 p.
2. **Peeter Burk.** Theoretical study of gas-phase acid-base equilibria. Tartu, 1994, 96 p.
3. **Victor Lobanov.** Quantitative structure-property relationships in large descriptor spaces. Tartu, 1995, 135 p.
4. **Vahur Mäemets.** The ^{17}O and ^1H nuclear magnetic resonance study of H_2O in individual solvents and its charged clusters in aqueous solutions of electrolytes. Tartu, 1997, 140 p.
5. **Andrus Metsala.** Microcanonical rate constant in nonequilibrium distribution of vibrational energy and in restricted intramolecular vibrational energy redistribution on the basis of Slater's theory of unimolecular reactions. Tartu, 1997, 150 p.
6. **Uko Maran.** Quantum-mechanical study of potential energy surfaces in different environments. Tartu, 1997, 137 p.
7. **Alar Jänes.** Adsorption of organic compounds on antimony, bismuth and cadmium electrodes. Tartu, 1998, 219 p.
8. **Kaido Tammeveski.** Oxygen electroreduction on thin platinum films and the electrochemical detection of superoxide anion. Tartu, 1998, 139 p.
9. **Ivo Leito.** Studies of Brønsted acid-base equilibria in water and non-aqueous media. Tartu, 1998, 101 p.
10. **Jaan Leis.** Conformational dynamics and equilibria in amides. Tartu, 1998, 131 p.
11. **Toonika Rinken.** The modelling of amperometric biosensors based on oxidoreductases. Tartu, 2000, 108 p.
12. **Dmitri Panov.** Partially solvated Grignard reagents. Tartu, 2000, 64 p.
13. **Kaja Orupõld.** Treatment and analysis of phenolic wastewater with microorganisms. Tartu, 2000, 123 p.
14. **Jüri Ivask.** Ion Chromatographic determination of major anions and cations in polar ice core. Tartu, 2000, 85 p.
15. **Lauri Vares.** Stereoselective Synthesis of Tetrahydrofuran and Tetrahydropyran Derivatives by Use of Asymmetric Horner-Wadsworth-Emmons and Ring Closure Reactions. Tartu, 2000, 184 p.
16. **Martin Lepiku.** Kinetic aspects of dopamine D_2 receptor interactions with specific ligands. Tartu, 2000, 81 p.
17. **Katrin Sak.** Some aspects of ligand specificity of P2Y receptors. Tartu, 2000, 106 p.
18. **Vello Pällin.** The role of solvation in the formation of iotsitch complexes. Tartu, 2001, 95 p.
19. **Katrin Kollist.** Interactions between polycyclic aromatic compounds and humic substances. Tartu, 2001, 93 p.

20. **Ivar Koppel.** Quantum chemical study of acidity of strong and superstrong Brønsted acids. Tartu, 2001, 104 p.
21. **Viljar Pihl.** The study of the substituent and solvent effects on the acidity of OH and CH acids. Tartu, 2001, 132 p.
22. **Natalia Palm.** Specification of the minimum, sufficient and significant set of descriptors for general description of solvent effects. Tartu, 2001, 134 p.
23. **Sulev Sild.** QSPR/QSAR approaches for complex molecular systems. Tartu, 2001, 134 p.
24. **Ruslan Petrukhin.** Industrial applications of the quantitative structure-property relationships. Tartu, 2001, 162 p.
25. **Boris V. Rogovoy.** Synthesis of (benzotriazolyl)carboximidamides and their application in relations with *N*- and *S*-nucleophyles. Tartu, 2002, 84 p.
26. **Koit Herodes.** Solvent effects on UV-vis absorption spectra of some solvatochromic substances in binary solvent mixtures: the preferential solvation model. Tartu, 2002, 102 p.
27. **Anti Perkson.** Synthesis and characterisation of nanostructured carbon. Tartu, 2002, 152 p.
28. **Ivari Kaljurand.** Self-consistent acidity scales of neutral and cationic Brønsted acids in acetonitrile and tetrahydrofuran. Tartu, 2003, 108 p.
29. **Karmen Lust.** Adsorption of anions on bismuth single crystal electrodes. Tartu, 2003, 128 p.
30. **Mare Piirsalu.** Substituent, temperature and solvent effects on the alkaline hydrolysis of substituted phenyl and alkyl esters of benzoic acid. Tartu, 2003, 156 p.
31. **Meeri Sassian.** Reactions of partially solvated Grignard reagents. Tartu, 2003, 78 p.
32. **Tarmo Tamm.** Quantum chemical modelling of polypyrrole. Tartu, 2003. 100 p.
33. **Erik Teinmaa.** The environmental fate of the particulate matter and organic pollutants from an oil shale power plant. Tartu, 2003. 102 p.
34. **Jaana Tammiku-Taul.** Quantum chemical study of the properties of Grignard reagents. Tartu, 2003. 120 p.
35. **Andre Lomaka.** Biomedical applications of predictive computational chemistry. Tartu, 2003. 132 p.
36. **Kostyantyn Kirichenko.** Benzotriazole – Mediated Carbon–Carbon Bond Formation. Tartu, 2003. 132 p.
37. **Gunnar Nurk.** Adsorption kinetics of some organic compounds on bismuth single crystal electrodes. Tartu, 2003, 170 p.
38. **Mati Arulepp.** Electrochemical characteristics of porous carbon materials and electrical double layer capacitors. Tartu, 2003, 196 p.
39. **Dan Cornel Fara.** QSPR modeling of complexation and distribution of organic compounds. Tartu, 2004, 126 p.
40. **Riina Mahlapuu.** Signalling of galanin and amyloid precursor protein through adenylate cyclase. Tartu, 2004, 124 p.

41. **Mihkel Kerikmäe.** Some luminescent materials for dosimetric applications and physical research. Tartu, 2004, 143 p.
42. **Jaanus Kruusma.** Determination of some important trace metal ions in human blood. Tartu, 2004, 115 p.
43. **Urmas Johanson.** Investigations of the electrochemical properties of polypyrrole modified electrodes. Tartu, 2004, 91 p.
44. **Kaido Sillar.** Computational study of the acid sites in zeolite ZSM-5. Tartu, 2004, 80 p.
45. **Aldo Oras.** Kinetic aspects of dATP α S interaction with P2Y₁ receptor. Tartu, 2004, 75 p.
46. **Erik Mölder.** Measurement of the oxygen mass transfer through the air-water interface. Tartu, 2005, 73 p.
47. **Thomas Thomberg.** The kinetics of electroreduction of peroxodisulfate anion on cadmium (0001) single crystal electrode. Tartu, 2005, 95 p.
48. **Olavi Loog.** Aspects of condensations of carbonyl compounds and their imine analogues. Tartu, 2005, 83 p.
49. **Siim Salmar.** Effect of ultrasound on ester hydrolysis in aqueous ethanol. Tartu, 2006, 73 p.
50. **Ain Uustare.** Modulation of signal transduction of heptahelical receptors by other receptors and G proteins. Tartu, 2006, 121 p.
51. **Sergei Yurchenko.** Determination of some carcinogenic contaminants in food. Tartu, 2006, 143 p.
52. **Kaido Tämm.** QSPR modeling of some properties of organic compounds. Tartu, 2006, 67 p.
53. **Olga Tšubrik.** New methods in the synthesis of multisubstituted hydrazines. Tartu, 2006, 183 p.
54. **Lilli Sooväli.** Spectrophotometric measurements and their uncertainty in chemical analysis and dissociation constant measurements. Tartu, 2006, 125 p.
55. **Eve Koort.** Uncertainty estimation of potentiometrically measured pH and pK_a values. Tartu, 2006, 139 p.
56. **Sergei Kopanchuk.** Regulation of ligand binding to melanocortin receptor subtypes. Tartu, 2006, 119 p.
57. **Silvar Kallip.** Surface structure of some bismuth and antimony single crystal electrodes. Tartu, 2006, 107 p.
58. **Kristjan Saal.** Surface silanization and its application in biomolecule coupling. Tartu, 2006, 77 p.
59. **Tanel Tätte.** High viscosity Sn(OBu)₄ oligomeric concentrates and their applications in technology. Tartu, 2006, 91 p.
60. **Dimitar Atanasov Dobchev.** Robust QSAR methods for the prediction of properties from molecular structure. Tartu, 2006, 118 p.
61. **Hannes Hagu.** Impact of ultrasound on hydrophobic interactions in solutions. Tartu, 2007, 81 p.

62. **Rutha Jäger.** Electroreduction of peroxodisulfate anion on bismuth electrodes. Tartu, 2007, 142 p.
63. **Kaido Viht.** Immobilizable bisubstrate-analogue inhibitors of basophilic protein kinases: development and application in biosensors. Tartu, 2007, 88 p.
64. **Eva-Ingrid Rõõm.** Acid-base equilibria in nonpolar media. Tartu, 2007, 156 p.
65. **Sven Tamp.** DFT study of the cesium cation containing complexes relevant to the cesium cation binding by the humic acids. Tartu, 2007, 102 p.
66. **Jaak Nerut.** Electroreduction of hexacyanoferrate(III) anion on Cadmium (0001) single crystal electrode. Tartu, 2007, 180 p.
67. **Lauri Jalukse.** Measurement uncertainty estimation in amperometric dissolved oxygen concentration measurement. Tartu, 2007, 112 p.
68. **Aime Lust.** Charge state of dopants and ordered clusters formation in CaF₂:Mn and CaF₂:Eu luminophors. Tartu, 2007, 100 p.
69. **Iiris Kahn.** Quantitative Structure-Activity Relationships of environmentally relevant properties. Tartu, 2007, 98 p.
70. **Mari Reinik.** Nitrates, nitrites, N-nitrosamines and polycyclic aromatic hydrocarbons in food: analytical methods, occurrence and dietary intake. Tartu, 2007, 172 p.
71. **Heili Kasuk.** Thermodynamic parameters and adsorption kinetics of organic compounds forming the compact adsorption layer at Bi single crystal electrodes. Tartu, 2007, 212 p.
72. **Erki Enkvist.** Synthesis of adenosine-peptide conjugates for biological applications. Tartu, 2007, 114 p.
73. **Svetoslav Hristov Slavov.** Biomedical applications of the QSAR approach. Tartu, 2007, 146 p.
74. **Eneli Härk.** Electroreduction of complex cations on electrochemically polished Bi(*hkl*) single crystal electrodes. Tartu, 2008, 158 p.
75. **Priit Möller.** Electrochemical characteristics of some cathodes for medium temperature solid oxide fuel cells, synthesized by solid state reaction technique. Tartu, 2008, 90 p.
76. **Signe Viggor.** Impact of biochemical parameters of genetically different pseudomonads at the degradation of phenolic compounds. Tartu, 2008, 122 p.
77. **Ave Sarapuu.** Electrochemical reduction of oxygen on quinone-modified carbon electrodes and on thin films of platinum and gold. Tartu, 2008, 134 p.
78. **Agnes Kütt.** Studies of acid-base equilibria in non-aqueous media. Tartu, 2008, 198 p.
79. **Rouvim Kadis.** Evaluation of measurement uncertainty in analytical chemistry: related concepts and some points of misinterpretation. Tartu, 2008, 118 p.
80. **Valter Reedo.** Elaboration of IVB group metal oxide structures and their possible applications. Tartu, 2008, 98 p.

81. **Aleksei Kuznetsov.** Allosteric effects in reactions catalyzed by the cAMP-dependent protein kinase catalytic subunit. Tartu, 2009, 133 p.
82. **Aleksei Bredihhin.** Use of mono- and polyanions in the synthesis of multisubstituted hydrazine derivatives. Tartu, 2009, 105 p.
83. **Anu Ploom.** Quantitative structure-reactivity analysis in organosilicon chemistry. Tartu, 2009, 99 p.
84. **Argo Vonk.** Determination of adenosine A_{2A}- and dopamine D₁ receptor-specific modulation of adenylate cyclase activity in rat striatum. Tartu, 2009, 129 p.
85. **Indrek Kivi.** Synthesis and electrochemical characterization of porous cathode materials for intermediate temperature solid oxide fuel cells. Tartu, 2009, 177 p.
86. **Jaanus Eskusson.** Synthesis and characterisation of diamond-like carbon thin films prepared by pulsed laser deposition method. Tartu, 2009, 117 p.
87. **Marko Lätt.** Carbide derived microporous carbon and electrical double layer capacitors. Tartu, 2009, 107 p.
88. **Vladimir Stepanov.** Slow conformational changes in dopamine transporter interaction with its ligands. Tartu, 2009, 103 p.
89. **Aleksander Trummal.** Computational Study of Structural and Solvent Effects on Acidities of Some Brønsted Acids. Tartu, 2009, 103 p.
90. **Eerold Vellemäe.** Applications of mischmetal in organic synthesis. Tartu, 2009, 93 p.
91. **Sven Parkel.** Ligand binding to 5-HT_{1A} receptors and its regulation by Mg²⁺ and Mn²⁺. Tartu, 2010, 99 p.
92. **Signe Vahur.** Expanding the possibilities of ATR-FT-IR spectroscopy in determination of inorganic pigments. Tartu, 2010, 184 p.
93. **Tavo Romann.** Preparation and surface modification of bismuth thin film, porous, and microelectrodes. Tartu, 2010, 155 p.
94. **Nadežda Aleksejeva.** Electrocatalytic reduction of oxygen on carbon nanotube-based nanocomposite materials. Tartu, 2010, 147 p.
95. **Marko Kullapere.** Electrochemical properties of glassy carbon, nickel and gold electrodes modified with aryl groups. Tartu, 2010, 233 p.
96. **Liis Siinor.** Adsorption kinetics of ions at Bi single crystal planes from aqueous electrolyte solutions and room-temperature ionic liquids. Tartu, 2010, 101 p.
97. **Angela Vaasa.** Development of fluorescence-based kinetic and binding assays for characterization of protein kinases and their inhibitors. Tartu 2010, 101 p.
98. **Indrek Tulp.** Multivariate analysis of chemical and biological properties. Tartu 2010, 105 p.
99. **Aare Selberg.** Evaluation of environmental quality in Northern Estonia by the analysis of leachate. Tartu 2010, 117 p.
100. **Darja Lavõgina.** Development of protein kinase inhibitors based on adenosine analogue-oligoarginine conjugates. Tartu 2010, 248 p.

101. **Laura Herm.** Biochemistry of dopamine D₂ receptors and its association with motivated behaviour. Tartu 2010, 156 p.
102. **Terje Raudsepp.** Influence of dopant anions on the electrochemical properties of polypyrrole films. Tartu 2010, 112 p.
103. **Margus Marandi.** Electroformation of Polypyrrole Films: *In-situ* AFM and STM Study. Tartu 2011, 116 p.
104. **Kairi Kivirand.** Diamine oxidase-based biosensors: construction and working principles. Tartu, 2011, 140 p.
105. **Anneli Kruve.** Matrix effects in liquid-chromatography electrospray mass-spectrometry. Tartu, 2011, 156 p.
106. **Gary Urb.** Assessment of environmental impact of oil shale fly ash from PF and CFB combustion. Tartu, 2011, 108 p.
107. **Nikita Oskolkov.** A novel strategy for peptide-mediated cellular delivery and induction of endosomal escape. Tartu, 2011, 106 p.
108. **Dana Martin.** The QSPR/QSAR approach for the prediction of properties of fullerene derivatives. Tartu, 2011, 98 p.
109. **Säde Viirlaid.** Novel glutathione analogues and their antioxidant activity. Tartu, 2011, 106 p.
110. **Ülis Sõukand.** Simultaneous adsorption of Cd²⁺, Ni²⁺, and Pb²⁺ on peat. Tartu, 2011, 124 p.
111. **Lauri Lipping.** The acidity of strong and superstrong Brønsted acids, an outreach for the “limits of growth”: a quantum chemical study. Tartu, 2011, 124 p.
112. **Heisi Kurig.** Electrical double-layer capacitors based on ionic liquids as electrolytes. Tartu, 2011, 146 p.
113. **Marje Kasari.** Bisubstrate luminescent probes, optical sensors and affinity adsorbents for measurement of active protein kinases in biological samples. Tartu, 2012, 126 p.
114. **Kalev Takkis.** Virtual screening of chemical databases for bioactive molecules. Tartu, 2012, 122 p.
115. **Ksenija Kisseljova.** Synthesis of aza-β³-amino acid containing peptides and kinetic study of their phosphorylation by protein kinase A. Tartu, 2012, 104 p.
116. **Riin Rebane.** Advanced method development strategy for derivatization LC/ESI/MS. Tartu, 2012, 184 p.
117. **Vladislav Ivaništšev.** Double layer structure and adsorption kinetics of ions at metal electrodes in room temperature ionic liquids. Tartu, 2012, 128 p.
118. **Irja Helm.** High accuracy gravimetric Winkler method for determination of dissolved oxygen. Tartu, 2012, 139 p.
119. **Karin Kipper.** Fluoroalcohols as Components of LC-ESI-MS Eluents: Usage and Applications. Tartu, 2012, 164 p.
120. **Arno Ratas.** Energy storage and transfer in dosimetric luminescent materials. Tartu, 2012, 163 p.

121. **Reet Reinart-Okugbeni.** Assay systems for characterisation of subtype-selective binding and functional activity of ligands on dopamine receptors. Tartu, 2012, 159 p.
122. **Lauri Sikk.** Computational study of the Sonogashira cross-coupling reaction. Tartu, 2012, 81 p.
123. **Karita Raudkivi.** Neurochemical studies on inter-individual differences in affect-related behaviour of the laboratory rat. Tartu, 2012, 161 p.
124. **Indrek Saar.** Design of GalR2 subtype specific ligands: their role in depression-like behavior and feeding regulation. Tartu, 2013, 126 p.
125. **Ann Laheäär.** Electrochemical characterization of alkali metal salt based non-aqueous electrolytes for supercapacitors. Tartu, 2013, 127 p.
126. **Kerli Tõnurist.** Influence of electrospun separator materials properties on electrochemical performance of electrical double-layer capacitors. Tartu, 2013, 147 p.
127. **Kaija Põhako-Esko.** Novel organic and inorganic ionogels: preparation and characterization. Tartu, 2013, 124 p.
128. **Ivar Kruusenberg.** Electroreduction of oxygen on carbon nanomaterial-based catalysts. Tartu, 2013, 191 p.
129. **Sander Piiskop.** Kinetic effects of ultrasound in aqueous acetonitrile solutions. Tartu, 2013, 95 p.
130. **Iлона Faustova.** Regulatory role of L-type pyruvate kinase N-terminal domain. Tartu, 2013, 109 p.
131. **Kadi Tamm.** Synthesis and characterization of the micro-mesoporous anode materials and testing of the medium temperature solid oxide fuel cell single cells. Tartu, 2013, 138 p.
132. **Iva Bozhidarova Stoyanova-Slavova.** Validation of QSAR/QSPR for regulatory purposes. Tartu, 2013, 109 p.
133. **Vitali Grozovski.** Adsorption of organic molecules at single crystal electrodes studied by *in situ* STM method. Tartu, 2014, 146 p.
134. **Santa Veikšina.** Development of assay systems for characterisation of ligand binding properties to melanocortin 4 receptors. Tartu, 2014, 151 p.
135. **Jüri Liiv.** PVDF (polyvinylidene difluoride) as material for active element of twisting-ball displays. Tartu, 2014, 111 p.
136. **Kersti Vaarmets.** Electrochemical and physical characterization of pristine and activated molybdenum carbide-derived carbon electrodes for the oxygen electroreduction reaction. Tartu, 2014, 131 p.
137. **Lauri Tõntson.** Regulation of G-protein subtypes by receptors, guanine nucleotides and Mn²⁺. Tartu, 2014, 105 p.
138. **Aiko Adamson.** Properties of amine-boranes and phosphorus analogues in the gas phase. Tartu, 2014, 78 p.
139. **Elo Kibena.** Electrochemical grafting of glassy carbon, gold, highly oriented pyrolytic graphite and chemical vapour deposition-grown graphene electrodes by diazonium reduction method. Tartu, 2014, 184 p.

140. **Teemu Näykki.** Novel Tools for Water Quality Monitoring – From Field to Laboratory. Tartu, 2014, 202 p.
141. **Karl Kaupmees.** Acidity and basicity in non-aqueous media: importance of solvent properties and purity. Tartu, 2014, 128 p.
142. **Oleg Lebedev.** Hydrazine polyanions: different strategies in the synthesis of heterocycles. Tartu, 2015, 118 p.
143. **Geven Piir.** Environmental risk assessment of chemicals using QSAR methods. Tartu, 2015, 123 p.
144. **Olga Mazina.** Development and application of the biosensor assay for measurements of cyclic adenosine monophosphate in studies of G protein-coupled receptor signaling. Tartu, 2015, 116 p.
145. **Sandip Ashokrao Kadam.** Anion receptors: synthesis and accurate binding measurements. Tartu, 2015, 116 p.
146. **Indrek Tallo.** Synthesis and characterization of new micro-mesoporous carbide derived carbon materials for high energy and power density electrical double layer capacitors. Tartu, 2015, 148 p.
147. **Heiki Erikson.** Electrochemical reduction of oxygen on nanostructured palladium and gold catalysts. Tartu, 2015, 204 p.
148. **Erik Anderson.** *In situ* Scanning Tunnelling Microscopy studies of the interfacial structure between Bi(111) electrode and a room temperature ionic liquid. Tartu, 2015, 118 p.
149. **Girinath G. Pillai.** Computational Modelling of Diverse Chemical, Biochemical and Biomedical Properties. Tartu, 2015, 140 p.
150. **Piret Pikma.** Interfacial structure and adsorption of organic compounds at Cd(0001) and Sb(111) electrodes from ionic liquid and aqueous electrolytes: an *in situ* STM study. Tartu, 2015, 126 p.
151. **Ganesh babu Manoharan.** Combining chemical and genetic approaches for photoluminescence assays of protein kinases. Tartu, 2016, 126 p.
152. **Carolin Siimenson.** Electrochemical characterization of halide ion adsorption from liquid mixtures at Bi(111) and pyrolytic graphite electrode surface. Tartu, 2016, 110 p.
153. **Asko Laaniste.** Comparison and optimisation of novel mass spectrometry ionisation sources. Tartu, 2016, 156 p.
154. **Hanno Evard.** Estimating limit of detection for mass spectrometric analysis methods. Tartu, 2016, 224 p.
155. **Kadri Ligi.** Characterization and application of protein kinase-responsive organic probes with triplet-singlet energy transfer. Tartu, 2016, 122p.