



Su, Rong and Coupland, Jeremy and Leach, Richard K. (2017) Calibration of coherence scanning interferometry and the effects of defocus. In: Focus on Microscopy 2017, 9-12 April, 2017, Bordeaux, France.

**Access from the University of Nottingham repository:**

[http://eprints.nottingham.ac.uk/42299/1/Abstract\\_FOM\\_v2%5B1%5D.pdf](http://eprints.nottingham.ac.uk/42299/1/Abstract_FOM_v2%5B1%5D.pdf)

**Copyright and reuse:**

The Nottingham ePrints service makes this work by researchers of the University of Nottingham available open access under the following conditions.

This article is made available under the University of Nottingham End User licence and may be reused according to the conditions of the licence. For more details see:  
[http://eprints.nottingham.ac.uk/end\\_user\\_agreement.pdf](http://eprints.nottingham.ac.uk/end_user_agreement.pdf)

**A note on versions:**

The version presented here may differ from the published version or from the version of record. If you wish to cite this item you are advised to consult the publisher's version. Please see the repository url above for details on accessing the published version and note that access may require a subscription.

For more information, please contact [eprints@nottingham.ac.uk](mailto:eprints@nottingham.ac.uk)

See discussions, stats, and author profiles for this publication at: <https://www.researchgate.net/publication/316119625>

# Calibration of coherence scanning interferometry and the effects of defocus

Conference Paper · April 2017

---

CITATIONS

0

READS

53

**3 authors:**



Rong Su

University of Nottingham

15 PUBLICATIONS 25 CITATIONS

[SEE PROFILE](#)



Jeremy Michael Coupland

Loughborough University

127 PUBLICATIONS 852 CITATIONS

[SEE PROFILE](#)



Richard Leach

University of Nottingham

295 PUBLICATIONS 1,764 CITATIONS

[SEE PROFILE](#)

**Some of the authors of this publication are also working on these related projects:**



Precision Additive Metal Manufacturing (PAM<sup>2</sup>) [View project](#)



Reference algorithms and metrology on aspherical and freeform optical lenses (FreeFORM) [View project](#)

All content following this page was uploaded by [Richard Leach](#) on 14 April 2017.

The user has requested enhancement of the downloaded file. All in-text references [underlined in blue](#) are added to the original document and are linked to publications on ResearchGate, letting you access and read them immediately.

## Calibration of coherence scanning interferometry and the effects of defocus

Rong Su,<sup>1</sup> Jeremy Coupland<sup>2</sup> and Richard Leach<sup>1</sup>

<sup>1</sup>The University of Nottingham, UK; <sup>2</sup>Loughborough University, UK

E-mail: rong.su@nottingham.ac.uk

**KEY WORDS:** transfer function, point spread function, defocus, calibration, interferometry.

Coherence scanning interferometry (CSI) is a well-established technique for 3D measurement of surface topography with sub-nanometre precision in the axial direction. As with most 3D optical imaging systems, the performance of CSI depends strongly on the local tilt and curvature of the sample surface. Based on 3D linear systems theory, the performance of CSI can be characterised in terms of the 3D transfer function (TF) in the spatial frequency domain or the 3D point spread function (PSF) in the spatial domain [1,2]. From the measurement of a precision sphere, a CSI system can be calibrated and partly corrected based on the so-called “foil model” of the surface [3]. A recent study has investigated the tilt and curvature dependent errors in CSI, and demonstrated that an aberration-free CSI system is capable of measuring the topography of surfaces with varying tilt with sub-nanometre accuracy [4]. When defocus is present in a CSI system, the measurement accuracy and resolution of the system are degraded. Usually, a Mirau-type interferometer is used in CSI for lenses with 50 $\times$  magnification (NA of 0.55) and an offset of the axial position of the reference mirror may cause defocus aberration. We demonstrate here (see figure 1), the theoretically calculated 3D TF and PSF of a CSI system with 0.55 NA at different conditions of defocus, and the corresponding fringes from a spherical surface. The results show that defocus causes distortion of the modulus and phase of the TF, and modifies the PSF. The reduced fringe contrast in the tilted surface regions may reduce the detectable area and cause significant errors when calculating the surface topography.

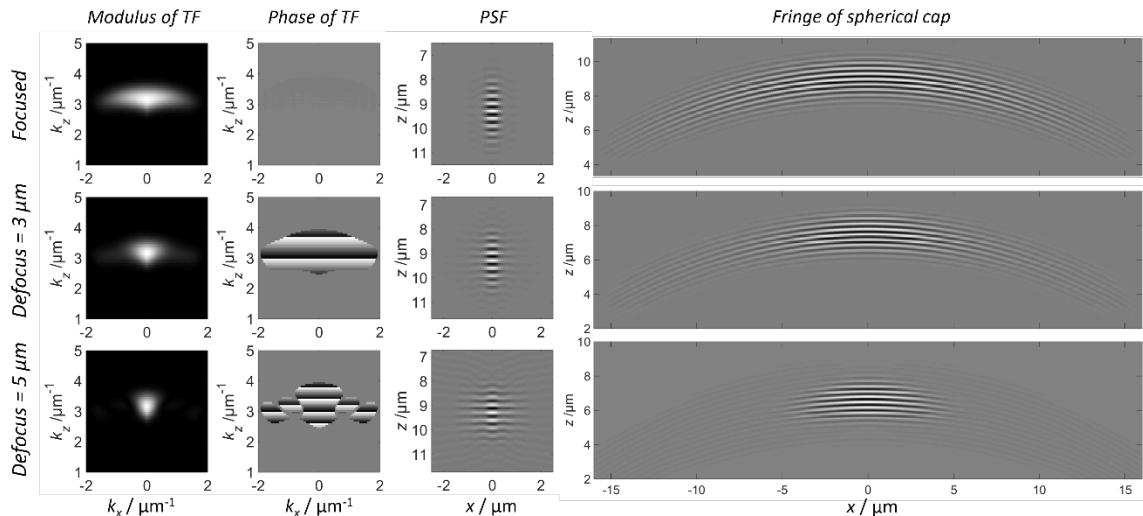


Figure 1. Effects of defocus in CSI

- [1] J. M. Coupland and J. Lobera, “Holography, tomography and 3D microscopy as linear filtering operations,” *Meas. Sci. Technol.* 19, 07010 (2008).
- [2] J. M. Coupland, R. Mandal, K. Palodhi, and R. K. Leach, “Coherence scanning interferometry: linear theory of surface measurement,” *Appl. Opt.* 52, 3662-3670 (2013).
- [3] R. Mandal, J. M. Coupland, R. K. Leach, and D. Mansfield, “Coherence scanning interferometry: measurement and correction of three-dimensional transfer and point-spread characteristics,” *Appl. Opt.* 53, 1554-1563 (2014).

[4] R. Su, Y. Wang, J. M. Coupland, and R. K. Leach, “On tilt and curvature dependent errors and the calibration of coherence scanning interferometry,” *Opt. Express*, 25, (2017).