



INSTITUTO POLITÉCNICO DE LISBOA

**ESCOLA SUPERIOR DE TECNOLOGIA DA SAÚDE DE
LISBOA**

**STEREOTACTIC BODY RADIATION THERAPY
IN LUNG CANCER
PATIENT POSITIONING: ARMS UP vs. ARMS DOWN
A DOSIMETRIC EVALUATION**

CÁTIA BARREIRA

Orientadora: PROF. MARGARIDA EIRAS

**MESTRADO EM RADIAÇÕES APLICADAS ÀS TECNOLOGIAS DA
SAÚDE – Terapia com Radiações**

Lisboa, 2016

INSTITUTO POLITÉCNICO DE LISBOA

**ESCOLA SUPERIOR DE TECNOLOGIA DA SAÚDE DE
LISBOA**

**STEREOTACTIC BODY RADIATION THERAPY
IN LUNG CANCER
PATIENT POSITIONING: ARMS UP vs. ARMS DOWN
A DOSIMETRIC EVALUATION**

CÁTIA BARREIRA

Orientadora: PROF. MARGARIDA EIRAS

MESTRADO EM RADIAÇÕES APLICADAS ÀS TECNOLOGIAS DA
SAÚDE

Lisboa, 2016

**STEREOTACTIC BODY RADIATION THERAPY
IN LUNG CANCER
PATIENT POSITIONING: ARMS UP vs. ARMS DOWN
A DOSIMETRIC EVALUATION**

A Escola Superior de Tecnologia da Saúde de Lisboa tem o direito, perpétuo e sem limites geográficos, de arquivar e publicar esta dissertação através de exemplares impressos reproduzidos em papel ou de forma digital, ou por qualquer outro meio conhecido ou que venha a ser inventado, e de a divulgar através de repositórios científicos e de admitir a sua cópia e distribuição com objectivos educacionais ou de investigação, não comerciais, desde que seja dado crédito ao autor e editor e que tal não viole nenhuma restrição imposta por artigos publicados que estejam incluídos neste trabalho.

AGRADECIMENTOS

Em primeiro lugar gostaria de agradecer à Fundação Champalimaud, na pessoa do Dr. Nuno Pimentel por ter acreditado neste projeto desde início e permitir a recolha de dados no serviço de radioterapia – obrigado pelo voto de confiança.

Queria agradecer à técnica coordenadora Graça Coelho, por tantas vezes ter tido paciência para o agendamento dos doentes que seriam incluídos na amostra do projecto. Um agradecimento também à equipa de radioterapeutas da TAC, que em muito me ajudaram e tiveram o cuidado, de fazer a “minha” aquisição de imagens, mesmo quando eu não pude estar presente.

Gostaria de agradecer também a preciosa ajuda da Dra Paula, que me ensinou tudo o que foi necessário para este projecto, no que diz respeito ao contorno de volumes, e agradecer-lhe também a motivação que me deu.

Queria deixar um agradecimento geral ao departamento de física, por me responderem a todas as questões que fui colocando ao longo do projecto e por se mostrarem sempre tão disponíveis. Agradeço também ao Eng. Joep Stroom por me ter dado noções básicas e por me ter resolvido alguns ‘acidentes de percurso’.

Agradecer em especial à Eng. Sandra Vieira, por aceitar este desafio, por ter dispensado tanto tempo para me ensinar a planear e ter tanta paciência para o meu projeto – obrigado por me ter ‘acolhido’ tão bem e por estar sempre tão presente.

Agradeço à minha orientadora Prof. Margarida Eiras pela disponibilidade mostrada e pelos conselhos dados ao longo da elaboração deste projeto.

Agradeço também a todos os profissionais do serviço de radioterapia do Hospital da Luz de Setúbal, por se terem mostrado sempre tão disponíveis em ajudar-me e por serem um exemplo a seguir de profissionalismo.

Aos meus pais e à minha irmã, que incutiram em mim os valores que considero importantes na realização deste projecto: o esforço e a dedicação para o poder terminar. A eles agradeço o apoio que me deram desde o início deste mestrado.

Aos meus amigos, que reclamaram o tempo que dispensei para este projeto dando-me forças para continuar com o espírito positivo.

A todos os que foram importantes para esta etapa, o meu mais sincero obrigado.

“Your work is going to fill a large part of your life, and the only way to be truly satisfied is to do what you believe is great work. And the only way to do great work is to love what you do.

If you haven't found it yet, keep looking. Don't settle. As with all matters of the heart, you'll

know when you find it.”

Steven Paul Jobs

RESUMO

A radioterapia estereotáxica (SBRT) tem mostrado bons resultados no tratamento do cancro do pulmão. O movimento respiratório dos órgãos depende do doente, da posição dos braços e da imobilização. Esta pode ser feita com ou sem a ajuda de acessórios como o compressor abdominal que quando os tumores são localizados nos lobos inferiores e perto do diafragma se torna vantajoso, mas se for colocado com elevada pressão pode aumentar o movimento respiratório. O posicionamento sem acessórios rígidos de imobilização deve ser acompanhado de imagens diárias para minimizar os erros de *set-up* e ter uma elevada precisão no volume a irradiar. O objectivo deste estudo é fazer uma avaliação dosimétrica de planeamentos de SBRT com arcoterapia volumétrica de intensidade modulada (VMAT) em dois posicionamentos diferentes: braços para cima e braços ao longo do corpo. Numa amostra de quatro doentes, para cada posicionamento foram adquiridas imagens de Tomografia Computorizada (TC) e imagens de quatro Dimensões de Tomografia Computorizada (4DCT) e tendo sido feita uma reconstrução *mid-ventilation*. Foram estudadas várias variáveis, entre as quais, volumes e doses para os volumes-alvo e órgãos de risco e unidades monitor. Não foram encontradas diferenças significativas entre as variáveis estudadas. Podendo concluir-se que o posicionamento do doente deve ser escolhido de acordo com as suas dificuldades, devendo ser confortável, estável e reprodutível. Em alguns casos, e em doentes em que o movimento respiratório seja de grande amplitude, o posicionamento com os braços ao longo do corpo pode ter a vantagem de diminuir o movimento respiratório e consequentemente o volume alvo interno (ITV).

Palavras-chave: radioterapia esterotáxica (SBRT); cancro do pulmão; imobilização do alvo; posicionamento; posição dos braços.

ABSTRACT

Stereotactic Body Radiation Therapy (SBRT) has been shown good results in lung cancer patients. Respiratory motion of internal organs depends on patient, arms position and the type of immobilization devices used. For patient immobilization can be used rigid fixation devices or not. Abdominal compression can be advantageous for lung tumors in lower lobe or close to diaphragm, but if placed with too much pressure it can increase tumor motion and target volume. Without rigid fixation devices daily images are important to minimize set up errors and have high precision in the irradiated volume. The aim of this study is to evaluate dosimetric SBRT plans with Volumetric Modulated Arc Therapy (VMAT) in different positions: arms up and arms down. Four SBRT lung cancer patients were included in the sample. A Computed Tomography (CT) and a four-Dimensional Computed Tomography (4DCT) was acquired and a mid-ventilation was reconstructed. The analyzed variables were volumes, doses – targets and organs at risk – and total of monitor units (the sum of all arcs). No statistically significant differences were found between the studied variables. Patient position should be chosen according to patients' difficulties and comfort in order to make a comfortable, stable and reproducible position. In patients with a large respiratory motion amplitude, position with arms down can have advantages because respiratory motion decreases, decreasing the margins for internal target volume (ITV).

Key-words: SBRT; lung cancer; target immobilization; patient position; arms position; arms up; arms down.

Índice geral

Introdução geral	1
Stereotactic Body Radiation Therapy in lung cancer: patient positioning and target immobilization – a literature review	2
1. Introduction	2
2. Materials and Methods	3
3. Results	3
3.1 Intrafraction tumor motion	3
3.2 Patient Positioning	4
3.2.1 Rigid fixation devices	4
3.2.2 Non rigid fixation devices	6
4. Discussion	6
5. Conclusion	7
6. References	7
Stereotactic Body Radiation Therapy in lung cancer: arms ups vs. arms down - a dosimetric evaluation	12
1. Introduction	12
2. Materials and Methods	13
2.1 Patient eligibility	13
2.2 Patient immobilization and CT acquisition	14
2.3 Midventilation reconstruction process	14
2.4 Contouring organs at risk and target volume	15
2.5 VMAT plans	15
2.6 Evaluation criteria and statistical analysis	16
3. Results	16
3.1 Patients tumors and anatomic characteristics	16
3.2 Statistical results	17
4. Discussion	18
5. Conclusion	19
6. References	19
Conclusão geral	27

Índice de tabelas

Stereotactic Body Radiation Therapy in lung cancer: patient positioning and target immobilization – a literature review

Table 1 - Summary of the most important criteria in the analyzed studies 11

Stereotactic Body Radiation Therapy in lung cancer: arms ups vs. arms down - a dosimetric evaluation

Table 1 - Organs at risk contoured for each patient 24

Table 2 - SBRT dose tolerance limits (Timmerman, 2011) 24

Table 3 - Mean values for the percentage of lung volume receiving xGy 25

Table 4 - Total of monitor units per patient, mean, standard desviation and p-value 26

Índice de figuras

Stereotactic Body Radiation Therapy in lung cancer: arms ups vs. arms down - a dosimetric evaluation

Fig. 1 - Research process: steps for all patients	23
Fig. 2 - Mid-ventilation reconstruction process	23
Fig. 3 - Contouring - a) Ring b) PTVcal: the sum of PTV1, PTV2 and PTV3	24
Fig. 4 - Target position in each respiratory phase in L-R (left-right), I-S (inferior-superior) and A-P (anterior-posterior) directions a) arms up b) arms down	25
Fig. 5 - Dmax, Dmean and Dmin for each patient and all patient mean doses	25
Fig. 6 - Total of monitor units: the variability of data	26

Introdução geral

O cancro do pulmão é um dos cancros com maior taxa de mortalidade, a nível mundial. Para esta patologia, existem várias terapêuticas, sendo a cirurgia a terapêutica mais recomendada. Muitas vezes existem co-morbilidades por parte do doente, ou até localizações anatómicas que a tornam impossível de executar. Nestes casos, são analisadas outras opções terapêuticas como a quimioterapia e/ou radioterapia. A radioterapia é um tratamento alternativo para tumores inoperáveis e para metástases. A radioterapia estereotáxica (SBRT) é uma técnica que utiliza o escalonamento de dose para um maior controlo tumoral. Esta, tem como principal característica a dose biológica efectiva (BED), pois é administrada ao doente uma elevada dose num curto período de tempo, 1 a 5 frações, enquanto minimiza a dose nos tecidos adjacentes, sendo feita através de uma alta precisão no alvo, doses conformacionais e consequentemente um elevado fall-off de dose. Deste modo, o posicionamento e a sua reprodutibilidade assumem uma elevada importância, podendo ser executáveis através de dispositivos de imobilização rígidos ou não-rígidos. Apesar disto, a posição dos braços continua um tema por estudar. O posicionamento e o conforto do doente tornam-se aspetos muito importantes na utilização de técnicas que administram uma elevada dose. O doente deve estar posicionado confortavelmente com a ajuda dos acessórios de posicionamento onde o seu peso deve ser distribuído uniformemente durante. O posicionamento standard utilizado para tumores do pulmão é a colocação dos braços para cima, contudo, este nem sempre é possível devido às co-morbilidades dos doentes. Neste seguimento, o posicionamento é feito com os braços para baixo, surgindo a necessidade de estudar o tema, através de uma comparação dosimétrica, feita em doentes com tumores de pulmão. Para isso foram comparados planeamentos com a técnica arcoterapia volumétrica de intensidade modulada (VMAT) aplicando uma fracção única de 24Gy.

O objetivo deste projecto de investigação é fazer uma revisão de literatura que enquadre a importância do posicionamento em tumores do pulmão, assim como, perceber se o posicionamento com os braços para baixo pode ser uma opção de posicionamento sem prejuízo para a qualidade/características dosimétricas do planeamento.

Os artigos que se seguem foram construídos em inglês com vista a serem publicados em revistas internacionais da área e por este motivo, são os únicos elementos em língua estrangeira.

Stereotactic Body Radiation Therapy in lung cancer: patient positioning and target immobilization – a literature review

Cátia Barreira¹; Margarida Eiras, PhD²;

¹Student of master: Radiations Applied to Health Technologies – Radiation Therapy

Corresponding author: catiabarreira@hotmail.com

²Escola Superior de Tecnologias da Saúde de Lisboa

Abstract: Lung cancer is the leading cause of cancer-related deaths worldwide. Radiotherapy is an alternative treatment for inoperable tumors and also for patients with slow growing metastatic lung tumors. Dose escalation has been an important issue to improve local tumor control and overall survival. Stereotactic Body Radiation Therapy has been gaining a large interest over the past few years, using high dose per fraction, sharp dose gradients and high-precision target localization. Respiratory motion of internal organs depends on patients, arms patient position and the type of immobilization devices used. Patient immobilization can be enforced with or without rigid fixation devices. Abdominal compression can be advantageous for lung tumors in lower lobe or close to diaphragm, but if placed with too much pressure it can increase tumor motion and target volume. Despite of this we can conclude that all positions have advantages. Without rigid fixation devices daily images are important to minimize set up errors to have high precision in the irradiated volume. With technology available in the treatment room and with advanced treatment planning systems, a question for the future can be made “Are arms above head, in lung cancer patients, the only option to achieve a good dosimetric plan?”

Keywords: SBRT; lung cancer; patient immobilization; respiratory motion; arm position.

1. Introduction

Lung cancer is the leading cause of cancer-related deaths worldwide.¹ Surgery remains the treatment of choice but many patients are inoperable due to their compromised pulmonary reserve, cardiac function, or significant co-morbidities.²⁻⁵ Radiotherapy is an alternative treatment for inoperable tumors and also for patients with slow growing metastatic lung tumors.⁶ Traditionally this treatment has a total dose of 50-70 Gy in 1.8-2 Gy per fraction.^{2,4,6} Dose escalation has been important to improve local tumor control and overall survival.^{4,6} However, dose escalation by conventional fractionated radiotherapy has the risk of increasing normal tissue toxicity.⁶ Stereotactic Body Radiation Therapy (SBRT) has been gaining a large interest over the past few years, in small target volumes because uses high doses in 1-5 fractions and increases the local control.^{2,7,8} This technique also uses sharp

dose gradients and high-precision target localization (image in the treatment room).^{2,5,8,9} To reduce uncertainties in targeting, important technical considerations in SBRT include:¹⁰

- 1) stable and reproducible patient positioning;
- 2) high-quality imaging for treatment planning;
- 3) accurate target and Organs At Risk delineation (OAR);
- 4) advanced treatment planning algorithms;
- 5) image-guidance systems capable of performing in the sub-millimeter range;
- 6) robust quality assurance methods.

Excessive intra-fraction patients' motion compromise target and OAR dose distribution.¹⁰ Two important factors are patients' position and immobilization. This literature review has the aim to enlighten the major issues in patient position/target immobilization in lung cancer patients.

2. Materials and methods

For this review, the main databases specialized in systematic reviews were used: B-ON, PubMed, SciELO, Cochrane Library, Research Gate and RCIPL (Scientific Repository produced by Instituto Politécnico de Lisboa). The first search was made with the key words – SBRT; lung cancer; patient immobilization; patient position - and sixty-six articles were found. After reading all the abstracts eighteen articles were selected. From these articles the references were analyzed and twelve more articles were added. In total thirty articles were included in this literature review, five of them were already literature reviews and were included because it add value to this review. There was no filter applied in terms of time line because SBRT is a relatively recent technique, neither in terms of patient follow-up. For that, inclusion criteria were:

- 1) Treatment type: SBRT;
- 2) Patient type: only patients with primary or metastatic lung cancer;
- 3) Results measurements: dosimetric data from comparison of distinct positions, tumor tracking and immobilization; respiratory motion.

Scientific literature published between January 1999 and June 2015, was systematically reviewed. Table1 shows summary of the most important criteria found in the analyzed articles.

3. Results

3.1 Intrafractional tumor motion

At rest, a healthy person breathes 12 to 15 times per minute. Respiratory motion, volume and frequency – in the same person – can change with biochemical conditions, body position, abdominal contents and emotional conditions.^{11,12} Respiratory muscles motion is

also altered by pathological conditions as pleural adhesion after pleuritis, thoracic surgery, thoracic irradiation, diabetes mellitus, hypothyroidism, chest pain, malnutrition and muscle fatigue. Respiratory motion of internal organs depends on body's position, arms' position and the type of immobilization devices used.

Inspiration requires contraction of diaphragm and external intercostal muscles located between the ribs. Diaphragm contraction causes it to move downward and increases vertical dimension of thoracic cavity. Diaphragm contraction produces a 75% change in intra-thoracic volume during resting inspiration. External intercostals contract to elevate lower ribs and push the sternum outward, increasing the anteroposterior dimension of thoracic cavity. Lung volume is different between inspiration and expiration at the same pressure. In voluntary active expiration, internal intercostal muscles contract and pull the rib cage downward, and abdominal muscles increase abdominal pressure which forces the diaphragm up.¹¹ Many authors studied the mean amplitude in superior-inferior (SI) direction and found that tumors in lower lobes and not attached to rigid structures had a larger motion than tumors in upper-lobe.¹¹⁻¹³ Plathow et al. studied safety margins of 3.4mm for tumors in upper region, 4.5mm for middle region and 7.2mm for lower region.¹³ Shirato et al. showed that cardiac motion influence in tumor motion between 1 to 4 mm in left-right (LR) axis and 1 to 2 mm in remaining axis.¹¹ Factors as comorbidities, performance status, age and gender can influence intrafractional target shifts. It is known that patients older than seventy-five had larger shifts during treatment and the male patients had larger shifts than females.^{5, 14,15}

3.2 Patient positioning

The most important SBRT characteristic is delivery of higher biologic effective dose (BED) over a shorter period of time, while minimizing normal tissue exposure to high dose radiation.^{9,16,17} That is only possible with two major characteristics: patient position and image guided systems in the treatment room. Position should offer comfort to patients, reproducibility and accuracy to treatment. Patient immobilization can be enforced with commercially available devices – rigid fixation devices - e.g. stereotactic frames, vacuum systems or thermoplastic masks to reduce set-up uncertainties^{12,18} or without rigid devices to immobilize the patient but with motion-controlled treatment systems.^{2,5,14,17}

3.2.1 Rigid fixation devices

Several articles reported patient position with stereotactic frame. One of the most important steps in patient positioning for SBRT is ensuring that patients are comfortably immobilized in the frame, the weight has to be uniformly distributed and supported to avoid patient's tendency to readjust his weight during treatment.¹⁹ Authors concluded that a frame-based

position allows a simple and effective tumor motion control^{8,18,19} and a better target position accuracy.^{4,16} Waldeland et al. analyzed thirty patients positioned with stereotactic frame and abdominal compression, showed that conventional margins applied to the tumor were sufficient to cover the Internal Target Volume (ITV) by the prescription dose.²⁰ Gutierrez et al. showed with twenty lung cancer patients that both BodyFix® and Body Pro-Lok™ systems were user-friendly, fast to position and immobilize the patient providing reproducible, accurate and efficient positioning.^{8,21} Shah et al. concluded that stereotactic frame is more accurate than other position devices, saying that with stereotactic frame a 5 mm target margin appear adequate to incorporate ITV but do not appear to be sufficient for BodyFix® immobilization.⁴

Abdominal compression

Abdominal compression plate is placed on patient's abdomen 3 to 4 cm below the costal margin of the ribs and below the xiphoid. The placement of this compressor is critical, if it is placed in a superior position it can be a potential to fracture ribs if enough pressure is applied and if it is placed too low it is less effective in decreasing diaphragm motion.¹⁹ Several authors reported the advantage of using the abdominal compression,^{9,16,22} reinforcing it as a major advantage in tumors in the lower lobes^{2,12,16,23} and in lesions close to the diaphragm. If tumors are large enough, abdominal compression can be associated with an interesting ITV reduction. For other lobes, the compressor can provide a smaller benefit or even induce unwanted effects such as larger tumor motion and ITV increase.^{3,12,24,25} That is why most of the authors reported that abdominal compressor should be used only when it adds advantages to tumor motion control.^{12,23} Negoro et al. showed with eighteen patients, that the tumor motion decreases from 8-20mm to 2-11mm with abdominal compression and stereotactic frame. They concluded that this immobilization had the disadvantage not to detect patients rotation along the body axis.²² Han *et al.* found that abdominal compression is superior reducing SI and overall respiratory tumor motion and it is faster in set-up time and more comfortable, than *BodyFix*®. Intrafraction tumor motion had no significant difference between three positions.²

Thermoplastic masks

Despite of being a usual positioning device in head and neck cancer, in thoracic cancer it is not very common to use thermoplastic masks. Aoki et al. analyzed twenty patients (T₁₋₂N₀M₀ and tumor respiratory movement no more than 10mm) position with both arms raised and immobilized with a mask with a custom-made head rest. These authors concluded that, for SBRT with a 54 Gy total dose in nine fractions, this position can be an alternative for lung cancer patients because they can achieve an acceptable tumor motion control.²⁶ Other

authors compared vacuum cushions and thermoplastic masks in 73 fraction, 246 CBCT images analyzed and their results showed that thermoplastic mask can offer a better and easier reproducibility and significantly less intrafraction set up displacements, when compared with vacuum cushions.¹⁶

3.2.2 Non rigid fixation devices

With the technology used in the treatment room, some authors argue that positioning can be changed and made it simple for the patient.^{2,5,14,17} Authors observed that a rigid tight whole body immobilization can cause a certain patient discomfort during treatment and that can cause patient movement.^{14,15} Several articles analyzed showed that the image before, during and or after treatment can improve the shift results using a simple position without stereotactic frame.^{2,5,6,27} Alderliesten et al. concluded with thirty-six patients that the accuracy found for 3D surface imaging system is sufficient for monitoring intrafraction tumor motion purposes in frameless SBRT for female patients.⁵ Dachele et al. studied thirty patients with their arms above head and a foam to support their knees, with Real-time Position Management (RPM) and treatment planning with Volumetric Modulated Arc Therapy (VMAT). In this study they concluded that it is possible to make a stable position without rigid immobilization for SBRT patients.¹⁰ Sonke et al. treated sixty-six tumors without a rigid immobilization and with free breathing, reported that this positioning can be precise when treatment is guided with 4D-CBCT. These authors concluded that the use of alpha cradle and the body frame increase skin dose and are logistically more challenging than a non-rigid positioning.¹⁷ Shen et al. showed a major role of Active Breathing Control (ABC) even with frame positioning. Respiratory tumor motion was less than 3mm, but without ABC technique helping to control tumor motion they recommend a uniform PTV margin of 5mm axial and 10mm SI to be added for stereotactic lung radiotherapy when image guidance is not used.⁶ This conclusion it is supported also by other authors.^{28,29}

4. Discussion

To irradiate the tumor precisely and to decrease irradiated volume of OAR, various methods have been developed. The American Association of Physicists in Medicine classified five major categories:³⁰

- 1) Motion-encompassing method;
- 2) Respiratory-gating method;
- 3) Breath-hold method;
- 4) Forced shallow-breathing with abdominal compression method;
- 5) Real-time tumor-tracking method.

This shows the importance of considering both patient, target tumor and motion-management strategy for high-precision radiotherapy.¹⁰ In various articles the conclusions about respiratory tumor motion are very enlightening. Tumors in lower lobes had the largest variations and in these tumors abdominal compression has advantages decreasing tumor respiratory motion, if it is well placed, because of that, abdominal compression should be evaluated during the CT scan, otherwise it can increase respiratory tumor motion.

Patient position should have a balance between patient comfort, accuracy and reproducible position for treatment, if these parameters aren't accomplished we can compromise the treatment and increase set up errors. Before, SBRT was done only with stereotactic frame, after many position studies rigid position can be replaced to a simple positioning. Balance between patients' position and use of rigid devices need to take into account the type of image technology available in the treatment room. For example, a non-rigid positioning is acceptable when image acquisition is daily.

5. Conclusion

Despite of this we can conclude that all positions have advantages but it is important in SBRT minimize set up errors and have high precision in the irradiated volume.

In lung cancer patients, one of the most important issue is patient performance status, and the positioning should be adapted according patient limitations. With that and technology available in the treatment room, a question for the future can be made "Are arms above head, in lung cancer patients, the only option to achieve a good dosimetric plan?"

6. References

1. Parkin DM, Bray F, Ferlay J, Pisani P. Global cancer statistics, 2002. *A Cancer Journal to Clinicians* 2005;55: 74–108.
2. Han K, Cheung P, Basran P, Poon I, Yeung L, Lochray F. A comparison of two immobilization systems for stereotactic body radiation therapy of lung tumors. *Radiotherapy and Oncology*. 2012; 95: 103-108.
3. Richmond N, Pilling K, Peedel C, Shakespeare D, Walker C. Positioning accuracy for lung stereotactic body radiotherapy patients determined by on-treatment cone-beam CT imagin. *The British Journal of Radiology*. 2012; 85:819-823.
4. Shah C, Grills I, Kestin L, McGrath S, Ye H, Martin S, *et al.*. Intrafraction variation of mean tumor position during image-guided hypofractionated stereotactic body radiotherapy for lung cancer. *Int. J. Radiation Oncology Biol. Phys.* 2012; 82(5): 1636–1641.

5. Alderliesten T, Sonke J, Betgen A, Vliet-Vroegindeweij C, Remeijer P. 3D surface imaging for monitoring intrafraction motion in frameless stereotactic body radiotherapy of lung cancer. *Radiotherapy and Oncology*. 2012; 105: 155-160.
6. Shen Y, Zhang H, Wang J, Zhong R, Jiang X, Xu Q, *et al.*. Hypofractionated radiotherapy for lung tumors with online cone beam CT guidance and active breathing control. *Radiation Oncology*. 2010; 5: 19-28
7. Qiao X, Tullgren O, Lax I, Sirzén F, Lewensohn R. The role of radiotherapy in treatment of stage I non-small cell lung cancer. *Lung Cancer* 2003;41:1–11.
8. Gutiérrez A, Stathakis S, Crownover R, Esquivel C, Shi C, Papanikolaou N. Clinical evaluation of an immobilization for stereotactic body radiotherapy using helical tomotherapy. *Medical Dosimetry*. 2011; 36(2): 126-129.
9. Li W, Purdie TG, Taremi M, Fung S, Brade A, Cho BCJ, *et al.*. Effect of Immobilization and performance status on intrafraction motion for stereotactic lung radiotherapy: analysis of 133 Patients. *Int. J. Radiation Oncology Biol. Phys.* 2011; 81(5): 1568–1575.
10. Dahele M, Verbakel W, Cuijpers J, Slotman B, Senan S. An analysis of patient positioning during stereotactic lung radiotherapy performed without rigid external immobilization. *Radiotherapy and Oncology*. 2012; 104: 28-32.
11. Shirato H, Seppenwoolde Y, Kitamura K, Onimura R, Shimizu S. Intrafractional tumor motion: lung and liver. *Seminars in Radiation Oncology*. 2004; 14 (1) 10–18, 2004.
12. Bouilhol G, Ayadi M, Rit S, Thengumpallil S, Schaerer J, Vandemeulebroucke J, *et al.*. Is abdominal compression useful in lung stereotactic body radiation therapy? A 4DCT and dosimetric lobe-dependent study. *Physica Medica*. 2013; 29(4): 333–340.
13. Plathow C, Ley S, Fink C, Puderbach M, Hosch W, Schmähel A, *et al.*. Analysis of intrathoracic tumor mobility during whole breathing cycle by dynamic MRI. *Int. J. Radiation Oncology Biol. Phys.* 2004; 59: 952-959
14. Liu H, Khan R, Nugent Z, Krobutschek K, Dunscombe P, Lau H. Factors influencing intrafractional target shifts in lung stereotactic body radiation therapy. *Practical Radiation Oncology*. 2014; 4: 45-51.
15. Watanabe M, Onidhi H, Kuriyama K, Komiyama T, Marino K, Araya M, *et al.*. Intrafractional set up errors in patients undergoing non-invasive fixation using an immobilization system during hypofractionated stereotactic radiotherapy for lung tumors. *Journal of Radiation Research*. 2013; 54: 762-768.
16. Navarro-Martin A, Cacicedo J, Leaman O, Sancho I, Garcia E, Navarro V, *et al.*. Comparative analysis of thermoplastic mask versus vacuum cushions in stereotactic body radiotherapy. *Radiation Oncology*. 2015; 10: 176-182.

17. Sonke J, Rossi M, Wolthaus J, van Herk M, Damen E, Belderbos J. Frameless stereotactic body radiotherapy for lung cancer using four-dimensional cone beam CT guidance. *Int. J. Radiation Oncology Biol. Phys.* 2009; 74: 567–574.
18. Zhou J, Uhl B, Dewitt K, Young M, Taylor B, Fei D, *et al.*. Image-guided stereotactic body radiotherapy for lung tumors using bodyloc with omotherapy: clinical implementation and set-up accuracy. *Medical Dosimetry.* 2010; 35(1): 12–18.
19. Murray B, Forster K, Timmerman R. Frame-based immobilization and targeting for stereotactic body radiation therapy. *Medical Dosimetry.* 2007; 32(2): 86-91.
20. Waldeland E, Ramberg C, Arnesen M, Helland A, Brustugun O, Malinen E. Dosimetric impact of a frame-based strategy in stereotactic radiotherapy of lung tumors. *Acta Oncologica.* 2012; 51: 603-609.
21. Baba F, Shibamoto Y, Tomita N, Ikeya-Hashizume C, Oda K, Ayakawa S, *et al.*. Stereotactic body radiotherapy for stage I lung cancer small lung metastasis: evaluation of an immobilization system for suppression of respiratory tumor movement and preliminary results. *Radiation Oncology.* 2009; 4:15.
22. Negoro Y, Nagata Y, Aoki T, Mizowaki T, Araki N, Takayama K, *et al.*. The effectiveness of an immobilization device in conformal radiotherapy for lung tumor: reduction of respiratory tumor movement and evaluation of the daily setup accuracy. *Int. J. Radiation Oncology Biol. Phys.* 2001; 50(4): 889-898.
23. Dobashi S, Sugane T, Mori S, Asakura H, Yamamoto N, Kumagai M, *et al.*. Intrafractional respiratory motion for charged particle lung therapy with immobilization assessed by four-dimensional computed tomography. *Journal of Radiation Research.* 2011; 52: 96-102.
24. Foster R, Meyer J, Iyengar P, Pistenmaa D, Timmerman R, Choy H, *et al.*. Localization Accuracy and Immobilization Effectiveness of a Stereotactic Body Frame for a Variety of Treatment Sites. *Int. J. Radiation Oncology Biol. Phys.* 2013; 87(5): 911-916.
25. Hansen A., Petersen J., Hoyer M.; Internal movement, set-up accuracy and margins for stereotactic body radiotherapy using a stereotactic body frame. *Acta Oncologica.* 2006; 45: 948-952.
26. Aoki M, Abe Y, Kondo H, Hatayama Y, Kawaguchi H, Fujimori A, *et al.*. Clinical outcome of stereotactic body radiotherapy of 54 Gy in nine fractions for patients with localized lungtumor using a custom-made immobilization system. *Radiat Med.* 2007; 25: 289-294.
27. Peguret N, Dahele M, Cuijpers J, Slotman B, Verbakel W. Frameless high dose rate stereotactic lung radiotherapy: intrafraction tumor position and delivery time. *Radiotherapy and Oncology.* 2013; 10: 419-422.

- 28.** Lim D, Yi B, Mirmiran A, Dhople A, Sunthalingam M, D'Souza W. Optimal beam arrangement for stereotactic body radiation therapy delivery in lung tumors. *Acta Oncologica*. 2010; 49: 219-224
- 29.** Nevinny-Stickel M, Sweeney R, Bale R, Posch A, Auberger T, Lukas P. Reproducibility of patient positioning for fractionated extracranial stereotactic radiotherapy using a double-vacuum technique. *Strahlenther Onkol* 2004, 180:117-122.
- 30.** American Association Physicists in Medicine. The management of respiratory motion in radiation oncology. *AAPM Reports*. 2006. 91.

Table 1 - Summary of the most important criteria in the analyzed studies

<u>Criteria</u>	<u>Number of studies</u>
Sample size:	
- n < 30	11
- n ≥ 30	14
- Reviews	5
Type of study:	
- Comparative	8
- Descriptive	22
Main theme:	
- Patient positioning	12
- Target immobilization	9
- Patient positioning and Target immobilization	9
Total:	30

Stereotactic Body Radiation Therapy in lung cancer: arms up vs. arms down - a dosimetric evaluation

Cátia Barreira,¹ Margarida Eiras,² Sandra Vieira,³ Paula Buitrago,³ Graça Coelho,³
Nuno Pimentel,³ Carlo Greco³

¹Student of master: Radiations Applied to Health Technologies – Radiation Therapy

Corresponding author: catiabarreira@hotmail.com

²Lisbon School of Health Technology

³Radiation Oncology Department, Champalimaud Foundation for the Unknown - Lisbon

ABSTRACT

Aim: The aim of this study is to evaluate dosimetric Stereotactic Body Radiation Therapy (SBRT) plans with Volumetric Modulated Arc Therapy (VMAT) in lung cancer with different positions: arms up and arms down.

Materials and methods: Four SBRT lung cancer patients (2 males and 2 females) were included in the sample. A Computed Tomography (CT) and a four-Dimensional Computed Tomography (4DCT) was acquired and a mid-ventilation was reconstructed for each position. The analyzed structures were: volumes – CTV, ITV, PTV and organs at risk (OARs), maximum dose (Dmax), mean dose (Dmean) and minimum dose (Dmin); OARs - Dmax, Dmean and the dose received by the volume (cc) specified by the constraints; V_{10Gy} , V_{15Gy} and V_{20Gy} – as the volume receiving (x) Gy for the lung; Total of monitor units (the sum of all arcs); Volume that received 6, 12, 18 and 20.4 Gy.

Results: No statistically significant differences were found, but the following values were lower with arms up: target volumes, heart volume; lung total - Dmean; spinal cord - the dose received by 1.2 cc; the volume that received 6, 18 and 20.4 Gy and the spherical diameter of the volume that received 18 Gy. The lung volumes –right, left and total- were lower with arms down.

Findings: There were no statistical differences between plans, despite of the position with arms down having more tissue irradiated, that doesn't compromise PTV coverage and it doesn't mean more dose in OAR. Patient position should be chosen according to patients' difficulties and comfort in order to make a stable and reproducible position.

Keywords: SBRT; lung cancer; patient positioning; arms up; arms down; dosimetric evaluation

1. Introduction

Stereotactic Body Radiation Therapy (SBRT) is an effective alternative for inoperable early stage lung cancer and lung metastases.¹⁻⁴ SBRT delivery high doses in 1-5 fractions to improve local tumor control.^{1,5} The most important SBRT characteristic is higher biologic effective dose (BED) over a short period of time, while minimizing the normal tissue exposure.^{4,6-11} This technique can only be done with high target precision, reduced tumor

margins, high conform prescription dose, sharp dose fall-off away from the target, as well as mechanical requirements such as rigid immobilization and accurate patient positioning.^{3,4} Typically a four-Dimensional Computed Tomography (4DCT) is used to estimate target motion.⁵ The 4DCT is a correlation between Computed Tomography (CT) image acquisition with breathing cycle, to analyze the variables that affect respiratory motion which allows to contour the target margins.^{4,5,12} Minimizing normal tissue irradiation in SBRT by using 4DCT scans can reduce the risk of late normal tissue toxicity associated with hypofractionated SBRT schemes.¹² The success of SBRT is based on accurate treatment planning and accurate treatment delivery. In lung cancer different uncertainties have been described, which can reduce the treatment accuracy.^{4,13} Patient immobilization can be achievable with rigid devices like stereotactic frame or vacuum systems^{1,3,14,15} or can be achievable with non-rigid devices.^{7,16-18} Arm position remains an unexplored area of research. While most lung cancer patients are treated with their arms up, many are frail and unable to comfortably maintain this position. It has been assumed that plans with beams entering through the arms are suboptimal and also particularly sensitive to arm repositioning variability.¹⁹ With Volumetric Modulated Arc Therapy (VMAT) it is possible to avoid the angle irradiation where arms could be included in the beam. It is possible that treating with arms down might improve patient stability and comfort, which decreases movement during setup and treatment, leading to improved dosimetric accuracy, and that adverse dosimetry of beams entering through the arms would be ameliorated by an arc geometry.¹⁹

The aim of this study is to understand if it is possible to have a SBRT-VMAT dosimetric plan with arms down that achieve the same dosimetric goals as the plan with arms up.

2. Materials and Methods

2.1 Patient eligibility

Since February to May 2016 all lung cancer patients with medical indication for SBRT were followed. Patients were excluded for the sample:

- 1) Patients with nasogastric tubes;
- 2) Patients that planning images were acquired only in the PET-CT (Positron Emission Tomography-Computed Tomography) – software reconstruction problems;
- 3) Patients without the 4DCT well reconstructed.

All four patients in the sample (2 males and 2 females) went through a process where many steps were taken (fig.1).

2.2 Patient immobilization and CT acquisition

The first step in patient position for SBRT is ensuring that patients are comfortably immobilized in the position that they will be treated. A comfortable immobilization is when patient's weight is uniformly distributed and supported.²⁰ All four patients were positioned with an arm support which provides comfort to patients' upper body. This device has a headrest and an arms support that can be changed in order to adapt to patients' anatomy. An abdominal compression was applied by an inflatable abdominal compressor that was placed approximately 3 to 4 cm below the costal margin of the ribs and inferior to the xiphoid. This compressor was inflated to have a comfortable pressure, balancing the fact that too much pressure will increase respiratory motion amplitude. For that, pressure was adapted for each patient. Patients were instructed to have a free breathing during image acquisition, and to avoid deep respiratory or breath-hold movements. All the CT were acquired with *Philips Brilliance Big Bore (software version 2.4.10)*. Respiratory cycle signal was monitored with *Bellows System (Philips Medical Systems)* a non-metallic system to avoid image artifact. This system uses an elastic strap that was attached above the abdominal compressor at the xiphoid to record the respiratory signal. Thoracic movement with respiration was detected by a sensor and this generates a waveform signal that represents the respiratory cycle. The software has graphical information about patients' respiratory cycle and acquires images in 10 respiratory cycles - 10 phases. Reconstruction is automatically made by Philips software. The phases were defined as 0% to 100%, that means each phase represents 10% of acquired respiratory motion and each phase has the same number of slices, nearly 150 slices. For all patients, the first step was CT acquisition with arms up after that 4DCT was acquired. After this procedure position was change and it was acquired the CT and 4DCT with arms along the body (arms down). In arms down no precautions were taken in terms of reproducibility. After image acquisition, 4DCT images and CT images were analyzed to make sure that they were well reconstructed.

2.3 Mid-ventilation reconstruction process

The major intra-fractional geometrical uncertainties in lung cancer treatment are due to respiratory and cardiac motion.^{21,22} By eliminating these uncertainties, it allows a margin reduction, and it decreases volume of irradiated normal tissue which allows a dose escalation. A single free-breathing CT is often used for radiotherapy planning for lung tumors. However, respiration-induced tumor motion during acquisition causes artifacts in tumor shape and position, because CT acquires a stack of images without time information from the tumor motion, thus obtaining a set of arbitrary snapshots of moving structures. To overcome this problem, time-resolved 4DCT scanning techniques were developed. This set

provides temporal and spatial motion information that can be used to optimize treatment-planning. However, the available commercial treatment-planning systems cannot handle a 4D CT data set as input for treatment-planning.²³ To be able to make a reliable comparison between both CT images (arms up vs. arms down) a mid-ventilation reconstruction was performed to reform the images as they were in the same respiratory cycle position. For each patient the mid-ventilation process was repeated twice, for arms up and for arms down. For both processes the same reference phase was chosen, the steps are represented in fig.2.

2.4 Contouring organs at risk and target volumes

Each patient had two mid-ventilation CT, for both mid-ventilations the same Organs At Risk (OAR) and target volumes were contoured, except for patient2 it was the only patient with humerus contoured, as it is shown in table 1. For target volumes: Clinical Target Volume (CTV), Internal Target Volume (ITV) and Planning Target Volume (PTV) were contoured. All volumes were contoured by the same person to avoid intra and inter-observational errors and contouring variations, corrected by the same Radiation Oncologist. CTV was contoured with both anatomical and biological information (PET). From CTV to ITV one margin of 2 mm isotropically was added, to account for residual errors in patient position. But, as we know tumor respiratory motion is likely to be anisotropic,²⁴ after analyzing and measuring respiratory motion in 4DCT, margins were changed in the directions where movement was larger than 2 mm. PTV was created from ITV adding a symmetric margin of 3 mm. A ring-shaped volume was created in all patients to achieve a conformational dose around PTV, it was created automatically from PTV with a 20 mm and 5 mm outer margin from PTV (fig.3a). For patient1 a volume (PTVcalc) was created through the sum of three PTVs (fig.3b). For patient 3 and 4, PTV included OARs and, for them a PTVcal was created, an automatic subtraction of OAR from PTVs.

2.5 VMAT plans

Rapidarc[®](Varian) is a relatively recently introduced VMAT technique based on simultaneous optimization of Multi-Leaf Collimator (MLC) shapes, dose rate and gantry rotation speed. In this article, VMAT is defined as a technique with the characteristics above-mentioned.

The first step was to create a plan and specify if plan intention: curative. After this, the number of fractions and total dose needed to be defined, as well as the machine to treat this plan – *TrueBeam*[®](Varian). Dose prescription was 24 Gy in one fraction, for all patients. The energy defined was 10 MV - FFF (Flattening Filter Free) with dose rate of 2400 MU/min. In this study, all the dosimetric plans were made with VMAT, arc therapy with continuous radiation delivery is a potentially decreasing treatment time per fraction without

compromising the target coverage. One VMAT advantage is to have a IMRT quality plans delivered in less time, which means a decrease in intrafraction variation. Despite of this, VMAT plans have a major disadvantage – lower doses over a large volume, increasing the probability of second malignancies.^{25,26} In the plans, energy 10 MV-FFF was used because it has the advantage of a higher maximum dose rate of 2400MU/min possible on Varian linear accelerators, compared with 1400MU/min for 6MV-FFF.²⁶ The isocenter was chosen in PTV geometrical center of each CT. After that, arc geometry was defined, as well as the number of arcs - two or four arcs were used. All arcs, collimator and MLC were constructed to fit PTV or PTVcalc. The plan was calculated with the algorithm AAA - Anisotropic Analytical Algorithm (*version 11.0.31*) and were optimize to have the following dosimetric goals:

- 1) To have a good dose coverage - minimum 98% in PTV or PTVcalc;
- 2) To have hotpoints - maximum under 111% - inside CTV;
- 3) To have a 50% and 75% isodoseline uniform around PTV;
- 4) To have all OAR with an acceptable dose according table 2 dose constraints for SBRT-single dose of 24Gy.²⁷

In some plans these characteristics could not be followed, but all the plans were approved by the same physical engineer.

2.6 Evaluation criteria and statistical analysis

The following structures were analyzed:

- 1) Volumes: targets and oars;
- 2) Target: CTV, ITV and PTV – maximum dose (Dmax), mean dose (Dmean) and minimum dose (Dmin);
- 3) OARs: Dmax, Dmean and the dose received by the volume (cc) specified in table 2 (eg: the dose received by the trachea in 4cc);
- 4) V_{10Gy} , V_{15Gy} and V_{20Gy} – as the volume receiving (x) Gy for the lung;
- 5) Total of monitor units (the sum of all arcs);
- 6) Volume that received 6, 12, 18 and 20.4 Gy that represents 25, 50, 75 and 85% of prescribed dose;
- 7) The spherical diameter of the volume above-mentioned.

It was performed by Wilcoxon Test in the statistical program SPSS (*version 22.0*). The p-value less than 0.05 was considered statistically significant.

3. Results

3.1 Patients tumors and anatomic characteristics

-Patient 1: no anatomic differences were found between contoured volumes.

-Patient 2: CTV was in lung upper lobe. The comparison between contoured volumes in both CT scans shows differences: when patients have arms down CTV becomes closer to thoracic wall and brachial plexus is lower. Because of that, there are dose differences in these OAR. Because CTV was in superior lobe, humerus was contoured. When patient has arms down the humerus is lower and receives more dose: Dmax 2.4 vs. 6.3 Gy and Dmean 0.2 vs. 1.5 Gy (arms up vs. arms down).

-Patient 3: no anatomic differences were found between contoured volumes.

- Patient 4: There were no differences between CTV anatomic localization, in both positions and because CTV was in middle lobe. There are differences in amplitude of respiratory motion, as fig.4 shows with the graphic scale. With arms up the scale amplitude is [-6 ; 6] mm and with arms down the scale amplitude is [-0.15 ; 0.30] mm. That difference in the respiratory amplitude can be justified with the fact that the patient was overweight and with arms down it was easier to breathe. For the plan with arms down, an avoidance sector was made like it should be done if the plan was irradiated.

3.2 Statistical results

Comparing the plans, there is no statistically significant differences between all the variables, despite of that, we can conclude:

- 1) Volumes:
 - i. all the target volumes are slightly smaller with arms up (PTV and CTV p-value=0.068 and ITV p-value=0.066);
 - ii. The lungs (right, left and total volume) are slightly smaller with arms down (p-value=0.068)
 - iii. The heart is slightly bigger with arms down (p-value=0.068)
- 2) Targets:
 - i. PTV - Dmin with arms down is slightly lower (fig. 5).
- 3) OARs:
 - i. Lung total volume (the sum of right and left lung) - Dmean had a lower value with arms up (p-value=0.066 and mean=2.9 vs 3.1 Gy);
 - ii. Spinal cord - the dose received by 1.2cc had a lower value with arms up (p-value=0.068 and mean=4.2 vs 5.43 Gy).
- 4) V_{10Gy} , V_{15Gy} and V_{20Gy} - these values are slightly larger when patients are with arms down (table 3).
- 5) Total of monitor units: in three patients the sum of monitor units is larger with the arms up (table 4), but the variability of data and the range larger with the arms up

[8000;13701] make the data with no statistically significant difference (p-value= 0.144 - fig.6).

- 6) Volume that received 6, 18 and 20.4 Gy had a lower value with arms up (p-value=0.068 and mean: 1380.86; 303.4; 6.08; vs 1550.97; 329.93; 263.76 cc respectively).
- 7) The spherical diameter of the volume that received 18 Gy had a lower value with arms up (p-value=0.066 and mean=6.55 vs 6.95 cm).

4. Discussion

The aim of this study is to evaluate dosimetric plans with different arm position and make a comparison between them, to see if it is possible to achieve the same dosimetric goals for both plans. Our results show that, from a statistical standpoint, there were no differences between plans. Despite arms down having more tissue irradiated, this position doesn't compromise PTV coverage and it doesn't mean more dose in OAR.

The type of immobilization devices selected can decrease dose to the target volume and decrease tumor control rate.²⁸ Solberg *et al.* were treating patients with their arms at their sides, with a full-length vacuum bag, to provide a better reproducibility and to improve patient comfort.²⁹ Shultz *et al.* studied in fourteen patients the dosimetric evaluation between two different plans. All of his fourteen patients were treated with arms down, and to be able to make a comparison between both positions, they remove the arms digitally. In their conclusions they found statistically significant differences between PTVmax and conformity index defined as the ratio of the 50% isodose volume to PTV volume, however, the absolute differences were both less than 5%. They also showed differences in the percent of total lung tissue receiving a minimum dose of 10, 20 or 30Gy: V_{10Gy} , V_{20Gy} and V_{30Gy} . They concluded that there is no evidence to support the hypothesis that with arms down lead to clinically loss of plan quality in thoracic SBRT when VMAT is used.¹⁹

Patients with thoracic and abdominal cancer are commonly positioned with arms up, despite the arm position not being specified by the Radiation Therapy Oncology Group (RTOG). Position with arms up is the first choice because of three concerns:¹⁹

- 1) Beam attenuation by ipsilateral arm which can be translated as an inferior dosimetry;
- 2) Arm location is difficult to replicate from the setup to treatment which can affect the dosimetry accuracy;
- 3) The treatment with arms down imposes unnecessary radiation exposure to the arm which can be translated, later in secondary malignancies.

In SBRT one of the major concerns is secondary effects of a high dose in lung tissue. Another concern of toxicity were the effects on the central bronchus, pulmonary artery,

esophagus, heart and spinal cord, for which a hypofractionated dose had not been followed up for a sufficiently long time.³⁰ The biggest advantage in SBRT is the higher BED. The various doses and dose fractionation combination used in lung cancer are easily compared by the use of BED. Several articles concluded that higher BED ($\geq 100\text{Gy}$) achieves high rates of local control.³¹⁻³³ But to do this technique a good technology in the treatment room is necessary.

In this study no statistically significant differences were found, so we can conclude that patient position should be chosen according to patients' co-morbidities and comfort in order to make a stable and reproducible position. In patients with a large respiratory motion amplitude, position with arms down can have advantages, decreasing respiratory motion and margins for ITV and with that the PTV. Despite of not finding statistically significant differences between the monitor units, we believe that the position with the arms up had larger values because, in all patients, it was the first plan that was made, and only after finding the ideal plan, we were able to plan the patients with the arms down. In comparison between the volume that received 6, 18 and 20.4 Gy, it is understandable that, with the arms up the values were lower. For that, we can conclude that arms position need to be balanced between patients' amplitude respiratory motion, co-morbidities and the fact that with arms down it will irradiate more volume of healthy tissue despite of lung volume can be smaller.

This study had limitations: the biggest limitation was sample size with only four patients we cannot generalize the results for all the population. Another limitation was the fact that arm reproducibility was not taken into account in positioning with arms down. We know in fact that arms' position and their rotation can affect treatment accuracy. Despite of this, planning with VMAT, is clinically possible to do an avoidance sector from one rotation angle to another one which included the arms.

5. Conclusion

We find no evidence to support the hypothesis that arms down position leads to a clinically significant loss of plan quality, when SBRT-VMAT is used for a single fraction of 24 Gy in lung cancer patients. For that, and for more conclusions we suggest more studies to be able to have a generalized conclusion.

6. References

1. Bouilhol G, Ayadi M, Rit S, Thengumpallil S, Schaerer J, Vandemeulebroucke J, *et al.* Is abdominal compression useful in lung stereotactic body radiation therapy? A 4DCT and dosimetric lobe-dependent study. *Physica Medica*. 2013; 29(4): 333–340.

2. Waldeland E, Ramberg C, Arnesen M, Helland A, Brustugun O, Malinen E. Dosimetric impact of a frame-based strategy in stereotactic radiotherapy of lung tumors. *Acta Oncologica*. 2012; 51: 603-609.
3. Gutiérrez A, Stathakis S, Crownover R, Esquivel C, Shi C, Papanikolaou N. Clinical evaluation of an immobilization system for stereotactic body radiotherapy using helical tomotherapy. *Medical Dosimetry*. 2011; 36(2): 126-129.
4. Heinzerling J, Anderson J, Papiez L, Boike T, Chien S, Zhang G, *et al*. Four-dimensional computed tomography scan analysis of tumor and organ motion at varying levels of abdominal compression during stereotactic treatment of lung and liver. *Int. J. Radiation Oncology Biol, Phys*. 2008; 70: 1571-1578.
5. Lohr F, Debus J, Frank C, Herfarth K, Pastyr O, Rhein B, *et al*. Noninvasive patients fixation for extracranial stereotactic radiotherapy. *Int. J. Radiation Oncology Biol. Phys*. 1999, 45(2): 521-527.
6. Navarro-Martin A, Cacicedo J, Leaman O, Sancho I, Garcia E, Navarro V, *et al*. Comparative analysis of thermoplastic mask versus vacuum cushions in stereotactic body radiotherapy. *Radiation Oncology*. 2015; 10: 176-182.
7. Sonke J, Rossi M, Wolthaus J, van Herk M, Damen E, Belderbos J. Frameless stereotactic body radiotherapy for lung cancer using four-dimensional cone beam CT guidance. *Int. J. Radiation Oncology Biol. Phys*. 2009; 74: 567–574.
8. Li W, Purdie TG, Taremi M, Fung S, Brade A, Cho BCJ, *et al*. Effect of Immobilization and performance status on intrafraction motion for stereotactic lung radiotherapy: analysis of 133 Patients. *Int. J. Radiation Oncology Biol. Phys*. 2011; 81(5): 1568–1575.
9. Masi L, Casamassima F, Menichelli C, Pasciuti K, Doro R, Polli C, *et al*. On-line image guidance for frameless stereotactic radiotherapy of lung malignances by cone beam CT: comparison between target localization and alignment on bony anatomy. *Acta Oncologica*. 2008; 47: 1422-1431.
10. Lim D, Yi B, Mirmiran A, Dhople A, Sunthalingam M, D'Souza W. Optimal beam arrangement for stereotactic body radiation therapy delivery in lung tumors. *Acta Oncologica*. 2010; 49: 219-224.
11. Hansen A., Petersen J., Hoyer M.; Internal movement, set-up accuracy and margins for stereotactic body radiotherapy using a stereotactic body frame. *Acta Oncologica*. 2006; 45: 948-952.
12. Underberg R, Lagerwaard F, Cuijpers J, Slotman B, Koste J, Senan S. Four-dimensional ct scans for treatment planning in stereotactic radiotherapy for stage I lung cancer. *Int. J. Radiation Oncology Biol. Phys*. 2004; 60 (4): 1283-1290.
13. Guckenberger M, Krieger T, Richter A, Baier K, Wilbert J, Sweeney R, *et al*. Potential of image-guidance, gating and real-time tracking to improve accuracy in pulmonary

- stereotactic body radiotherapy. *Radiotherapy and Oncology*, vol. 91, no. 3, pp. 288–295, 2009.
14. Zhou J, Uhl B, Dewitt K, Young M, Taylor B, Fei D, *et al.* Image-guided stereotactic body radiotherapy for lung tumors using bodyloc with omotherapy: clinical implementation and set-up accuracy. *Medical Dosimetry*. 2010; 35(1): 12–18.
 15. Luo G, Gopalakrishnan M, Zhang Y, Bautista J, Mallett H, Metha M, *et al.* Patient Setup Accuracy and Immobilization Errors during Lung, Spine, and Liver Stereotactic Body Radiation Therapy Delivery: Preliminary Experience using a Body Fix with Dual Vacuum Immobilization and a Robotic Couch. *Proceeding of the 53rd Annual ASTRO Meeting*.
 16. Alderliesten T, Sonke J, Betgen A, Vliet-Vroegindeweij C, Remeijer P. 3D surface imaging for monitoring intrafraction motion in frameless stereotactic body radiotherapy of lung cancer. *Radiotherapy and Oncology*. 2012; 105: 155-160.
 17. Han K, Cheung P, Basran P, Poon I, Yeung L, Lochray F. A comparison of two immobilization systems for stereotactic body radiation therapy of lung tumors. *Radiotherapy and Oncology*. 2012; 95: 103-108.
 18. Liu H, Khan R, Nugent Z, Krobutschek K, Dunscombe P, Lau H. Factors influencing intrafractional target shifts in lung stereotactic body radiation therapy. *Practical Radiation Oncology*. 2014; 4: 45-51
 19. Shultz D, Jang S, Hanlon A, Diehn M, Loo Jr. B, Maxim P. The effect of arm position on the dosimetry of thoracic stereotactic ablative radiation therapy using volumetric modulated arc therapy. *Practical Radiation Oncology*. 2014; 4: 192-197.
 20. Murray B, Forster K, Timmerman R. Frame-based immobilization and targeting for stereotactic body radiation therapy. *Medical Dosimetry*. 2007; 32(2): 86-91.
 21. Shirato H, Seppenwoolde Y, Kitamura K, Onimura R, Shimizu S. Intrafractional tumor motion: lung and liver. *Seminars in Radiation Oncology*. 2004; 14 (1) 10–18, 2004.
 22. Jochem W.H. Wolthaus, Christoph Schneider, Jan-Jakob Sonke, *et al.* Mid-ventilation CT scan construction from four-dimensional respiration-correlated CT scans for radiotherapy planning of lung cancer patients. *Int. J. Radiation Oncology Biol. Phys.* 2006; 65: 1560-1571.
 23. Wolthaus J, Sonke J, vanHerk M, Damen E. Image quality optimization: reconstruction of a time-averaged mid-position CT scan for radiotherapy planning of lung cancer patients using deformable registration. *Medical Physics*. 2008; 35.
 24. Liu H, Balter P, Tutt T, Choi B, Zhang J, Wang C, *et al.* Assessing respiration-induced tumor motion and internal target volume using four-dimensional computed tomography for radiotherapy of lung cancer. *Int. J. Radiation Oncology Biol. Phys* 2007; 68: 531–540.

25. McGrath S, Matuszak M, Yan D, Kestin L, Martinez A, Grills I. Volumetric modulated arc therapy for delivery of hypofractionated stereotactic lung radiotherapy: A dosimetric and treatment efficiency analysis. *Radiotherapy and Oncology*. 2010; 95: 153-157.
26. Ong C, Verbakel W, Dahele M, Cuijpers J, Slotman B, Senan S. Fast Arc Delivery for Stereotactic Body Radiotherapy of Vertebral and Lung Tumors. *Int. J. Radiation Oncology Biol. Phys.* 2011; 83 (1): 137-143.
27. Grimm J, LaCouture T, Croce R, Yeo I, Zhu Y, Xue J. Dose tolerance limits and dose volume histogram evaluation for stereotactic body radiotherapy. *Journal of Applied Clinical Medical Physics*. 2011; 12 (2).
28. Park J, Ye S, Kim H, Park J. Dosimetric effects of immobilization devices on SABR for lung cancer using VMAT technique. *Journal of Applied Clinical Medical Physics*. 2014; 16(1): 273-282.
29. Solberg T, Medin P, Mullins J, Li S. Quality assurance of immobilization and target localization systems for frameless stereotactic cranial and extracranial hypofractionated radiotherapy. *Int. J. Radiation Oncology Biol. Phys.* 2008; 71(1): 131-135.
30. Nagata Y, Wulf J, Lax I, Timmerman R, Zimmermann F, Stojkovski I, *et al.* Stereotactic Radiotherapy of Primary Lung Cancer and Other Targets: Results of Consultant Meeting of the International Atomic Energy Agency. *Int. J. Radiation Oncology Biol. Phys.* 2011; 79 (3): 660-669.
31. McGarry R, Papiez L, Williams M, Whitford T, Timmerman R. Stereotactic body radiation therapy of early-stage non-small-cell lung carcinoma: Phase I study. *Int. J. Radiation Oncology Biol. Phys.* 2005; 63 (4): 1010-1015.
32. Trakul N, Chang C, Harris J, Phil M, Chapman C, Rao A, *et al.* Tumor volume-adapted dosing in stereotactic ablative radiotherapy of lung tumors. *Int. J. Radiation Oncology Biol. Phys.* 2012; 84 (1):231-237.
33. Onishi H, Araki T, Shirato H, Nagata Y, Hiraoka M, Gomi K, *et al.* Stereotactic hypofractionated high-dose irradiation for stage I nonsmall cell lung carcinoma. *American cancer society*. 2004; 101 (7): 1623-1631.
34. Wolthaus J, Schneider, Sonke J, Herk M, Belderbos J, Rossi M, *et al.* A simple method to reconstruct a representative mid-ventilation CT scan from 4D respiration correlated CT scans for radiotherapy treatment planning of lung cancer patients. *The international Journal of Medical Physics Research and practice*. 2006; 33.

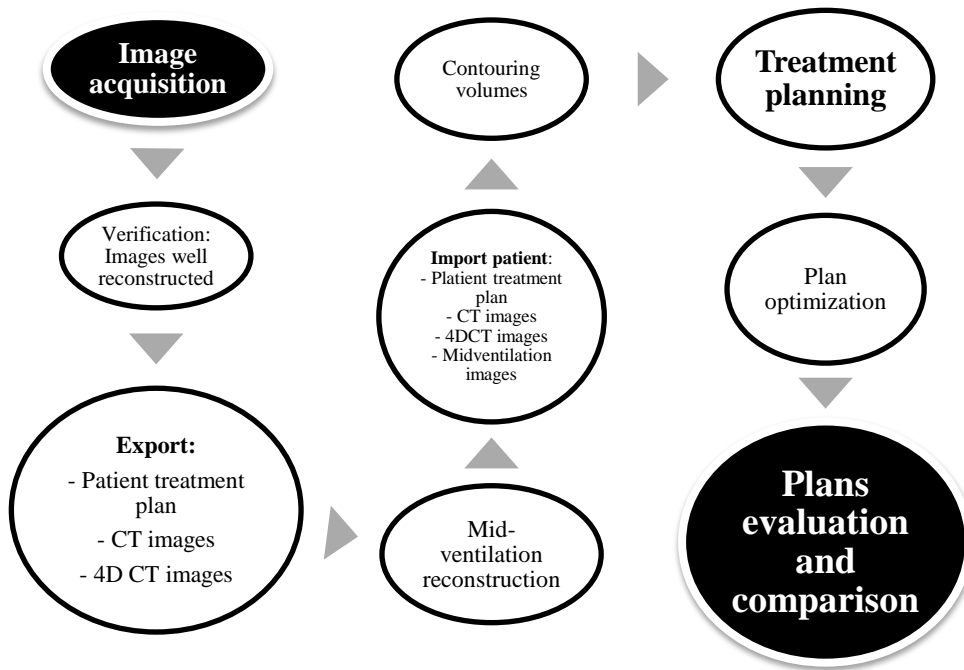


Fig. 1 - Research process: steps for all patients

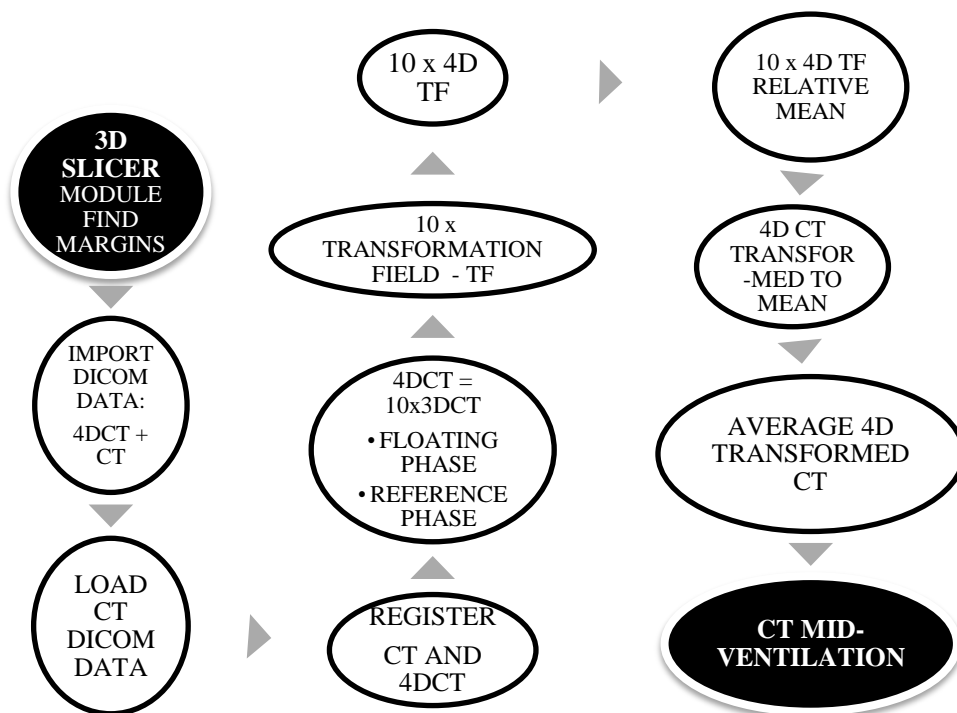


Fig. 2 - Mid-ventilation reconstruction process

Table 1 - Organs at risk contoured for each patient

Patient	Location	OAR	
1	Metastasis in RSL – 3 lesions	- Right Lung - Left Lung - Total Lung volume (R+L) - Spinal cord - Large Airways (R+L) - Small airways (R) - Trachea	- Heart - Aorta - Esophagus - Great vessels - Thoracic wall - Brachial plexus - Humerus (only for patient2)
2	Metastasis in RSL		
3	RSL with local invasion		
4	RML		

*RSL = right superior lobe; RML= right middle lobe.




Fig. 3 - Contouring - a) Ring b) PTVcal: the sum of PTV1, PTV2 and PTV3

Table 2 - SBRT dose tolerance limits (Timmerman, 2011)²⁷

Organ	Vol. (cc)	Vol. Limit (Gy)	Max Limit (Gy)
Aorta and major vessels	10 cc	31 Gy	37 Gy
Brachial Plexus	3 cc	14 Gy	17.5 Gy
Esophagus	5 cc	11.9 Gy	15.4 Gy
Heart	15 cc	16 Gy	22 Gy
Lung (Right+Left)	1500 cc	7 Gy	
	1000 cc	7.4 Gy	
Ribs (Thoracic wall)	1 cc	22 Gy	30 Gy
Small airways	0.5 cc	12.4 Gy	13.3 Gy
Spinal Cord	0.35 cc	10 Gy	14 Gy
	1.2 cc	7 Gy	
Trachea	4 cc	10.5 Gy	20.2 Gy




Fig. 4 - Target position in each respiratory phase in L-R (left-right), I-S (inferior-superior) and A-P (anterior-posterior) directions **a**) arms up **b**) arms down




Fig. 5- Dmax, Dmean and Dmin for each patient and all patient mean doses

Table 3 – Mean and standard deviation (sd) values for the percentage of lung volume receiving x Gy.

Lung	Mean (sd)		p-value
	Arms up	Arms down	
V _{10Gy}	13.3 (9.1)	14.35 (9.48)	0.593
V _{15Gy}	7.98 (6.47)	8.83 (6.16)	1
V _{20Gy}	4.48 (3.33)	5.1 (3.5)	0.285

Table 4 – Total of monitor units

UM	Arms up	Arms down	p-value
Patient 1	13701	8118	n.a
Patient 2	10228	8522	
Patient 3	8000	8784	
Patient 4	12774	6334	
Mean (sd)	11 175.75 (2 576.49)	7 939.5 (1 104.84)	0.144




Fig. 6 - Total of monitor units: the variability of data

Conclusão geral

O posicionamento do doente deve ser um compromisso entre o conforto do doente e um posicionamento reprodutível para o tratamento, se este compromisso não for exequível a precisão do tratamento pode ser posta em causa devido ao aumento de erros de *set up*. O posicionamento pode ser feito com ou sem dispositivos de imobilização rígidos. A sua escolha deve ser feita tendo em conta o tipo de imagem/tecnologia disponível na sala de tratamento. A SBRT impõe um posicionamento com elevada precisão, respeitando sempre as co-morbilidades e o conforto do doente de forma a ser um posicionamento estável e reprodutível. Em alguns doentes o posicionamento com os braços para baixo pode ser vantajoso por diminuir a amplitude do movimento respiratório e consequentemente o volume a irradiar - PTV. Não foram encontradas diferenças estatisticamente significativas entre as variáveis em estudo, apesar disso, são notórias as diferenças nos valores das unidades monitor que se podem justificar com o facto do planeamento com os braços para cima ser feito sempre em primeiro lugar. Existe também uma diferença perceptível na variável do volume que recebe x Gy que tem valores inferiores no posicionamento com os braços para cima. Existe também uma ligeira diferença no volume do pulmão, sendo os valores inferiores com os braços ao longo do corpo. Assim, pode concluir-se que a posição dos braços deve ser um compromisso entre a amplitude respiratória que o posicionamento provoca, as co-morbilidades do doente e entre o facto de irradiar mais tecido são com os braços para baixo.

Para futuros projetos e na mesma linha de investigação poderia estudar-se o impacto da variação da amplitude do movimento tumoral com os diferentes posicionamentos. Esta pragmática pode ser aplicada a patologias que variem com o movimento respiratório, como por exemplo, tumores de fígado.