



# LUND UNIVERSITY

## A prolonged postinspiratory pause enhances CO<sub>2</sub> elimination by reducing airway dead space.

Uttman, Leif; Jonson, Björn

*Published in:*  
Clinical Physiology and Functional Imaging

*DOI:*  
[10.1046/j.1475-097X.2003.00498.x](https://doi.org/10.1046/j.1475-097X.2003.00498.x)

2003

[Link to publication](#)

*Citation for published version (APA):*  
Uttman, L., & Jonson, B. (2003). A prolonged postinspiratory pause enhances CO<sub>2</sub> elimination by reducing airway dead space. *Clinical Physiology and Functional Imaging*, 23(5), 252-256. <https://doi.org/10.1046/j.1475-097X.2003.00498.x>

*Total number of authors:*  
2

### General rights

Unless other specific re-use rights are stated the following general rights apply:  
Copyright and moral rights for the publications made accessible in the public portal are retained by the authors and/or other copyright owners and it is a condition of accessing publications that users recognise and abide by the legal requirements associated with these rights.

- Users may download and print one copy of any publication from the public portal for the purpose of private study or research.
- You may not further distribute the material or use it for any profit-making activity or commercial gain
- You may freely distribute the URL identifying the publication in the public portal

Read more about Creative commons licenses: <https://creativecommons.org/licenses/>

### Take down policy

If you believe that this document breaches copyright please contact us providing details, and we will remove access to the work immediately and investigate your claim.

LUND UNIVERSITY

PO Box 117  
221 00 Lund  
+46 46-222 00 00

# A prolonged postinspiratory pause enhances CO<sub>2</sub> elimination by reducing airway dead space

Leif Uttman and Björn Jonson

Department of Clinical Physiology, University Hospital, Lund, Sweden

## Summary

### Correspondence

Leif Uttman, Department of Clinical Physiology, University Hospital, SE-221 85 Lund, Sweden  
E-mail: leif.uttman@klinfys.lu.se

### Accepted for publication

Received 22 November 2002;  
accepted 18 February 2003

### Key words

artificial respiration; breath tests; capnography; pulmonary gas exchange; swine

**Background:** CO<sub>2</sub> elimination per breath ( $V_{\text{CO}_2, \text{T}}$ ) depends primarily on tidal volume ( $V_{\text{T}}$ ). The time course of flow during inspiration influences distribution and diffusive mixing of  $V_{\text{T}}$  and is therefore a secondary factor determining gas exchange. To study the effect of a postinspiratory pause we defined 'mean distribution time' (MDT) as the mean time given to inspired gas for distribution and diffusive mixing within the lungs. The objective was to quantify changes in airway dead space ( $V_{\text{Daw}}$ ), slope of the alveolar plateau (SLOPE) and  $V_{\text{CO}_2, \text{T}}$  as a function of MDT in healthy pigs.

**Methods:** Ten healthy pigs were mechanically ventilated. Airway pressure, flow and partial pressure of CO<sub>2</sub> were recorded during resetting of the postinspiratory pause from 10% (baseline) to, in random order, 0, 5, 20 and 30% of the respiratory cycle. The immediate changes in  $V_{\text{Daw}}$ , SLOPE,  $V_{\text{CO}_2, \text{T}}$ , and MDT after resetting were analyzed.

**Results:**  $V_{\text{Daw}}$  in percent of  $V_{\text{T}}$  decreased from 29 to 22%, SLOPE from 0.35 to 0.16 kPa per 100 ml as MDT increased from 0.51 to 1.39 s. Over the same MDT range,  $V_{\text{CO}_2, \text{T}}$  increased by 10%. All these changes were statistically significant.

**Conclusion:** MDT allows comparison of different patterns of inspiration on  $V_{\text{Daw}}$  and gas exchange. Estimation of the effects of an altered ventilator setting on exchange of CO<sub>2</sub> can be done only after about 30 minutes, while the transient changes in  $V_{\text{CO}_2, \text{T}}$  may give immediate information. MDT affects gas exchange to an important extent. Further studies in human subjects in health and in disease are needed.

## Introduction

A low tidal volume ( $V_{\text{T}}$ ) appears to be a crucial factor for lung protective ventilation in the acute respiratory distress syndrome. When low  $V_{\text{T}}$  is used to provide lung protective ventilation, respiratory acidosis may be partly balanced by an increased respiratory rate (RR) (ARDS Network, 2000). In itself, a low  $V_{\text{T}}$  leads to increased dead space fraction. A short duration of inspiration that follows from an increased RR may then further compromise gas exchange by uneven distribution and inadequate mixing of  $V_{\text{T}}$  in the alveolar space. Different means to reduce dead space have been suggested. For instance, replacement of passive humidifiers with active ones, tracheal gas insufflation and aspiration of dead space implies that the interface between 'fresh and old' gas is moved distally already at the beginning of inspiration (Jonson *et al.*, 1990; De Robertis *et al.*, 1999; Richecoeur *et al.*, 1999). Furthermore, a ventilator setting that facilitates diffusion may reduce dead space by allowing this interface to move proximally before the end of

inspiration. Accordingly, the dead space related to the airways represents function as well as anatomy. Rather than the term 'anatomical dead space' we prefer the term airway dead space that should be read as 'functional airway dead space'. Several studies in health or in disease show a decrease in dead space or PaCO<sub>2</sub> when using a postinspiratory pause (Fuleihan *et al.*, 1976; Dammann *et al.*, 1978; Lachmann *et al.*, 1982; Wolff *et al.*, 1989a; Mercat *et al.*, 2001). However, positive effects of inspiratory patterns intended to improve gas exchange have not always been observed (Johansson, 1975; Johansson & Löfström, 1975; Dammann *et al.*, 1978; Al-Saady & Bennett, 1985; Markström *et al.*, 2000). Partly diverging results may reflect methodological limitations. Recently, a known method allowing high accuracy of dead space determination in intensive care was further refined (Beydon *et al.*, 2002). A method to compensate for inevitable changes in  $V_{\text{T}}$  can be based on mathematical modelling of the alveolar plateau in the single breath test for CO<sub>2</sub> (SBT-CO<sub>2</sub>) (Uttman & Jonson, 2002). In the present study, we introduce the term 'mean distribution time'

(MDT), which is the mean time given to inspired gas for distribution and diffusive mixing within the lungs. MDT was varied by changing the duration of the postinspiratory pause at volume controlled ventilation with constant flow. The objective was to quantify changes in airway dead space ( $V_{Daw}$ ), slope of the alveolar plateau (SLOPE) and CO<sub>2</sub> elimination per breath ( $V_{CO_2,T}$ ) as a function of MDT in healthy pigs.

## Methods

### Materials

The local Ethics Board of Animal Research approved the experimental protocol. Ten pigs of the Swedish native breed, mean weight 29.5 kg (23.0–33.5), were fasted overnight with free access to water. Seven of these animals were the same as in (Uttman & Jonson, 2002). The animals were premedicated with azaperon (7 mg kg<sup>-1</sup>), anaesthetized with ketamin (5 mg kg<sup>-1</sup>), intubated with a 7.0 mm ID tracheal tube and connected to a ventilator (ServoVentilator 900C, Siemens-Elma, Solna, Sweden). Ventilation was volume controlled with a square inspiratory flow pattern. At baseline setting RR was 20 min<sup>-1</sup>, inspiratory time 33%, postinspiratory pause time ( $T_p$ ) 10% and positive end-expiratory pressure 6 cm H<sub>2</sub>O. The baseline minute ventilation was adjusted to achieve PaCO<sub>2</sub> 4.5–5 kPa. A mainstream analyzer (CO<sub>2</sub> Analyzer 930, Siemens-Elma, Solna, Sweden) measured partial pressure of CO<sub>2</sub> in expired and inspired gas ( $P_{CO_2}$ ). Anaesthesia was maintained by continuous infusion of ketamin (17 mg kg<sup>-1</sup> h<sup>-1</sup>), midazolam (1.7 mg kg<sup>-1</sup> h<sup>-1</sup>) and pancuronium bromide (0.5 mg kg<sup>-1</sup> h<sup>-1</sup>). The ventilator/computer system used for data recording has previously been described (Svantesson et al., 1997). Signals from the ventilator and CO<sub>2</sub> analyzer representing flow rate, airway pressure and  $P_{CO_2}$  were sampled by a personal computer at the frequency of 50 Hz. Compliance of the tracheal tube and ventilator tubing was measured *in vitro*. There were no dropouts among the animals.

### Protocol

After preparation of the animals a stabilization period of 30 min was allowed. A recruitment manoeuvre was performed by inflating the lungs with a pressure of 35 cm H<sub>2</sub>O for 10 s to eliminate atelectasis and standardize lung volume history and conditions among the animals. The system was tested for leakage. A continuous record of a study sequence comprised the following elements: 10 normal breaths, 20 breaths of a different  $T_p$ , 10 normal breaths.  $T_p$  was changed by manual switch of the  $T_p$  control of the ventilator from 10 to 0, 5, 20 and 30% of the respiratory cycle, in randomized order.

### Data analysis

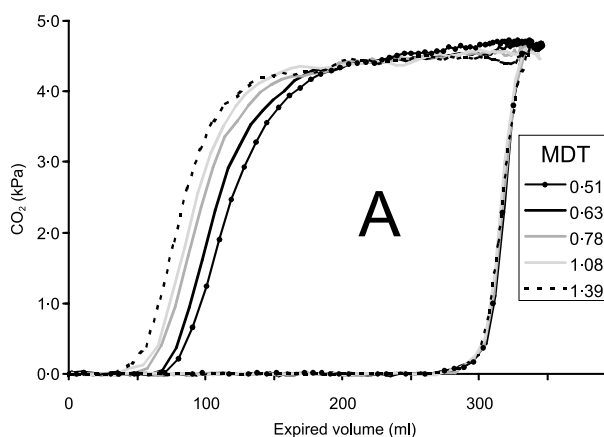
Data sampled during a study sequence were transferred to a spreadsheet for analysis (Excel 97, Microsoft Corp., WA, USA).

Measured flow rate was corrected for the compliance in the tubing in order to obtain airway flow rate ( $\dot{V}_{aw}$ ). The expiratory flow signal was normalized by a correction factor so that expired volume equalled inspired volume. The correction factor obtained at  $T_p$  10% was applied to all recordings.  $V_T$  was calculated by integration of expired  $\dot{V}_{aw}$ . Airway dead space distal to the CO<sub>2</sub> sensor was determined according to an algorithm of (Wolff & Brunner, 1984) that was modified to correct for a sloping alveolar plateau (Åström et al., 2000) in accordance with principles previously described (Wolff et al., 1989b). Airway dead space distal to the tip of the tracheal tube ( $V_{Daw}$ ) was calculated by subtracting the dead space volume of the tracheal tube and CO<sub>2</sub> analyzer (16 ml).  $V_{CO_2,T}$  was calculated as the difference between expired volume of CO<sub>2</sub> and that re-inspired from the Y-piece and adjacent tubing, which corresponds to the area within the SBT-CO<sub>2</sub> loop (Fig. 1) (Uttman & Jonson, 2002). From an equation describing the alveolar plateau its SLOPE was calculated at the volume halfway between  $V_{Daw}$  and  $V_T$  (Beydon et al., 2002). Technical limitations and flux of gas from tubing to the subject in the first phase of a postinspiratory pause caused small variations in  $V_T$  and thereby in  $V_{CO_2,T}$ . The effect on  $V_{CO_2,T}$  caused by  $V_T$  variation was not an issue of this study and was accordingly corrected for. How  $V_{CO_2,T}$  varies with  $V_T$  can be determined from the end-tidal alveolar slope and end-tidal  $P_{CO_2}$  in the SBT-CO<sub>2</sub> (Uttman & Jonson, 2002).  $V_{CO_2,T}$  was normalized to the lowest  $V_T$  observed as was end-tidal  $P_{CO_2}$ .

For a certain pattern of inspiration including the postinspiratory pause, MDT was calculated from all samples during a recorded inspiration as:

$$MDT = \frac{\sum (\dot{V}_{aw} \cdot \Delta t \cdot t_{dist})}{\sum (\dot{V}_{aw} \cdot \Delta t)} = \frac{\sum (\dot{V}_{aw} \cdot t_{dist})}{\sum (\dot{V}_{aw})} \quad (1)$$

where  $\Delta t$  is the sampling interval (0.02 s) and  $t_{dist}$  is the time left for distribution of the particular gas sample until start of expiration.

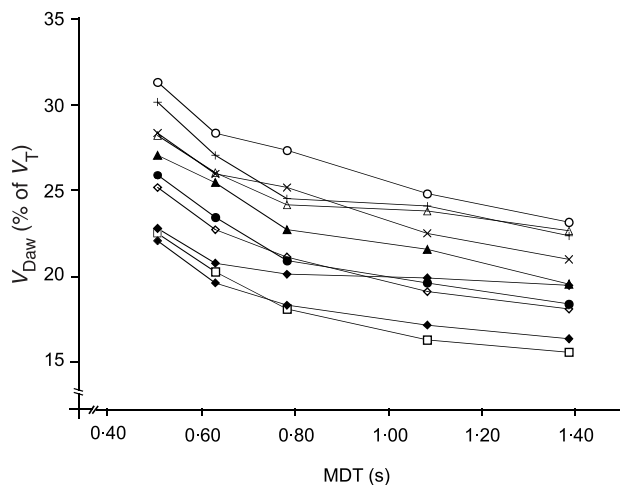
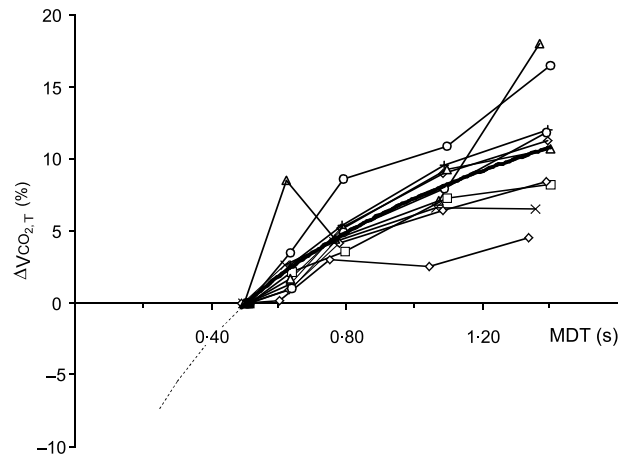


**Figure 1** The single breath test for CO<sub>2</sub> in a representative animal at different mean distribution time (MDT). Longer MDT resulted in a left-hand shift of the sharp ascending expiratory limb of the loop. This corresponds to a decrease in airway dead space and an increase in tidal CO<sub>2</sub> elimination (area A). The slope of the alveolar plateau decreased with MDT.

**Table 1** Consequences of postinspiratory pause.

$T_p$ (%)	MDT (s) mean $\pm$ SD	$V_{Daw}$ (% of $V_T$ ) mean $\pm$ SEM	$V_{CO_2,T}$ (ml) mean $\pm$ SEM	SLOPE (kPa per 100 ml) mean $\pm$ SEM	$P_{CO_2,ET}$ (kPa) mean $\pm$ SEM	$P_{plateau}$ (cm H <sub>2</sub> O) mean $\pm$ SEM
0	0.51 $\pm$ 0.01	29 $\pm$ 1.0	8.0 $\pm$ 0.57	0.35 $\pm$ 0.04	4.8 $\pm$ 0.12	—
5	0.63 $\pm$ 0.01	27 $\pm$ 0.9	8.1 $\pm$ 0.56	0.26 $\pm$ 0.02	4.7 $\pm$ 0.13	15.1 $\pm$ 0.5
10	0.78 $\pm$ 0.01	25 $\pm$ 0.9	8.3 $\pm$ 0.59	0.24 $\pm$ 0.03	4.7 $\pm$ 0.12	14.8 $\pm$ 0.5
20	1.08 $\pm$ 0.02	24 $\pm$ 0.9	8.6 $\pm$ 0.60	0.14 $\pm$ 0.01	4.7 $\pm$ 0.12	14.7 $\pm$ 0.5
30	1.39 $\pm$ 0.02	22 $\pm$ 0.8	8.8 $\pm$ 0.60	0.16 $\pm$ 0.02	4.7 $\pm$ 0.14	15.0 $\pm$ 0.5

MDT, mean distribution time;  $V_{Daw}$ , airway dead space;  $V_{CO_2,T}$ , tidal CO<sub>2</sub> elimination;  $P_{CO_2,ET}$ , end-tidal  $P_{CO_2}$ ;  $P_{plateau}$ , postinspiratory plateau pressure.

**Figure 2** Airway dead space ( $V_{Daw}$ ) as a function of mean distribution time (MDT) in each subject.**Figure 3** Tidal CO<sub>2</sub> elimination change ( $\Delta V_{CO_2,T}$ ) as a function of mean distribution time (MDT). Individual curves (thin lines) and regression line (heavy line), with extrapolation (broken line).

### Statistical methods

Data are presented as mean  $\pm$  SD. Two-way ANOVA was used to study variations of different parameters with MDT. Student's paired two-tailed *t*-test was used to analyze differences among parameters observed at MDT 0.51 s ( $T_p$  0%) and other values of MDT. Non-linear regression was used to establish the relationship between  $V_{CO_2,T}$  and MDT.

### Results

$V_T$  was  $286 \pm 42$  ml, corresponding to  $9.7 \pm 1.0$  ml kg<sup>-1</sup>.  $V_T$  increased with on average 4 ml when  $T_p$  increased from 0 to 5% and remained at that level at longer  $T_p$ . The end-expiratory flow was 0 at  $T_p$  0% to  $T_p$  20% and increased to  $0.05 \pm 0.04$  l s<sup>-1</sup> at  $T_p$  30%. Plateau pressure measured at the end of the postinspiratory pause showed only minor variations with  $T_p$  (Table 1). For the different  $T_p$  MDT varied from 0.51 to 1.39 s with a coefficient of variation between animals of less than 2% (Table 1). Figure 1 shows the SBT-CO<sub>2</sub> for the different MDT in a representative animal. As appears from Fig. 2,  $V_{Daw}$  decreases non-linearly with MDT in

each animal. The decrease in  $V_{Daw}$  resulted in an increase in  $V_{CO_2,T}$  as illustrated in Fig. 1.

Longer MDT led to lower SLOPE and lower end-tidal  $P_{CO_2}$  (ANOVA,  $P < 0.001$  for both) (Table 1). Effects on  $V_{CO_2,T}$ , related to changes of the alveolar plateau, were calculated from changes in the area below the alveolar plateau. When  $T_p$  increased from 0 to 30%, the observed changes of the alveolar plateau did not influence  $V_{CO_2,T}$  ( $P > 0.05$ ).

When  $T_p$  increased from 0 to 30%, implying that MDT changed from 0.51 to 1.39 s,  $V_{CO_2,T}$  in percent of the value at  $T_p$  0% increased as shown in Fig. 3. The change in  $V_{CO_2,T}$  ( $\Delta V_{CO_2,T}$ ) was expressed according as follows:

$$\Delta V_{CO_2,T} = 7.24 + 10.6 \ln(\text{MDT}) \quad (r = 0.86, P < 0.001) \quad (2)$$

### Discussion

At volume controlled ventilation with constant inspiratory flow, this study shows that a postinspiratory pause enhances CO<sub>2</sub> elimination by reducing  $V_{Daw}$ . The uniform results indicate that it is possible to detect even modest changes in  $V_{Daw}$  and CO<sub>2</sub> elimination. These changes follow immediately after resetting. In contrast, stabilization of  $P_{aCO_2}$  following a change in CO<sub>2</sub>

elimination takes several minutes (Farhi & Rahn 1955; Taskar et al., 1995) and may be obscured by physiological instability. The determination of MDT according to Eq. (1) was robust as indicated by low scatter (Table 1).

As this study has its focus on methodological and conceptual development it has several limitations. Healthy pigs do not have collateral ventilation (Woolcock & Macklem, 1971). Furthermore, as airway resistance is low, different lung units probably fill and empty nearly synchronously. Obviously, the results cannot be applied on humans in whom collateral ventilation may equilibrate ventilation non-homogeneity. This may be particularly important in obstructive lung disease.

The end-expiratory flow indicated the presence of auto-PEEP at  $T_P$  30%. An estimate based on previous observations of expiratory resistance in healthy pigs (Uttman & Jonson, 2002) suggests that auto-PEEP was less than 0.5 cm H<sub>2</sub>O. That auto-PEEP was unimportant was further supported by the nearly constant postinspiratory plateau pressure (Table 1). If benefits of a prolonged MDT are obtained by prolongation of inspiration at the expense of expiratory time, a deleterious degree of auto-PEEP may result, particularly in the presence of airway obstruction. A more favourable approach may then be to prolong MDT by changing the flow wave pattern of inspiration. However, we only studied constant inspiratory flow. Pressure controlled ventilation, which particularly in Scandinavia is frequently used, results in a decelerating inspiratory flow. When airway resistance varies within the lung such a flow rate leads to a more even ventilation (Jansson & Jonson, 1972). One rational of decelerating flow is, indeed, to prolong MDT and to promote even gas distribution and diffusion. Obviously, the limitations of this study merit further studies with different flow patterns in humans with different nature of lung pathology.

MDT was conceived with the prospect that it is applicable to all patterns of inspiration. The algorithm of MDT (Eq. 1) dictates that any symmetrical inspiratory waveform will have the same MDT, provided that inspiratory time is constant. The validity of this assumption is supported by that ventilation with square and sine inspiratory waveforms give rise to the same CO<sub>2</sub> elimination reflected by equal PaCO<sub>2</sub> (Dammann et al., 1978). Notably, a decelerating or accelerating inspiratory flow pattern will have longer and shorter MDT, respectively, compared to symmetrical flow waveforms. Different waveforms have been studied in humans with indistinct results (Johansson, 1975; Johansson & Löfström, 1975; Dammann et al., 1978; Al-Saady & Bennett, 1985; Markström et al., 2000). Such studies merit to be repeated with modern technique.

The effect of a longer  $T_P$  on  $V_{Daw}$  indicates a movement in the proximal direction of the 'distal boundary of dead space' (Bowes et al., 1985). As the total airway cross-section area decreases rapidly with each bronchial generation in the cranial direction (Weibel, 1963), the rate of this movement must be expected to decline in a non-linear fashion, as was found (Fig. 2). The rationale of using a logarithmic equation is based on this concept. When MDT is falling towards zero no time is available for diffusion, which is a prerequisite for exchange of gas within the

respiratory zone. On the other hand, after a long time for gas distribution the interface between alveolar gas and fresh gas would by diffusion have reached a level in the airways at which the fast drop in total cross-section area would render diffusion more and more inefficient.

The variation in  $V_{Daw}$  we observed corresponds to about 0.7 ml kg<sup>-1</sup> body weight, which is not trivial with respect to lung protective strategies. In the clinic, it might be desirable to use high RR. If we allow ourselves to extrapolate MDT to 0.25 s (RR 40,  $T_P$  0%), as shown in Fig. 3,  $V_{CO_2,T}$  would in comparison to MDT 0.51 drop by about 7% and further increase dead space. This would enhance problems related to hypercapnia when  $V_T$  is restricted to 6 ml kg<sup>-1</sup> (ARDS Network, 2000).

The effect of a longer  $T_P$  on SLOPE implies a more even  $P_{CO_2}$  in lung units, which empty non-synchronously. This can either be due to equilibration between parallel units caused by pendelluft or by equilibration along longitudinally oriented units in terms of distal and more proximal alveoli (Fletcher, 1980). In principle, one cannot from external global observations differentiate between these models (West, 1971). One can only speculate that low peripheral resistance in healthy pigs might prevent significant uneven ventilation between parallel lung units. Time-dependent equilibration between proximal and more distal alveoli offers a more likely explanation. Anyway, the more even alveolar concentration reflected by a lower SLOPE after a long  $T_P$  was not so important so as to significantly reduce  $V_{CO_2,T}$ .

Our results agree with previous findings that a postinspiratory pause enhances CO<sub>2</sub> elimination (Fuleihan et al., 1976; Dammann et al., 1978; Lachmann et al., 1982; Wolff et al., 1989a; Mercat et al., 2001). In the present study, we used the shortest possible tubing (compliance 0.45 ml per cm H<sub>2</sub>O). In spite of that, about 4 ml was re-distributed from the tubing to the lungs when a postinspiratory pause was applied. If we had not corrected  $V_{CO_2,T}$  for the increase in  $V_T$ , effects of a postinspiratory pause in itself would have been overestimated. In the clinic, both longer tubing and a larger drop in airway pressure at transition to the pause may cause larger  $V_T$  variation. In comparison to previous studies, the methodological development is considered to increase the validity and accuracy of the results, which increased the ability to quantify changes in dead space related to modest changes in MDT.

In conclusion, the concept MDT was introduced to allow comparison of different patterns of inspiration with respect to  $V_{Daw}$  and gas exchange. Estimation of the effects of an altered ventilator setting on exchange of CO<sub>2</sub> can be done after about 30 min, while the transient changes in  $V_{CO_2,T}$  may give immediate information. MDT affects gas exchange to such an extent that it may be of importance for optimisation of ventilator setting. Further studies on human subjects in health and in disease are needed.

## Acknowledgments

This study was supported by the Swedish Research Council (02872) and the Swedish Heart-Lung Foundation. We

acknowledge the contribution of Dr Lars Nordström (†2001) for his inspiration and unpublished ideas behind the concept of MDT.

## References

- Al-Saady N, Bennett ED. Decelerating inspiratory flow waveform improves lung mechanics and gas exchange in patients on intermittent positive-pressure ventilation. *Intensive Care Med* (1985); **11**: 68–75.
- ARDS Network. Ventilation with lower tidal volumes as compared with traditional tidal volumes for acute lung injury and the acute respiratory distress syndrome. *N Engl J Med* (2000); **342**: 1301–1308.
- Åström E, Niklason L, Drefeldt B, Bajc M, Jonson B. Partitioning of dead space – a method and reference values in the awake human. *Eur Respir J* (2000); **16**: 659–664.
- Beydon L, Uttman L, Rawal R, Jonson B. Effects of positive end-expiratory pressure on dead space and its partitions in acute lung injury. *Intensive Care Med* (2002); **28**: 1239–1245.
- Bowes CL, Richardson JD, Cumming G, Horsfield, K. Effect of breathing pattern on gas mixing in a model with asymmetrical alveolar ducts. *J Appl Physiol* (1985); **58**: 18–26.
- Dammann JF, Mcaslan TC, Maffeo, CJ. Optimal flow pattern for mechanical ventilation of the lungs. 2. The effect of a sine versus square wave flow pattern with and without an end-inspiratory pause on patients. *Crit Care Med* (1978); **6**: 293–310.
- De Robertis E, Sigurdsson SE, Drefeldt B, Jonson B. Aspiration of airway dead space. A new method to enhance CO<sub>2</sub> elimination. *Am J Respir Crit Care Med* (1999); **159**: 728–732.
- Farhi LE, Rahn H. Gas stores of the body and the unsteady state. *J Appl Physiol* (1955); **7**: 472–484.
- Fletcher R. The single breath test for CO<sub>2</sub>, Thesis (1980), Lund University.
- Fuleihan SF, Wilson RS, Pontoppidan, H. Effect of mechanical ventilation with end-inspiratory pause on blood-gas exchange. *Anesth Analg* (1976); **55**: 122–130.
- Jansson L, Jonson B. A theoretical study on flow patterns of ventilators. *Scand J Respir Dis* (1972); **53**: 237–246.
- Johansson H. Effects on breathing mechanics and gas exchange of different inspiratory gas flow patterns in patients undergoing respirator treatment. *Acta Anaesthesiol Scand* (1975); **19**: 19–27.
- Johansson H, Löfström JB. Effects on breathing mechanics and gas exchange of different inspiratory gas flow patterns during anaesthesia. *Acta Anaesthesiol Scand* (1975); **19**: 8–18.
- Jonson B, Similowski T, Levy P, Viires N, Pariente R. Expiratory flushing of airways: a method to reduce deadspace ventilation. *Eur Respir J* (1990); **3**: 1202–1205.
- Lachmann B, Jonson B, Lindroth M, Robertson B. Modes of artificial ventilation in severe respiratory distress syndrome. Lung function and morphology in rabbits after wash-out of alveolar surfactant. *Crit Care Med* (1982); **10**: 724–732.
- Markström A, Hedlund A, Lichtwarck-Aschoff M, Nordgren A, Sjöstrand U. Impact of different inspiratory flow patterns on arterial CO<sub>2</sub> tension. *Ups J Med Sci* (2000); **105**: 17–29.
- Mercat A, Diehl JL, Michard F et al. Extending inspiratory time in acute respiratory distress syndrome. *Crit Care Med* (2001); **29**: 40–44.
- Richecoeur J, Lu Q, Vieira SR et al. Expiratory washout versus optimization of mechanical ventilation during permissive hypercapnia in patients with severe acute respiratory distress syndrome. *Am J Respir Crit Care Med* (1999); **160**: 77–85.
- Svantesson C, Drefeldt B, Jonson B. The static pressure-volume relationship of the respiratory system determined with a computer-controlled ventilator. *Clin Physiol* (1997); **17**: 419–430.
- Taskar V, John J, Larsson A, Wetterberg T, Jonson B. Dynamics of carbon dioxide elimination following ventilator resetting. *Chest* (1995); **108**: 196–202.
- Uttman L, Jonson B. Computer-aided ventilator resetting is feasible on the basis of a physiological profile. *Acta Anaesthesiol Scand* (2002); **46**: 289–296.
- Weibel ER. *Morphometry of the Human Lung* (1963). Springer-Verlag, Berlin.
- West JB. Causes of carbon dioxide retention in lung disease. *N Engl J Med* (1971); **284**: 1232–1236.
- Wolff G, Brunner JX. Series dead space volume assessed as the mean value of a distribution function. *Int J Clin Monit Comput* (1984); **1**: 177–181.
- Wolff G, Brunner J, Weibel W, Bowes C. Alveolar efficiency for CO<sub>2</sub> elimination and series dead space volume, both are affected by the ventilatory pattern. *Appl Cardiopulm Pathol* (1989a); **2**: 309–314.
- Wolff G, Brunner J, Weibel W, Bowes C, Muchenberger R, Bertschmann W. Anatomical serial dead space volume: concept and measurement in clinical praxis. *Appl Cardiopulm Pathol* (1989b); **2**: 299–307.
- Woolcock AJ, Macklem PT. Mechanical factors influencing collateral ventilation in human, dog, and pig lungs. *J Appl Physiol* (1971); **30**: 99–115.