



The University of
Nottingham

UNITED KINGDOM · CHINA · MALAYSIA

Taggar, Jaspal S. and Coleman, Tim and Lewis, Sarah and Heneghan, Carl and Jones, Matthew (2015) Accuracy of methods for diagnosing atrial fibrillation using 12-lead ECG: a systematic review and meta-analysis. *International Journal of Cardiology*, 184 . pp. 175-183. ISSN 1874-1754

Access from the University of Nottingham repository:

<http://eprints.nottingham.ac.uk/44936/1/J%20Taggar%20Int%20J%20Cardiol%202015.pdf>

Copyright and reuse:

The Nottingham ePrints service makes this work by researchers of the University of Nottingham available open access under the following conditions.

This article is made available under the Creative Commons Attribution Non-commercial No Derivatives licence and may be reused according to the conditions of the licence. For more details see: <http://creativecommons.org/licenses/by-nc-nd/2.5/>

A note on versions:

The version presented here may differ from the published version or from the version of record. If you wish to cite this item you are advised to consult the publisher's version. Please see the repository url above for details on accessing the published version and note that access may require a subscription.

For more information, please contact eprints@nottingham.ac.uk

Accuracy of methods for diagnosing atrial fibrillation using 12-lead ECG: A systematic review and meta-analysis

Jaspal S Taggar¹, Tim Coleman², Sarah Lewis³, Carl Heneghan⁴, Matthew Jones⁵

1 University of Nottingham; This author takes responsibility for all aspects of the reliability and freedom from bias of the data presented and their discussed interpretation

2 University of Nottingham; This author takes responsibility for all aspects of the reliability and freedom from bias of the data presented and their discussed interpretation

3 University of Nottingham; This author takes responsibility for all aspects of the reliability and freedom from bias of the data presented and their discussed interpretation

4 University of Oxford; This author takes responsibility for all aspects of the reliability and freedom from bias of the data presented and their discussed interpretation

5 University of Nottingham; This author takes responsibility for all aspects of the reliability and freedom from bias of the data presented and their discussed interpretation

Address for correspondence:

Dr Jaspal Taggar
Division of Primary Care,
University of Nottingham,
Room C34, Medical School,
Queen's Medical Centre,
Nottingham,
NG7 2UH
Email: Jaspal.taggar@nottingham.ac.uk
Tel: +44 115 8230462
Fax: +44 115 82 30214

Funding:

The study was supported by an NIHR/School for Primary Care Research GP Career Progression Fellowship and Research Capability Funding from Nottingham City Clinical Commissioning Group.

The funding bodies had no role in the design, conduct, interpretation and writing of the report for this research.

Views and opinions expressed in this article are those of the authors and do not necessarily reflect those of the National Institute for Health Research (NIHR) or Nottingham City Clinical Commissioning Group (CCG).

Conflicts of interest:

CH receives payment for running educational courses at the University of Oxford and University of Oxford ISIS consulting services for external teaching and training. He also receives royalties for books (Evidence Based Toolkit series by Blackwell BMJ Books). All other authors report no relationships that could be construed as a conflict of interest.

Keywords: Atrial fibrillation; electrocardiogram; diagnostic accuracy

ABSTRACT

Background: Screening for Atrial fibrillation (AF) using 12-lead-electrocardiograms (ECG) has been recommended; however, the best method for interpreting ECGs to diagnose AF is not known. We compared accuracy of methods for diagnosing AF from ECGs.

Methods: We searched MEDLINE, EMBASE, CINAHL and LILACS until March 24, 2014. Two reviewers identified eligible studies, extracted data and appraised quality using the QUADAS-2 instrument. Meta-analysis, using the bivariate hierarchical random effects method, determined average operating points for sensitivities, specificities, positive and negative likelihood ratios (PLR, NLR) and enabled construction of Summary Receiver Operating Characteristic (SROC) plots.

Results: 10 studies investigated 16 methods for interpreting ECGs (n=55,376 participant ECGs). The sensitivity and specificity of automated software (8 studies; 9 methods) were 0.89 (95% CI 0.82-0.93) and 0.99 (95% CI 0.99-0.99), respectively; PLR 96.6 (95% C.I 64.2-145.6); NLR 0.11 (95% C.I 0.07-0.18). Indirect comparisons with software found healthcare professionals (5 studies; 7 methods) had similar sensitivity for diagnosing AF but lower specificity [sensitivity 0.92 (95% CI 0.81-0.97), specificity 0.93 (95% CI 0.76-0.98), PLR 13.9 (95% C.I 3.5-55.3), NLR 0.09 (95% C.I 0.03-0.22)]. Sub-group analyses of primary care professionals found greater specificity for GPs than nurses [GPs: sensitivity 0.91 (95% C.I 0.68-1.00); specificity 0.96 (95% C.I 0.89-1.00). Nurses: sensitivity 0.88 (95% C.I 0.63-1.00); specificity 0.85 (95% C.I 0.83-0.87)].

Conclusions: Automated ECG-interpreting software most accurately excluded AF, although its ability to diagnose this was similar to all healthcare professionals. Within primary care, the specificity of AF diagnosis from ECG was greater for GPs than nurses.

BACKGROUND

Atrial fibrillation (AF) is the most common sustained cardiac arrhythmia and has a prevalence that increases with age.¹ AF is associated with significant morbidity, mortality and impaired quality of life, most notably from its associated four to five fold increased risk of ischaemic stroke, and poses a significant public health burden.^{2,3}

Screening for AF in primary care has been found to be an effective strategy for detecting AF.^{4,5} The SAFE trial, set in primary care, found opportunistic pulse palpation and confirmatory 12-lead electrocardiogram (ECG) significantly increased the detection of incident AF cases when compared to routine practice in patients over 65 years old.⁴ Consequently, this approach to AF screening, combined with the appropriate provision of antithrombotic therapy, has been proposed as a population intervention to reduce the burden of thromboembolic complications.⁶

A sub-study of the SAFE trial investigated the accuracy of 12-lead ECG diagnoses of AF made by GPs, nurses and automated software in primary care.⁷ Mant et al. found, as compared to ECG diagnoses made by cardiologists, interpretive software had a significantly greater specificity than all methods for diagnosing AF. However, the sensitivities for GPs, nurses and software for AF diagnosis were substantially lower and similar across all groups, and suggested the accuracy in primary care using any single method was insufficient for screening.

A recent narrative literature review of methods for detecting AF reported substantial variation in the accuracy of ECG diagnoses made by primary care practitioners, although, to date, there has been no systematic evaluation of the evidence for the range of different methods for diagnosing AF using 12-lead ECG. This systematic review therefore aimed to identify the range of methods for interpreting whether or not 12-lead ECGs show AF, and to compare their diagnostic accuracies.

METHODS

Search strategy and selection criteria

This study was conducted in accordance with guidelines and methods for systematic reviews and meta-analyses of diagnostic tests.⁸⁻¹¹ We searched MEDLINE, EMBASE, Cumulative Index to Nursing & Allied Health (CINAHL) and Latin American and Caribbean Health Sciences Information System (LILACS) in all languages published from inception until 24th March 2014 (See appendix for search terms). Additionally, the reference lists of national guidelines, review articles and eligible studies were hand-searched to identify potential studies. We included all randomised trials and observational studies that i) recruited participants ≥ 18 years of age, ii) investigated any method for interpreting 12-lead ECGs to show AF (the index test) with 12-lead ECG diagnoses of AF made by a trained specialist (the reference standard), iii) involved healthcare professionals in making AF diagnoses and iv) sufficient data available to enable the calculation of diagnostic accuracy. Studies that investigated invasive or echocardiographic methods for diagnosing AF were excluded, as these methods would not be translatable into routine screening practice. After the removal of duplicate citations, two reviewers (JT and MJ) independently screened citations for relevance and reviewed full-text articles using the predetermined eligibility criteria. Any disagreements were resolved by consensus with a third reviewer (TC).

Data extraction

Two reviewers (JT and MJ) independently extracted data using a pre-specified data extraction form. Any disagreements were resolved by consensus with a third reviewer (TC). The lead authors of studies for which reported data were insufficient to calculate diagnostic accuracy were contacted to ascertain missing data.

Study quality was appraised using the Quality Assessment of Diagnostic Accuracy Studies-2 (QUADAS-2) instrument.^{10, 12} Additionally, the studies were graded using the quality scale reported by Van den Bruel et al;¹³ studies were rated as grade A if they fulfilled all QUADAS-2 criteria. Studies were graded D if there was no or unclear verification of the index test findings with the reference standard, or if

the index test results were interpreted un-blinded to the results of the reference test. Studies where there was an unduly long time delay between index and reference test, or where the reference test was not independent of the index test, or where the reference test was interpreted un-blinded to the results of the index test were graded C. Remaining studies which did not fall in to these categories were graded B.

Statistical analysis

We constructed 2x2 contingency tables to enable the calculation of sensitivity and specificity for each method of diagnosing AF as measures of diagnostic accuracy, and we used the bivariate hierarchical random effects method to determine the average operating points for sensitivity and specificity, which enabled construction of Summary Receiver Operating Characteristic (SROC) plots with 95% prediction regions.¹¹ We also calculated positive likelihood ratios (PLR) and negative likelihood ratios (NLR) for each method of diagnosing AF. Unlike sensitivity and specificity, likelihood ratios make explicit the impact of the test result on the probability of the disease. To minimise heterogeneity we analysed the results a priori grouped according to method of diagnosing AF, and diagnostic accuracy was assessed by comparison of sensitivities and specificities with respective 95% confidence intervals. Sub-group analyses were planned according to study quality and groups of healthcare professionals in primary care. We used univariate random effects meta-analysis to derive pooled estimates for sensitivity and specificity when there were less than four studies within sub-groups as the bivariate model is unreliable in this context. Heterogeneity is presumed in meta-analyses of diagnostic test studies and the I^2 statistic cannot be reliably used for its assessment.¹¹ We therefore described heterogeneity by variation in the outcomes from included studies and our pooled estimates by visual inspection of the SROC plots and how close individual studies lie to the predicted ROC curve.¹¹ An assessment of publication bias was made according to categories of method for detecting AF using Deek's Funnel plot asymmetry test; a P-value<0.10 was used to signify the presence of publication

bias. Analyses were conducted using Stata Version 11.0 and Review Manager 5.2 for quality assessments.

RESULTS

We identified, after the removal of duplicate records, 4,426 potential citations, of which 62 were identified as relevant for detailed evaluation (figure 1). After full-text review, 10 studies were included in the final analyses (table 1).¹⁴⁻²³ There was one study that met selection criteria for which there were insufficient data for reported outcomes (table 2).²⁴

Study characteristics

Of the 10 studies included in our review (table 1), there was one randomised trial,¹⁸ two case-control^{22, 23} and seven cross-sectional studies.^{14-17, 19-21} The 10 studies investigated a total of 16 methods of diagnosing AF (a total of 55,376 participant ECGs), which were categorised into two intervention groups: 1) automated software (eight studies; nine diagnostic methods)¹⁴⁻²¹ and, 2) any healthcare professional (five studies; seven diagnostic methods).^{17, 18, 21-23} Sub-groups of healthcare professional were defined as: secondary care physicians (two studies; two diagnostic methods) and^{17, 22} primary care professionals (three studies; five diagnostic methods),^{18, 21, 23} the latter comprising GPs (three studies)^{18, 21, 23} and practice nurses (two studies).^{18, 23}

Across studies without a case control design, the prevalence of AF ranged from 6.7% to 18.6%. (See Table 1). The three studies conducted in a primary care setting included participants over 65 years of age and recruited patients eligible for AF screening.^{18, 21, 23} However, the remainder of studies were conducted using patients with existing cardiac pathologies in a secondary care setting.

For five studies, the reference standard was 12-lead ECG interpreted by at least two cardiologists. Of the remaining studies, four used ECG interpretation by a single cardiologist as the reference standard and one study used two trained secondary care clinicians.¹⁴

Quality assessment

Figure 2 shows the methodological quality of included studies according to QUADAS-2 criteria was generally low. Five studies with the lowest methodological quality (D-grade) were due to the methodological interpretation of the reference standard being unclear or at high risk of bias. One

study was graded as category C because it was unclear whether the reference standard was interpreted without knowledge of the index test.

Data synthesis

Automated software was found to have a pooled sensitivity of 0.89 (95% CI 0.82-0.93) and specificity of 0.99 (95% CI 0.99-0.99) for diagnosing AF using 12-lead ECG. (Figure 3) This corresponded with a PLR of 96.6 (95% C.I 64.2-145.6) and NLR of 0.11 (95% C.I 0.07-0.18). In contrast, the pooled specificity for the accuracy of any healthcare professional diagnosing AF (Figure 4) was lower than automated software although there was a similar sensitivity of this method for interpreting ECGs; sensitivity 0.92 (95% CI 0.81-0.97), specificity 0.93 (95% CI 0.76-0.98), PLR 13.9 (95% C.I 3.5-55.3), NLR 0.09 (95% C.I 0.03-0.22).

Figure 5 shows the sensitivity and specificity for diagnosing AF by primary care professionals was relatively high [sensitivity 0.96 (95% CI 0.66-1.00), specificity 0.94 (95% CI 0.85-0.98), PLR 15.4 (95% C.I 5.9-40.3), NLR 0.05 (95% C.I 0.00 to 0.49)]. The sub-group analyses for categories of GPs and nurses (figure 6) suggest this may be driven by a greater specificity of GPs' AF diagnoses [GPs: sensitivity 0.91 (95% C.I 0.68-1.00); specificity 0.96 (95% C.I 0.89-1.00) when compared to nurses: sensitivity 0.88 (95% C.I 0.63-1.00); specificity 0.85 (95% C.I 0.83-0.87)].

Visual inspection of the SROC plots (figure 7) confirms there was substantial variation in the outcomes from studies investigating the accuracy of clinicians' 12-lead ECG diagnosis and suggests heterogeneity amongst these studies was greater than the automated software studies.

There was no evidence of publication bias for studies of any clinician ($p=0.29$) or any primary care clinician diagnosis ($p=0.19$). However, studies of software ECG interpretation suggested the presence of publication bias, ($p=0.02$), with the possible underrepresentation of smaller studies with a lower accuracy of diagnosing AF. Bivariate sub-group analyses were similar after exclusion of studies with the lowest quality [Software: sensitivity 0.82 (95% C.I 0.73-0.88), specificity 0.99 (95% C.I 0.98-0.99); any healthcare professionals: sensitivity 0.92 (95% C.I 0.81-0.97), specificity 0.91 (95% C.I 0.70-0.98);

any primary care professionals: sensitivity 0.93 (95% C.I 0.67-0.99), specificity 0.92 (95% C.I 0.85-0.96)].

DISCUSSION

This review of 10 studies found automated software analysis had a borderline greater specificity for AF diagnosis than healthcare professional interpretation of 12-lead ECGs. The sensitivities of automated software, any healthcare professionals and primary care professionals for interpreting 12-lead ECGs to diagnose AF were similar.

Strengths and limitations

To our knowledge, this study is the first systematic review and meta-analysis of different methods for interpreting 12-lead ECGs to diagnose AF. A strength of our study was the use of a standardised protocol that is consistent with published guidelines for systematic reviews of diagnostic test studies. Moreover, we used a comprehensive search strategy that included contacting authors of potentially relevant studies. Our findings indicated a probable lack of publication bias for studies of clinicians' 12-lead ECG diagnoses of AF. However, there was the possibility of publication bias for studies investigating automated software and this may limit the validity of the findings for this diagnostic modality. One study was excluded due to the insufficient reporting of outcome data to enable meta-analysis and this could have influenced our findings. However, the number of misdiagnoses of AF was similar to that of other studies investigating the accuracy of automated software for making ECG diagnoses of AF and the impact of excluding this study is likely to be minimal. Only one of the nine included studies adopted a prospective design and there were a number of inherent methodological weaknesses in other studies as reflected by our appraisal of study quality. No studies were judged to have met all QUADAS-2 criteria. However, our bivariate sub-group analyses that excluded studies judged to have the lowest (grade D) methodological quality found similar outcomes to our primary analyses, and strengthens the validity of our findings. Most studies were conducted in a secondary care setting and there was substantial variation in the proportion of patients with AF. This limits the generalisability of our findings to unselected primary care populations that AF screening is intended for. However, the measures used to determine diagnostic accuracy in our study are prevalence independent and, consequently, our findings could be translatable to populations in different

healthcare settings. There was heterogeneity amongst the studies within all categories of methods for diagnosing AF and this is likely to be attributable to differences in study population and design. This variation was least for studies of automated software and strengthens the validity of findings for this approach to AF diagnosis. Heterogeneity was greatest for the category of any healthcare professionals' interpretation of 12-lead ECGs and is likely to arise from differences in professional groups and clinical expertise.

Findings in context of previous research

Our review identified automated software and healthcare professional interpretation of 12-lead ECGs as methods for diagnosing AF. Furthermore, we also analysed the interpretation of ECGs in a restricted group of primary care professionals. Our findings for automated software, using sensitivity and specificity as measures of diagnostic accuracy, are consistent with those from the SAFE study.^{4, 7, 18} Due to the significantly higher specificity of this diagnostic modality, our findings suggest software is the best method for correctly identifying patients with normal 12-lead ECGs and minimising the risk of false positive diagnoses of AF.

The sensitivities of all methods for diagnosing AF were similar, although these were sufficiently low to give rise to false negative AF diagnoses. As compared to any healthcare professionals' ECG interpretation, the point estimates for sensitivity and specificity were reassuringly high for AF diagnoses made by primary care professionals. However, our sub-group analyses suggest this may be attributable to better 12-lead ECG interpretation by GPs; in comparison to GPs, nurses were found to have a significantly lower specificity for diagnosing AF. The point estimates for the accuracy of primary care clinicians' AF diagnoses contrast with outcomes from the SAFE study. The SAFE trial was the largest, pragmatic study of AF screening in primary care⁴ and secondary analyses of the trial data suggest the accuracy of GP and nurse AF diagnoses was substantially lower than our findings.⁷ Although data from SAFE were included in our meta-analyses, the difference in outcomes between

this study and our pooled results may arise from the statistical approach used for data synthesis; random effects meta-analysis would have provided greater weighting to the smaller, low quality studies that reported a higher diagnostic accuracy arising from primary care professionals, thus inflating the pooled estimates in our review. Moreover, the primary care studies investigating the accuracy of diagnosing AF are likely to have included self-selecting practices with an interest in AF and it is possible that the accuracy of diagnosing arrhythmia by primary care professionals in routine practice could be even lower than that found in the SAFE trial and our review.

The current gold-standard test for diagnosing AF is 12-lead ECG^{6, 25} and consensus recommends this should be interpreted by competent healthcare professionals as part of AF screening.²⁶ Both systematic and opportunistic screening for AF using 12-lead ECG in patients over 65 years was found to be an effective approach for improving the detection of this arrhythmia.⁴

Screening for AF is likely to be implemented in primary care and, consequently, healthcare professionals in this setting would be expected to undertake screening activities. It is unclear what the optimal service configurations are for delivering such a screening programme and both GPs and nurses may be expected to undertake the role of diagnosing AF. Our findings suggest there is potential for combining mixed modalities of ECG interpretation for the diagnosis of AF. Certainly, automated software has potential utility for the triage of ECGs and exclusion of patients with normal ECG findings. However, correctly diagnosing AF using software interpretation alone has a limited sensitivity resulting in the potential for incorrect exclusion of AF, and interpreting ECGs to verify the presence of AF in this circumstance is likely to require additional interpretation from a competent healthcare professional.²⁶ The findings of this review suggest the accuracy of correctly making AF diagnoses by primary care professionals, in particular nurses, could be improved. It is therefore conceivable that the skills of healthcare professionals in this setting would need improving to ensure the effectiveness of screening is not undermined.

The opinions of primary care professionals about AF screening are not known and a greater understanding of the barriers, facilitators and learning needs of these important stakeholder groups, in particular nurses, is required before screening can be implemented optimally. Furthermore, studies that investigate optimal service configurations for diagnosing AF in primary care and how these translates into better detection rates would help plan the delivery of an effective national AF screening programme.

Conclusions

Automated software had the greatest specificity for AF diagnosis using 12-lead ECG than healthcare professional diagnosis of this arrhythmia. Although the accuracy of diagnosing AF in primary care is reassuring, this is driven by GP's diagnosis of AF. If a national AF screening programme is introduced into primary care it is possible that the skills of GPs and nurses for making 12-lead ECG diagnoses of AF could be improved to ensure the effectiveness of screening is not undermined.

REFERENCES

1. Davis RC, Hobbs FD, Kenkre JE, Roalfe AK, Iles R, Lip GY and Davies MK. Prevalence of atrial fibrillation in the general population and in high-risk groups: the ECHOES study. *Europace*. 2012;14:1553-9.
2. The Stroke Risk in Atrial Fibrillation Working Group. Independent predictors of stroke in patients with atrial fibrillation: A systematic review. *Neurology*. 2007;69:546-554.
3. Stewart S, Murphy NF, Walker A, McGuire A and McMurray JJ. Cost of an emerging epidemic: an economic analysis of atrial fibrillation in the UK. *Heart*. 2004;90:286-92.
4. Fitzmaurice DA, Hobbs FD, Jowett S, Mant J, Murray ET, Holder R, Raftery JP, Bryan S, Davies M, Lip GY and Allan TF. Screening versus routine practice in detection of atrial fibrillation in patients aged 65 or over: cluster randomised controlled trial. *Bmj*. 2007;335:383.
5. Moran PS, Flattery MJ, Teljeur C, Ryan M and Smith SM. Effectiveness of systematic screening for the detection of atrial fibrillation. *Cochrane Database Syst Rev*. 2013;4:CD009586.
6. Camm AJ, Lip GY, De Caterina R, Savelieva I, Atar D, Hohnloser SH, Hindricks G and Kirchhof P. 2012 focused update of the ESC Guidelines for the management of atrial fibrillation: an update of the 2010 ESC Guidelines for the management of atrial fibrillation. Developed with the special contribution of the European Heart Rhythm Association. *Eur Heart J*. 2012;33:2719-47.
7. Mant J, Fitzmaurice DA, Hobbs FD, Jowett S, Murray ET, Holder R, Davies M and Lip GY. Accuracy of diagnosing atrial fibrillation on electrocardiogram by primary care practitioners and interpretative diagnostic software: analysis of data from screening for atrial fibrillation in the elderly (SAFE) trial. *Bmj*. 2007;335:380. Epub 2007 Jun 29.
8. Bossuyt PM and Leeflang MM. Chapter 6: Developing Criteria for Including Studies. In: *Cochrane Handbook for Systematic Reviews of Diagnostic Test Accuracy Version 0.4* [updated September 2008]. 2008.
9. de Vet HCW, Eisinga A, Riphagen II, Aertgeerts B and Pewsner D. Chapter 7: Searching for Studies. In: *Cochrane Handbook for Systematic Reviews of Diagnostic Test Accuracy Version 0.4* [updated September 2008]. 2008.
10. Reitsma JB, Rutjes AWS, Whiting P, Vlassov VV, Leeflang MMG and Deeks JJ. Chapter 9: Assessing methodological quality. In: Deeks JJ, Bossuyt PM, Gatsonis C (editors), *Cochrane Handbook for Systematic Reviews of Diagnostic Test Accuracy Version 1.0.0*. 2009.
11. Macaskill P, Gatsonis C, Deeks JJ, Harbord RM and Takwoingi Y. Chapter 10: Analysing and Presenting Results. In: Deeks JJ, Bossuyt PM, Gatsonis C (editors), *Cochrane Handbook for Systematic Reviews of Diagnostic Test Accuracy Version 1.0*. 2010.
12. Whiting PF, Rutjes AW, Westwood ME, Mallett S, Deeks JJ, Reitsma JB, Leeflang MM, Sterne JA and Bossuyt PM. QUADAS-2: a revised tool for the quality assessment of diagnostic accuracy studies. *Ann Intern Med*. 2011;155:529-36.
13. Van den Bruel A, Thompson MJ, Haj-Hassan T, Stevens R, Moll H, Lakhanpaul M and Mant D. Diagnostic value of laboratory tests in identifying serious infections in febrile children: systematic review. *Bmj*. 2011;342.
14. Bourdillon PJ and Kilpatrick D. Clinicians, the Mount Sinai program and the Veterans' Administration program evaluated against clinico-pathological data derived independently of the electrocardiogram. *Eur J Cardiol*. 1978;8:395-412.
15. Davidenko JM and Snyder LS. Causes of errors in the electrocardiographic diagnosis of atrial fibrillation by physicians. *J Electrocardiol*. 2007;40:450-6.
16. Gregg RE, Zhou SH, Lindauer JM, Feild DQ and Helfenbein ED. Where do derived precordial leads fail? *J Electrocardiol*. 2008;41:546-52.
17. Hakacova N, Tragardh-Johansson E, Wagner GS, Maynard C and Pahlm O. Computer-based rhythm diagnosis and its possible influence on nonexpert electrocardiogram readers. *J Electrocardiol*. 2012;45:18-22.

18. Hobbs FDR, Fitzmaurice DA, Mant J, Murray E, Jowett S, Bryan S, Raftery J, Davies M and Lip G. A randomised controlled trial and cost-effectiveness study of systematic screening (targeted and total population screening) versus routine practice for the detection of atrial fibrillation in people aged 65 and over. The SAFE study. *Health Technology Assessment* 2005;9:iii-iv, ix-x, 1-74.
19. Poon K, Okin PM and Kligfield P. Diagnostic performance of a computer-based ECG rhythm algorithm. *J Electrocardiol.* 2005;38:235-8.
20. Reddy BRS, Taha B, Swiryn S, Silberman R and Childers R. Prospective evaluation of a microprocessor-assisted cardiac rhythm algorithm: Results from one clinical center. *J Electrocardiol.* 1998;30:28-33.
21. Rhys G, Azhar M and Foster A. Screening for atrial fibrillation in patients aged 65 years or over attending annual flu vaccination clinics at a single general practice. *Quality in Primary Care.* 2013;21:131-140.
22. Shiyovich A, Wolak A, Yacobovich L, Grosbard A and Katz A. Accuracy of diagnosing atrial flutter and atrial fibrillation from a surface electrocardiogram by hospital physicians: analysis of data from internal medicine departments. *Am J Med Sci.* 2010;340:271-5.
23. Somerville S, Somerville J, Croft P and Lewis M. Atrial fibrillation: a comparison of methods to identify cases in general practice. *Br J Gen Pract.* 2000;50:727-9.
24. Bogun F, Anh D, Kalahasty G, Wissner E, Bou Serhal C, Bazzi R, Weaver WD and Schuger C. Misdiagnosis of atrial fibrillation and its clinical consequences. *Am J Med.* 2004;117:636-42.
25. National Institute for Health and Care Excellence. Atrial Fibrillation: CG180. 2014.
26. Royal College of Physicians of Edinburgh. RCPE UK Consensus Conference on "Approaching the comprehensive management of Atrial Fibrillation: Evolution or revolution?" 2012.

TABLES

Table 1: Characteristics of included studies

Study	Setting, population & sample size	AF Prevalence/ proportion (%)	Study Design†	Index test(s)	Reference test	Outcomes	Quality grading
Bourdillon 1978 ¹⁴	UK; secondary care; 221 ECGs of adult subjects	18.6	CS	Software interpretation (Mount Sinai)	2 clinicians, independent interpretation	Test 1: Sensitivity 0.85; specificity 0.98	C
Davidenko 2007 ¹⁵	USA; secondary care; 35,508 consecutive ECGs were reviewed	7.9	CS	Software diagnosis (Marquettes)	Interpretation by several cardiologists with a group consensus	Sensitivity 0.97; specificity 1.00	D
Gregg 2008 ¹⁶	UK; secondary care; database of 50,000 hospital ECGs; 1,785 randomly selected	6.1	CS	Software interpretation	Interpreted by 2 cardiologists	Sensitivity 0.89; specificity 0.99	D
Hakacova 2012 ¹⁷	Sweden; secondary care; total of 576 ECGs from 503 participants with a mean age of 64 years	10.4	CS	Test 1: Non expert secondary care clinician Test 2: Software A Test 3: Software B	Interpreted by 2 expert cardiologists	Test 1: Sensitivity 0.86; specificity 0.99 Test 2: Sensitivity 0.92; specificity 0.99 Test 3: Sensitivity 0.68; specificity 0.98	B
Hobbs 2005 ¹⁸	UK; primary care; 9,866 patients aged ≥ 65 years, 2595 ECGs were reviewed	6.8 6.7 8.4	RCT	Test 1: General practitioner interpretation Test 2: Practice nurse interpretation	Interpreted by 2 consultant cardiologists independently, with a third if arbitration was needed	Test 1: Sensitivity 0.80; specificity 0.92 Test 2: Sensitivity 0.77; specificity 0.85 Test 3: Sensitivity 0.83; specificity 0.99	B

				Test 3: Biolog software interpretation			
Poon 2005 ¹⁹	USA; secondary care; 4,297 consecutive ECGs were reviewed	6.3	CS	Software interpretation (not specified)	Cardiologist interpretation	Sensitivity 0.91; specificity 0.99	D
Reddy 1998 ²⁰	USA; secondary care; 10,352 ECGs were reviewed	8	CS	Mac-rhythm software interpretation	Cardiologist interpretation	Sensitivity 0.88; specificity 0.99	D
Rhys 2013 ²¹	UK; primary care; patients ≥65 years recruited from flu clinics; 32 ECGs reviewed	6.3	CS	Test 1: Software interpretation Test 2: General practitioner interpretation	ECG interpreted by cardiologist	Test 1: Sensitivity 1; specificity 1 Test 2: Sensitivity 1; specificity 1	D
Shiyovich 2010 ²²	Israel; secondary care; 268 patient's ECGs	81.7	CC	Secondary care clinician interpretation	Interpretation by 2 senior cardiologists	Sensitivity 0.97; specificity 0.31	B
Somerville 2000 ²³	UK; Primary care; 86 patients recruited from one general practice, 86 ECGs reviewed	31.5 30.2	CC	Test 1: Practice nurse interpretation Test 2: General practitioner interpretation	Interpreted by consultant cardiologist	Test 1: Sensitivity 0.97; specificity 0.88 Test 2: Sensitivity 1; specificity 0.98	B

†CC = Case-control study; CS = cross-sectional study; RCT = Randomised controlled Trial; C = Cohort study

Table 2: Characteristics includable studies with insufficient data.

Author/Year	Setting, population & sample size	Study design	Intervention	Comparator	Reported outcomes	Reason for exclusion
Bogun 2004 ²⁴	USA; secondary care; database of 2298 ECGs from 1085 patients	Cross sectional	Software interpretation using GE Marquette 12 SE or MACR programs, overread by cardiologists	Interpretation by 2 electrophysiologists	442 (19%) of the 2298 ECGs had an incorrect computer interpretation of AF in 382 (35%) of patients	Number of true AF, false AF, missed AF, and non AF were not reported

FIGURES

Figure 1: Study selection and stratification

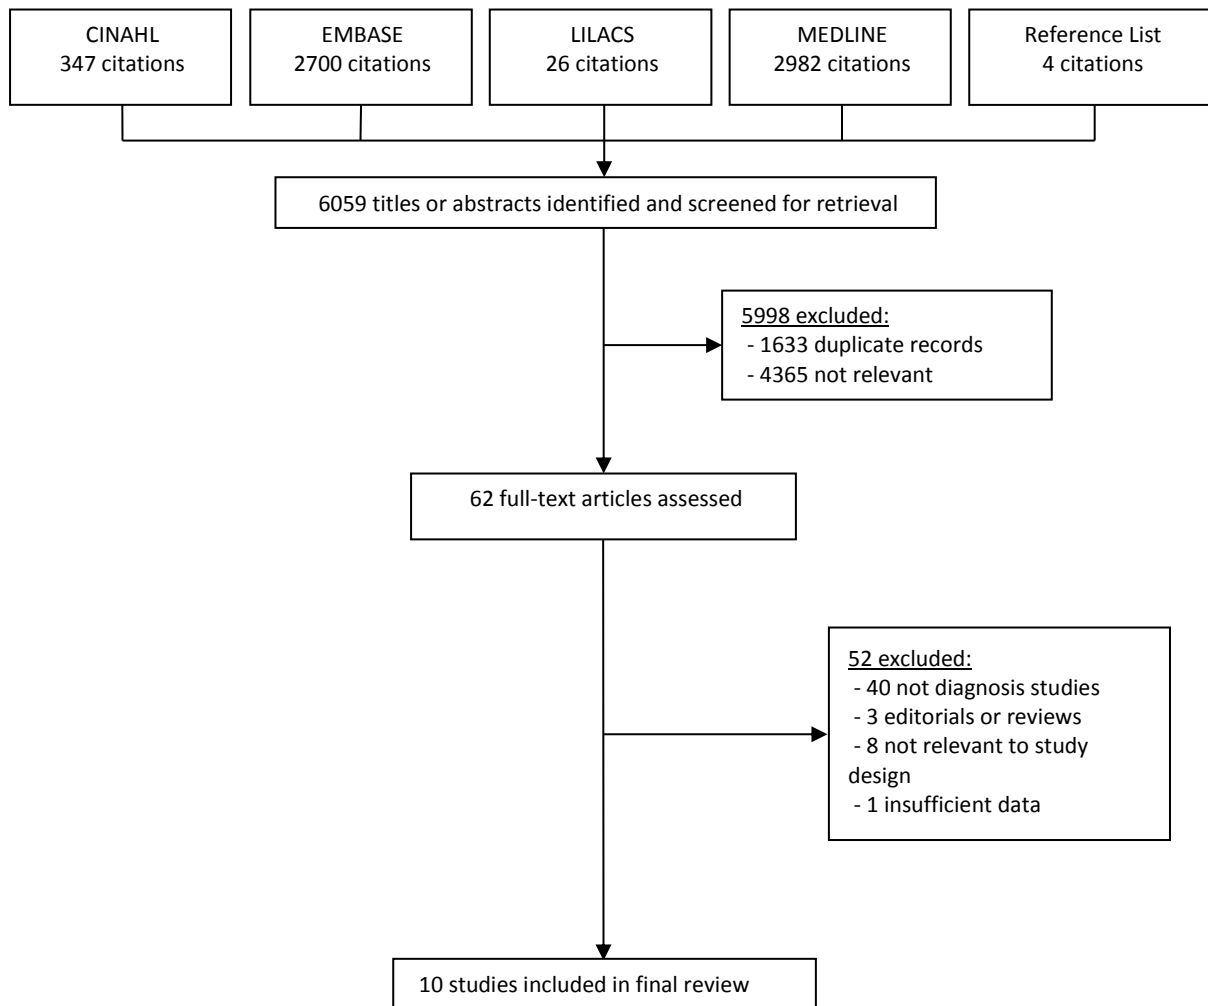


Figure 2: Study quality according to QUADAS-2 criteria

	<u>Risk of Bias</u>					<u>Applicability Concerns</u>			
	Patient Selection	Index Test: Software diagnosis	Index Test: Clinician diagnosis	Reference Standard	Flow and Timing	Patient Selection	Index Test: Software diagnosis	Index Test: Clinician diagnosis	Reference Standard
Bourdillon 1978	?	+		+	+	+	+		+
Davidenko 2007	+	+		?	-	+	+		+
Gregg 2008	?	+		?	+	+	+		+
Hakacova 2012	+	+	+	+	+	+	+	+	+
Hobbs 2005	+	+	+	+	+	+	+	+	+
Poon 2005	?	+		?	+	+	+		+
Reddy 1998	-	+		?	-	+	+		+
Rhys 2013	-	+	+	-	-	?	+	+	+
Shiyovich 2010	-		+	+	+	+		+	+
Somerville 2000	-		+	+	-	+		+	+




 High	 Unclear	 Low
--	---	---

Figure 3: Sensitivity and specificity of 12-lead ECG interpretation using automated software

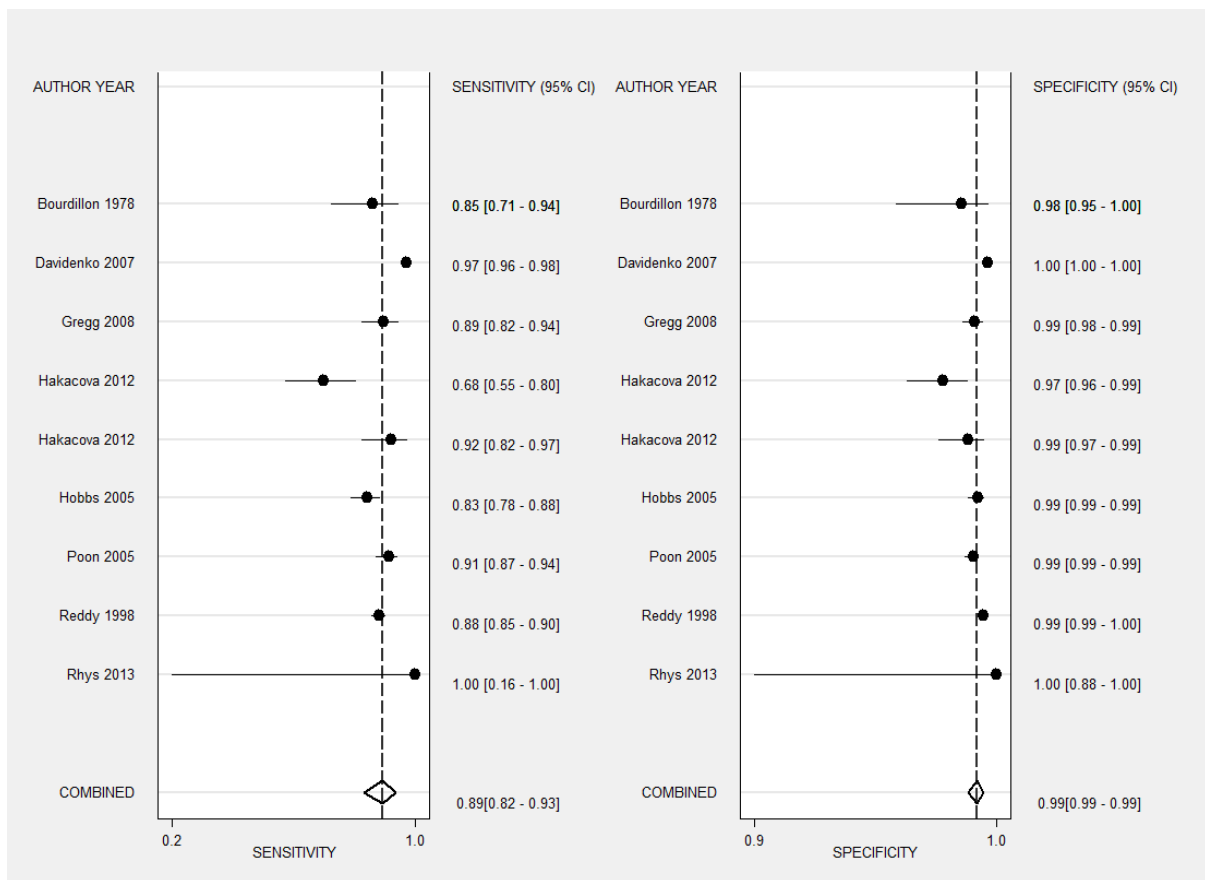


Figure 4: Sensitivity and specificity of 12-lead ECG interpretation by any healthcare professional

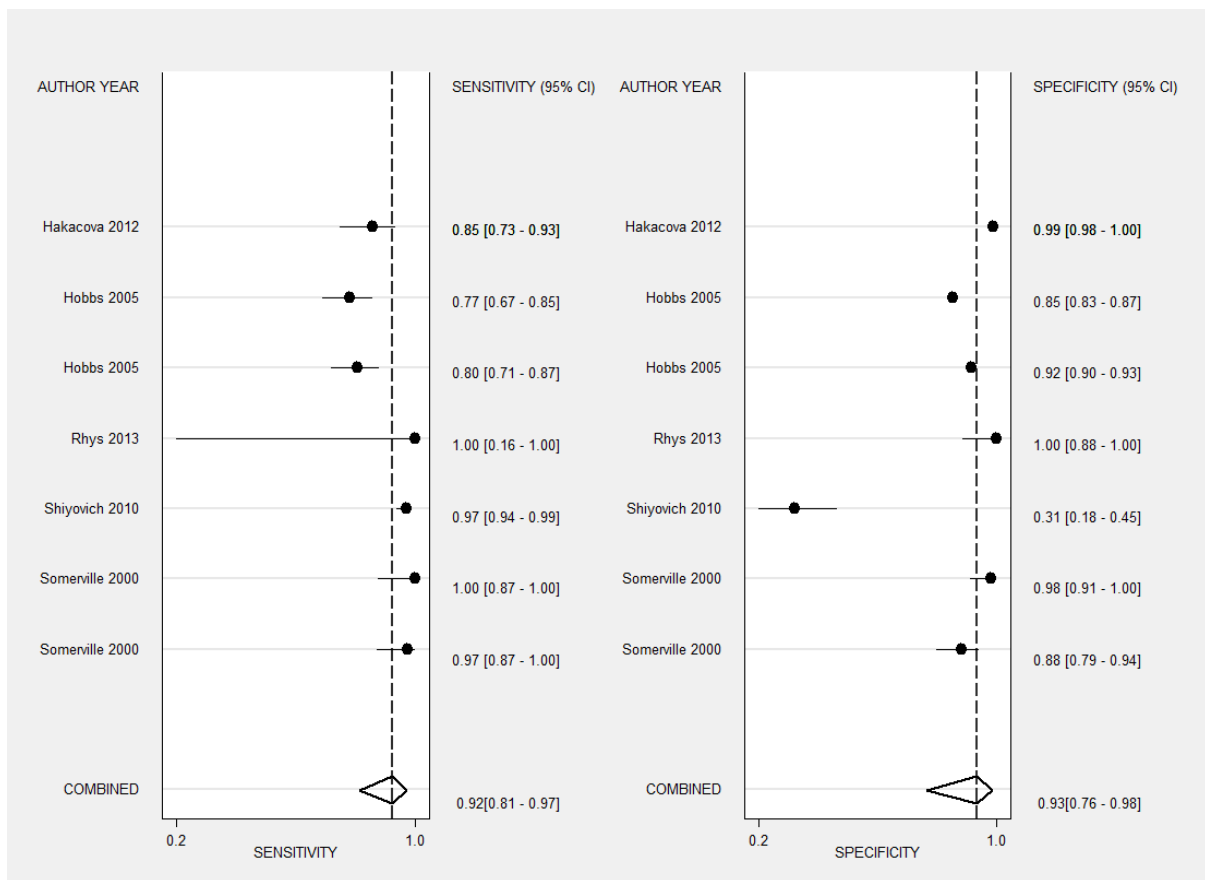


Figure 5: Sensitivity and specificity of 12-lead ECG interpretation by primary care professionals

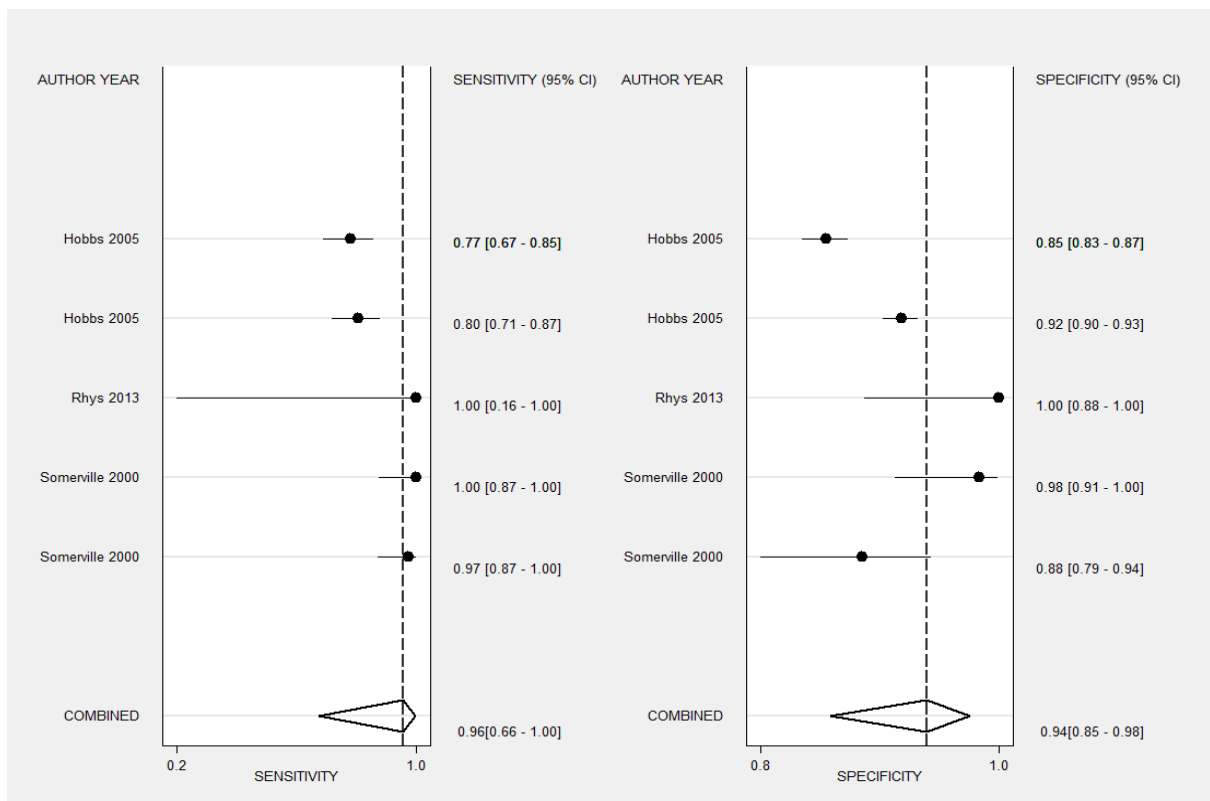


Figure 6: Sub-group analyses of the sensitivity and specificity of 12-lead ECG interpretation by GPs and practice nurses

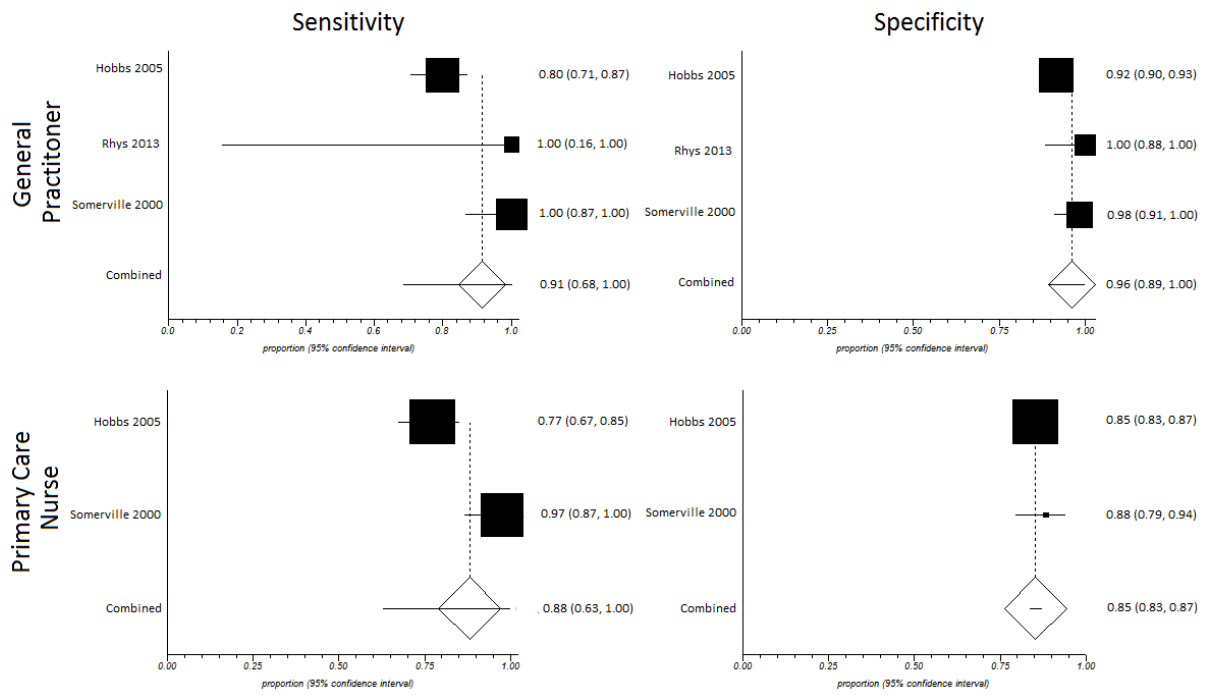


Figure 7: Summary Receiver Operating Characteristic (SROC) plots for the accuracy of 12-lead ECG interpretation by software, any clinician, and primary care clinician

