

October 1970

Brief 70-10531

NASA TECH BRIEF



NASA Tech Briefs announce new technology derived from the U.S. space program. They are issued to encourage commercial application. Tech Briefs are available on a subscription basis from the Clearinghouse for Federal Scientific and Technical Information, Springfield, Virginia 22151. Requests for individual copies or questions relating to the Tech Brief program may be directed to the Technology Utilization Division, NASA, Code UT, Washington, D.C. 20546.

Economic Method for Measuring Ultra-Low Flow Rates of Fluids

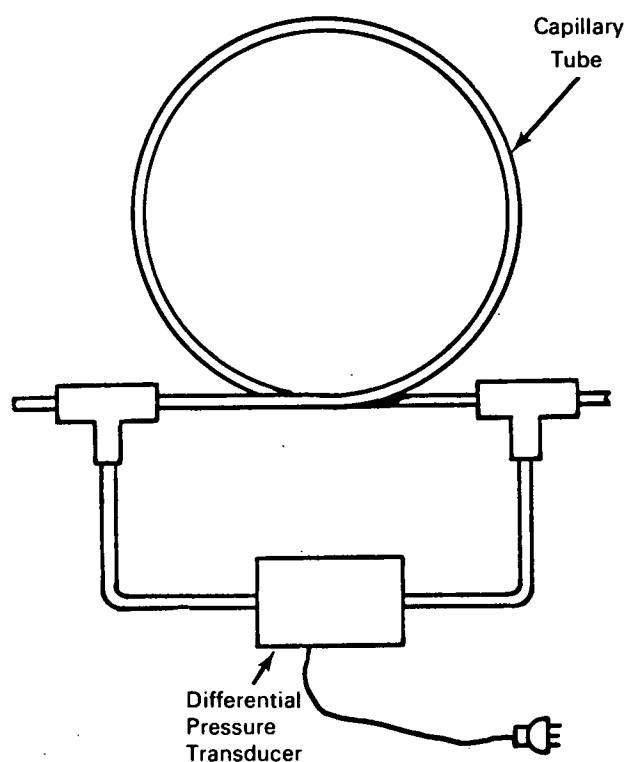


Figure 1. Capillary Tube Flowmeter

A capillary tube flowmeter has been designed to measure ultra-low flows of corrosive and other liquids. The method used is economical and should be of interest to the chemical industry.

A differential pressure transducer is used which measures the linear pressure drop across a coil of capillary tubing. Through calibration with water and analytical conversion, flow rates of very corrosive fluids (such as chlorine trifluoride and liquid fluorine)

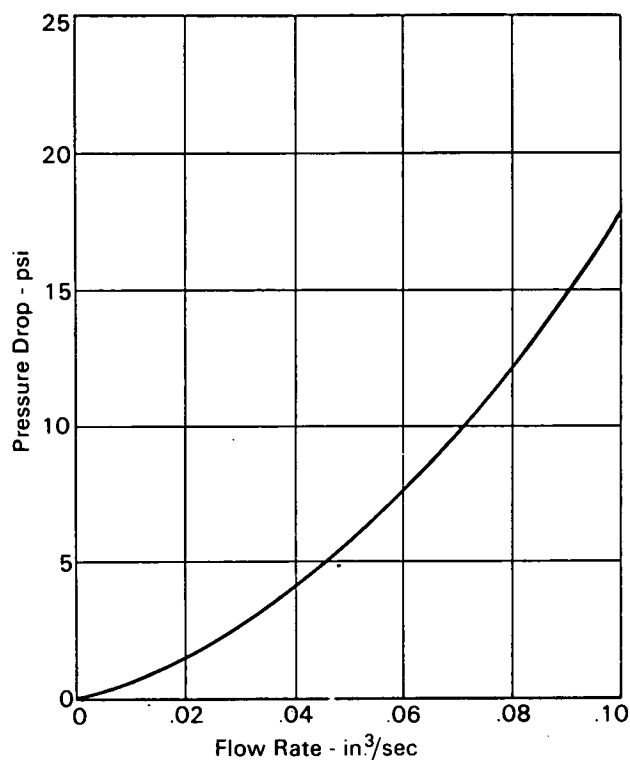


Figure 2. Capillary Tube Flowmeter - Pressure Drop Versus Flow Rate for Chlorine Trifluoride

as low as 0.005 gpm can be measured with reasonable accuracy.

The essential elements of the capillary tube flowmeter, shown in Figure 1, include 4 feet of 1/16-in. tubing and a differential pressure transducer. The flowmeter operates on the principle that for laminar flow in the tube, the pressure drop is proportional to the flow rate. Since the capillary tube is smaller in diameter than the rest of the system's lines, reducers

(continued overleaf)

are required at each end of the line. The abrupt changes in line size are also sensed by the differential pressure transducer and should follow the pressure drop function. The total pressure drop which a transducer will thus sense is expressed by the formula

$$P = K_1 Q^2 + K_2 Q$$

where Q is the fluid flow, and K_1 and K_2 are functions of the fluid flowing through the meter and the meter geometry. The calibration test using water results in one set of values for K_1 and K_2 . Once the meter has been calibrated with water, it is simple to modify the equation for any liquid. The coefficients K_1 and K_2 are proportional to the viscosity and density ratios of the liquid to water, respectively. Applying the viscosity and density for chlorine trifluoride, the result is

$$P = 1314Q^2 + 45.7Q$$

which is shown graphically in Figure 2.

During valve opening and closing transients, flow measurements cannot be made because of cavitation or water hammer in the differential pressure transducer lines. Once the valve transient has damped out, the flowmeter reading can be made with reasonable

accuracy. The flowmeter error at the design flow rate of about $0.03 \text{ in.}^3/\text{sec}$ is $\pm 0.002 \text{ in.}^3/\text{sec}$ if a differential pressure transducer error of $\pm 0.25 \text{ psi}$ is assumed. The flow rate error can be shown mathematically to be a function of pressure differential and pressure differential error.

Note:

No additional documentation is available. Specific questions, however, may be directed to:

Technology Utilization Officer
NASA Pasadena Office
4800 Oak Grove Drive
Pasadena, California 91103
Reference: B70-10531

Patent status:

No patent action is contemplated by NASA.

Source: J.A. Bogdanovic and W.F. Keller of
Northrop Corp.
under contract to
NASA Pasadena Office
(NPO-12064)