

# NASA TECH BRIEF

*Lyndon B. Johnson Space Center*



NASA Tech Briefs announce new technology derived from the U.S. space program. They are issued to encourage commercial application. Tech Briefs are available on a subscription basis from the National Technical Information Service, Springfield, Virginia 22151. Requests for individual copies or questions relating to the Tech Brief program may be directed to the Technology Utilization Office, NASA, Code KT, Washington, D. C. 20546.

## Oxygen Cocoon for Patients Under Intensive Care

### The problem:

A few medical centers in this country treat burn patients in a high oxygen environment at an increased atmospheric pressure. Special chambers are required for this purpose, along with special attendants. At the present time the attendants are exposed to the 100-percent oxygen environment and increased pressure as well as the patient. This environment is very hazardous from the standpoint of flammability and mildly toxic to the operator, if he is expected to care for several patients in a single day.


### The solution:

A relatively inexpensive cocoon is under development which would provide a more comfortable

environment for the patient, and a safer environment for the operator as well as the patient.

### How it's done:

The cocoon (see figure) is made from Teflon film. It is 8 feet (2.4 m) long and 2.5 feet (0.8 m) in diameter. It includes a full-length, pressure-sealing zipper on the top side. The bottom part is a 7-foot by 2-foot (2.1-m by 0.6-m) rigid pad constructed of burn-resistant material, to support the lying patient. On one end, the cocoon includes an oxygen supply port which is connected to an oxygen feeding apparatus. An exhaust port is on the other end. In addition, there are gloved access ports provided for attendants and the patient.

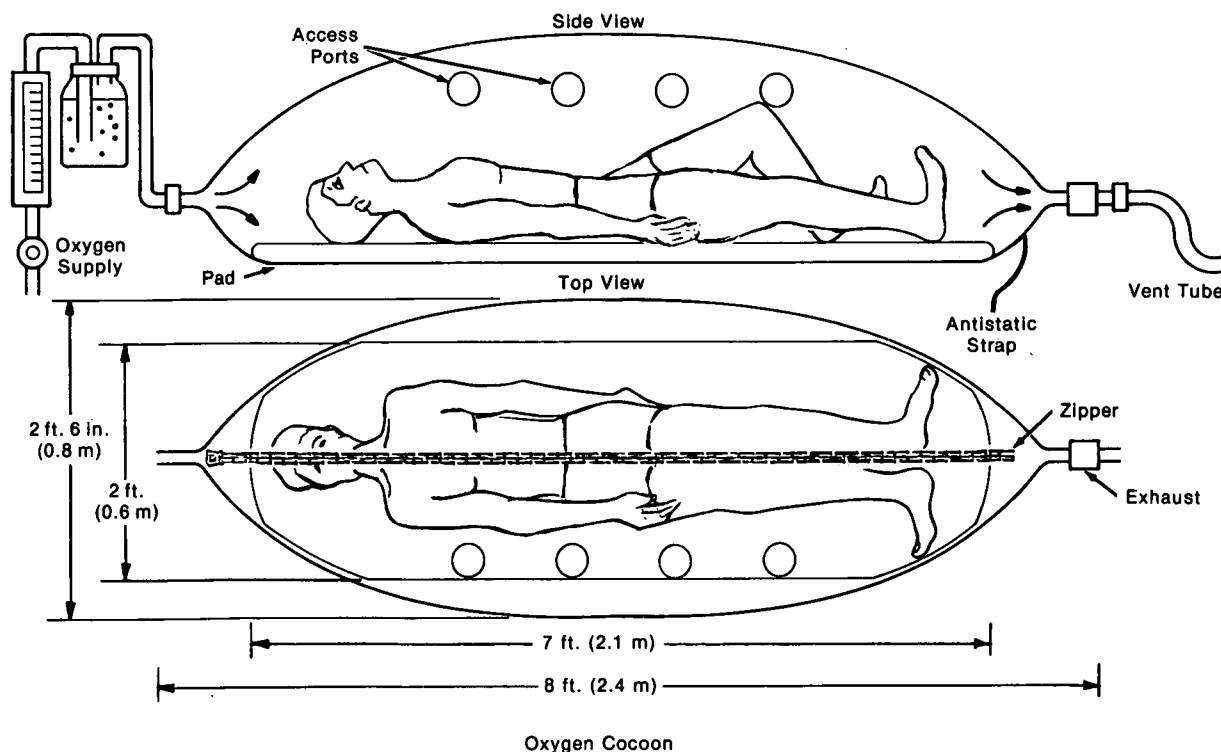

(continued overleaf)

The patient is placed on the cocoon pad with his head toward the oxygen supply port. The cocoon then is placed in a hyperbaric chamber which normally accepts several cocoons. When the chamber pressure reaches 2 atmospheres, the cocoon supply port is opened to admit oxygen. Oxygen flows from the head toward the patient's feet and out through the exhaust port. A number of patients in cocoons can be treated in this way simultaneously.

The cocoon has other uses as well. It can be supplied by filtered air to protect a patient who is highly susceptible to infection. It also can be used to isolate a patient with a serious contagious disease by filtering the air exhausted from the cocoon. Children and adults who cannot tolerate oxygen masks can also be placed in cocoons for more comfort. Oxygen can then be vented outside, greatly reducing the fire hazard in the room.

**Note:**

Requests for further information may be directed to:

Technology Utilization Officer  
Johnson Space Center  
Code AT3  
Houston, Texas 77058  
Reference: TSP75-10079

**Patent status:**

NASA has decided not to apply for a patent.

Source: J. W. Maas (U.S.A.F.)  
Johnson Space Center  
(MSC-12663)