


Psychomotor Vigilance Task Evaluation for Touchscreen Devices

Lucia Arsintescu



Background of PVT

- PVT-192 – widely used in laboratory studies
- Palm-PVT – 5-min widely used in field studies.
- Various PVTs developed for laptop use and hand-held mobile devices.



Background of PVT

PVT-192

- Bulky, used on laboratory
- Cannot be used by multiple subjects
- Subjects have to declare their handedness in advance
- LED display
- Running-timer stimulus
- Immediate feedback
- ISI – 2-10s following a rectangular distribution

Palm-PVT

- Small, easy to carry around – used in the field
- Can be used easily by multiple subjects (distinguished by study code and name)
- Handedness can be entered just before first session
- LCD display
- Black-and-white circular target
- Feedback is provided at the end of each session
- Uses N discrete foreperiods determined by a user-specified step size and then randomizes without replacement in blocks of $2N$.


Study goal

- To develop and validate a PVT for touchscreen devices that would have the same characteristics as PVT-192.



NASA - PVT

- It has the same features as PVT-192
 - ISI interval 2-10 sec, randomly (rectangular distribution)
 - Stimulus represented by a milliseconds-counter in a small rectangular box
 - Left and right areas predefined on the screen to serve as left or right buttons
 - Immediate feedback

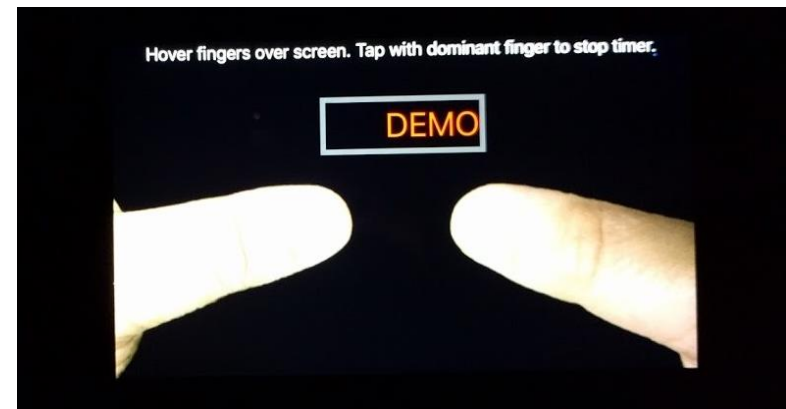


NASA-PVT

- Presence of FS or ERR on screen when participants react too fast to the stimulus or use the wrong finger to answer to the stimulus.
- The handedness can be entered at the beginning of the first session.
- It can be used by multiple subjects (change study code and id).



Study protocol/Participants

- 10 participants (5 males, 5 females) between 19 and 38 years of age (M = 25.1, SD = 6.17)

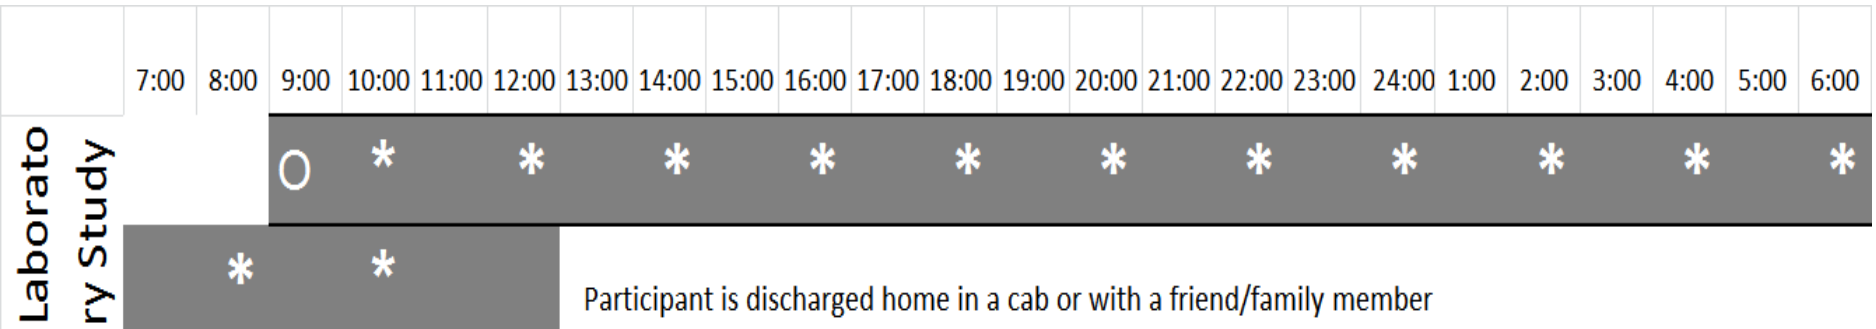


O = Orientation

* = 5-min PVT-192, 5-min Nasa-PVT


Touchscreen device latency

- Latency - the time between user action (touches the screen) and the system's response.



Touchscreen device latency

- Device latency = 77.42 (16.77).
- The mean device latency was subtracted from each PVT trial before analyzing the PVT data.

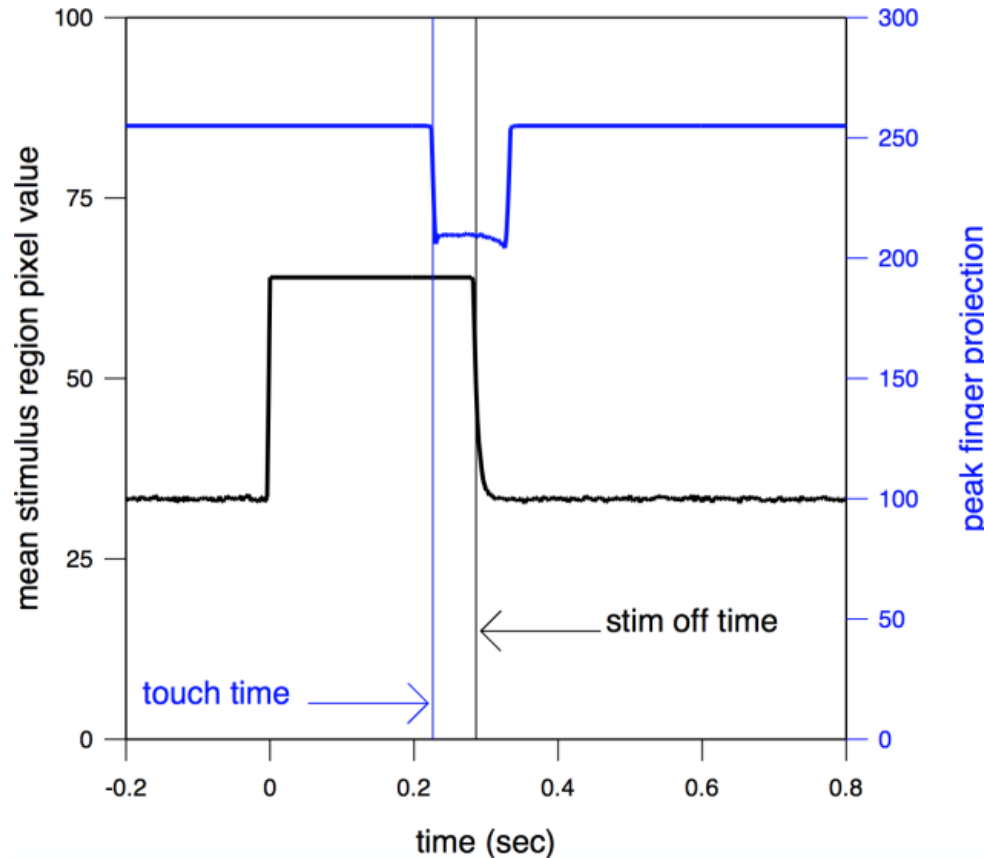


PVT outcome

- Mean $1/RT$ - reciprocal response time or response speed, measured in seconds.
- Lapses - the cumulative number of RTs exceeding 500 ms.
- Fastest 10%RT - the fastest 10% of response times for all trials. It indicates the best performance a participant is capable of producing.
- Slowest 10% $1/RT$ (cognitive slowing) - the slowest 10% of reciprocal response times for all trials. It indicates the vigilance response slowing.
- Mixed effects ANOVA with 2 two within subjects factors: Time and PVT type.


Mean 1/RT

- Main effect of time ($p < .001$) The mean 1/RT of both PVTs became worse over time.
- Significant linear decrease in performance over time for both PVTs.
- Main effect of PVT ($p = .001$). The mean 1/RT for the two PVTs were significantly different overall.




Lapses

- Main effect of time ($p < .001$). The mean lapses of both PVTs. increased significantly across time
- Significant linear increase in lapses over time for both PVTs.
- No main effects of PVT.




Slowest 10% of 1/RT

- Main effect of time ($p < .001$) The mean slowest 10% 1/RT of became significantly worse across time.
- Significant linear decrease in performance over time for both PVTs.
- Main effect of PVT ($p < .01$).

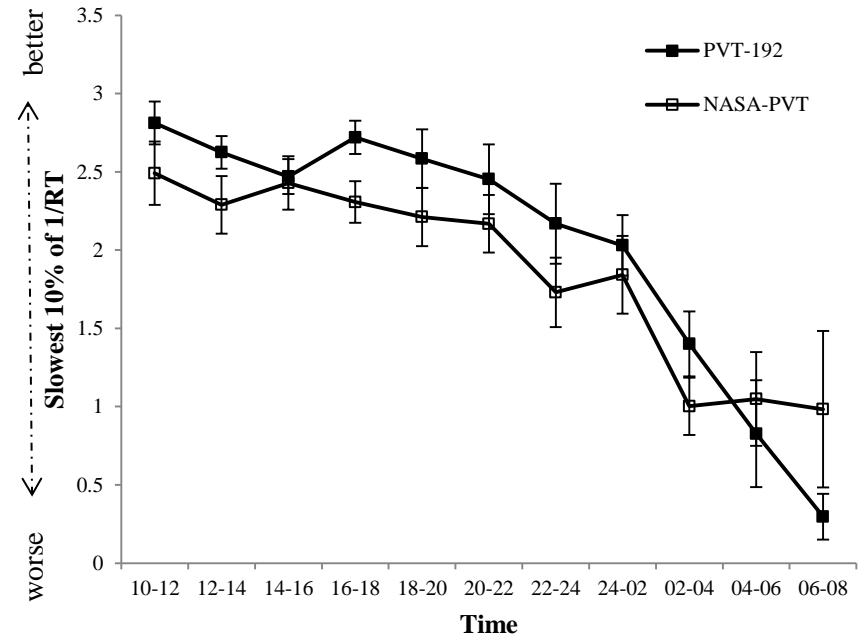


Fastest 10% RT

- Main effect of time ($p < .001$) The mean fastest 10% RT of both PVTs changed significantly across time.
- Significant linear increase over time for both PVTs.
- Main effect of PVT ($p < .05$).




Conclusions

- NASA-PVT follows the same shape and is similar on mean RTs and lapses after the latency cutoff was applied.
- Our results are limited to acute sleep deprivation.
- Future studies -
- Problems with touchscreen devices: latency, double touch, variability within and between subjects.



Problems with touchscreen devices

- Latency
- Double touch
- Variability of latency between trials in the same test for the same subject
- Variability of latency between subjects



Contributors

Success of this project would not have been possible without the assistance and hard work of the following people:

San Jose State University
Research Foundation

Nathan Feick
Patrick Cravalho
Zachary Caddick
Kevin Gregory
Lily Wong
Su Wei Heng

NASA Ames Research Center

Kenji H. Kato
Leland Stone
Erin E. Flynn-Evans