

Continuous sub-Kelvin cooling from an adiabatic demagnetization refrigerator

Mark O. Kimball¹, Peter. J. Shirron¹, Edgar R. Canavan¹, Bryan L. James¹, Michael A. Sampson¹, and Richard V. Letmate²

¹ NASA / Goddard Space Flight Center

² ATA Aerospace

Why the need for sub-Kelvin cooling in space flight?




- Astro-H / XRISM uses an array of 36 bolometers with absorbers tuned to soft-X-ray energies. They require 50 mK to reach stated sensitivity less than 7 eV



- PIPER uses two Backshort-Under-Grid (BUG) superconducting transition-edge sensors (TES) detectors developed at NASA/GSFC measure signal (> 5000 pixels). TES tuned to ~ 100 mK temperature range




- PIXIE (proposed) will use an array of infrared-sensitive bolometers to measure the polarization of the cosmic microwave background (CMB). Temperature requirement

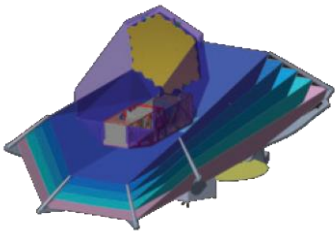


- Origins Space Telescope (proposed) contains three instruments that require sub-Kelvin cooling. All three use TES detectors operating at 50 mK. At this temperature, the sensitivity will be limited by the sky background.


Adiabatic Demagnetization Refrigeration

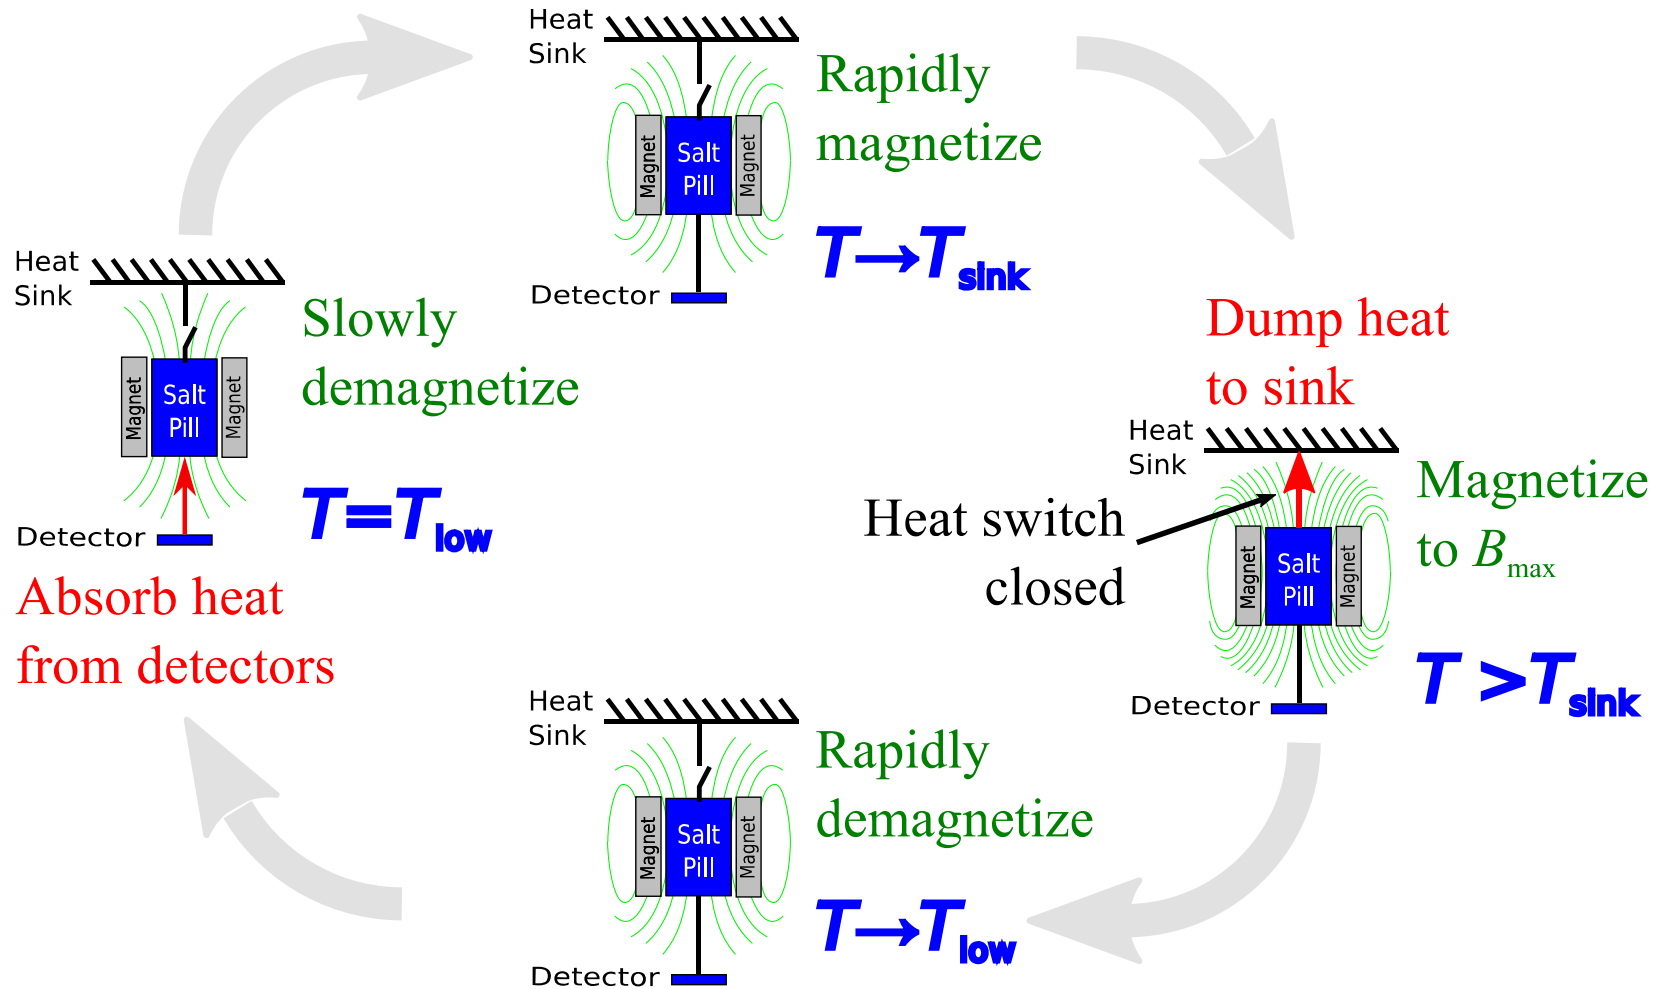

ADR Multi-Stage System

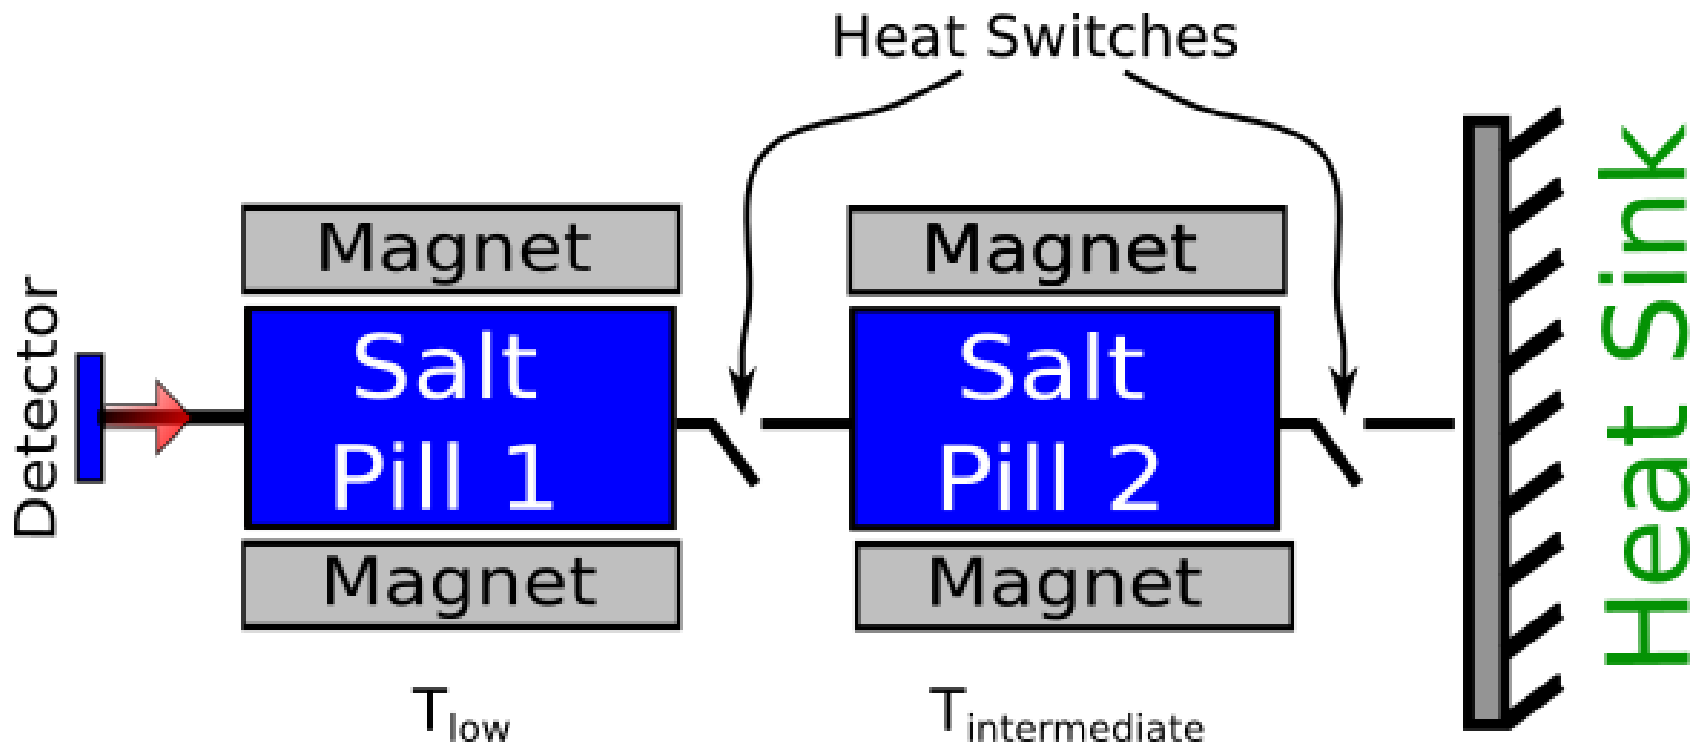

Continuous ADR

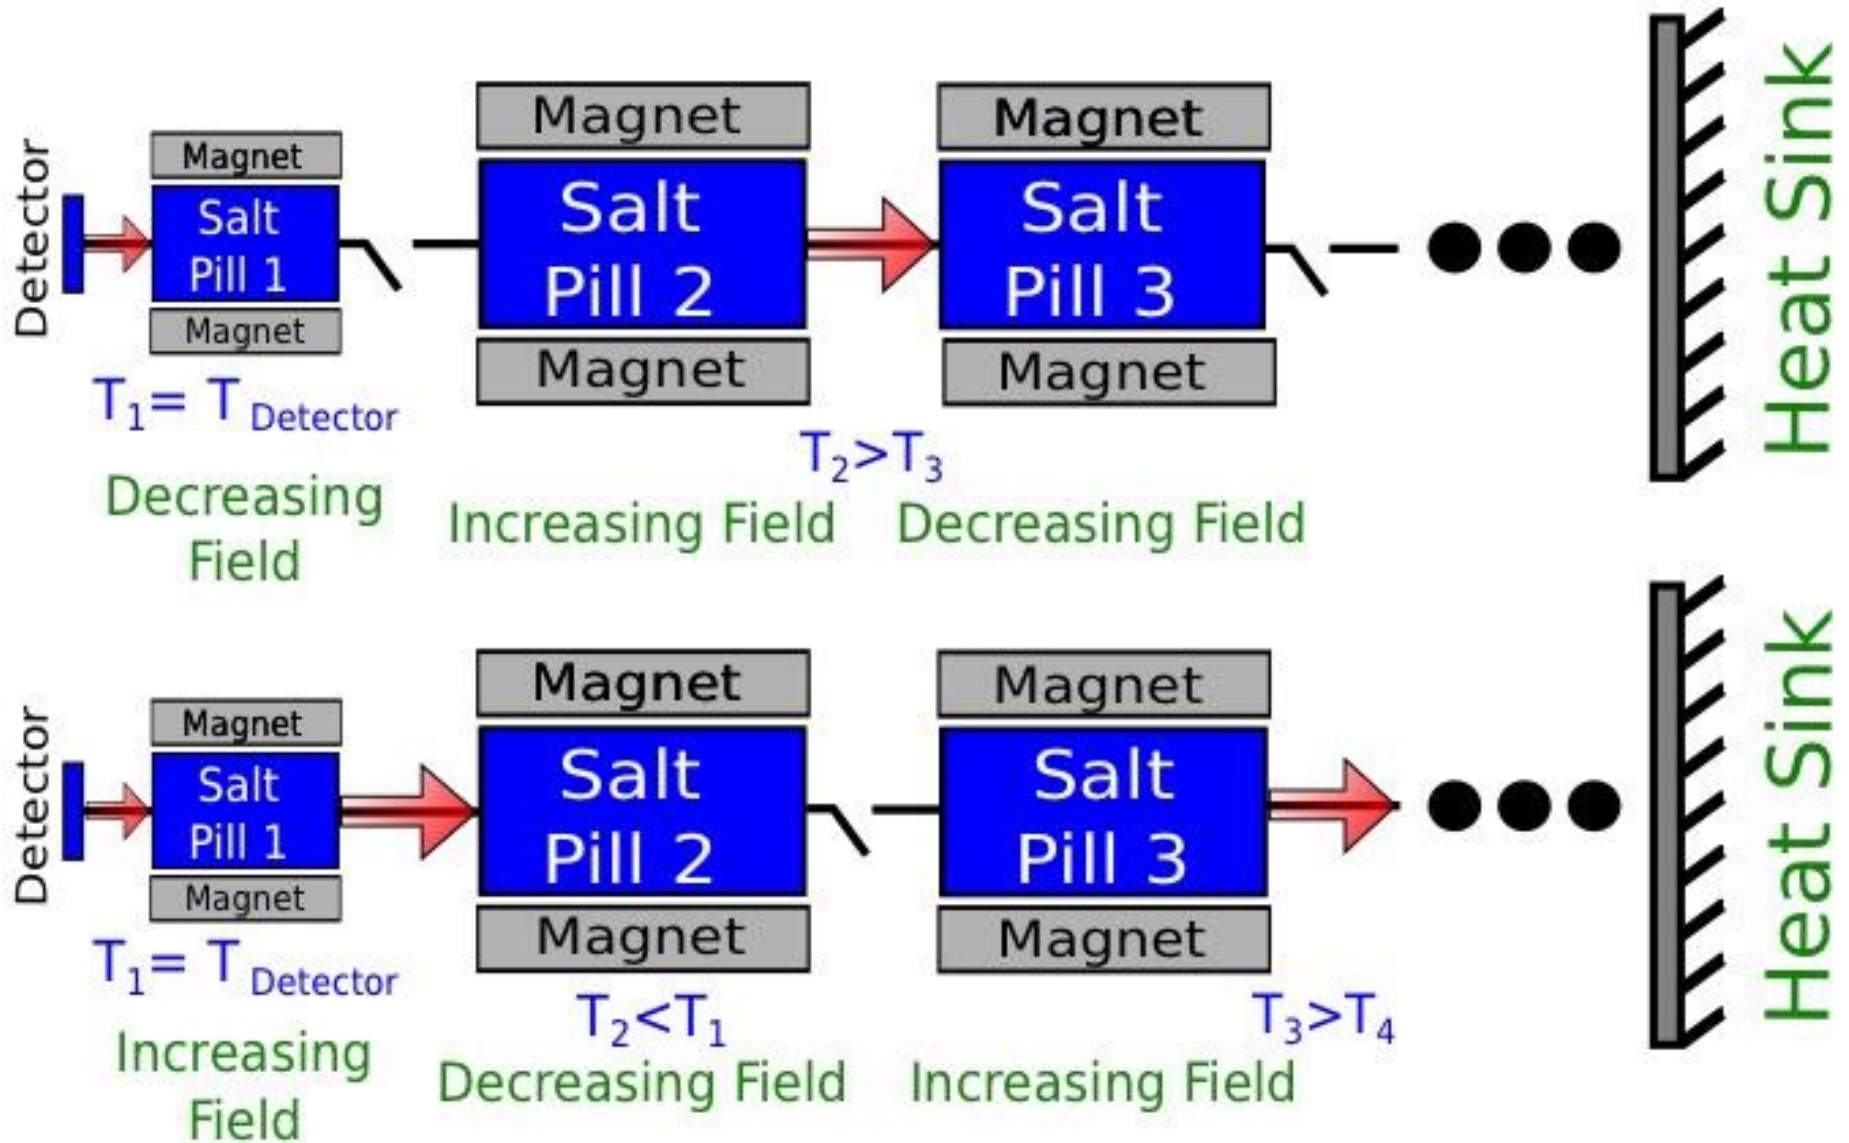

CADR built for External Mission



4 Stages

- ① 45 g CPA [0.100 K]
- ② 100 g CPA [0.375 -> 0.09 K]
- ③ 100 g CPA [1.4 -> 0.275 K]
- ④ 82 g GGG [4.2 -> 1.2 K]

Heat Switches

- ① Superconducting Switch (1 -> 2)
- ② Passive Gas-Gap (2 -> 3)
- ③ Passive Gas-Gap (3 -> 4)
- ④ Internal Passive Gas-Gap (4 -> H.S.)

CADR built for PIPER Mission



4 Stages

- ① 45 g CPA [0.100 K]
- ② 100 g CPA [0.375 -> 0.09 K]
- ③ 100 g CPA [1.4 -> 0.275 K]
- ④ 82 g GGG [3 -> 1.2 K]

Heat Switches

- ① Superconducting Switch (1 -> 2)
- ② Passive Gas-Gap (2 -> 3)
- ③ Passive Gas-Gap (3 -> 4)
- ④ Internal Passive Gas-Gap (4 -> H.S.)


Same CADR; Different Configurations

4 Stages

- ① 45 g CPA [0.100 K]
- ② 100 g CPA [0.375 -> 0.09 K]
- ③ 100 g CPA [1.4 -> 0.275 K]
- ④ 82 g GGG [3 -> 1.2 K]

Heat Switches

- ① Superconducting Switch (1 -> 2)
- ② Passive Gas-Gap (2 -> 3)
- ③ Passive Gas-Gap (3 -> 4)
- ④ Internal Passive Gas-Gap (4 -> H.S.)

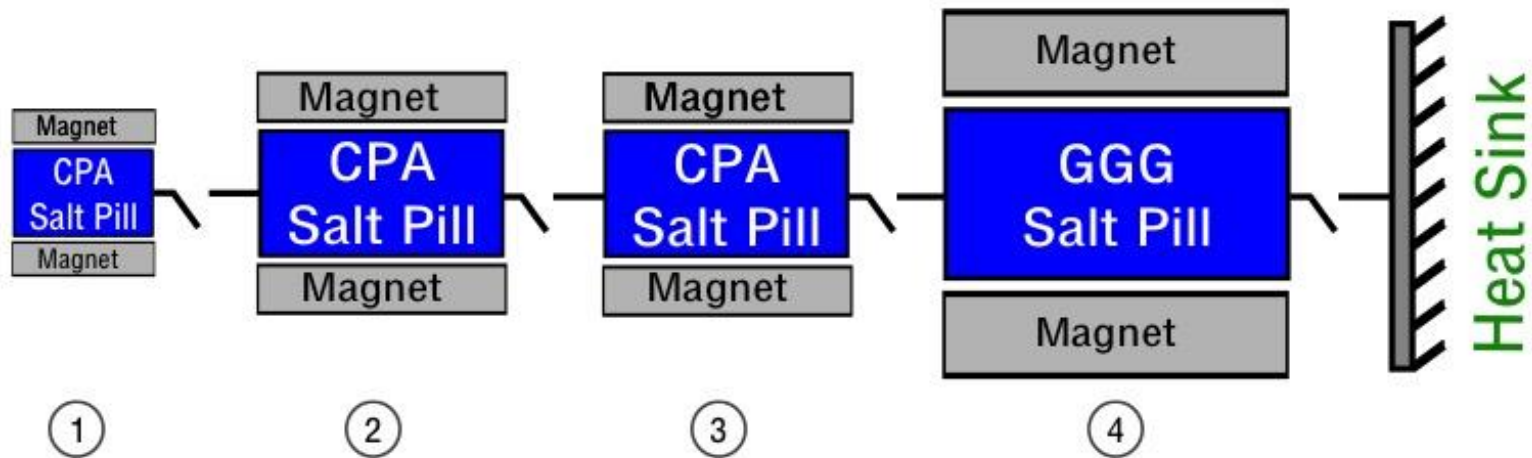



Passive Gas-Gap Heat Switches



- Passively closes when temperature of associated stage warms above some value
 - More thermodynamically efficient since no additional heat added to system to activate
- Thin (0.127 mm) titanium outer shell
- Gold-plated copper innards consist of interleaved fins with a 0.36 mm gap between when assembled
- Getter typically sintered stainless pucks or the copper fins themselves




Stage 4 Passive GGHS Internal to Stage

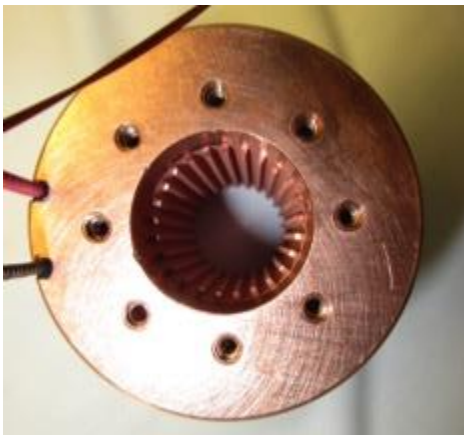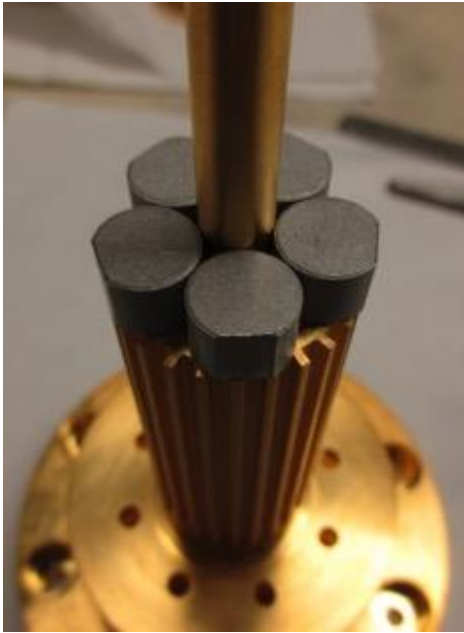


- One set of “fins” is the salt pill
- Other set the magnet itself
 - ~ 0.4 mm gap between adjacent pair of fins
- Sintered 300 CRES getters epoxied onto the pill provide attractive surface for He-3
 - If ^3He between sets of fins, switch on
 - When ^3He to CRES binding energy greater than some temperature, switch turns off
- Room-temperature fill level sets the transition temperature
 - 4 torr fill provides transition ~ 1.2 K



Superconducting Heat Switch

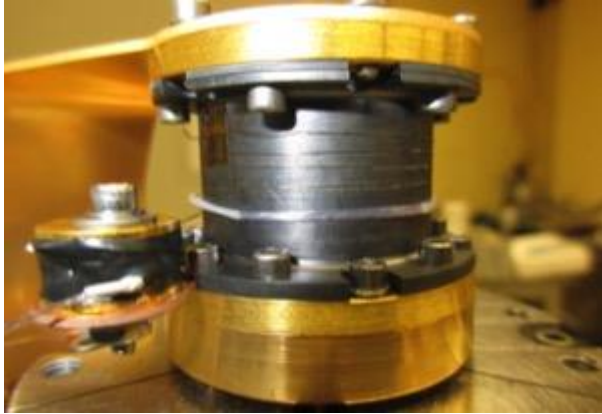

- Positioned between stages 1 and 2
- Two halves of switch separated by a length of lead wire
 - When lead in superconducting state, switch open
 - When lead in normal state, switch closed
 - Magnetic field from Helmholtz coil switches state
- Quick switching time
- Works in a temperature regime where gas in a GGHS is absorbed fully

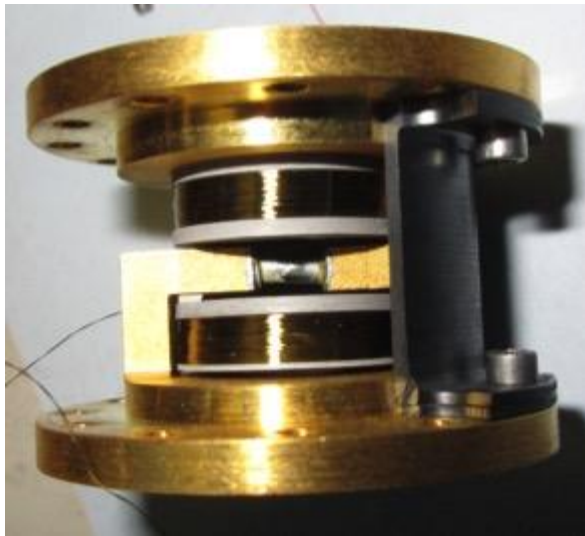


S2,3 Salt Pill Suspensions

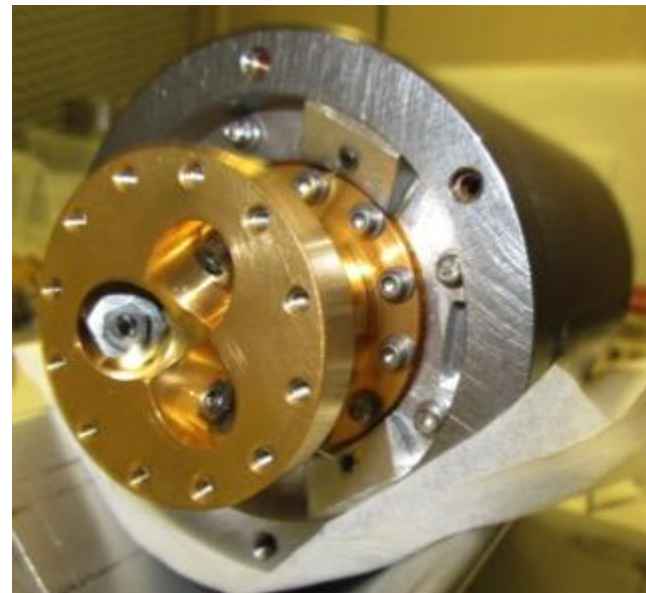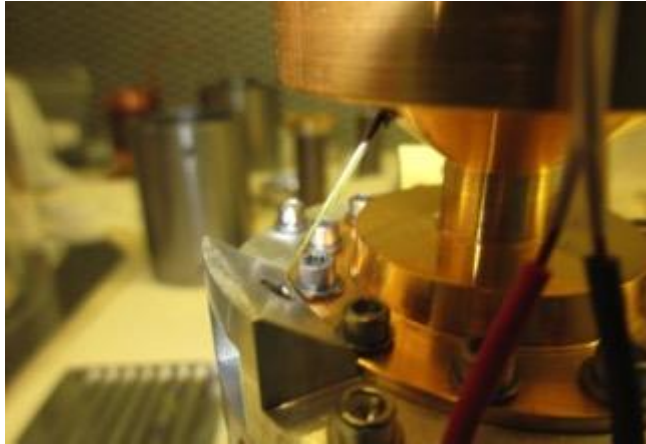

A total of 6 Kevlar bundles suspend the paramagnetic salt pill within the bore of a superconducting magnet


- Magnet temperature: 3 K
- Pill temperatures often below 1 K
- Kevlar assemblies made on the bench then installed
 - Button head screw on outside attachment point
 - “D-shaped” screw threaded through inner attachment point
 - Tensioned via a nut and locked with a second nut
- Estimated heat lead from 3 to 0.1 K: 4.4 μW

S4 Salt Pill Suspension




- 300 CRES bellows isolates one end
- Thin Vespel SP1 spool provides structural support
- Six Kevlar bundles suspend other end


Plots of Temperatures and Currents

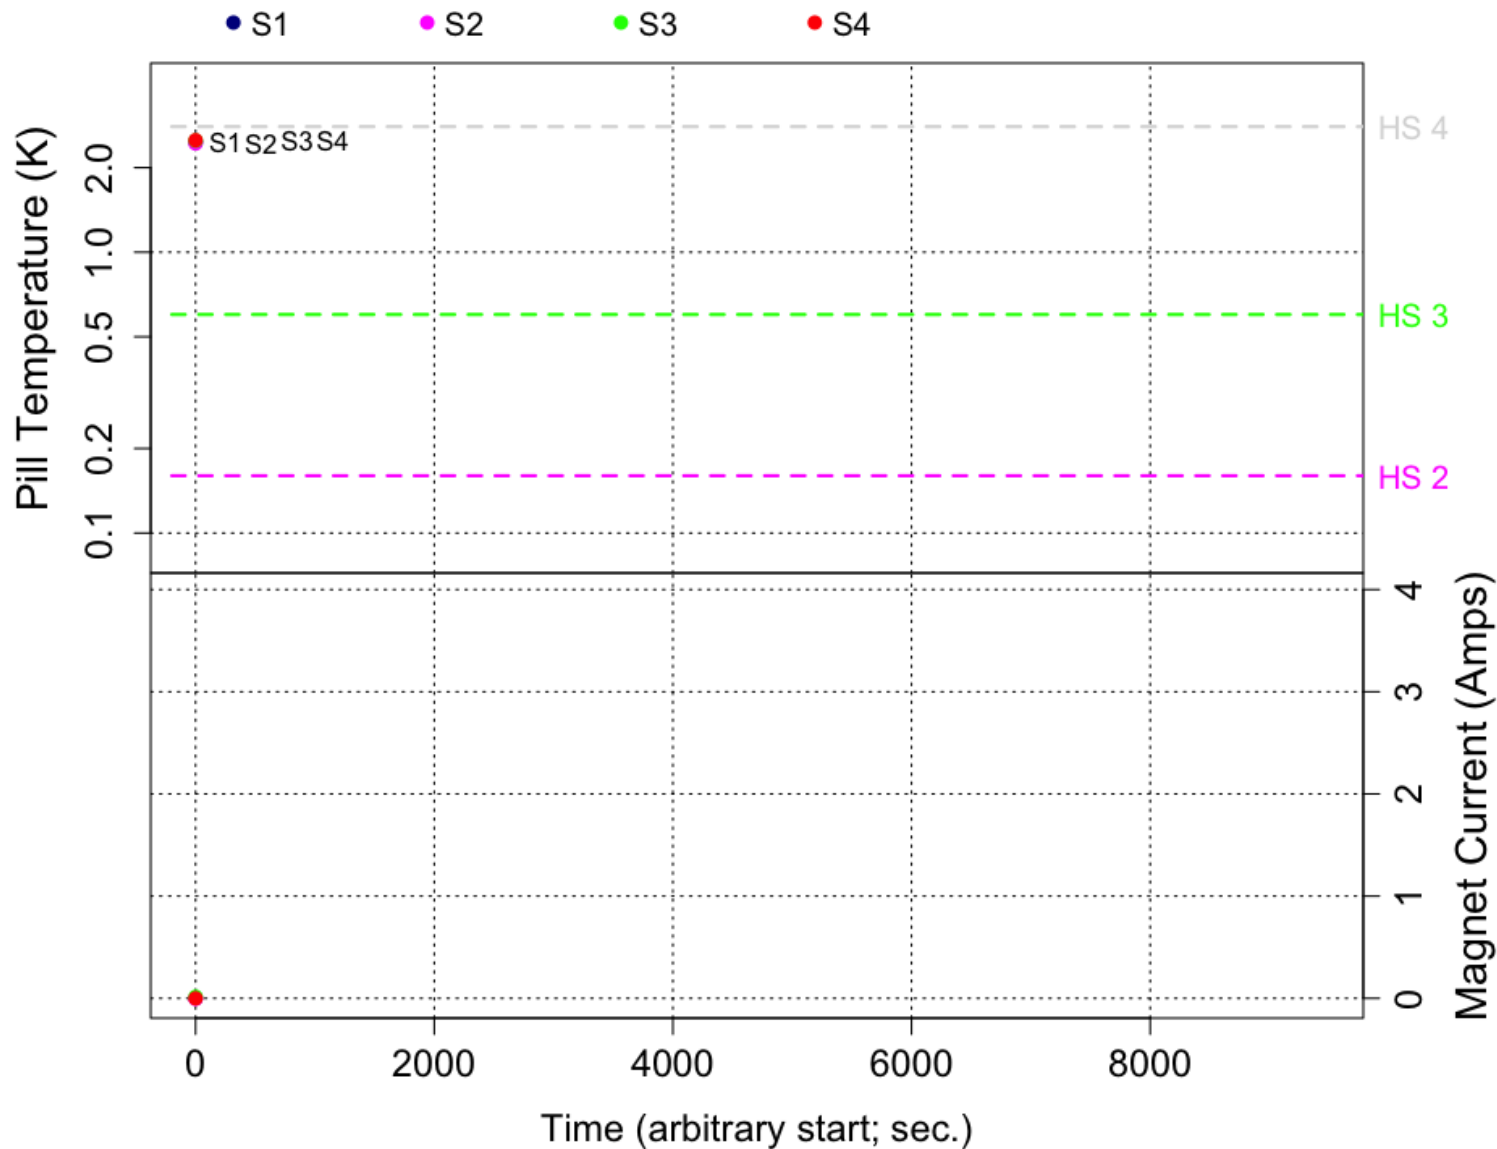

Plots of Temperatures and Currents

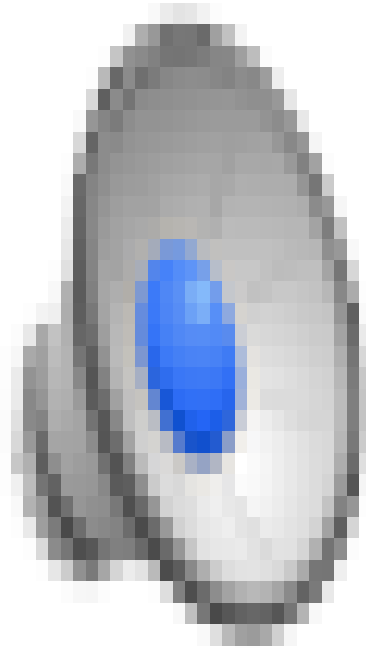

Heat Lift etc.

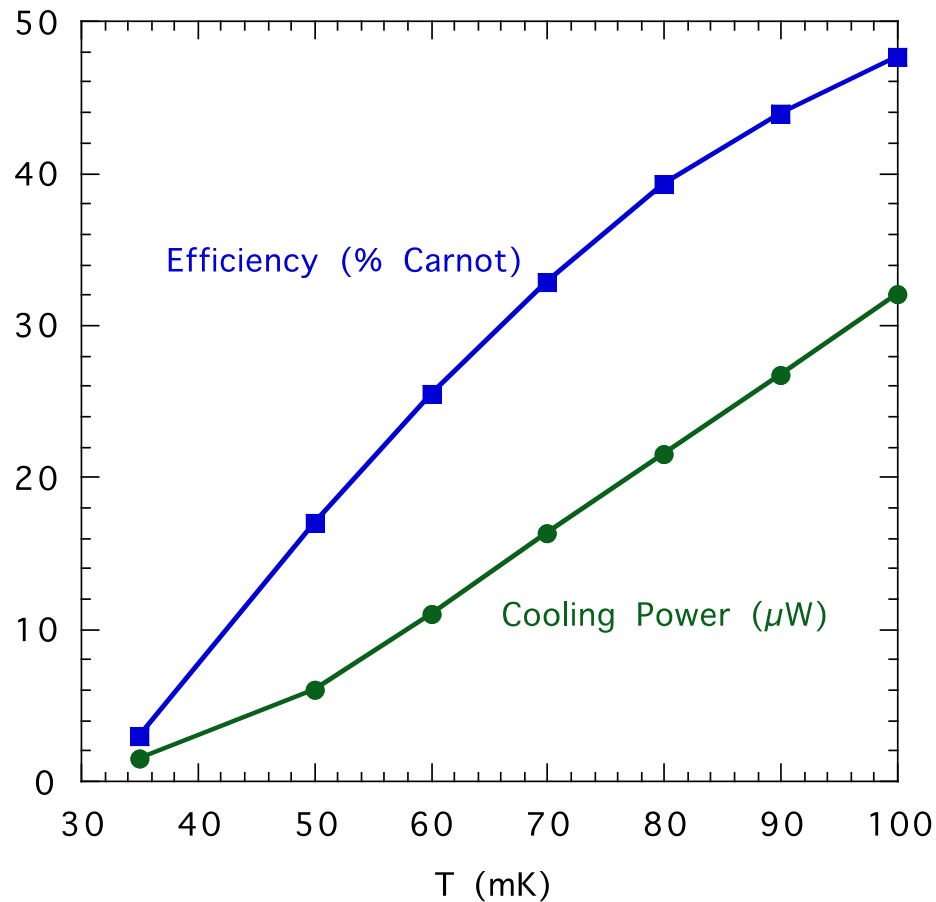


* Cooling power in addition to parasitic heat loads

CADR was developed using research money provided by NASA/GSFC in the early 2000's (Shirron *et al.*)

- Measured cooling powers and overall efficiency measured for that system
- Taking data on new system now and will compare the two systems
 - Expect new system to have a lower available cooling power due to stronger Kevlar suspensions

Many Possibilities

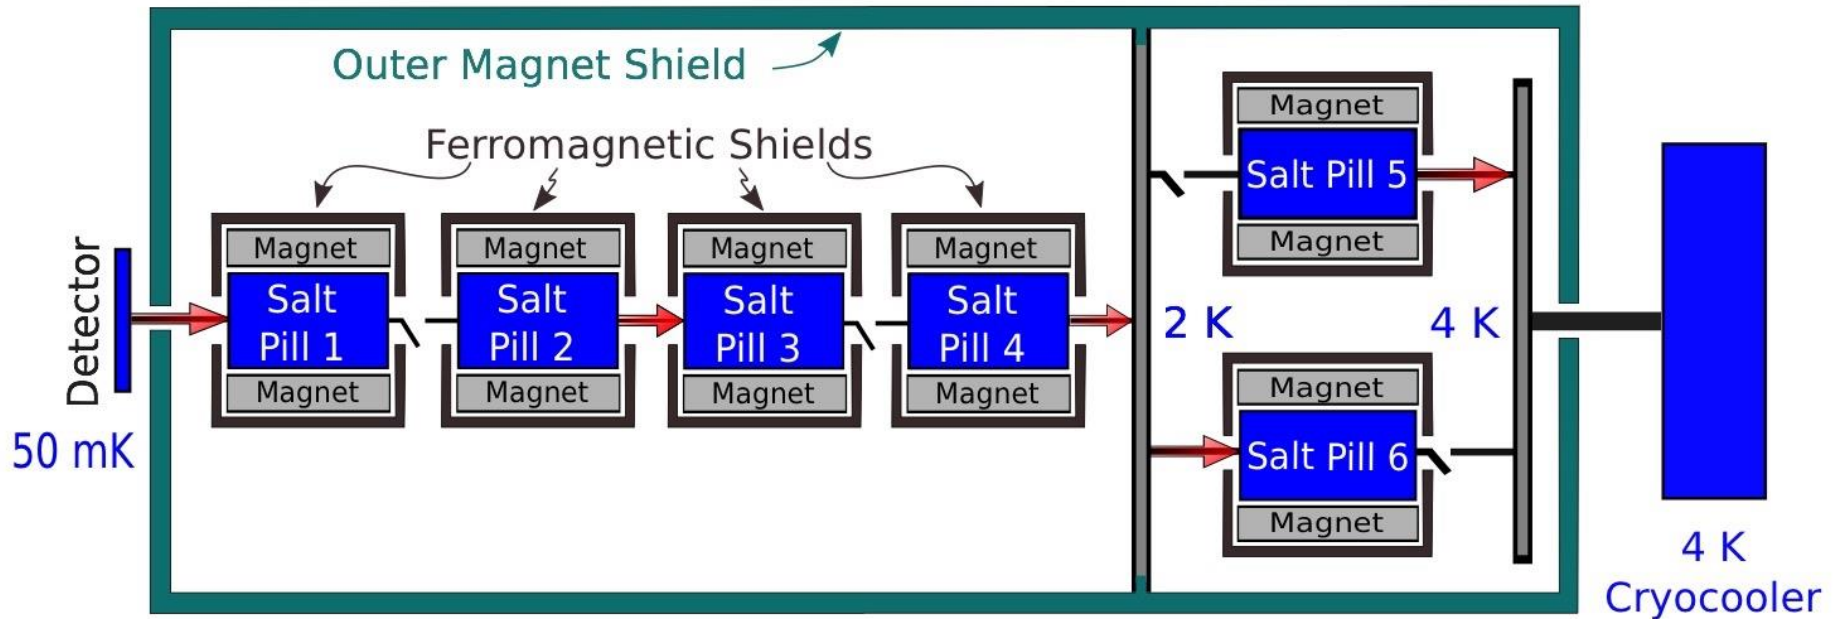

Two, or more, unique continuous temperatures possible

- Asynchronous CADR
- In this example, one is a 2 K, the other 0.050 K

Summary

- Both 4-stage continuous ADRs built for the PIPER balloon mission and our external partner have completed testing
- One cooler demonstrated continuous operation below 45 mK with a total heat lift of $> 5 \mu\text{W}$ at that temperature
 - Includes parasitic heat to coldest stage two stages
 - Usable cooling power decreased by testing environment (vibrational heating from cooler in one case)
 - Need to modify environment by either dampening cooler or moving to flight Dewar cooled via liquid helium
- Second cooler modified to work from a 4.2 K liquid helium bath
 - Demonstrated greater than $6 \mu\text{W}$ heat lift in addition to parasitic heating while at 80 mK
- Since the CADR has a higher cooling power for the same mass as a single-shot system, we are now baselining this technology will be baselined for future missions