

EFFECT OF ORGANOTIN SPECIES ON THE EMISSION SIGNAL IN ICP-AES

Javier Montiel, Luis Gras and Juan Mora

Department of Analytical Chemistry, Nutrition and Bromatology

University of Alicante, P.O. Box 99, 03080 Alicante (Spain)

javier.montiel@ua.es



INTRODUCTION

It is generally accepted that the analytical response in ICP-AES is not influenced by the chemical form of the analyte. Nevertheless, differences between signals of organometallic and inorganic compounds of the same analyte have been reported [1,2]. Thus, it has been proved that inorganic tin solutions provide higher emission signals than organotin ones. Moreover, this behaviour has been observed operating with different spray chambers and experimental conditions[3].

The aim of this work is to evaluate the analyte chemical form on the emission signal in ICP-AES. To this end, different tin solutions have been analysed using a pneumatic concentric nebulizer coupled to a cyclonic spray chamber. The effect of the liquid and gas flow rates on the aerosol drop size distribution, solution transport rate and emission signal in ICP-AES have been studied.

REFERENCES:

- (1) L.C. Alves, M.G. Minnich, D.R. Wiederin, R.S. Houk, J. Anal. At. Spectrom., 9, 399 (1994).
- (2) C. Rivas, L. Ebden, S.J. Hill, J. Anal. Spectrom., 11, 1147 (1996).
- (3) J. Montiel, J. Mora, Influence of the analyte chemical form and the sample introduction system on the analysis of organotin compounds by ICP-AES, Euroanalysis XIII, Salamanca, 2004.

EXPERIMENTAL

➤ 10 ppm Sn in EtOH 0.75% from: SnCl_4 ; $^n\text{BuSnCl}_3$ (MBT); $^n\text{Bu}_2\text{SnCl}_2$ (DBT); $^n\text{Bu}_2\text{SnCl}_2$ (DTBT)

➤ Sample introduction system:



➤ ICP-AES operating conditions:

PERKIN ELMER OPTIMA 4300 DV

RF Power (W)	1300
Plasma gas flow rate (L/min)	15
Auxiliar gas flow rate (L/min)	0,2
Nebulizer gas flow rate, Q_g (L/min)	0,6
Liquid flow rate , Q_l , (mL/min)	0,2 - 1,0
i.d. injector (mm)	1,2
Sample and integration time (s)	Automatic
Torch position (mm)	15
Vision view	axial

RESULTS

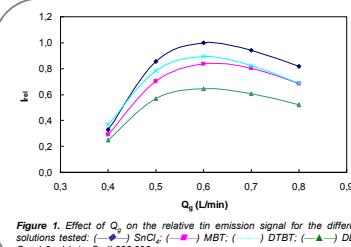


Figure 1. Effect of Q_l on the relative tin emission signal for the different solutions tested: (—●—) SnCl_4 ; (—●—) MBT; (—○—) DTB; (—▲—) DBT. $Q_g = 1.0 \text{ mL/min}$. Sn II 283.998 nm


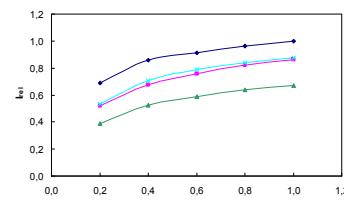


Figure 2. Effect of Q_l on the relative tin emission signal for the different solutions tested: (—●—) SnCl_4 ; (—●—) MBT; (—○—) DTB; (—▲—) DBT. $Q_g = 0.6 \text{ mL/min}$. Sn II 283.998 nm

$$I_{\text{SnCl}_4} > I_{\text{DTBT}} \approx I_{\text{MBT}} > I_{\text{DBT}}$$

EMISSION SIGNAL DEPENDS ON THE TIN COMPOUND

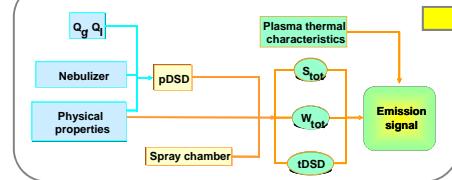

- There is no effect of analyte chemical form on:
 - × Primary droplet size distribution (pDSD) (1)
 - × Tertiary droplet size distribution (tDSD) (2)
 - × Solvent transport rate (3)
 - × Plasma characteristics (4)
- For a given Q_l , the analyte transport rate, W_{tot} , is independent on the analyte and the solution employed.

Q_l (mL/min)	Analyte	Blank*	SnCl_4	MBT	DBT	DTBT
0,2	Mg	0.50 ± 0.06	0.57 ± 0.02	0.59 ± 0.05	0.53 ± 0.06	0.56 ± 0.06
0,2	Mn	0.52 ± 0.07	0.54 ± 0.03	0.54 ± 0.05	0.48 ± 0.05	0.52 ± 0.05
1,0	Mg	1.62 ± 0.11	1.67 ± 0.13	1.66 ± 0.11	1.74 ± 0.02	1.9 ± 0.2
1,0	Mn	1.74 ± 0.12	1.63 ± 0.09	1.67 ± 0.05	1.77 ± 0.04	1.8 ± 0.3

* Ethanolic matrix without Sn




Figure 3. Primary droplet size distributions for the different solutions tested: (—●—) SnCl_4 ; (—●—) MBT; (—○—) DTB; (—▲—) DBT; ($Q_g = 0.6 \text{ mL/min}$, $Q_l = 1.0 \text{ mL/min}$)




Figure 4. Tertiary droplet size distributions for the different solutions tested: (—●—) SnCl_4 ; (—●—) MBT; (—○—) DTB; (—▲—) DBT; ($Q_g = 0.6 \text{ mL/min}$, $Q_l = 1.0 \text{ mL/min}$)




Figure 5. Effect of Q_l on the relative carbon emission signal for the different solutions tested: (—●—) SnCl_4 ; (—●—) MBT; (—○—) DTB; (—▲—) DBT; ($Q_g = 0.6 \text{ mL/min}$, $Q_l = 1.0 \text{ mL/min}$)




Figure 6. Effect of Q_l on the magnesium ratio MgII/MgI for the different solutions tested: (—●—) SnCl_4 ; (—●—) MBT; (—○—) DTB; (—▲—) DBT; ($Q_g = 0.6 \text{ mL/min}$)

COMPOUND VOLATILITY




Figure 7. Analyte mass distribution of the primary aerosol (including a hypothetic value of the cut diameter of the spray chamber, d_c)

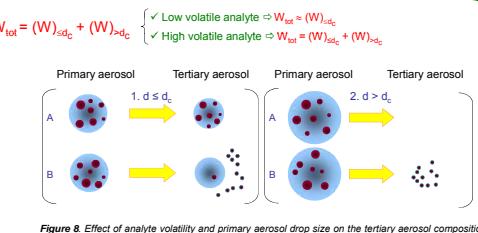


Figure 8. Effect of analyte volatility and primary aerosol drop size on the tertiary aerosol composition.
1. Analyte initially contained in drops with diameter equal or less to d_c .
2. Analyte initially contained in drops with diameters higher than d_c : A: Low volatile analyte; B: High volatile analyte.

Compound	Boiling Point (°C)
MgCl_2	1410
MnCl_2	2160
SnCl_4	110
DTB*	210
MBT*	240
DBT*	300

* Estimated values (T-H-E rule).

$$(W_{\text{tot}})_{\text{SnCl}_4} > (W_{\text{tot}})_{\text{DTBT}} = (W_{\text{tot}})_{\text{MBT}} > (W_{\text{tot}})_{\text{DBT}}$$

$$I_{\text{SnCl}_4} > I_{\text{DTBT}} \approx I_{\text{MBT}} > I_{\text{DBT}}$$

THE HIGHER COMPOUND VOLATILITY THE HIGHER EMISSION SIGNAL IN ICP-AES