

# SI-Traceable Calibration of Satellite Microwave Radiometers

Edward Kim NASA/GSFC

Derek Houtz, Dazhen Gu, William Emery  
US National Institute of Standards and Technology  
University of Colorado, Boulder  
WSL (ETH)

Ville Kangas, ESA/ESTEC, Metop-SG  
Takaaki Ishikawa, Mitsubishi Electric Corporation  
William Bell, ECMWF

Acknowledgements: David Walker, NIST retired

# Outline

## Background (what)

- SI-traceable Microwave Radiometer calibration

## Motivation (why)

- NWP, FCDR

## Technology (how)

- NIST blackbody target

## Standards

## Status & Future Plans

## CAVEAT

- Ongoing work !!
- “The answer” not completely known

# Satellite MW Radiometer Cal Example

Example: ATMS



On-board Blackbody target

Cosmic MW Background


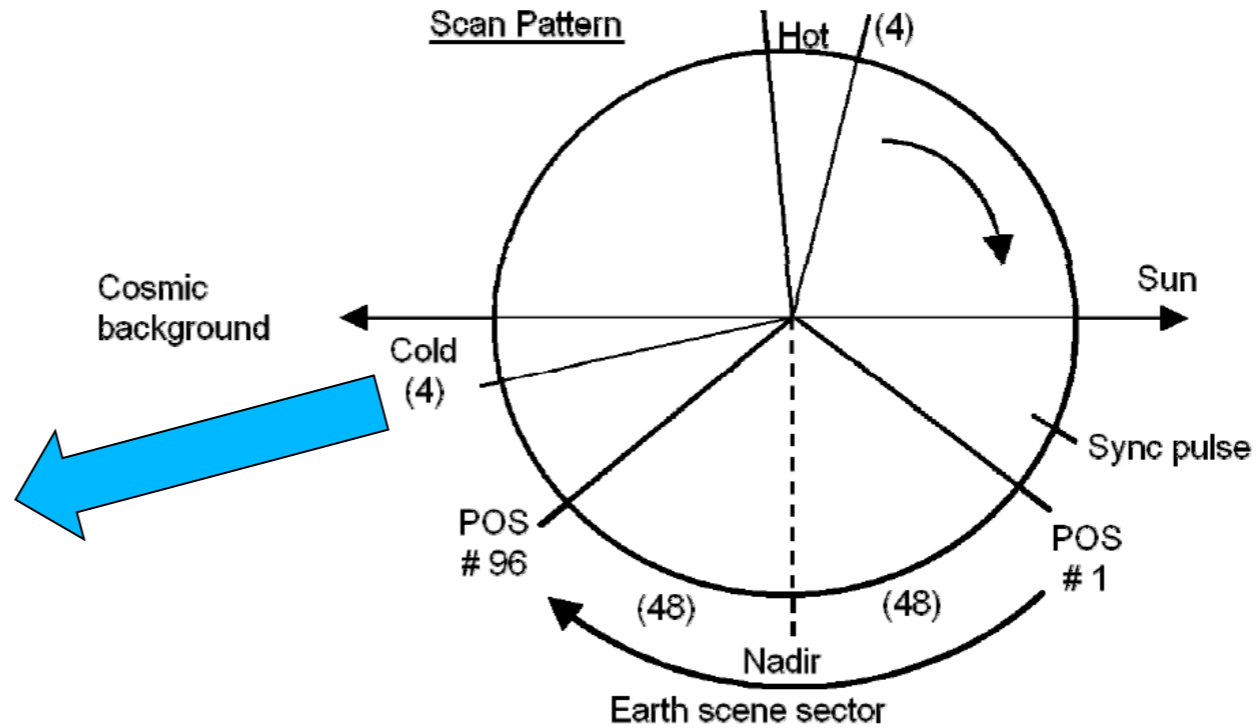


Figure 6. Scan sequence (flight direction is toward the reader)


# Typical MW Radiometer TB Calibration

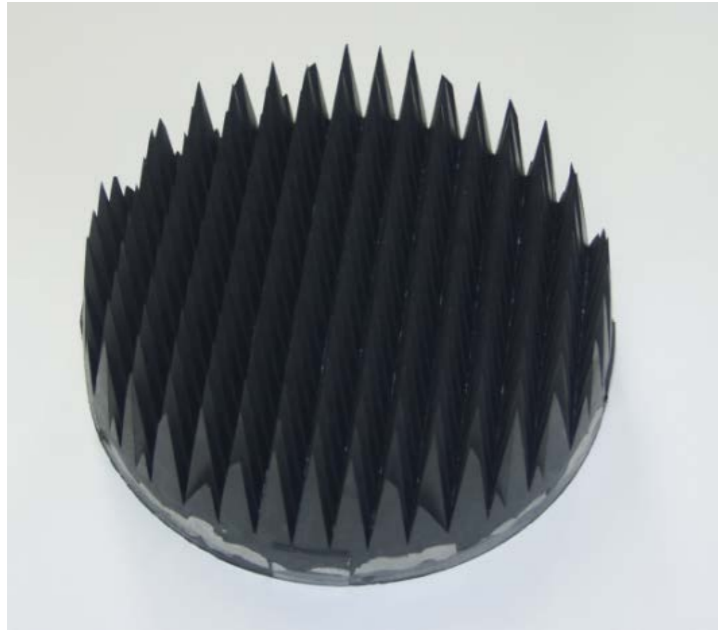

Typical black body used to calibrate satellite MW radiometers: 2D array of pyramids

(highly simplified version)

- Build your radiometer as linear as practical
- Point it at 2 calibration targets (1 hot, 1 cold) to determine the cal curve (a line)
- Cal targets are typically black bodies with emissivity  $\sim 1$ , so TB = physical temperature

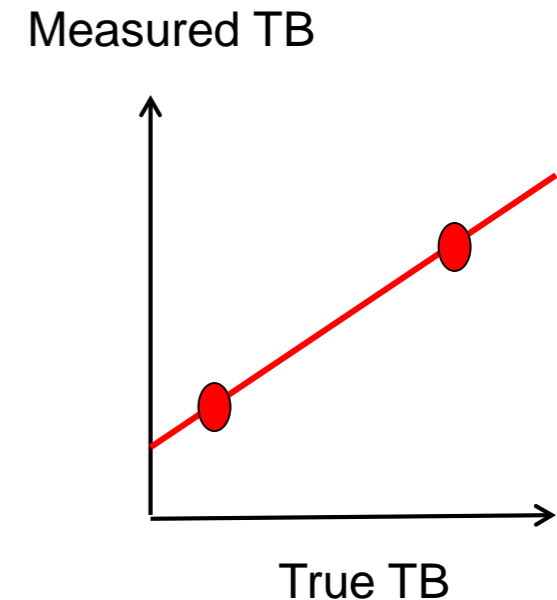

# What “SI traceable” **is not**

- Traceability implies a rigorous uncertainty assessment—**true**
- Using an SI unit as the standard provides a well-defined reference —**true**
- Your measurement will have unusually good accuracy—**not necessarily**
- In other words, just because you know the size of your error bars very well, doesn't guarantee that the error bars are small

# SI-traceable *inter-calibration* of Satellite MW Radiometers

- My *personal* forecast (so not NOAA or NASA policy): future sounder obs will need to combine smallsats + anchor sounders like ATMS, MWS
- Example: GPM constellation—"X-cal" effort has harmonized TBs with respect to one member radiometer (GMI)
- According to NIST, this is inter-comparison, not inter-calibration because the reference (GMI) isn't traceable to a standard
- Adding traceability to a standard would make it inter-calibration
- Traceability to a SI standard would be SI-traceable intercalibration
- Traceability to a standard implies absolute calibration
- Traceability to which SI unit?

GSICS Annual Meeting, Kim et al

# GNSS-RO and Tb Standards

- GNSS-RO is SI-traceable through frequency standards.
  - Connected to atmospheric Temperature & Humidity via density & refraction modeling
  - Relies on 1-2 GHz signals chosen for low sensitivity to atmosphere
  - Spatial coverage: best altitude range 8-25 km, 300 km horizontal resolution, ~1 km height resolution
  - **Creates reliable long-term RO data record**
- MW Radiometry can be SI-traceable with T<sub>B</sub> standards.
  - More direct connection to atmospheric Temperature & Humidity via radiative transfer
  - Relies on 18-183 GHz bands chosen for high sensitivity to atmospheric temperature & humidity
  - Finer horizontal resolution, similar vertical resolution, wider altitude range
  - **Creates reliable long-term T<sub>B</sub> data records**
- **Comparable uncertainties achievable: 0.1--1 K (single retrieval)**
- **Strengths & limitations are complementary**

GSICS Annual Meeting, Kim et al


# Motivation

- Inter-calibration for constellation systems
- Absolute TB calibration
- Benefits to NWP and FCDRs
- What is not addressed by SI-traceable TB cal?



# Benefit to Constellation Systems

- Constellation systems need TB inter-calibration
- Example: anchor sounders + smallsat sounders
- Pre-launch inter-calibration can reduce burden on post-launch inter-cal
- Still want post-launch inter-cal to handle issues like footprint matching, but the portion due to just TB inter-cal would be well-quantified by SI-traceable TB calibration
- Post-launch traceable inter-cal also appears possible, which would extend traceability to on-orbit
- Pre- or post-launch inter-cal would provide immunity to temporal gaps

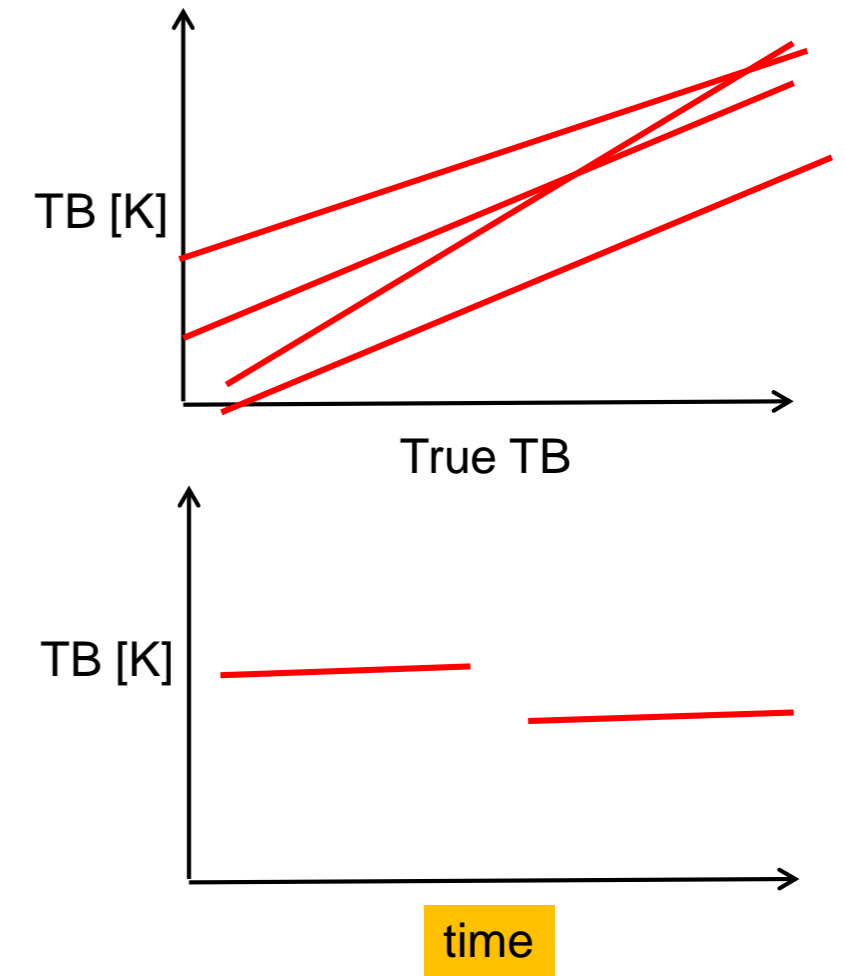


GSICS Annual Meeting, Kim et al

# Benefit to NWP forecasting

- NWP & climate models subtract biases
- Bias sources include:
  - 1) Radiometer sensor
  - 2) Radiative transfer model (RTM)
  - 3) Forecast model
- Bias corrections are larger than forecast model errors
- Bias from RTM & forecast models (#2 & #3) are often artificially assigned to sensor bias (#1) in order not to disturb the models
- This is unphysical
- Impedes progress in actually fixing the models (thus presumably improving forecasts)

# The potential benefits of improved radiometric calibration for NWP and climate reanalysis

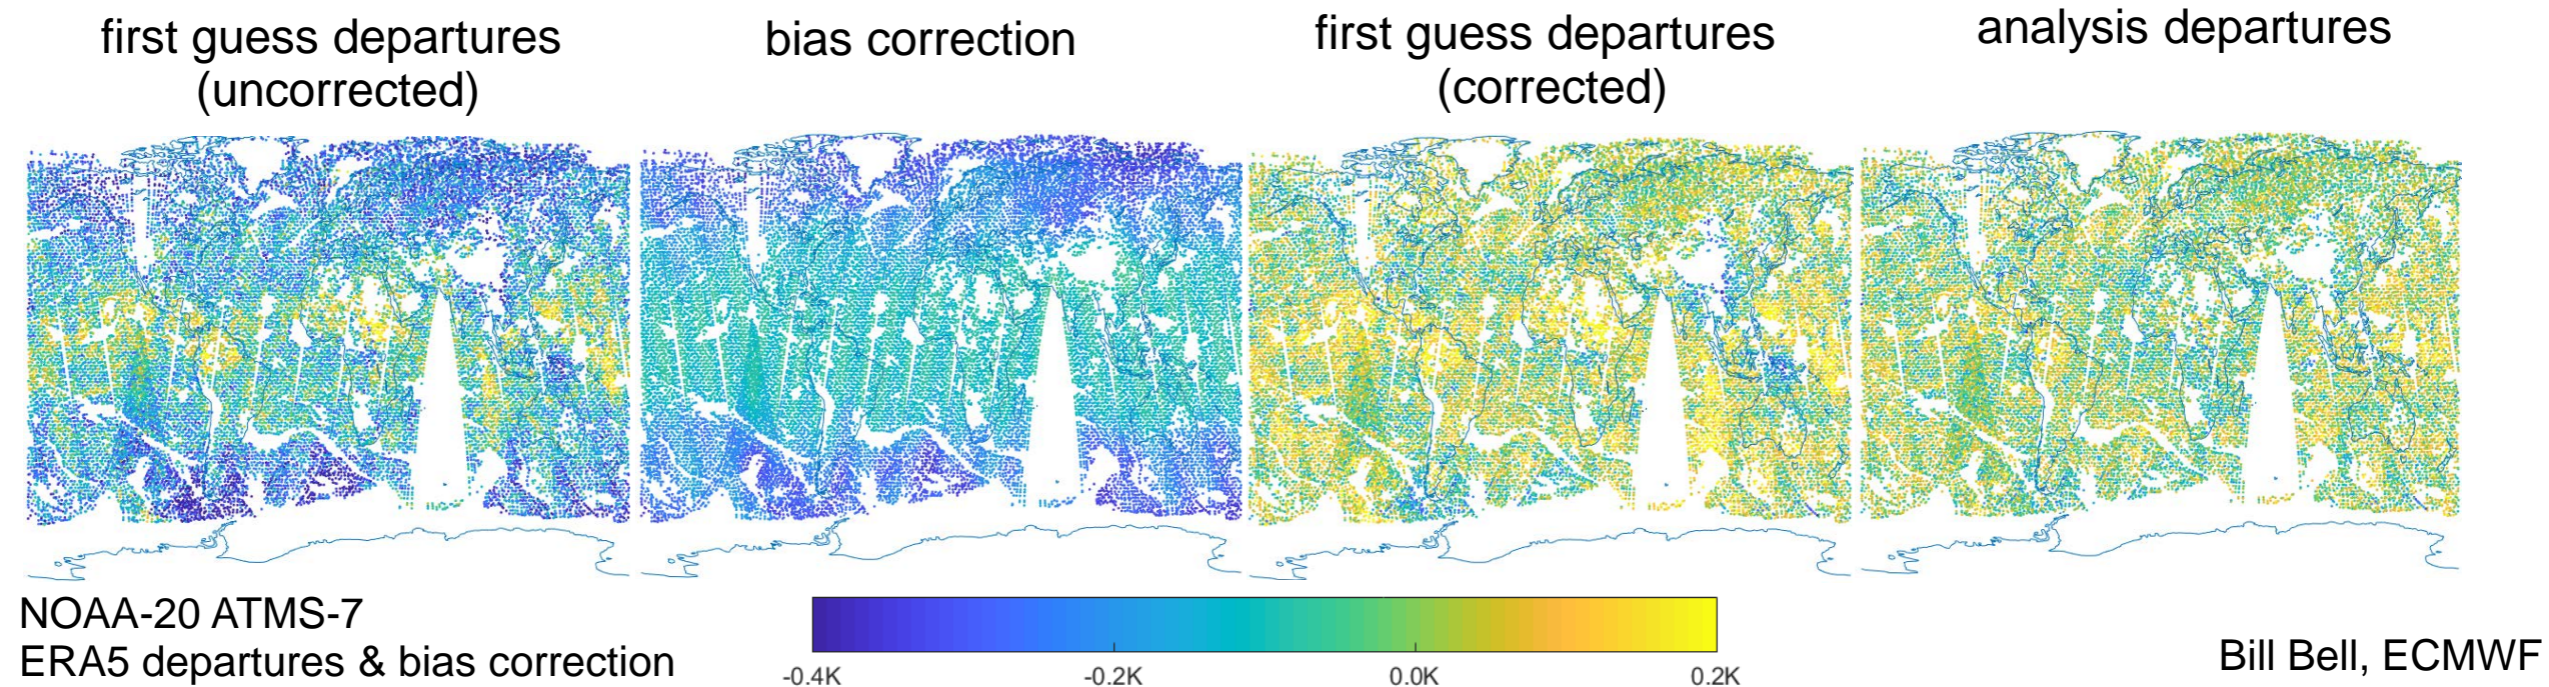


- Forecast model errors are  $\sim 0.1\text{K}$  for mid-trop. T- sounding channels
- Bias corrections (parametrised, accounting for radiometric & spectral biases, RT & forecast model biases) are larger
- Improved, traceable, absolute radiometric calibration would help:
  - Partition & bound the contribution due to radiometric uncertainties
  - Reduce the magnitude of residual biases being assimilated
  - Reduce analysis uncertainties (as RT model and forecast model biases are also, inevitably, reduced in time)

GSICS Annual Meeting, Kim et al



# Fundamental Climate Data Records (FCDRs)

- Focus on TB FCDR
  - decades-long time-series of TB
- TB FCDR is foundation for various geophysical retrievals
- Used to look for climate trends
- Need to remove calibration jumps when transitioning sensors
- Or bridging gaps
- Should help separate calibration drifts from real climate trends

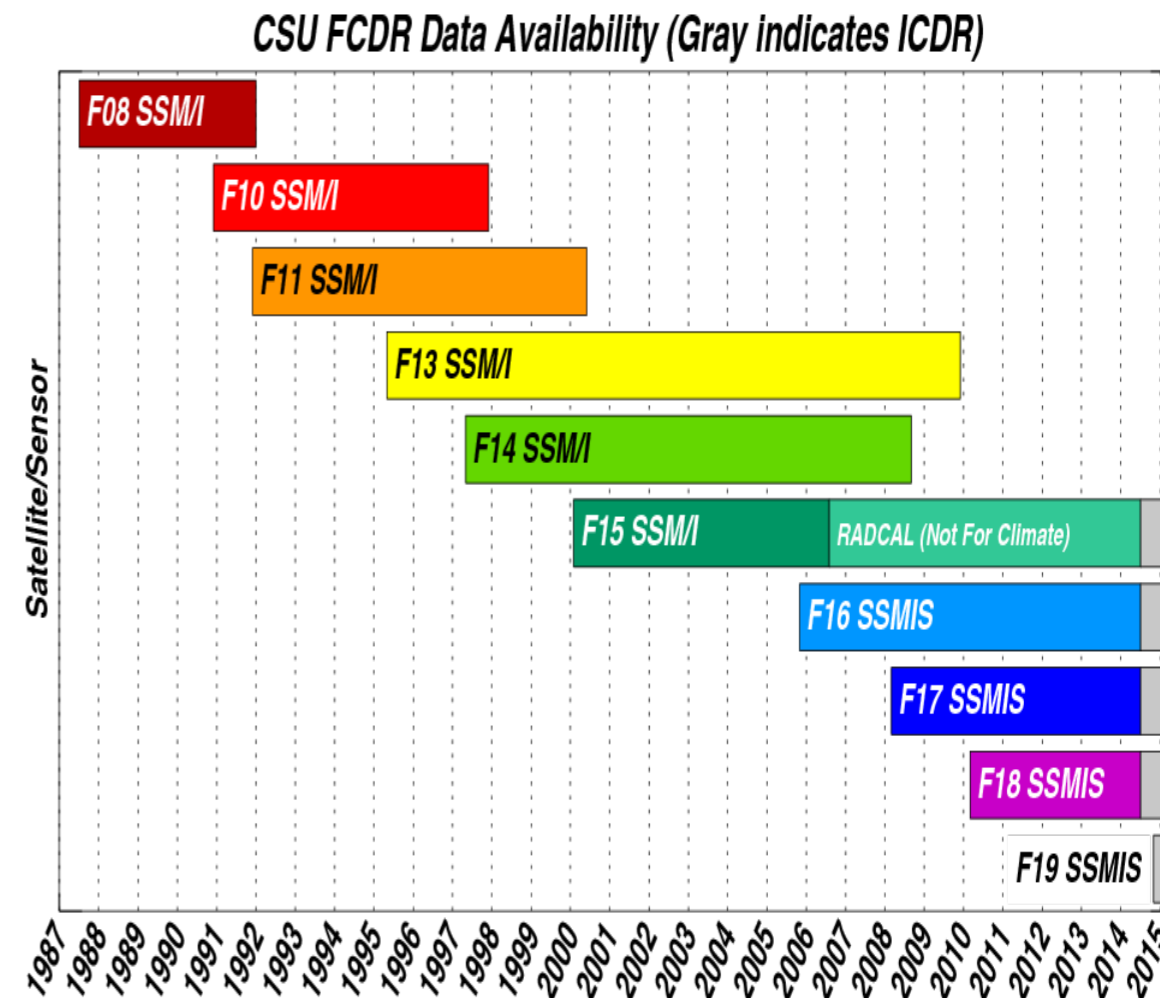

Pre-launch *traceable* TB calibration would help attribute uncertainties properly & better quantify them

# What SI-traceable TB Cal Does Not Address

- Careful! Total TB = f(footprint, scaling, amplitude)
  - Traceable TB cal helps quantify the amplitude uncertainty
  - Still need other techniques to address the effects of the footprints & scaling
  - What is addressed via harmonization or homogenization and what is addressed by SI-traceable TB cal is TBD

# The Technology of Traceable TB Calibration

- NIST blackbody target
- Traceable calibration methodology
- Formal standards
- Upcoming satellite mw radiometers

# NIST Blackbody Calibration Standard

Broadband passive microwave blackbody

NIST primary standard; traceable to SI kelvin

18-220 GHz design frequency range

Result of Derek Houtz's PhD thesis

Design requirements:


Maximize emissivity

Minimize temperature gradients

Variable temperature operation

Minimize IR radiation effects

Compatible with ATMS (2 targets: 12 & 23 cm dia.)

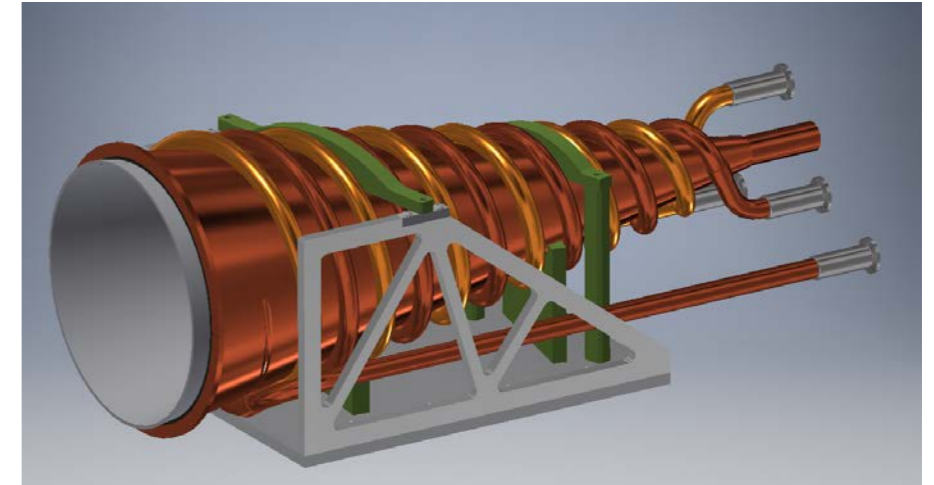


Hollow  
Cone  
geometry



GSICS Annual Meeting, Kim et al

# Traceable Calibration Methodology

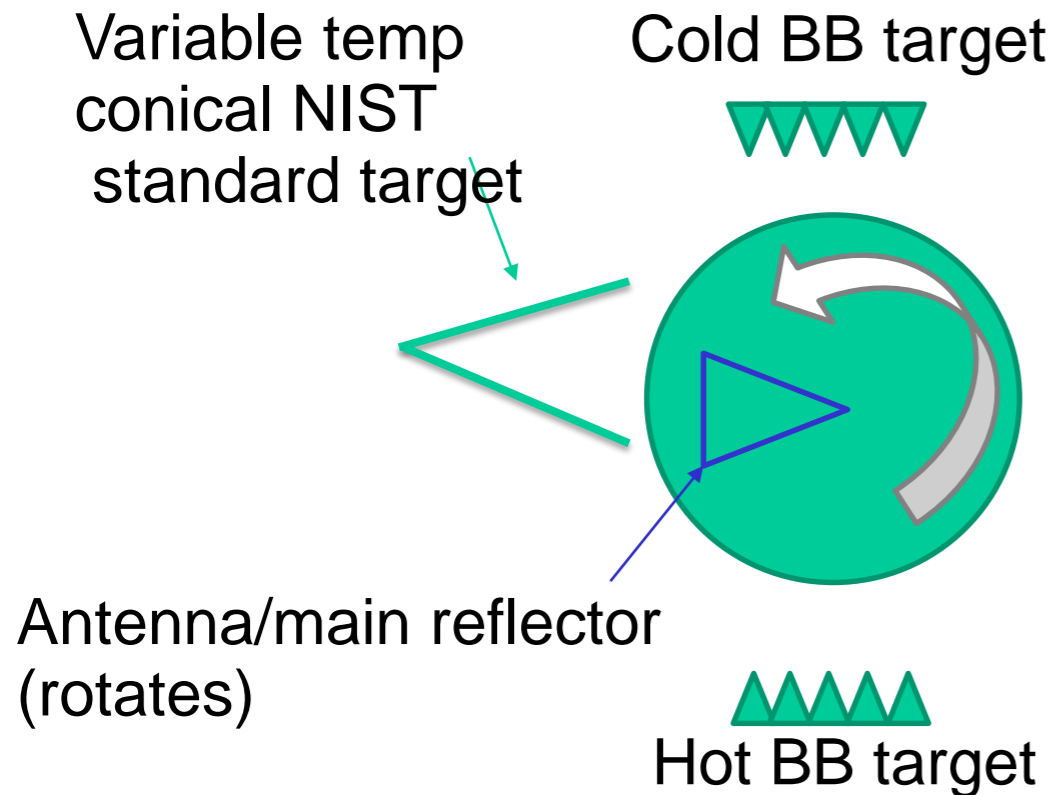

## Basic methodology:

- Alternately viewing reference target(s) while adjusting new target until radiometer raw response (counts) matches
- Results in transfer of cal to new target/system
- Status: additional engineering work needed
  - Thermal uniformity
  - Temperature range
  - Temperature sensors
  - Vacuum compatibility
  - adjust for coupling geometry

GSICS Annual Meeting, Kim et al



# Formal Standards for MW Radiometer Calibration

**ISO 20930:2018--approved**

Space systems — Calibration requirements for satellite-based passive microwave sensors

**IEEE** Geoscience and Remote Sensing Society (GRSS) has just started to explore whether to create an IEEE standard for calibration of all microwave radiometers (including ground & airborne)


# Potential Opportunities to Calibrate Future Satellite MW Radiometers

- Metop-SG radiometers (particularly MWI, MWS)
- ATMS beginning on JPSS-3 or 4
- AMSR x ?
- Cubesat radiometers
- Other future sounders & imagers

# Radiometers under development at ESA

## Microwave Sounder (MWS)

24 channels, 23 GHz - 230 GHz  
155 kg, 190 W  
1m x 1.5m x 0.6m

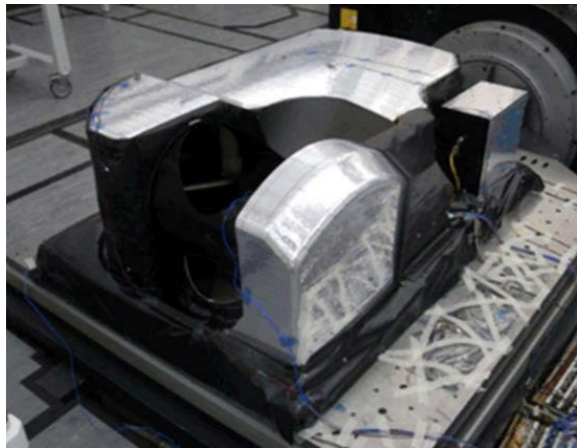


## Microwave Imager (MWI)

26 channels (18.7 to 183 GHz)  
285 kg (150 kg rotating), 250 W  
2m x 1.4m x 1.4m



## Ice Cloud Imager (ICI)

13 channels (183 to 664 GHz)  
175 kg (68 kg rotating @45rpm), 130 W  
1.3m x 1.6m x 0.8m

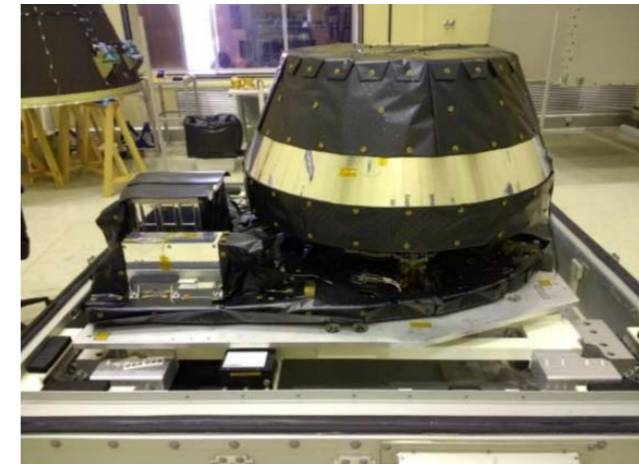

3 flight models each will be launched between 2022 and 2036,  
providing operations at least until mid-2040's  
MWS and MWI could benefit from SI traceability as similar instruments are operational or planned

Ville Kangas, ESA

GSICS Annual Meeting,  
Kim et al

ESA Unclassified – For Official Use



European Space Agency

6 March 2019




GSICS Annual Meeting, Kim et al



19

# Radiometers under development at NASA

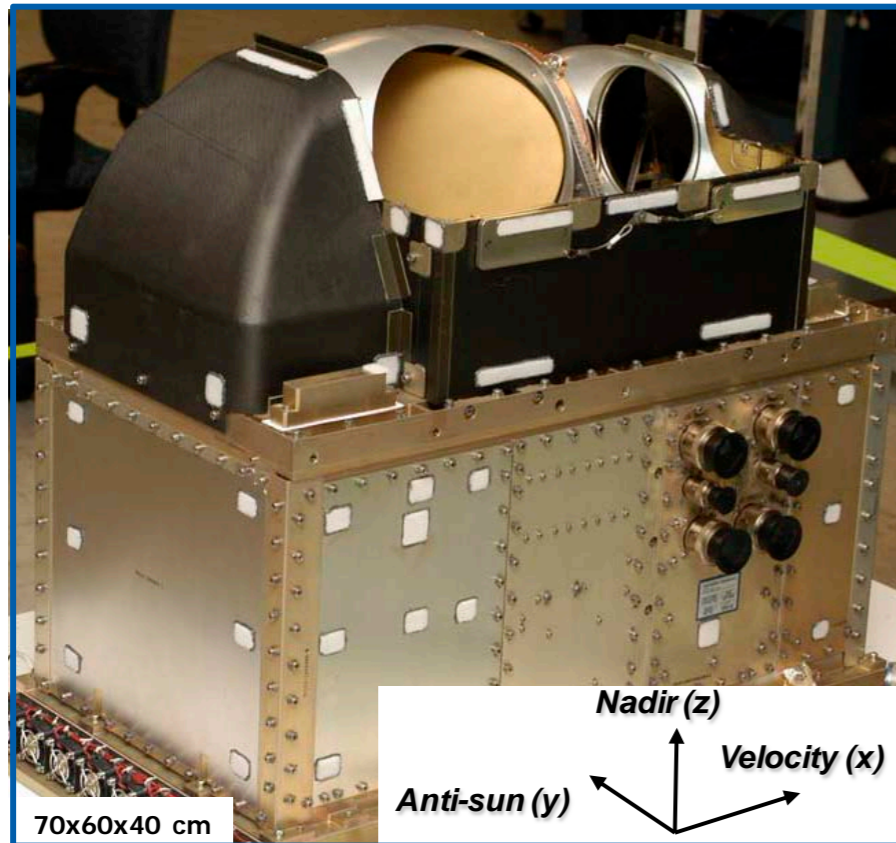

ATMS

on



JPSS-2/3/4

# Status and Future Plans

## Status:

- NIST prototype conical blackbody standard for TB has been designed/fabricated for 18-220 GHz
- Enables traceability to SI-kelvin & incorporation of rigorous standards-level quantification of Type A and Type B uncertainties
- Physical blackbody standard would enable rigorous pre & post-launch inter-calibration of constellation systems plus long time-series records (e.g., FCDRs) including gaps
- Absolute TB calibration would permit more realistic NWP uncertainty allocation (eventually leading to better forecasts) & enhance our ability to generate FCDRs from TB observations
- New standard ISO 20930 for satellite MW radiometer calibration

## Future Plans:

- Additional development and analysis work on conical BB target; demonstrate practical calibration transfer to satellite instrument (ATMS?)
- Possible use with future Metop-SG radiometers and/or ATMS on JPSS-3 or 4
- IEEE standard being considered for MW radiometer cal (all MW radiometers, not just satellite)



# May 20, 2019

## World Metrology Day

- Basic definitions of fundamental SI units will be updated
  - All 7 fundamental SI units will be quantum-based
- Example expected outcomes:
  - SI kilogram definition will go from a metal block to quantum-based
  - **SI kelvin definition will become entirely quantum-based**
  - <https://www.bipm.org/en/measurement-units/rev-si/>



# Thank you!

ed.kim@nasa.gov

+1-301-614-5653