



Concomitant B1 Field in Low-Field MRI: Potential Contributions to TRASE Image Artefacts

Christopher Bidinosti, Pierre-Jean Nacher, Geneviève Tastevin

► To cite this version:

Christopher Bidinosti, Pierre-Jean Nacher, Geneviève Tastevin. Concomitant B1 Field in Low-Field MRI: Potential Contributions to TRASE Image Artefacts. Joint annual meeting ISMRM-ESMRMB 2018, Proc. of the Intl. Soc. Mag. Reson. Med., Jun 2018, Paris, France. pp.2670. hal-02366411

HAL Id: hal-02366411

<https://hal.archives-ouvertes.fr/hal-02366411>

Submitted on 15 Nov 2019

HAL is a multi-disciplinary open access archive for the deposit and dissemination of scientific research documents, whether they are published or not. The documents may come from teaching and research institutions in France or abroad, or from public or private research centers.

L'archive ouverte pluridisciplinaire **HAL**, est destinée au dépôt et à la diffusion de documents scientifiques de niveau recherche, publiés ou non, émanant des établissements d'enseignement et de recherche français ou étrangers, des laboratoires publics ou privés.

Copyright

Concomitant B₁ Field in Low-Field MRI: Potential Contributions to TRASE Image Artefacts

Christopher P Bidinosti¹, Pierre-Jean Nacher², and Geneviève Tastevin²

¹Department of Physics, University of Winnipeg, Winnipeg, MB, Canada, ²Laboratoire Kastler Brossel, ENS-PSL Research University, CNRS, UPMC-Sorbonne Université, Collège de France, Paris, France

Synopsis

TRansmit Array Spatial Encoding (TRASE) MRI uses trains of rf pulses produced by transmit coils which generate transverse fields of uniform magnitude and spatially varying directions. These coils also unavoidably generate concomitant rf fields, which in turn affect magnetisation dynamics during rf flips in low-field NMR. Bloch's equation are numerically solved to show that π -pulses imperfectly reverse transverse magnetisation and that the resulting error in azimuthal angle linearly increases with B_1/B_0 , with the number of pulses in the TRASE pulse train, and with distance from the coil axis in the sample. This may induce significant image distortions or artefacts. Supporting experiments performed at 2 mT will be reported.

Introduction

TRansmit Array Spatial Encoding (TRASE)^{1,2} is a pulsed MRI technique that involves B₁-field phase gradients for rf excitation and k-space traversal within echo trains. Dedicated transmit coils and repeated series of π -pulses with positive and negative phase gradients are needed for image acquisition. Ideal phase gradients correspond to uniform B₁ magnitude in the transverse plane and linear variation of B₁ direction along the encoding axis. With careful transmit coil design, the target homogeneity of B₁ amplitude can be achieved. But, to accommodate for changes in B₁ orientation, concomitant rf field components necessarily exist. For a z-axis phase gradient, for instance, the leading concomitant component (B_{1z}) can be expected to have a negligible contribution to the rf-driven evolution in high field and may simply contribute to rf power deposition.² In contrast, time evolution in low field, where B₁ magnitude is not much smaller than B₀, may be influenced both by the counter-rotating component of an oscillating transverse field³ and by the concomitant component B_{1z}. Here we analyse the NMR dynamics and focus, in particular, on the deviations in time evolution that occur for one or several π -rotations applied by spiral transmit coils designed for TRASE imaging.^{4,5}

Methods

Numerical solutions of Bloch's equation are computed using compiled C or Mathematica programs for a simple analytical model (a field of perfectly uniform transverse magnitude) and for the exact field map of the transmit coil used in current low-field TRASE studies⁵ (Fig. 1). Different types of rf pulses and pulse sequences are considered, acting either on longitudinal or transverse magnetisation. Emphasis is placed on resonant and near-resonant inversion pulses, for which the influence of pulse shape and duration is investigated. Experimental tests on thermally polarised imaging phantoms (slab-shaped containers filled with doped water) are under way at 2 mT (83.682 kHz). Assessments are performed for series of π -pulses from spiral coils with a combination of techniques, such as usual 2D imaging (with B₀-field magnitude gradients) or phase mapping by NMR interferometry.⁶

Results

Figure 1 shows a prototype spiral coil and displays computed field maps. The helicoidal field pattern has a linear z-dependence of its phase $\varphi(z)=kz$ (with a pitch coefficient $k=0.12\text{ cm}^{-1}$) and a fairly uniform magnitude of the transverse component, B_{1t} (aligned with the y-axis, at the coil centre). The (mainly) x-dependent concomitant rf field component, B_{1z}(x) = k x B_{1t}, satisfies the $\text{rot}(\mathbf{B}_1)=0$ Maxwell's equation under the assumption of perfectly uniform B_{1t}. However, this approximation breaks down for distances from the z-axis of order $a/2$ and the actual field maps, which satisfy both $\text{rot}(\mathbf{B}_1)=0$ and $\text{div}(\mathbf{B}_1)=0$, are needed for reliable NMR simulations. Figure 2 displays magnetisation trajectories (in the rotating frame) during rf π -pulses computed for sample elements in the z=0 plane, lying either on the coil axis (left: x=0; hence, B_{1z}=0) and off axis (right: $kx=1 = B_{1z}/B_{1t}$, chosen for clear effects). They allow for a comparison between evolution perturbed by the counter-rotating component alone (see³ for further details) or in combination with the concomitant component B_{1z}. In both cases, the trajectory features depend on the initial magnetization state. On axis, in spite of deviations from rotating wave approximation (RWA) trajectories, perfect inversion is achieved. Off axis, B_{1z} yields deviations with distinct time variation and maximal amplitudes but, most notably, induces a phase shift α for the East-West trajectory endpoint. This shift increases with B₁ magnitude and distance from the spiral coil axis and is found to amount to $\alpha = \alpha_0 k y/N_\pi$, where $\alpha_0 = 58^\circ$ and $N_\pi = B_{1t}/B_0$ is the ratio between the π -pulse duration and the rf period. As a result, for a TRASE phase-encoding sequence comprising tens of pulses, the expected cumulated added rotation can exceed 90°.

Discussion

In TRASE MRI, trains of PI pulses from a pair of coils are expected to create magnetisation patterns which only depend on the geometry of the coils, e.g., only depend on z for spiral coils such as in Fig.1 (x or y dependence may also be achieved, for instance with "Maxwell-type" coils²). However, we have shown that the concomitant rf field B_{1z} modifies the phase pattern imprinted on the transverse magnetization in such a way that, to first order, geometrical planes where phase is uniform are no longer perpendicular to the encoding direction but tilted. This tilt, which linearly increases with the field intensity ratio B₁/B₀, may induce significant image distortions or artefacts, an issue which will need to be addressed.

Acknowledgements

Support from CNRS and ENS for joint work is gratefully acknowledged (CP B.).

References

1. JC Sharp et al., Magn Reson Med 63:151 (2010); NMR Biomed, 26: 1602 (2013).
2. Q Deng et al., Magn Reson Imaging 31:891 (2013).
3. CP Bidinosti et al, this conference
4. CP Bidinosti et al., Proc. ISMRM 18 (2010) p. 1509.
5. P-J Nacher et al., Proc ESMRMB15, Magn. Reson. Mater. Phy. 28 Suppl. 1 (2015) p. S64.
6. L Darrasse et al., Magn Reson Imaging 5:559 (1987).

Figures

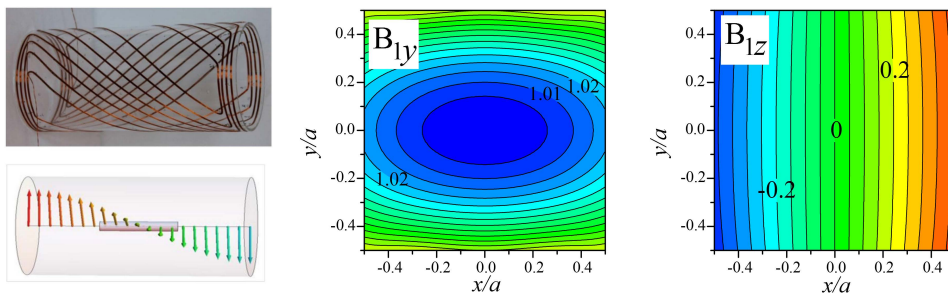


Figure 1: Left: photograph of a spiral coil used for z-encoding in low-field TRASE experiments³ and sketch of the transverse rf field directions it generates. The spiral coil pitch is $k=0.12 \text{ cm}^{-1}$. Right: computed maps of the transverse and longitudinal field components in the central xy plane, scaled to the field B_C at the coil centre (coil radius: $a=6.5 \text{ cm}$). Over the same domain, B_{1x}/B_C (not displayed) remains smaller than 0.02, hence the transverse field has a very uniform direction and amplitude. As expected for this near-uniform field, B_{1z} only depends on x , with the expected linear variation (see text) over a wide domain.

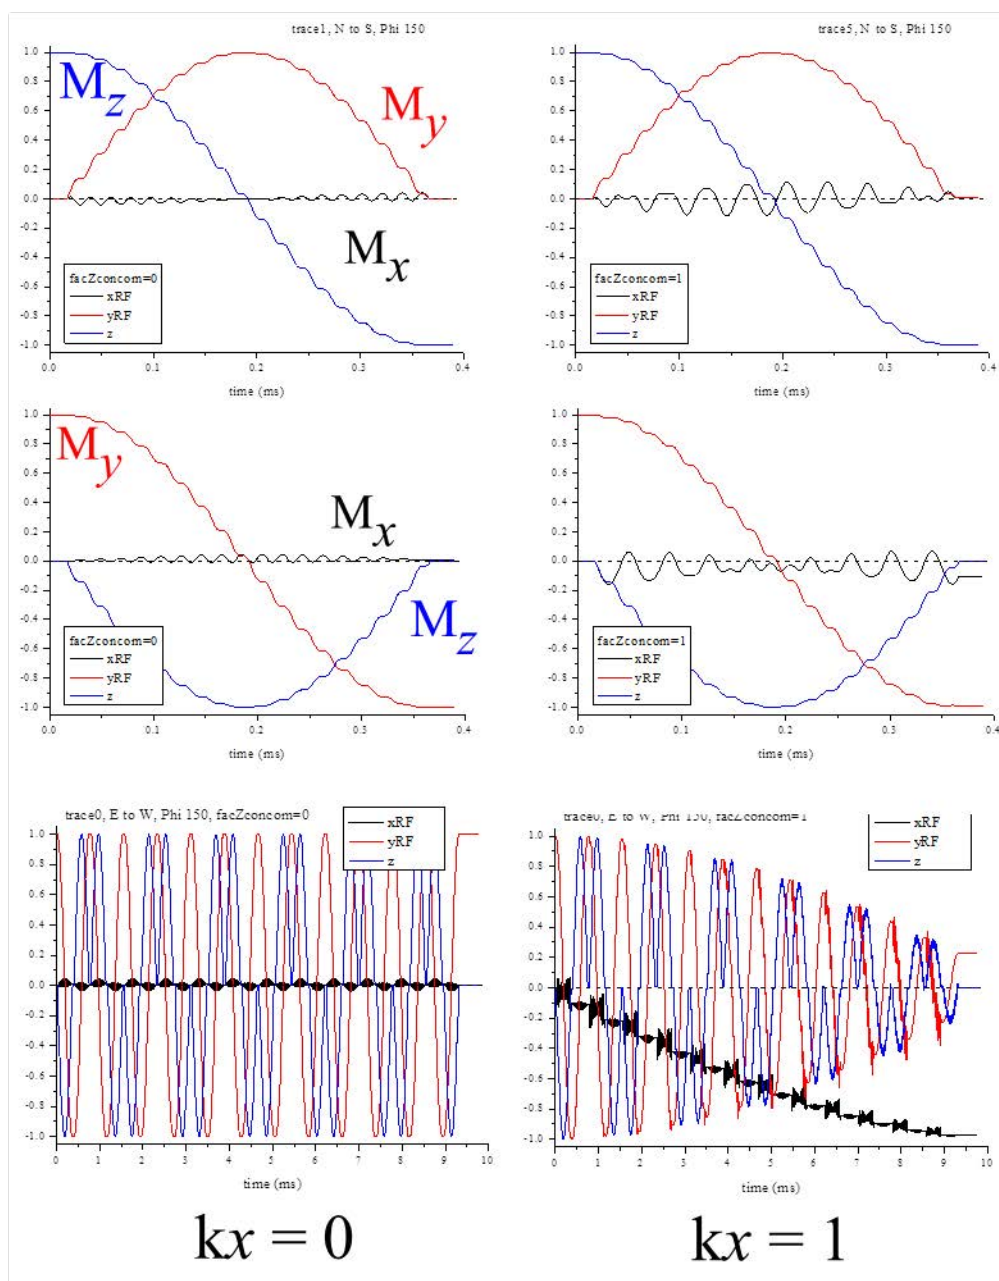


Figure 2: Time-evolution of the 3 components of the magnetisation undergoing a π -rotation driven by a 9-period-long rectangular rf pulse ($N_\pi=9$). Top row: N to S; middle row: E to W trajectories. On-axis ($kx=0$), the trajectories are affected by the counter-rotating part of the oscillating rf field but the endpoints correspond to exact π rotations. Off-axis, the added concomitant field component B_{1z} induces significant deviations of the x -component of the magnetisation. Moreover, the endpoint of a π pulse on initially transverse magnetisation reveals a significant phase shift. Bottom row: these phase shifts add up for chained TRASE π -pulses.