

J Vect Borne Dis 44, March 2007, pp. 69–71

Effect of EDTA and ACD on blood storage for the detection of *Plasmodium falciparum* by PCR

P.K. Patibandla^a, V. Venkatesh^a, G.G. Agarwal^b, S. Awasthi^c, N. Husain^d, R.C. Ahuja^e, S. Swastika^a & S.K. Agarwal^a

^aDepartment of Microbiology, King George's Medical University, Lucknow; ^bDepartment of Statistics, University of Lucknow, Lucknow; ^cDepartment of Paediatrics, ^dDepartment of Pathology, ^eDepartment of Medicine and CEU, King George's Medical University, Lucknow, India

Key words ACD – EDTA – malaria – PCR – *Plasmodium falciparum*

Blood samples are extensively used for PCR-based diagnosis of microbial infections and screening for blood banking¹. It is not possible to do PCR with fresh blood samples each time. This preliminary study is aimed to compare the effect of blood storage (–20°C) on PCR for detecting *Plasmodium falciparum* in the two most commonly used anticoagulants such as ethylenediaminetetra acetic acid (EDTA) and acid citrate dextrose (ACD)^{2,3}.

The study was conducted in Department of Microbiology, King George's Medical University (KGMU), Lucknow, Uttar Pradesh, India. The protocol was approved by the institutional ethical committee, KGMU, Lucknow. Informed consent was obtained from relatives of the patients.

Seven microscopy and rapid diagnostic test (RDT) positive blood samples for falciparum malaria, three microscopy and RDT negative (healthy persons) blood samples (Haemoglobin $\leq 12\%$) were collected in EDTA and ACD anticoagulants and stored at –20°C for a period varying between 2 and 10 months.

These samples were collected before start of the antimalarial therapy during the period from August 2005 to April 2006. All patients had acute febrile illness and later they had responded to antimalarial

therapy. Giemsa stained thick and thin blood films were observed under microscope. RDT for detecting the HRP-2 antigen of *P. falciparum* was performed using a commercially available kit (Paracheck Pf, Orchid Biomedical Systems, Goa, India) and results were interpreted as per manufacturer's instructions.

The protocols according to Patsoula *et al*⁴, and Witoon *et al*⁵, were followed on EDTA and ACD stored blood. Either of these methods in their exact format could not work in our settings. The reason may be that these authors had used fresh EDTA and sodium dodecyl sulphate blood. So we selected primer sets used by these authors but standardised PCR mix and PCR protocol in our laboratory which produced optimal results.

The rapid DNA extraction method according to Michael *et al*⁶, and Raj *et al*⁷ was selected with a few modifications. Briefly, 500 μ l of ice-cold 5 mM sodium phosphate (pH-8) was added to 20 μ l of venipuncture blood and vortexed. After centrifugation for 6 min/14500 rpm in a micro centrifuge tube at 4°C, the supernatant was discarded. The pellet was suspended in 100 μ l PBS containing 0.01% saponin and washed twice with same buffer by repeating the above steps of vortexing and centrifugation. After washing, the pellet was suspended in 50 μ l of sterile

triple distilled water, vortexed and boiled for 20 min at 100°C. It was again vortexed before use for PCR. PCR was done separately for both sets of primers on all ten samples in the month of June 2006. Two primer sets were used as follows:

Primer set 1 (Patsoula *et al*⁴)

PL3 (5' ATGGCC GTT TTT AGT TCG TG 3')
PL5 (5' ACG CGT GCA GCC TAG TTT AT 3')

Primer set 2 (Witoon *et al*⁵)

PF1 (5' GCT ACA TATGCT AGT TGC CAG AC 3')
PF2 (5' CGT GTACCA TAC ATC CTA CCA AC 3')

For primer set 1, PCR reaction was performed in a mix, with a final volume of 50 µl containing 1 × PCR buffer, 1.5 mM MgCl₂, 0.2 mM dNTP mix, 20 pm of each PL3 and PL5 primer 2.5 units Taq-DNA polymerase (Invitrogen, Brazil). For primer set 2 reaction mix was same as above except that primers used were PF1 and PF2.

In each run, an initial 4-min denaturation at 94°C was followed by 35 cycles, each of denaturation at 94°C for 30 sec, annealing at 52°C for 35 sec, extension at 72°C for 30 sec, and then a final extension at 72°C for 5 min. PTC100 (MJ Research, Watertown, mass model, USA) was used in all experiments. The PCR products were subjected to electrophoresis in 1.5% agarose gel (Fig. 1).

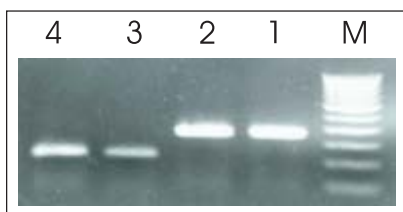


Fig. 1: Agarose gel electrophoresis pattern of PCR products from *P. falciparum* positive long-term stored blood samples. Lanes 1, 2 (primer set 1) and lanes 3, 4 (primer set 2) produced 346 bp and 206 bp with EDTA, ACD respectively, M–100 bp ladder

For primer set 1, EDTA stored blood gave 100% (7/7) sensitivity and 100% (3/3) specificity whereas ACD stored blood gave only 14.28% (1/7) sensitivity and 100% (3/3) specificity. For primer set 2, EDTA stored blood gave 57.14% (4/7) sensitivity and 100% (3/3) specificity, whereas ACD stored blood gave only 28.57% (2/7) sensitivity and 100% (3/3) specificity.

The results from our preliminary study showed that EDTA with primer set 1 produced positive results from blood samples stored as old as 10 months, whereas EDTA with primer set 2, produced positive results for blood samples old up to eight months only. These results along with the results of ACD (both sets of primers) are shown in Fig. 2.

This suggests that long-term EDTA stored blood (–20°C) when used with Patsoula *et al*⁴, primer and our standardised PCR mixture and cycles produced results with 100% sensitivity and 100% specificity, however, there was decrease in sensitivity with ACD stored blood with both sets of primers. One of the

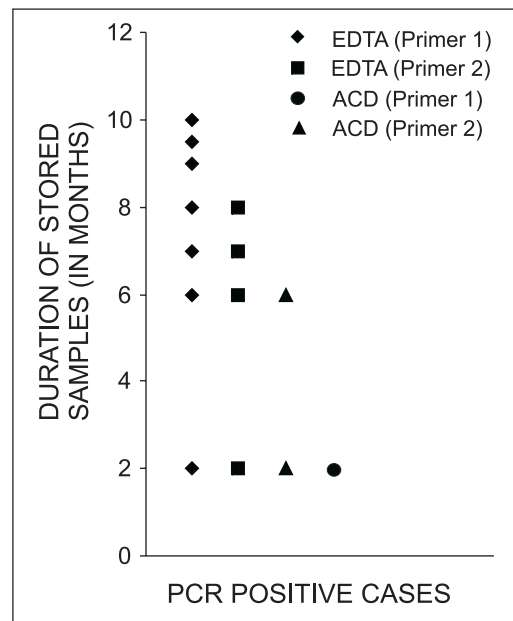


Fig. 2: Effect of duration of blood storage in EDTA and ACD anticoagulants on PCR for detecting *P. falciparum* malaria

reasons could be that the dilution effect caused by the liquid formulation of ACD decreased the nucleic acid recovery⁸⁻¹⁰. However, the exact reasons are not known.

So based on this preliminary study EDTA appeared to be a better anticoagulant than ACD for delayed blood processing in case of PCR analysis for *P. falciparum*. Our analysis, though, based on a small sample size, produced optimal results. However, a study is needed with a large number of stored blood samples to get a stronger evidence of the above results.

Acknowledgement

This work was supported by Intramural Faculty Grants 2005 awarded to Dr. V. Venkatesh, King George's Medical University, Lucknow, India.

References

1. Waleed Abu Al-Soud, Peter Rådström. Purification and characterization of PCR-inhibitory components in blood cells. *J Clin Microbiol* 2001; 39: 485-93.
 2. Viroj Wiwanitkit. A note in the acid citrate dextrose tube in the present usage. *Haematology* 2003; 6: 407-8.
 3. Nicole Lam YL, Timothy Rainer H, Rossa Chiu WK, Dennis Lo YM. EDTA is a better anticoagulant than heparin or citrate for delayed blood processing for plasma DNA analysis. *Clin Chem* 2004; 50: 256-7.
 4. Patsoula E, Spanakos G, Sofianatou D, Parara M, Vakalis NC. A single-step, PCR-based method for the detection and differentiation of *Plasmodium vivax* and *P. falciparum*. *Ann Trop Med Parasitol* 2003; 97: 15-21.
 5. Witoon Tirasophon, Piengchan Rajkulchai, Mathurose Ponglikitmonkol, Prapon Wilairat, Vichai Boonsaeng, Sakol Panyim. A highly sensitive, rapid and simple polymerase chain reaction-based method to detect human malaria (*Plasmodium falciparum* and *Plasmodium vivax*) in blood samples. *Am J Trop Med Hyg* 1994; 51: 308-13.
 6. Michael Foley, Lisa Ranford-Cartwright C, Hamza Babiker A. Rapid and simple method for isolating malaria DNA from fingerprick samples of blood. *Mol Biochem Parasitol* 1992; 53: 241-3.
 7. Raj Dipak Kumar, Mishra Sasmita, Das Bibhu Ranjan, Dash Aditya Prasad. *Plasmodium falciparum* Pfs 25 gene promoter has no polymorphism in natural isolates of eastern India. *Acta Protozool* 2005; 44: 289-92.
 8. Dickover RE, Herman SA, Saddiq K, Wafer D, Dillon M, Bryson YJ. Optimization of specimen-handling procedures for accurate quantitation of levels of human immunodeficiency virus RNA in plasma by reverse transcriptase PCR. *J Clin Microbiol* 1998; 36: 1070-3.
 9. Ginocchio CC, Wang X, Kaplan MH, Mulligan G, Witt D, Romano JW, Cronin M, Carroll R. Effects of specimen collection, processing, and storage conditions on stability of human immunodeficiency virus type 1 RNA levels in plasma. *J Clin Microbiol* 1997; 35: 2886-93.
 10. Holodniy M, Mole L, Yen-Lieberman B, Margolis D, Starkey C, Carroll R, Spahlinger T, Todd J, Jackson JB. Comparative stabilities of quantitative human immunodeficiency virus RNA in plasma from samples collected in vacutainer CPT, vacutainer PPT, and standard vacutainer tubes. *J Clin Microbiol* 1995; 33: 1562-6.
- Corresponding author:* Phani Kumar Patibandla, Department of Microbiology, King George's Medical University, Lucknow-226 003, India.
E-mail: phani_pati@rediffmail.com

Received: 27 June 2006

Accepted in revised form: 3 January 2007