

Educational Notes in Research Methodology and Medical Statistics DOI: 10.22114/ajem.v0i0.158

Sample Size Calculation Guide - Part 4: How to Calculate the Sample Size for a Diagnostic Test Accuracy Study based on Sensitivity, Specificity, and the Area Under the ROC Curve

Ahmed Negida^{1,2*}, Nadien Khaled Fahim³, Yasmin Negida¹

1. Faculty of Medicine, Zagazig University, Zagazig, El-Sharkia, Egypt.
2. Neurosurgery Department, School of Medicine, Bahçeşehir University, Istanbul, Turkey.
3. Clinical Program, Faculty of Pharmacy, Zagazig University, Zagazig, Egypt.

*Corresponding author: Ahmed Negida; Email: ahmed01251@medicine.zu.edu.eg, ahmed.said.negida@gmail.com

Published online: 2019-05-19

INTRODUCTION

In the previous educational articles, we explained how to calculate the sample size for a rate or a single proportion, for an independent cohort study, and for an independent case-control study (1-3). In this article, we will explain how to calculate the sample size for a diagnostic test accuracy study based on sensitivity, specificity, or the area under the ROC curve.

WHEN TO USE THE SAMPLE SIZE CALCULATION PROCEDURE OF DIAGNOSTIC PERFORMANCE

The methods explained hereafter should be used in the case that the diagnostic performance of your new test (new device, survey, or biomarker) is expressed as sensitivity, specificity, or area under the ROC curve. The definitions of sensitivity, specificity, or area under the ROC curve were explained by us in previous education editorials (4, 5).

• SAMPLE SIZE CALCULATION BASED ON SENSITIVITY OR SPECIFICITY

We will use the sample size calculation methods of Buderer et al.1996 (6). In this method, we need first to calculate the TP+FN for sensitivity and the TN+FP for specificity through the following equation.

$$TP + FN = Z^2 \times \frac{\text{Sensitivity} (1 - \text{Sensitivity})}{W^2}$$

$$TN + FP = Z^2 \times \frac{\text{Specificity} (1 - \text{Specificity})}{W^2}$$

Where Z, the normal distribution value, is set to 1.96 as corresponding with the 95% confidence interval, W, the maximum acceptable width of the 95% confidence interval, is set to 10%, and the expected sensitivity and specificity are defined based on the estimates from previous studies.

The next step is to calculate N required for sensitivity and N required for specificity through

the following equations:

N required for sensitivity

$$\frac{TP + FN}{P}$$

N required for specificity

$$\frac{TN + FP}{1 - P}$$

EXAMPLE: A STUDY TO EVALUATE THE ACCURACY OF BLOOD PRESSURE TO HEIGHT RATIO AS A DIAGNOSTIC TOOL FOR HYPERTENSION AMONG ADOLESCENTS

Assume that we will conduct a study to estimate the accuracy of blood pressure to height ratio as a diagnostic tool for hypertension in adolescents in Egypt. Therefore, we will enroll a group of adolescents including those with hypertension and those without hypertension. Each subject will be screened twice, first time by the gold standard test (reference test), then by the new test (blood pressure to height ratio).

A previous similar study reported a sensitivity of 90% and specificity of 90% while the prevalence rate of hypertension in Egyptian adolescents was 5% (7).

To calculate the sample size required for this study, we apply the above-mentioned equations and the results were as follows:

$$TP + FN = 34.5$$

$$TN + FP = 34.5$$

Then, we calculate the N required for sensitivity and the N required for specificity, as follows:

N required for sensitivity

$$\frac{TP+FN}{P} = \frac{34.5}{0.05} = 691 \text{ participants}$$

N required for specificity

$$\frac{TN+FP}{1-P} = \frac{34.5}{1-0.05} = 36 \text{ participants}$$

Total required sample size

$$691 + 36 = 728 \text{ participants}$$

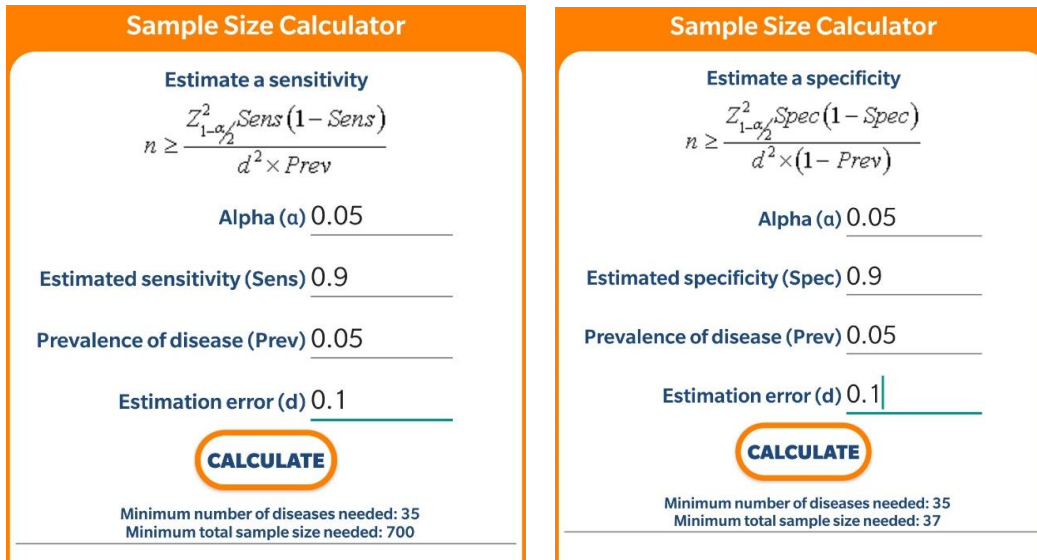


Figure 1: shows calculating the sensitivity and specificity by an android app

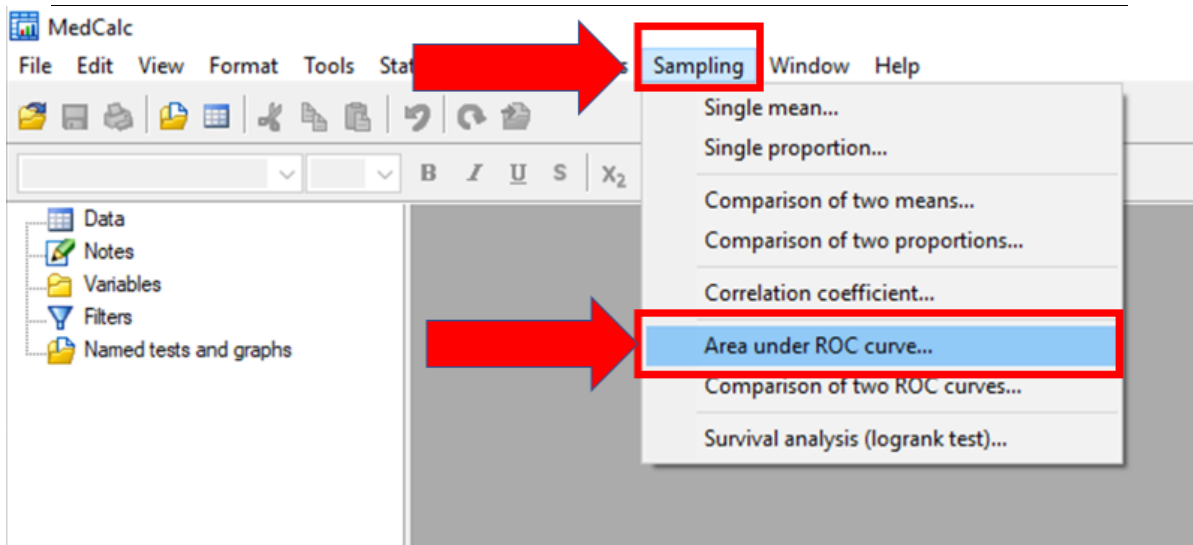


Figure 2: MedCalc menu

Therefore, in this study, should include 691 participants with hypertension and 36 participants without hypertension yielding a total sample size of 728 participants.

These equations were programmed by a Vietnamese biostatistician into an android app named “statistics and sample size pro”. By providing the same inputs, we obtain similar estimates (Figure 1).

• **SAMPLE SIZE CALCULATION BASED ON THE AREA UNDER THE ROC CURVE**

This will require to provide the following inputs in MedCalc software

1. Expected AUC

2. Null value of the AUC (usually 50% is the null value)
3. Ratio between negative and positive cases

EXAMPLE: A STUDY TO EVALUATE THE ACCURACY OF CSF LACTATE IN DISCRIMINATING THE BACTERIAL MENINGITIS FROM ENTEROVIRAL MENINGITIS.

Assume that we will conduct a study to estimate the accuracy of CSF lactate to discriminate bacterial meningitis from enteroviral meningitis. Therefore, we will enroll a group of patients with acute meningitis including those with bacterial meningitis and those with enteroviral meningitis. For each CSF specimen, bacterioscopy, bacterial antigen latex agglutination test and CSF bacterial

culture will be performed as a standard test (reference test), then the CSF lactate will be estimated (new test).

A previous study by Manomaivat et al. showed that the AUC of CSF lactate was 94% for discriminating bacterial meningitis from enteroviral meningitis (8). The ratio between negative and positive cases was 525/662.

In order to calculate the sample size required for our new study, we will provide the inputs to MedCalc software as follows:

First, open the software then select "sampling" for sample size calculation options then, select "area under the ROC curve" (Figure 2). Finally, submit the data and check the table for the calculation results. As shown in figure 3, the results table shows a sample size of 11 patients (5 cases of enteroviral meningitis and 6 cases of bacterial meningitis) corresponding with a 5% alpha error and a 10% beta error.

The screenshot shows the 'Sampling: area under ROC curve' window in MedCalc. The 'Type I and II error' section has Type I error (Alpha, Significance) set to 0.05 and Type II error (Beta, 1-Power) set to 0.10. The 'Input' section has Area under ROC curve set to 0.94, Null Hypothesis value set to 0.50, and Ratio of sample sizes in negative / positive groups set to 525/662. The 'Results' section, highlighted with a red box, shows: Number of positive cases required: 6, Number of negative cases required: 5, and Total sample size (both groups together): 11. Below this is a table for Type I Error - Alpha and Type II Error - Beta.

		Type I Error - Alpha			
		0.20	0.10	0.05	0.01
Type II Error - Beta	0.20	3 + 3	4 + 4	6 + 5	9 + 8
	0.10	4 + 4	5 + 4	6 + 5	10 + 8
	0.05	4 + 4	6 + 5	7 + 6	11 + 9
	0.01	5 + 4	7 + 6	9 + 8	13 + 11

Figure 3: The results table

REFERENCES

1. Fahim NK, Negida A. Sample Size Calculation Guide - Part 1: How to Calculate the Sample Size Based on the Prevalence Rate. *Adv J Emerg Med.* 2018;2(4):e50.
2. Fahim NK, Negida A. Sample Size Calculation Guide - Part 2: How to Calculate the Sample Size for an Independent Cohort Study. *Adv J Emerg Med.* 2019;3(1):e12.
3. Fahim NK, Negida A, Fahim AK. Sample Size Calculation Guide - Part 3: How to Calculate the Sample Size for an Independent Case-control Study. *Adv J Emerg Med.* 2019;3(2):e20.
4. Safari S, Baratloo A, Elfil M, Negida A. Evidence Based Emergency Medicine; Part 5 Receiver Operating Curve and Area under the Curve., *Emerg (Tehran).* 2016;4(2):111-3.
5. Baratloo A, Hosseini M, Negida A, Ashal GE. Part 1: Simple Definition and Calculation of Accuracy, Sensitivity and Specificity. *Emerg(Tehran).* 2015;3(2):48-9.
6. Buderer NM. Statistical methodology: I. Incorporating the prevalence of disease into the sample size calculation for sensitivity and specificity. *Acad Emerg Med.* 1996;3(9):895-900.
7. Abolfotouh MA, Sallam SA, Mohammed MS, Loutfy AA, Hasab AA. Prevalence of Elevated Blood Pressure and Association with Obesity in Egyptian School Adolescents. *Int J Hypertens.* 2011;2011: 952537.
8. Domingues RB, Fernandes GBP, de M Leite FBV, Senne C. Performance of lactate in discriminating bacterial meningitis from enteroviral meningitis. *Rev Inst Med Trop Sao Paulo.* 2019;61: e24.