

P-19

NASA CASE NO. ARC 12014-1PRINT FIG 1

## NOTICE

The invention disclosed in this document resulted from research in aeronautical and space activities performed under programs of the National Aeronautics and Space Administration. The invention is owned by NASA and is, therefore, available for licensing in accordance with the NASA Patent Licensing Regulation (14 Code of Federal Regulations 1245.2).

To encourage commercial utilization of NASA-owned inventions, it is NASA policy to grant licenses to commercial concerns. Although NASA encourages nonexclusive licensing to promote competition and achieve the widest possible utilization, NASA will consider the grant of a limited exclusive license, pursuant to the NASA Patent Licensing Regulations, when such a license will provide the necessary incentive to the licensee to achieve early practical application of the invention.

Address inquiries and all applications for license for this invention to NASA/Ames Research Center, Patent Counsel, Mail Stop 200-11, Moffett Field, CA 94035-1000.

Serial Number: 08/125,888  
 Filing Date: 9/24/93  
 Patent No: \_\_\_\_\_  
 Date Patent Issued: \_\_\_\_\_

NASA/ARC

(NASA-Case-ARC-12014-1) SYSTEM FOR  
 IMPROVING MEASUREMENT ACCURACY OF  
 TRANSDUCER BY MEASURING TRANSDUCER  
 TEMPERATURE AND RESISTANCE CHANGE  
 USING THERMOELECTRIC VOLTAGES  
 Patent Application (NASA. Ames  
 Research Center) 19 p

N94-29361

Unclass

G3/35 0003665

Invention Abstract

## SYSTEM FOR IMPROVING MEASUREMENT ACCURACY OF TRANSDUCER BY MEASURING TRANSDUCER TEMPERATURE AND RESISTANCE CHANGE USING THERMOELECTRIC VOLTAGES

The present invention generally relates to a system for improving the measurement accuracy of a variable resistance transducer such as strain gauge. The system generates two voltages. The first voltage is a function of the resistance change measured by the transducer, and the second voltage is representative of the ambient temperature of the transducer. These generated voltages are achieved with very few lead wires and without the need for a second transducer. In addition, the measurements are uncontaminated by lead wire resistance effects.

Referring to Figure 1, transducer 6 receives current  $I$  from current reversing switch 2 in the forward and reverse direction via thermocouple conductors 4. Transducer 6 outputs first and second measured voltages  $V_a$  and  $V_b$  responsive to current  $I$  in the forward and reverse directions, respectively. Finally, addition/subtraction circuit 10 receives the first and second measured voltages  $V_a$  and  $V_b$  via conductors 8 and adds the first and second voltages to derive the resistance change and subtracts the first and second voltages to derive the thermoelectric effects which can be used to determine the temperature of transducer 6.

The present invention has industrial application for accurately measuring resistance changes and temperature unaffected by parasitic resistances encountered resulting from environmental or external conditions. The attractive features of the present invention is the minimization of the amount of conductors required for measuring temperature and resistance changes as well as using parasitic voltages in the system to determine the temperature of the transducer.

INVENTORS: Karl F. Anderson and Allen R. Parker, Jr.  
EMPLOYER: NASA-AMES RESEARCH CENTER  
SERIAL NO.: 08/125,888  
FILING DATE: 9/24/93

Title

SYSTEM FOR IMPROVING MEASUREMENT ACCURACY OF  
TRANSDUCER BY MEASURING TRANSDUCER TEMPERATURE  
AND RESISTANCE CHANGE USING THERMOELECTRIC  
5 VOLTAGES

Origin of the Invention

The invention described herein was made by employees of the  
United States Government and may be manufactured and used by or  
10 for the Government for governmental purposes without the payment of  
any royalties thereon or therefor.

BACKGROUND OF THE INVENTIONField of the Invention

15 The present invention generally relates to a system for improving  
the measurement accuracy of a variable resistance transducer such as  
a strain gauge. The system generates two voltages. The first voltage is  
a function of the resistance change measured by the transducer, and the  
20 second voltage is representative of the ambient temperature of the  
transducer. These generated voltages are achieved with very few lead  
wires and without the need for a second transducer. In addition, the  
measurements are uncontaminated by lead wire resistance effects.

Description of the Related Art

25 Several approaches are currently available for measuring  
resistance and temperature parameters in variable resistance  
transducers. These approaches are generally based on using separate  
transducers and wiring from the measurement system to the article to  
30 be measured. For example, the classic Wheatstone bridge electrical

circuit is typically used for measuring small variations in resistance, for example, to measure resistance changes when a strain gage is used as a transducer. The Wheatstone bridge may also include a second resistor to compensate for the temperature effects experienced by the main  
5 transducer resistance. An additional method of removing measurement error encountered when using the Wheatstone bridge includes measuring the transducer temperature using a separate thermocouple or resistance temperature device (RTD).

In addition, constant current excitation has been used in an  
10 attempt to achieve a linear output and avoid parasitic resistance problems when measuring resistance and temperature using, for example, a transducer. Constant current excitation can also achieve double the output voltage for a given power dissipation in the resistance transducer when compared to voltage divider circuits such as the  
15 Wheatstone bridge. "Constant Current Loop Signal Conditioning", the subject of a pending patent application, Serial No. 08,018,128, filed February 16, 1993, is an innovative form of constant current signal conditioning that uses a form of output voltage processing to completely eliminate lead wire resistance effect. Constant current loop signal  
20 conditioning is also discussed in NASA Technical Memorandum 104260 by Karl F. Anderson, "The Constant Current Loop: A New Paradigm for Resistance Signal Conditioning." Both the Patent Application Serial No. 08/018,128 and the NASA Technical Memorandum 104260 are hereby incorporated by reference.

25 One of the problems encountered using the Wheatstone bridge is that the output is generally nonlinear with respect to the resistance change. Within the Wheatstone bridge are found various electrical connections and lead wires that attach the resistance to be measured to the rest of the Wheatstone bridge circuit. The Wheatstone bridge circuit  
30 may also contain additional components, such as slip rings for

connecting rotating machinery and fuses for electrical fault protection. These various parasitic (i.e., present but undesirable) resistances will themselves vary due to the thermal, mechanical, chemical and other conditions of the environment. This variation in resistance may develop errors in measurement which are not always practical or easy to correct.

An example of a circuit known in the art which attempts to reduce the effects of parasitic resistance is a circuit which connects three wires to a remote variable resistor disposed in the environment. This three-wire circuit attempts to electrically subtract the parasitic resistance variations in each of the current carrying leads connected to the variable resistor. The parasitic resistances are effectively canceled at the output of the Wheatstone bridge by connecting the leads of adjacent arms of the Wheatstone bridge. This approach is effective in moderate temperature environments. The measurement system becomes less sensitive due to the increase in circuit resistance caused by the lead wires. In addition, since the wires and associated components are not identical, in severe temperature environments, the parasitic resistances vary greatly. This results in an unreliable output and inaccurate measurement. Thus, the prior art has been unable to measure resistance changes and temperatures which are unaffected by parasitic resistances or voltages.

It is, therefore, desirable to reliably measure resistance changes and temperature unaffected by external conditions such as parasitic lead wire resistances and thermoelectric effects which cause measurement errors. In addition, it is also desirable to minimize the number of conductors required for measuring resistance changes and temperature. Further, it is desirable to measure temperature in the presence of parasitic resistances resulting from environmental or external conditions.

### SUMMARY OF THE INVENTION

5 It is an object of the present invention to provide a system for accurately measuring resistance changes and temperature unaffected by parasitic resistances encountered in the system resulting from environmental or external conditions.

It is another object of the present invention to provide a system which minimizes the amount of conductors required for measuring temperature and resistance changes.

10 It is further an object of the present invention to provide a system which measures temperature due to environmental or external conditions using parasitic voltages caused by temperature gradients along parasitic resistances in the system.

15 To achieve these and other objects, the present invention provides a constant current loop measuring system for measuring a property including the temperature of a sensor responsive to an external condition being measured. The measuring system includes thermocouple conductors connected to the sensor, sensing first and second induced voltages responsive to the external condition. In addition, the measuring system includes current generating and reversing means for generating a constant current, and for supplying the constant current to the thermocouple conductors in forward and reverse directions generating first and second measured voltages, and determining means for receiving the first and second measured voltages from the current generating and reversing means, and for determining the temperature of the sensor responsive to the first and second measured voltages.

25 These together with other objects and advantages which will be subsequently apparent, reside in the details of construction and operation as more fully hereinafter described and claimed, with reference  
30

being had to the accompanying drawings forming a part hereof, wherein like numerals refer to like elements throughout.

### BRIEF DESCRIPTION OF THE DRAWINGS

5 Fig. 1 is a block diagram of the basic construction of the resistance and thermoelectric measuring system of the present invention;

Fig. 2a is a schematic diagram of the resistance and thermoelectric measuring system of the present invention.

10 Fig. 2b is a schematic diagram of a low noise version of the circuit depicted in Fig. 2a.

Fig. 3 is a schematic diagram of another embodiment of the resistance and thermoelectric measuring system of the present invention having multiple transducers.

15

### DETAILED DESCRIPTION OF THE PREFERRED EMBODIMENTS

Fig. 1 is a block diagram of the basic construction of the present invention. In Fig. 1, transducer 6 receives current  $I$  from current reversing switch 2 in the forward and reverse direction via thermocouple conductors 4. Transducer 6 outputs first and second measured voltages  $V_a$  and  $V_b$  responsive to current  $I$  in the forward and reverse directions, respectively. Finally, addition/subtraction circuit 10 receives the first and second measured voltages  $V_a$  and  $V_b$  via conductors 8 and adds the first and second voltages to derive the resistance change and subtracts the first and second voltages to derive the thermoelectric effects which can be used to determine the temperature of transducer 6.

25

Fig. 2a is a schematic diagram of the resistance and temperature measuring system of the first embodiment of the present invention. In Fig. 2a, single series circuit loop 11 includes constant current regulator

$I_{reg}$  which maintains current  $I$  at an essentially constant level within a predetermined range regardless of variations in the other components in the current loop. Parasitic resistances ( $R_{w1}$ ,  $R_{w2}$ ,  $R_{w3}$  and  $R_{w4}$ ) are present throughout the measuring system as illustrated and represent, for example, resistances in the lead wires of the measuring system, connection between the components of the measuring system or fault protection circuit elements included in the measuring system. For simplicity, these resistances will be referred to as "parasitic" resistances. Parasitic resistance  $R_{w1}$  and  $R_{w2}$  are positioned in the measuring system to carry the regulated excitation current  $I$  generated by the constant current regulator  $I_{reg}$  in circuit loop 11. A reference resistance  $R_{ref}$  is in series with the current regulator  $I_{reg}$ .

The present invention utilizes a variable-resistance type transducer 6, such as a strain gauge, having a total resistance  $R_g$ . The resistance  $R_g$  comprises a fundamental resistance  $R$  in series with a variable resistance  $\Delta R$  which represents the change in the transducer resistance resulting from the parameter measured by the transducer (stress, strain, etc.). Dissimilar metals (e.g., chromel, alumel, etc.) are used in output sensing wires 14 and 16 and they function as a thermocouple. Wires 12 and 18, which carry excitation current, are also implemented with dissimilar metals which are typically (but not necessarily) of the same material as wires 14 and 16, respectively. The voltage or electromagnetic force (emf) generated from the connection of sensing wire 14 to transducer 6 is represented by  $V_{1a}$ , whereas the voltage generated from the connection of sensing wire 16 to transducer 6 is represented by  $V_{1b}$ . The polarities of these voltages are dependent on the juxtaposition of the dissimilar metals. In order to generate voltages  $V_{1a}$  and  $V_{1b}$ , there must be a temperature gradient along sensing wires 14 and 16. By the law of intermediate metals, the connections to



transducer 6 do not change the net thermoelectric voltage as long as the connections remain at the same temperature. This same law permits thermally contacting thermocouple conductors to a third material without introducing error voltages as long as the third material has the same temperature at both contact points. Herein, the ends of wires 12, 14, 16 and 18 remote from transducer 6 are kept at the same temperature by isothermal reference area 20. In Fig. 2a, the four wires extending to the right of area 20 (and proceeding to switches S1 and S4) are typically copper. The temperature of isothermal reference area 20 is measured by a conventional temperature transducer (not shown) to enable the calibration of the thermocouple wires.

An indication of the sensitivity of the resistance measurement system of the present invention may be obtained by introducing a known change in calibration resistance  $\Delta R_{cal}$ . To introduce the known change in calibration resistance, a calibration resistor  $R_{cal}$  is connected via single pole single throw (SPST) switch S2 in parallel with reference resistor  $R_{ref}$ . Both calibration resistor  $R_{cal}$  and reference resistor  $R_{ref}$  are fixed resistors in a controllable environment. The known change in calibration resistance  $\Delta R_{cal}$  can be represented by the following equation:

$$\Delta R_{cal} = R_{ref} - [ (R_{ref})(R_{cal}) / (R_{ref} + R_{cal}) ] \quad (1)$$

This calibration method introduces a known change in resistance similar to the unknown change in resistance  $\Delta R$  of transducer resistance  $R_g$ . That is, during this calibration method,  $\Delta R$  equals half of  $\Delta R_{cal}$ . Since current  $I$  is regulated to be constant by current regulator  $I_{reg}$ , the calibration output magnitude is not a function of transducer resistance  $R_g$  or any parasitic resistances such as resistances  $R_{w1}$  or  $R_{w2}$  in circuit

loop 11. Thus, the overall sensitivity of the measurement system to resistance change is calibrated as a function of the change of transducer resistance  $\Delta R$  which equals  $\Delta R_{cal}/2$ .

In order to achieve the required measurements, constant current  
 5 I generated by current regulator  $I_{reg}$  which flows through transducer resistance  $R_g$  is periodically reversed as currents  $I_a$  and  $I_b$  by switch S1. Switch S1 is switched from position a to position b after a sufficient time period to obtain measured voltage  $V_a$ , and switched from position b to position a to obtain measured voltage  $V_b$ . Switch S1 may be, for  
 10 example, a conventional double pole, double throw switch implemented by field effect transistor switches. Accordingly, two separate outputs are obtained responsive to the position of switch S1; measured voltage  $V_a$  when switch S1 is in position a, and measured voltage  $V_b$  when switch S1 is in position b. Measured voltages  $V_a$  and  $V_b$  are sensed in a  
 15 conventional high-impedance manner so that essentially no current is permitted to flow through thermocouple wires 14 and 16 and respective resistances  $R_{w3}$  and  $R_{w4}$ . Thus, there is essentially no voltage drop caused by current flowing through thermocouple wires 14 and 16 to be considered. Accordingly, when insignificant current is drawn while  
 20 measuring voltages  $V_a$  and  $V_b$ , the circuit equations are as follows:

$$V_a = + [(V_{1a}) + (V_{1b})] + I(R+\Delta R) \quad (2)$$

$$V_b = - [(V_{1a}) + (V_{1b})] + I(R+\Delta R) \quad (3)$$

25 In order to eliminate voltages  $V_{1a}$  and  $V_{1b}$  to determine the change in resistance  $\Delta R$ , equations (2) and (3) are added together and summed with  $-V_{ref}$  resulting in the following equation when  $R_{ref} = 2R$ :

$$V_a + V_b - V_{ref} = 2I (\Delta R) \quad (4)$$

which shows the resistance change  $\Delta R$  as a function of measured voltages  $V_a$ ,  $V_b$  and  $V_{ref}$ . In addition, transducer resistance change  $\Delta R$  is not a function of, or effected by, thermocouple wire resistances  $R_{w1}$  -  $R_{w4}$  or induced voltage sources  $V_{1a}$  and  $V_{1b}$ . Therefore, the indicated transducer resistance change  $\Delta R$  will not be influenced by thermoelectric or other induced voltage effects. Also, since current  $I$  is regulated to be constant by current regulator  $I_{reg}$ , measured voltages  $V_a$  and  $V_b$  and reference voltage  $V_{ref}$  are not influenced by any other resistances which may exist and cause undesirable voltage drops in the current loop. Further, any zero offset may be made arbitrarily small by choosing or adjusting reference resistor  $R_{ref}$  to a resistance value that approaches approximately twice the initial resistance value  $R$  of transducer resistance  $R_g$ .

In addition to the resistance change which may be derived and measured from the measuring system of the present invention, the thermoelectric voltage is also measured using thermocouple wires 14, and 16 which are, as indicated above, comprised of dissimilar alloys to generate a thermoelectric voltage when exposed to a temperature gradient. Thus, in order to determine the thermoelectric voltage, equations (1) and (2) are subtracted yielding the following equation:

$$V_a - V_b = 2(V_{1a} + V_{1b}) \quad (5)$$

25

Equation (5) derives the thermoelectric voltage from measured voltages  $V_a$  and  $V_b$ . Since the elements of the transducer model such as transducer resistance  $R_g$ , lead wire resistances  $R_{w1}$ - $R_{w4}$  do not appear in equation (5), the difference between the measured voltages  $V_a$  and  $V_b$

is not influenced by changes in the transducer or lead wire resistances. Note that equation (5) yields an output voltage which is twice the thermocouple output voltage between thermocouple wires 14 and 16. The transducer temperature is then determined from a thermocouple reference table utilizing the following known information: one half of the measured output voltage ( $V_a - V_b$ ), the measured temperature of isothermal reference over 20 and the specific alloys used in the thermocouple wires. One such thermocouple reference table is the International Practical Temperature Scale (IPTS)-68 developed by the National Bureau of Standards (NBS). This table is reproduced in the Temperature Handbook of the Complete Measurement and Control Handbooks of Encyclopedia generated by OMEGA Engineering, Inc. of Stamford, Connecticut.

In Fig. 2a, multiplexer S3 is employed to perform the arithmetic functions of equations (4) and (5). It produces output voltages  $V_o$  and  $V_{\Delta R}$  equal to  $(V_{1a} + V_{1b})$  and  $\Delta R$ , respectively, at terminals 28 and 29, respectively. Multiplexer S3 is a schematic depiction of a dual-signal flying capacitor multiplexer comprising many capacitors and switches. Voltage  $V_o$  is produced by two series-connected capacitors which are charged to  $V_a$  and  $V_b$ , respectively. The capacitors are connected in a polarity arrangement such that the voltage at terminals 28 is  $(V_a - V_b)$  which varies directly as  $(V_{1a} + V_{1b})$ . Voltage  $V_{\Delta R}$  is produced by three series-connected capacitors which are charged to  $V_a$ ,  $V_b$ , and  $V_{ref}$ , respectively. The capacitors are interconnected in such a manner that the output voltage at terminals 29 is  $(V_a + V_b - V_{ref})$  which varies directly as  $\Delta R$ . Thus,  $V_o$  is a direct function of  $(V_{1a} + V_{1b})$  and  $V_{\Delta R}$  is a direct function of  $\Delta R$ .

Fig. 2b depicts an alternate circuit for deriving voltages  $V_o$  and  $V_{\Delta R}$  with one transducer. In the circuit of Fig. 2b, multiplexer S3 is

utilized to perform only the sampling and holding of voltages  $V_a$  and  $V_b$ . The configuration of Fig. 2b transfers voltages from a floating input to a grounded output and achieves a lower noise floor at the cost of a few additional components. Integrated circuit instrumentation amplifiers  
5 40, 41, 42 and 43 are employed to perform the arithmetic functions of equations (4) and (5). The instrumentation amplifiers provide very high impedance at the input terminals, amplify with a selected gain, and deliver an output voltage referenced to the electrical potential of the reference terminal.

10           Amplifier 40 produces  $V_o$  by the subtraction of  $+V_b$  at its inverting input from  $+V_a$  at its non-inverting input. The reference terminal of amplifier 40 is connected to analog common. This arrangement produces  $(V_a - V_b)$  at terminals 28 which varies directly as  $(V_{1a} - V_{1b})$ . Voltage  $V_{\Delta R}$  is produced by amplifier 41. Amplifier 42  
15 inverts  $+V_b$  to produce  $-V_b$ . Capacitor  $C$  absorbs switching transients on  $V_{ref}$ . Amplifier 43 inverts to produce  $-V_{ref}$ . Amplifier 41 has  $+V_a$  connected to the non-inverting input,  $-V_b$  connected to the inverting input and  $-V_{ref}$  connected to the reference input. This arrangement produces  $(V_a + V_b - V_{ref})$  at terminals 29 which varies directly as  $\Delta R$ .  
20 Thus  $V_o$  is a direct function of  $(V_{1a} + V_{1b})$  and  $V_{\Delta R}$  is a direct function of  $\Delta R$ .

The flying capacitor multiplexer may, for example, utilize integrated circuit analog multiplexer switches using field effect transistors. These analog multiplexer switches are commercially  
25 available with drive circuitry all integrated into the same package, and can also accommodate voltage levels as high as 10 volts. Preferably, the switch leakage current should be under 10 nanoamperes (nA), the "on" resistance less than 1,000 $\Omega$ , and the common mode rejection ratio greater than 100dB. The capacitors in the S3 multiplexer should

5 nominally be 0.1 microfarad ( $\mu\text{F}$ ) with low dielectric leakage (such as metalized polypropylene film capacitors). The magnitude of the capacitance does not need to be either precise or stable since the only function of the capacitors is to transfer and store electrical charge with minimal loss. As the capacitors remain charged to nearly constant levels in operation, no significant current surges occur in the circuit and the signal-to-noise ratio is high.

10 Additionally, switching in dual-signal multiplexer S3 is synchronized so that none of the capacitors are connected to transducer resistance  $R_g$  or reference resistance  $R_{\text{ref}}$  during the time when electrical transients are generated when switch S1 reverses constant current I. This ensures that the capacitors are connected to steady-state voltages, thereby minimizing the errors caused by charge transfer between capacitors and assuring that a minimum of current flows  
15 through thermocouple wires 14 and 16 and resistances  $R_{w3}$  and  $R_{w4}$ . Thus, multiplexer S3 is able to add and subtract voltage drops typically from one to two volts across resistances ranging from 60 to 1,000 ohms with errors typically no greater than  $0.5\mu\text{V}$  using the above approach.

20 SPDT switch S4 makes it easy to determine the effects of unwanted noise (common mode voltages). Examples of paths for unwanted noise energy to enter transducer 6 and/or the circuit coupled thereto are electrostatic coupling, electromagnetic coupling and thermal gradients across material discontinuities causing additional thermally induced electrical potentials. Mechanical energy can also develop  
25 unwanted electrical effects by various means including changing the dimensions and thereby the inductance of a conductor carrying constant current and by changing the spacing between conductors acting as a capacitor holding a constant charge.

A direct indication of any effect on the measurement system caused by common mode voltages is obtained by activating switch S4. The closure results in the sensing of the voltage at one end of transducer 6 and avoids sensing potentials  $V_{1a}$  and  $V_{1b}$  and the voltage drop across transducer 6. Any resulting non-zero indication at terminals 28 or 29 is thus caused by either common mode rejection problems or a malfunctioning meter used to measure voltage at the output terminals 28 and 29.


Figure 3 is a schematic diagram of another embodiment of the present invention. In this embodiment three transducers are featured rather than one. Only six thermocouple wires 32, 33, 34, 35, 36 and 37 are needed for this system. Resistances  $R_{w1-w6}$  represent the parasitic resistances in the thermocouple wires. Thermocouple wires 33, 34, 35 and 36 couple the thermoelectric potentials to dual-signal multiplexers 22, 24 and 26, and line 39 couples voltage  $V_{ref}$  to the three multiplexers. Output voltages  $V_{01-03}$  are a function of the respective transducer temperatures and output voltages  $V_{\Delta R1}-V_{\Delta R3}$  are representative of the resistance changes in the respective transducers.

The many features and advantages of the invention are apparent from the detailed specification, and thus, it is intended by the appended claims to cover all such features and advantages of the invention which fall within the true spirit and scope of the invention. Further, since numerous modifications and variations will readily occur to those skilled in the art, it is not desired to limit the invention to the exact construction and operation illustrated and described, and accordingly, all suitable modifications and equivalents may be resorted to, falling within the scope of the invention.

ABSTRACT OF THE DISCLOSURE

5 A constant current loop measuring system measures a property including the temperature of a sensor responsive to an external condition being measured. The measuring system includes thermocouple conductors connected to the sensor, sensing first and second induced voltages responsive to the external condition. In addition, the measuring system includes a current generator and reversor generating a constant current, and supplying the constant current to the thermocouple conductors in forward and reverse directions generating first and second measured voltages, and a  
10 determining unit receiving the first and second measured voltages from the current generator and reversor, and determining the temperature of the sensor responsive to the first and second measured voltages.



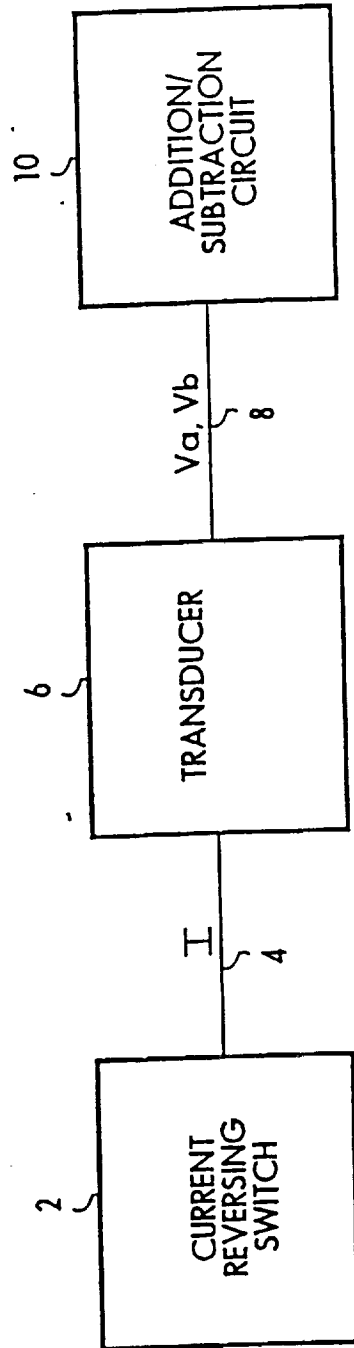

**Fig. 1**

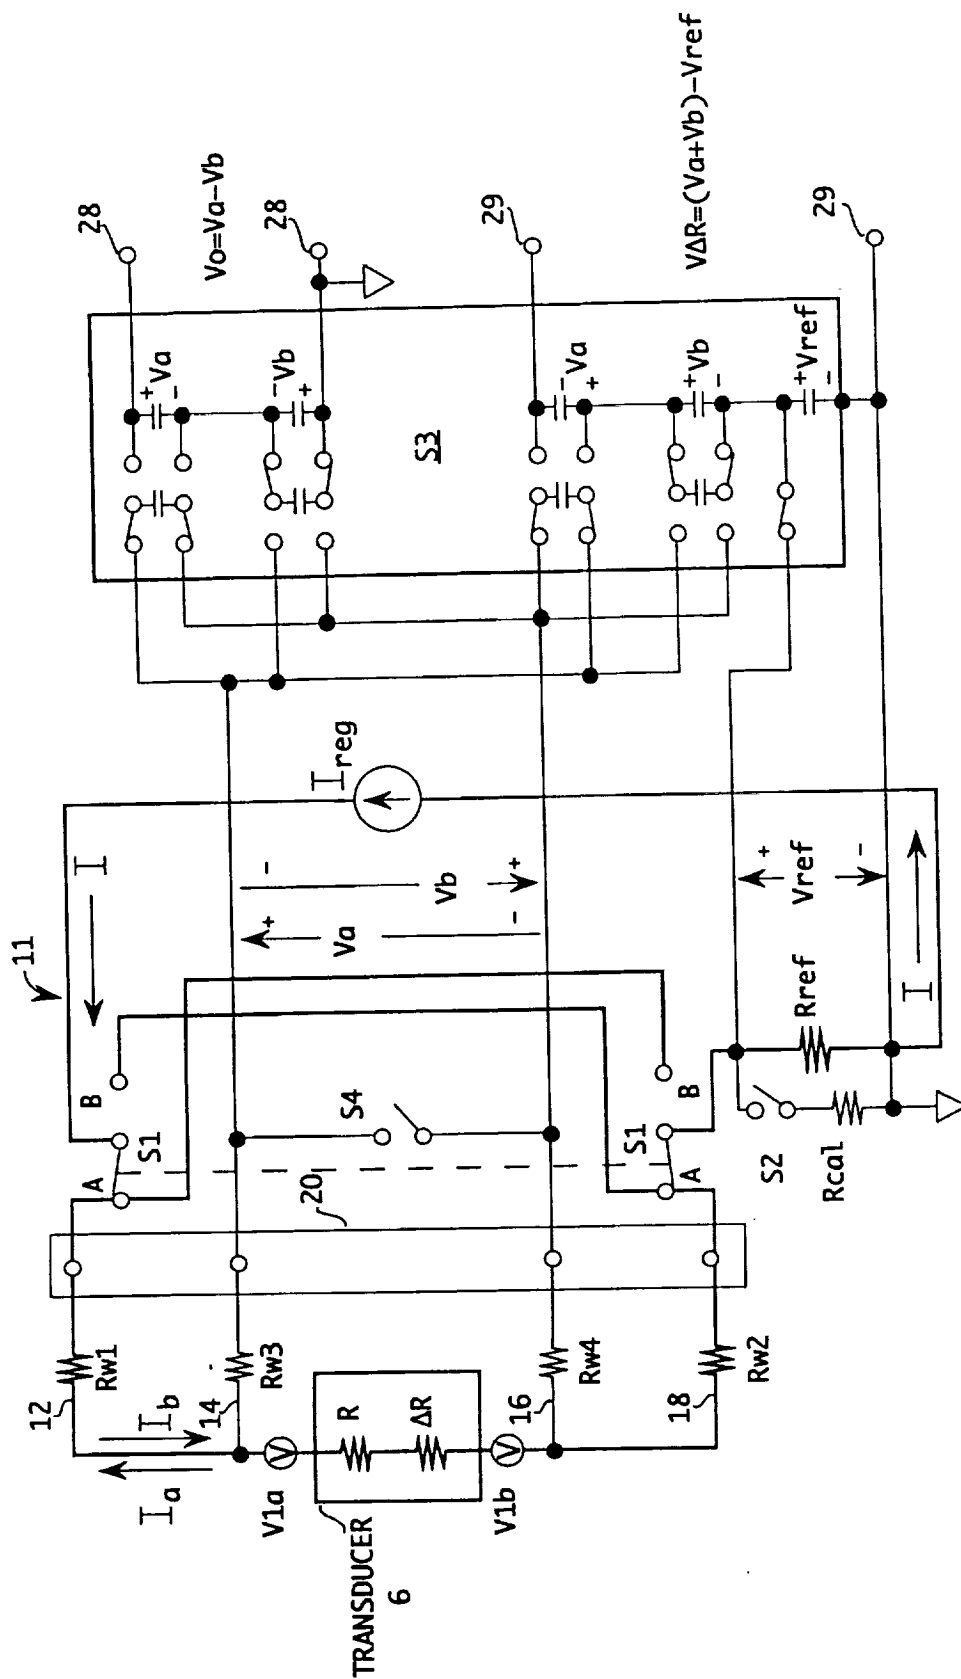


Fig. 2a

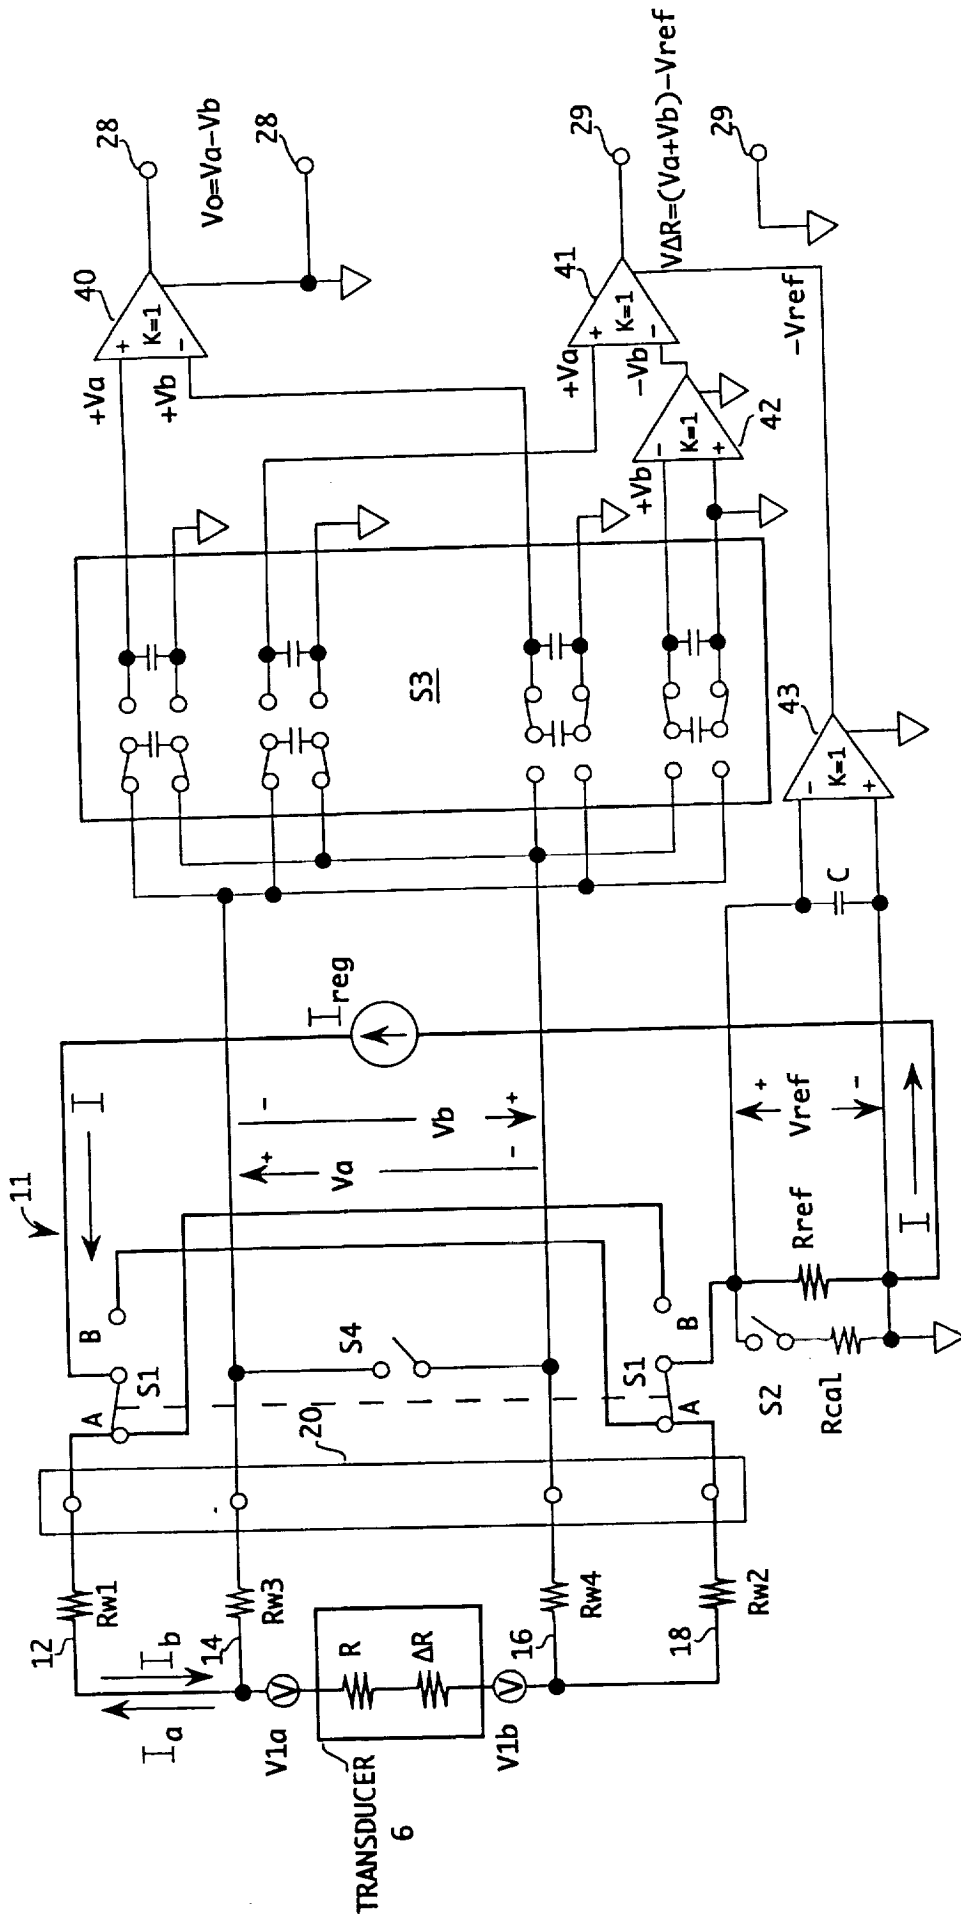


Fig. 2b

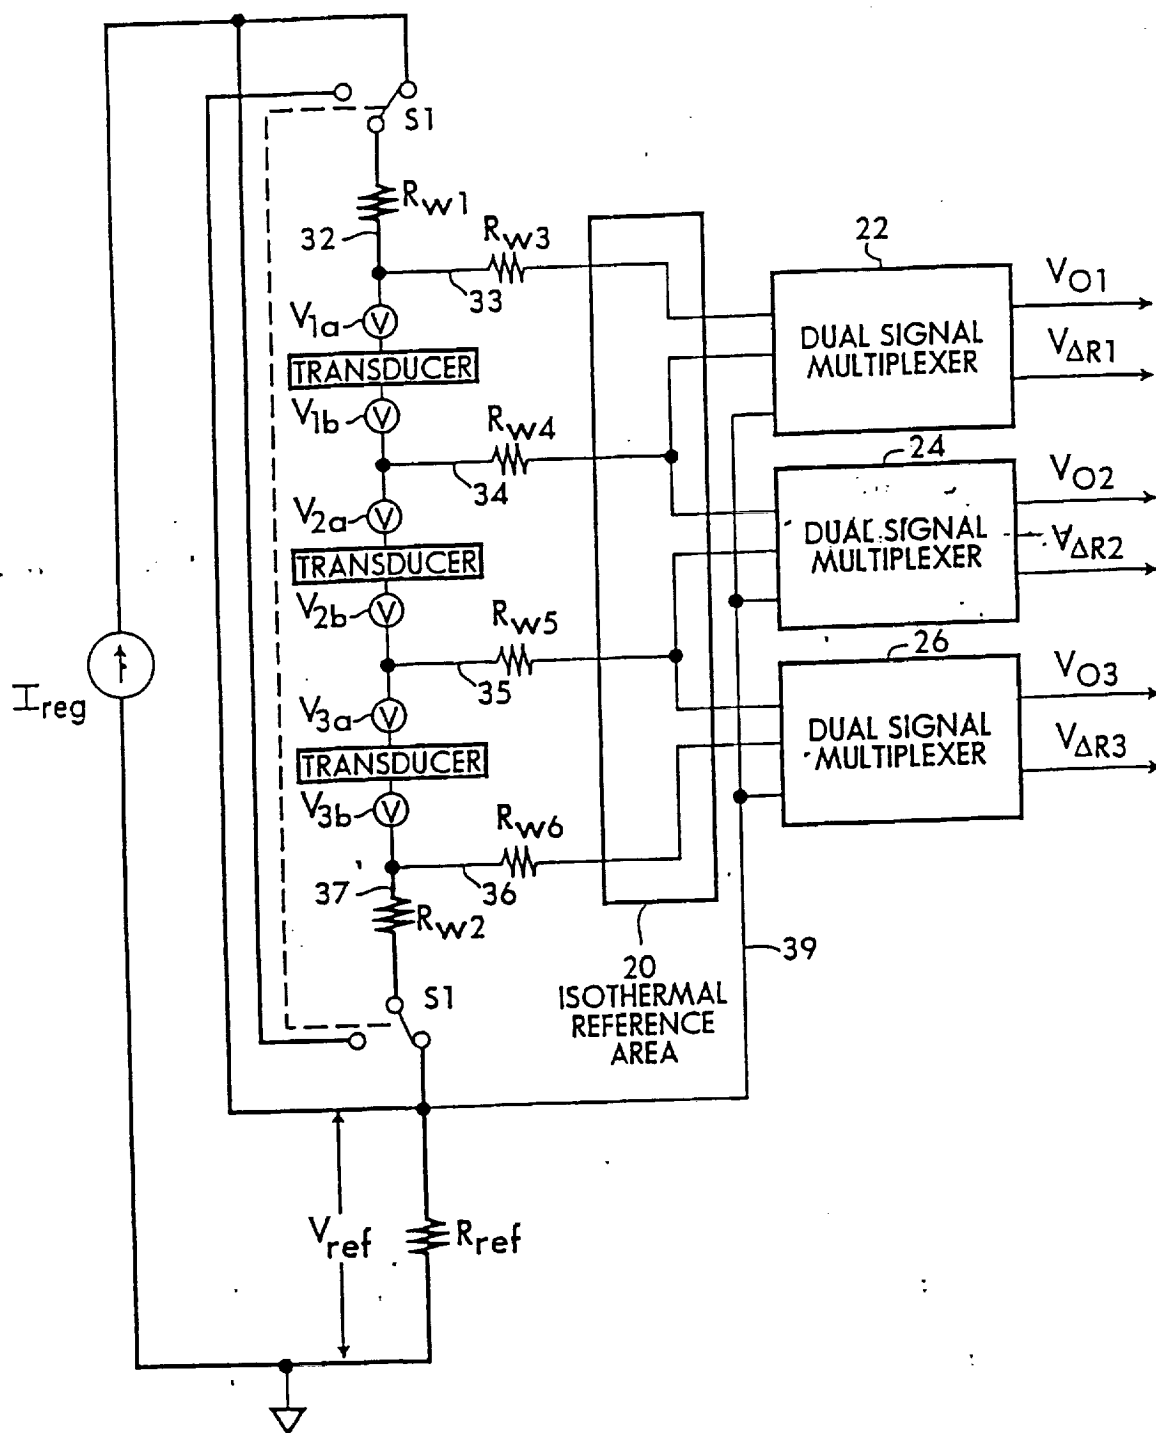


Fig. 3