

SOUTHWEST RESEARCH INSTITUTE

POST OFFICE DRAWER 28510 • 6220 CULEBRA ROAD • SAN ANTONIO, TEXAS, USA. 78228-0510 • (210) 684-5111 • TELEX 244846

NASA-CR-194832

MEMORANDUM

December 1, 1993

TO: Bill Johnson, NASA Wallops Space Flight Center

FROM: Jim Sharber and John Scherrer

SUBJECT: Interim Status Report, Contract NAG5-671 (SwRI Project 15-3822)

Handwritten notes:
11P
11P
11P

(NASA-CR-194832) [PULSAUR 2]
Interim Status Report (Southwest
Research Inst.) 11 p

INTRODUCTION

PULSAUR II is a sounding rocket experiment to investigate the pulsating aurora and related phenomena. The payload consists of a complementary set of instruments designed specifically to look at the pulsating aurora. The project will be managed by the Norwegian Space Center, with integration in Norway. The rocket is due for launch in January 1994 from the Andoya rocket range. Southwest Research Institute has been funded by Grant NAG5-671 to provide an electron sensor for this campaign. It is a "top-hat" electron spectrometer, referred to as AREA (Angle Resolving Energy Analyzer), and is based on the electron sensor developed for the CENTAUR mission.

ACCOMPLISHMENTS

Fabrication

Since the last report, final fabrication and assembly tasks were completed. This included conformal coating of all printed circuit boards, staking of all loose components and screws and final programming of the instrument. Figures 1 through 4 are photos of the completed packages. Figure 5 is a detailed photo showing the inside of the power supply box which provides regulated low voltage, microchannel plate bias voltage and the deflection plate sweep voltage.

After the mechanical parts of the sensor were machined, they were then coated with chem film and Aerodag. These parts, which included the inner and outer deflection plate, repelling grid, "top-hat" plate and miscellaneous stand-offs were sent to England for integration to the remaining sensor parts.

Correlator Checkout

A representative from the University of Sussex came to SwRI to support the integration and check-out of the correlator electronics. After approximately two weeks of debugging, the total system was working satisfactorily. The correlator electronics were then conformal coated and staked. Figure 6 is a photo of the correlator electronics.

N94-23484

Unclas

63/19 0201706

Sensor Checkout at MSSL

While the correlator was being tested here at SwRI, the sensor was being put through preliminary high voltage tests, noise tests and first order calibration at MSSL in England. Figure 7 and 8 are photos of the AREA sensor. During these preliminary noise checks, it was determined that there was a higher-than-expected background noise.

Sensor Checkout at SwRI

The bulk of the effort during this time period was spent trying to reduce the background count rate. This included replacement of the amplifier threshold resistors to decrease the instruments sensitivity, increasing the gap between high voltage areas, smoothing all sharp corners and points, and applying thick conformal coating to high voltage areas. This effort lowered the noise to a level which we could tolerate (see next section).

Checkout of the AREA instrument was performed at several levels: sensor only, one channel of the sensor with flight electronics with and without flight power supply, and full-up end-to-end system check with all flight electronics using the ground support equipment.

Calibration

The PULSAUR instrument calibration consisted of making detailed measurements of energy and angular resolution for a representative set of anodes, i.e. four anodes, located approximately 90° apart on the circular anode pattern. In addition, in order to determine the relative throughput factor of each of the 24 anodes, relative responses from each channel were measured. This was done by peaking the count in each channel in energy, theta, and phi for a given potential difference between the top-hat plates and recording the values. (Theta and phi are calibration reference angles and correspond to elevation and orthogonal-to-elevation angles on the rocket.)

The calibration measurements yielded results that compared very favorably with the simulation results of the MSSL group. The value of energy resolution for an energy angle scan run was typically 26% with very little variation at the four anodes measured. The deflection sensitivity (deflection constant) was typically 6.0 eV/V. The curves for the Anode 23 measurements are shown in Figure 9, which shows the three standard values of energy resolution ($\Delta E/E$) and deflection sensitivity.


An angular response measurement (phi) of this same anode (Figure 10) shows a value of 10.6° at the FWHM and a value of 18.0° at the 10% points. The angular response perpendicular to that one (theta) is determined primarily by the sector size of the anode, and is slightly less than 15°. This was confirmed by direct measurement as the instrument was rotated about its central axis.

Many anodes contained noise in excess of our expectations with noise levels between 30 and 2000 counts/sec. (The latter value is an extreme case, but most values were in the low hundreds. Also note that the count/sec is to be divided by 200 to obtain the count/accumulation period in the experiment.) Noise counts were recorded for all anodes at deflection voltages of 0, 1000, 2000, and 3000 V in order to be able to produce a "noise mask" for data analysis.

Integration at Norway


Following calibration, the instrument was sent to Norway for integration on to the sounding rocket. During integration, it was determined that in order for the AREA data stream to match the Norwegian telemetry stream, we were required to invert the AREA data and shift it by one half a clock pulse. The instrument was then sent back to SwRI for this purpose. After approximately two weeks, it was sent back to Norway where integration was successfully accomplished.

We are now awaiting launch in January of 1994.

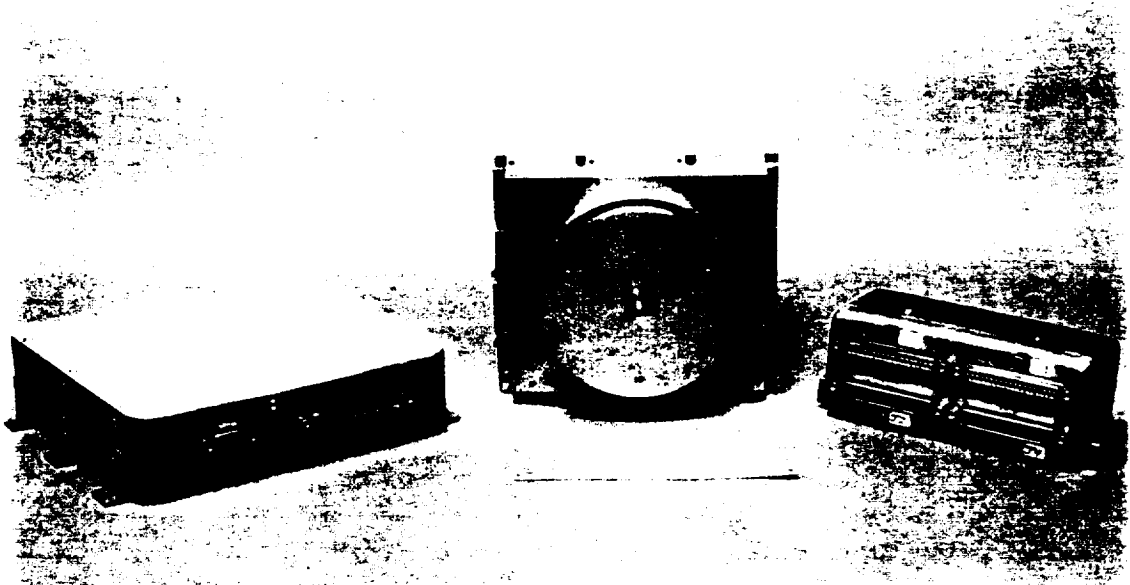


AREA POWER UNIT, SENSOR PACKAGE, AND JUNCTION BOX

Figure 1

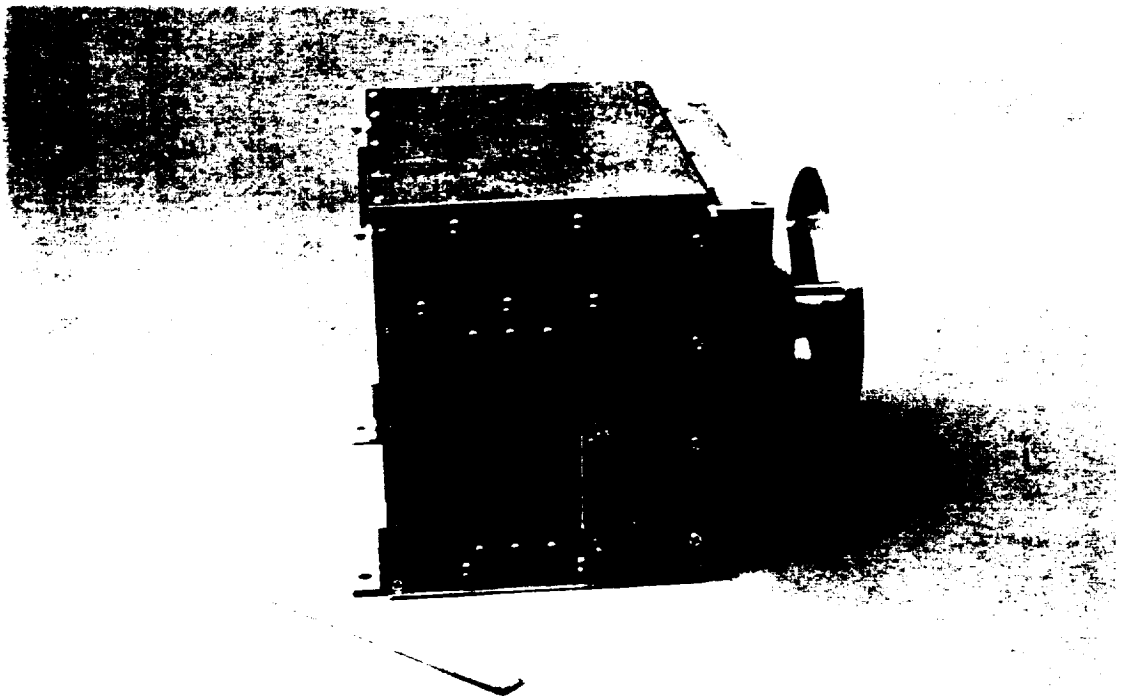


AREA SENSOR PACKAGE, CONTAINING DEFLECTION PLATES
AND DIGITAL ELECTRONICS

Figure 2

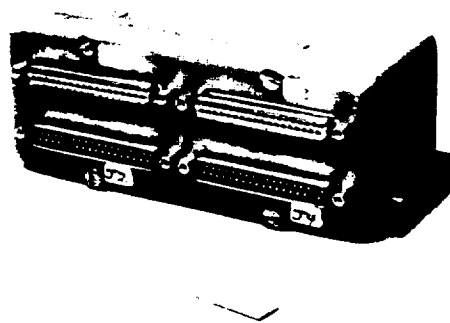

JUNCTION BOX

Figure 3

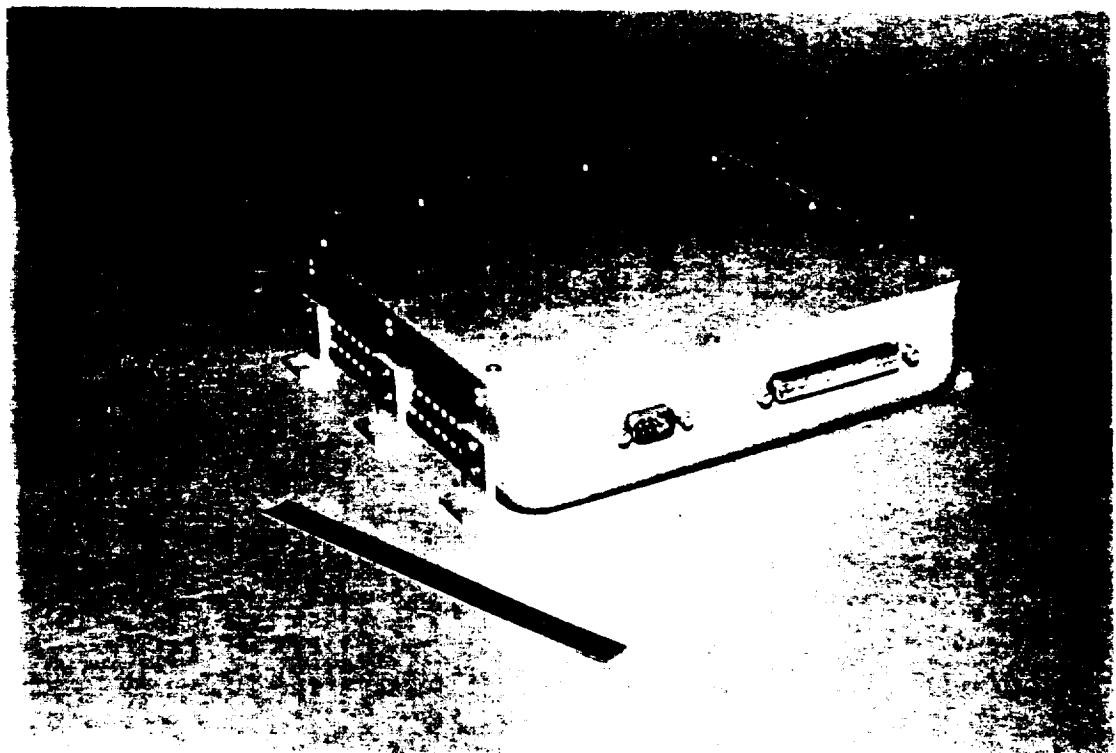

POWER UNIT

Figure 4

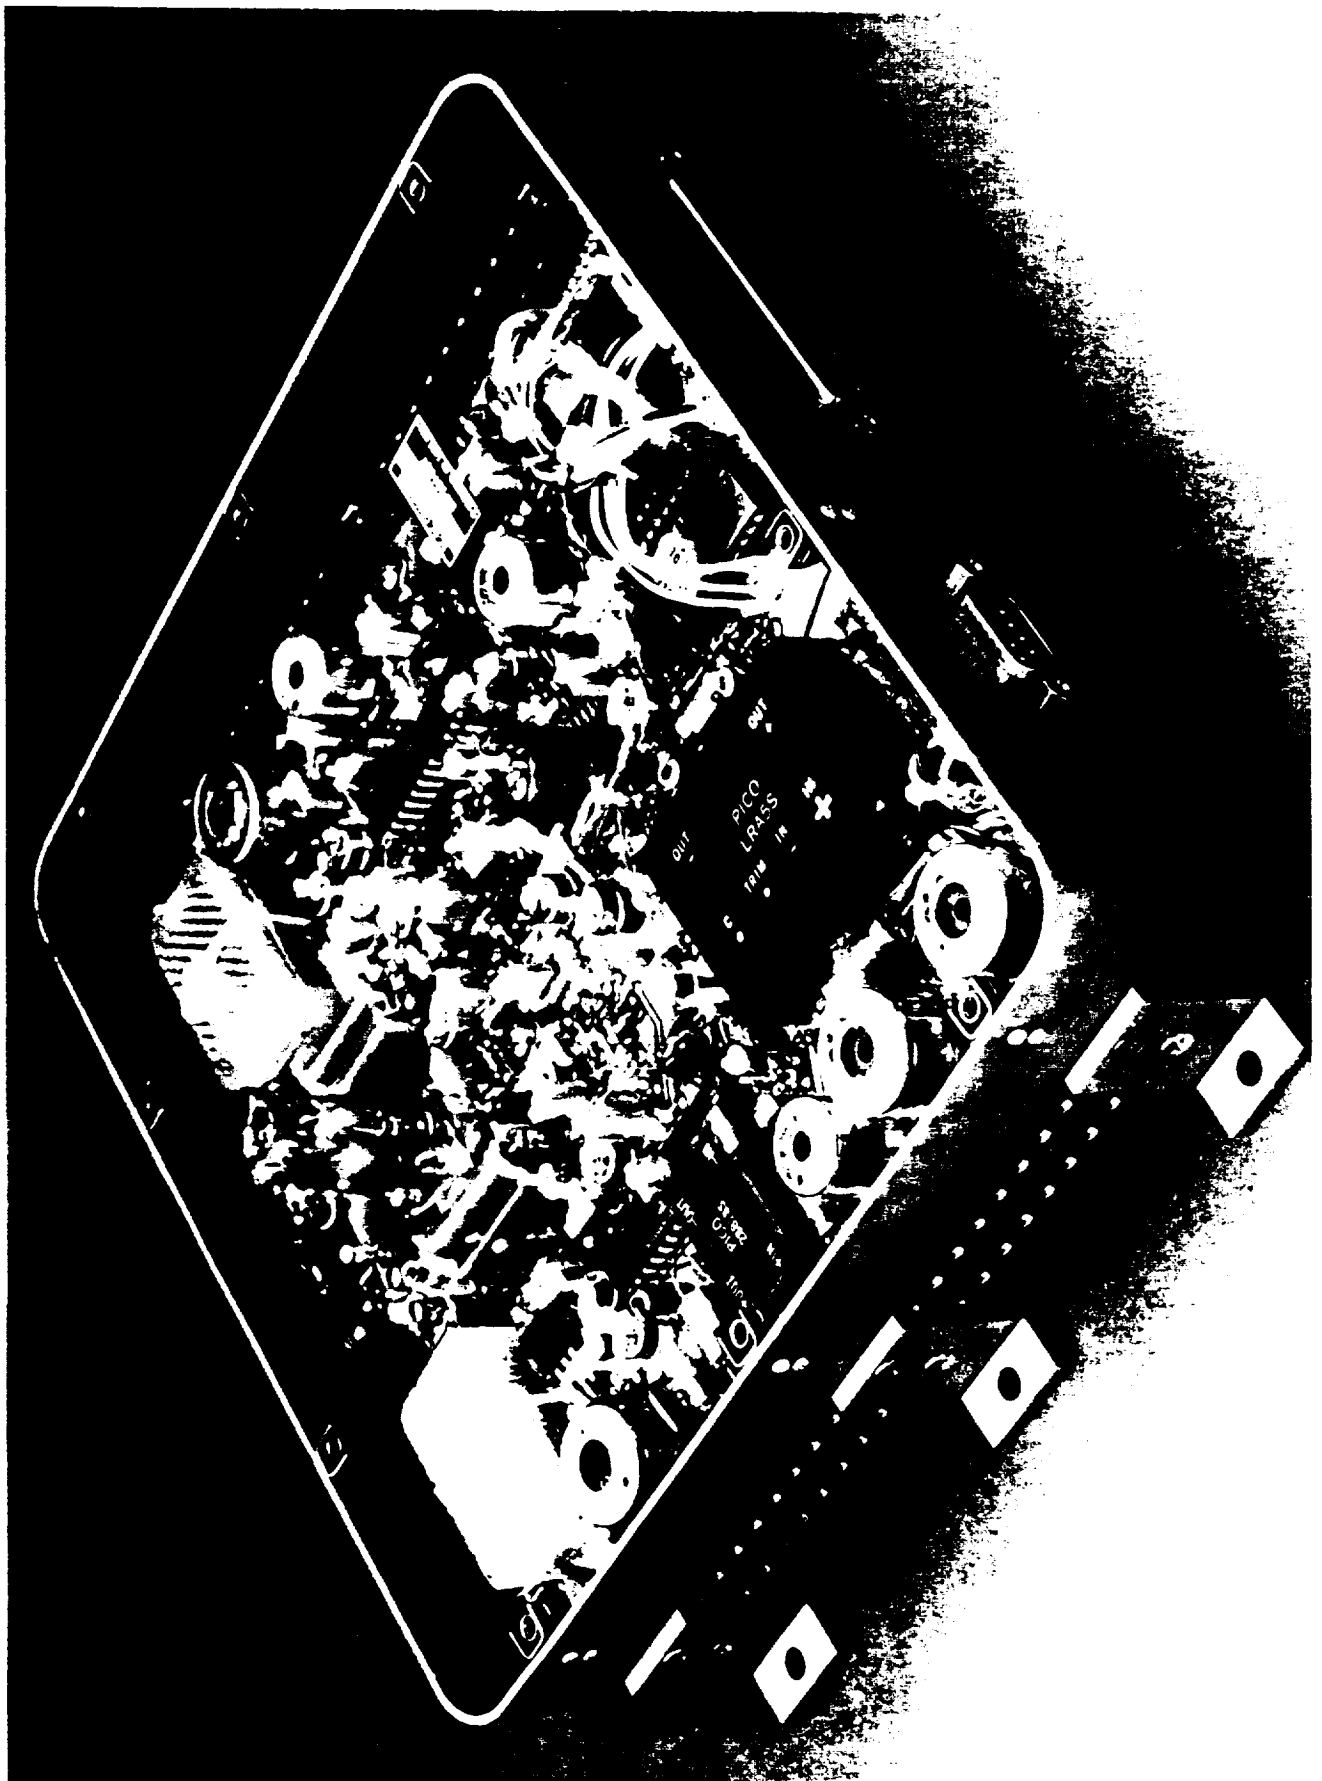


Figure 5. Pulsaur AREA
Power Supply

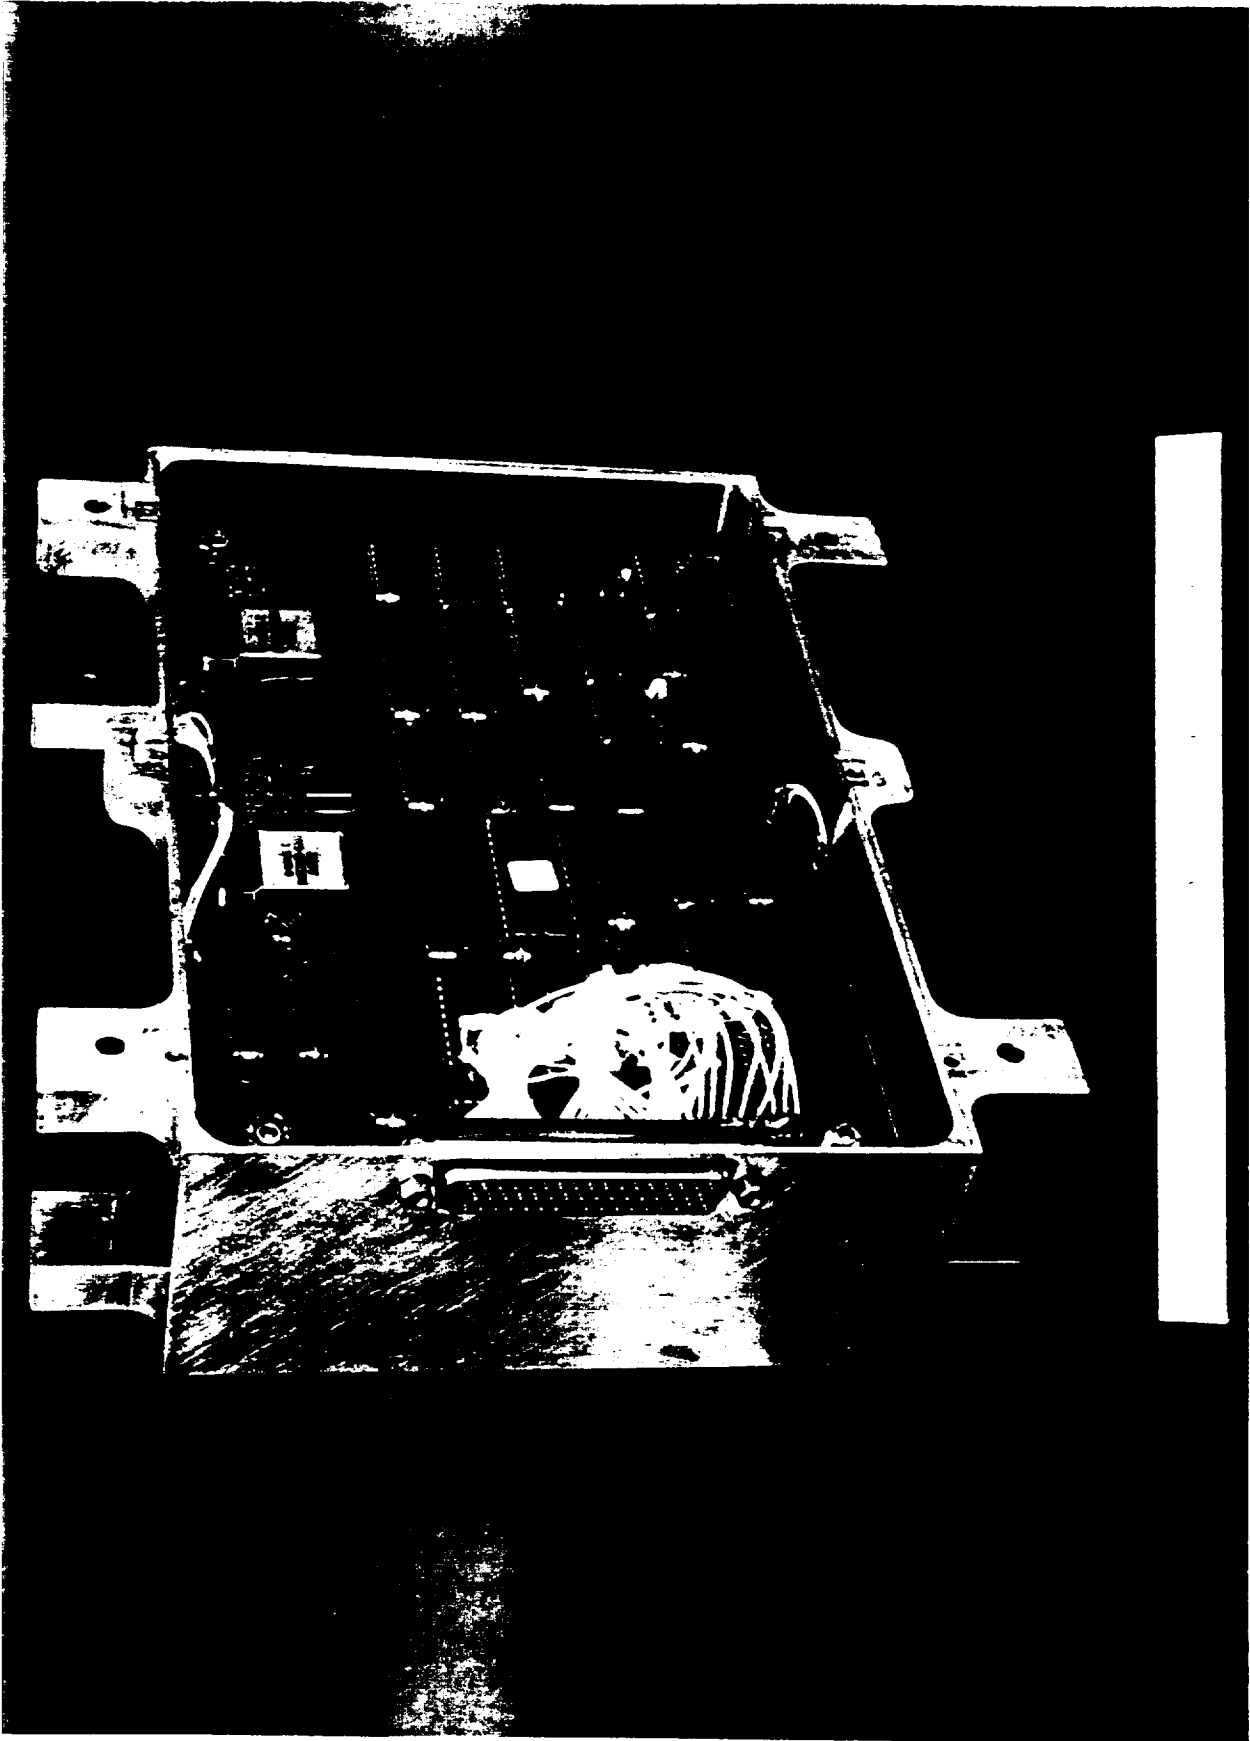


Figure 6. Pulsaur AREA
Correlator Electronics

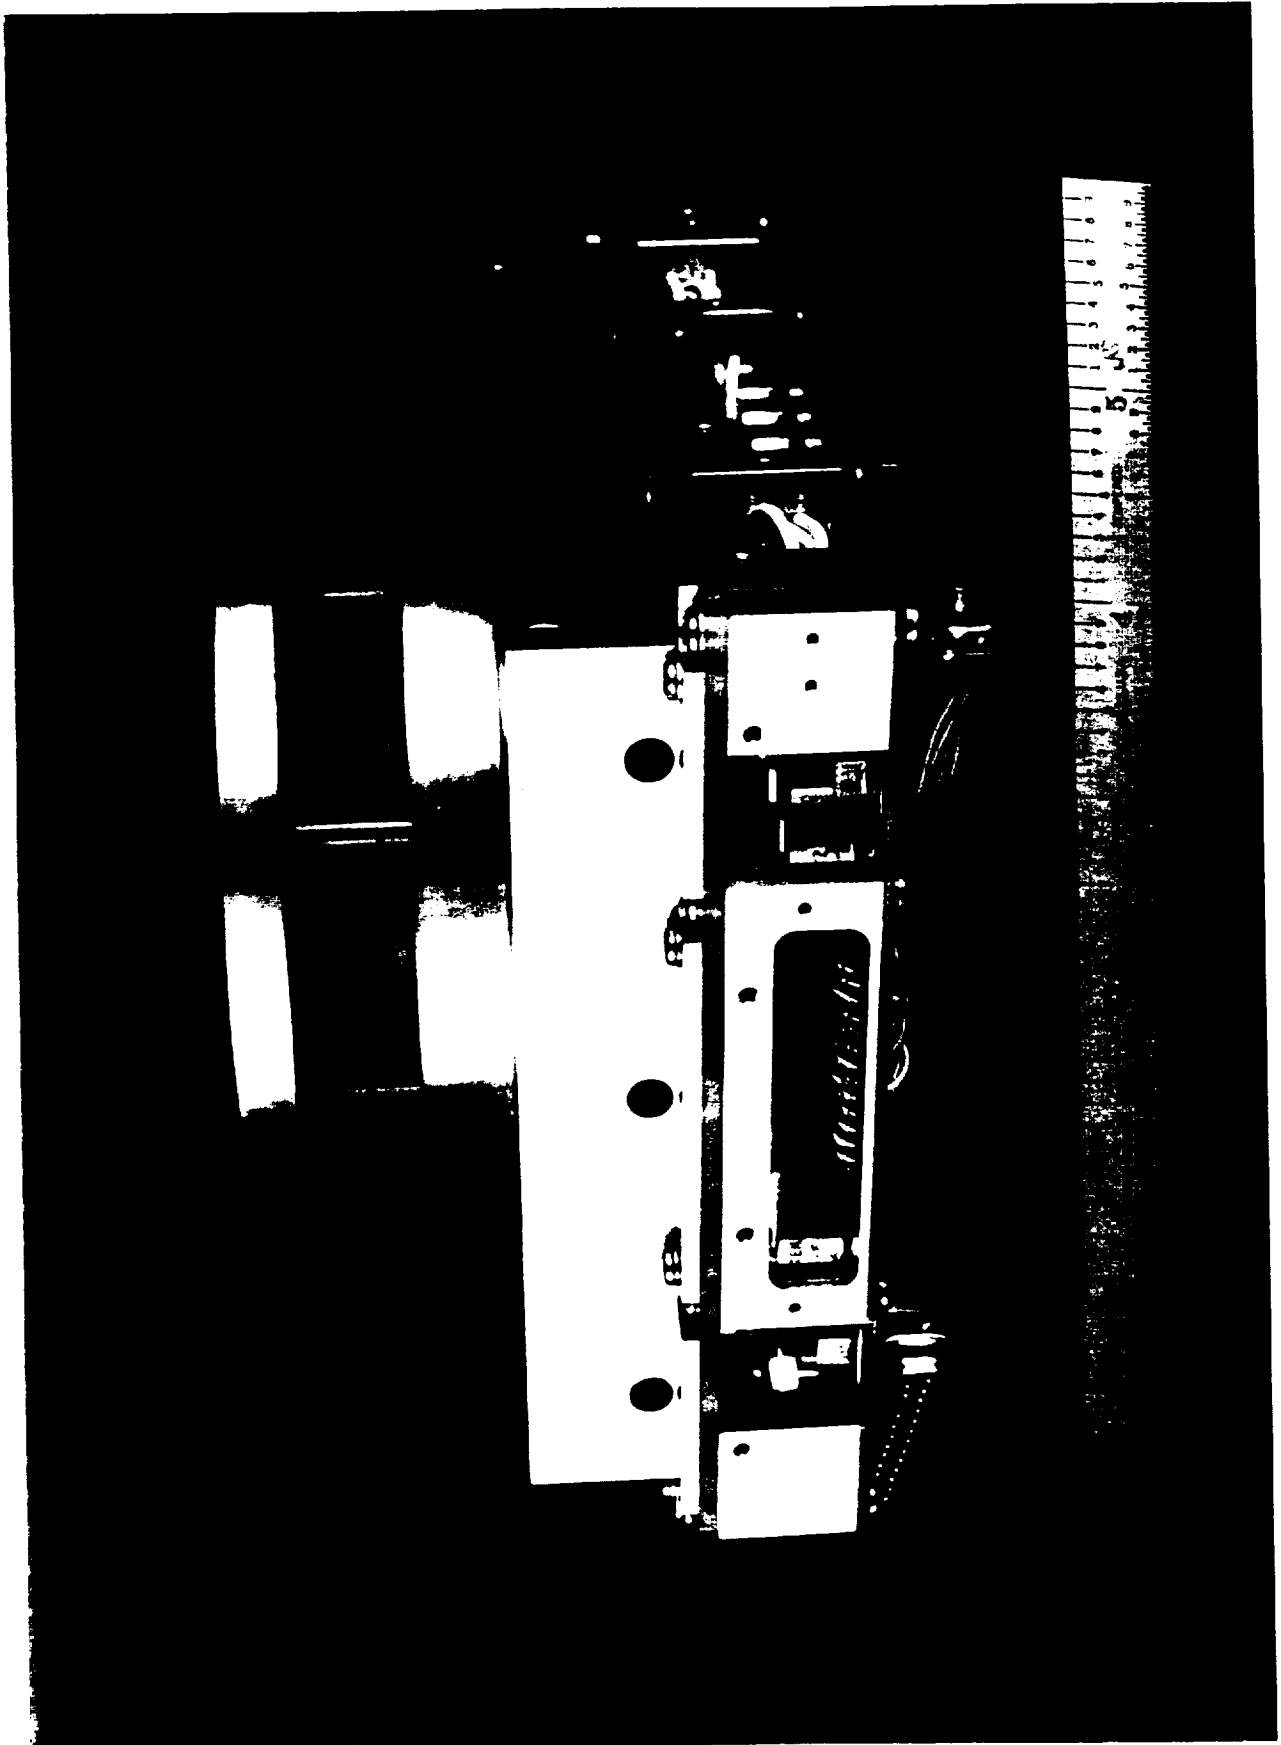


Figure 7. Pulsaur AREA Sensor

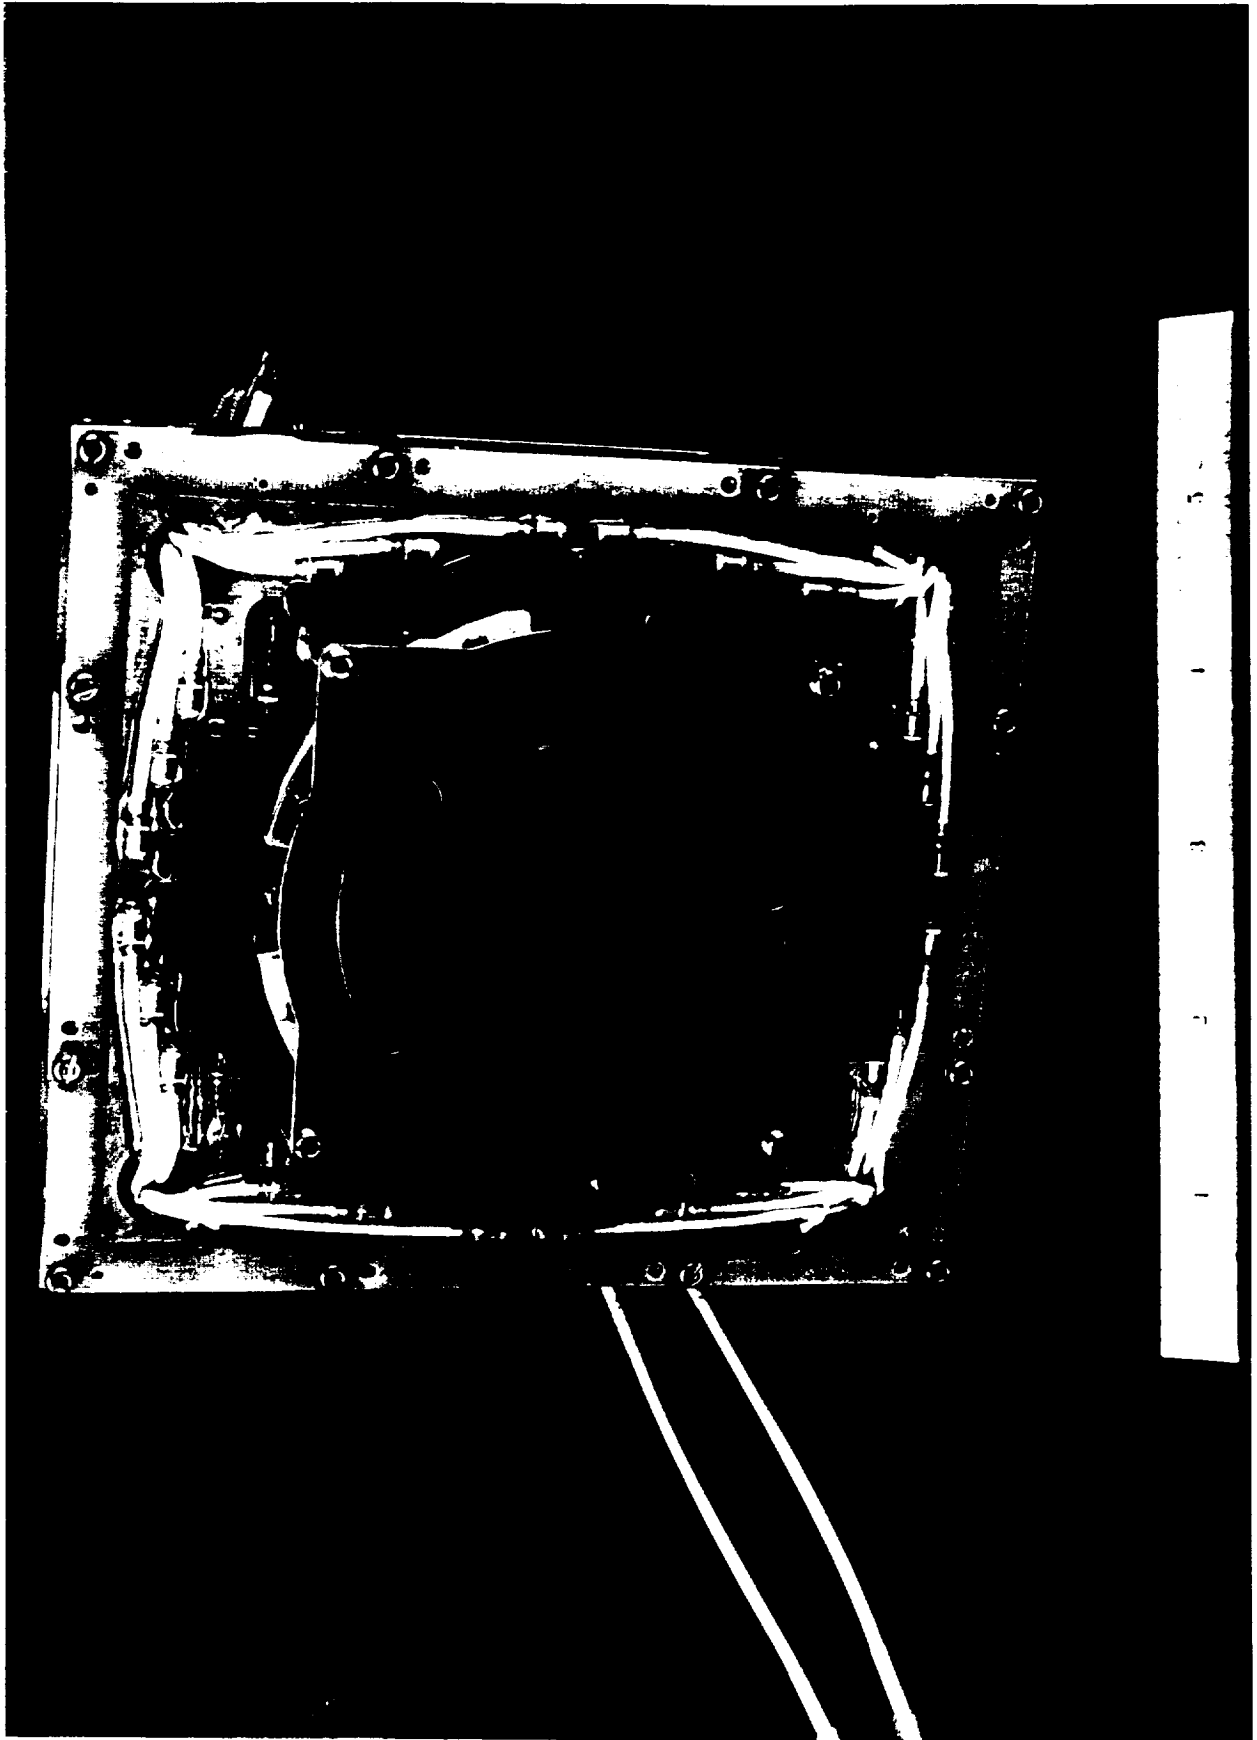


Figure 8. Pulsaur AREA Sensor
w/Outer Deflection
Plate Removed

ELECTRON BEAM ENERGY INTEGRATION

Plot # 1765.000
 Date Recorded: 93210
 Date Processed: 03-AUG-93
 Theta = 0.000

INSTRUMENT: 1-23

Voltage = 1000.000

Only graph data points used for these calculations:
 data integral: 1530546805.120

Arithmetic mean calculations

CR: 837270.055
 ELECTRON BEAM ENERGY : 6151.453
 ELECTRON BEAM ENERGY I: 5186.288
 Sensitivity: 6.151

Median calculations

CR: 880288.376
 ELECTRON BEAM ENERGY : 6056.781
 ELECTRON BEAM ENERGY I: 5204.190
 Sensitivity: 6.057

Most probable value calculations

CR: 927314.000
 ELECTRON BEAM ENERGY : 5896.430
 ELECTRON BEAM ENERGY I: 5223.879
 Sensitivity: 5.896

All data points used for these calculations:
 data integral: 1598841321.080

Arithmetic mean calculations

CR: 837608.699
 ELECTRON BEAM ENERGY : 6150.749
 ELECTRON BEAM ENERGY I: 5186.430
 Sensitivity: 6.151

Median calculations

CR: 881882.208
 ELECTRON BEAM ENERGY : 6052.980
 ELECTRON BEAM ENERGY I: 5204.854
 Sensitivity: 6.053

Most probable value calculations

CR: 927314.000
 ELECTRON BEAM ENERGY : 5896.430
 ELECTRON BEAM ENERGY I: 5223.877
 Sensitivity: 5.896

CR/2: 418635.027
 FWHM: 1667.953
 ELECTRON BEAM ENERGY U: 6854.242
 Resolution: 0.271

CR/2: 440144.188
 FWHM: 1609.993
 ELECTRON BEAM ENERGY U: 6814.183
 Resolution: 0.266

CR/2: 463657.000
 FWHM: 1548.234
 ELECTRON BEAM ENERGY U: 6772.113
 Resolution: 0.263

CR/2: 418804.349
 FWHM: 1667.491
 ELECTRON BEAM ENERGY U: 6853.921
 Resolution: 0.271

CR/2: 440941.104
 FWHM: 1607.874
 ELECTRON BEAM ENERGY U: 6812.728
 Resolution: 0.266

CR/2: 463657.000
 FWHM: 1548.236
 ELECTRON BEAM ENERGY U: 6772.113
 Resolution: 0.263

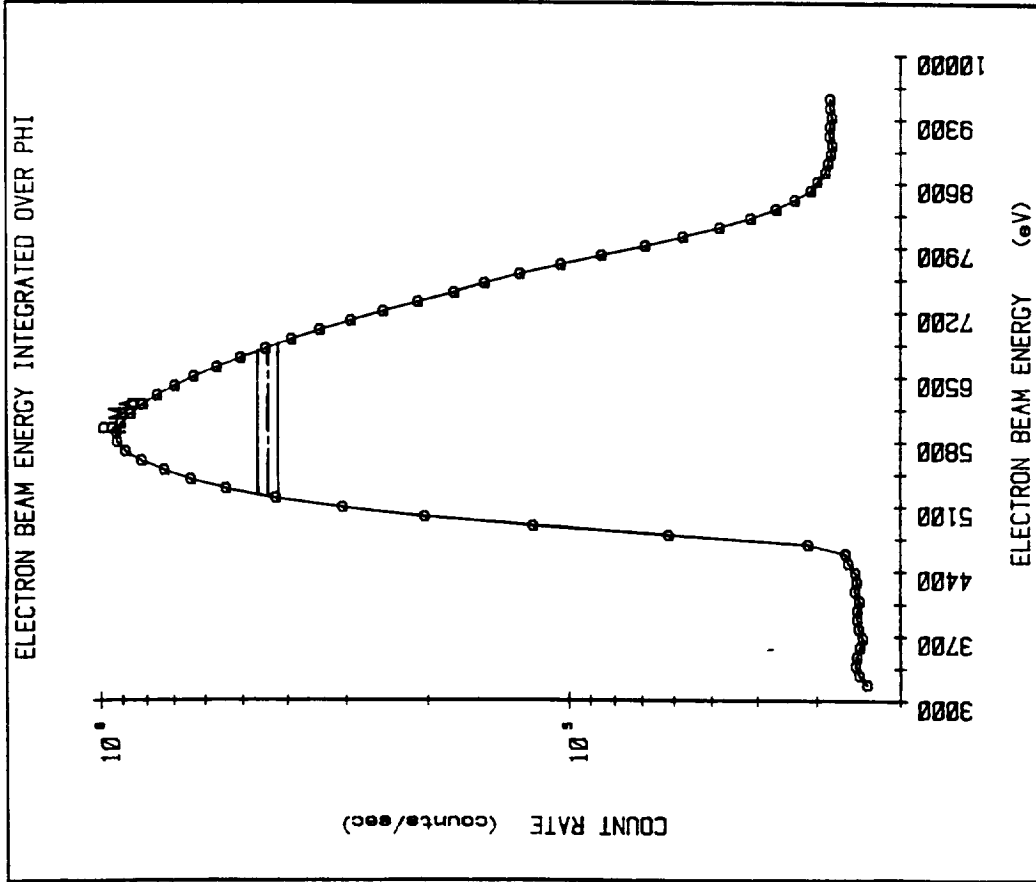


Figure 9. Energy Response and Deflection Sensitivity Measurements -- Anode 23

PHI INTEGRATION

Plot # 1766.00
 Date Recorded 93210
 Date Processed 03-AUG-93
 Theta = 0.00

INSTRUMENT: 1-23
 Voltage = 1000.00

Only graph data points used for these calculations:

Single least squares line calculations
 $Y = (-68996.60)X + (725649.54)$ Coeff. of determination: 0.99
 Data integral: 7627452.19 Line integral: 5797620.38
 FWHM: 10.58 PHI peak: -0.06 CR: 729827.07
 PHI 1: -5.35 PHI 2: 5.23 CR/2: 364913.54
 Arithmetic mean: -0.15

Split least squares calculations
 left line calculations
 $Y = (66499.50)X + (720395.83)$ Coeff. of determination: 0.99
 Data integral: 3501574.40 Line integral: 3029629.02
 FWHM: -5.39 PHI peak: -0.06 CR: 716369.49
 PHI 1: -5.45 PHI 2: -0.06 CR/2: 358184.75
 right line calculations
 $Y = (-71897.92)X + (739299.31)$ Coeff. of determination: 0.98
 Data integral: 3791526.30 Line integral: 2803341.67
 FWHM: 5.17 PHI peak: -0.06 CR: 743652.51
 PHI 1: -0.06 PHI 2: 5.11 CR/2: 371826.25

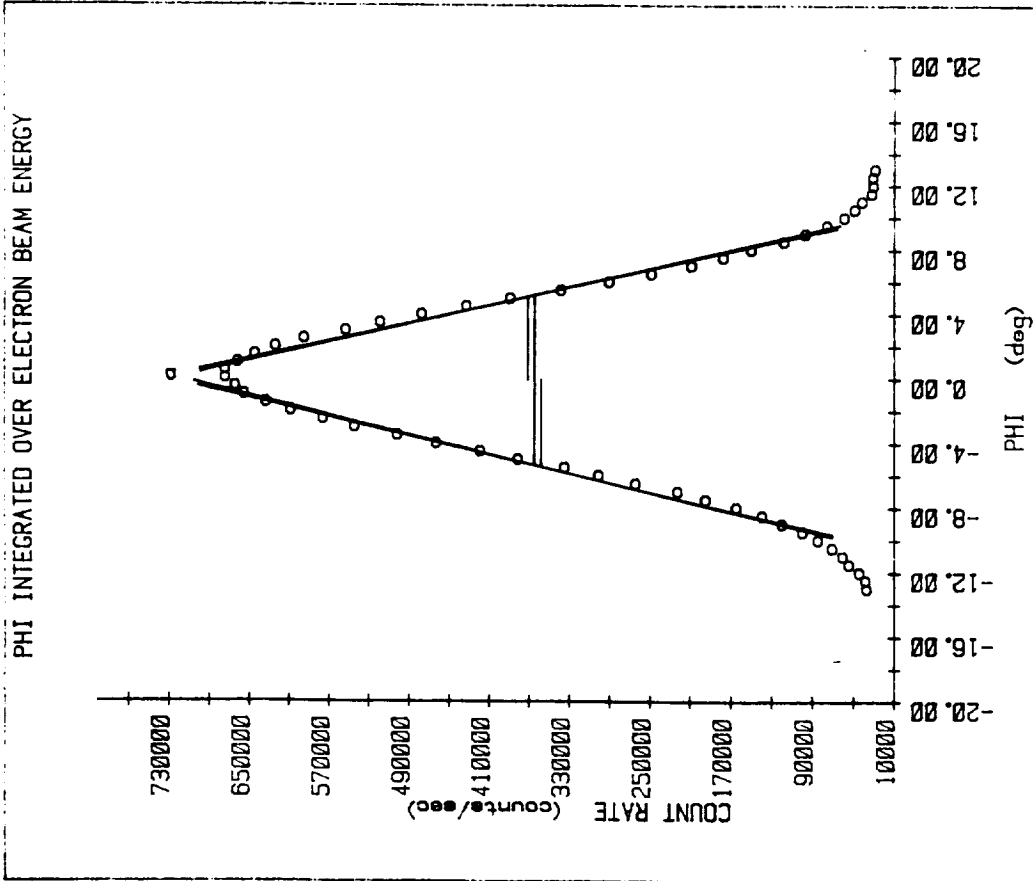


Figure 10. Angular Response in Phi -- Anode 23