

1st World Congress on Ga-68 and Peptide Receptor Radionuclide Therapy, THERANOSTICS,
Bad Berka, Germany June 23-26, 2011

P-023

Development of ⁶⁸Ge/⁶⁸Ga Generator at ANSTO

Van So Le*, Michael Izard, Paul Pellegrini and Myint Zaw

ANSTO LifeSciences, Australian Nuclear Science and Technology Organisation
Locked Bag 2001 Kirrawee DC, NSW, 2232, Australia

* E-mail: slv@ansto.gov.au

A ⁶⁸Ge/⁶⁸Ga generator combined with an automated ⁶⁸Ga eluate purification unit was developed to produce ⁶⁸Ga solution suitable for labelling peptide ligands for PET radiopharmaceutical applications. The sorbent of a Ti-Zr ceramic structure [1] was used as a generator column packing material. The SEM picture of micro- and mesoporosity of these materials is shown in Figure 1a. Its X-ray diffraction presents a tetragonal nano-crystalline structure.

The adsorption capacity for Ge⁴⁺ ions is approximately 120 mg Ge per gram sorbent in 0.1 M HCl solution. The distribution coefficient K_d > 10000 mL/g for carrier-free ⁶⁸Ge⁴⁺ ions and 2 mL/g for ⁶⁸Ga³⁺ were evaluated in 0.1 M HCl solution. A 1.0 g weight sorbent column was used for immobilizing the parent nuclide ⁶⁸Ge and ⁶⁸Ga was eluted from the column with 3- 4 mL 0.05 – 0.1 M HCl solution. The ⁶⁸Ge breakthrough in ⁶⁸Ga eluate was around 10⁻³ % for a generator of 18 mCi ⁶⁸Ge activity.

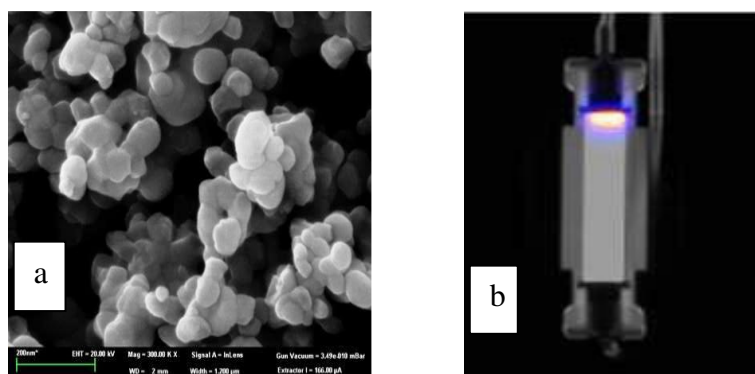


Figure 1. (a) SEM picture of Ti-Zr ceramic sorbent used for loading ⁶⁸Ge/⁶⁸Ga generator column; (b) PET imaging of the ⁶⁸Ge/⁶⁸Ga generator column after 300 ⁶⁸Ga elution cycles

The PET imaging picture of the ⁶⁸Ga generator column after 300 elution cycles (Figure 1b) showed no significant spreading and drift of ⁶⁸Ge zone along the column. ⁶⁸Ga eluate of around 5 mL volume in 0.1 M HCl solution was purified on a small cation exchanger column with an aqueous alcohol solution mixture of hydrochloric acid, ascorbic acids and halide salts. An alkali solution was used for elution of ⁶⁸Ga from the ion exchange resin column to obtain a purified ⁶⁸Ga solution which is conditioned with acidic solution to obtain a final ⁶⁸Ga product of pH=3-4 in 0.75 mL

0.5 M NaCl or 0.5 M sodium acetate solution. The metallic contamination <20 nano grams per mL were found in this product solution. The organic solvent free ^{68}Ga solution product of acidity suitable for coordination chemistry based labelling of the peptide ligands was successfully used for preparation of DOTATATE and DOTATOC PET radiopharmaceuticals.

The process of ^{68}Ga elution from the generator followed by ^{68}Ga eluate purification was performed using a low-cost automation bench-top system [2]. This system is designed (Fig. 2) based on the timing sequence of seven processing steps without feedback control. The variable flow rate of eluents used for elution/purification in this system also ensure the optimisation of operating times with respect to different adsorption/ desorption kinetics of ^{68}Ga ion species, which is controlled by the sorbent and ion exchange resin used in the generator and purification columns.



Figure 1: ^{68}Ga generator (housed in the lead container in the lower part of the system) and processing unit with the eluents for ^{68}Ga eluate purification (in the upper part) together with a control unit at the bottom right.

References

1. Van So Le, Sorbent material, Patent, PCT/AU2011/000245
2. Van So Le, ^{68}Ga Gallium purification, Patent, PCT/AU2011/000244