

Meeting abstract

141 Volumetric cardiac quantification using three dimensional dual phase whole heart MRI

Sergio A Uribe Arancibia*, Tarinee Tangchaoren, Victoria Parish, Ivo Wolf, Reza Razavi, Gerald Greil and Tobias Schaeffter

Address: King's College London, Division of Imaging Sciences, London, UK

* Corresponding author

from 11th Annual SCMR Scientific Sessions
Los Angeles, CA, USA. 1–3 February 2008

Published: 22 October 2008

Journal of Cardiovascular Magnetic Resonance 2008, **10**(Suppl 1):A42 doi:10.1186/1532-429X-10-S1-A42This abstract is available from: <http://jcmr-online.com/content/10/S1/A42>

© 2008 Arancibia et al; licensee BioMed Central Ltd.

Introduction

Cardiac ventricular volumes are usually assessed using Simpson's rule over short axis (SA) cines of the heart acquired during breath-holds. This technique is challenging for ill patients and segmentation is difficult due to non isotropic resolution. Recently, a new approach was proposed that calculates the ventricle volumes from two non-angulated isotropic cardiac scans of the whole heart (end-systolic, ES, and end-diastolic, ED) (1). However, this approach results in a relatively long overall scan time. To overcome this limitation we propose acquiring the two volumes in one free-breathing scan using quasi independent navigator beams for each cardiac phase. The aim of this study is to evaluate this new acquisition scheme and compare the EDV, ESV and stroke volumes (SV) obtained using this technique with the traditional multiple 2D (M2D) scans and with flow measurements.

Methods

3D dual phase acquisition scheme

A 3D triggering b-SSFP turbo field echo sequence was modified to enable the acquisition of two cardiac phases at a user defined time (Figure 1). The sequence was implemented on a 1.5 T Philips clinical scanner. A free breathing scan was realized by enabling one navigator beam before data acquisition for each cardiac phase. They were used to prospectively validate or invalidate acquired *k*-space data for each cardiac phase quasi independently.

Experiments

A prospective study was performed in ten patients and five healthy volunteers. EDV, ESV and SV were obtained and compared from the following imaging acquisitions, M2D SA cine, free breathing flow scans in the aorta and pulmonary artery and the new dual phase scan (imaging parameters are summarized in Table 1). The M2D and flow data were analyzed using commercially available software (Philips View forum). Analysis of the 3D data sets were performed using a semiautomatic segmentation [1,2]. Bland Altman analyses and T-test analyses were used to assess agreement between the measurements.

Table 1: Imaging parameters of MR scans

| Parameter | Multi slice 2D | 3D dual phase | Flow |
|---------------------|----------------|-----------------|---------------|
| FOV ** (FH-AP-RL*) | 390 × 255 × 96 | 280 × 240 × 140 | 300 × 270 |
| Acquired Resolution | 2 × 2 × 8 | 2 × 2 × 2 | 2.1 × 2.1 |
| TR/TE | 2.9/1.5 | 3.8/1.9 | 4.7/2.6 |
| TFE factor | 9 – 13 | 15–20 | 3 – 4 |
| Temporal Resolution | 30 ms | 60 ms | 20–40 ms |
| Nr cardiac Phases | 20–30 | 2 | 20–40 |
| Flip angle | 60 | 60 | 15 |
| Triggering modality | Retrospective | Trigger | Retrospective |
| Averages | 1 | 1 | 3 |

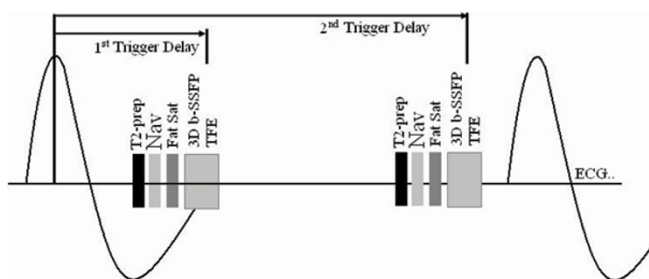


Figure 1
Sequence diagram of the 3D dual phase scan.

Results

3D dual cardiac phase scan

Reformatted slices in one volunteer are shown in Figure 2. The time of the 3D scan was $7:54 \pm 1:42$ [min:sec], with an scan-efficiency of $47\% \pm 7\%$ due to respiratory gating.

Statistical analysis

No statistical difference was found for the measured ESV and EDV comparing the 2D and 3D technique (see Bland-Altman plot in Figure 3). Bland-Altman plots of SV comparison of the 3D technique with flow measurements and with the M2D method are shown in Figure 4. It is noticeable that equivalent results were obtained for both ventricles for all approaches. Range and mean data from intra and inter observer variability using the 3D and the M2D method are shown in Table 2.

Conclusion

We have introduced an acquisition scheme that allows precise cardiac volume quantification in a single free breathing scan. The new 3D dual phase technique offers a series of advantages over the traditional M2D approach such as minimal scan planning, isotropic resolution and a good definition of the cardiac valves. Severely ill, sedated patients and those with congenital heart diseases may benefit from the proposed method, since it is a patient friendly scan and provides both morphological and cardiac volume information.

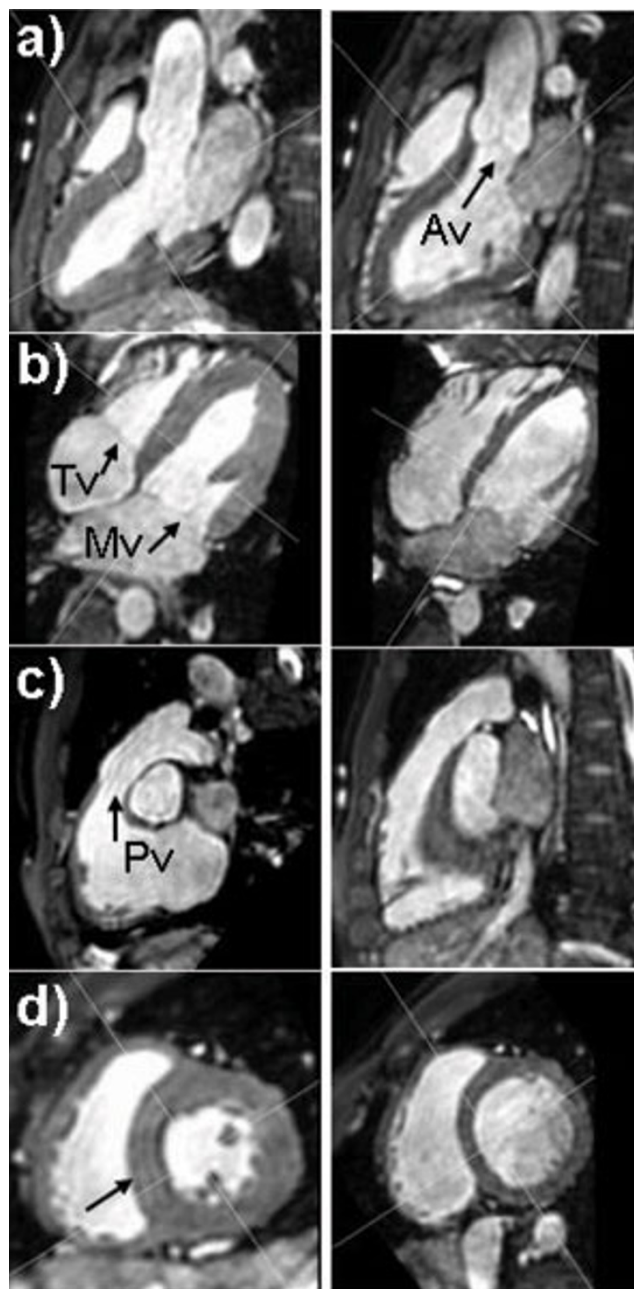


Figure 2
Reformatted images during systole (left) and diastole (right). Arrows show the definition of different valves (a, b, d) and myocardium (d).

Table 2: Intra and inter observer variability for the 3D and M2D method

| | Range | difference (%) | Mean | difference (%) |
|--------------------|---------------|----------------|------|----------------|
| | LV | RV | LV | RV |
| Intra observer 3D | [-7.3; 10.6] | [-7.0; 2.5] | 2.3 | -0.9 |
| Inter observer 3D | [-11.0; 12.5] | [-8.3; 17.7] | 3.6 | 6.0 |
| Intra observer M2D | [-30.9; 9.1] | [-12.2; 9.6] | -5.8 | -2.6 |
| Inter observer M2D | [-21.9; 8.3] | [-19.5; 9.8] | -5.3 | -5.5 |

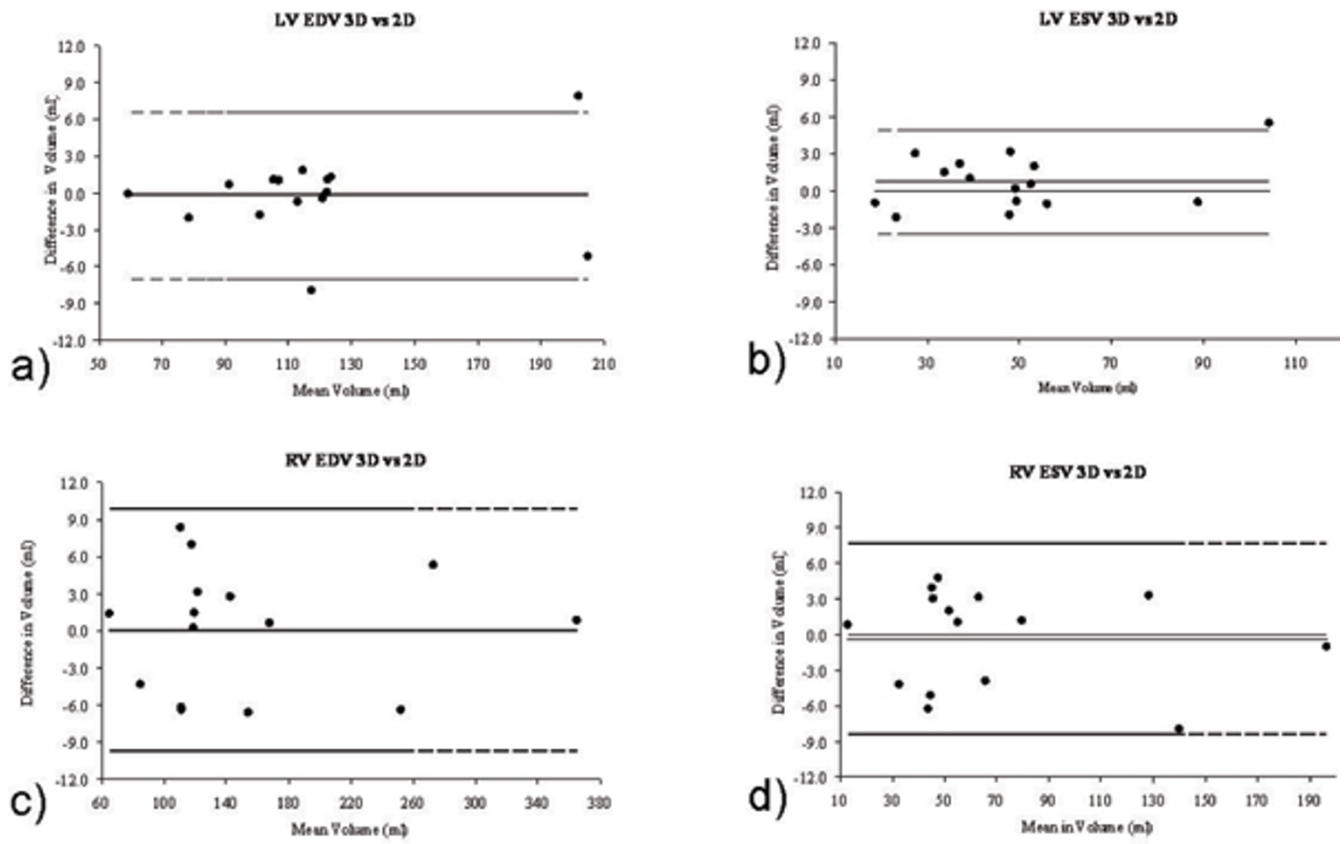


Figure 3
Comparison of EDV (a, c) and ESV (b, d) between the 3D and the M2D method for the LV (a, c) and RV (b, d).

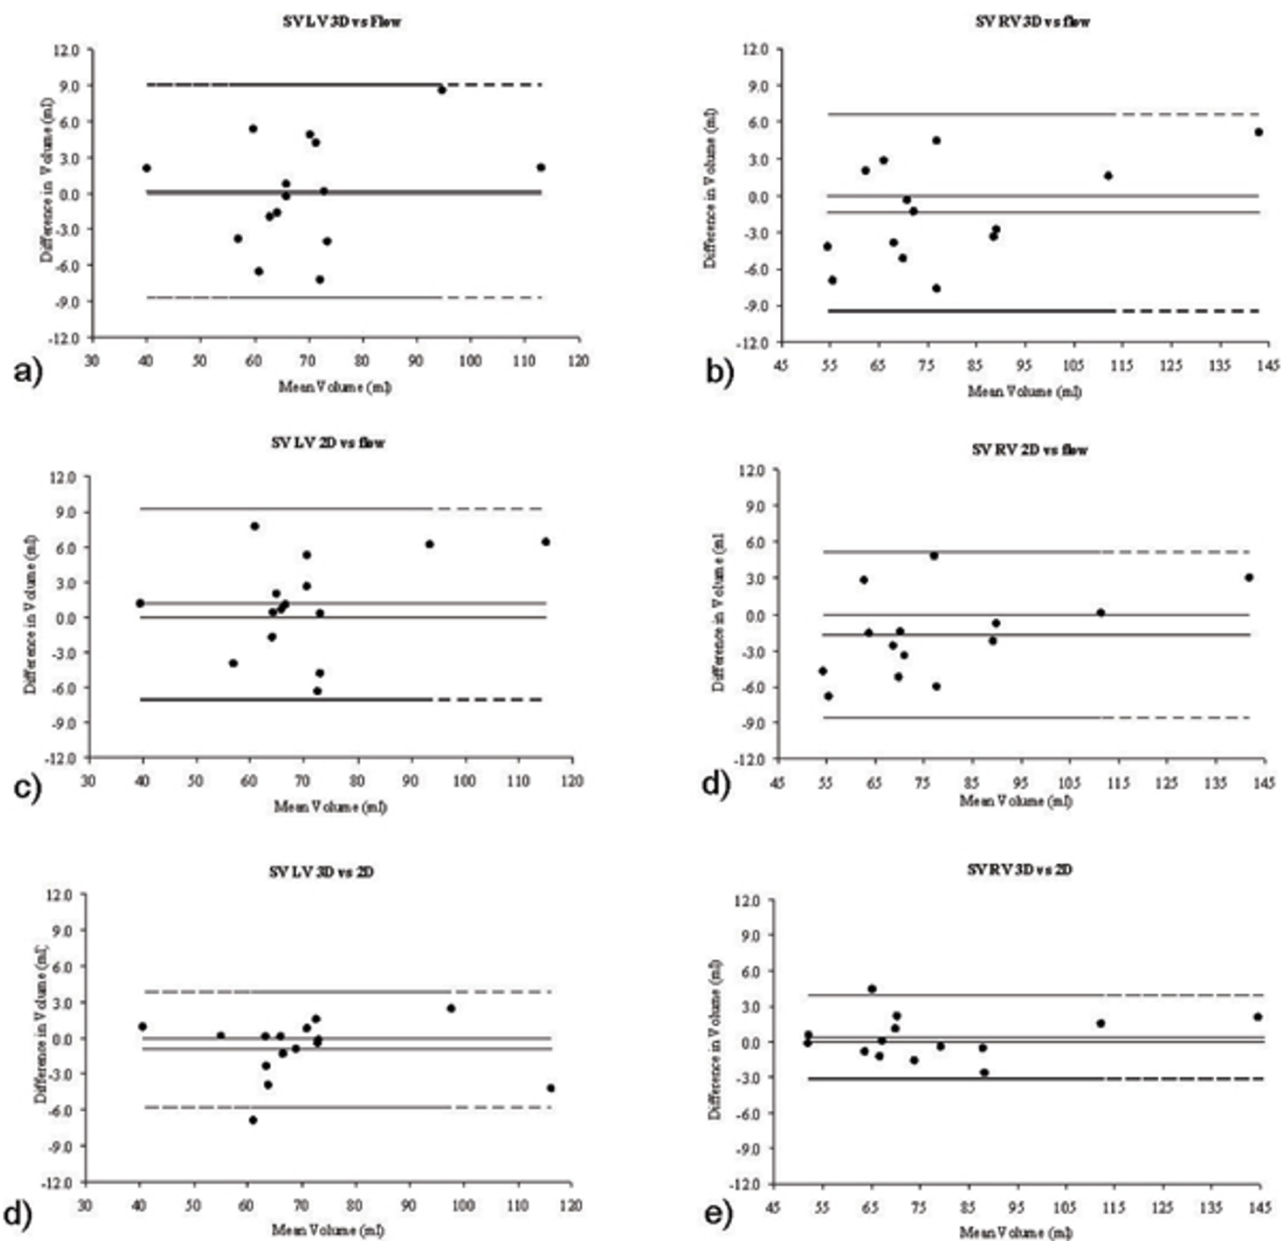


Figure 4
SV comparison between different a, b) 3D vs flow and c, d) M2D vs flows and d, e) 3D vs M2D for LV (a, c, e) and RV (b, d, f).

References

1. Greil GF, et al.: *J Magn Reson Imaging* 2007.
2. Bottger T, et al.: *Acad Radiol* 2007.

Publish with **BioMed Central** and every scientist can read your work free of charge

"BioMed Central will be the most significant development for disseminating the results of biomedical research in our lifetime."
Sir Paul Nurse, Cancer Research UK

Your research papers will be:

- available free of charge to the entire biomedical community
- peer reviewed and published immediately upon acceptance
- cited in PubMed and archived on PubMed Central
- yours — you keep the copyright

Submit your manuscript here:
http://www.biomedcentral.com/info/publishing_adv.asp

