



## Nanostructured ZnO for biosensing applications

XU ChunXiang<sup>1\*</sup>, YANG Chi<sup>1</sup>, GU BaoXiang<sup>2</sup> & FANG ShengJiang<sup>1</sup>

<sup>1</sup> State Key Laboratory of Bioelectronics, School of Electronic Science and Engineering, Southeast University, Nanjing 210096, China;

<sup>2</sup> Department of Resources and Environment Engineering, Henan Institute of Engineering, Zhengzhou 450000, China

Received July 5, 2012; accepted September 3, 2012; published online May 6, 2013

Based on the unique properties, nanostructured ZnO could provide a stable immobilization for biomolecules retaining their biological activity. It has been recently developed as a nice candidate for the construction of biosensors with enhanced analytical performance. In this paper, we reviewed the progress in adapting nanostructured ZnO for several predominantly in biosensing applications based on enzymic reaction, immunoreaction, and molecular competition. We also described several important considerations when working with nanostructured ZnO mainly centered on the fabrications of ZnO and appropriate strategies for biosensor construction (e.g. modified electrodes and multilayered immobilization).

**ZnO, biosensor, Zn alloy**

**Citation:** Xu C X, Yang C, Gu B X, et al. Nanostructured ZnO for biosensing applications. *Chin Sci Bull*, 2013, 58: 2563–2566, doi: 10.1007/s11434-013-5714-5

Semiconductor biosensor is based on combining the properties of biologically active materials with those of inorganic crystalline materials that translate the biological properties into electronic signals. These signals can then be processed to identify the properties of biological elements. [1]. Zinc oxide has attracted much attention particularly due to its widely applications in optics, optoelectronics, sensors, and actuators [2,3]. The biocompatibility, low toxicity, high electron mobility and easy fabrication of ZnO are favorable for biosensing [4–7]. Moreover, it has a high isoelectric point (IEP) of about 9.5, which makes it suitable for adsorption of proteins with low IEPs via electrostatic interactions [7]. Meanwhile, ZnO has probably the richest variety of different nanostructures which is benefit for biosensor design. So far, ZnO combs, nanotubes and nanorods have been employed to enzyme biosensor, immunosensor and other type sensor [8–12]. Especially, ZnO quantum dots (QDs) which have similar size as the biomolecules provide a good interactive environment for the biomarker [13,14]. The scope of this article is focused on our recent research

progress on interaction/integration of ZnO QDs and ZnO one-dimensional (1-D) nanostructure with biomolecules for sensor applications.

### 1 ZnO quantum dots biosensor

ZnO QDs as high aspect nanoparticles with high IEP have been promised as probes for ultrasensitive detection of cancer biomarkers [13,14]. Their fluorescent properties have enabled ZnO QDs to be used as labels for in vitro assays to quantify biomarkers, for example, the conjugates of ZnO QDs with antibodies, aptamers, oligonucleotides, or peptides can act as the target cancer markers. ZnO QDs have also been exploited for electrochemical detection on the basis of their elemental compositions besides optical approach. Owing to the amplification effect originating from dissolving ZnO QDs, and the highly sensitive nature of electrochemical stripping detection, the sensitivity of electrochemical detection methods for cancer biomarkers is very high.

Carbohydrate antigen 19-9 (CA 19-9) is a preferred label for pancreatic tumor. It is a malignant tumor and difficult to


\*Corresponding author (email: [xcxseu@seu.edu.cn](mailto:xcxseu@seu.edu.cn))

be early diagnosed in current clinical medicine [15]. In our previous work [16], using ZnO QDs as electrochemical and fluorescent labels, a sandwich-type sensitive immunoassay was developed based on immunoreactions between the antibody and antigen to detect the antigen CA19-9. Stripping voltammetry and photoluminescence were conducted to carry out an efficient immunoassay based on the electrochemical and optical properties of ZnO QDs. The immunosensor showed high sensitivity, stability, and reproducibility. The spectral measurement presented a linear range from 1 to 180  $\text{U mL}^{-1}$  with a detection limit of  $0.25 \text{ U mL}^{-1}$ . The detection limit was further reduced to  $0.04 \text{ U mL}^{-1}$  and the linear range was extended from 0.1 to  $180 \text{ U mL}^{-1}$  by square wave voltammetry (SWV) analysis, as shown in Figure 1. The specificity experiments were further verified by competition experiments to evaluate the association of CA 19-9 antigen with QD labeled CA 19-9 antibody probe in the presence of increasing concentrations of nonspecific latent membrane protein competitors. The results show that ZnO QD-based immunosensor has a good specificity for CA 19-9 detection.


ZnO QDs were also employed in the lectin biosensor. As we know, as compared to the immunosensor, the lectin biosensor could obviate time-consuming, high cost and denaturation in existing methods. More important, some lectins were found to be as specific as antibody binds to a specific antigen and applied in the biosensor [17]. We report a direct electrochemical biosensor for the detection of allergy chicken ovomucoid (CHOM) based on bioconjugates of ZnO QDs binding CHOM [18]. The CHOM bioconjugates is formed through electrostatic interaction between positively charged QDs and negatively charged protein. Concanavalin A (Con A) was employed as a recognition element for the CHOM bioconjugates. The extent detection was accomplished by electrochemical SWV analysis of cadmium released by acid from the captured quantum dots. The biosensor shows concentration-dependent SWV development by capturing CHOM-functionalized ZnO QDs on Con A-coated chips and has a detection limit of  $1 \text{ ng mL}^{-1}$ . As an important criterion for any analytical tool, the biosensor shows acceptable specificity towards CHOM.

Although the above proposed method makes the analyte was detected directly through electrochemical of the ZnO-analyte bioconjugates captured on Con A substrate, the analytes have to be labeled each time. To avoid this problem, a substitution method was developed using carcinoembryonic antigen (CEA) as a model. The basic principle is that the ZnO-CEA bioconjugates could be replaced by the analyte CEA captured on the Con A substrate in advance because the former combined more weakly than the later combined with Con A. The analyte CEA is monitored by electrochemical of the undisplacement ZnO-CEA bioconjugates on the Con A substrate [19]. The assay was based on the competition between a quantum dots labeled CEA and analyte CEA using concanavalin A as the recognition element [20]. The extent of completion was monitored by the square wave stripping voltammetry. The results show that the sensor demonstrated an acceptable precision, reproducibility and storage stability.

The competition method is expected to develop an approach for multi-analytic determination simultaneously by tagging each biomolecule with different QDs. As an example, the pharmacology (QP) of cetuximab (C225), a monoclonal antibody directed against colorectal cancer, and the biomarker of the cancer, CEA were designed to analyze quantitatively. In order to find the optimal dose for each individual patient, we usually need to get the dynamic changes of CEA (biomarker of the colorectal) and C225 in advance. Thus, simultaneous detection of CEA and C225 is the first step toward an assay for QP of C225. We developed a ZnO and CdSe QDs-based multi-analyte biosensor for simultaneous determination of CEA and the corresponding therapeutic drug C225, as shown in Figure 2 [21]. The assay is based on the competition between a quantum dots labeled glycans and target glycans using lectins as the recognition element. The dual-analytic biosensor detected CEA and C225 in the range from  $1 \text{ ng mL}^{-1}$  to  $400 \mu\text{g mL}^{-1}$  by stripping voltammetry. The biosensor developed here for the simultaneous detection of the biomarkers and therapeutic drugs is expected to develop as a potential technique for quantitative pharmacology.

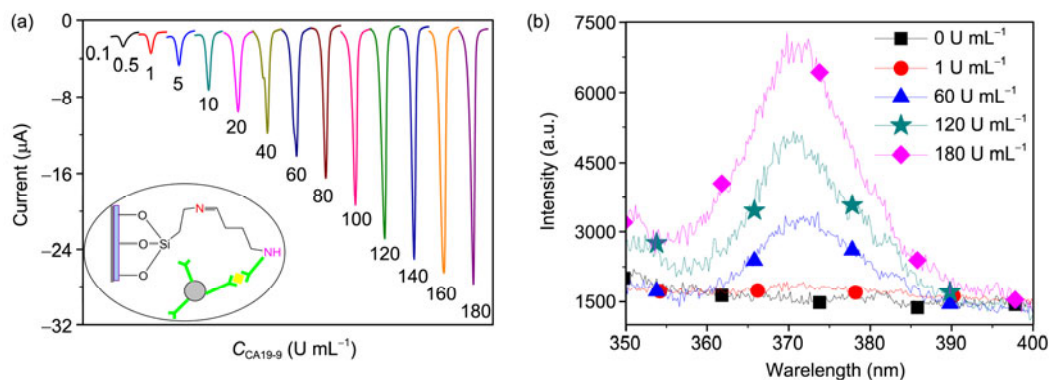

**Figure 1** (a) SWV curves of the pending-solution with the series concentration of CA 19-9 inserted with protocol of sandwich-immunosensor; (b) the UV PL spectra of the immunosensors with series CA19-9 concentration.

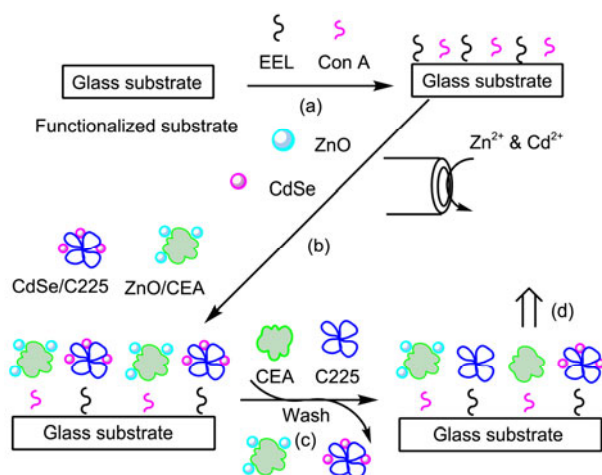

**Figure 2** Fabrication and sensing process of ZnO and CdS QD-based biosensor for simultaneous detection of CEA and C225. (a) Substrate functionalization and lectins (EEL and Con A) immobilization; (b) assembly of bioconjugates (ZnO/CEA and CdSe/C225) on lectin layer; (c) analytes addition and displacement; (d) SWV detection of the remnant QDs.

## 2 1-D nano-ZnO biosensor


1-D ZnO nanomaterials were used as carriers with large surface to increase the loading amount of enzymes. 1-D nanostructured ZnO is favor to immobilization of various enzymes and is facilitate to the electron transfer between the redox centers of enzymes and the electrochemical electrode [22,23].

The conventional ZnO modified electrode are almost fabricated by post-pasting of ZnO [24–27], which did not enable robust mechanical adhesion and electrical contact

between the nanostructured ZnO and the electrode. It is desirable to improve the electrical contact and sensing performance if ZnO nanostructured electrodes *in situ* synthesized without using any organic reagent. Therefore, we developed the method that the gold electrode was coated by a thin layer of Zn-Au alloy to improve the nucleation for *in situ* growth of ZnO nanostructures and to further improve the performance of the biosensor, which was constructed by immobilizing tyrosinase (Tyr) on the ZnO nanostructures for phenol detection [28]. Electrochemical measurements, Fourier transform infrared and scanning electron microscopic analyses demonstrated that the Tyr was stably adsorbed on the ZnO nanostructures surface with bioactivity for phenol oxidation. The biosensor reached the sensitivity was as high as  $103.08 \mu\text{A}/(\text{mmol L}^{-1})$  at  $C_{\text{phenol}} > 20 \mu\text{mol L}^{-1}$  and was  $40.76 \mu\text{A}/(\text{mmol L}^{-1})$  at  $C_{\text{phenol}} < 20 \mu\text{mol L}^{-1}$ . The detection limit of  $0.623 \mu\text{mol L}^{-1}$  was obtained.

To improve the performance, the poly (sodium 4-styrenesulfonate) and horseradish peroxidase (HRP) were alternatively immobilized on ZnO nanostructures repeatedly [29]. The amount of HRP on the ZnO nanostructures surface increased along with the modified-layer increase. Electrochemical measurement analysis demonstrated that the HRP kept bioactivity for  $\text{H}_2\text{O}_2$  detection without an electron transfer mediator. The multilayered HRP sensors exhibited a wide linear range and low detection limit. The sensitivity of the biosensor increased with the immobilized HRP layers from the lowest value of  $58.15 \mu\text{A}/(\text{mmol L}^{-1})$  for five layers.

Unique structured nanocomposite also can facilitate the direct electron transfer between redox proteins and the electrodes [22,23] and therefore improve the performance of the biosensor. Consequently, a ZnO/Cu nanocomposite *in situ*

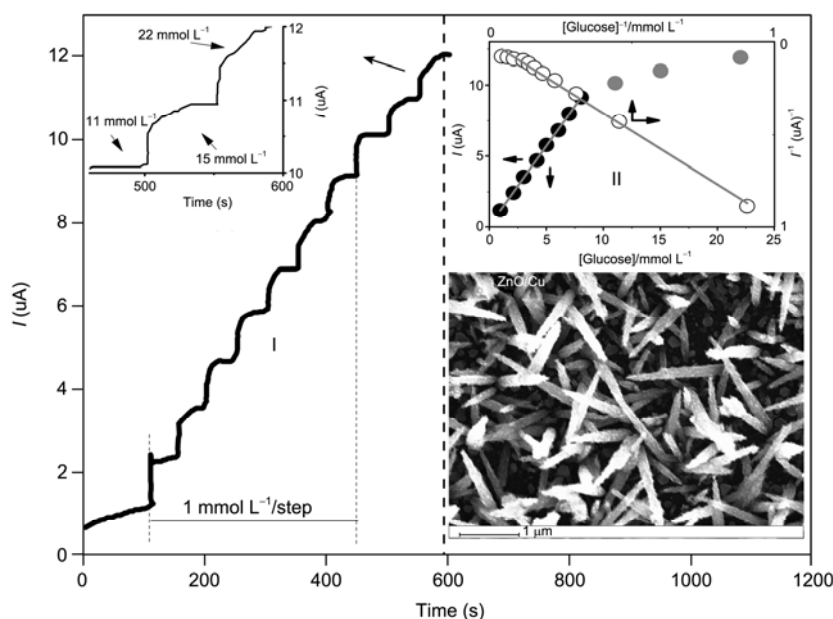

**Figure 3** Amperometric response of the biosensor to different concentrations of glucose in PBS (0.1 mol/L, pH 7.4) at an applied potential of  $-0.39 \text{ V}$ . Inset II: The calibration curve (current versus glucose concentration) and Lineweaver-Burk plot (current $^{-1}$  versus concentration $^{-1}$ ) from curve I. Inset upper right: SEM of the ZnO/Cu nanocomposite.

directed growth on electrode was prepared and applied in biosensor [30]. SEM images demonstrate that the morphology of ZnO/Cu nanocomposite has a large specific surface area, which is favorable to immobilize the biomolecules and realize the direct electron transfer between the electrode surface and the redox protein (Figure 3). As a model, this ZnO/Cu nanocomposite is employed for immobilization of GOx and the construction of the glucose biosensor. Direct electron transfer of GOx is achieved at ZnO/Cu nanocomposite with a high heterogeneous electron transfer rate constant of  $0.67 \pm 0.06 \text{ s}^{-1}$ . The electrochemical assay also showed specificity for the detection of glucose and demonstrated a dynamic range of 1–9  $\text{mmol L}^{-1}$  with detection limit of  $0.04 \text{ mmol L}^{-1}$ . Such ZnO/Cu nanocomposite provides a good matrix for direct electrochemistry of enzymes and mediator-free enzymatic biosensors.

### 3 Conclusions

The unique properties of ZnO and the ease of ZnO nanostructure fabrication make this material suitable for biosensor applications. The examples have briefly summarized the interaction/integration of ZnO QDs and ZnO 1-D nanostructures with biomolecules. The next challenge of modified electrodes is their applicability for the *in vivo* detection and its stability. Many researchers concentrate on ease, user-friendly, less interference, and commercially available electrodes. In this aspect, ZnO nanostructures have an important role to play in near future. The versatility of properties and formation of nanostructures affords the promise for its applications in chemical and biochemical biosensors.

*This work was supported by the National Natural Science Foundation of China (60725413 and 60976002), the National Basic Research Program of China (2011CB302004) and the Ministry of Education (309015).*

- Yogeswaran U, Chen S M. A review on the electrochemical sensors and biosensors composed of nanowires as sensing material. *Sensors*, 2008, 8: 290–313
- Pearson S J, Norton D P, Ip K, et al. Recent progress in processing and properties of ZnO. *Progress in Materials. Prog Mater Sci*, 2005, 50: 293–340
- Sun X W, Kwok H S. Optical properties of epitaxially grown zinc oxide films on sapphire by pulsed laser deposition. *J Appl Phys*, 1999, 86: 408–411
- Tian Z R R, Voigt J A, Liu J, et al. Biomimetic arrays of oriented helical ZnO nanorods and columns. *J Am Chem Soc*, 2002, 124: 12954–12955
- Wei A, Sun X W, Wang J X, et al. Enzymatic glucose biosensor based on ZnO nanorod array grown by hydrothermal decomposition. *Appl Phys Lett*, 2006, 89: 123902-1-3
- Dong Z F, Tian Y, Yin X, et al. Physical vapor deposited zinc oxide nanoparticles for direct electron transfer of superoxide dismutase. *Electrochem Commun*, 2008, 10, 818–820
- Degen A, Kosec M. Effect of pH and impurities on the surface charge of zinc oxide in aqueous solution. *J Eur Ceram Soc*, 2000, 20: 667–673
- Dorfman A, Kumar N, Hahn J. Nanoscale ZnO-enhanced fluorescence detection of protein interactions. *Adv Mater*, 2006, 18: 2685–2690
- Asif M H, Nur O, Willander M, et al. Selective calcium ion detection with functionalized ZnO nanorods-extended gate MOSFET. *Biosens Bioelectron*, 2009, 24: 3379–3382
- Dai Z, Shao G, Hong J, et al. Immobilization and direct electrochemistry of glucose oxidase on a tetragonal pyramid-shaped porous ZnO nanostructure for a glucose biosensor. *Biosens Bioelectron*, 2009, 24: 1286–1291
- Rahman M M, Umar A, Sawada K. Ultra-sensitive cholesterol biosensor based on low-temperature grown ZnO nanoparticles. *Electrochem Commun*, 2009, 11: 118–121
- Zhao J, Wu D, Zhi J. A novel tyrosinase biosensor based on biofunctional ZnO nanorod microarrays on the nanocrystalline diamond electrode for detection of phenolic compounds. *Bioelectrochemistry*, 2009, 75: 44–49
- Somers R C, Bawendi M G, Nocera D G. CdSe nanocrystal based chem-/bio-sensors. *Chem Soc Rev*, 2007, 36: 579–591
- Gill R, Zayats M, Willner I. Semiconductor quantum dots for bioanalysis. *Angew Chem Int Ed*, 2008, 47: 7602–7625
- Barbara S, Antonina H S, Witold K, et al. Tissue polypeptide specific antigen (TPS), a marker for differentiation between pancreatic carcinoma and chronic pancreatitis: A comparative study with CA 19-9. *Cancer*, 2000, 89: 83–88
- Gu B X, Xu C X, Yang C, et al. ZnO quantum dot labeled immunosensor for carbohydrate antigen 19-9. *Biosens Bioelectron*, 2011, 26: 2720–2723
- Zhang X, Teng Y, Fu Y, et al. Lectin-based biosensor strategy for electrochemical assay of glycan expression on living cancer cells. *Anal Chem*, 2010, 82: 9455–9460
- Yang C, Gu B X, Xu C X, et al. Self-assembled ZnO quantum dot bioconjugates for direct electrochemical determination of allergen. *J Electroanal Chem*, 2011, 660: 97–100
- Yang C, Xu C X, Wang X M, et al. A displacement assay for the sensing of carbohydrate using zinc oxide biotracers. *Electrochim Acta*, 2012, 60: 50–54
- Chen J P. Performance of affinity biosensors with competitive displacement mechanism. *J Chem Tech Biotechnol*, 1993, 56: 213–211
- Yang C, Xu C X, Wang X M, et al. Quantum-dot-based biosensor for simultaneous detection of biomarker and therapeutic drug: First steps toward an assay for quantitative pharmacology. *Analyst*, 2012, 137: 1205–1209
- Yang M, Qu F, Li Y, et al. Direct electrochemistry of hemoglobin in gold nanowire array. *Biosens Bioelectron*, 2007, 23: 414–420
- Xiao Y, Li C M. Nanocomposites: From fabrications to electrochemical bioapplications. *Electroanalysis*, 2008, 20: 648–662
- Lu X, Zhang H, Ni Y, et al. Porous nanosheet-based ZnO microspheres for the construction of direct electrochemical biosensors. *Biosens Bioelectron*, 2008, 24: 93–98
- Wu S, Ju H X, Liu Y. Conductive mesocellular silica-carbon nanocomposite foams for immobilization, direct electrochemistry, and biosensing of proteins. *Adv Funct Mater*, 2007, 17: 585–592
- Bao S J, Li C M, Zang J F, et al. New nanostructured TiO<sub>2</sub> for direct electrochemistry and glucose sensor applications. *Adv Funct Mater*, 2008, 18: 591–599
- Chen L Y, Gu B X, Zhu G P, et al. Tyrosinase biosensor based on zinc oxide nanorods. *Nano*, 2007, 2: 281–284
- Gu B X, Xu C X, Zhu G P, et al. Tyrosinase immobilization on zinc nanorods for phenol detection. *J Phys Chem B*, 2009, 113: 377–381
- Gu B X, Xu C X, Zhu G P, et al. Layer by layer immobilized horseradish peroxidase on zinc oxide nanorods for biosensing. *J Phys Chem B*, 2009, 113: 6553–6557
- Yang C, Xu C X, Wang X M. ZnO/Cu Nanocomposite: A platform for direct electrochemistry of enzymes and biosensing applications. *Langmuir*, 2012, 28: 4580–4585