

ORAL PRESENTATION

Open Access

RF induced heating of pacemaker/ICD lead-tips during MRI Scans at 1.5T and 3T: evaluation in cadavers

Volkan Acikel^{2*}, Patrick Magrath^{2,1}, Scott E Parker², Peng Hu², Holden H Wu², J Paul Finn², Daniel B Ennis^{2,1}

From 19th Annual SCMR Scientific Sessions
Los Angeles, CA, USA. 27-30 January 2016

Background

Studies about the safety of MRI exams for patients with pacemakers/ICDs at 1.5T have been reported [Nazarian S, et al. *Annals of internal medicine* 155.7 (2011): 415-424.]. Of most concern is possible heating of the lead-tips in contact with the myocardium. Little is known about the relative safety of 3T MRI exams for these patients and in vivo lead-tip heating data is difficult, if not impossible, to obtain. Our objective was to measure lead-tip heating directly in human cadavers with pacemakers/ICDs at both 3.0T and 1.5T.

Methods

Cadavers (N = 5, 3 male, Table 1, part 1) with existing pacemakers had fiberoptic temperature probes implanted adjacent to right atrial (RA), right ventricular (RV) and/or abandoned lead-tips under x-ray guidance. Whole-body

CT was used to estimate lead-tip to probe-tip distances. Cadavers were exposed to 15-minutes of 4 W/kg whole body SAR at both 1.5T and 3T (Siemens Avanto and Prisma) for five isocenter positions: 6 cm superior to the chin (LM₁) and in four 15 cm increments inferior to LM₁ (LM₂ to LM₅) in order to evaluate lead-tip heating as a function of the device's position relative to isocenter (i.e. different MRI exams). Maximum temperature increases at the lead-tip were reported as ΔT_{Max} (temperature difference between the baseline before the MRI sequence and peak heating after 15-minutes).

Results

All temperature probes were ≤ 10 mm from the lead-tip (Table 1, part 2). Figure 1 shows ΔT_{Max} for 1.5T and 3T for each probe. Maximum heating was observed at the LM₂ and LM₃ isocenter positions for which the whole

Table 1 Part 1 is the table that shows vital statistics of the cadavers. Part 2 is the table that shows the lead tip to probe tip distances

Part 1	Gender	Weight (kg)	Height (cm)	BMI	Age				
Cadaver 1	Male	54	167	19.4	93				
Cadaver 2	Female	36	147	16.7	99				
Cadaver 3	Male	58	177	18.5	85				
Cadaver 4	Male	45	172	15.2	93				
Cadaver 5	Female	68	167	24.4	87				
Part 2	Cadaver 1	Cadaver 2 RA lead	Cadaver 3	Cadaver 4 RA lead	Cadaver 4 RV lead	Cadaver 5 RA lead	Cadaver 5 RV lead	Cadaver 5 Abandoned lead	
Lead tip to probe tip distance	6.4 mm	3.4 mm	10 mm	2 mm	9 mm	6.5 mm	7.6 mm	4 mm	

²Department of Radiological Sciences, University of California Los Angeles, Los Angeles, CA, USA

Full list of author information is available at the end of the article

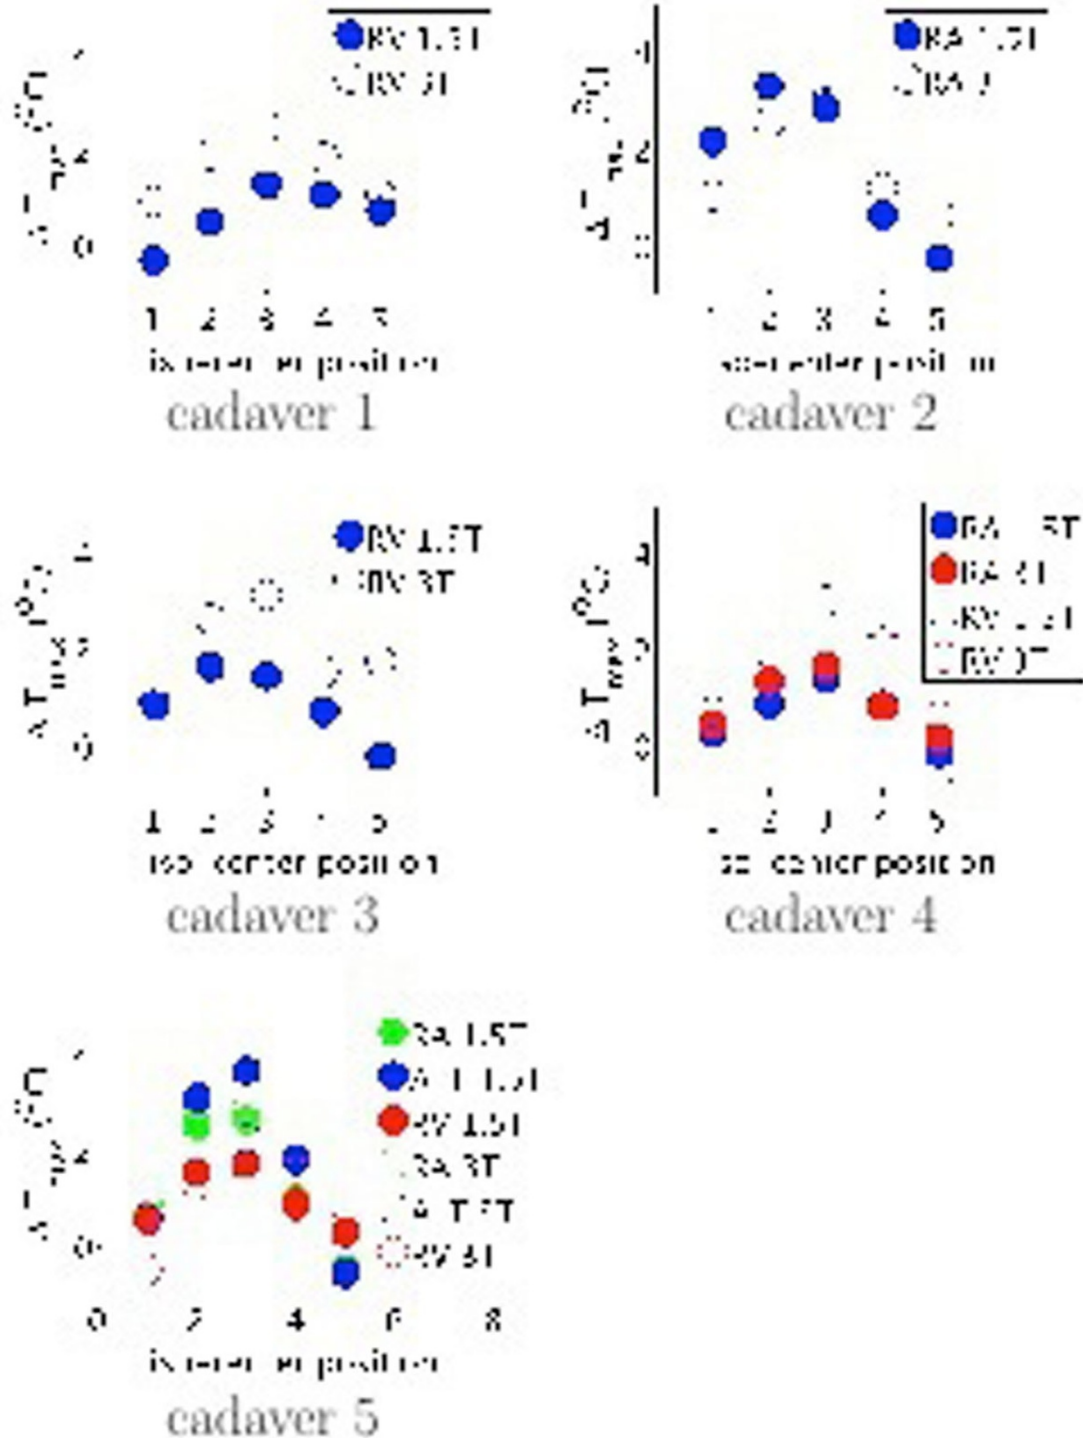


Figure 1 ΔT_{Max} for each isocenter position. Cadavers 1 and 3 have single chamber pacemakers (RV leads); cadavers 2, 4, and 5 have dual chamber pacemakers (RA and RV lead). Cadaver 5 also had 10 abandoned leads. For single chamber pacemakers a temperature probe was placed at the lead-tip and the remaining temperature probes were placed in remote tissue for reference. For dual chamber pacemakers, the temperature probes were placed at the RA and RV lead-tips and two probes were placed in remote tissue for reference. For the cadaver with abandoned leads two temperature probes were placed close to the lead-tips connected to the pacemaker and one probe was placed close to lead-tip of one abandoned lead (ALT). Note that in cadaver 2 the RV temperature probe was not close enough to the RV lead-tip (accidentally partially withdrawn) to obtain temperature data.

implant was inside the body transmit coil. ΔT_{Max} was $>2\text{C}$ for 7 of 25 cases at 1.5T and for 12 of 25 cases at 3T, but never exceeded 4C.

Conclusions

These data do not indicate a substantial difference between lead-tip heating at 1.5T and 3T, nor do they indicate $\Delta T_{\text{Max}} > 4\text{C}$ despite the lack of cooling due to tissue perfusion. Continued evaluation is warranted and on-going.

Authors' details

¹Department of Bioengineering, University of California Los Angeles, Los Angeles, CA, USA. ²Department of Radiological Sciences, University of California Los Angeles, Los Angeles, CA, USA.

Published: 27 January 2016

doi:10.1186/1532-429X-18-S1-O121

Cite this article as: Acikel et al.: RF induced heating of pacemaker/ICD lead-tips during MRI Scans at 1.5T and 3T: evaluation in cadavers. *Journal of Cardiovascular Magnetic Resonance* 2016 **18**(Suppl 1):O121.

Submit your next manuscript to BioMed Central and take full advantage of:

- Convenient online submission
- Thorough peer review
- No space constraints or color figure charges
- Immediate publication on acceptance
- Inclusion in PubMed, CAS, Scopus and Google Scholar
- Research which is freely available for redistribution

Submit your manuscript at
www.biomedcentral.com/submit

