

# SPIN-ECHO NUCLEAR MAGNETIC RESONANCE EVIDENCE FOR COMPLEXING OF SODIUM IONS IN MUSCLE, BRAIN, AND KIDNEY

FREEMAN W. COPE

*From the Biochemistry Division, Aerospace Medical Research Laboratory,  
U. S. Naval Air Development Center, Warminster, Pennsylvania 18974*

**ABSTRACT**  $\text{Na}^+$  in muscle, brain, and kidney is shown by spin-echo nuclear magnetic resonance (NMR) to consist of two fractions with different NMR parameters. The slow fraction of  $\text{Na}^+$  in these tissues has NMR relaxation times  $T_1$  and  $T_2$  of  $10\text{--}15 \times 10^{-3}$  sec, which is approximately 4–5 times shorter than for  $\text{Na}^+$  in aqueous NaCl solution. The slow fraction may represent  $\text{Na}^+$  dissolved in structured tissue water. The fast fraction of tissue  $\text{Na}^+$ , which is shown to represent approximately 65% of the total tissue  $\text{Na}^+$  concentration, has  $T_2$  less than  $1 \times 10^{-3}$  sec, which resembles the values of  $T_2$  observed for  $\text{Na}^+$  complexed by synthetic ion-exchange resins. One is drawn to the conclusion that approximately 65% of total  $\text{Na}^+$  in muscle, brain, and kidney is complexed by tissue macromolecules.

## INTRODUCTION

The classical picture of the cell as a membranous bag containing inorganic ions and proteins dissolved in liquid water is widely accepted. Belief in the classical picture seems to come from its simplicity and from historical precedent. Experimental evidence for its validity is scarce. Important contradictions are contained within the classical picture, the most conspicuous of which is that the ion pumps which must be postulated in order to maintain the observed ion concentration gradients against measured leakages would require 1500–3500% of the total energy produced by the cell (1).

Because of serious deficiencies of the classical theory, a small minority of investigators have taken an entirely different view of the cell. They regard the cell as an organized, nonliquid phase consisting of macromolecules embedded in semicrystalline water.  $\text{Na}^+$  and  $\text{K}^+$  are believed mostly to be complexed to cell macromolecules and to have low solubility in semicrystalline cell water. A basis for comprehensive theoretical analysis of the minority view of the cell has been developed by Ling (1, 2) using statistical mechanical concepts, under the name of the "association-induction hypothesis." A less comprehensive but simpler treatment of cellular ion complexing

using mass-action methods has been presented by Troshin (3, 4). A simple non-equilibrium thermodynamic treatment of cellular ion leakage phenomena has been derived from the application of solid-state physical concepts by Cope (5-7).

Much progress has occurred in recent years toward experimental proof of the minority view, including evidence for structuring of cell water, and for complexing of  $\text{Na}^+$  and  $\text{K}^+$ . Cell water seems probably to consist of multiple polarized layers (8, 9). Nuclear magnetic resonance (NMR) evidence strongly supports the idea that cell water possesses more structure than liquid water (22, 23). Evidence for  $\text{Na}^+$  complexing has come from several sorts of measurements. Equilibrium binding studies of Troshin (3, 4) and Ling (1) showed that the equilibria of  $\text{Na}^+$  between cell and solution conformed to the Langmuir adsorption isotherm, with a correction for a minor fraction of  $\text{Na}^+$  dissolved in intracellular water. Cation-sensitive intracellular microelectrode measurements (10-13) have been interpreted to indicate that 70% of intracellular  $\text{Na}^+$  of muscle was in some form that excluded it from contact with the microelectrode.

NMR analysis of  $\text{Na}^+$  has great advantages over other methods for the study of complexing of  $\text{Na}^+$  in tissues (14, 15, 6, 16, 17). First, the position of the NMR line of  $\text{Na}^+$  is much different from that of all other ions such as  $\text{H}^+$ ,  $\text{K}^+$ , or  $\text{Cl}^-$ . Hence, the results of NMR analysis are free from those uncertainties which confuse the interpretation of conductivity and electrode measurements. Second, the width of the steady-state NMR line of  $\text{Na}^+$  is dependent upon the chemical and physical environment surrounding the individual  $\text{Na}^+$  ion. Therefore, the width of the steady-state NMR line may indicate whether the  $\text{Na}^+$  ion is surrounded by an environment like that in free solution, or by some other environment. The same advantages of NMR may be applied to the study of  $\text{K}^+$  complexing in biological systems (18, 19).

These properties of the steady-state NMR spectrum have been exploited by Cope (6, 14, 15), Rotunno et al. (16), Ling and Cope (18), and Czeisler et al. (17) to provide strong evidence for complexing of  $\text{Na}^+$  in tissues. The steady-state NMR spectrum of muscle (14, 15, 17, 18), brain (15), kidney (15), and frog skin (16) showed 60-75% depressions of peak height compared to the same concentrations of  $\text{Na}^+$  in free solution, with little change in line width. A similar picture had been observed previously in ion-exchange resin by Jardetzky and Wertz (20). These authors (20) interpreted  $\text{Na}^+$  in wet ion-exchange resin to consist of two fractions: (a) a fraction of  $\text{Na}^+$  dissolved in water which showed the usual NMR spectrum of  $\text{Na}^+$ , and (b) a fraction of  $\text{Na}^+$  complexed by the ion-exchange resin, which markedly shortened the NMR relaxation time to produce a steady-state NMR spectrum of  $\text{Na}^+$  that was so broad and low that it was invisible to NMR because it was obscured by instrumental noise. The broadening of the NMR spectrum of  $\text{Na}^+$  complexed by ion-exchange resin has been shown directly by Czeisler et al. (17). The steady-state NMR picture observed in tissues was interpreted in the same way to indicate that 60-75% of  $\text{Na}^+$  in tissues was broadened to NMR invisibility by complexing with macromolecules, while the second smaller fraction was in free

solution in tissue water, and therefore had its usual steady-state NMR spectrum (6, 14–19).

It was possible that the above two-fraction interpretation might be wrong. The presence of only a single fraction of tissue  $\text{Na}^+$  with NMR relaxation times ( $T_1$  and/or  $T_2$ ) moderately different from  $\text{Na}^+$  in liquid water could under some circumstances also give a depression of height with unchanged width of the steady-state NMR spectrum (21). Such a change in  $T_1$  or  $T_2$  of  $\text{Na}^+$  might result from the probable structured state of tissue water (22, 23). Errors of interpretation due to instrumental problems might also have been present in the original steady-state NMR studies (6, 14–16, 18). However, a sophisticated study of the instrumental subtleties of the steady-state NMR behavior of muscle  $\text{Na}^+$  has just appeared which confirms the two-fraction interpretation (Czeisler et al., 17). The present paper provides additional confirmation of the two-fraction hypothesis by *spin-echo* NMR of  $\text{Na}^+$  in muscle, brain, and kidney, and provides direct measurements of NMR relaxation times of both fractions of  $\text{Na}^+$  in each of these tissues.

## METHODS

### A. Spin-Echo NMR

A 2 ml volume of solution or tissue in a glass test tube of 14 mm i.d. was centered in the NMR probe. Sample temperatures were  $25^\circ \pm 1^\circ\text{C}$  except where otherwise stated. The experiments were performed at the NMR resonance of  $^{23}\text{Na}$  at  $10 \times 10^6$  Hz and 8879 gauss. The magnetic field was produced by either of two different Varian 12-inch diameter electromagnets, each with a gap of 1.75 inches. The first magnet had auxiliary shim coils to increase the homogeneity of magnetic field. Because the second magnet lacked such coils, it had a relatively poor homogeneity. In some situations, the difference in homogeneity necessitated a difference in technique of measurement of  $T_2$ , as will be described later in the paper. The NMR probe, in which the sample was placed, had separate transmitter and receiver coils. The measurements used a Model PS-60AW spin-echo NMR spectrometer (Nuclear Magnetic Resonance Specialties, Inc., New Kensington, Pa.), with the addition of a low-noise preamplifier placed close to the probe, and extra RC filtering after the receiver, the phase detected output of which was fed into a D.C. amplifier with a gain of  $10 \times$  or  $100 \times$ , which led into an averaging computer (Model TDH-9 of Princeton Applied Research Corp., Princeton, N. J.; or CAT Model 400A of Technical Instruments, Corp., North Haven, Conn.; or Model 5480A of Hewlett-Packard Co., Palo Alto, Calif.). The spectrometer was also modified to put both first and second pulses through the same transmitter channel, so that phase drifts for both pulses were equal. The modifications and accessories listed above provided the high signal-to-noise ratio which was necessary to measure accurately the low concentrations of  $\text{Na}^+$  in tissues. In order to plot  $T_1$  and  $T_2$  decay curves more completely, the spectrometer was modified to allow continuous adjustment of the time between pairs of pulses, instead of the stepwise control provided on the standard instrument. An attenuator with 1% accuracy and zero phase shift was included in the receiver to facilitate quantitative comparisons between different  $\text{Na}^+$  concentrations. All measurements of time were calibrated against a crystal oscillator, which had an accuracy of 0.001%.

The procedures for spectrometer adjustment were conventional and have been described previously (22). The  $90^\circ$  pulse had a width of approximately  $77 \times 10^{-6}$  sec and a peak-to-peak

height of approximately 460 v. Repetition rate of the pulse pattern was 4 per sec except where stated otherwise. The techniques for measuring free induction decay,  $T_1$ , and  $T_2$  were conventional, except for the extensive use of RC filtering and computer averaging, which were necessary to achieve sufficient accuracy in the measurement of the low concentrations of  $\text{Na}^+$  in tissues. Free induction decay was measured after a single  $90^\circ$  pulse. Echoes were recorded for a  $90^\circ$ - $180^\circ$  pulse pattern. Then transverse NMR relaxation time ( $T_2$ ) was measured from the time for the height of the echo to decay to  $1/e$  of a previous value. In some cases,  $T_2$  for  $\text{Na}^+$  in tissues or ion-exchange resins was much shorter than the free induction decay which would have been produced by magnetic inhomogeneity. In these cases,  $T_2$  was measured from the decay time of the single exponential decay of the free induction signal. Longitudinal relaxation time ( $T_1$ ) was measured as described by Hahn (24) and Boehme and Eisner (25). The height of the free induction decay after the second pulse of a  $90^\circ$ - $90^\circ$  pair was measured for various values of pulse separation ( $\tau$ ) and was subtracted from the height of the free induction decay after the first pulse. A plot of the logarithm of these differences vs.  $\tau$  yielded a straight line, from which the time to decay to  $1/e$  of a previous value was estimated, which provided a value of  $T_1$ .

Quantitative analysis of  $\text{Na}^+$  concentration from the height of the free induction decay used the following procedure. To measure concentration of  $\text{Na}^+$  independently of changes in *shape* of the free induction decay, it is necessary to use the initial height of the curve, i.e., the height at the start of the decay curve immediately after the end of the transmitted pulse. For aqueous solutions of  $\text{Na}^+$  with either magnet, and with tissue samples with the low homogeneity magnet, free induction decays were observed to follow a gaussian pattern (Fig. 1), provided that total RC filtering was small enough to avoid excessive prolongation of the transmitted pulse artifact. The initial height was obtained by extrapolation to  $t = 0$  of a linear graph of  $\log h$  vs.  $t^2$  of the free induction decay curve ( $t =$  time after end of  $90^\circ$  pulse,  $h =$  height of the curve). For tissue samples in the high homogeneity magnet, the short  $T_2$  converted the free induction decay into a single exponential shape, so that initial height was determined by extrapolation to  $t = 0$  of a graph of  $\log h$  vs.  $t$ . The initial height has the same constant of proportionality to  $\text{Na}^+$  concentration regardless of the shape or decay time of the free induction decay curve. This is true in theory, and was proven experimentally for the case of D in  $\text{D}_2\text{O}$  (22), and was confirmed for  $\text{Na}^+$  in the presence of paramagnetic ions (see later in the present paper). Therefore, concentrations of  $\text{Na}^+$  can be calculated on the assumption of direct proportionality of initial height of the free induction decay to  $\text{Na}^+$  concentration (Fig. 3), using a 0.1 N NaCl standard measured immediately before or afterwards and at the same temperature. It was observed that the constant of proportionality between sodium concentration and height of the spin-echo NMR signals varied by less than approximately 10% over a period of weeks, which indicated good stability of the electronic equipment.

### B. Chemical and Biological

5 g of each ion-exchange resin in the acid form was treated with 25 ml of 1 N NaOH, which was then decanted. The resin was then washed five times with 25 ml volumes of water. The resin was allowed to settle for 5 min, the last wash water was decanted, and the wet resin was packed up to a 2 ml mark in a test tube for NMR analysis.

Tissue samples were obtained from white male rats (200–300 g body weight) as soon as possible after killing by cervical dislocation, so that all spin-echo NMR measurements were completed within 1 hr after death of the rat, except where stated otherwise. Muscle was cut from the thigh in approximately 0.5 g pieces. The brain was removed intact, except for separation of the cerebellum. Kidneys were cut into quarters. All tissues were blotted to remove

blood and extracellular fluid insofar as possible. Pieces of tissue were then packed up to a 2 ml mark in glass test tube (14 mm I.D.) for NMR measurements. Total  $\text{Na}^+$  in all tissue samples was determined by steady-state NMR analysis after ashing to destroy organic molecules which might complex  $\text{Na}^+$ , using a method described previously, which gave tissue  $\text{Na}^+$  analyses agreeing within 4% of results obtained by flame photometry (15). 2 ml samples of 50 mM NaCl solutions showed recoveries averaging 98% after ashing and analysis by the above technique.

## I. SPIN-ECHO NMR OF $\text{Na}^+$ IN SIMPLE SYSTEMS

In steady-state NMR spectroscopy, the sample is irradiated continuously with radio-frequency energy. In spin-echo NMR spectroscopy, however, the sample is irradiated with brief pulses of radio-frequency energy, and radio signal emission from the sample is measured following the incident pulses. By this technique, one may measure three different sorts of NMR relaxations or decays of  $\text{Na}^+$ , which are free induction decay, transverse relaxation time ( $T_2$ ), and longitudinal relaxation time ( $T_1$ ). Briefly stated,  $T_1$  measures decay by longitudinal flipping of Na nuclei,  $T_2$  measures the sum of decay due to the flipping plus any dephasing which is random causing loss of phase memory, and free induction is the sum of these two plus additional dephasing for which phase memory exists, due to macroscopic magnetic inhomogeneities. A more comprehensive but elementary discussion of these phenomena was presented in a previous publication (22).

The expected phenomena of spin-echo NMR of  $\text{Na}^+$  were observed in aqueous solutions of NaCl. Fig. 1 shows the free induction decay observed after a  $90^\circ$  pulse, and the echo after a  $90^\circ$ - $180^\circ$  pulse pair. Free induction decay shape conformed approximately to a gaussian curve with respect to time (Fig. 2). Echo decay for aqueous NaCl followed a single exponential decay from which  $T_2$  was measured. Decay of the height of the free induction decay after the second pulse of a  $90^\circ$ - $90^\circ$  pattern also conformed to a single exponential in accord with the theory of Hahn (24), and from which  $T_1$  was measured.

A brief study was made of the NMR relaxation times of  $\text{Na}^+$  in various aqueous solutions. At a temperature of  $20^\circ \pm 1^\circ\text{C}$  in aqueous 0.1 N NaCl,  $\text{Na}^+$  showed  $T_2$  values of 52, 58, 60, 51, and  $59 \times 10^{-3}$  sec (mean =  $56 \times 10^{-3}$  sec) and  $T_1$  values of 54, 60, 51, 57, and  $53 \times 10^{-3}$  sec (mean =  $55 \times 10^{-3}$  sec). These measurements agree well with a previous study of Eisenstadt and Friedman (26), whose data on  $\text{Na}^+$  as a function of concentration shows  $T_2 = T_1 = 56 \times 10^{-3}$  sec for 0.1 N NaCl. The addition of 0.1 N HCl, 0.1 N KOH, 0.1 M  $\text{MgSO}_4$ , or 0.1 M citric acid did not change  $T_2$  of 0.1 N NaCl significantly. The addition of 0.1 M  $\text{K}_2\text{HPO}_4$  shortened  $T_2$  by approximately 15%. The addition of 0.1 M  $\text{MnCl}_2$  or 0.1 M  $\text{CuSO}_4$  shortened  $T_2$  by approximately 30%. Previously, Jardetzky (27) had found paramagnetic cations to be without significant effect on the steady-state NMR spectrum of  $\text{Na}^+$ . The shortenings of  $T_2$  by paramagnetic ions observed here are apparently too small to have revealed themselves under the steady-state experimental conditions used by Jardetzky (27).

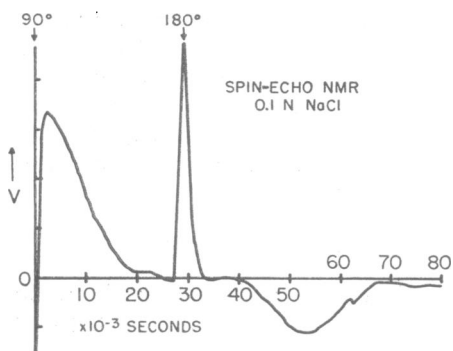


FIGURE 1

FIGURE 1 Free induction decay and echo of aqueous 0.1 N NaCl.  $V$  is the voltage output in arbitrary units of the pulsed NMR spectrometer, which is plotted against time. Sample is 2 ml of 0.1 N NaCl at  $T = 25^\circ\text{C}$ . The initial  $90^\circ$  pulse is followed by emission by the sample of the free induction decay. A  $180^\circ$  pulse is then applied, which is followed on equal time later by emission of an echo. The magnetic field of the high homogeneity magnet deliberately has been made less homogeneous than the best obtainable with this magnet in order to make the free induction decay and echo narrow for ease of observation. RC filtering of approximately  $0.75 \times 10^{-3}$  sec is applied to the spectrometer output, and 100 measurements have been averaged to improve signal-to-noise ratio. Repetition rate of the  $90^\circ$ - $180^\circ$  pulse pair is 4 per sec.

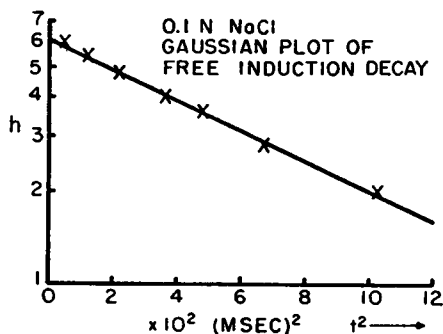


FIGURE 2

FIGURE 2 Gaussian plot of free induction decay of  $\text{Na}^+$  in aqueous solution. The high homogeneity magnet was used. On the vertical axis, the log of voltage output ( $h$ ) of the pulsed NMR spectrometer following a single  $90^\circ$  pulse at a repetition rate of 4 per sec is plotted in arbitrary units against  $t^2$ , where  $t$  is time after the  $90^\circ$  pulse. The sample is 2 ml of 0.1 N NaCl at  $25^\circ\text{C}$ . This data is an average of six measurements. The approximate linearity of this plot indicates conformity to a gaussian curve, which allows a linear extrapolation to  $t^2 = 0$  to determine the initial height of the free induction decay.

Initial heights of the free induction decay of various concentrations of  $\text{Na}^+$  in NaCl solutions were measured as described in the Methods section. The data plotted in Fig. 3 show that this method of analysis for  $\text{Na}^+$  yields a linear standard curve. The initial height of the free induction decay of 0.1 N NaCl was observed not to be significantly changed by the addition of any of the following: 0.1 N HCl, 0.1 N KOH, 0.1 M  $\text{MgSO}_4$ , 0.1 M  $\text{K}_2\text{HPO}_4$ , or 0.1 M citric acid. The addition of paramagnetic ions (0.1 M  $\text{MnCl}_2$  or 0.1 M  $\text{CuSO}_4$ ) also had no significant effect on the initial height of the free induction decay of  $\text{Na}^+$ , even though these ions shortened  $T_2$  by 30%, as described in the previous paragraph. This confirms for the case of Na the conclusion drawn from previous studies of D in  $\text{D}_2\text{O}$  (22), that the initial height of the free induction decay is a valid measure of  $\text{Na}^+$  concentration even when  $T_2$  varies.

A brief study was made of  $\text{Na}^+$  in gelatin gels. Incorporation of 0.1 N NaCl into a 5 or 10% gelatin gel was observed to have no effect on the initial height of the free induction decay of  $\text{Na}^+$ . However,  $T_2$  of  $\text{Na}^+$  was shortened by 28 and 45% respectively when 0.1 N NaCl was incorporated into a 5 or 10% gelatin gel. This effect might result from rapid exchange of dissolved  $\text{Na}^+$  with a fraction of  $\text{Na}^+$

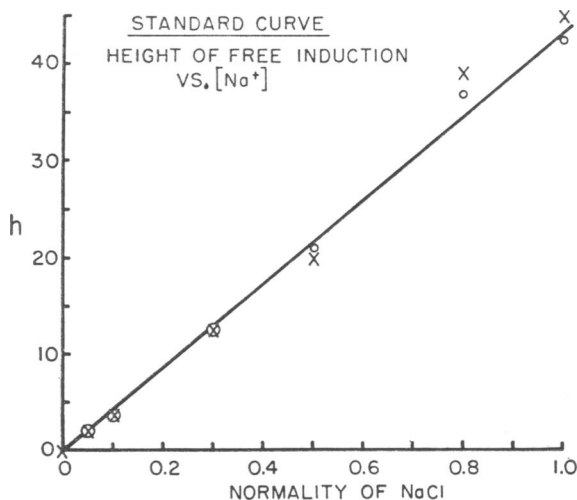


FIGURE 3 Standard curve of initial height of free induction decay vs.  $\text{Na}^+$  concentration. On the abscissa is plotted  $\text{Na}^+$  concentration for 2 ml volumes of aqueous  $\text{NaCl}$  solutions at  $25^\circ\text{C}$ . On the ordinate,  $h$  represents in arbitrary units the initial height of the free induction decay after a single  $90^\circ$  pulse. The two sets of points, depicted by crosses and circles, represent two sets of measurements on the same samples.  $h$  was determined by extrapolation of the gaussian decay curve to  $t = 0$  as described in the Methods section. Each free induction decay curve was an average of 200 measurements performed at a repetition rate of 4 per sec. RC filtering of  $0.75 \times 10^{-3}$  sec was applied to the output of the pulsed NMR spectrometer. The high homogeneity magnet was used.

complexed by gelatin. However, the present author knows of no studies suggesting complexing of  $\text{Na}^+$  by gelatin. Another possible explanation is suggested by the small but real changes in the NMR behavior of water in gelatin gels (22), which suggest that water in gelatin gels has slightly more structure than liquid water. Increased water structure would produce increased electric field gradients, which would be expected to interact with the quadrupole electric moment of the  $\text{Na}$  nucleus to cause faster NMR relaxation of  $\text{Na}^+$ , as observed for  $\text{Na}^+$  in gelatin.

## II. SPIN-ECHO NMR OF $\text{Na}^+$ COMPLEXED BY ION-EXCHANGE RESINS

Jardetzky and Wertz (20) have interpreted *steady-state* NMR measurements of  $\text{Na}^+$  in ion-exchange resin preparations to indicate that complexing of  $\text{Na}^+$  by the resin produced an NMR spectrum that was so broad and low that it was obscured by instrumental noise. A marked broadening of the steady-state NMR spectrum of  $\text{Na}^+$  complexed by ion-exchange resin was observed directly by Czeisler et al. (17). In the present study, packed, wet Dowex 50 resin in the  $\text{Na}^+$  form was analyzed by pulsed NMR. For  $\text{Na}^+$  in the resin, the free induction decay following a single  $90^\circ$  pulse was much shorter than that of  $\text{Na}^+$  in aqueous solution and was a simple exponential decay instead of the gaussian curve which was seen with aqueous solu-

TABLE I  
 $T_2$  AND  $T_1$  OF  $\text{Na}^+$  COMPLEXED BY ION-EXCHANGE RESINS

Resin name	Resin structure	$T_2(\times 10^{-3} \text{ sec})$		$T_1(\times 10^{-3} \text{ sec})$	
		Data	Mean	Data	Mean
Dowex 50 ( $\times 8$ )	Polystyrene- $\text{SO}_3\text{Na}$	1.4, 1.3, 1.4, 1.3, 1.4, 1.3	1.35	2.75, 2.2	2.5
Amberlite IRC-50	Acrylic-COONa	0.33, 0.36	0.34		
Amberlite IR-100	Polyphenol- $\text{CH}_2\text{SO}_3\text{Na}$	0.24, 0.23	0.24		
Aqueous solution of 1 N NaCl (ref. 26)			56.00		56.0

RC filtering of  $0.02 \times 10^{-3}$  sec time constant was used for the Dowex 50 measurements. Filtering of  $0.05 \times 10^{-3}$  sec was used for the other resins.

tions. For  $\text{Na}^+$  in Dowex 50 subjected to a  $90^\circ$ - $180^\circ$  pulse pattern, echoes could not be seen unless the pulse interval was shortened to approximately the time constant of the free induction decay, so that the echoes overlapped the free induction decay. Therefore, it was clear that the short free induction decay observed for  $\text{Na}^+$  in wet Dowex 50 must be determined by  $T_2$ .  $T_2$  measured from free induction decays of  $\text{Na}^+$  in wet Dowex 50 averaged  $1.35 \times 10^{-3}$  sec (Table I), compared with a  $T_2$  value of  $55 \times 10^{-3}$  sec for  $\text{Na}^+$  in aqueous 1 N NaCl solution. By the  $90^\circ$ - $90^\circ$  pulse technique,  $T_1$  for  $\text{Na}^+$  in Dowex 50 was observed to average  $2.5 \times 10^{-3}$  sec (Table I) compared with  $55 \times 10^{-3}$  sec for aqueous 1 N NaCl solution.  $T_2$  measured for  $\text{Na}^+$  in packed wet preparations of two other ion-exchange resins (Amberlite IRC-50 and IR-100) showed even greater shortenings to mean values of  $0.35 \times 10^{-3}$  and  $0.25 \times 10^{-3}$  sec respectively (Table I). These measurements indicate that complexing by ion-exchange resins shortens  $T_2$  of  $\text{Na}^+$  by 40–200 times. Fast NMR relaxation is indeed what one would expect for a Na atom whose quadrupole electric moment interacts with the large electric field gradients present at a charged complexing site. The observed shortening of NMR relaxation time is consistent with previous evidence for marked broadening of the steady-state NMR line of complexed  $\text{Na}^+$  (17, 20).

### III. SPIN-ECHO NMR OF $\text{Na}^+$ IN MUSCLE, BRAIN, AND KIDNEY

Preliminary study of  $\text{Na}^+$  in fresh brain or kidney by pulsed NMR using a single  $90^\circ$  pulse with a filtering time constant  $0.1 \times 10^{-3}$  sec yielded a free induction decay curve which consisted of a sum of two different components: (A) an initial component which decayed as a single exponential with a decay time of approximately  $1 \times 10^{-3}$  sec, superimposed on (B) a slower component which had a gaussian shape, decaying over  $3\text{--}4 \times 10^{-3}$  sec, which was the decay produced by inhomogeneities of the field of the magnet used, and was identical with the free induction



decay observed with aqueous NaCl solutions. This indicated that tissue Na<sup>+</sup> consisted of two distinct fractions. The task was then undertaken to measure the NMR relaxation times of each of the two fractions independent of the other, and to determine the concentrations of the two fractions.

First, the *slow* fraction of tissue Na<sup>+</sup> was studied.  $T_2$  of the slow fraction was determined from the decay of the height of the echo as a function of time after a 90°-180° pulse pair. Only times longer than approximately  $3 \times 10^{-3}$  sec were used, in order that signal emission from the fast fraction would no longer be of significant magnitude. Echo decays obtained from muscle, brain, and kidney showed a single exponential pattern (Fig. 4), from which  $T_2$  was measured.  $T_2$  for the slow fraction of Na<sup>+</sup> in muscle, brain, and kidney showed mean values in the range of  $9\text{--}14 \times 10^{-3}$  sec (Table II), which compares with a value of  $56 \times 10^{-3}$  sec for aqueous 0.1 N NaCl solution.  $T_1$  for the slow fraction of tissue Na<sup>+</sup> was determined from the measurement of height of the second pulse of a 90°-90° pulse pair as a function of time at times longer than  $3 \times 10^{-3}$  sec which yielded a single exponential curve (Fig. 5).  $T_1$  for the slow fraction of Na<sup>+</sup> in muscle and brain showed values resembling those measured for  $T_2$  (Table II), which is moderately shorter than  $T_1$  of aqueous NaCl.

The next problem was to determine the relative concentrations of the slow and fast fractions of Na<sup>+</sup> in tissues. This was accomplished by a measurement of the concentration of the slow fraction in a way which minimized errors due to the presence of the fast fraction. Subtraction of the concentration of the slow fraction

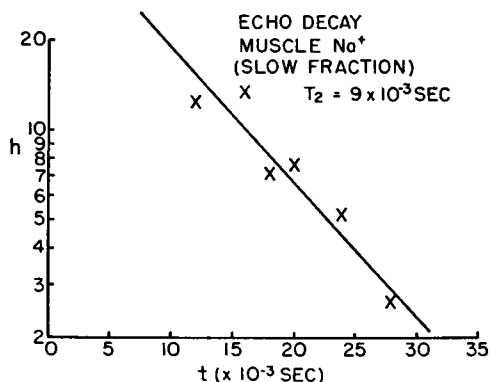


FIGURE 4 Echo decay for muscle Na<sup>+</sup> (slow fraction). Sample is 2 ml of fresh rat muscle at 26°C. Height ( $h$ ) of the echo following a 90°-180° pulse pattern was measured as a function of the time ( $t$ ) between the echo and the 90° pulse.  $h$  is expressed in arbitrary units.  $h$  on a log scale is plotted against  $t$ . From the straight line drawn through the data,  $T_2$  is estimated to be  $9 \times 10^{-3}$  sec, which is the time for  $h$  to decay to  $1/e$  of a previous value. Each data point shown here represents an average of 4800 measurements, performed at a rate of 16 per sec, with RC filtering of  $1 \times 10^{-3}$  sec time constant applied to the detector output. The low homogeneity magnet was used.

TABLE II  
 $T_1$  AND  $T_2$  OF SLOW FRACTION OF  $\text{Na}^+$  IN TISSUES

Specimen	$T_2(\times 10^{-3} \text{ sec})$		$T_1(\times 10^{-3} \text{ sec})$	
	Data	Mean	Data	Mean
Aqueous 0.1 N NaCl	52, 58, 60, 51, 59	56	54, 60, 51, 57, 53	55
“ “ “ (ref. 26)		56		56
Rat muscle	9, 16, 26, 11, 7	14	12, 10, 12, 12	12
Rat brain	11, 10, 9, 11, 11	10	14, 25, 12, 11	15
Rat kidney	8, 8, 10, 12, 8, 8	9		

This data was obtained under the experimental conditions given in Table III.

TABLE III  
 EXPERIMENTAL CONDITIONS FOR DATA OF TABLE II

Specimen and measurement	RC filtering ( $\times 10^{-3} \text{ sec}$ )	No. of repetitions averaged	Repetition rate  <i>repetitions/sec</i>
0.1 N NaCl— $T_2$	1	240	4
“ “ $T_1$	1	200	4
Muscle— $T_2$	1	4800	16
“ $T_1$	1	4800	16
Brain— $T_2$	1.5	200	4
“ $T_1$	1	1920	16
Kidney— $T_2$	1.5	400	4

Temperature of samples was maintained between 25° and 30°C. All measurements on tissues were completed within 1 hr after death of the rat, except those on muscle which sometimes required as long as 2 hr. Kidney and brain  $T_2$  measurements used a high homogeneity magnet, so that  $T_2$  was shorter than the free induction decay of a single 90° pulse and was measured from the latter. 0.1 N NaCl was measured with the high homogeneity magnet but used decay of echoes. Muscle  $T_2$  values were obtained from echo decays with the low homogeneity magnet. All other measurements used the low homogeneity magnet. An exception is the last value of  $T_1$  for muscle in Table II, which was obtained from the free induction decay with the high homogeneity magnet, used RC filtering of  $1.5 \times 10^{-3} \text{ sec}$ , and is an average of 2230 repetitions of a single 90° pulse at a rate of 11 repetitions per sec. Each value of  $T_2$  or  $T_1$  for tissue in Table II was obtained on tissue from a different rat.

of tissue  $\text{Na}^+$  from total tissue  $\text{Na}^+$  then yielded the concentration of the fast fraction.

The concentration of the slow fraction of tissue  $\text{Na}^+$  could in principle have been determined from the free induction curve following a single 90° pulse, which yielded the two-component curve described in the first paragraph of this section. This method would involve extrapolation of the slower, the gaussian, portion of the

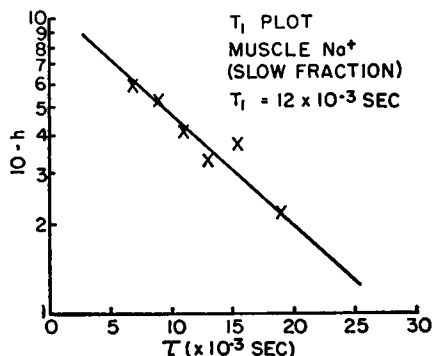


FIGURE 5  $T_1$  plot for muscle  $\text{Na}^+$  (slow fraction). Sample is 2 ml of fresh rat muscle at  $26^\circ\text{C}$ . Height ( $h$ ) of the free induction decay of the *second* pulse of a  $90^\circ$ - $90^\circ$  pulse pattern was measured as a function of time ( $\tau$ ) between pulses.  $h$  is expressed in arbitrary units. Height of the free induction decay of the first pulse was measured equal to 10.0.  $(10-h)$  on a log scale is plotted against  $\tau$ . From the straight line drawn through the data points,  $T_1$  is estimated to be  $12 \times 10^{-3}$  sec, which is the time for  $(10-h)$  to decay to  $1/e$  of a previous value. Each data point shown here represents an average of 4800 measurements, performed at a rate of 16 per sec, with RC filtering of  $1 \times 10^{-3}$  sec time constant applied to the detector output. The low homogeneity magnet was used.

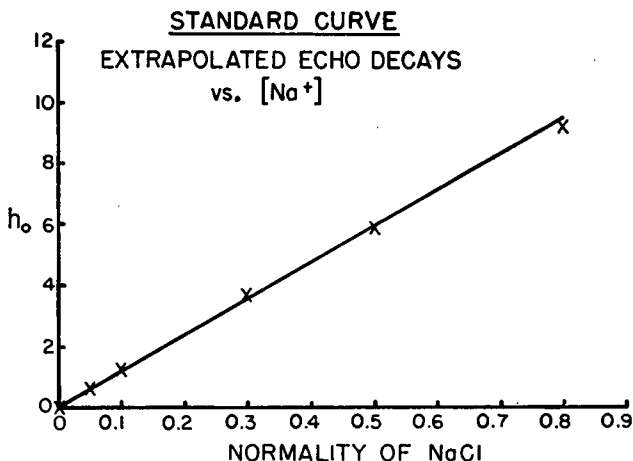


FIGURE 6 Standard curve of initial height of extrapolated echo decays vs.  $\text{Na}^+$  concentration. On the abscissa is plotted  $\text{Na}^+$  concentration in 2 ml volumes of aqueous  $\text{NaCl}$  solutions at  $25^\circ\text{C}$ . On the ordinate,  $h_0$  represents the height of the echo decay curve extrapolated on a semilog plot to  $t = 0$ . Each echo is an average of 200 measurements with a  $90^\circ$ - $180^\circ$  pulse pattern at a repetition rate of 4 per sec. RC filtering of  $0.5 \times 10^{-3}$  sec was used. The low homogeneity magnet was used.

curve back to  $t = 0$ , to yield the initial height of the free induction decay of the slow fraction, which could be compared with the same measure for a 0.1 N  $\text{NaCl}$  standard, to calculate the concentration of  $\text{Na}^+$  in the slow fraction. This method proved inaccurate because slight errors in adjustment of magnetic field to NMR resonance

caused large errors in shape of the slow portion of the free induction curve, so that gaussian extrapolations to  $t = 0$  showed large variability. This difficulty was eliminated by plotting echo decay curves of the slow fraction for times longer than  $3 \times 10^{-3}$  sec after a  $90^\circ$ - $180^\circ$  pulse pattern, and then extrapolating to  $t = 0$  the

TABLE IV  
CONCENTRATIONS OF SLOW AND FAST FRACTIONS  
OF TISSUE  $\text{Na}^+$

Rat No.	Type of tissue	Total $\text{Na}^+$	Slow fraction	Fast fraction	Per cent fast fraction
		<i>mmoles/liter</i>	<i>mmoles/liter</i>	<i>mmoles/liter</i>	%
1	Muscle	27	11	16	59
2	"	26	9	17	66
3	"	23	11	12	52
4	"	24	10	14	58
5	"	25	9	16	64
6	"	36	11	25	70
Mean	"				62
7	Brain	43	14	29	67
8	"	50	17	33	66
9	"	55	19	36	66
10	"	43	13	30	70
11	"	45	16	29	65
12	"	50	17	33	66
Mean	"				67
13	Kidney	59	24	35	59
14	"	64	20	44	70
15	"	65	20	45	70
16	"	66	22	44	68
17	"	55	19	36	66
Mean	"				67

Total tissue  $\text{Na}^+$  concentrations were measured by steady-state NMR after ashing (15). Concentration of the slow fraction (i.e. the fraction of tissue  $\text{Na}^+$  with a long ( $10$ - $15 \times 10^{-8}$  sec) NMR relaxation time) was measured by semilog extrapolation of the echo decay curve to  $t = 0$  to yield an initial height from which  $[\text{Na}^+]$  was determined by comparison with a similar measurement on an aqueous  $\text{NaCl}$  standard. Concentration of the fast fraction (i.e. the fraction of tissue  $\text{Na}^+$  with  $T_2 \cong 1 \times 10^{-8}$  sec) was calculated by subtraction of the concentration of the slow fraction from total  $\text{Na}^+$ . The fast fraction was also computed as per cent of total tissue  $\text{Na}^+$ . All concentrations are reported as per unit volume of fresh tissue. Echoes were measured after a  $90^\circ$ - $180^\circ$  pulse pattern at a repetition rate of 4 per sec with RC filtering of  $0.5 \times 10^{-3}$  sec on the detector output. Each echo-decay curve for tissue or  $\text{NaCl}$  standard was based on four echo heights of different pulse spacing longer than  $3 \times 10^{-3}$  sec. Each echo recording was an average of 700, 300, and 200 measurements for muscle, brain, or kidney respectively.

resulting single exponential decay curve. Thus, one obtained the initial height ( $h_0$ ) of the signal emitted by the slow fraction of tissue  $\text{Na}^+$  without errors due to signal emission from the fast fraction. Since  $h_0$  is theoretically and experimentally (Fig. 6) proportional to  $\text{Na}^+$  concentration, the concentration of the slow fraction of tissue  $\text{Na}^+$  was calculated by comparison of  $h_0$  of the tissue sample with the same measurement on a 0.1 N NaCl standard solution obtained immediately afterwards. To test experimentally the theoretical expectation that concentration of  $\text{Na}^+$  measured in this way would be independent of NMR relaxation time,  $h_0$  measured in 0.1 N NaCl was compared with values obtained for 0.1 N NaCl plus 0.5 M  $\text{CuSO}_4$  plus 15% gelatin, which shortened  $T_2$  to approximately  $10 \times 10^{-8}$  sec. Values of  $h_0$  obtained for the Cu-gelatin solution were 3.9, 3.5, 4.3, 3.7, and 3.1 (mean = 3.7) which were similar to the values observed for pure 0.1 N NaCl solution (3.9, 3.5, 3.6, 3.7, and 3.7 [mean = 3.7]). The same arbitrary units are used for both sets of measurements.

The relative concentrations of slow and fast fractions of  $\text{Na}^+$  measured in rat muscle, brain, and kidney are presented in Table IV, which shows that most  $\text{Na}^+$  (60–70%) in these tissues belongs to the fast fraction.

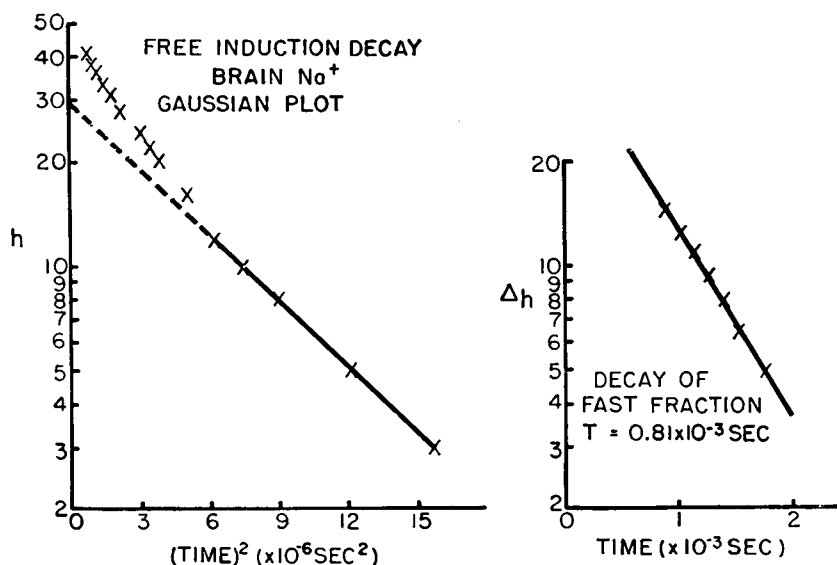


FIGURE 7 Measurement of  $T_2$  of fast fraction of brain  $\text{Na}^+$ . Left curve is gaussian plot of free induction decay of 2 ml of rat brain after a single  $90^\circ$  pulse with RC filtering =  $0.05 \times 10^{-8}$  sec and averaged 3720 times.  $h$  represents in arbitrary units the voltage emitted by the sample. The linear lower portion of the curve representing the magnetic inhomogeneity decay of the slow fraction of brain  $\text{Na}^+$  is extrapolated by the dotted line to  $t = 0$ , which reveals the presence of an additional fast fraction of brain  $\text{Na}^+$  at short times. The heights of the fast fraction ( $\Delta h$ ) were determined by subtracting the heights of the dotted extrapolation from the heights of the measured curve at the same times. The curve on the right shows a semilog plot of the free induction decay of the fast fraction ( $\Delta h$ ) as a function of time, which is linear, and from which  $T_2$  of the fast fraction of brain  $\text{Na}^+$  was measured.

Finally,  $T_2$  of the fast fraction of tissue  $\text{Na}^+$  was measured. Using the free induction decay after a single  $90^\circ$  pulse with only minimal RC filtering, the gaussian decay curve of the slow fraction of tissue  $\text{Na}^+$  was subtracted from the total curve to leave the free induction decay of the fast fraction of tissue  $\text{Na}^+$ , which showed single exponential decay from which  $T_2$  was measured (Fig. 7). This procedure was appropriate because  $T_2$  of the slow fraction was significantly *longer* than the decay time due to magnetic inhomogeneity, while  $T_2$  of the fast fraction was significantly *shorter* than the inhomogeneity decay. Details of this procedure are given in the captions of Fig. 7 and Table V.

Table V shows that  $T_2$  of the fast fraction of  $\text{Na}^+$  in muscle, brain, and kidney has values in the region of  $0.5\text{--}1.0 \times 10^{-3}$  sec, which resemble the values recorded for  $\text{Na}^+$  complexed by synthetic ion-exchange resins (Table I), but differ markedly from the  $T_2 = 56 \times 10^{-3}$  sec observed for  $\text{Na}^+$  in aqueous 0.1 N NaCl solutions.

We may summarize these observations by stating that the NMR behavior of  $\text{Na}^+$  is similar in muscle, brain, and kidney. 60–70% of tissue  $\text{Na}^+$  shows a fast NMR relaxation time resembling those measured for  $\text{Na}^+$  complexed by ion-exchange resins. Therefore, it seems reasonable to surmise that 60–70% of  $\text{Na}^+$  in tissue is complexed by tissue macromolecules. The remainder of tissue  $\text{Na}^+$  (the slow fraction) has NMR relaxation times only moderately faster than  $\text{Na}^+$  in aqueous solu-

TABLE V  
 $T_2$  OF FAST FRACTION OF TISSUE  $\text{Na}^+$

Rat No.	$T_2$ ( $\times 10^{-3}$ sec)		
	Muscle	Brain	Kidney
18	1.06	0.81	0.81
19	1.00	0.62	0.81
20	0.81	0.62	0.48
21	0.75	0.94	0.95
Mean	0.90	0.75	0.76

Samples are 2 ml of rat tissue within 1 hr postmortem at  $25^\circ \pm 1^\circ\text{C}$ . RC filtering on spectrometer is  $0.05 \times 10^{-3}$  sec. Free induction decays were measured after a single  $90^\circ$  pulse, repeated 32 times per sec, averaged on a  $10 \times 10^{-3}$  sec sweep. Number of repetitions averaged to give the free induction curve for each tissue are as follows: kidney, 1860; brain, 3720; muscle, 7440. Gaussian plot ( $\log h$  vs.  $t^2$ ) of each free induction curve was made. The linear portion of the plot at later times was linearly extrapolated back to  $t = 0$ , and was subtracted from the heights of the earlier portion of the measured curve (Fig. 7). The logarithm of difference height ( $\Delta h$ ) was plotted against  $t$  to yield a straight line, from which  $T_2$  of the fast fraction of  $\text{Na}^+$  was calculated. When this procedure was used with a sample of aqueous 0.05 N NaCl solution, no fast fraction of  $\text{Na}^+$  was detectable.

tion. Since evidence exists that cell water possesses more structure than liquid water (22, 23), it seems likely that the slow fraction represents  $\text{Na}^+$  dissolved in structured water of tissue. More structure may be expected to produce higher electric field gradients, which may be expected to interact with the quadrupole electric moment of Na to produce faster NMR relaxation than observed for  $\text{Na}^+$  in liquid water (22). Alternatively, the slow fraction might represent  $\text{Na}^+$  complexed by a type of site different from that which complexes the  $\text{Na}^+$  of the fast fraction.

Exchange between the  $\text{Na}^+$  of the fast and slow fractions must be relatively slow. Otherwise, the  $T_2$  decay curves of the two fractions would merge into a single exponential curve which would account for all of tissue  $\text{Na}^+$ .

These *spin-echo* NMR measurements of  $\text{Na}^+$  in tissues conform closely to the interpretations previously derived from *steady-state* NMR studies of tissue  $\text{Na}^+$  (14-18). The spin-echo NMR data agree well with other evidence of Ling (1, 2) and Troshin (3, 4) that most cellular  $\text{Na}^+$  is complexed, and that cell water is structured. The spin-echo data is *not* consistent with the classical hypothesis that cell  $\text{Na}^+$  is mostly free in solution in liquid water.

I wish to acknowledge my debt to Nuclear Magnetic Resonance Specialties, Co., New Kensington, Pa., for the loan of the high-homogeneity electromagnet on which some of these NMR measurements were made.

I am also indebted to the personnel of Nuclear Magnetic Resonance Specialties Co., especially to Mr. G. Donald Vickers, for assistance with a multitude of instrumental problems.

Received for publication 8 April 1970.

## REFERENCES

1. LING, G. N. 1969. *Int. Rev. Cytol.* **26**:1.
2. LING, G. N. 1960. *A Physical Theory of the Living State*. Blaisdell Publishing Company, New York.
3. TROSHIN, A. S. *Problems of Cell Permeability*. Original Russian edition published in Moscow. 1956. German translation published by Gustav Fischer Verlag, Jena. 1958. Revised English edition published by Pergamon Press Ltd., London. 1966.
4. TROSHIN, A. S. 1961. *In Membrane Transport and Metabolism*. A. Kleinzeller and A. Kotyk, editors. Academy Press Ltd., London.
5. COPE, F. W. 1965. *Bull. Math. Biophys.* **27**:99.
6. COPE, F. W. 1967. *Bull. Math. Biophys.* **29**:691.
7. COPE, F. W. 1970. *Adv. Biol. Med. Phys.* In press.
8. LING, G. N. 1965. *Ann. N.Y. Acad. Sci.* **125**:401.
9. COPE, F. W. 1967. *Bull. Math. Biophys.* **29**:583.
10. LEV, A. A. 1964. *Nature (London)*. **201**:1132.
11. LEV, A. A. 1964. *Biofizika*. **9**:686.
12. HINKE, J. A. M. 1959. *Nature (London)*. **184**:1257.
13. McLAUGHLIN, S. G. A., and J. A. M. HINKE. 1966. *Can. J. Physiol. Pharmacol.* **44**:837.
14. COPE, F. W. 1965. *Proc. Nat. Acad. Sci. U.S.A.* **54**:225.
15. COPE, F. W. 1967. *J. Gen. Physiol.* **50**:1353.
16. ROTUNNO, C. A., V. KOWALEWSKI, and M. CERELJIDO. 1967. *Biochim. Biophys. Acta.* **135**:170.
17. CZEISLER, J. L., O. G. FRITZ, and T. J. SWIFT. 1970. *Biophys. J.* **10**:260.
18. LING, G. N., and F. W. COPE. 1969. *Science (Washington)*. **163**:1335.
19. COPE, F. W., and R. DAMADIAN. 1970. *Nature (London)*. In press.

20. JARDETZKY, O., and J. E. WERTZ. 1960. *J. Amer. Chem. Soc.* **82**:318.
21. POPLE, J. A., W. G. SCHNEIDER, and H. J. BERNSTEIN. 1959. High Resolution Nuclear Magnetic Resonance. McGraw-Hill Book Company, New York.
22. COPE, F. W. 1969. *Biophys. J.* **9**:303.
23. HAZLEWOOD, C. F., B. L. NICHOLS, and N. F. CHAMBERLAIN. 1969. *Nature (London)*. **222**:747.
24. HAHN, E. L. 1950. *Phys. Rev.* **80**:580.
25. BOEHME, H., and M. EISNER. 1967. *J. Chem. Phys.* **46**:4242.
26. EISENSTADT, M., and H. L. FRIEDMAN. 1966. *J. Chem. Phys.* **44**:1407.
27. JARDETZKY, O. 1956. A Study of Interactions of Aqueous Sodium Ion by Nuclear Spin Resonance. Ph.D. Thesis. University of Minnesota, Minneapolis.