

Simulations and experimental demonstrations of encoding for X-ray coherent scatter

Danae Prokopiou^{a*}, Kerrie L. Smith^a, Keith Rogers^a, Priscila Paula^a, Paul Evans^b, Anthony Dicken^b and Simon Godber^c

^aCranfield Forensic Institute, Cranfield University, Shrivenham, SN6 8LA, England

^bThe Imaging Science Group, Nottingham Trent University, Nottingham, NG11 8NS, England

^cHALO X-ray Technologies, Nottingham Trent University, Nottingham, NG11 8NS, England

Correspondence email: d.prokopiou@cranfield.ac.uk

Synopsis Examples of encoding for X-ray diffraction experiments are presented. The encoding was shown to recover critical information from the experiments.

Abstract Diffraction data may be measured using approaches that lead to ambiguity in the interpretation of scattering distributions. Thus, the encoding and decoding of coherent scatter distributions have been considered with a view to enabling unequivocal data interpretation. Two encoding regimes are considered where encoding occurs between the X-ray source and sample, and where the encoder is placed between the sample and detector. In the first case, the successful recovery of diffraction data formed from the interrogation of powder samples with annular incident beams is presented using a coded aperture approach. In a second regime, encoding of Debye cones is shown to enable recovery of sample position relative to the detector. The errors associated with both regimes are considered and the advantages of combining both discussed.

Keywords: Focal construct geometry; X-ray diffraction; coded aperture; encoder

1. Introduction

Signal modulation through coded apertures (CAs) is a long established approach in X-ray astronomy (Mertz & Young, 1961; Ables, 1968; Dicke, 1968; Skinner, 1984; Busboom *et al.*, 1997) and nuclear medicine (Accorsi *et al.*, 2001; Martineau *et al.*, 2010; Mu *et al.*, 2009) for image recovery. Original applications include, for example, the use of Fresnel zone plates designed to behave as refractive optics within X-ray microscopes (Mertz & Young, 1961; Cannon & Fenimore, 1980). Applications involving the encoding of X-ray diffraction data are uncommon but recent high energy studies have shown a significant advantage for such approaches (Faust *et al.*, 2009; Schultz *et al.*, 2009).

IMPORTANT: this document contains embedded data - to preserve data integrity, please ensure where possible that the IUCr Word tools (available from <http://journals.iucr.org/services/docxtemplate/>) are installed when editing this document.

Conventionally when applying encoding, the intensity distribution on a detector $P(x,y)$ is formed from the correlation of a coded mask $A(x,y)$ with an object $O(x,y)$. An ideal mask would, in practice, be a pin-hole (δ -function), but this has limited transmissivity and thus the concept of masks with multiple pin-holes was developed (Ables, 1968; Dicke, 1968). A reconstruction or inverse function must be identified that transforms $P(x,y)$ into an accurate representation of $O(x,y)$. Several mask species with various pinhole spatial distributions have been proposed including random multi-pinhole arrays (Ables, 1968; Dicke, 1968; Cannon & Fenimore, 1980; Weiss *et al.*, 1977; Klotz *et al.*, 1974; Barrett & Swindell, 1981) and uniformly redundant arrays (URAs) (Busboom *et al.*, 1997; Cannon & Fenimore, 1980; Chen & Kishimoto, 2003; Fenimore & Cannon, 1978; Fenimore, 1978; Gottesman & Fenimore, 1989; Ding *et al.*, 2016). URAs can be particularly effective as the autocorrelation of these masks (the system point spread function, SPSF) approximates a δ -function and thus;

$$P(x,y)*A(x,y) \sim O(x,y) \quad (1)$$

where $*$ denotes the correlation operator.

Previous experimental imaging work has employed encoding masks in pre or post object positions (Ignatyer *et al.*, 2011; Olivo *et al.*, 2011). However, such approaches have rarely been employed to encode coherent scatter or aid in the interpretation of X-ray diffraction experiments. A notable exception is work recently reported by Duke University that has sought to encode recoverable information regarding the diffraction source to detector distance of multiple sources along a single axis (MacCabe *et al.*, 2012; Greenberg, Hassan, *et al.*, 2014; Greenberg, Krishnamurthy, *et al.*, 2014; Greenberg *et al.*, 2013). This made elegant use of a simple post-sample, comb aperture to encode Debye cones with an intensity modulation having a spatial frequency proportional to the source to detector distance (MacCabe *et al.*, 2012).

Herein, we introduce two unrelated approaches to the application of encoding for diffraction patterns when data is collected in transmission mode. In the first approach, a pre-sample annular mask (that has been shown previously to enhance diffracted intensity relative to a simple pencil beam (Rogers *et al.*, 2010; Evans *et al.*, 2010)) results in a scattering distribution that possesses an interpretive ambiguity. We show how this can be resolved using conventional coded aperture decoding algorithms that convolve the captured image with the coded mask (Ables, 1968; Fenimore & Cannon, 1978; Ballesteros *et al.*, 1996; Chen & Kishimoto, 2003). In the second approach (solving a different problem), we use post-sample encoders to determine the unknown position of either single or multiple diffraction sources and explore the precision with which this can be achieved.

Both coded aperture approaches introduced by this work have applications in areas where high speed identification is required, in particular where the sample's position within a volume is unknown. For

example, materials discrimination within the aviation security sector is relatively poor, thus the techniques can be exploited to identifying illicit materials within luggage.

2. Experimental

2.1. Pre-sample Encoding

The use of annular coded masks was examined some years ago for enhanced nuclear medicine imaging (Walton, 1973; Simpson, 1978). More recently, annular incident beam masks have been shown to provide a novel geometry within diffraction experiments that produce unique high intensity maxima (corresponding to Bragg peaks) along a single axis (Rogers *et al.*, 2010; Evans *et al.*, 2010). An annular beam also has the advantage for some applications of utilising a greater cross-section of the interrogating sample area when compared to traditional X-ray diffraction beams. This is important for applications such as security screening requiring simultaneous integration of a large volume, as well as when dealing with samples exhibiting some preferred orientations or large grain size (Chan *et al.*, 2010; Evans *et al.*, 2010; Rogers *et al.*, 2012). The scattering distribution measured in a plane parallel to the coded aperture consists of concentric ‘rings’ of high intensity formed from a superposition of multiple Debye cones. Unfortunately, the ring caustics are formed from both diverging and converging scatter cones and are thus difficult to interpret e.g. d-spacings cannot be directly calculated from the detector images unless scanning is applied. However, application of a traditional coded aperture approach is able to solve this problem. Consider a circular δ -function that is zero except at points on a circle of radius, c i.e. $\delta(r-c)$. The autocorrelation of this function is given by:

$$\int_0^{\infty} (\delta(r_0 - c)\delta(|\mathbf{r} - \mathbf{r}_0| - c)d^2r_0 = \frac{4c^2}{r\sqrt{4c^2 - r^2}} \quad (2)$$

where r and r_0 are two dimensional vectors with Cartesian co-ordinates (x, y) and (x_0, y_0) respectively and $|\mathbf{r}| = r$ (Barrett & Swindell, 1981). This has a relatively high intensity central maximum and a low intensity distribution between $0 < x < 2c$ and thus approximates a δ -function albeit with sidelobes.

The relationship presented in equation (1) was applied to the scattering distributions from a specimen by regarding the Debye cones as the ‘object’ to be recovered ($O(x,y)$) through convolution with the annular function, ($A(x,y)$). This method assumes that the material under examination is distributed homogeneously over the annular footprint of the incident beam and is experimentally illustrated within Fig. 1.

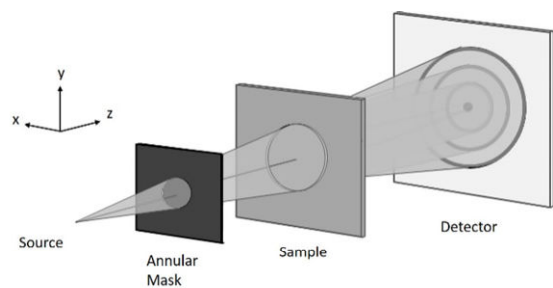


Figure 1 The experimental arrangement for the pre-sample encoding using an annular mask.

A simulation was used to illustrate the principle and develop the processing protocol. This involved convolving single FCG images with an image of the primary beam captured at the sample's position. A bandpass filter (filtered large structures down to 40 pixels and small structures up to 3 pixels) and thresholding (dc level removal) was then applied to the resulting image using ImageJ software (Schneider *et al.*, 2012). Further explanation and details on this process can be found in Prokopiou (2014). This protocol was subsequently followed using experimental data obtained with Zr filtered molybdenum radiation, an annular collimator (17.5 mm and 18 mm inner and outer diameters respectively) at 140 mm from the X-ray source, a ~ 0.2 mm thick aluminium oxide (Al_2O_3) sample at ~ 150 mm and a PIXIS 1024 (2D Gadox - Princeton Instruments) 13.3 x 13.3 mm area CCD detector with 1024 x 1024 pixels at 15 mm from the sample.

2.2. Post-sample Encoding

In addition to the coded aperture (CA) treatment in Section 2.1 used to recover the diffraction data, we have also employed simple post-sample encoding to determine unknown diffraction source positions. In this case using simple transmission geometry, an encoder is placed between the sample and detector plane to absorb completely relatively small areas of the scatter distributions (see Fig. 2). We explored the use of two novel encoders (linear and Archimedean spiral), each with a high open fraction of $\sim 90\%$. We have demonstrated the ability of these post-sample encoders to unambiguously encode conventional pencil beam diffraction data. The linear encoder was employed due to its simplicity, whereas the spiral was used to overcome potential limitations of the linear case (see section 3.2.1).

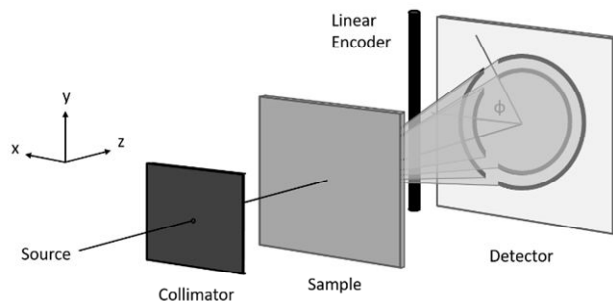


Figure 2 The experimental arrangement for the post-sample encoding using a simple linear encoder.

In both cases the sample to detector distance (D_{SD}) and Bragg angle of each diffraction maxima (θ) were determined independently using;

$$D_{SD} = D_{ED} \left[1 + \left(\frac{R_E}{R_D - R_E} \right) \right] \quad (3)$$

$$2\theta = \tan^{-1} \left(\frac{R_D - R_E}{D_{ED}} \right) \quad (4)$$

where D_{ED} is the encoder to detector distance, R_D and R_E are the radii of an arbitrary Debye ring at the detector plane and encoder plane, respectively (see Fig. 3). R_E may be determined for the linear encoder from $R_E = H/\cos\phi$ and for the spiral encoder from $R_E = a+b\phi$, where H is the encoder's lateral position relative to the primary X-ray beam, a & b are characteristics of the spiral, and ϕ is the azimuthal angle of encoding obscuration relative to the horizontal plane. The variables D_{ED} , H , a and b are fixed by the experiment and therefore measurement of ϕ and R_D for each Debye ring enables determination of D_{SD} and 2θ .

Initially, simulations were performed with McXtrace (Bergback Knudsen *et al.*, 2013) to examine various encoder geometries and forms. An error study was undertaken to explore how experimental uncertainties (e.g. encoder to detector distance) would propagate to estimations of sample position (distance D_{SD}) and 2θ .

Subsequently, experimental data were collected with a simple pencil beam transmission arrangement ($\text{CuK}\alpha$) and a GADDS (General Area Detector Diffraction System, supplied by Bruker) area detector. The encoders were formed from 0.5 mm diameter tungsten wire and the spiral was constructed as a simple single turn to avoid potential ambiguity arising from multiple encoding.

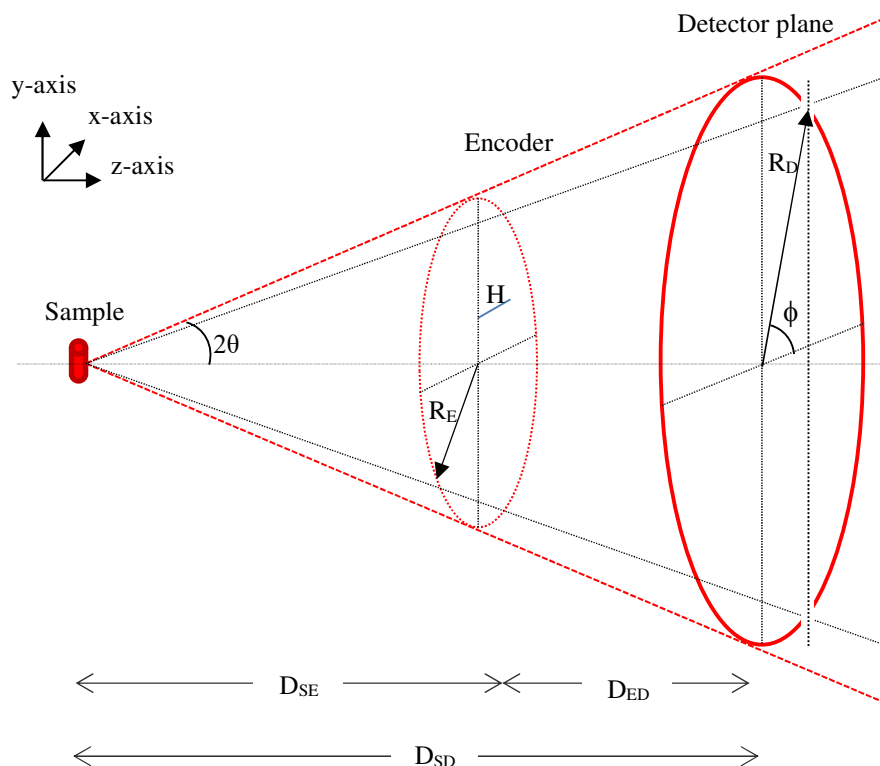


Figure 3 The geometric arrangement employed to record the 2D X-ray diffraction data encoded by a single post-sample encoder (in this example a linear encoder), when illuminated by a pencil beam.

3. Results and Discussion

3.1. Pre-sample encoding

Fig. 4a illustrates the result of a typical scattering distribution from an angular dispersive experiment in which a thin (~ 0.2 mm) plate of Al_2O_3 was illuminated with a pencil beam. The relatively small detector active area required 5×5 tiling in order to measure a minimum d -spacing of ~ 0.15 nm at the detector distance employed. The horizontal obscured rectangular area artefact was a result of limited x/y positioning of the sample stage. Fig. 4b shows a typical scatter pattern produced when using the pre-sample annular encoding mask. The apparent concentric rings should not be confused with the Debye rings observed during a pencil beam and flat detector conventional Laue type experiment; the central high intensity maxima shown in Fig. 4b is not the main interrogating X-ray beam. For further details on the geometrical origin of the concentric rings illustrated in Fig. 4b the reader could refer to Fig.1 of Evans *et al.* (2010).

This central high intensity results from the condition that $\frac{\text{annular radius}}{\text{Debye cone radius}} \sim 1$ for a particular set of diffracting planes. For this condition to be met, the sample (or detector) is translated along the primary beam axis until the annular radius = Debye cone radius (Rogers *et al.*, 2010). However, the

CA approach presented herein does not require this condition. For the purpose of this study, a mask incorporating an annular transparent region was employed as the coded aperture. As indicated by equation (2) and shown in Fig. 5, the autocorrelation of the annular mask approximates a δ -function, with sidelobes. Hence, an annular mask was convolved with the primary data collected at the detector. Fig. 4c shows the result of this convolution following the application of a bandpass filter and thresholding. Comparing this result with that from the pencil beam experiment shows that, at least qualitatively, the Debye cones have been accurately recovered. This was further demonstrated by a comparison of the diffractograms (see Fig. 4d) derived from the radial integration of data presented in Fig. 4a and Fig. 4c. The position of each diffraction peak's maximum intensity was obtained and compared to the corresponding peak in the recovered data via a residual sum of squares (RSS) analysis. The resulting RSS value was 0.02° (2θ) indicating a strong agreement between conventional diffraction data and recovered Debye cones in terms of peak positions. The source of discrepancies between relative intensities is due to (i) different sampling volumes and therefore different preferred orientations, and (ii) differences in Lorentz factors.

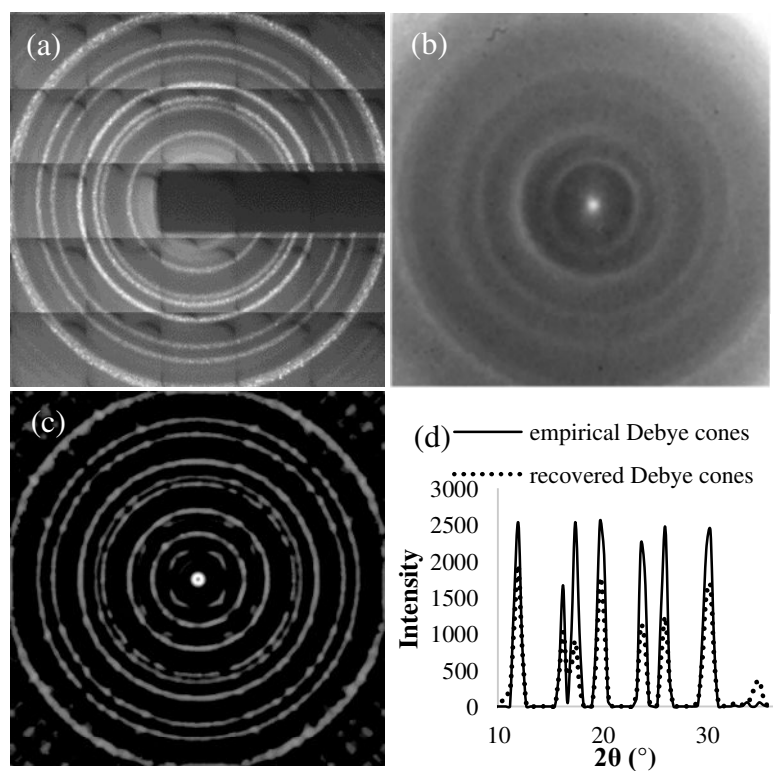


Figure 4 Experimental results of coded aperture processing. (a) Conventional pencil beam transmission diffraction data from a ~ 0.2 mm thick Al_2O_3 plate, (b) observed diffraction pattern from a ~ 0.2 mm thick Al_2O_3 plate with an annular pre-sample aperture, (c) recovered Debye rings following convolution of (b) with a captured image of the incident annular beam at the sample's z -position, (d) radial integration of (a) and (c).

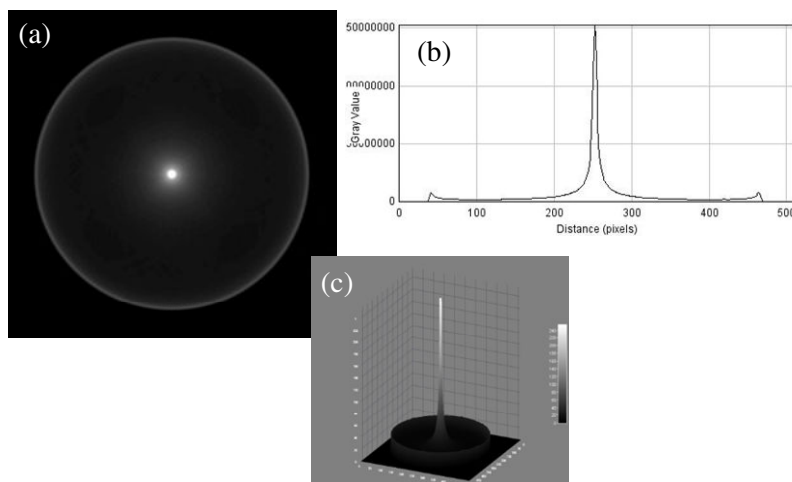


Figure 5 (a) 2D image of the autocorrelation of an annular aperture, (b) 2D profile plot of (a), and (c) 3D surface plot of (a).

3.2. Post-sample encoding

3.2.1. Linear encoder simulation

Simulations were conducted with calcite (CaCO_3) samples of thickness 0.05 mm illuminated with a pencil beam ($\text{CuK}\alpha$ radiation). Calcite was chosen as the diffraction data has a dominant diffraction maximum from the 104 reflection (thus enabling some clarity) and 0.05 mm allowed sufficient transmission to observe diffraction from multiple samples simultaneously. The offset distance of the linear encoder, H , and encoder to detector distance, D_{ED} , were systematically changed and coherent scatter distributions calculated at each point. The magnitude of the errors when determining the sample to detector distance (D_{SD}) from the inner 104 Debye cone was calculated via analytical error propagation and the results are shown in Fig. 6a. This demonstrates that the position of the linear encoder for minimising errors in estimated sample position occurs when the encoder to incident beam distance, H , is greatest and it is positioned close to the sample i.e. the distance between the linear encoder and detector, D_{ED} , is maximised. This is only true when the linear encoder interrupts the Debye cone, i.e. H is limited by the radius of the Debye cone at distance D_{ED} .

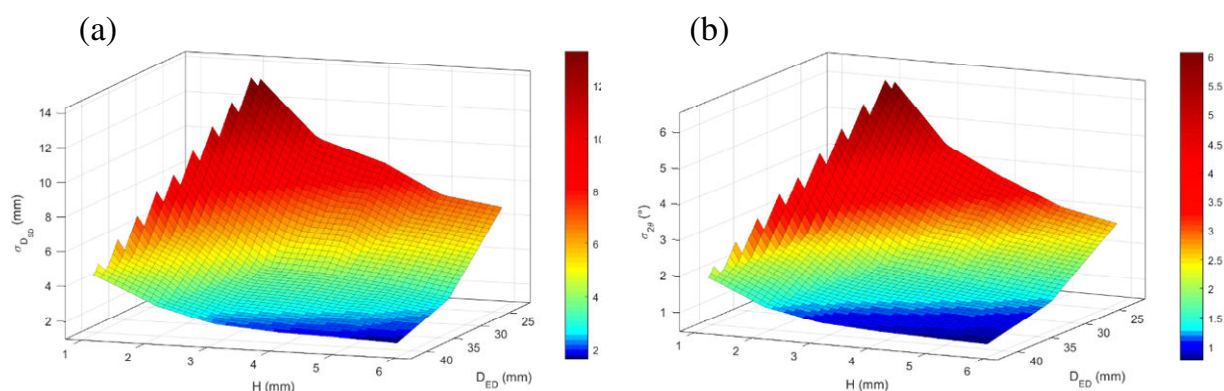


Figure 6 (a) 3D surface plot of sample to detector distance error and (b) 3D surface plot of error associated with measuring the scattering angle (2θ) calculated using the 104 reflection from the sample closest to the detector with a linear post-sample encoder.

The same trend can be observed when calculating the associated error of the scattering angle, 2θ , at each linear encoder location, Fig. 6b. Thus, errors in the determination of 2θ and sample position are minimised when D_{ED} and H are maximised, limited by the requirement of course that the encoder still interrupts the Debye cone. The most dominant source of error for these experimental conditions, with a 1% error in all variables, was associated with D_{ED} , the distance between the linear encoder and detector.

3.2.2. Linear encoder experimental

Initially, a sample of Al_2O_3 (plate) was placed at a known distance from the detector and the subsequent 2D scattering data used to calibrate critical encoder parameters, such as the encoder to detector distance (D_{ED}) and the encoder's lateral position relative to the primary X-ray beam (H). A series of experiments was then performed by collecting scattering data as the sample to detector distance was changed to confirm that the encoding behaved as predicted by equations (3) and (4) and the simulation.

A result from a multiplex sampling (>1 sample spatially separated along the primary axis) experiment is shown within Fig. 7a. Here, two thin samples (~ 0.05 mm) of calcite loaded cellulose were simultaneously placed within the primary beam at different distances from the detector. The scattering distribution is therefore the weighted sum of diffraction patterns from both samples. The obscurities formed by the encoder are clearly visible as vertical obscured regions and the encoding positions can be quantified from azimuthal plots such as those shown in Fig. 7b for the 104 calcite maxima corresponding to each sample.

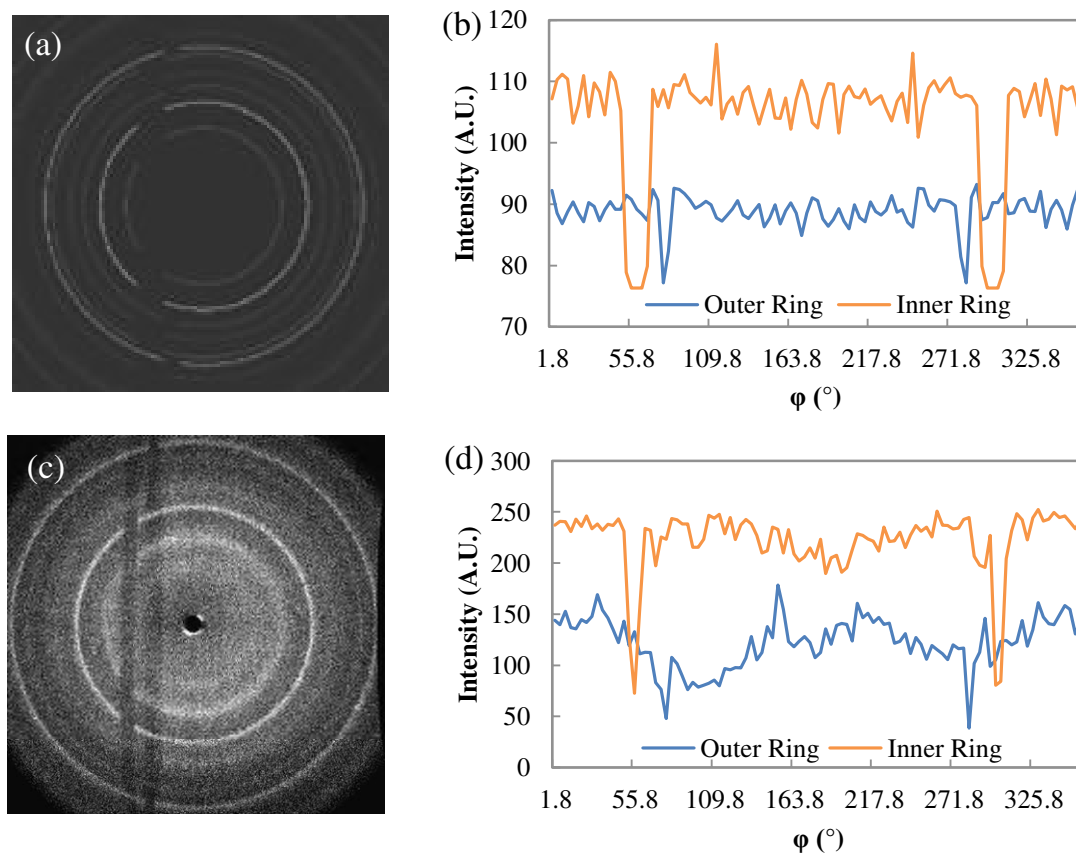


Figure 7 (a) Simulated image obtained with an off-centre linear encoder ($H = 6$ mm, $D_{ED} = 37$ mm) with two 0.05 mm thick calcite samples separated by 32 mm along the primary beam axis. The two brightest rings, from different calcite samples, have radii of 30 mm and 54 mm, respectively. (b) Azimuthal plots of simulated data (a) showing the encoding position for each high intensity Debye ring. (c) Diffraction pattern from a pair of calcite samples under the same experimental configuration as the simulations. (d) Azimuthal plots of experimental data (c).

Subsequent application of equations (3) and (4) is shown in Table 1, where the d-spacing and sample to detector distances are shown to be the same as those compared to their known values, within experimental errors. Thus, the position and d-spacing(s) (and therefore material phase) can, in principle, be determined with no *a priori* knowledge of the object position.

Table 1 Results of the linear encoding recovery. Samples 1 and 2 were placed at 60 mm and 92 mm respectively from the detector. The corresponding d-spacings for cellulose and calcite are 0.39002 nm and 0.3035 nm, respectively (ICDD database PDF 50-2241 and PDF 5-586).

Debye ring source	R_D (mm)	ϕ ($^\circ$)	Calculated sample to detector distance (mm)	Calculated d-spacing (nm)
Sample 1: Cellulose	25	47	59.9 ± 0.7	0.39 ± 0.02
Sample 1: Calcite	34	59	59.6 ± 0.6	0.30 ± 0.02
Sample 2: Cellulose	39	75	93.0 ± 0.6	0.39 ± 0.02
Sample 2: Calcite	52	78	91.1 ± 0.6	0.30 ± 0.02

3.2.3. Archimedean spiral encoder simulation

Simulations were also conducted with an Archimedean spiral encoder and two calcite samples of thickness 0.05 mm spatially separated along the primary beam axis. To illustrate the effectiveness of the approach, one of the plates was held stationary while the other was translated in 2 mm steps along the primary X-ray beam towards the stationary detector. The errors associated with determination of sample to detector distance (D_{SD}) and 2θ (from the 104 Debye cone) are shown in Fig. 8a and Fig. 8b, respectively.

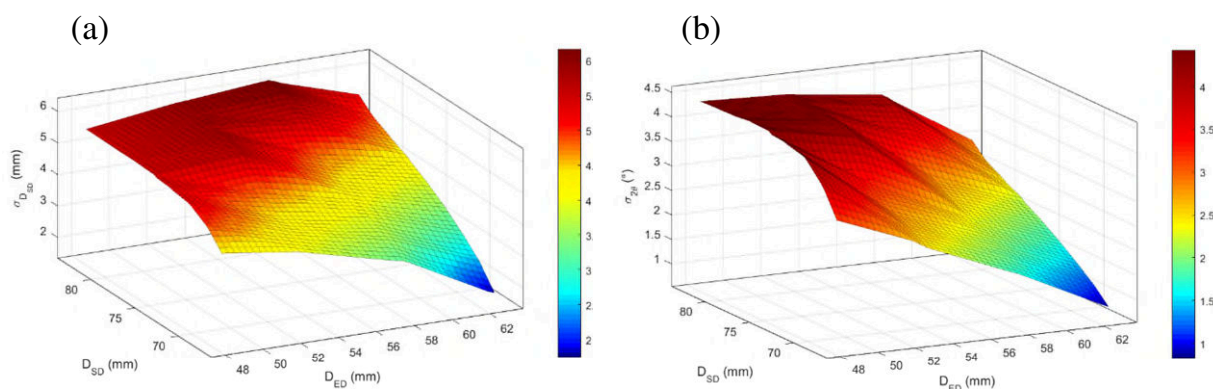


Figure 8 (a) 3D surface plot of sample to detector distance error and (b) 3D surface plot of error associated with measuring the scattering angle (2θ) calculated using the 104 calcite maxima from the sample closest to the detector with an Archimedean post-sample encoder.

As with the linear encoder, the position that minimises errors in scatter angle and sample position occurs when the spiral is closest to the sample, i.e. when D_{ED} is maximised. The error in the

calculated sample relative position was dominated by the measurement error in the encoder to detector distance. For the calculated scattering angle, 2θ , the greatest contributor to the total error was from the measurement error in Debye ring radius.

3.2.4. Archimedean spiral encoder experimental

Several experiments were performed including changing the sample to detector distance for a single sample and for multiple samples. One of the sample plates was held stationary while the other was translated in 2 mm steps along the primary X-ray beam towards the detector. To illustrate the encoding, Fig. 9 shows a sequence of scatter patterns collected from the two plate samples of calcite. The Debye cone encoding is apparent as limited opaque regions within each Debye ring. Using the dominant 104 scattering maxima, it is apparent that the encoding region associated with the translating sample appears to rotate simultaneously with a decrease in the associated Debye ring radius.

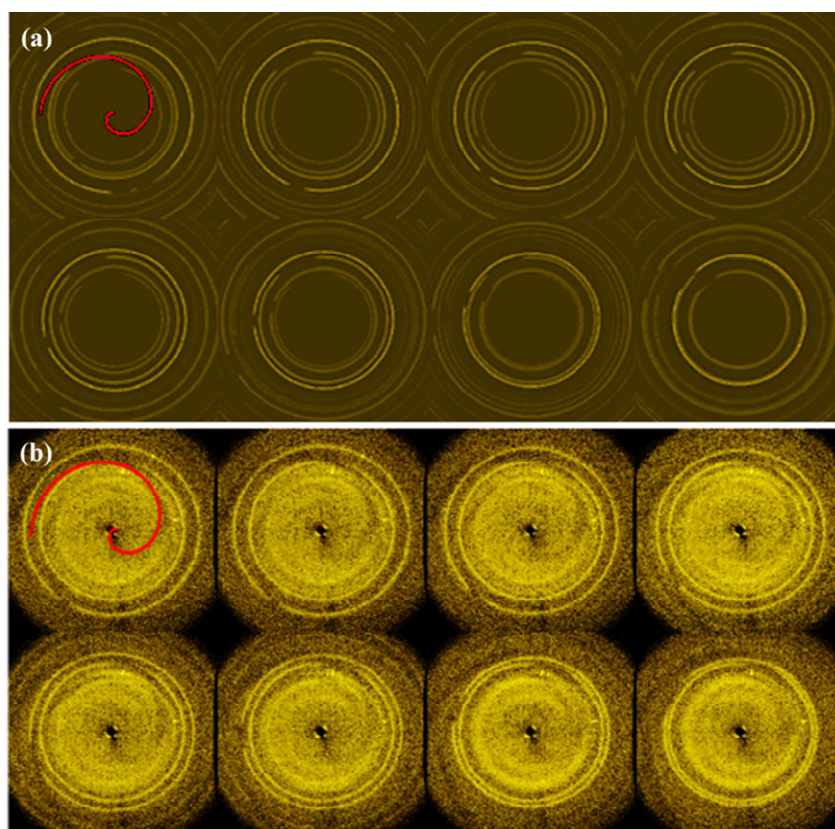


Figure 9 (a) A sequence of simulated images and (b) a sequence of diffraction patterns from of a pair of calcite samples spatially separated along the primary axis with a spiral encoder in front of the detector. The sequence was recorded as one of the samples was translated towards the detector face.

The radii of the Debye rings and their encoding ϕ angles were measured, and the scattering angles and sample to detector distances calculated at each translation step. The data is presented in Table 2, which indicates a good agreement with that expected for both parameters.

An analytical error analysis of these post-sample encoder geometries shows that the parameters with the most significant influence on estimated sample to detector distance and scatter angle are the encoder to detector distance and measured Debye ring radius, respectively.

For the linear encoder, a large wire to primary axis distance increases precision but unfortunately this coincides with a less accurate determination of ϕ and a limited d-spacing range.

Table 2 Results of the spiral encoding recovery. Sample 1 remained stationary while the sample to detector distance was incrementally increased for sample 2. The corresponding d-spacing for the 104 reflection of calcite is 0.3035 nm (ICDD database PDF 5-586).

Debye Ring Source	R_D (mm)	ϕ ($^\circ$)	R_E (mm)	Calculated d-spacing (nm)	Calculated Sample to Detector Distance (mm)	Measured Sample to Detector Distance (mm)
Sample 1: Fixed	37	165	6.7	0.30 ± 0.04	66.0 ± 0.5	67
Sample 2: Step 0	46	312	15.8	0.30 ± 0.03	82.6 ± 0.5	83
Sample 2: Step 1	45	304	15.2	0.31 ± 0.03	81.6 ± 0.5	81
Sample 2: Step 2	44	289	14.1	0.31 ± 0.03	79.6 ± 0.5	79
Sample 2: Step 3	42	268	12.6	0.31 ± 0.03	76.8 ± 0.5	77
Sample 2: Step 4	41	254	11.6	0.31 ± 0.03	75.1 ± 0.5	75
Sample 2: Step 5	40	234	10.4	0.30 ± 0.03	72.8 ± 0.5	73
Sample 2: Step 6	39	218	9.4	0.30 ± 0.03	71.0 ± 0.5	71

4. Conclusions

Two different methods for encoding angular dispersive, transmission diffraction data have been presented. We have shown how, by adopting a conventional coded aperture reconstruction process, conventional scattering distributions (i.e. Debye cones) may be recovered from the scattering patterns produced from an annular, pre-sample aperture. We have also shown how sample position and material phase information may be recovered through post-sample encoding. An application area which can benefit from both methods is detection of threat materials or illicit drugs in luggage or

parcels. The approach is currently the subject of study for employment within baggage screening systems.

The pre-sample annular coded aperture geometry was shown to produce a scattering pattern with several notable features. High intensity ‘condensation’ points at the centre of the patterns occur when the Debye cone radius and mask annular radius are equal. Interestingly perhaps, at sample positions where this condition is not true, then, in principle, there is no coherent scatter contribution at the diffraction pattern centre. Unfortunately, these scatter patterns are difficult to interpret; radially integrating produces diffractograms with two overlapping d-spacing scales due to the converging and diverging nature of the Debye cones. However, we have shown that these scatter patterns can be interpreted through convolution with the annular mask as a result of the near singular feature of the mask autocorrelation function. It can also be anticipated that using a mask annulus with a radius significantly greater than that of the Debye cones would produce an improved convolution reconstruction as the lobe extremes in the autocorrelation function (shown in Fig. 5) would contribute less to the final result. This is due to the fact that the lobe extremes present in the annulus’ autocorrelation function are the only source of reconstruction ‘confusion’ i.e. the only deviation from an ideal δ -function (see Fig. 5). We continued the simulation studies and these indicated that recovery was also effective with poorer S/N (in the measured data) or geometric distortion of the annular mask. However, the ambiguity in the Debye cones produced by this geometry means that the post-sample encoding solution demonstrated by Duke would be ineffective for this data (see below) (MacCabe *et al.*, 2012).

The second encoding approach introduced in this study, linear and spiral post-sample encoders, were shown to be effective at providing geometric and structural information. Material phase identification (through d-spacing determination) can be achieved with no *a priori* knowledge of the sample’s position relative to the detector. Linear and spiral encoders were shown to provide single axis positions with ~1% precision although accurate calibration was essential especially with the spiral encoder where small manufacturing errors (affecting *a* and *b*) significantly influence the derived parameters. Comparison of the induced errors from both encoders with 1% error in all their variables indicated that the Archimedean spiral yields a lower experimental error in the calculated D_{SD} distance (~7.5 times lower) than the linear encoder.

We anticipate that the combination of an incident beam annular mask and post-sample linear encoder has advantages over alternative coded aperture approaches. For example, a linear encoder (such as that described above) would provide sample position information, overcoming the inherent ambiguity in the converging and diverging Debye cones generated by conventional post-sample encoders. The convergence point acts as an inversion centre thus enabling discrimination between a converging and diverging Debye cone. Furthermore, such simple encoders have a high open fraction compared to conventional coded apertures and thus maximise the number of measured photons at the detector.

Acknowledgements With support of AWE plc.

References

- Ables, J. G. (1968). *Proceeding of the Astronomical Society of Australia* **1**, 172-173.
- Accorsi, R., Gasparini, F. & Lanza, R. C. (2001). *Nuclear Instruments and Methods in Physics Research A* **474**, 273-284.
- Ballesteros, F. J., Sanchez, F., Reglero, V., Porras, E., Perez, F. & Robert, A. (1996). *Proceedings 2nd INTEGRAL Workshop 'The Transparent Universe'*, pp. 357-360. St. Malo, France
- Barrett, H. H. & Swindell, W. (1981). *Radiological Imaging: The theory of image formation, detection, and processing*. New York: Academic Press.
- Bergback Knudsen, E., Prodi, A., Baltser, J., Thomsen, M., Kjaer Willendrup, P., Sanchez del Rio, M., Ferrero, C., Farhi, E., Haldrup, K., Vickery, A., Feidenhans'l, R., Mortensen, K., Meedom Nielsen, M., Friis Poulsen, H., Schmidt, S. & Lefmann, K. (2013). *Journal of Applied Crystallography* **46**, 679-696.
- Busboom, A., Schotten, H. D. & Elders-Boll, H. (1997). *Journal of Optical Society of America* **14**, 1058-1065.
- Cannon, T. M. & Fenimore, E. E. (1980). *Optical Engineering* **19**, 283-289.
- Chan, J., Evans, P., Wang, X., Godber, S., Peatfield, I., Rogers, K., Rogers, J. & Dicken, A. (2010). *Security Technology (ICCST), 2010 IEEE International Carnahan Conference*, 142-147.
- Chen, Y. W. & Kishimoto, K. (2003). *Review of Scientific Instruments* **74**, 2232-2235.
- Dicke, R. H. (1968). *The astrophysical journal* **153**, L101-105.
- Ding, J., Noshad, M. & Tarokh, V. (2016). *J. Opt. Soc. Am. A* **33**, 863-881.
- Evans, P., Rogers, K., Chan, J., Rogers, J. & Dicken, A. (2010). *Applied Physics Letters* **97**, 204101-204101 - 204101-204103.
- Faust, A. A., Rothschild, R. E., Leblanc, P. & McFee, J. E. (2009). *IEEE Transactions on Nuclear Science* **56**, 299-307.
- Fenimore, E. E. (1978). *Applied Optics* **17**, 3562-3570.
- Fenimore, E. E. & Cannon, T. M. (1978). *Applied Optics* **17**, 337-347.
- Gottesman, S. R. & Fenimore, E. E. (1989). *Applied Optics* **28**, 4344-4352.
- Greenberg, J., Krishnamurthy, K. & Brady, D. (2014). *Optics Letters* **39**, 111-114.
- Greenberg, J. A., Hassan, M., Krishnamurthy, K. & Brady, D. (2014). *Analyst* **139**, 709-713.
- Greenberg, J. A., Krishnamurthy, k., Lakshmanan, M., MacCabe, K., Wolter, S., Kapadia, A. & Brady, D. (2013). *Proceedings of SPIE* **8858**, 885813-885811 - 885813-885811.
- Ignatyer, K., Munro, P. R. T., Speller, R. D. & Olivo, A. (2011). *AIP Conference Proceedings* **1365**, 254-257.

- Klotz, E., Linde, R. & Weiss, H. (1974). *Optics Communications* **12**, 183-187.
- MacCabe, K., Krishnamurthy, K., Chawla, A., Marks, D., Samei, E. & Brady, D. (2012). *Optics Express* **20**, 16310-16320.
- Martineau, A., Rocchisani, J. M. & Moretti, J. L. (2010). *Nuclear Instruments and Methods in Physics Research A* **616**, 75-80.
- Mertz, L. & Young, N. O. (1961). *Proceeding of the International Conference on Optical Instruments and Techniques*, pp. 305-310. London: Chapman and Hall.
- Mu, Z., Hong, B., Li, S. & Liu, Y. H. (2009). *Medical Physics* **36**, 1533-1542.
- Olivo, A., Ignatyer, K., Munro, P. R. T. & Speller, R. D. (2011). *Nuclear Instruments and Methods in Physics Research A* **648**, S28-S31.
- Prokopiou, D. (2014). PhD thesis, Cranfield University.
- Rogers, K., Evans, P., Prokopiou, D., Dicken, A., Godber, S. & Rogers, J. (2012). *Nuclear Instruments and Methods in Physics Research Section A* **690**, 1-6.
- Rogers, K., Evans, P., Rogers, J., Chan, J. W. & Dicken, A. (2010). *J. Appl. Cryst.* **43**, 264-268.
- Schneider, C. A., Rasband, W. S. & Eliceiri, K. W. (2012). *Nature Methods* **9**, 671-675.
- Schultz, L. J., Wallace, M. S., Galassi, M. C., Hoover, A. S., Mocko, M., Palmer, D. M., Tonga, S. R., Kippen, R. M., Hynes, M. V., Toolin, M. J., Harris, B., McElroy, J. E., Wakeford, D. & Lanza, R. C. (2009). *Nuclear Instruments and Methods in Physics Research A* **608**, 267-274.
- Simpson, R. G. (1978). PhD thesis, The University of Arizona.
- Skinner, G. K. (1984). *Nuclear Instruments and Methods in Physics Research* **221**, 33-40.
- Walton, P. W. (1973). *Journal of Nuclear Medicine* **14**, 861-863.
- Weiss, H., Klotz, E., Linde, R., Rabe, G. & Tiemens, U. (1977). *Optica Acta* **24**, 305-325.